

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120921\
 Data File : PO083520.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Dec 2021 16:29
 Operator : AJ\MA
 Sample : M4967-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-11S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 01:23:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 07 13:18:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.940	3.944	1946836	655451	20.406	21.072
2)	SA Decachlor...	11.020	9.245	1238622	526804	17.339	16.148

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120921\
Data File : PO083520.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Dec 2021 16:29
Operator : AJ\MA
Sample : M4967-10
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-11S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 01:23:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120621.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 07 13:18:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

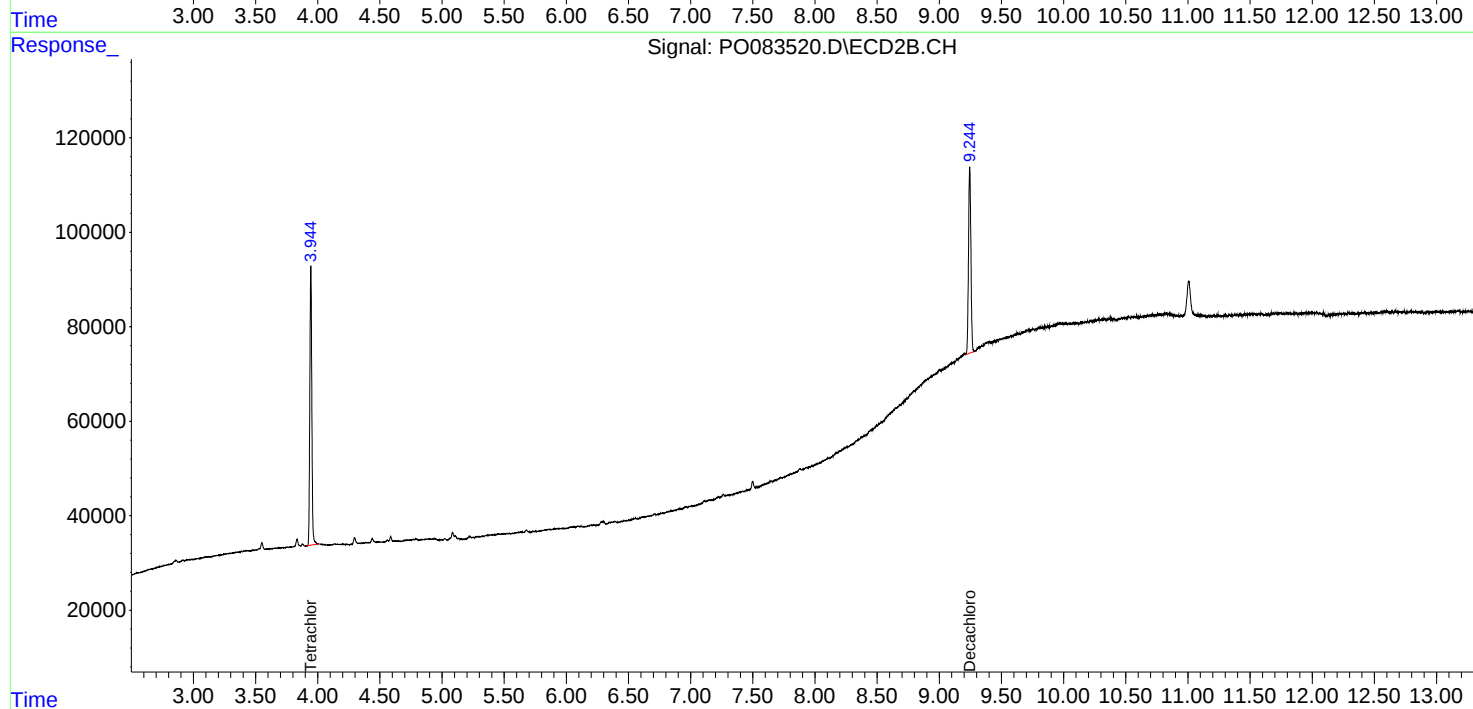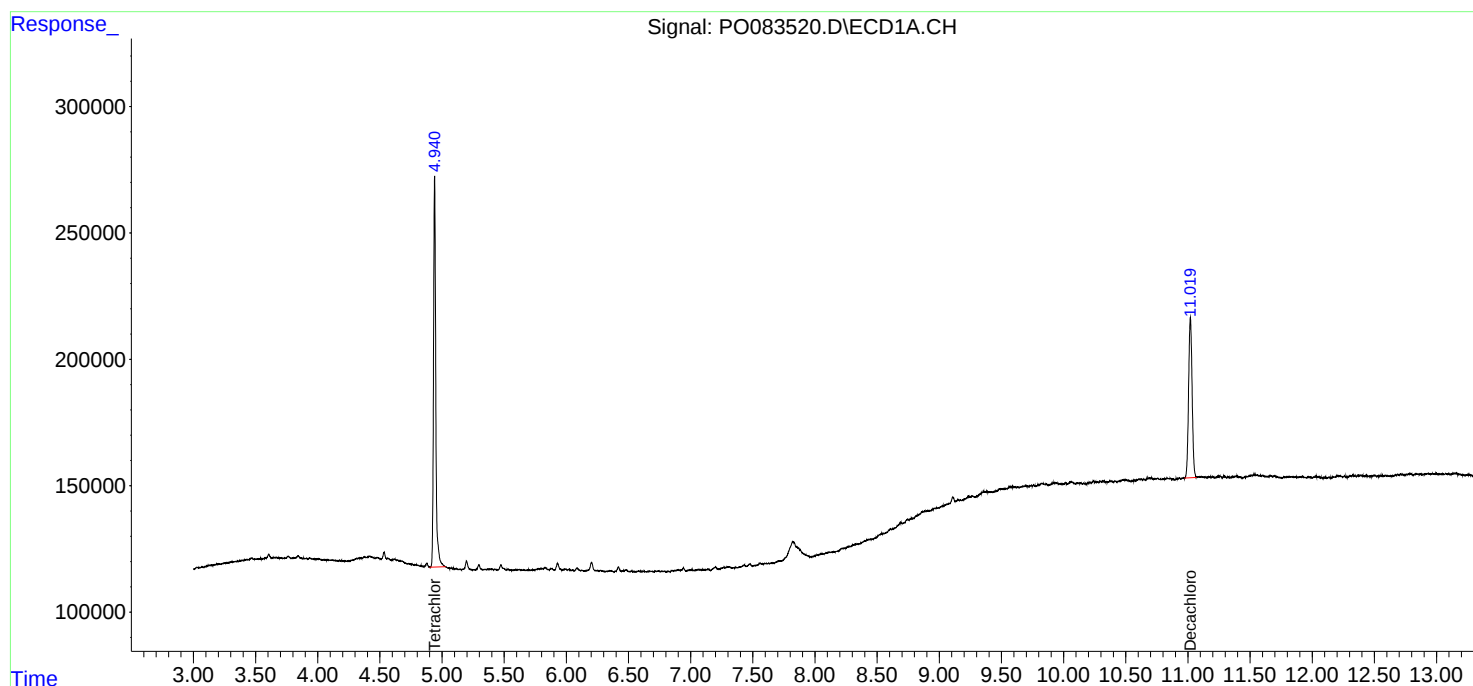


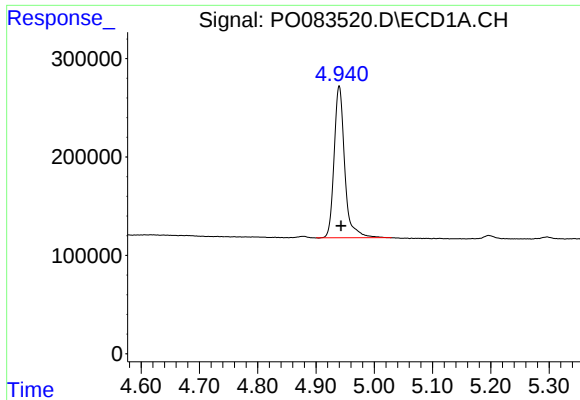

#1 Tetrachloro-m-xylene


R.T.: 4.940 min
Delta R.T.: -0.003 min
Response: 1946836
Conc: 20.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-11S

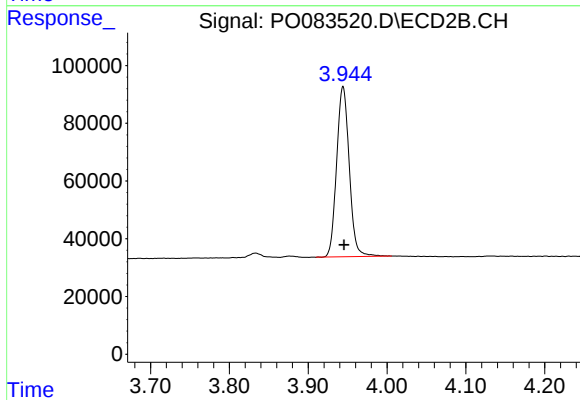


#1 Tetrachloro-m-xylene

R.T.: 3.944 min
Delta R.T.: -0.001 min
Response: 655451
Conc: 21.07 ng/ml

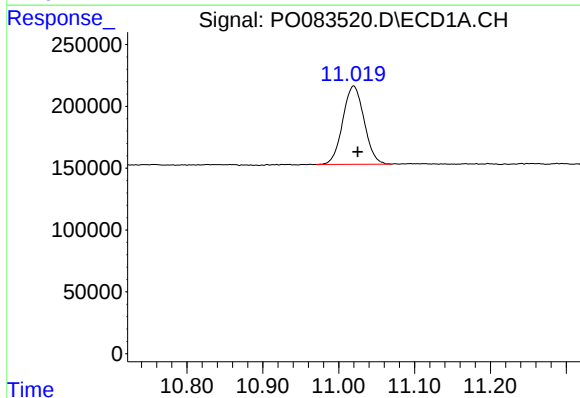

#2 Decachlorobiphenyl

R.T.: 11.020 min
Delta R.T.: -0.006 min
Response: 1238622
Conc: 17.34 ng/ml

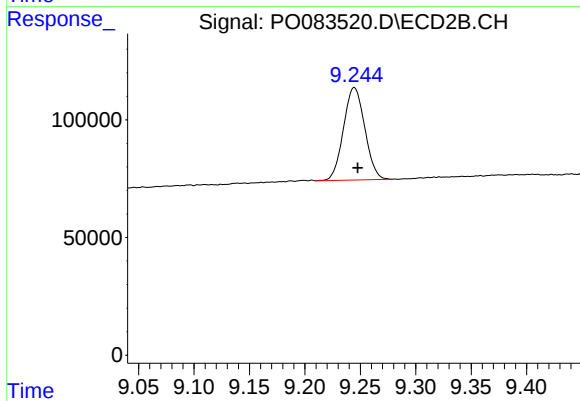

#2 Decachlorobiphenyl

R.T.: 9.245 min
Delta R.T.: -0.003 min
Response: 526804
Conc: 16.15 ng/ml