

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120921\
 Data File : PO083528.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Dec 2021 18:47
 Operator : AJ\MA
 Sample : M4980-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OK-03-120821

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 01:26:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 07 13:18:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.941	3.946	1948779	610212	20.426	19.617
2) SA Decachlor...	11.018	9.245	1514567	471811	21.201	14.462 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120921\
Data File : PO083528.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Dec 2021 18:47
Operator : AJ\MA
Sample : M4980-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
OK-03-120821

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 01:26:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120621.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 07 13:18:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

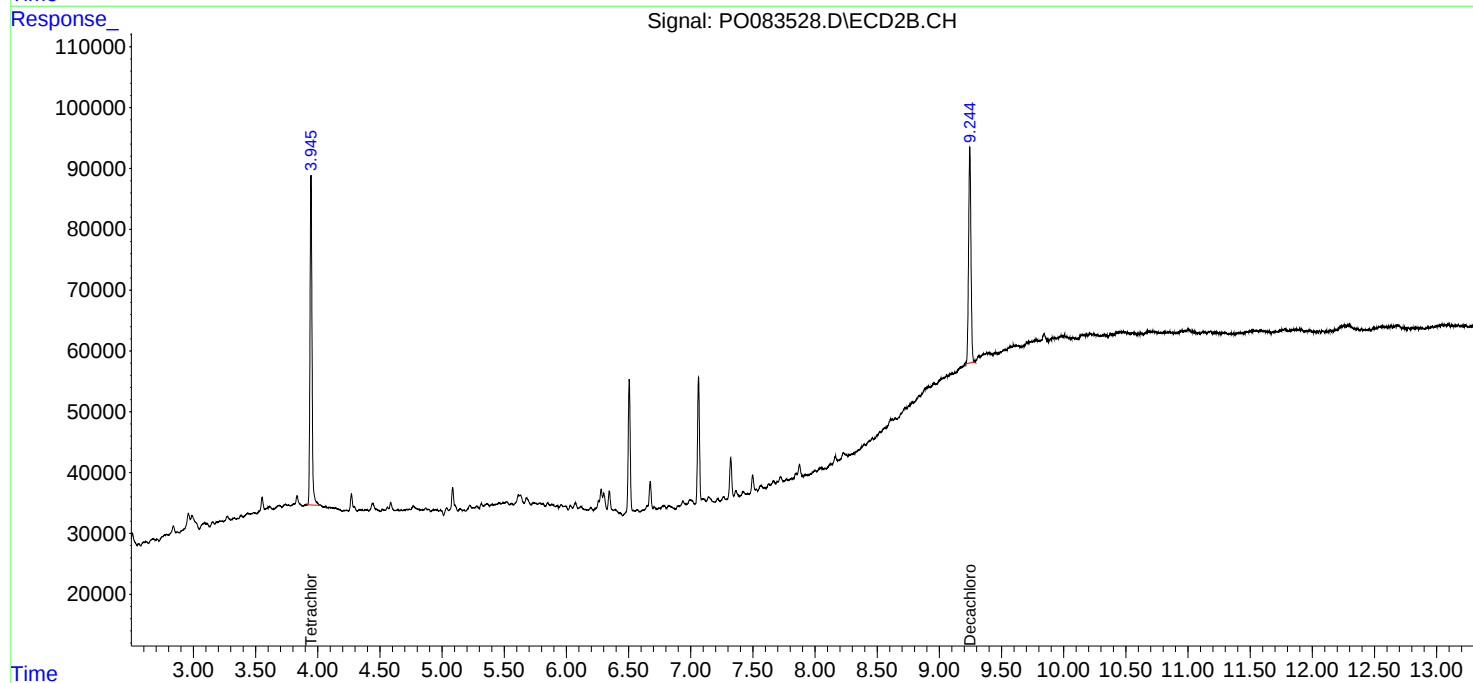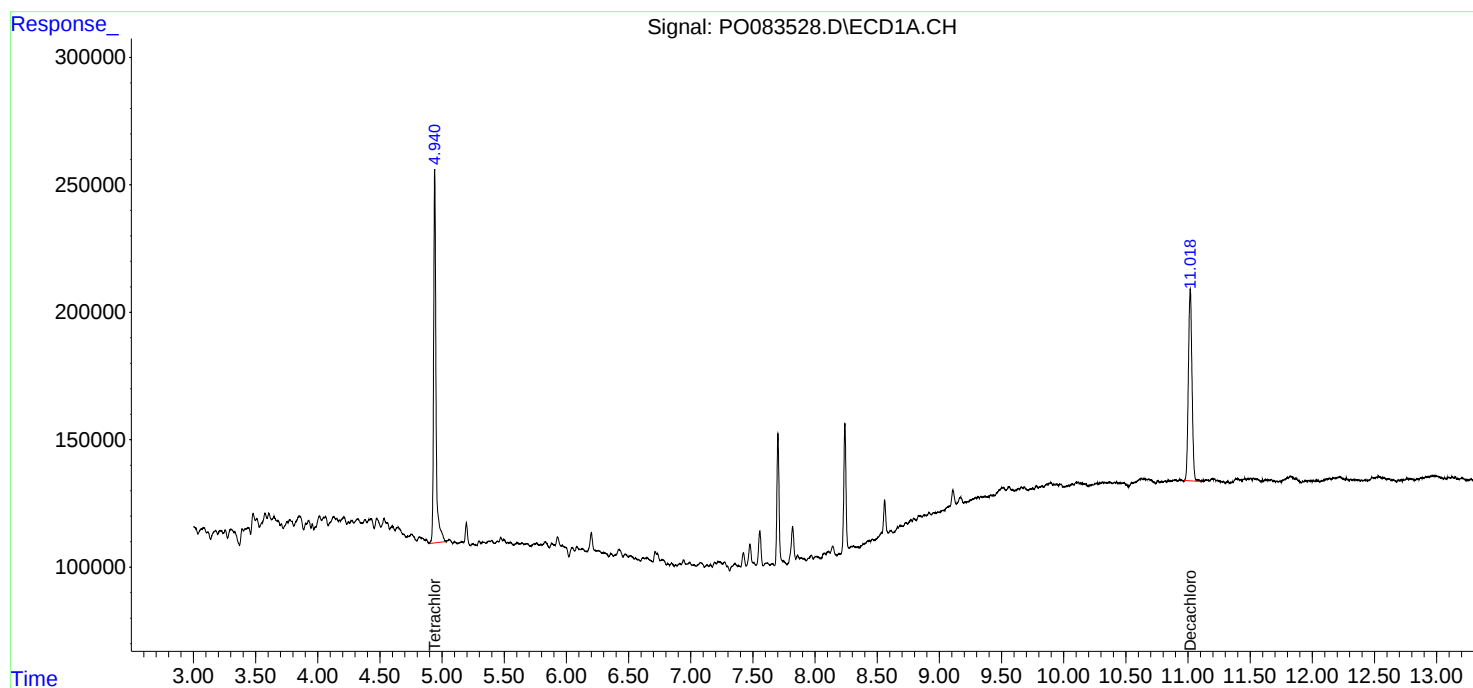


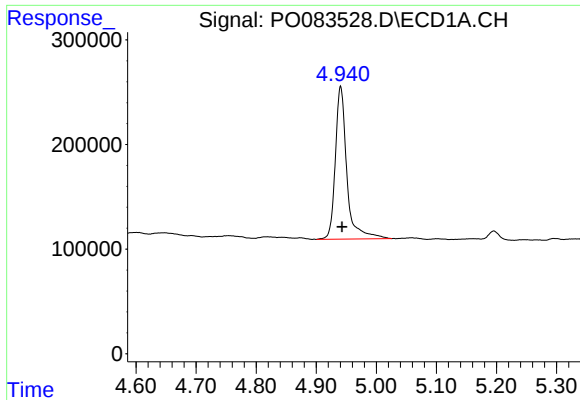

#1 Tetrachloro-m-xylene


R.T.: 4.941 min
Delta R.T.: -0.002 min
Response: 1948779
Conc: 20.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
OK-03-120821

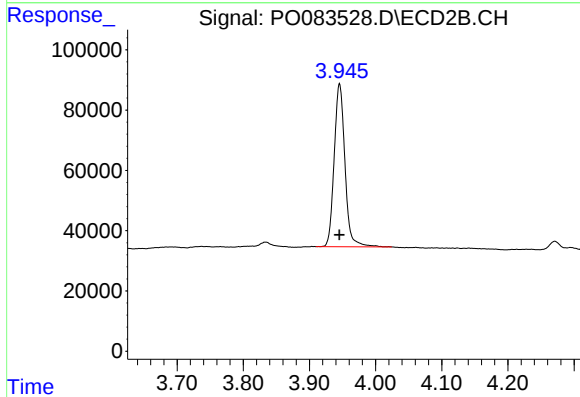


#1 Tetrachloro-m-xylene

R.T.: 3.946 min
Delta R.T.: 0.000 min
Response: 610212
Conc: 19.62 ng/ml

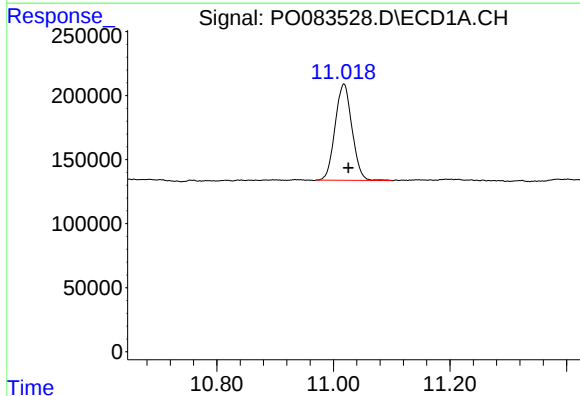

#2 Decachlorobiphenyl

R.T.: 11.018 min
Delta R.T.: -0.007 min
Response: 1514567
Conc: 21.20 ng/ml

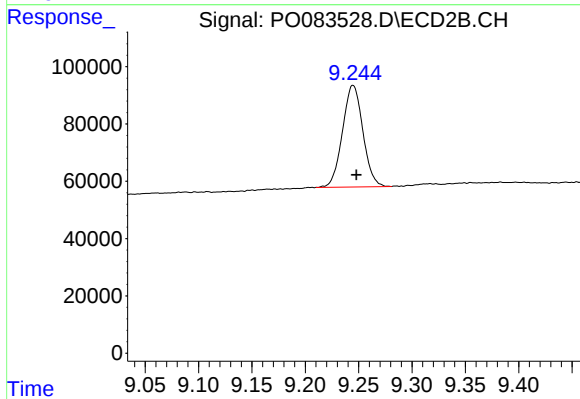

#2 Decachlorobiphenyl

R.T.: 9.245 min
Delta R.T.: -0.003 min
Response: 471811
Conc: 14.46 ng/ml