

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120922\
 Data File : PO091233.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Dec 2022 19:23
 Operator : YP/AJ
 Sample : N5912-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FMC-TOTE-1207

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/12/2022
 Supervised By :Ankita Jodhani 12/12/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 00:07:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112522.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Nov 28 11:25:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.295	3.479	14036250	89394425	4.151m	85.173m#
2) SA Decachlor...	10.044	8.473	7758523	3354817	2.921	3.455m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120922\
Data File : PO091233.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Dec 2022 19:23
Operator : YP/AJ
Sample : N5912-01
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FMC-TOTE-1207


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/12/2022
Supervised By :Ankita Jodhani 12/12/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 00:07:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112522.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Nov 28 11:25:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

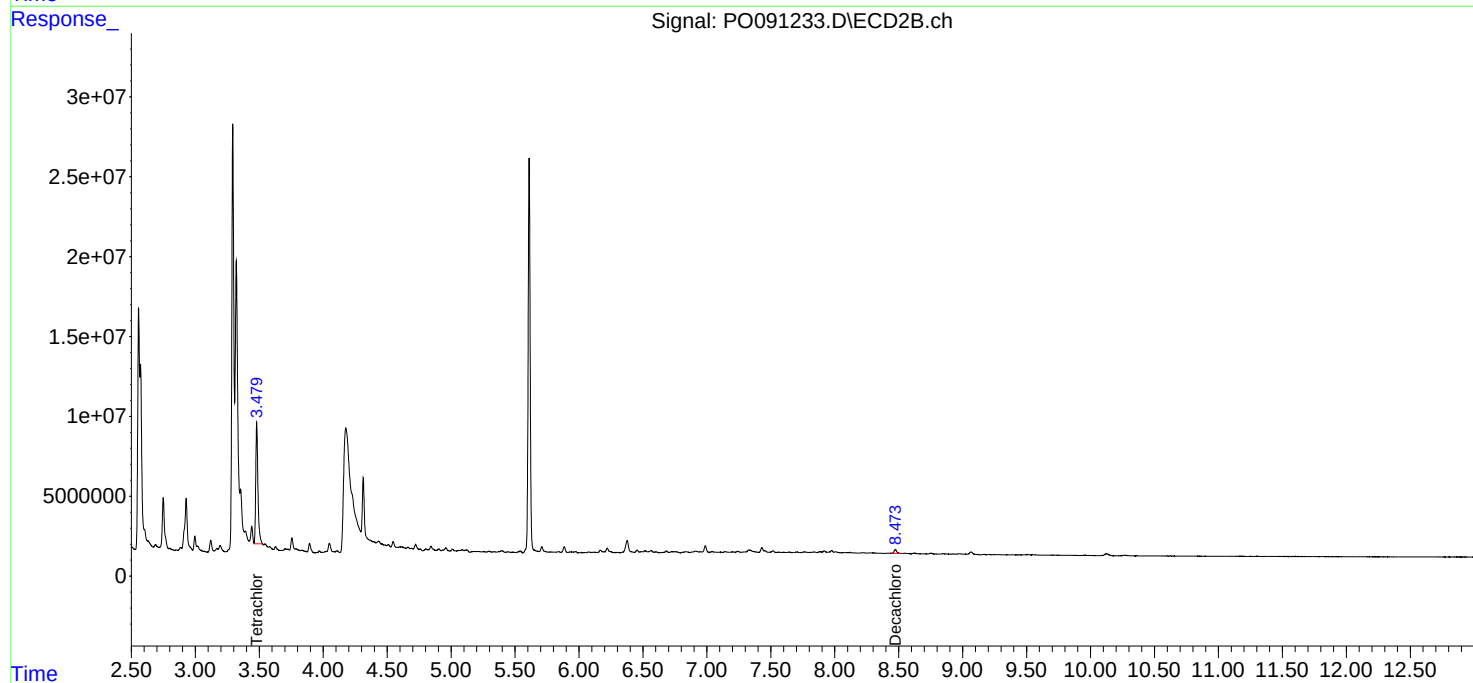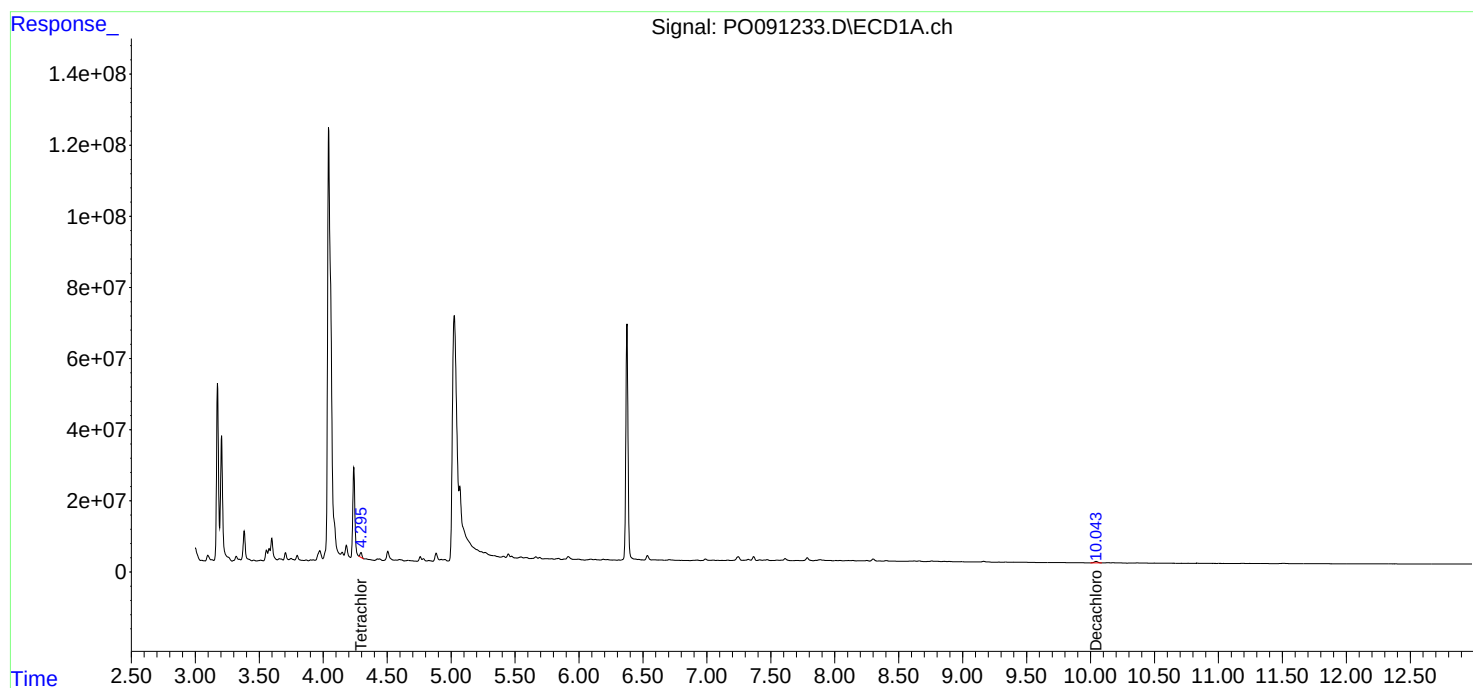

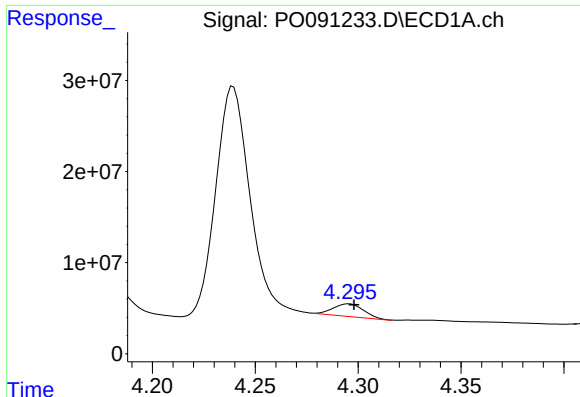


#1 Tetrachloro-m-xylene

R.T.: 4.295 min
Delta R.T.: -0.003 min
Response: 14036250
Conc: 4.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
FMC-TOTE-1207


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/12/2022
Supervised By :Ankita Jodhani 12/12/2022

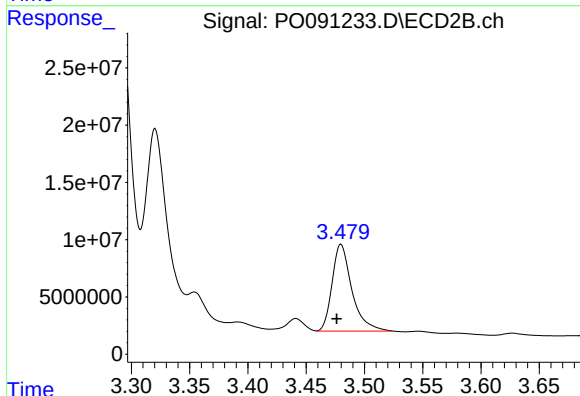


#1 Tetrachloro-m-xylene

R.T.: 3.479 min
Delta R.T.: 0.003 min
Response: 89394425
Conc: 85.17 ng/ml m

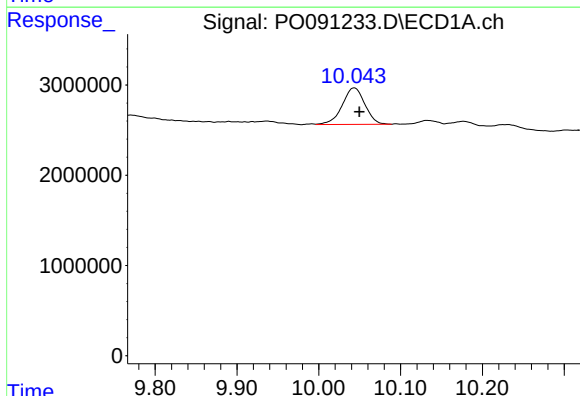

#2 Decachlorobiphenyl

R.T.: 10.044 min
Delta R.T.: -0.006 min
Response: 7758523
Conc: 2.92 ng/ml

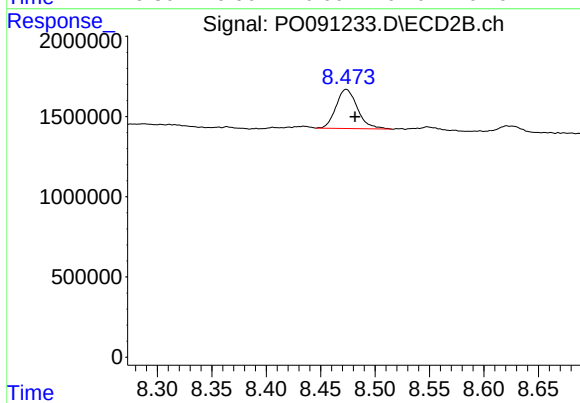

#2 Decachlorobiphenyl

R.T.: 8.473 min
Delta R.T.: -0.009 min
Response: 3354817
Conc: 3.46 ng/ml m