

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120924\
 Data File : PO108406.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Dec 2024 13:13
 Operator : YP/AJ
 Sample : P5174-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ROLL-OFF-COMP

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/10/2024
 Supervised By :Ankita Jodhani 12/10/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 01:35:59 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 05:58:15 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.709	3.708	95868068	55802900	11.019m	11.008m
2) SA Decachlor...	8.786	8.737	106.3E6	60778218	14.557m	15.685m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120924\
Data File : PO108406.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Dec 2024 13:13
Operator : YP/AJ
Sample : P5174-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
ROLL-OFF-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/10/2024
Supervised By :Ankita Jodhani 12/10/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 01:35:59 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 05:58:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

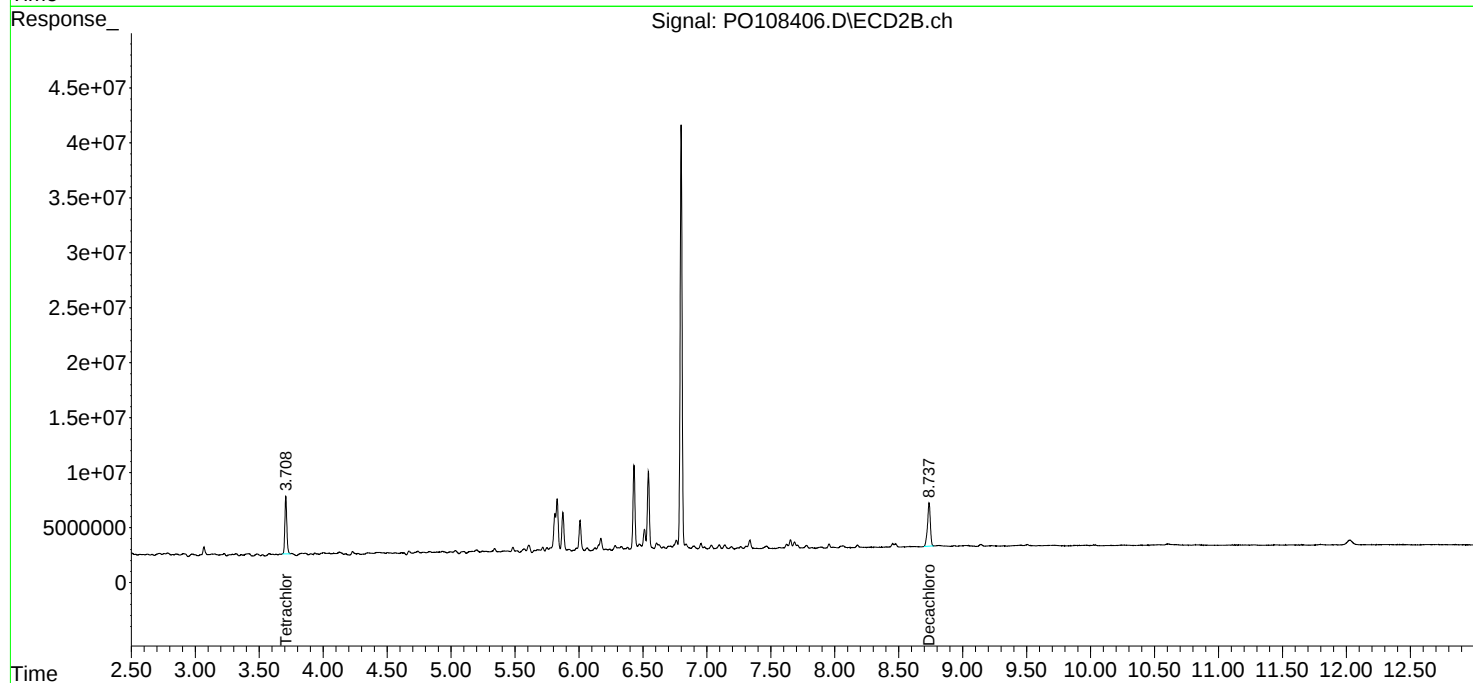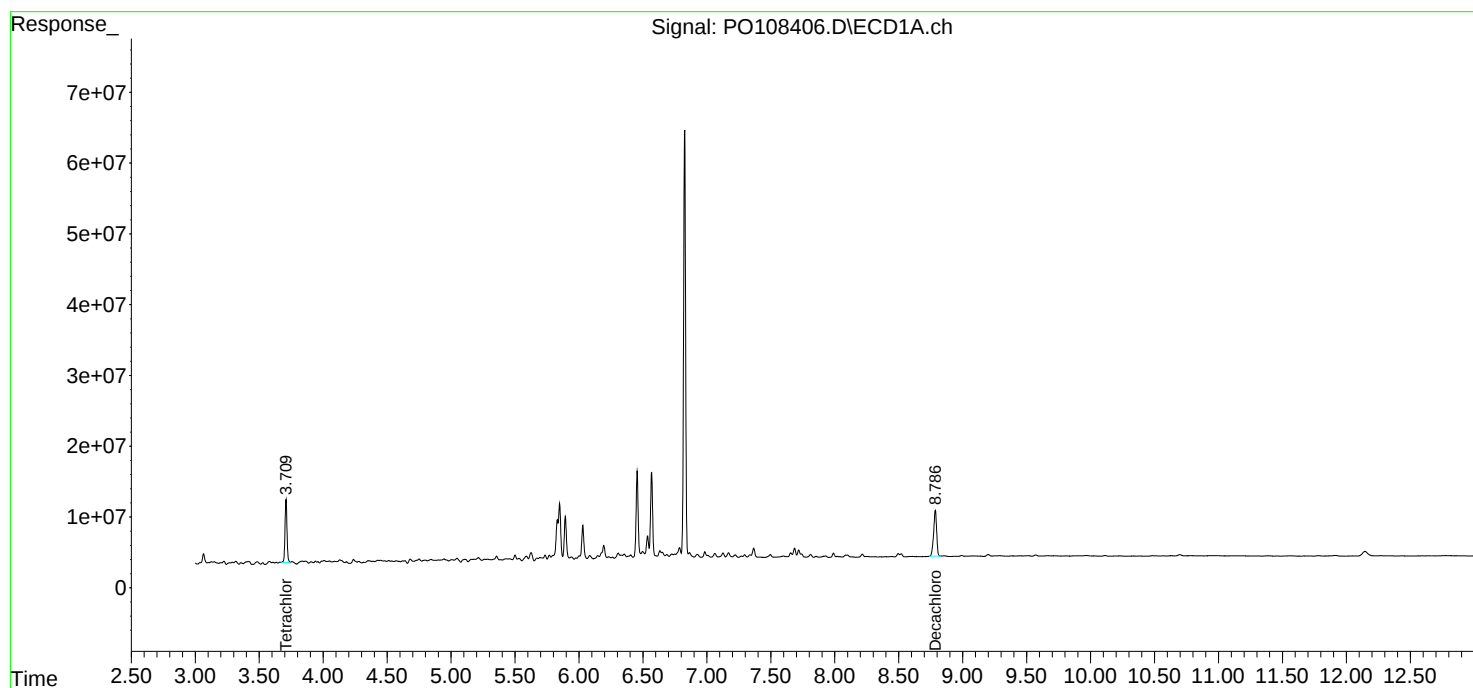

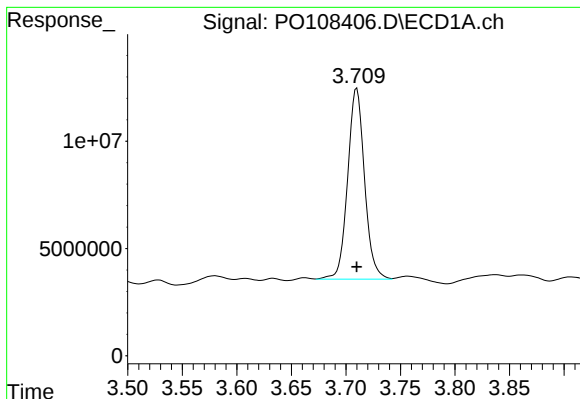


#1 Tetrachloro-m-xylene

R.T.: 3.709 min
Delta R.T.: 0.000 min
Response: 95868068
Conc: 11.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
ROLL-OFF-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/10/2024
Supervised By :Ankita Jodhani 12/10/2024

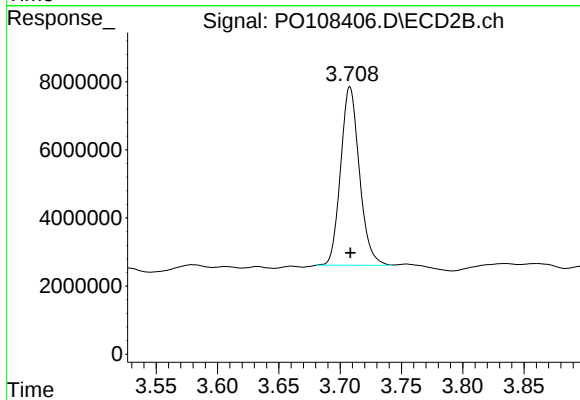


#1 Tetrachloro-m-xylene

R.T.: 3.708 min
Delta R.T.: 0.000 min
Response: 55802900
Conc: 11.01 ng/ml m

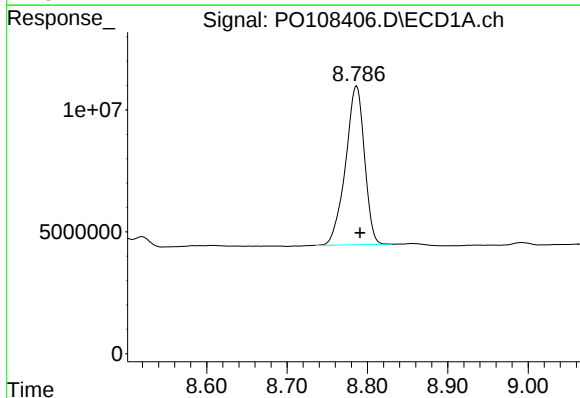

#2 Decachlorobiphenyl

R.T.: 8.786 min
Delta R.T.: -0.005 min
Response: 106327578
Conc: 14.56 ng/ml m

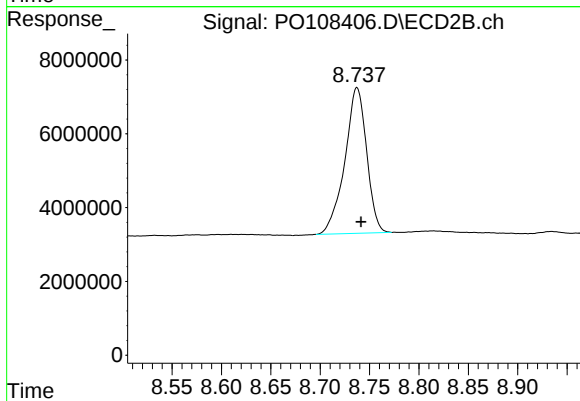

#2 Decachlorobiphenyl

R.T.: 8.737 min
Delta R.T.: -0.005 min
Response: 60778218
Conc: 15.69 ng/ml m