

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121020\
 Data File : PO073608.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Dec 2020 14:29
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 04:00:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 11 03:58:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
24)	L5	AR-1248-4	7.179f	0.000	8066	0	2.017 N.D. #
26)	L6	AR-1254-1	7.179	0.000	8066	0	2.125 N.D. #
28)	L6	AR-1254-3	7.809f	0.000	41373	0	6.752 N.D. #
33)	L7	AR-1260-3	8.589	0.000	4825	0	1.056 N.D. #
36)	L8	AR-1262-1	8.589	0.000	4825	0	0.645 N.D. #
38)	L8	AR-1262-3	9.456	0.000	8494	0	1.001 N.D. #
39)	L8	AR-1262-4	9.530f	0.000	3508	0	1.049 N.D. #
41)	L9	AR-1268-1	9.456	0.000	8494	0	0.596 N.D. #
42)	L9	AR-1268-2	9.530f	0.000	3508	0	0.285 N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121020\
Data File : PO073608.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Dec 2020 14:29
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 04:00:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 11 03:58:06 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

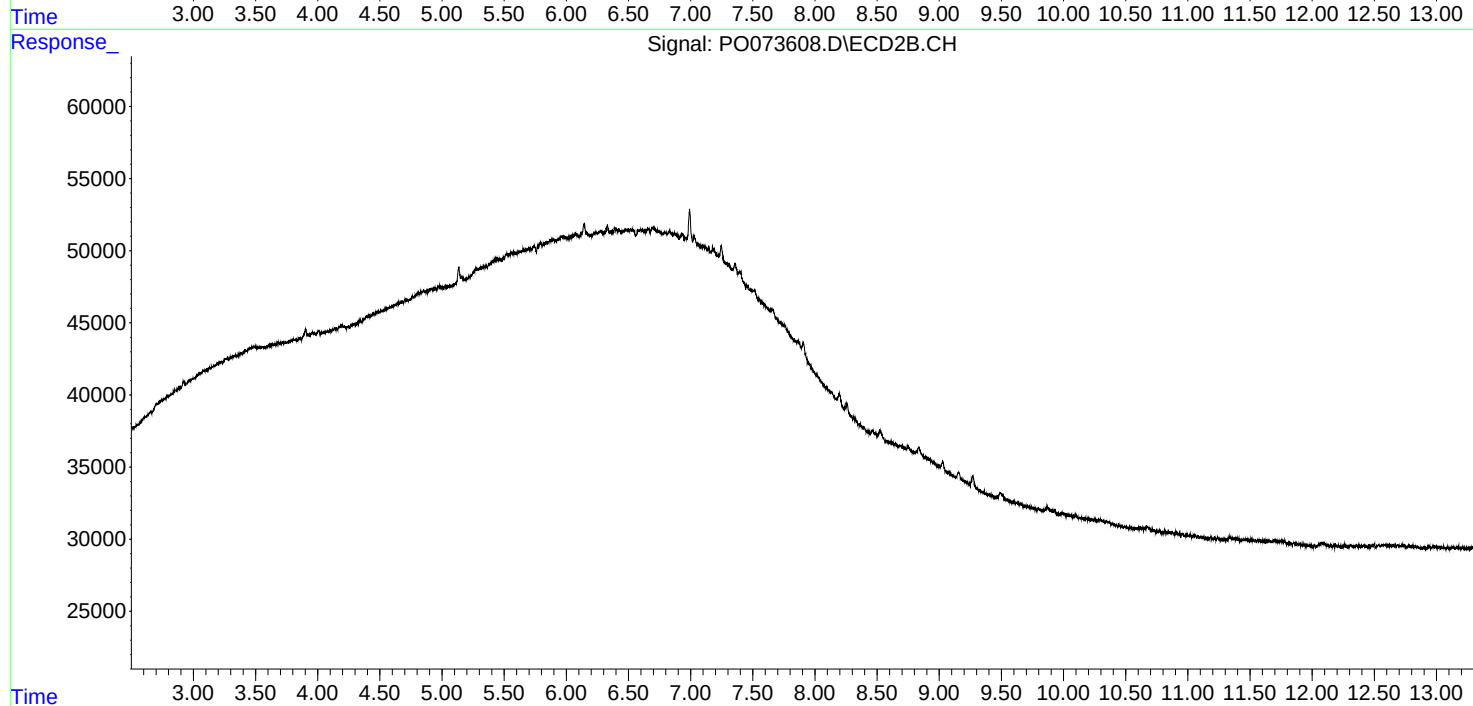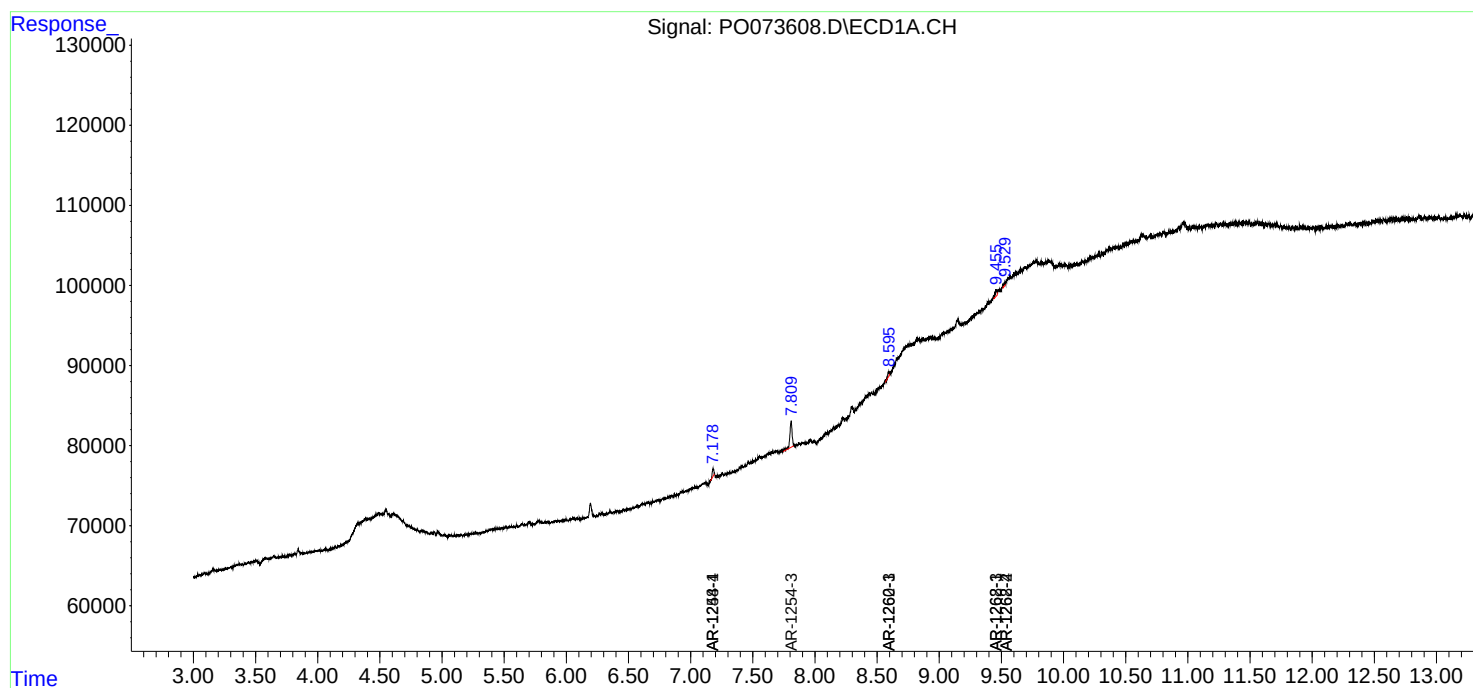


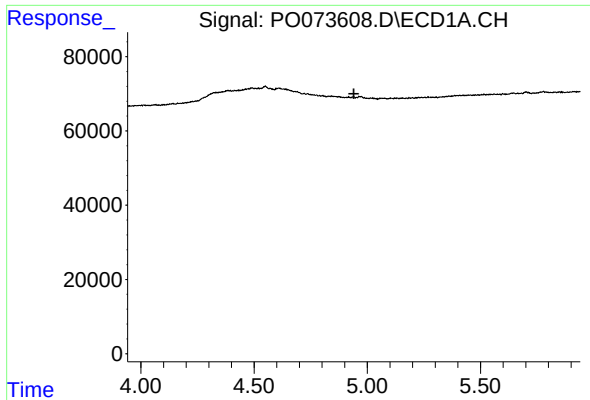

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.941 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
HEXANE

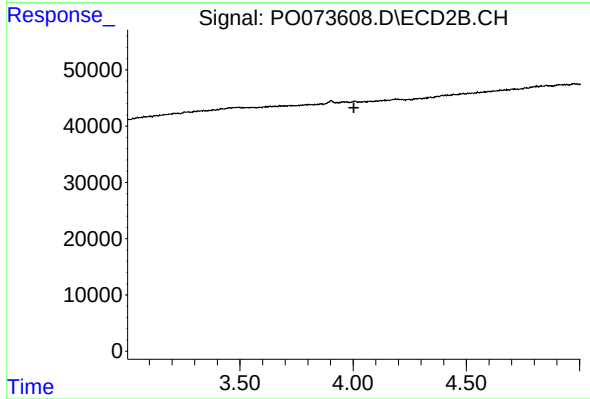


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.003 min
Response: 0
Conc: N.D.

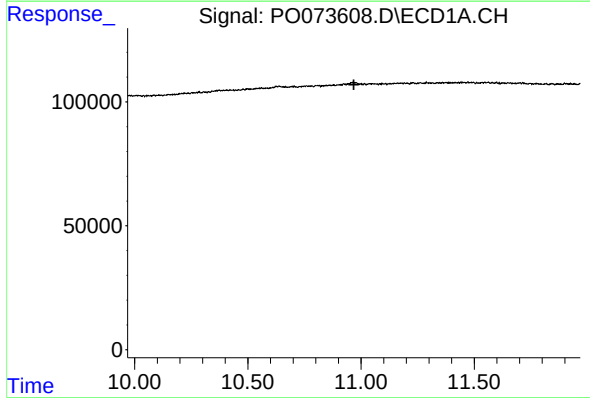


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.968 min
Response: 0
Conc: N.D.

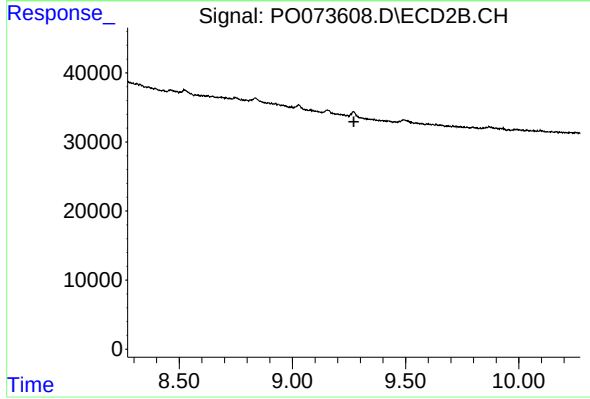

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 9.272 min
Response: 0
Conc: N.D.

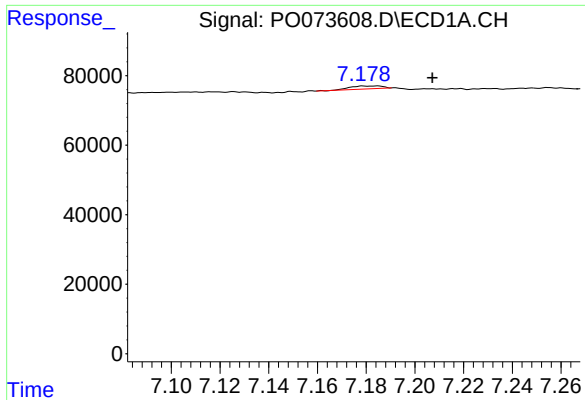

#24 AR-1248-4


R.T.: 7.179 min
Delta R.T.: -0.029 min
Response: 8066
Conc: 2.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
HEXANE

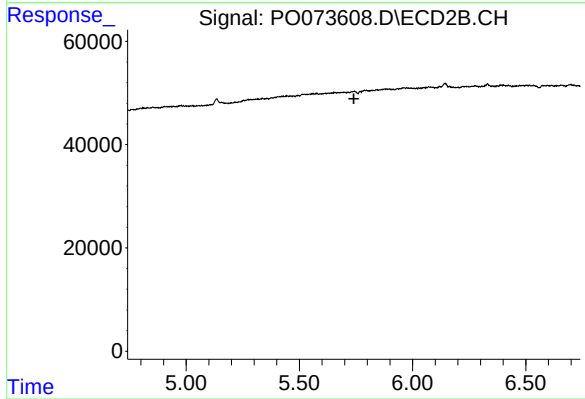


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.741 min
Response: 0
Conc: N.D.

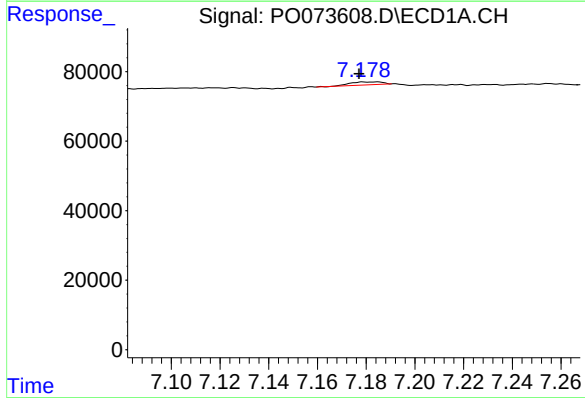


#26 AR-1254-1

R.T.: 7.179 min
Delta R.T.: 0.002 min
Response: 8066
Conc: 2.12 ng/ml

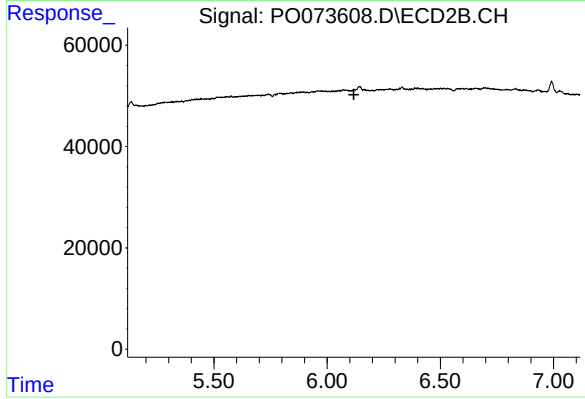

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 6.118 min
Response: 0
Conc: N.D.

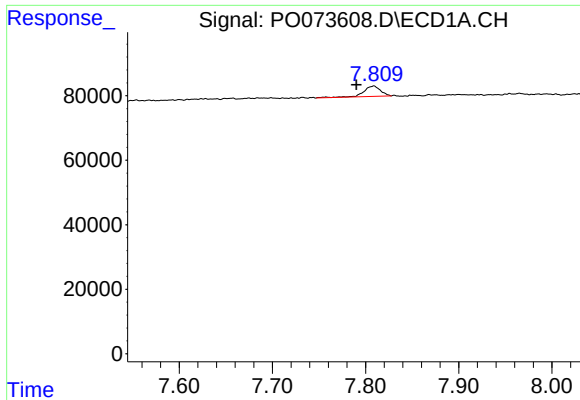

#28 AR-1254-3


R.T.: 7.809 min
Delta R.T.: 0.019 min
Response: 41373
Conc: 6.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
HEXANE

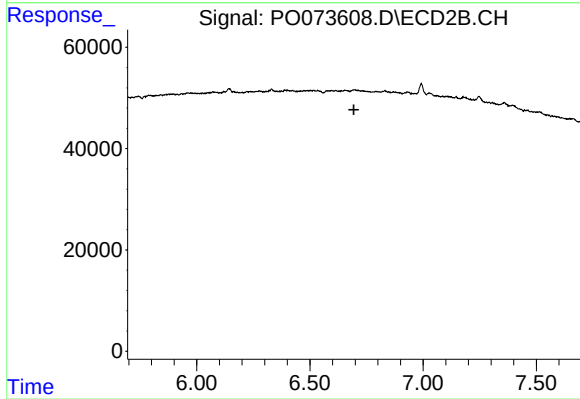


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.694 min
Response: 0
Conc: N.D.

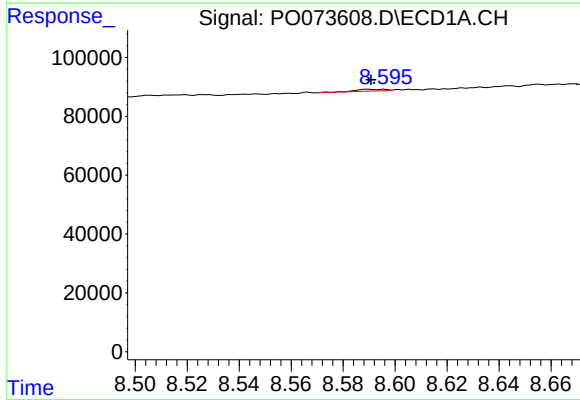


#33 AR-1260-3

R.T.: 8.589 min
Delta R.T.: -0.001 min
Response: 4825
Conc: 1.06 ng/ml

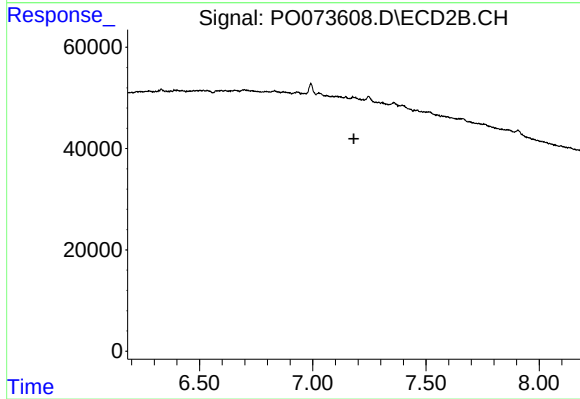

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T. : 7.182 min
Response: 0
Conc: N.D.

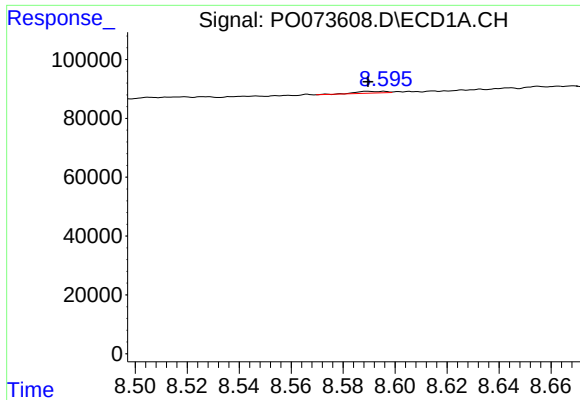

#36 AR-1262-1


R.T.: 8.589 min
Delta R.T.: 0.000 min
Response: 4825
Conc: 0.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
HEXANE

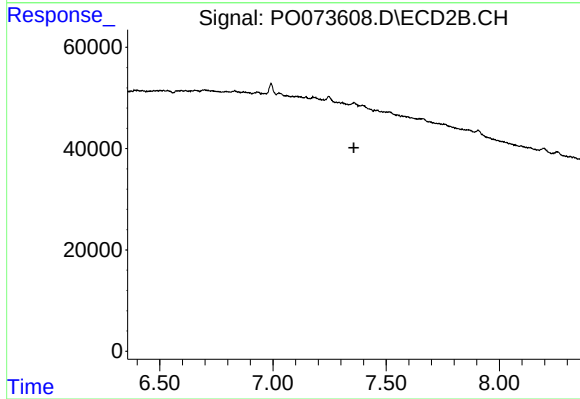


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.357 min
Response: 0
Conc: N.D.

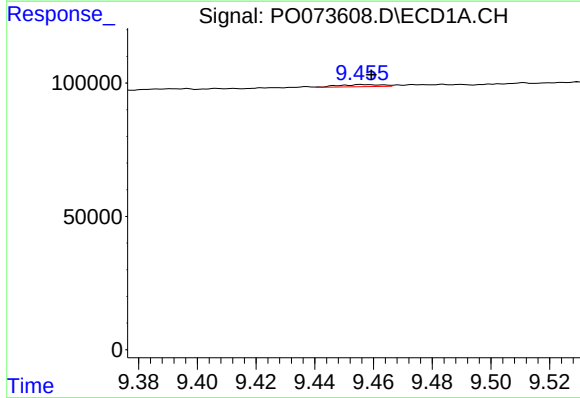


#38 AR-1262-3

R.T.: 9.456 min
Delta R.T.: -0.004 min
Response: 8494
Conc: 1.00 ng/ml

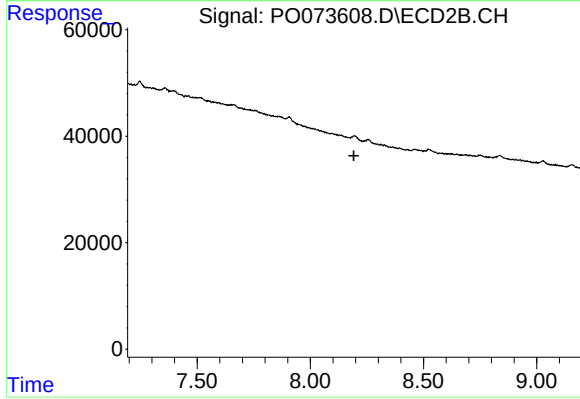

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 8.192 min
Response: 0
Conc: N.D.

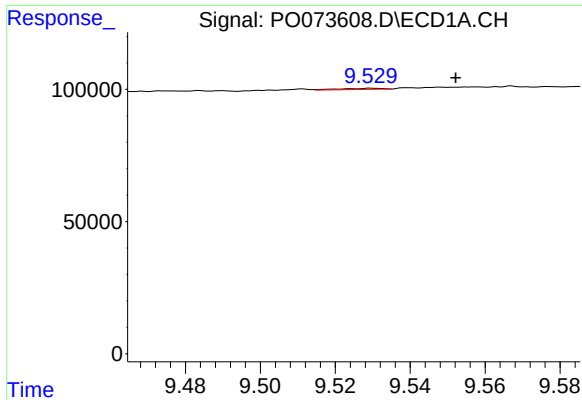

#39 AR-1262-4


R.T.: 9.530 min
Delta R.T.: -0.023 min
Response: 3508
Conc: 1.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
HEXANE

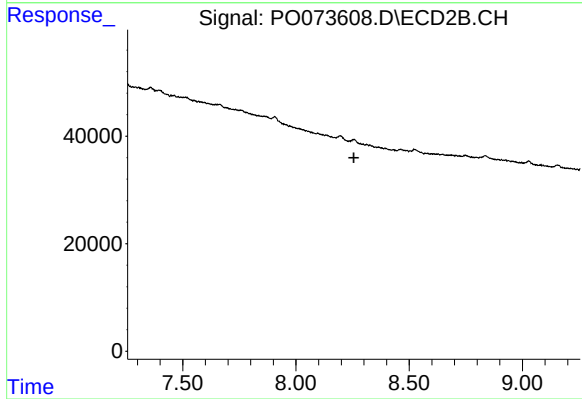


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 8.256 min
Response: 0
Conc: N.D.

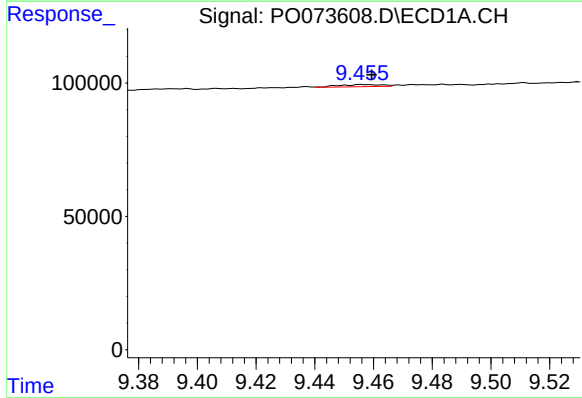


#41 AR-1268-1

R.T.: 9.456 min
Delta R.T.: -0.004 min
Response: 8494
Conc: 0.60 ng/ml

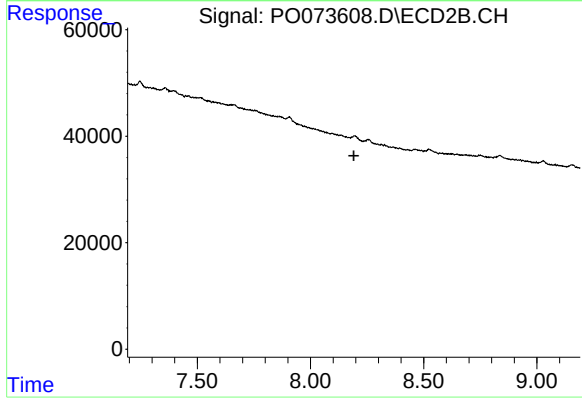

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T. : 8.192 min
Response: 0
Conc: N.D.

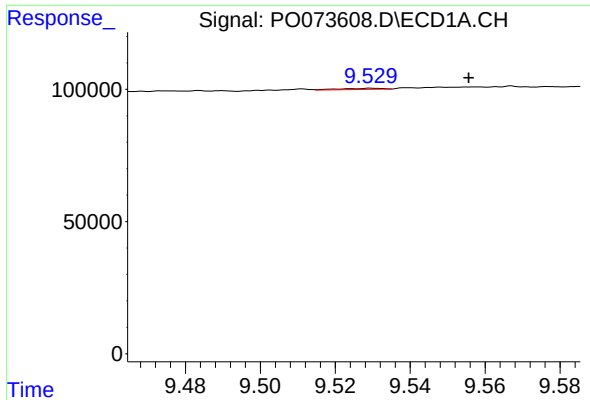

#42 AR-1268-2

R.T.: 9.530 min
Delta R.T.: -0.026 min
Response: 3508
Conc: 0.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
HEXANE

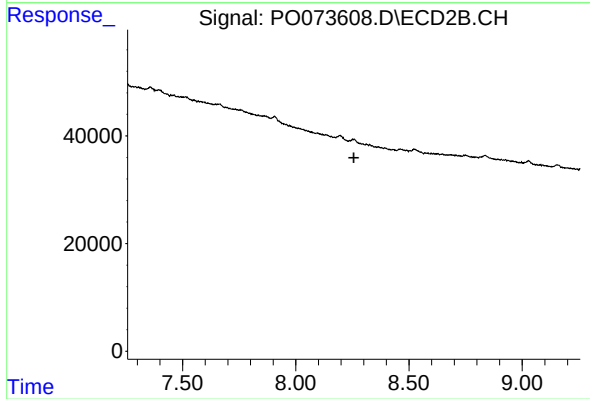

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 8.257 min
Response: 0
Conc: N.D.