

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121021\
 Data File : PO083562.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Dec 2021 20:27
 Operator : AJ\MA
 Sample : M4992-06
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SIMW-04-20211208

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 01:40:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 07 13:18:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.941	3.945	1717079	576039	17.998	18.519
2)	SA Decachlor...	11.020	9.245	1498367	581008	20.975	17.809

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121021\
Data File : P0083562.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Dec 2021 20:27
Operator : AJ\MA
Sample : M4992-06
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SIMW-04-20211208

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 01:40:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120621.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 07 13:18:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

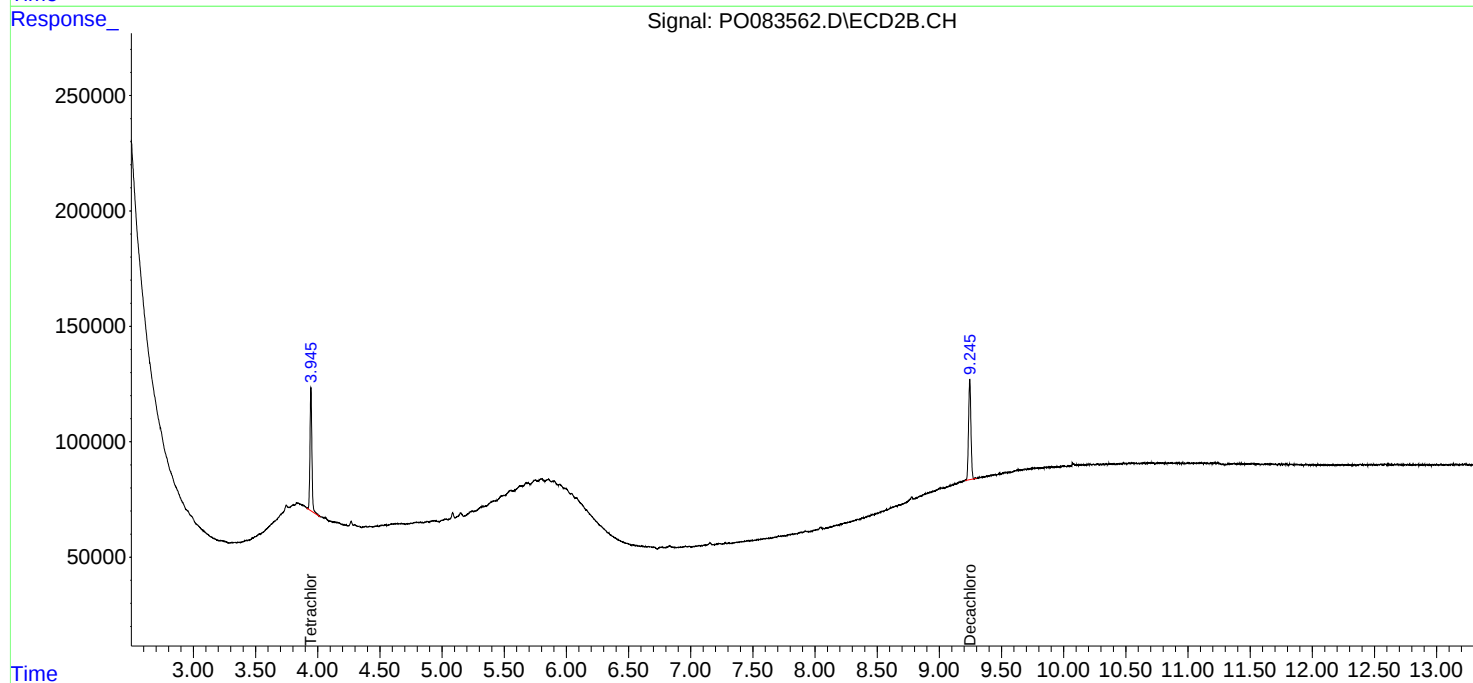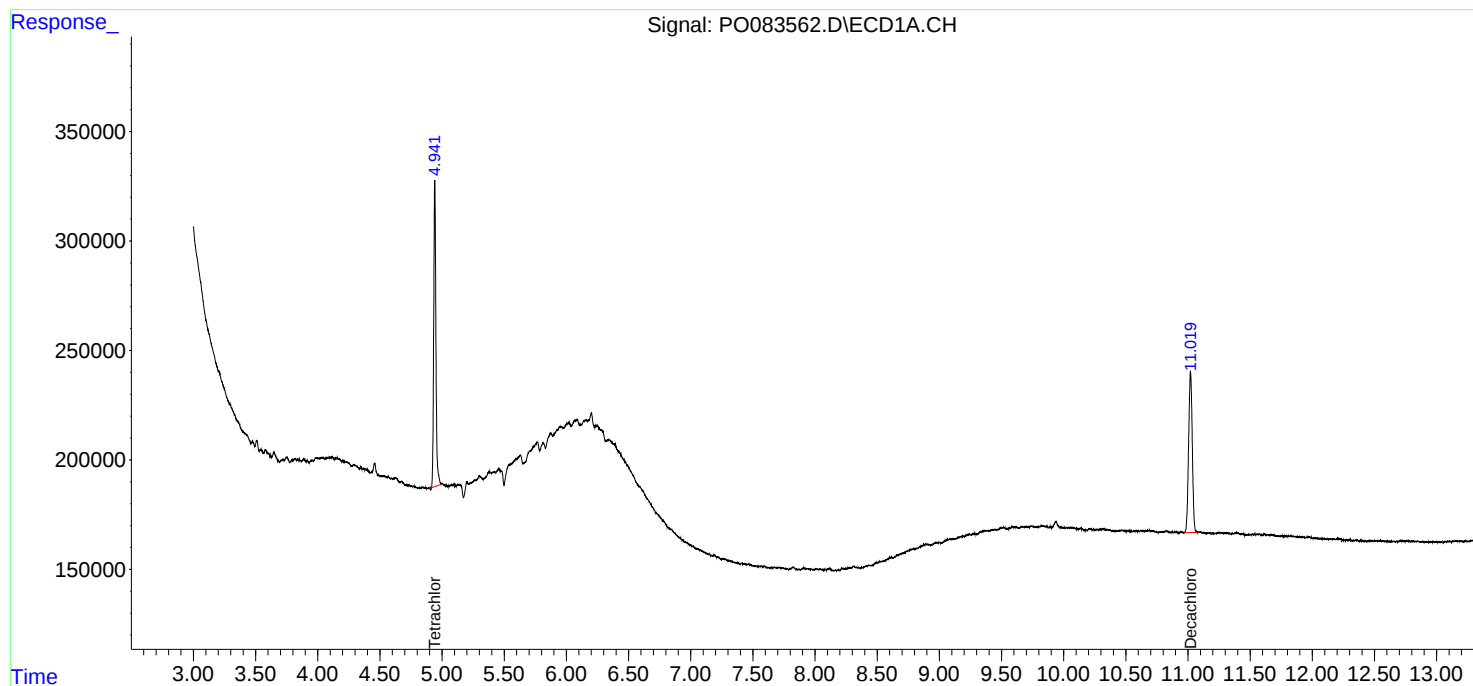


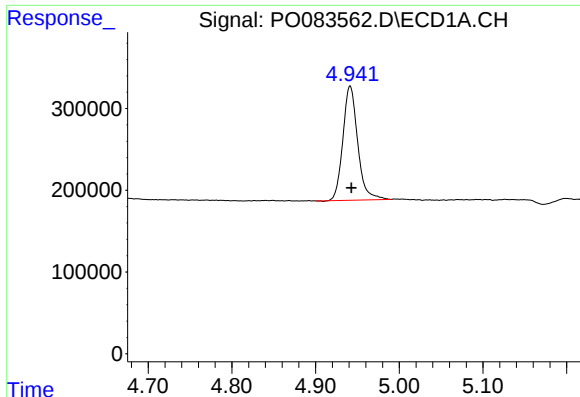

#1 Tetrachloro-m-xylene


R.T.: 4.941 min
Delta R.T.: -0.002 min
Response: 1717079
Conc: 18.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
SIMW-04-20211208

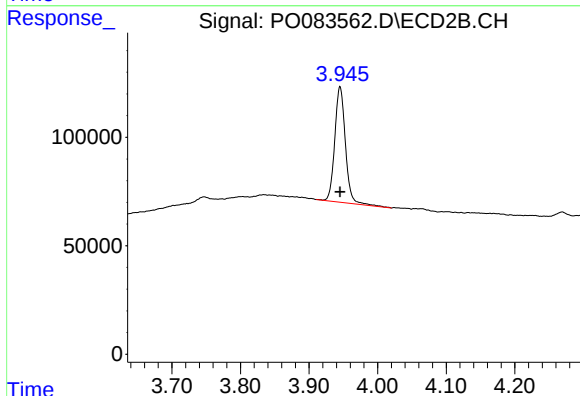


#1 Tetrachloro-m-xylene

R.T.: 3.945 min
Delta R.T.: 0.000 min
Response: 576039
Conc: 18.52 ng/ml

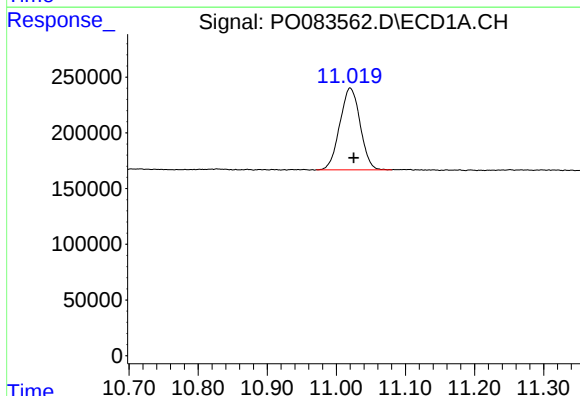

#2 Decachlorobiphenyl

R.T.: 11.020 min
Delta R.T.: -0.005 min
Response: 1498367
Conc: 20.97 ng/ml

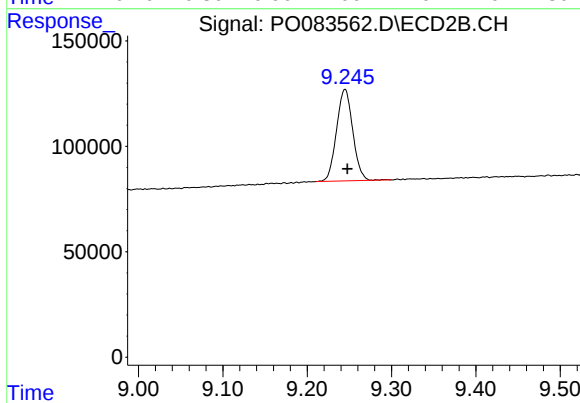

#2 Decachlorobiphenyl

R.T.: 9.245 min
Delta R.T.: -0.003 min
Response: 581008
Conc: 17.81 ng/ml