

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0121024\
 Data File : P0108456.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Dec 2024 19:14
 Operator : YP/AJ
 Sample : P5223-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TR-05-120924

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/11/2024
 Supervised By :Ankita Jodhani 12/11/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 00:36:02 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 05:58:15 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.708	3.706	99823315	65227136	11.474m	12.867
2) SA Decachlor...	8.783	8.732	90263848	57440301	12.358	14.824

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121024\
Data File : PO108456.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Dec 2024 19:14
Operator : YP/AJ
Sample : P5223-01
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TR-05-120924


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/11/2024
Supervised By :Ankita Jodhani 12/11/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 00:36:02 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 05:58:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

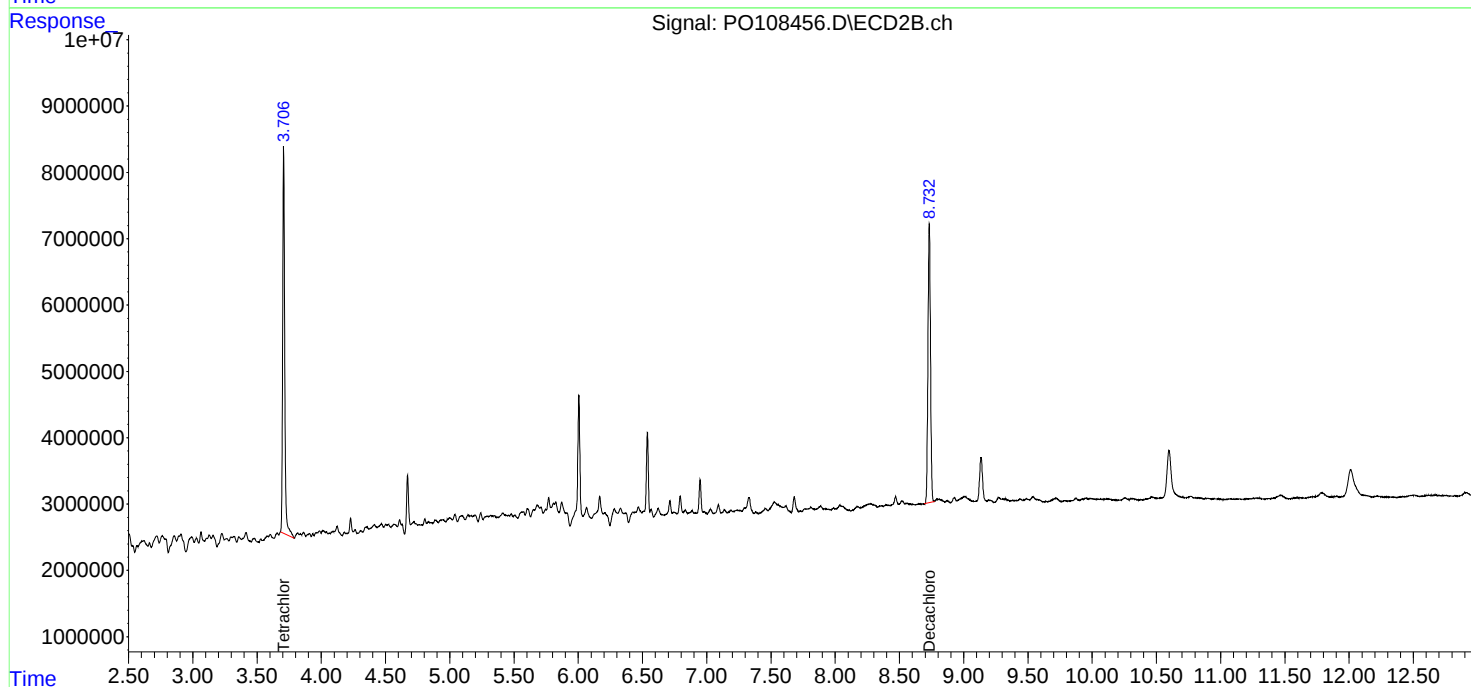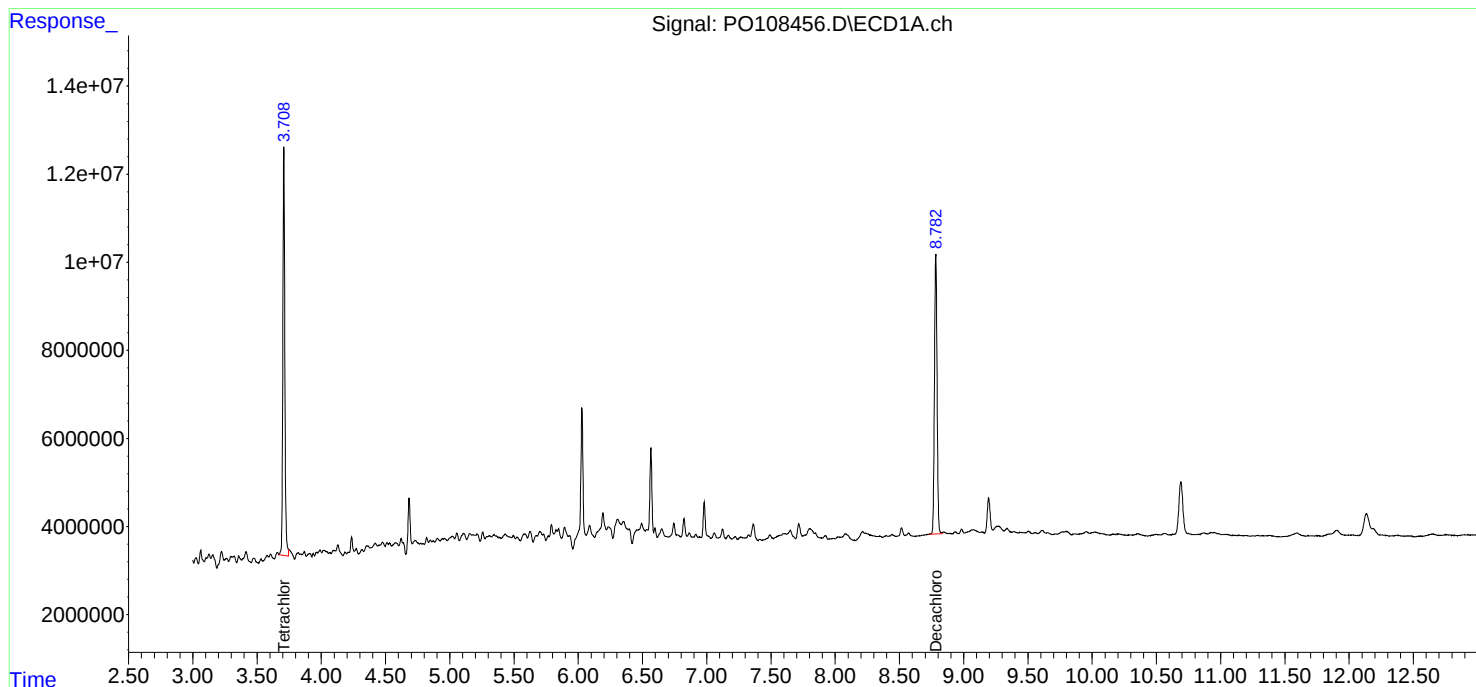

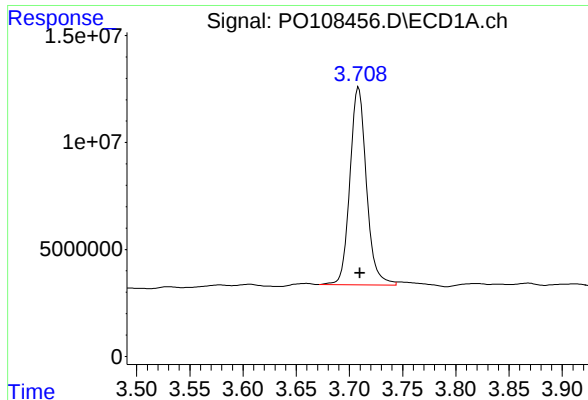


#1 Tetrachloro-m-xylene

R.T.: 3.708 min
Delta R.T.: -0.002 min
Response: 99823315
Conc: 11.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
TR-05-120924


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/11/2024
Supervised By :Ankita Jodhani 12/11/2024

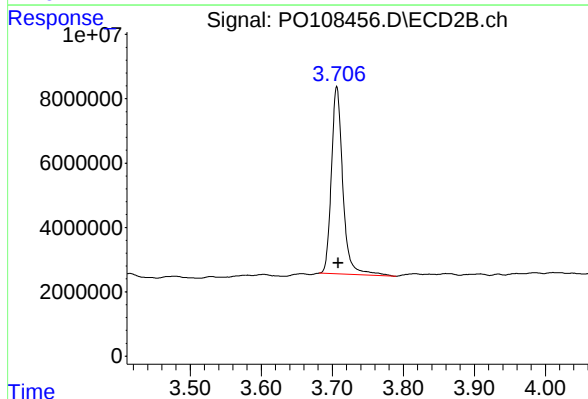


#1 Tetrachloro-m-xylene

R.T.: 3.706 min
Delta R.T.: -0.002 min
Response: 65227136
Conc: 12.87 ng/ml

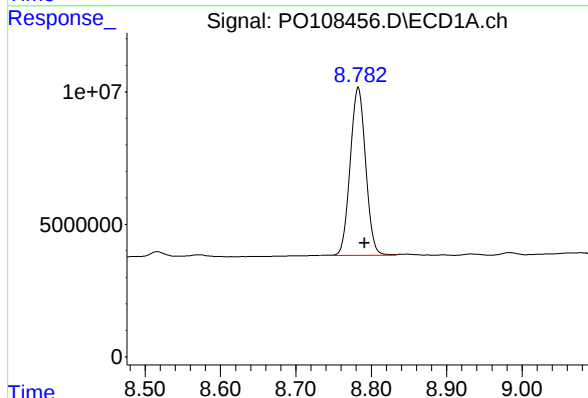

#2 Decachlorobiphenyl

R.T.: 8.783 min
Delta R.T.: -0.008 min
Response: 90263848
Conc: 12.36 ng/ml

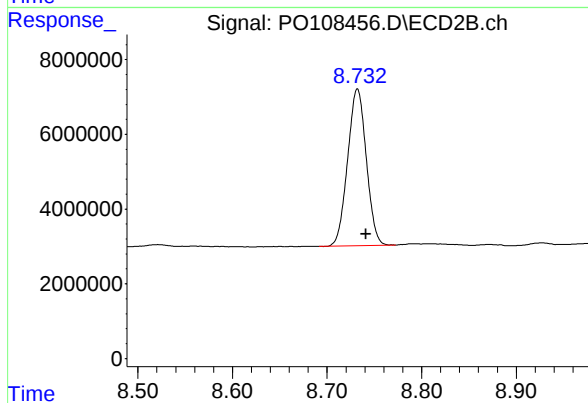

#2 Decachlorobiphenyl

R.T.: 8.732 min
Delta R.T.: -0.009 min
Response: 57440301
Conc: 14.82 ng/ml