

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121025\
 Data File : PO115701.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Dec 2025 13:22
 Operator : YP/AJ
 Sample : Q3812-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OR-02-120825

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 12/11/2025
 Supervised By :Yogesh Patel 12/11/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 00:46:23 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 05 02:11:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.335	3.637	141.3E6	106.7E6	18.189m	21.901
2) SA Decachlor...	9.917	8.623	107.7E6	74299332	20.474	17.278

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121025\
Data File : PO115701.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Dec 2025 13:22
Operator : YP/AJ
Sample : Q3812-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OR-02-120825


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 12/11/2025
Supervised By :Yogesh Patel 12/11/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 00:46:23 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120425.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 05 02:11:05 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

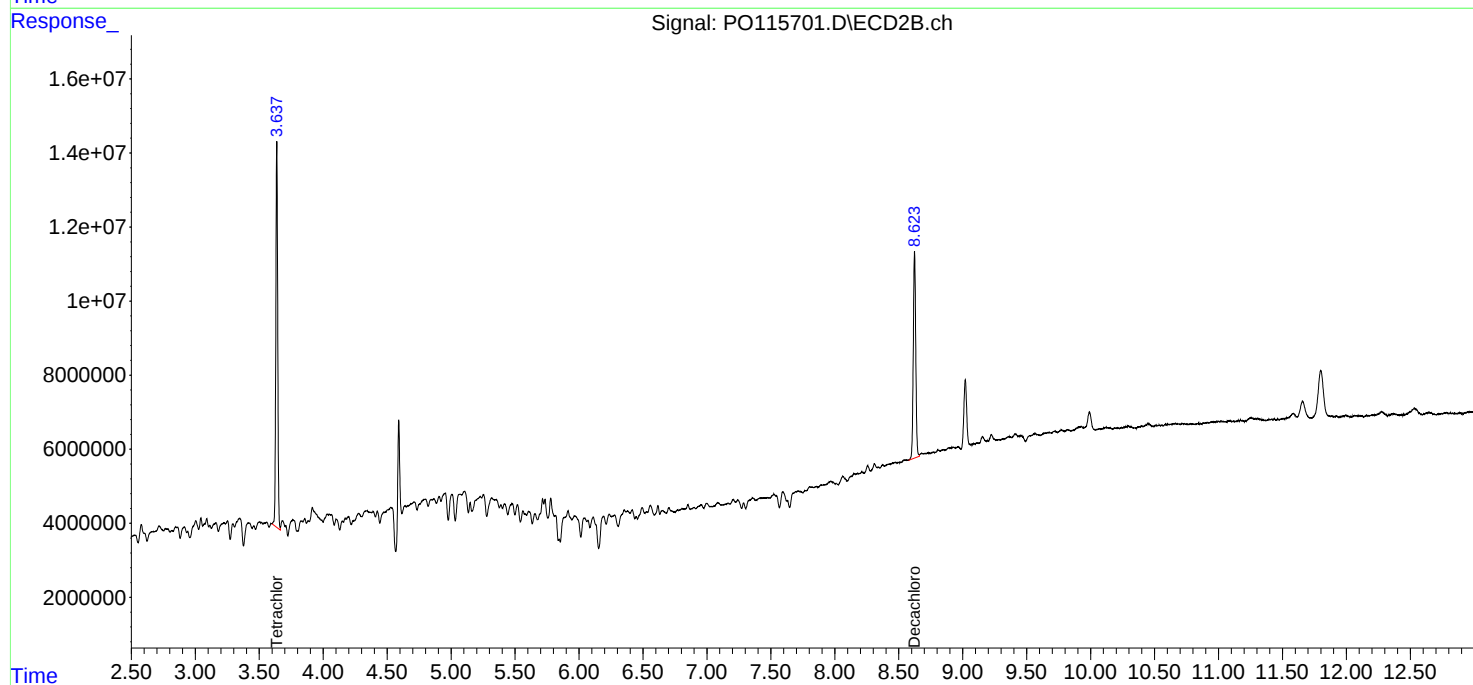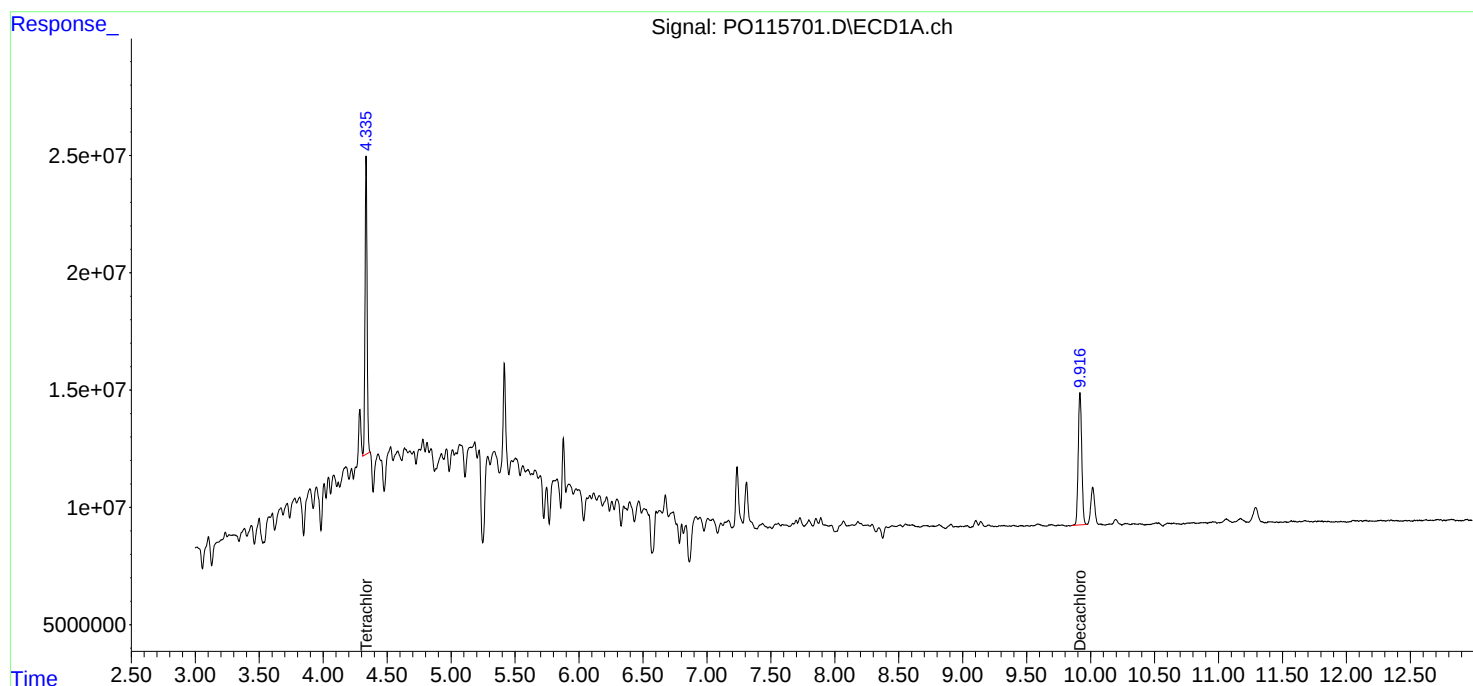

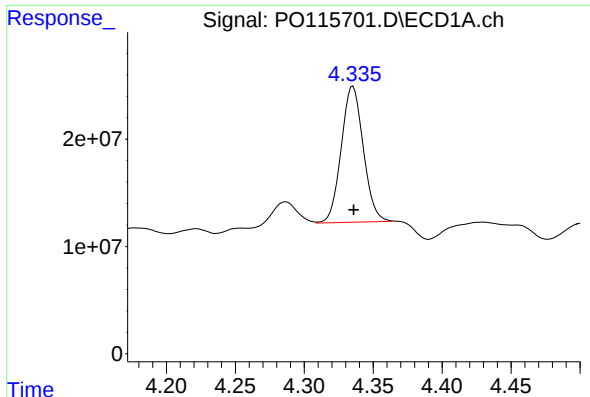

#1 Tetrachloro-m-xylene

R.T.: 4.335 min
Delta R.T.: -0.001 min
Response: 141280132
Conc: 18.19 ng/ml

Instrument :

ECD_O


ClientSampleId :

OR-02-120825

Manual Integrations


APPROVED

Reviewed By :Rahul Chavli 12/11/2025
Supervised By :Yogesh Patel 12/11/2025

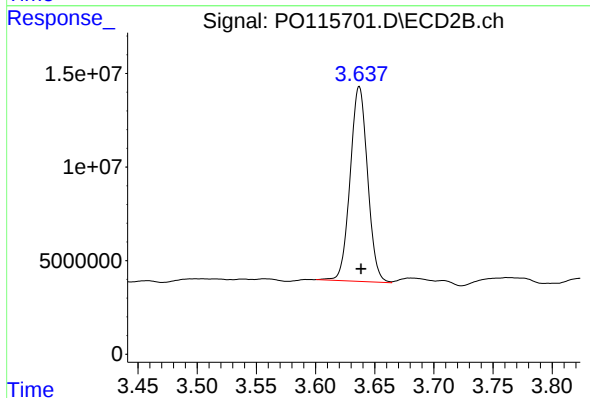


#1 Tetrachloro-m-xylene

R.T.: 3.637 min
Delta R.T.: -0.001 min
Response: 106733299
Conc: 21.90 ng/ml

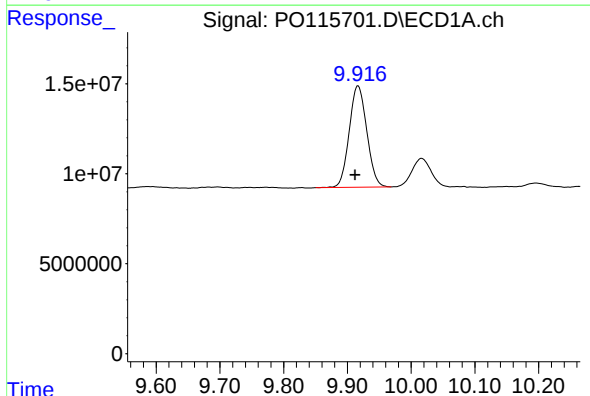

#2 Decachlorobiphenyl

R.T.: 9.917 min
Delta R.T.: 0.005 min
Response: 107715277
Conc: 20.47 ng/ml

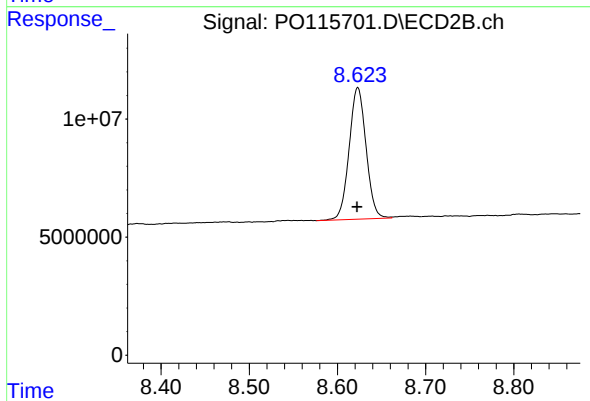

#2 Decachlorobiphenyl

R.T.: 8.623 min
Delta R.T.: 0.001 min
Response: 74299332
Conc: 17.28 ng/ml