

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0121120\
 Data File : P0073702.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Dec 2020 00:32
 Operator : DD\AJ
 Sample : L5033-05
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CS-47

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 01:29:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0121020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 11 03:58:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.938	4.000	1890649	1149153	20.679	21.425
2) SA Decachlor...	10.963	9.266	1779008	1075370	21.527	22.983
Target Compounds						
9) L2 AR-1221-2	5.291	0.000	24610	0	31.330	N.D. #
27) L6 AR-1254-2	7.416	0.000	108305	0	18.370	N.D. #
28) L6 AR-1254-3	7.808f	0.000	21209	0	3.462	N.D. #
32) L7 AR-1260-2	8.243f	0.000	44547	0	7.930	N.D. #
33) L7 AR-1260-3	8.619f	0.000	7491	0	1.639	N.D. #
36) L8 AR-1262-1	8.619f	0.000	7491	0	1.001	N.D. #
39) L8 AR-1262-4	9.530f	0.000	38928	0	11.639	N.D. #
42) L9 AR-1268-2	9.530f	0.000	38928	0	3.158	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121120\
Data File : P0073702.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Dec 2020 00:32
Operator : DD\AJ
Sample : L5033-05
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
CS-47

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 01:29:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 11 03:58:06 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

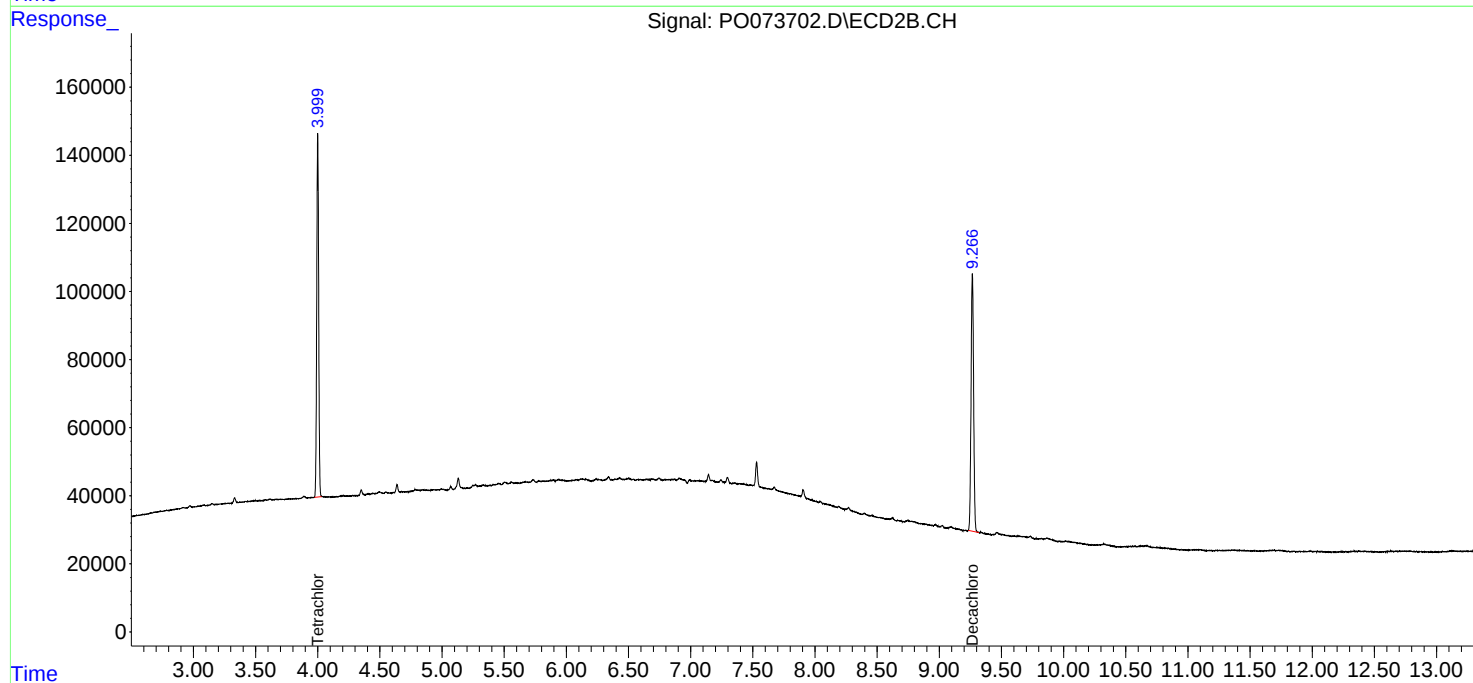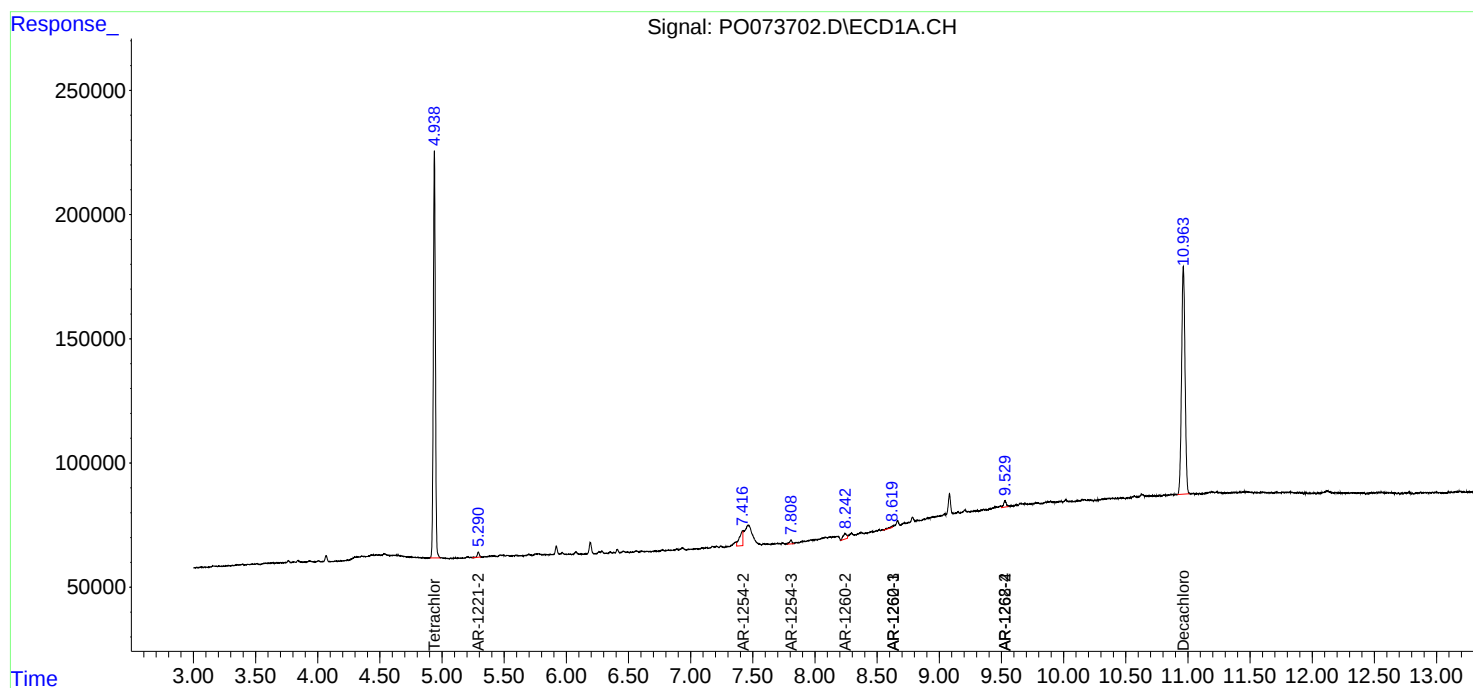


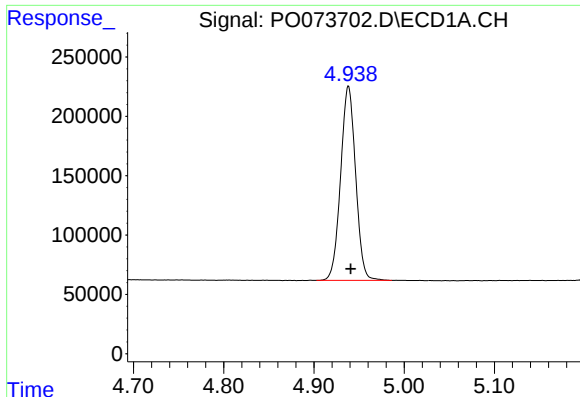

#1 Tetrachloro-m-xylene


R.T.: 4.938 min
Delta R.T.: -0.003 min
Response: 1890649
Conc: 20.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
CS-47

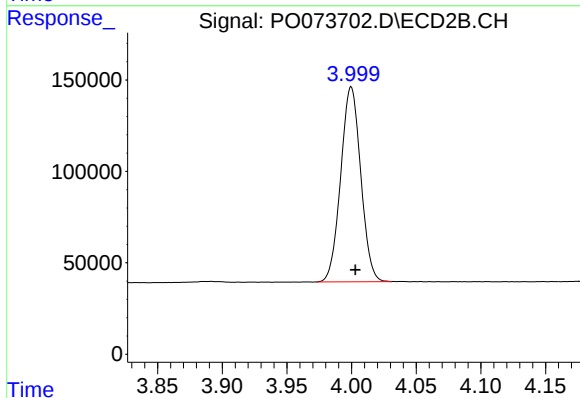


#1 Tetrachloro-m-xylene

R.T.: 4.000 min
Delta R.T.: -0.003 min
Response: 1149153
Conc: 21.42 ng/ml

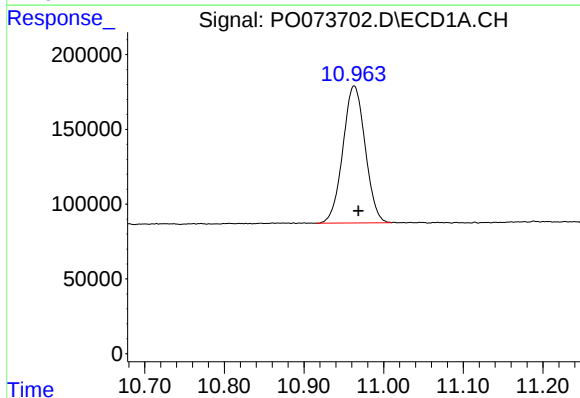


#2 Decachlorobiphenyl

R.T.: 10.963 min
Delta R.T.: -0.005 min
Response: 1779008
Conc: 21.53 ng/ml

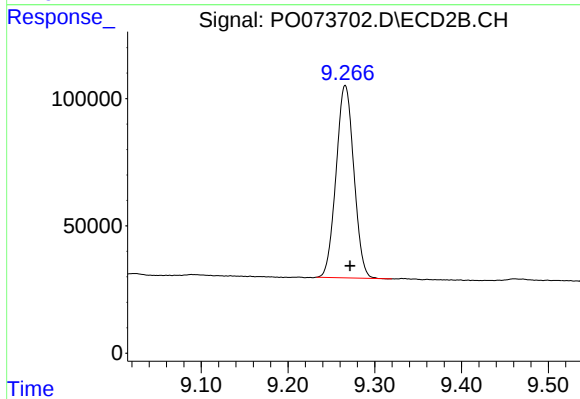

#2 Decachlorobiphenyl


R.T.: 9.266 min
Delta R.T.: -0.006 min
Response: 1075370
Conc: 22.98 ng/ml

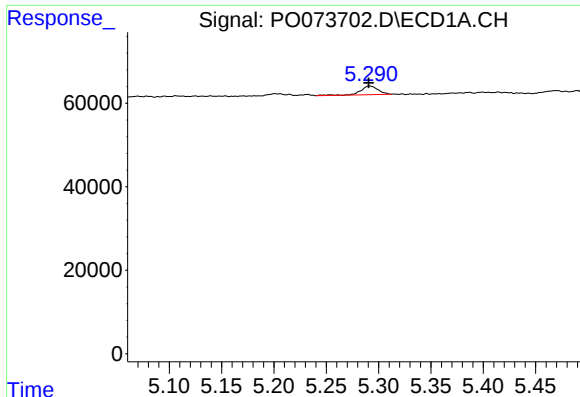

#9 AR-1221-2


R.T.: 5.291 min
Delta R.T.: 0.000 min
Response: 24610
Conc: 31.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
CS-47

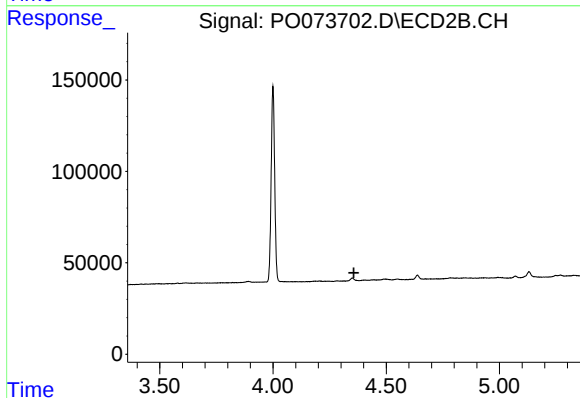


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.357 min
Response: 0
Conc: N.D.

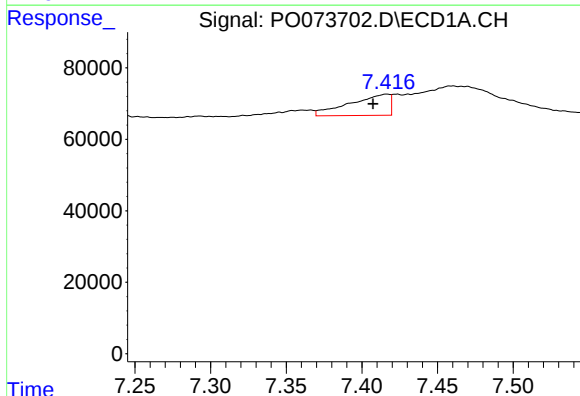


#27 AR-1254-2

R.T.: 7.416 min
Delta R.T.: 0.009 min
Response: 108305
Conc: 18.37 ng/ml

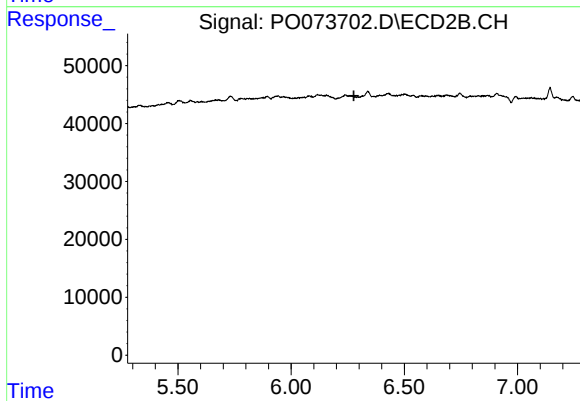

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T. : 6.277 min
Response: 0
Conc: N.D.

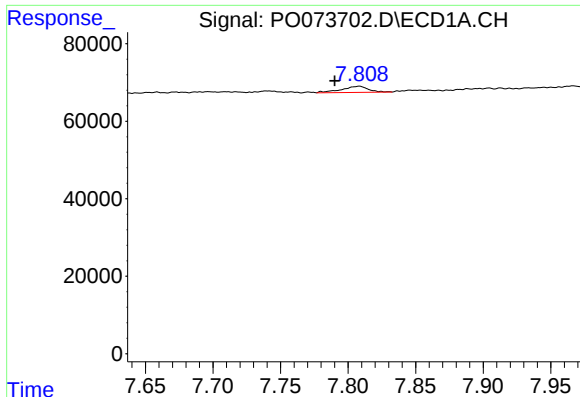

#28 AR-1254-3


R.T.: 7.808 min
Delta R.T.: 0.018 min
Response: 21209
Conc: 3.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
CS-47

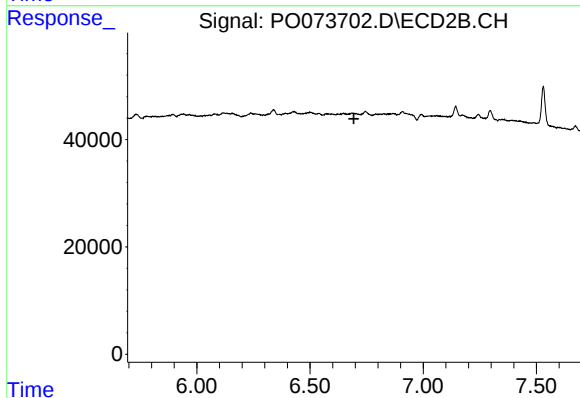


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.694 min
Response: 0
Conc: N.D.

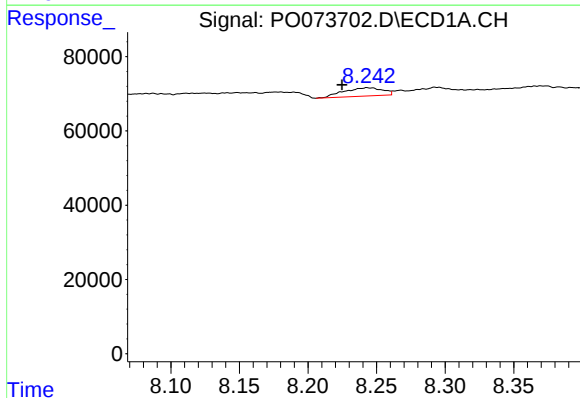


#32 AR-1260-2

R.T.: 8.243 min
Delta R.T.: 0.018 min
Response: 44547
Conc: 7.93 ng/ml

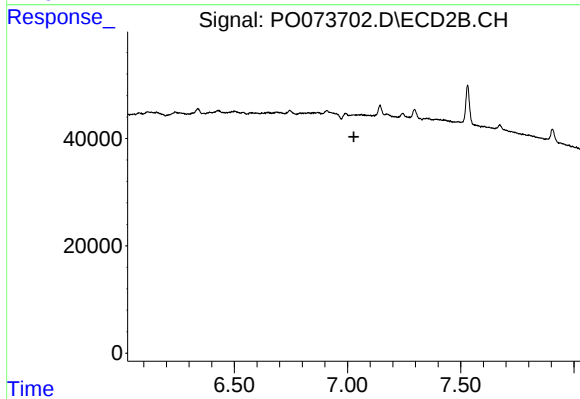

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 7.028 min
Response: 0
Conc: N.D.

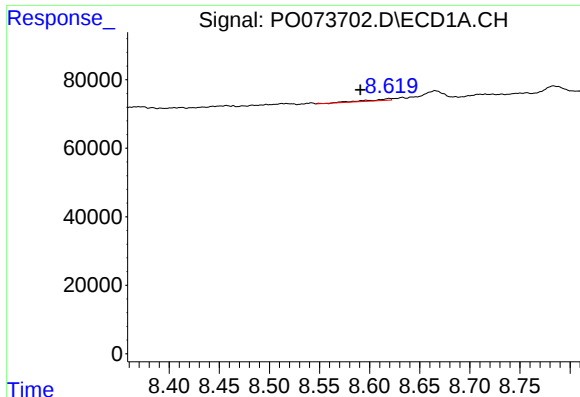

#33 AR-1260-3


R.T.: 8.619 min
Delta R.T.: 0.029 min
Response: 7491
Conc: 1.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
CS-47

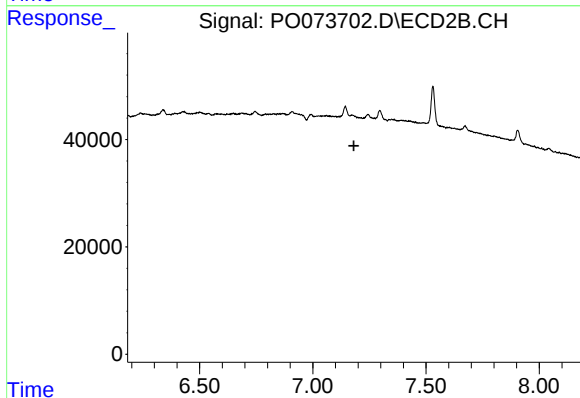


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 7.182 min
Response: 0
Conc: N.D.

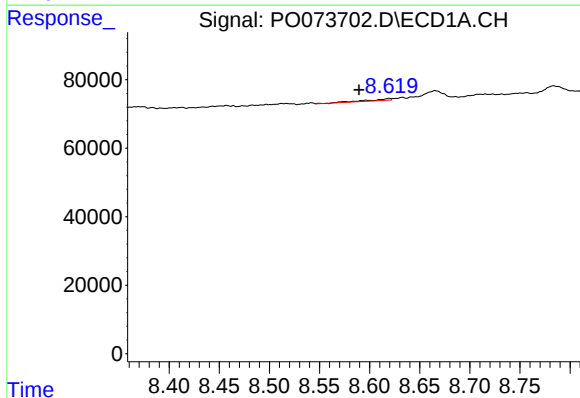


#36 AR-1262-1

R.T.: 8.619 min
Delta R.T.: 0.030 min
Response: 7491
Conc: 1.00 ng/ml

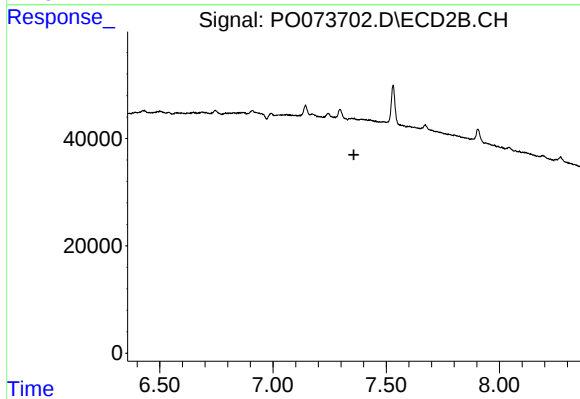

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T. : 7.357 min
Response: 0
Conc: N.D.

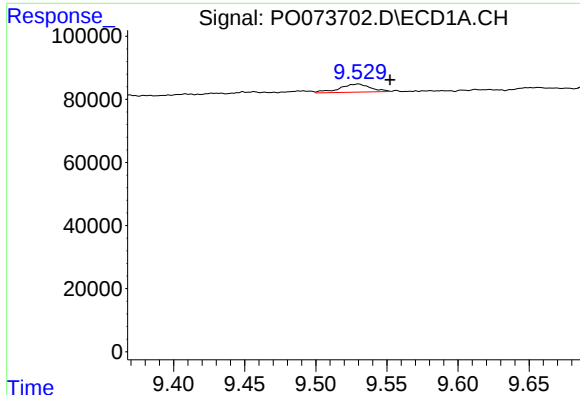

#39 AR-1262-4


R.T.: 9.530 min
Delta R.T.: -0.022 min
Response: 38928
Conc: 11.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
CS-47

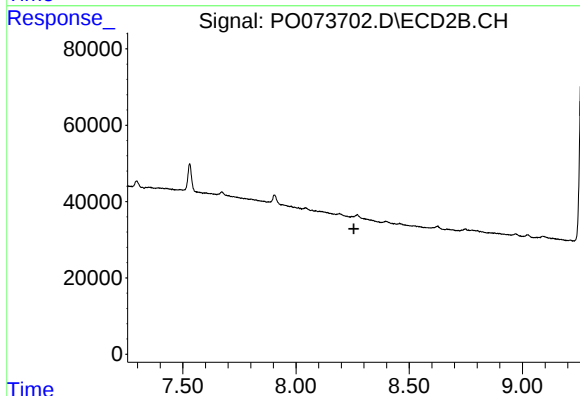


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 8.256 min
Response: 0
Conc: N.D.

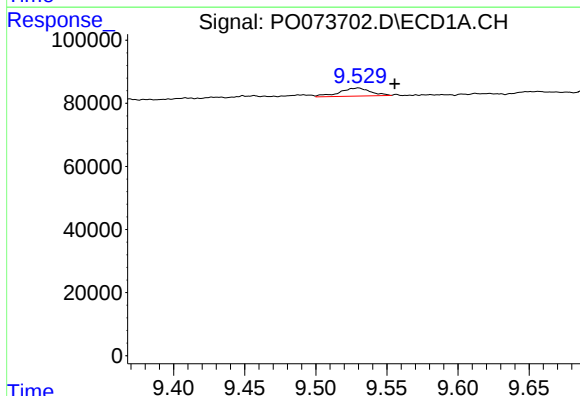

#42 AR-1268-2

R.T.: 9.530 min
Delta R.T.: -0.026 min
Response: 38928
Conc: 3.16 ng/ml

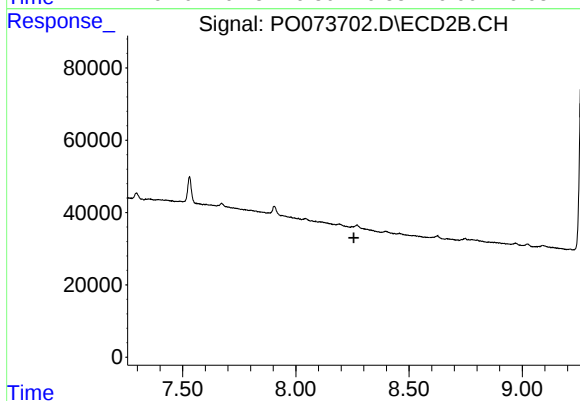

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 8.257 min
Response: 0
Conc: N.D.