

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0121120\
 Data File : P0073684.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Dec 2020 19:25
 Operator : DD\AJ
 Sample : L5018-02 20X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 KZZ093L-END-2

Manual Integrations
 APPROVED

Ankita
 12/14/2020 3:20:28 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 23:53:16 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0121020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 11 03:58:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.939	4.001	92096	63522	1.007m	1.184
2) SA Decachlor...	10.966	9.269	92496	53816	1.119	1.150

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121120\
Data File : PO073684.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Dec 2020 19:25
Operator : DD\AJ
Sample : L5018-02 20X
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
KZZ093L-END-2


Manual Integrations
APPROVED

Ankita
12/14/2020 3:20:28 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 23:53:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 11 03:58:06 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

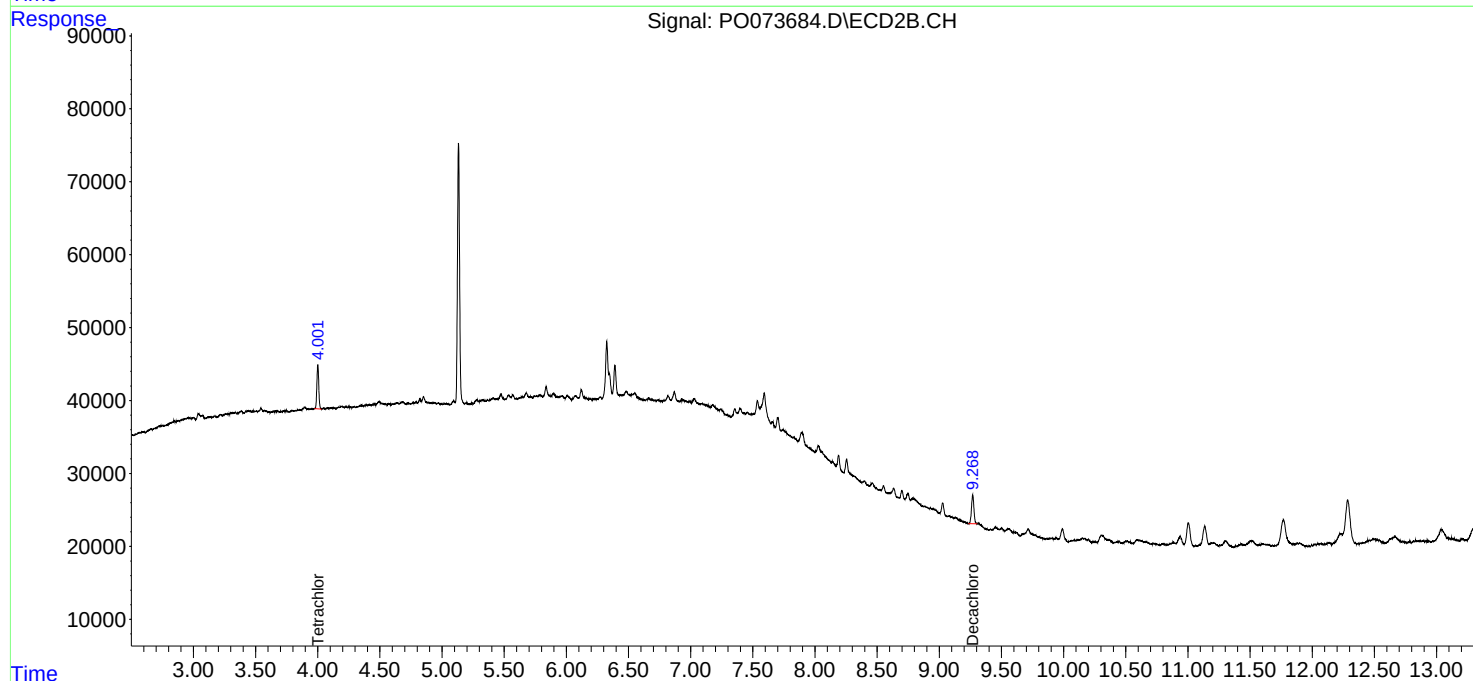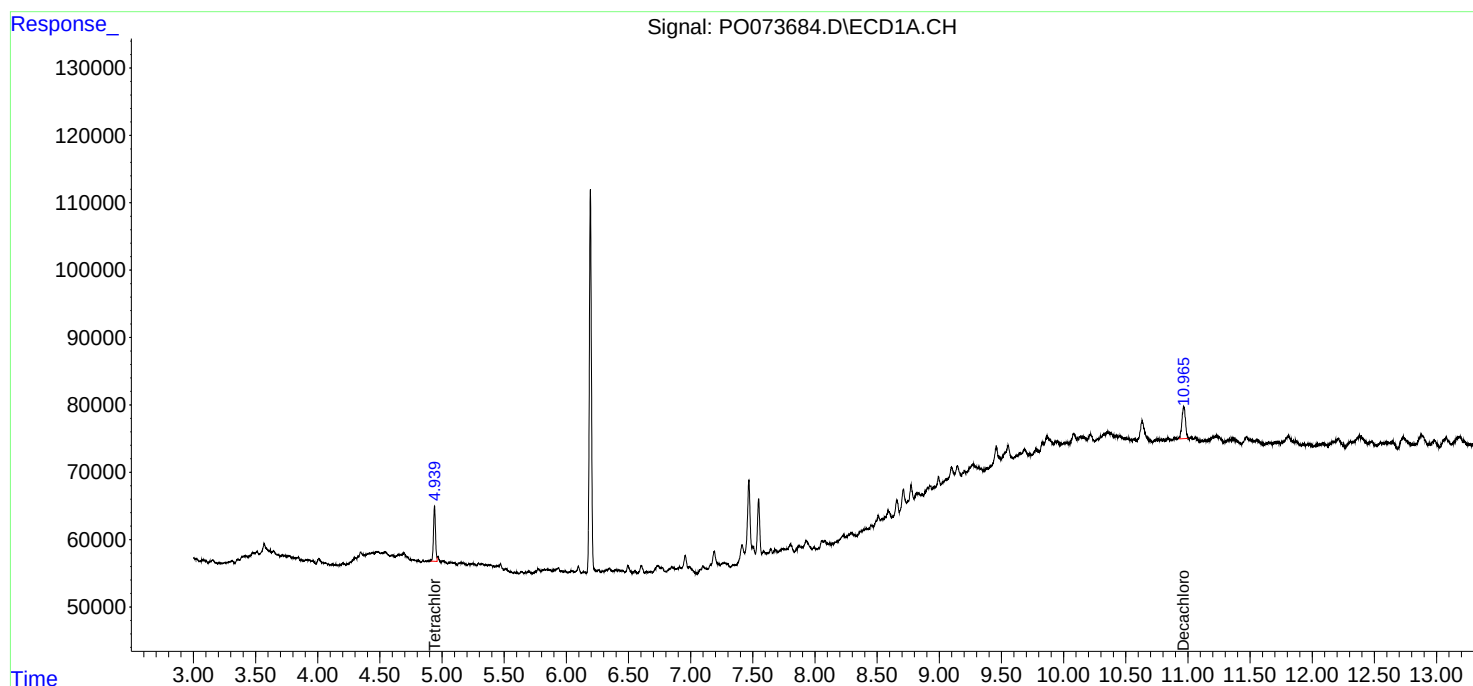

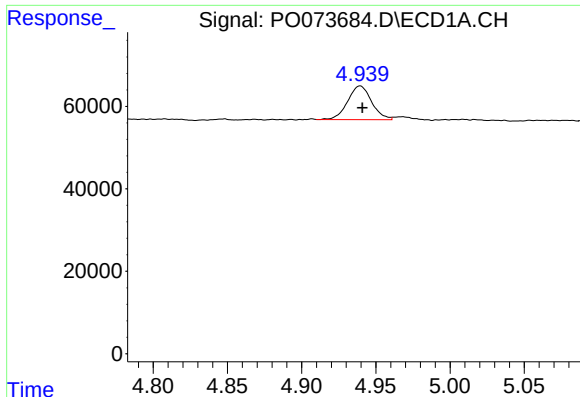


#1 Tetrachloro-m-xylene

R.T.: 4.939 min
Delta R.T.: -0.002 min
Response: 92096
Conc: 1.01 ng/ml m

Instrument :
ECD_O
ClientSampleId :
KZZ093L-END-2


Manual Integrations
APPROVED

Ankita
12/14/2020 3:20:28 PM

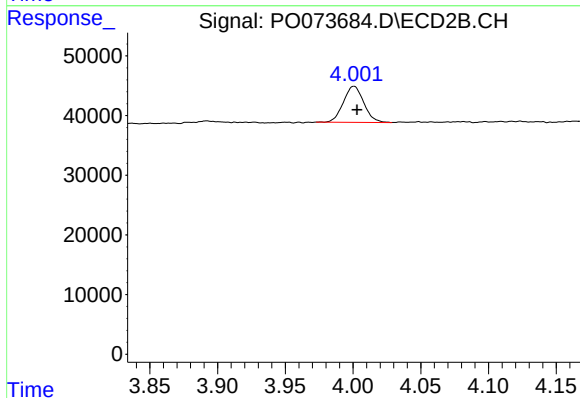


#1 Tetrachloro-m-xylene

R.T.: 4.001 min
Delta R.T.: -0.002 min
Response: 63522
Conc: 1.18 ng/ml

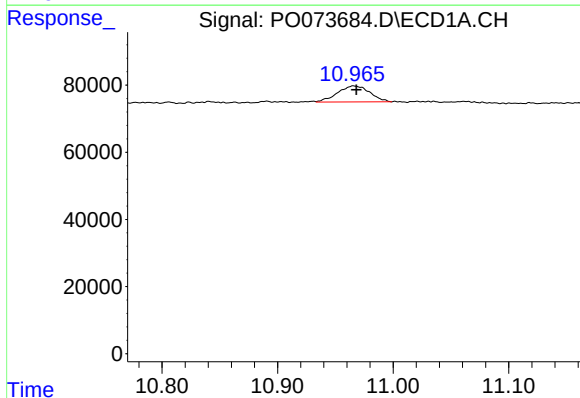

#2 Decachlorobiphenyl

R.T.: 10.966 min
Delta R.T.: -0.003 min
Response: 92496
Conc: 1.12 ng/ml

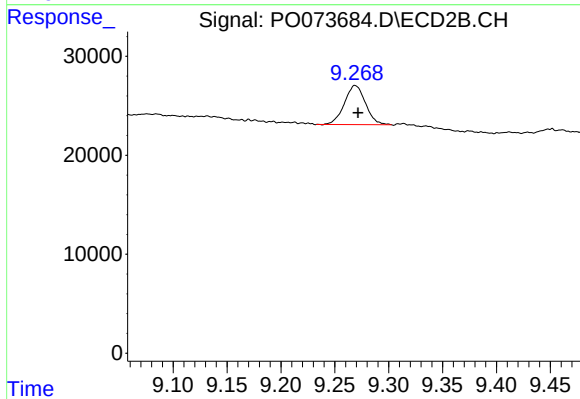

#2 Decachlorobiphenyl

R.T.: 9.269 min
Delta R.T.: -0.003 min
Response: 53816
Conc: 1.15 ng/ml