

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121120\
 Data File : PO073730.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Dec 2020 8:32
 Operator : DD\AJ
 Sample : L5009-03
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 KENS-B5-120920-13-15

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 14 00:35:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 11 03:58:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.941	4.000	2086064	1216787	22.817	22.686
2) SA Decachlor...	10.966	9.266	1651445	939315	19.984	20.075

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121120\
Data File : PO073730.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Dec 2020 8:32
Operator : DD\AJ
Sample : L5009-03
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
KENS-B5-120920-13-15

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 14 00:35:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 11 03:58:06 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

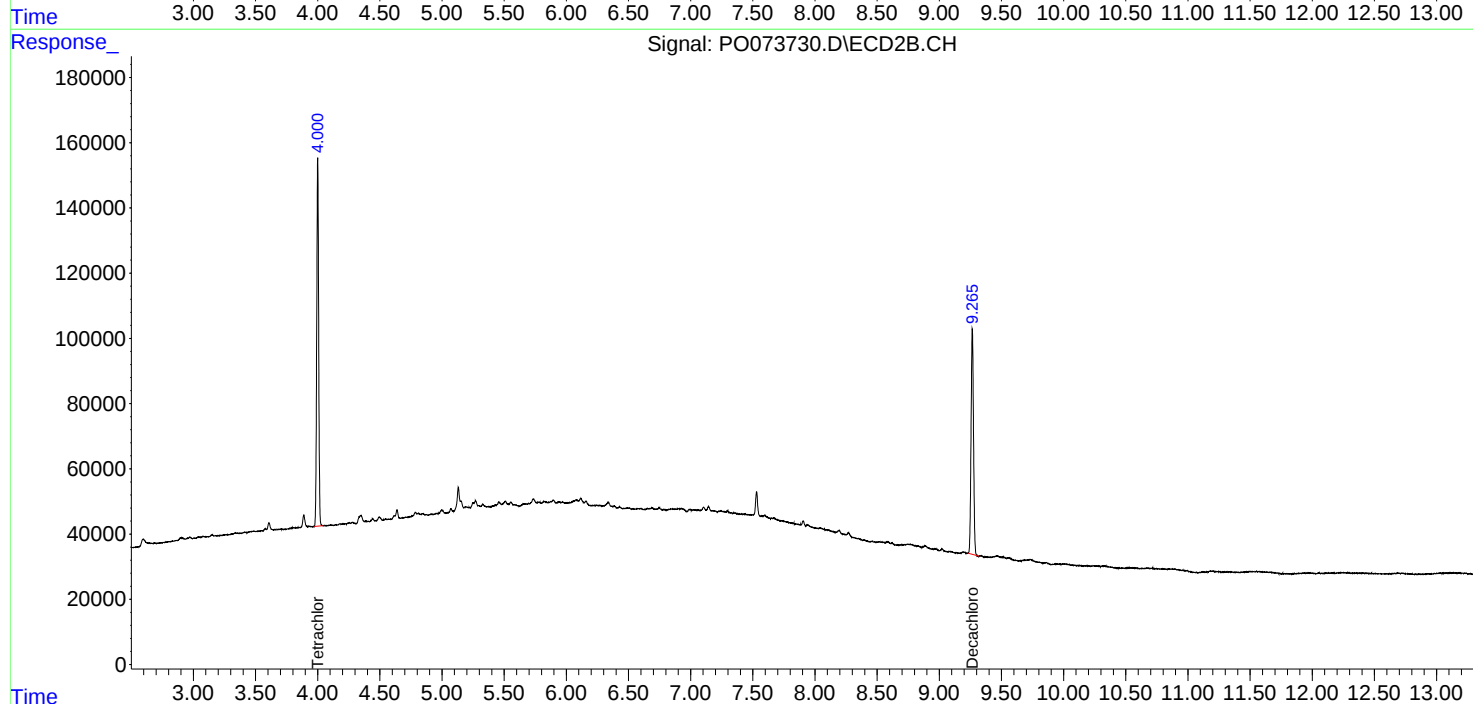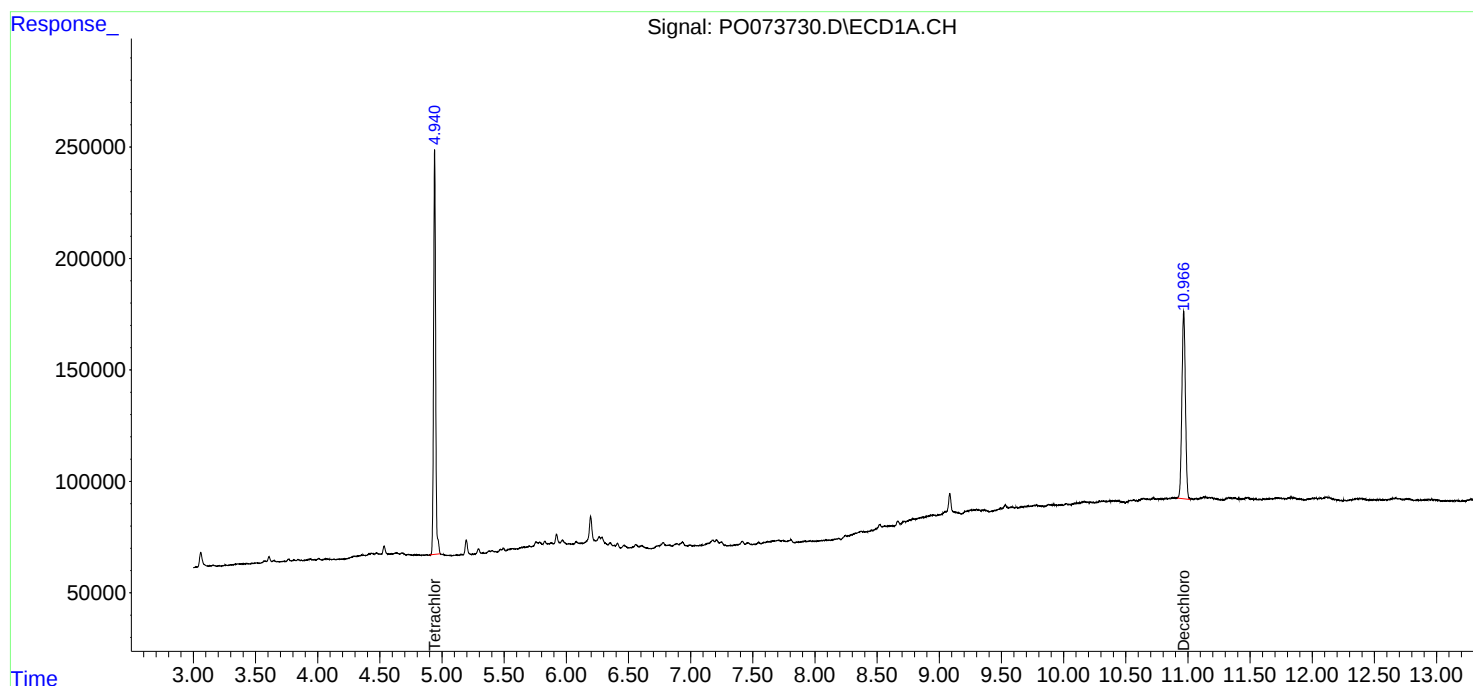


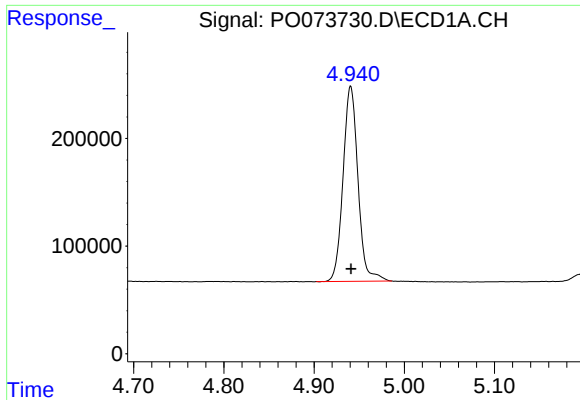

#1 Tetrachloro-m-xylene


R.T.: 4.941 min
Delta R.T.: 0.000 min
Response: 2086064
Conc: 22.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
KENS-B5-120920-13-15

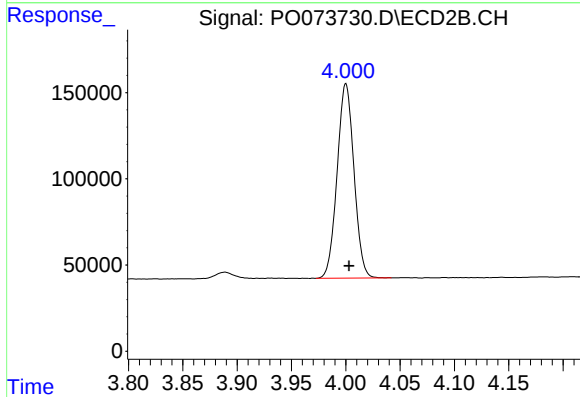


#1 Tetrachloro-m-xylene

R.T.: 4.000 min
Delta R.T.: -0.003 min
Response: 1216787
Conc: 22.69 ng/ml

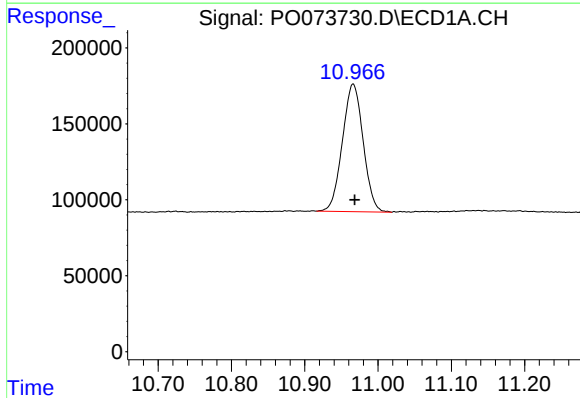

#2 Decachlorobiphenyl

R.T.: 10.966 min
Delta R.T.: -0.002 min
Response: 1651445
Conc: 19.98 ng/ml

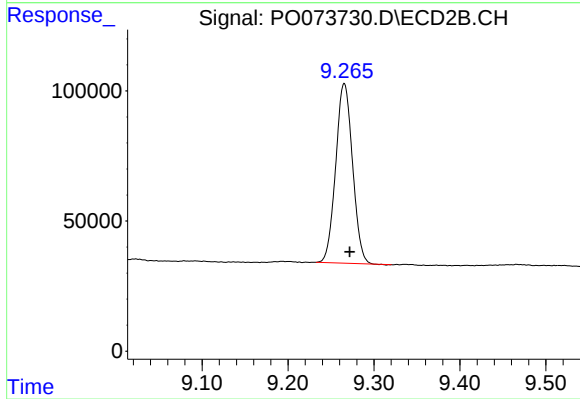

#2 Decachlorobiphenyl

R.T.: 9.266 min
Delta R.T.: -0.006 min
Response: 939315
Conc: 20.07 ng/ml