

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\PO121120\  
Data File : PO073736.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 12 Dec 2020 10:14  
Operator : DD\AJ  
Sample : L5019-02 20X  
Misc :  
ALS Vial : 70 Sample Multiplier: 1

Instrument :  
ECD\_O  
ClientSampleId :  
HIH021D-END-2

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Dec 14 00:37:20 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\PO121020.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Fri Dec 11 03:58:06 2020  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

-----  
System Monitoring Compounds

Target Compounds  
-----



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\PO121120\  
Data File : PO073736.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 12 Dec 2020 10:14  
Operator : DD\AJ  
Sample : L5019-02 20X  
Misc :  
ALS Vial : 70 Sample Multiplier: 1

Instrument :  
ECD\_O  
ClientSampleId :  
HIH021D-END-2

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Dec 14 00:37:20 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\PO121020.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Fri Dec 11 03:58:06 2020  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

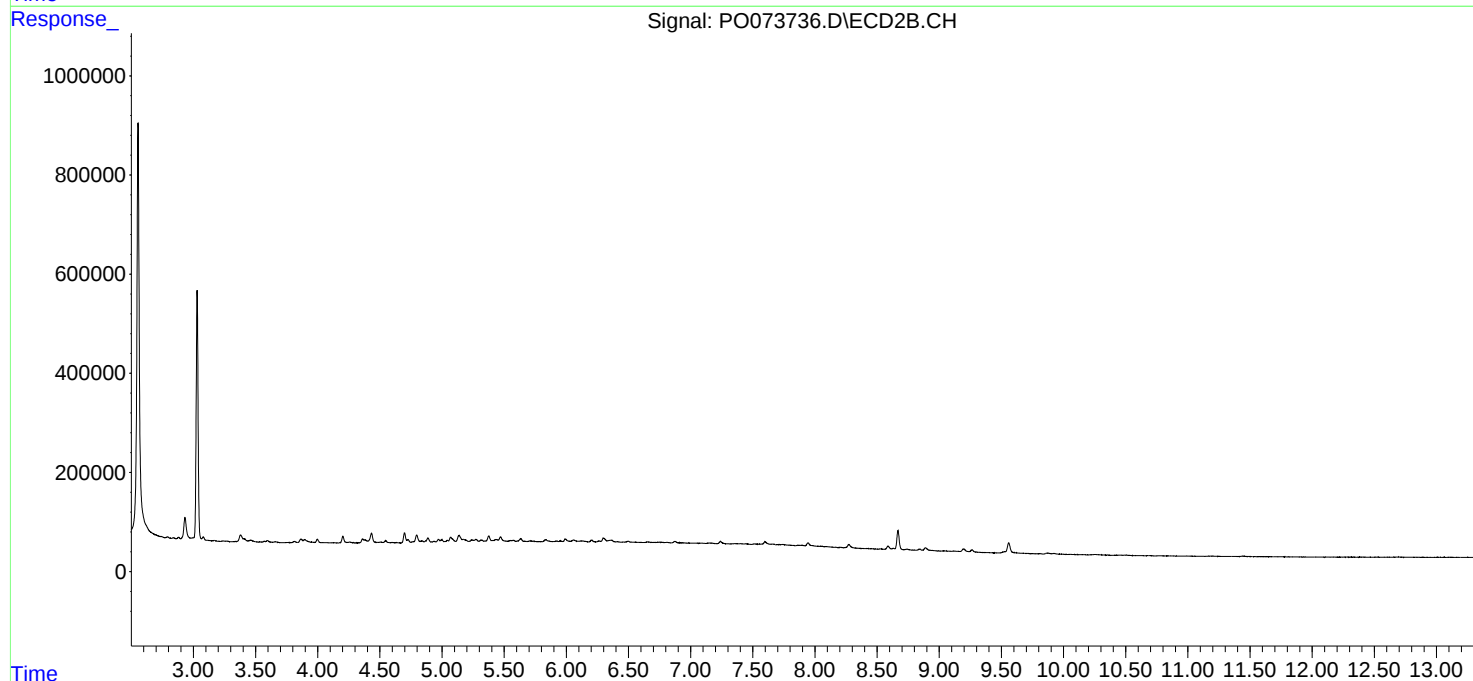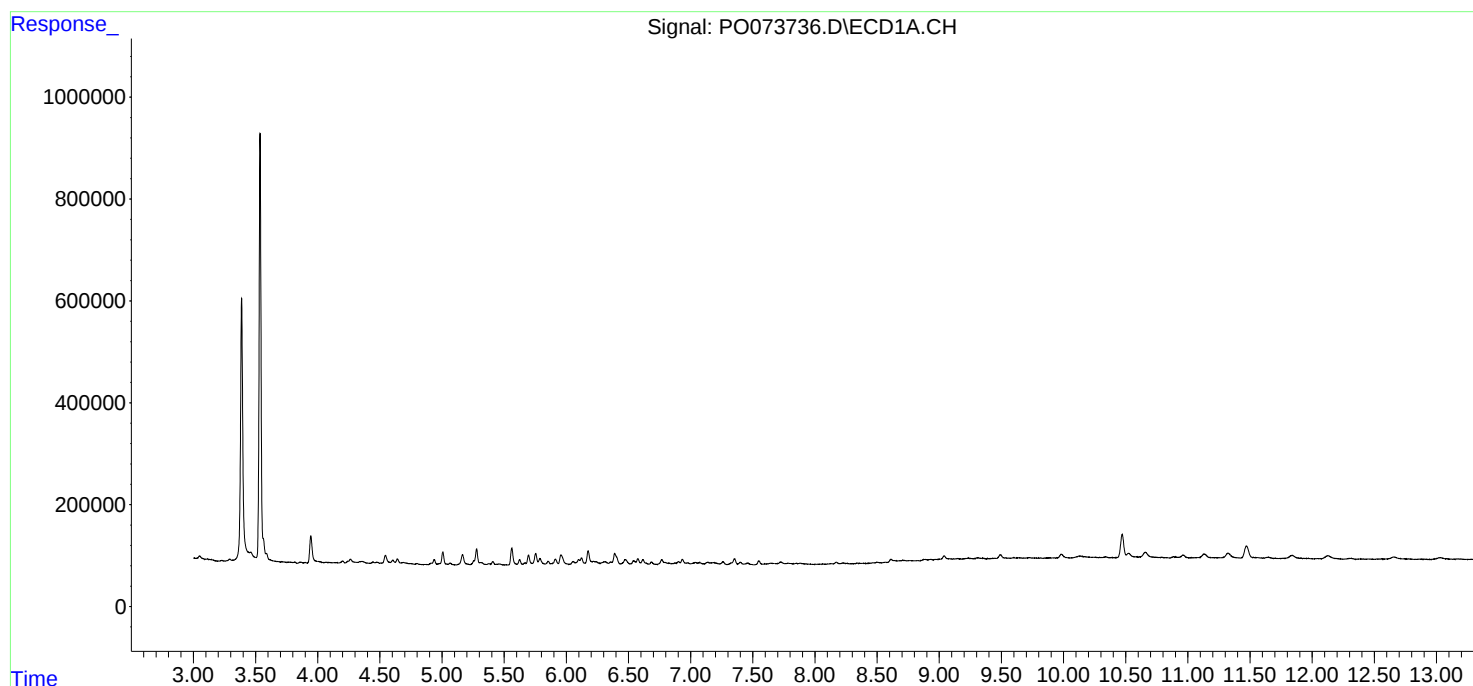


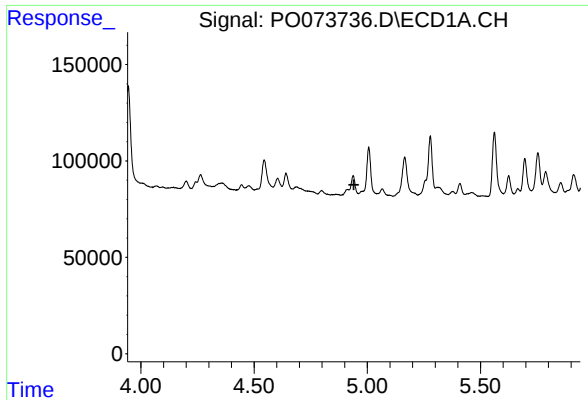

#1 Tetrachloro-m-xylene


R.T.: 0.000 min  
Exp R.T. : 4.941 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_O  
ClientSampleId :  
HIH021D-END-2

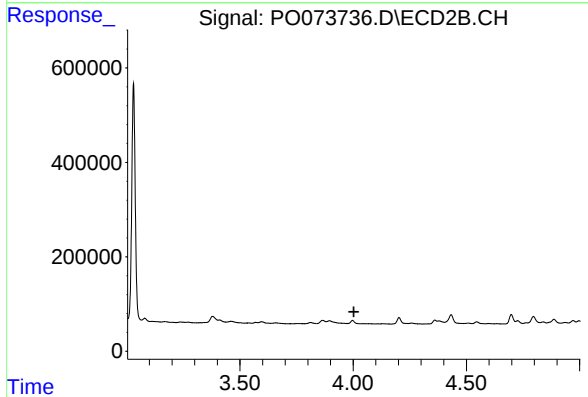


#1 Tetrachloro-m-xylene

R.T.: 0.000 min  
Exp R.T. : 4.003 min  
Response: 0  
Conc: N.D.

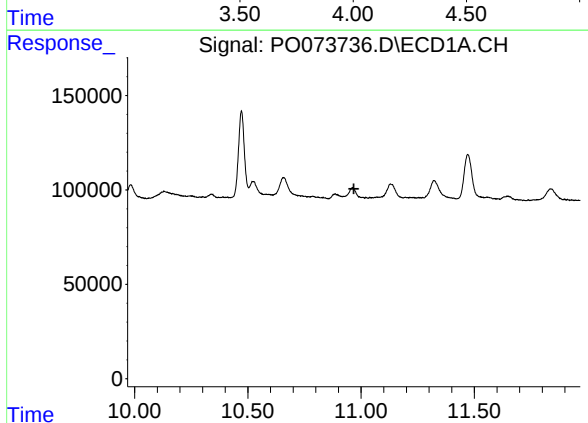

#2 Decachlorobiphenyl

R.T.: 0.000 min  
Exp R.T. : 10.968 min  
Response: 0  
Conc: N.D.

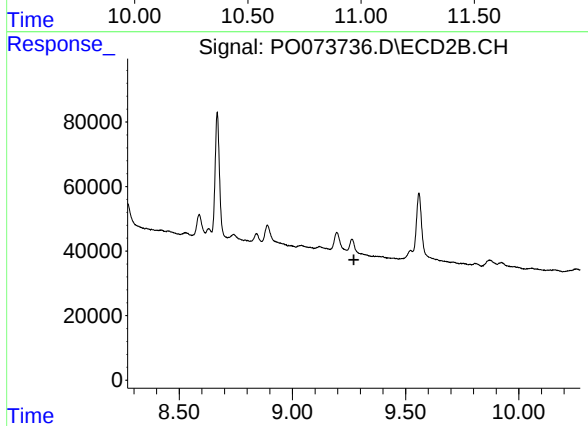

#2 Decachlorobiphenyl

R.T.: 0.000 min  
Exp R.T. : 9.272 min  
Response: 0  
Conc: N.D.