

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121123\
 Data File : PO100423.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Dec 2023 00:18
 Operator : YP/AJ
 Sample : 05738-09 10X
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HEC-99IZ-A

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/12/2023
 Supervised By :Ankita Jodhani 12/12/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 02:15:06 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Dec 11 00:11:33 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.472	3.698	2029353	1845193	0.810	0.848m
2) SA Decachlor...	10.346	8.783	1828188	2172984	1.310	1.347

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121123\
Data File : PO100423.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Dec 2023 00:18
Operator : YP/AJ
Sample : 05738-09 10X
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HEC-99IZ-A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/12/2023
Supervised By :Ankita Jodhani 12/12/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 02:15:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120823.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Dec 11 00:11:33 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

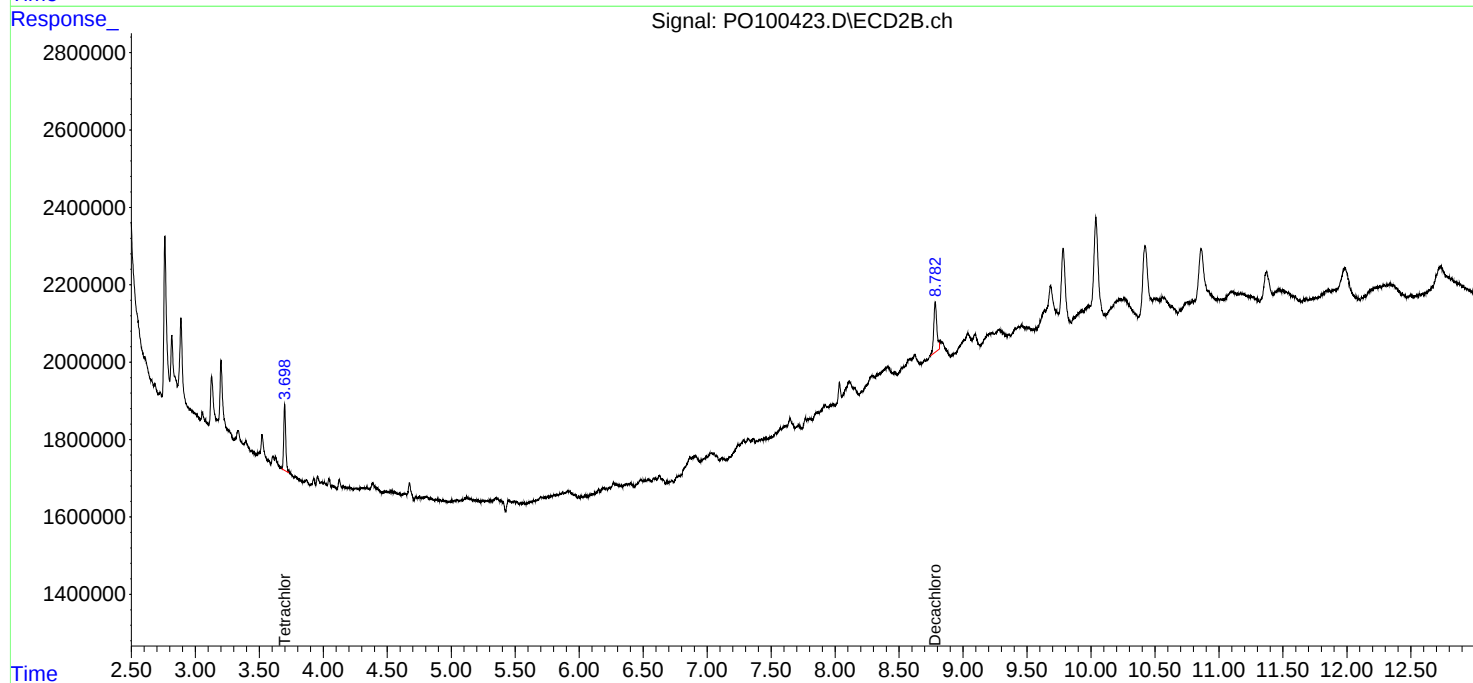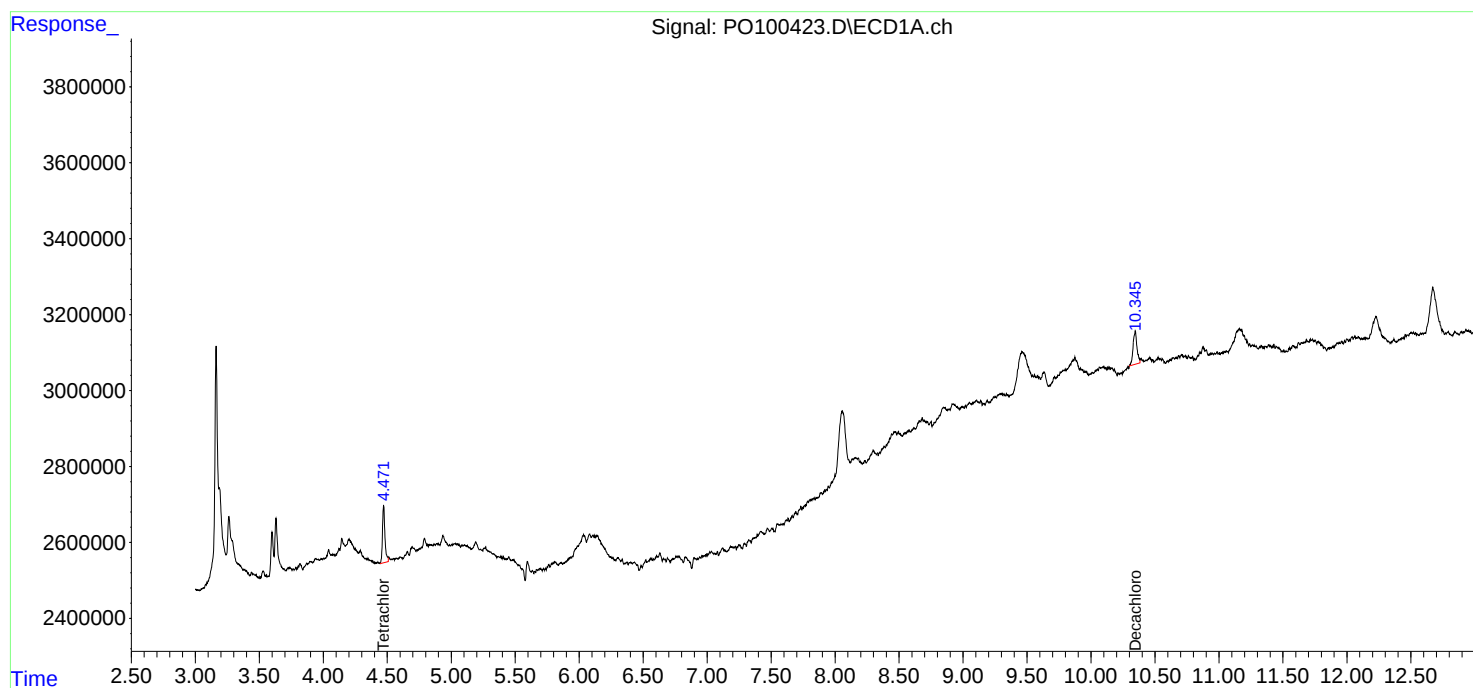

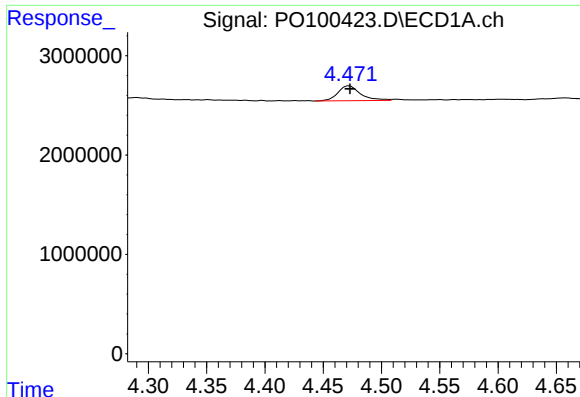


#1 Tetrachloro-m-xylene

R.T.: 4.472 min
Delta R.T.: 0.000 min
Response: 2029353
Conc: 0.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
HEC-99IZ-A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/12/2023
Supervised By :Ankita Jodhani 12/12/2023

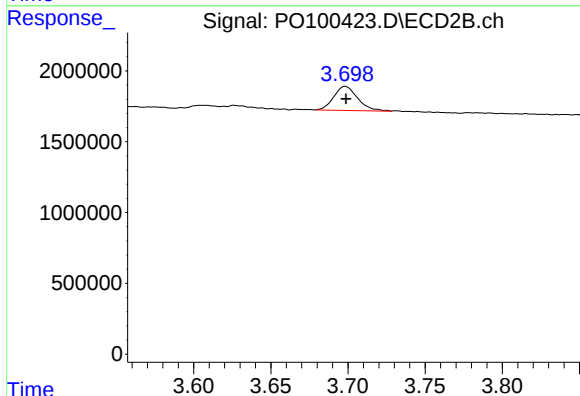


#1 Tetrachloro-m-xylene

R.T.: 3.698 min
Delta R.T.: -0.001 min
Response: 1845193
Conc: 0.85 ng/ml m

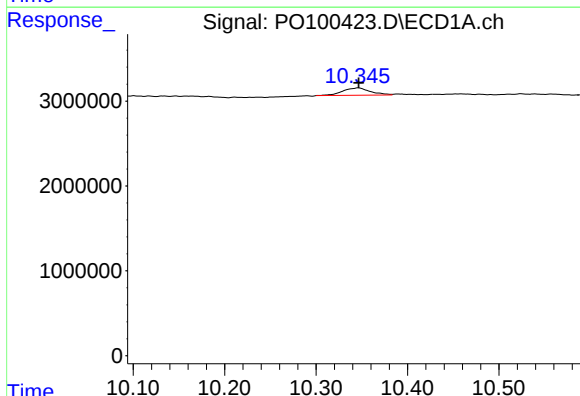

#2 Decachlorobiphenyl

R.T.: 10.346 min
Delta R.T.: 0.000 min
Response: 1828188
Conc: 1.31 ng/ml

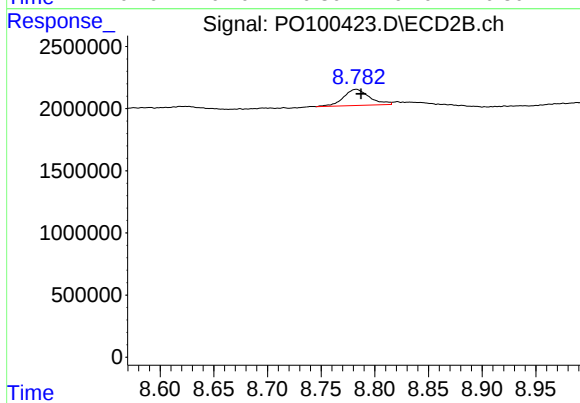

#2 Decachlorobiphenyl

R.T.: 8.783 min
Delta R.T.: -0.005 min
Response: 2172984
Conc: 1.35 ng/ml