

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121123\
 Data File : PO100429.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Dec 2023 02:00
 Operator : YP/AJ
 Sample : 05741-09 10X
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC-288026-

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/12/2023
 Supervised By :Ankita Jodhani 12/12/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 03:04:49 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Dec 11 00:11:33 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.472	3.699	2277146	2346192	0.909	1.078
2) SA Decachlor...	10.340	8.783	2090557	1735713	1.498	1.076m#
Target Compounds						
26) L6 AR-1254-1	6.523	5.615	4647706	4165921	54.641m	53.015
27) L6 AR-1254-2	6.746	5.763	6580499	4095937	52.967	58.170
28) L6 AR-1254-3	7.116	6.171	6148147	5679689	51.479	46.908
29) L6 AR-1254-4	7.404	6.401	4751494	3742949	68.517	56.999
30) L6 AR-1254-5	7.828	6.823	5805296	6174419	70.825	55.952

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121123\
Data File : PO100429.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Dec 2023 02:00
Operator : YP/AJ
Sample : 05741-09 10X
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BC-288026-


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/12/2023
Supervised By :Ankita Jodhani 12/12/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 03:04:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120823.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Dec 11 00:11:33 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

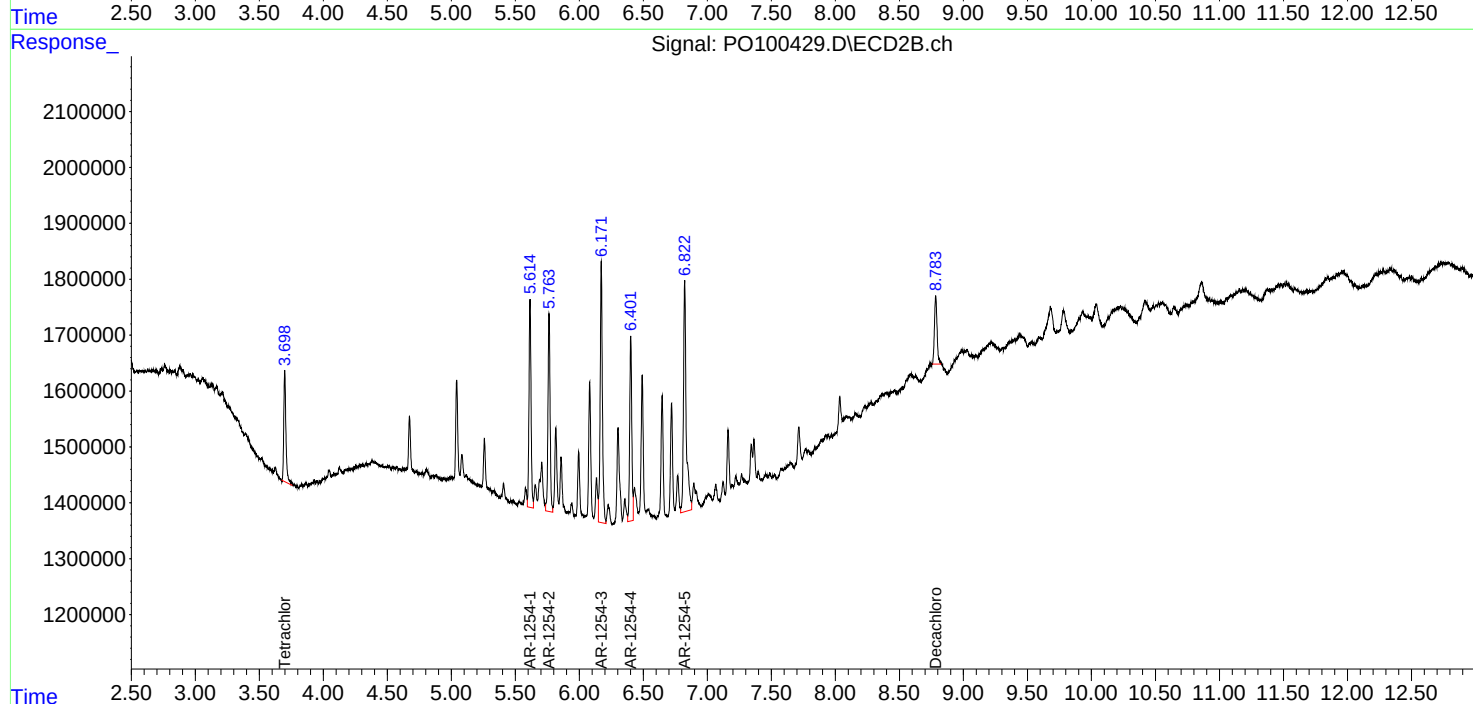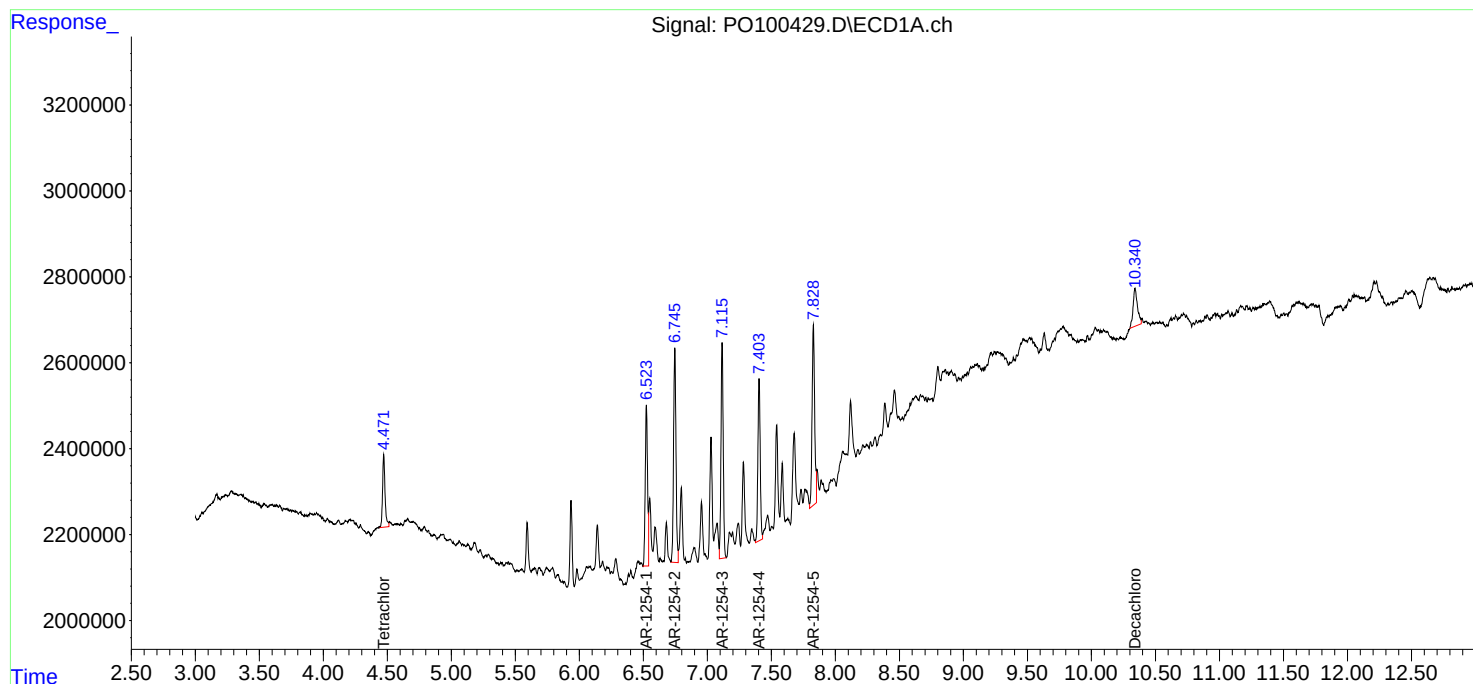

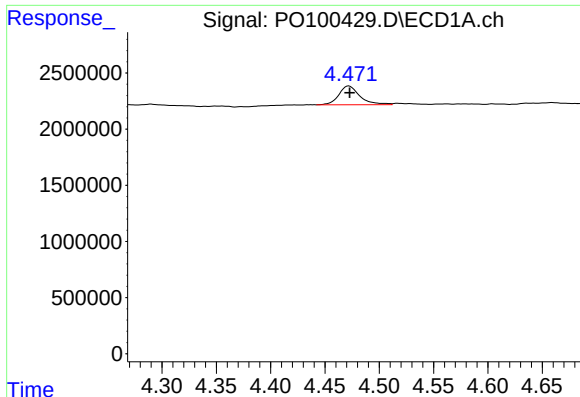


#1 Tetrachloro-m-xylene

R.T.: 4.472 min
Delta R.T.: -0.001 min
Response: 2277146
Conc: 0.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC-288026-


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/12/2023
Supervised By :Ankita Jodhani 12/12/2023

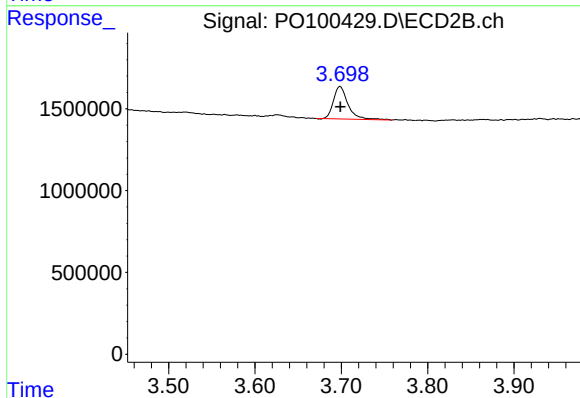


#1 Tetrachloro-m-xylene

R.T.: 3.699 min
Delta R.T.: 0.000 min
Response: 2346192
Conc: 1.08 ng/ml

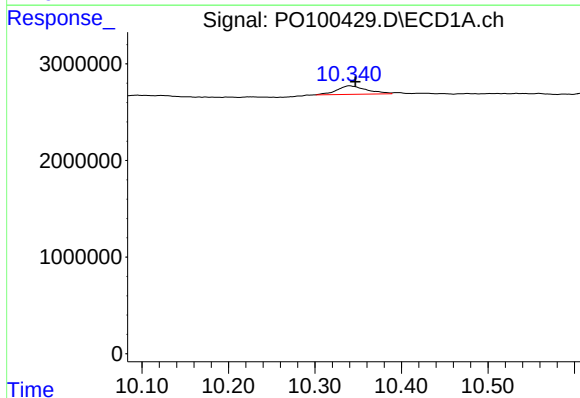


#2 Decachlorobiphenyl

R.T.: 10.340 min
Delta R.T.: -0.006 min
Response: 2090557
Conc: 1.50 ng/ml

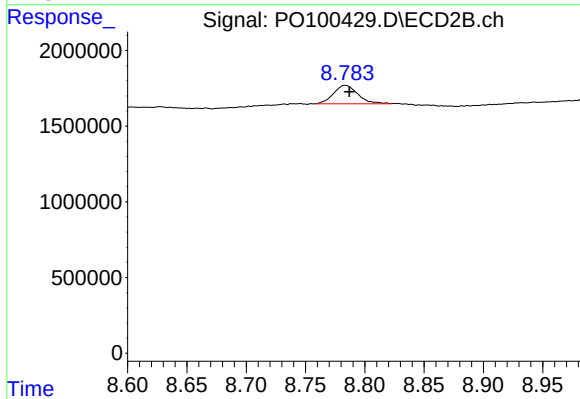

#2 Decachlorobiphenyl

R.T.: 8.783 min
Delta R.T.: -0.004 min
Response: 1735713
Conc: 1.08 ng/ml m

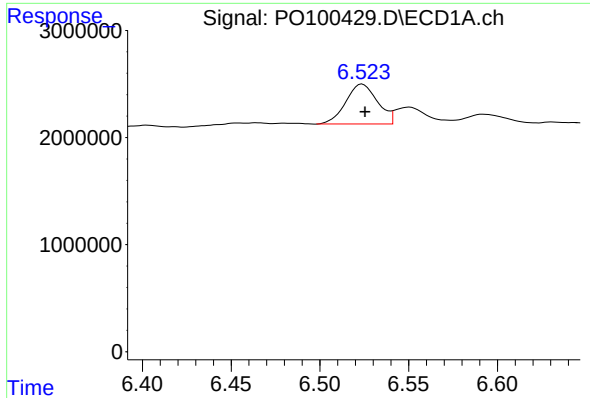


#26 AR-1254-1

R.T.: 6.523 min
Delta R.T.: -0.002 min
Response: 4647706
Conc: 54.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC-288026-


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/12/2023
Supervised By :Ankita Jodhani 12/12/2023

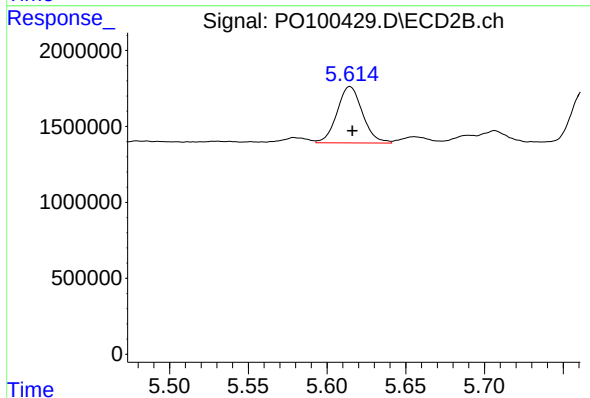


#26 AR-1254-1

R.T.: 5.615 min
Delta R.T.: -0.001 min
Response: 4165921
Conc: 53.02 ng/ml

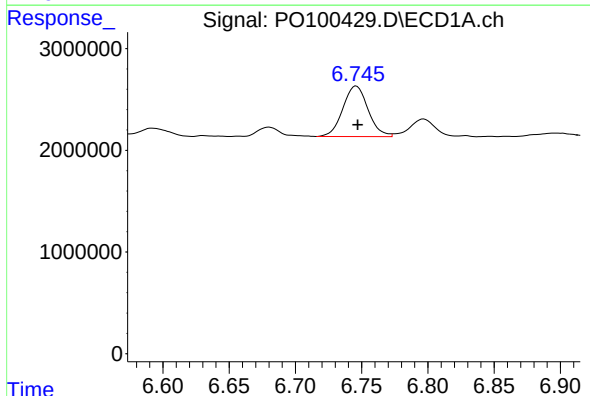


#27 AR-1254-2

R.T.: 6.746 min
Delta R.T.: -0.001 min
Response: 6580499
Conc: 52.97 ng/ml

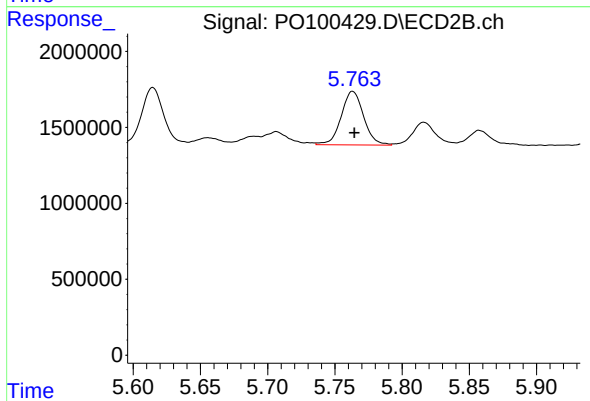

#27 AR-1254-2

R.T.: 5.763 min
Delta R.T.: -0.001 min
Response: 4095937
Conc: 58.17 ng/ml

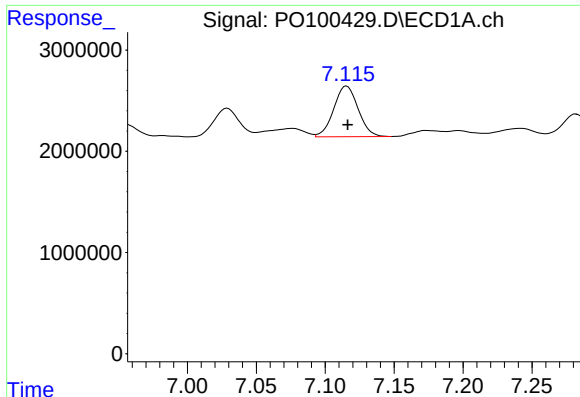


#28 AR-1254-3

R.T.: 7.116 min
Delta R.T.: 0.000 min
Response: 6148147
Conc: 51.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC-288026-


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/12/2023
Supervised By :Ankita Jodhani 12/12/2023

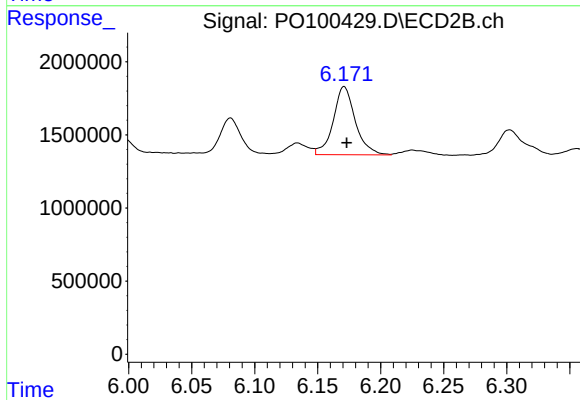


#28 AR-1254-3

R.T.: 6.171 min
Delta R.T.: -0.002 min
Response: 5679689
Conc: 46.91 ng/ml

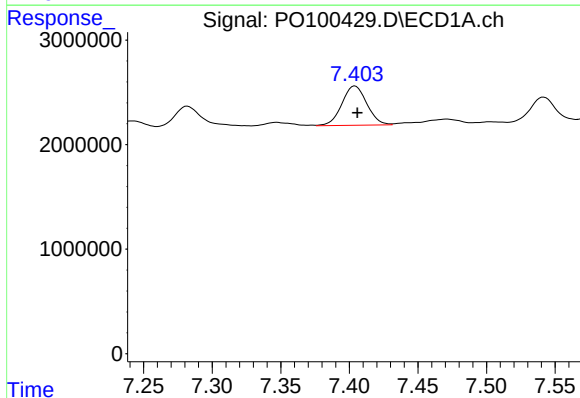


#29 AR-1254-4

R.T.: 7.404 min
Delta R.T.: -0.002 min
Response: 4751494
Conc: 68.52 ng/ml

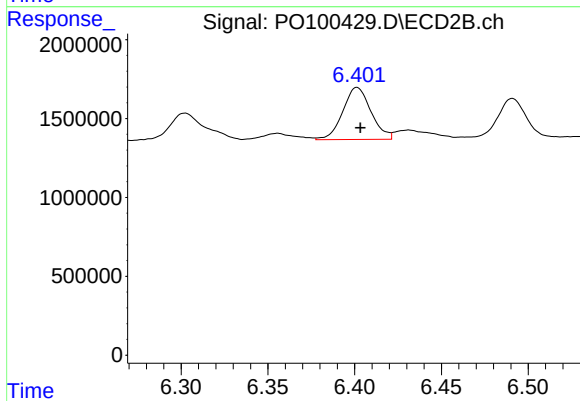

#29 AR-1254-4

R.T.: 6.401 min
Delta R.T.: -0.002 min
Response: 3742949
Conc: 57.00 ng/ml

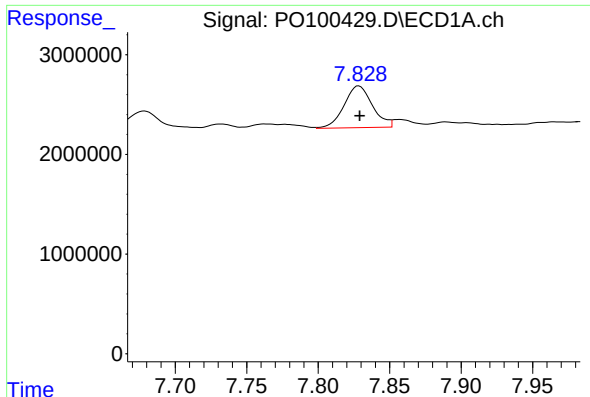


#30 AR-1254-5

R.T.: 7.828 min
Delta R.T.: 0.000 min
Response: 5805296
Conc: 70.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC-288026-

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/12/2023
Supervised By :Ankita Jodhani 12/12/2023

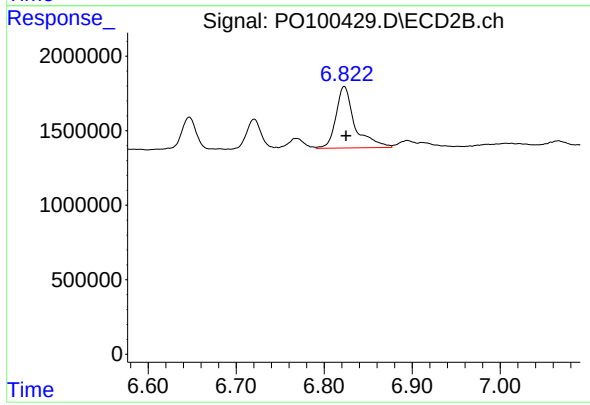

#30 AR-1254-5

R.T.: 6.823 min
Delta R.T.: -0.002 min
Response: 6174419
Conc: 55.95 ng/ml