

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121123\
 Data File : PO100435.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Dec 2023 09:30
 Operator : YP/AJ
 Sample : 05741-05RE 10X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC-260967-RE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/12/2023
 Supervised By :Ankita Jodhani 12/12/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 11:34:01 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Dec 11 00:11:33 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.471	3.697	2904452	2809792	1.160	1.291m
2) SA Decachlor...	10.339	8.782	5666784	5203066	4.060	3.225

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121123\
Data File : PO100435.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Dec 2023 09:30
Operator : YP/AJ
Sample : 05741-05RE 10X
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BC-260967-RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/12/2023
Supervised By :Ankita Jodhani 12/12/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 11:34:01 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120823.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Dec 11 00:11:33 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

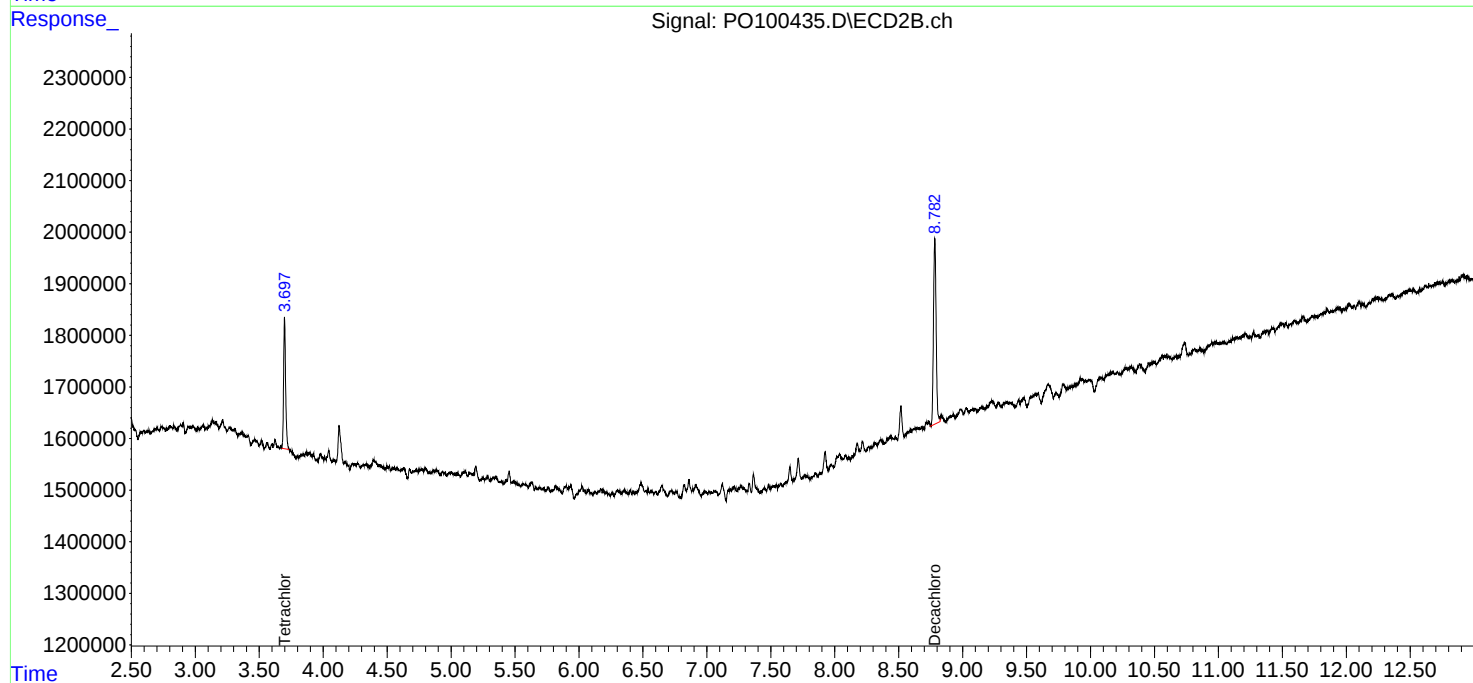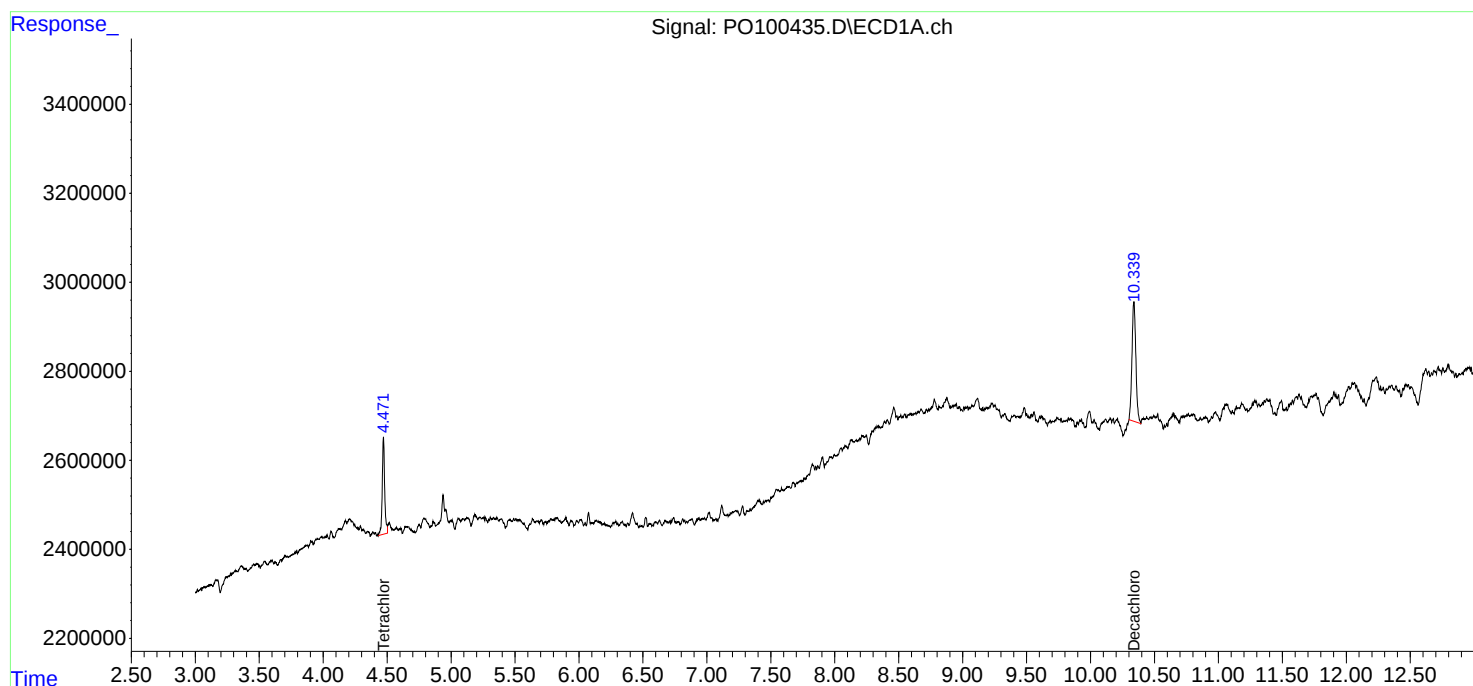

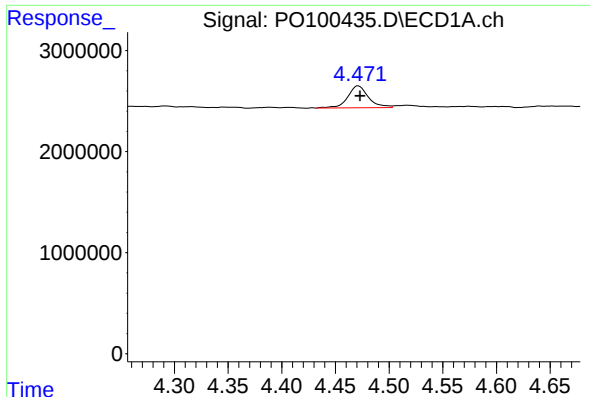

#1 Tetrachloro-m-xylene

R.T.: 4.471 min
Delta R.T.: -0.002 min
Response: 2904452
Conc: 1.16 ng/ml

Instrument :

ECD_O


ClientSampleId :

BC-260967-RE

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 12/12/2023
Supervised By :Ankita Jodhani 12/12/2023

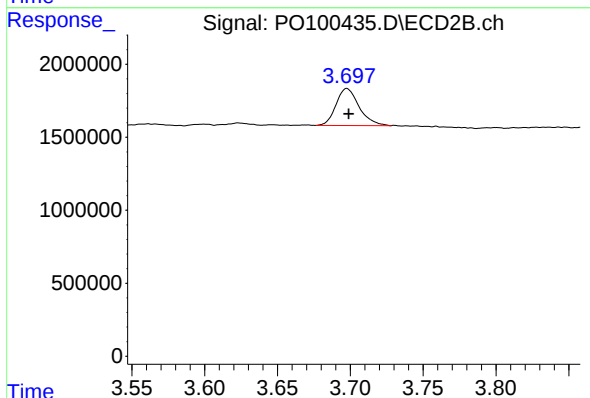


#1 Tetrachloro-m-xylene

R.T.: 3.697 min
Delta R.T.: -0.002 min
Response: 2809792
Conc: 1.29 ng/ml m

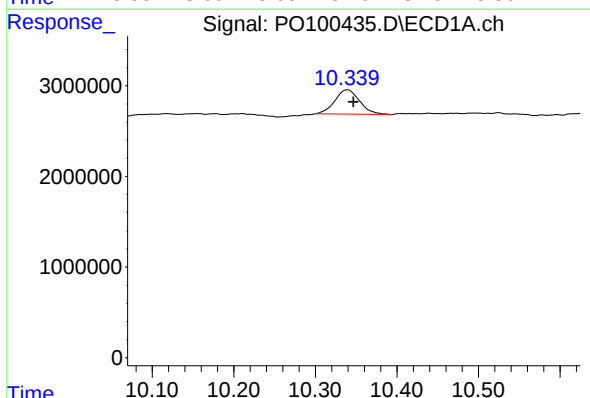

#2 Decachlorobiphenyl

R.T.: 10.339 min
Delta R.T.: -0.007 min
Response: 5666784
Conc: 4.06 ng/ml

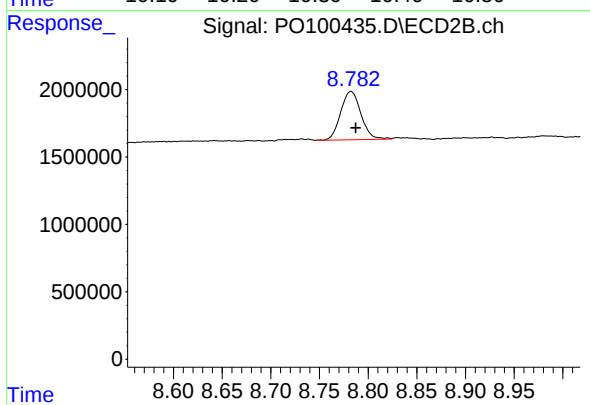

#2 Decachlorobiphenyl

R.T.: 8.782 min
Delta R.T.: -0.005 min
Response: 5203066
Conc: 3.22 ng/ml