

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0121124\
 Data File : P0108497.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Dec 2024 13:11
 Operator : YP/AJ
 Sample : P5219-03RE
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MR-CAM-012RE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/12/2024
 Supervised By :Ankita Jodhani 12/12/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 01:04:41 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 05:58:15 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.716	3.714	655.9E6	424.2E6	75.384m	83.676m
2) SA Decachlor...	8.793	8.742	68734736	50628205	9.410m	13.066m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121124\
Data File : PO108497.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Dec 2024 13:11
Operator : YP/AJ
Sample : P5219-03RE
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MR-CAM-012RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/12/2024
Supervised By :Ankita Jodhani 12/12/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 01:04:41 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 05:58:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

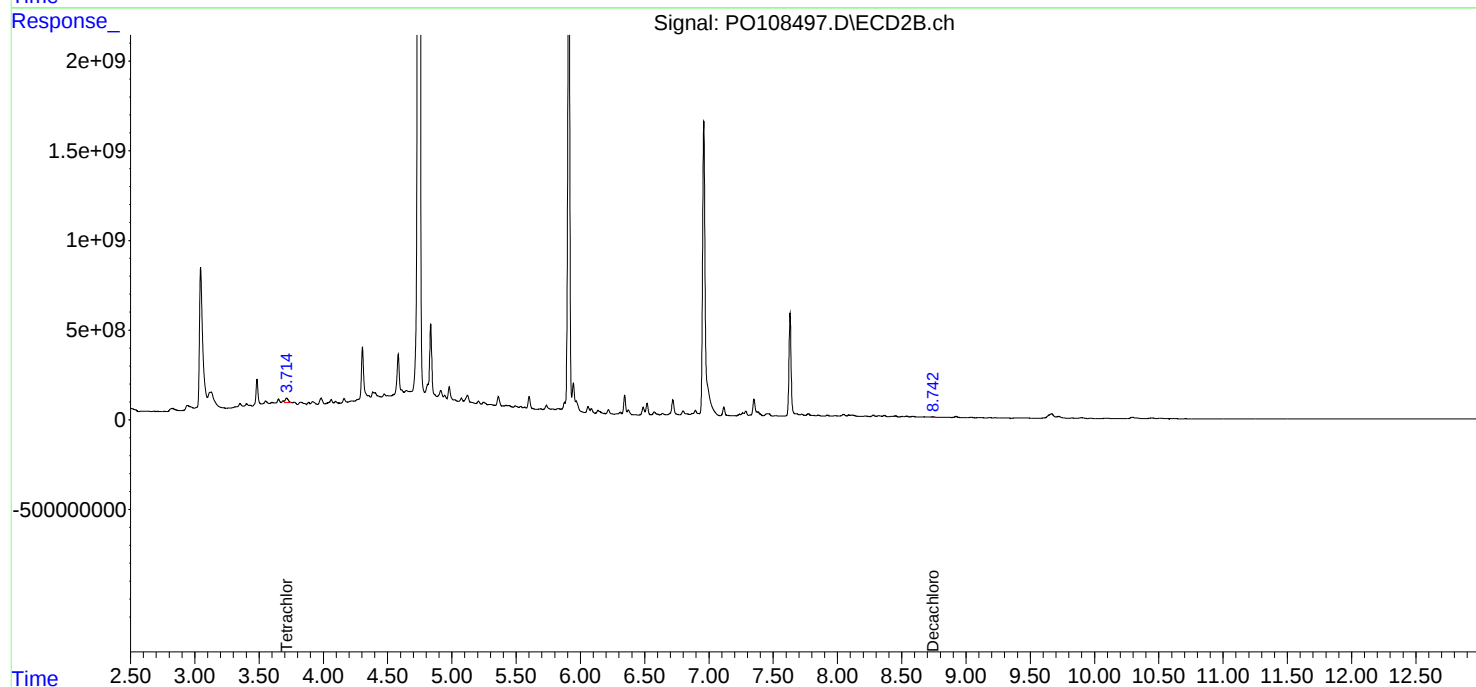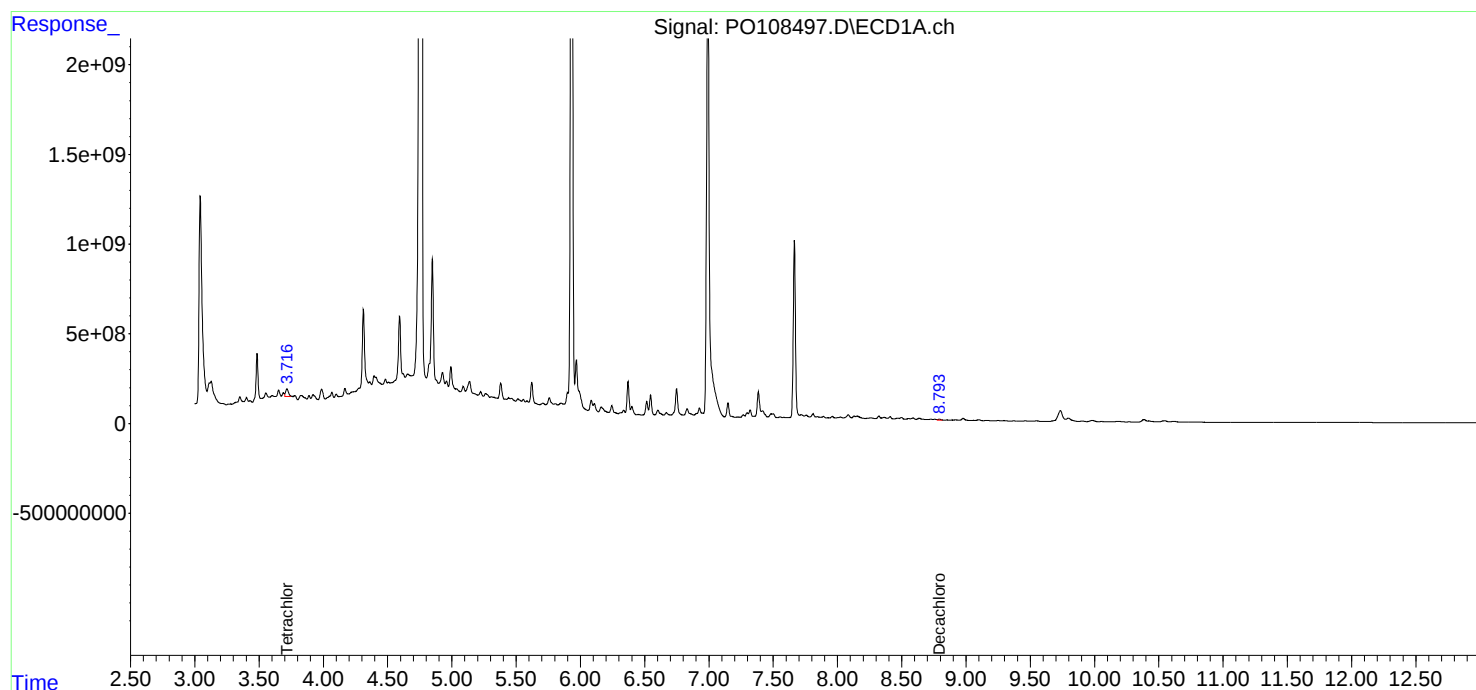

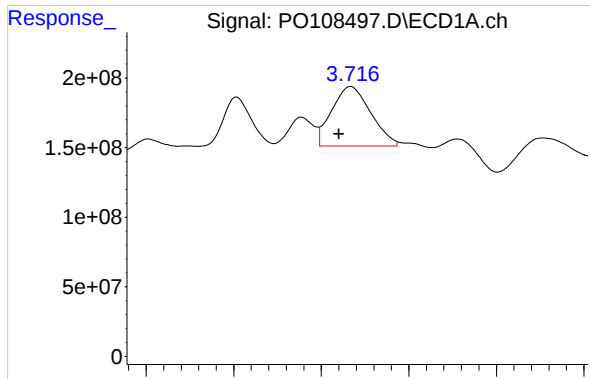


#1 Tetrachloro-m-xylene

R.T.: 3.716 min
Delta R.T.: 0.006 min
Response: 655851561
Conc: 75.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
MR-CAM-012RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/12/2024
Supervised By :Ankita Jodhani 12/12/2024

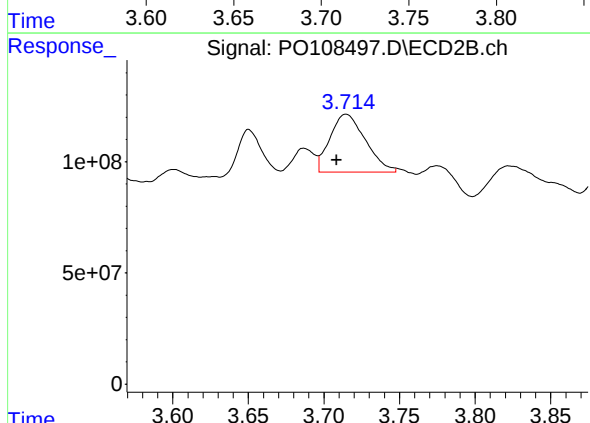


#1 Tetrachloro-m-xylene

R.T.: 3.714 min
Delta R.T.: 0.006 min
Response: 424186450
Conc: 83.68 ng/ml m

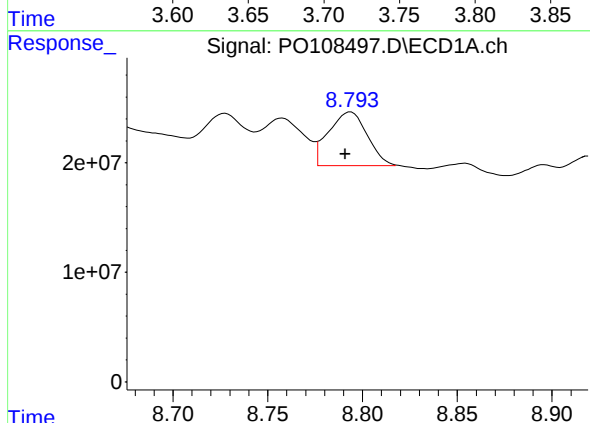

#2 Decachlorobiphenyl

R.T.: 8.793 min
Delta R.T.: 0.002 min
Response: 68734736
Conc: 9.41 ng/ml m

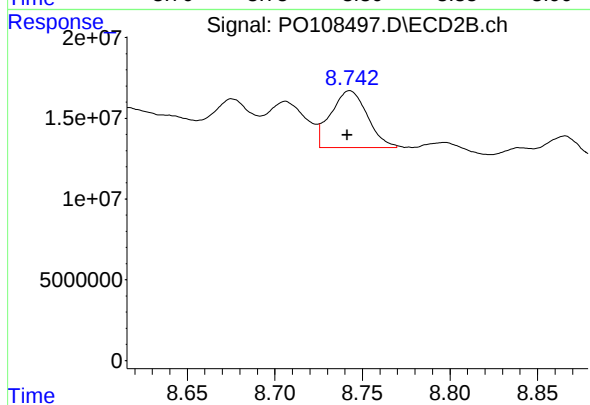

#2 Decachlorobiphenyl

R.T.: 8.742 min
Delta R.T.: 0.000 min
Response: 50628205
Conc: 13.07 ng/ml m