

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121125\
 Data File : PO115737.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Dec 2025 17:17
 Operator : YP/AJ
 Sample : Q3822-01 10X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AUD-25-0205

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 12/12/2025
 Supervised By :Yogesh Patel 12/12/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 01:12:59 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 05 02:11:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.335	3.637	11834311	9817483	1.524	2.015 #
2) SA Decachlor...	9.914	8.620	6013323	3447134	1.143	0.802m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121125\
Data File : PO115737.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Dec 2025 17:17
Operator : YP/AJ
Sample : Q3822-01 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AUD-25-0205


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 12/12/2025
Supervised By :Yogesh Patel 12/12/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 01:12:59 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120425.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 05 02:11:05 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

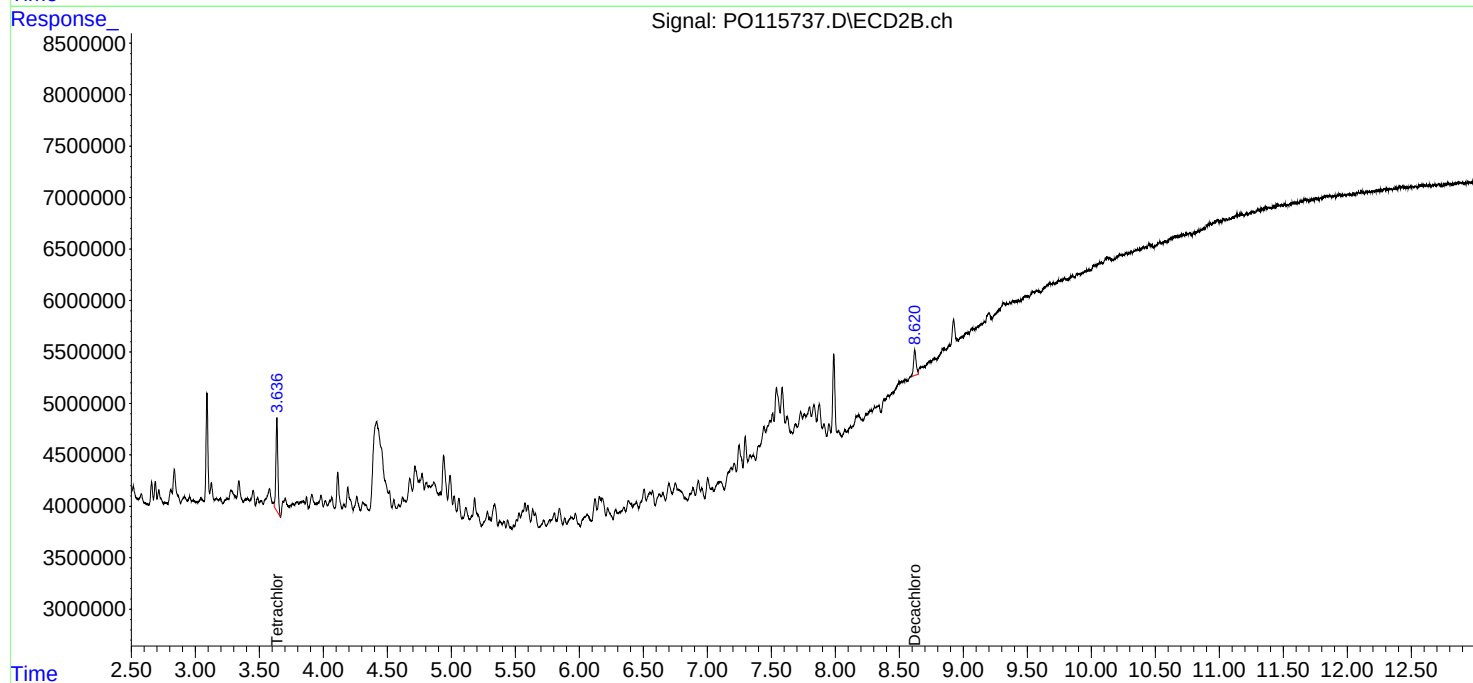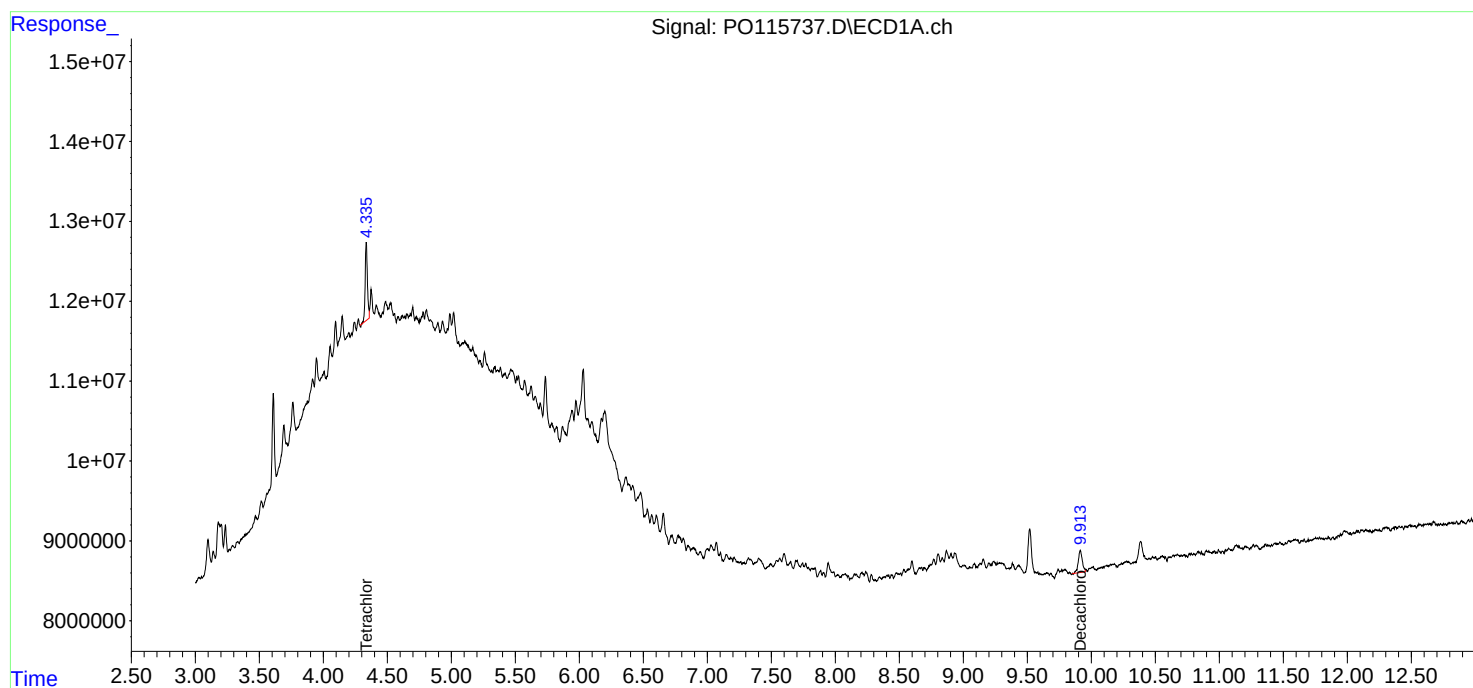

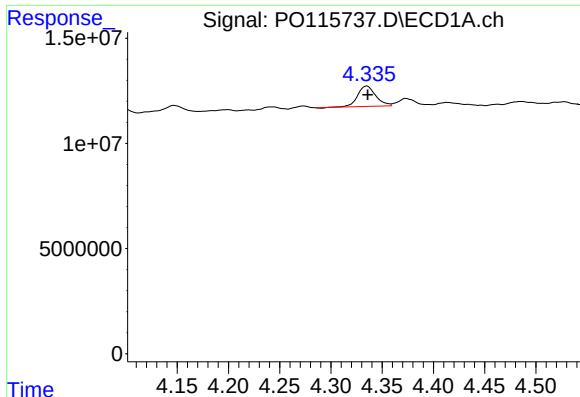

#1 Tetrachloro-m-xylene

R.T.: 4.335 min
Delta R.T.: 0.000 min
Response: 11834311
Conc: 1.52 ng/ml

Instrument :

ECD_O


ClientSampleId :

AUD-25-0205

Manual Integrations


APPROVED

Reviewed By :Rahul Chavli 12/12/2025
Supervised By :Yogesh Patel 12/12/2025

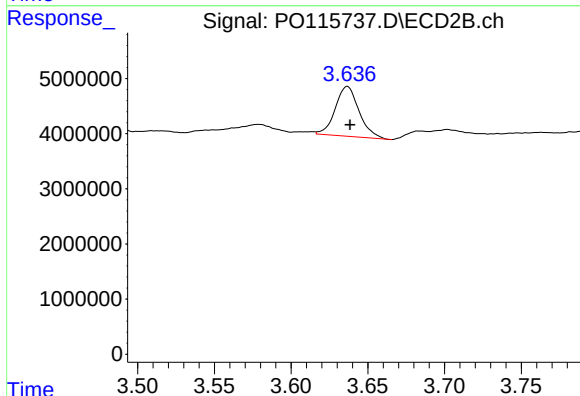


#1 Tetrachloro-m-xylene

R.T.: 3.637 min
Delta R.T.: -0.002 min
Response: 9817483
Conc: 2.01 ng/ml

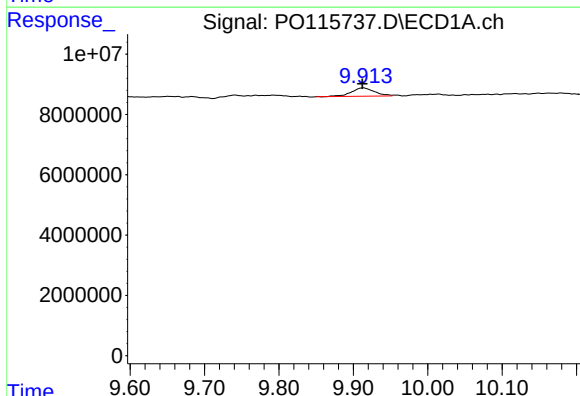

#2 Decachlorobiphenyl

R.T.: 9.914 min
Delta R.T.: 0.001 min
Response: 6013323
Conc: 1.14 ng/ml

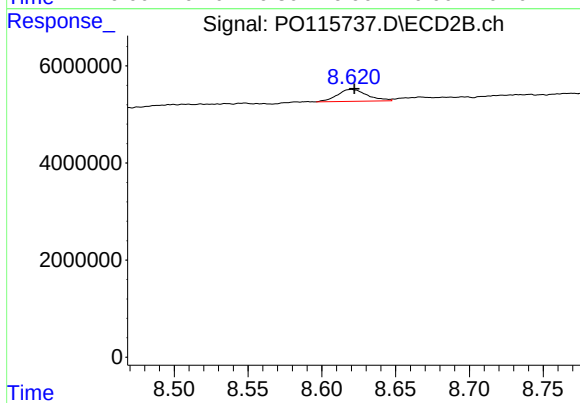

#2 Decachlorobiphenyl

R.T.: 8.620 min
Delta R.T.: -0.002 min
Response: 3447134
Conc: 0.80 ng/ml m