

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121222\
 Data File : PO091250.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Dec 2022 14:57
 Operator : YP/AJ
 Sample : N5964-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SU-518-COMP-03

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 20:34:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112522.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Nov 28 11:25:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.296	3.474	65145384	21169931	19.267	20.170
2) SA Decachlor...	10.041	8.474	46610731	19404160	17.548	19.986

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO121222\
Data File : PO091250.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Dec 2022 14:57
Operator : YP/AJ
Sample : N5964-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_0
ClientSampleId :
SU-518-COMP-03

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 20:34:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO112522.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Nov 28 11:25:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

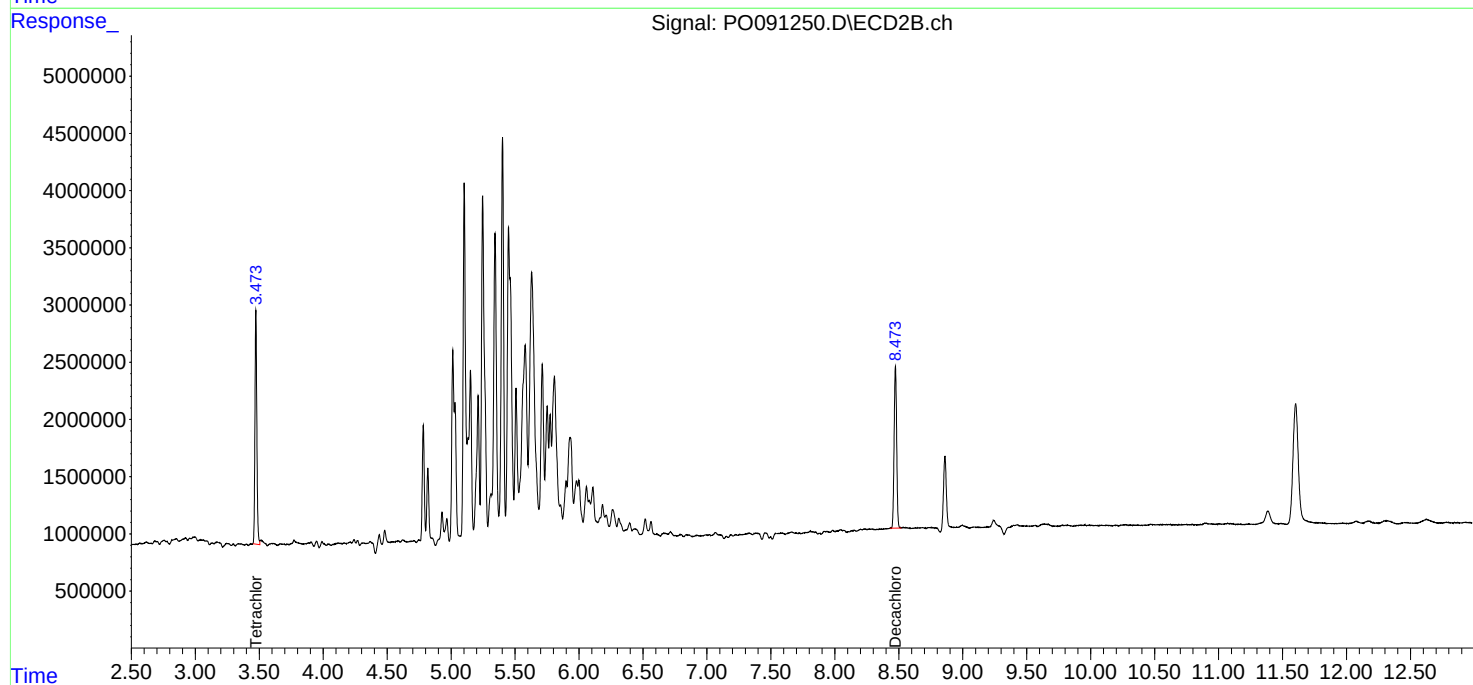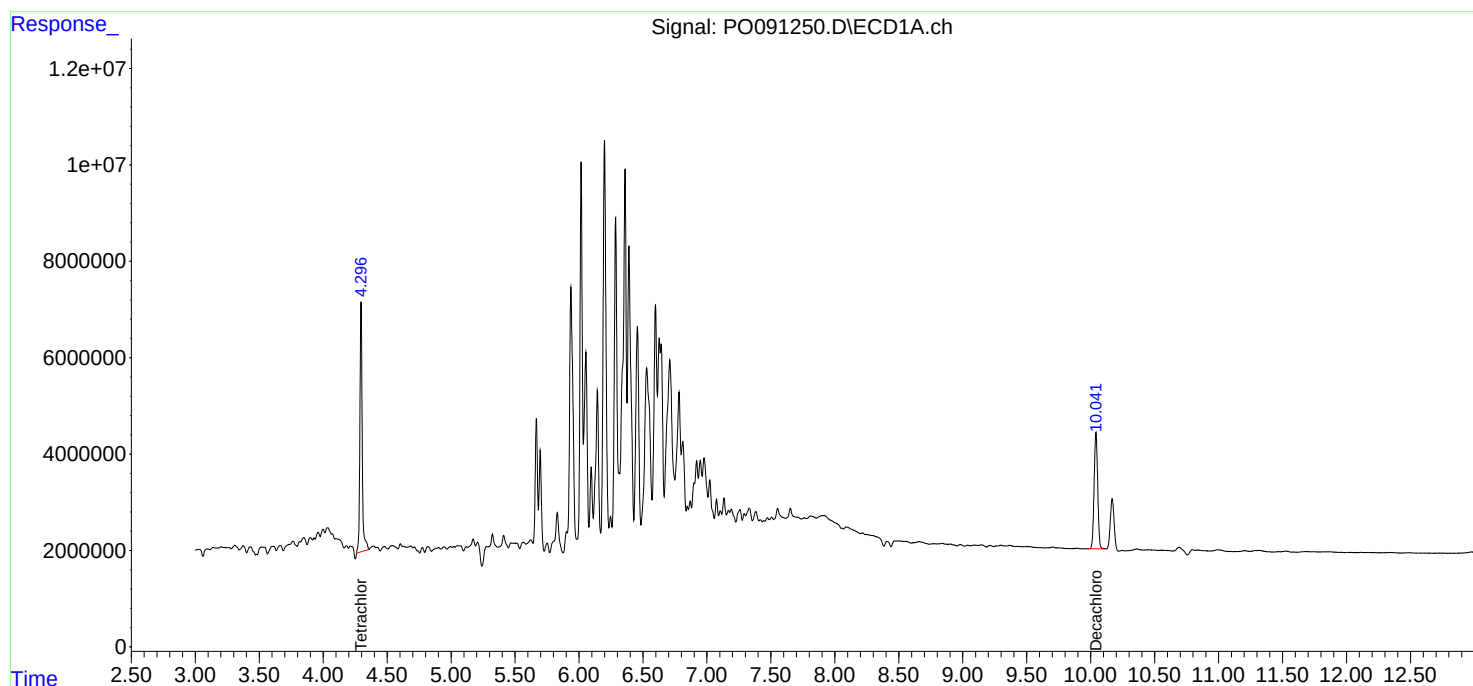


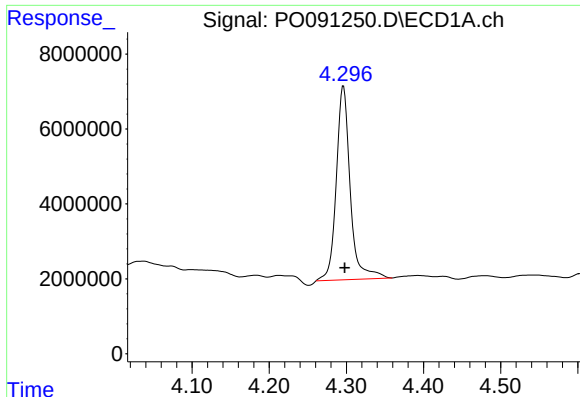

#1 Tetrachloro-m-xylene


R.T.: 4.296 min
Delta R.T.: -0.002 min
Response: 65145384
Conc: 19.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU-518-COMP-03

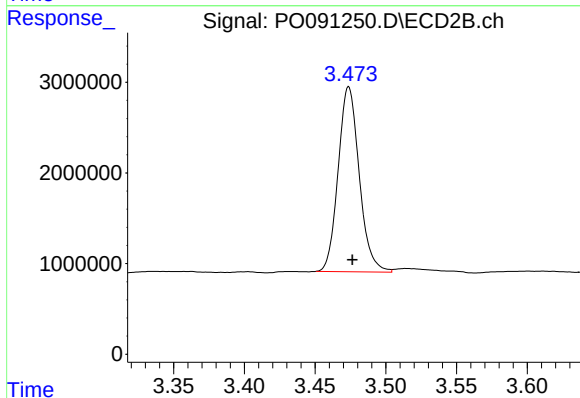


#1 Tetrachloro-m-xylene

R.T.: 3.474 min
Delta R.T.: -0.002 min
Response: 21169931
Conc: 20.17 ng/ml

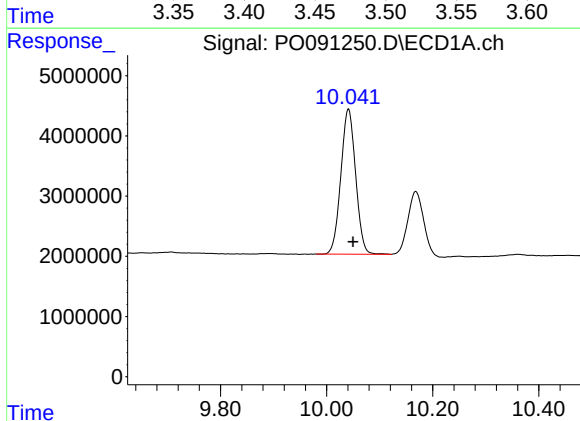

#2 Decachlorobiphenyl

R.T.: 10.041 min
Delta R.T.: -0.009 min
Response: 46610731
Conc: 17.55 ng/ml

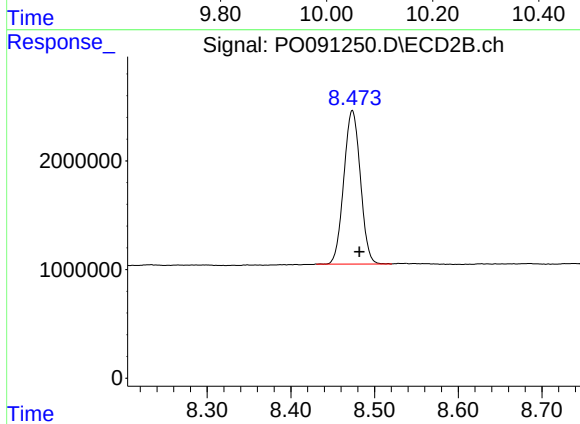

#2 Decachlorobiphenyl

R.T.: 8.474 min
Delta R.T.: -0.008 min
Response: 19404160
Conc: 19.99 ng/ml