

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0121224\
 Data File : P0108533.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Dec 2024 17:04
 Operator : YP/AJ
 Sample : P5243-01RE 10X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 1203RE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/13/2024
 Supervised By :Ankita Jodhani 12/13/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 13 01:26:31 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 05:58:15 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.716	3.712	52410723	19817277	6.024m	3.909m#
2) SA Decachlor...	8.780	8.728	9392477	6495880	1.286	1.676 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121224\
Data File : PO108533.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Dec 2024 17:04
Operator : YP/AJ
Sample : P5243-01RE 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
1203RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/13/2024
Supervised By :Ankita Jodhani 12/13/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 13 01:26:31 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 05:58:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

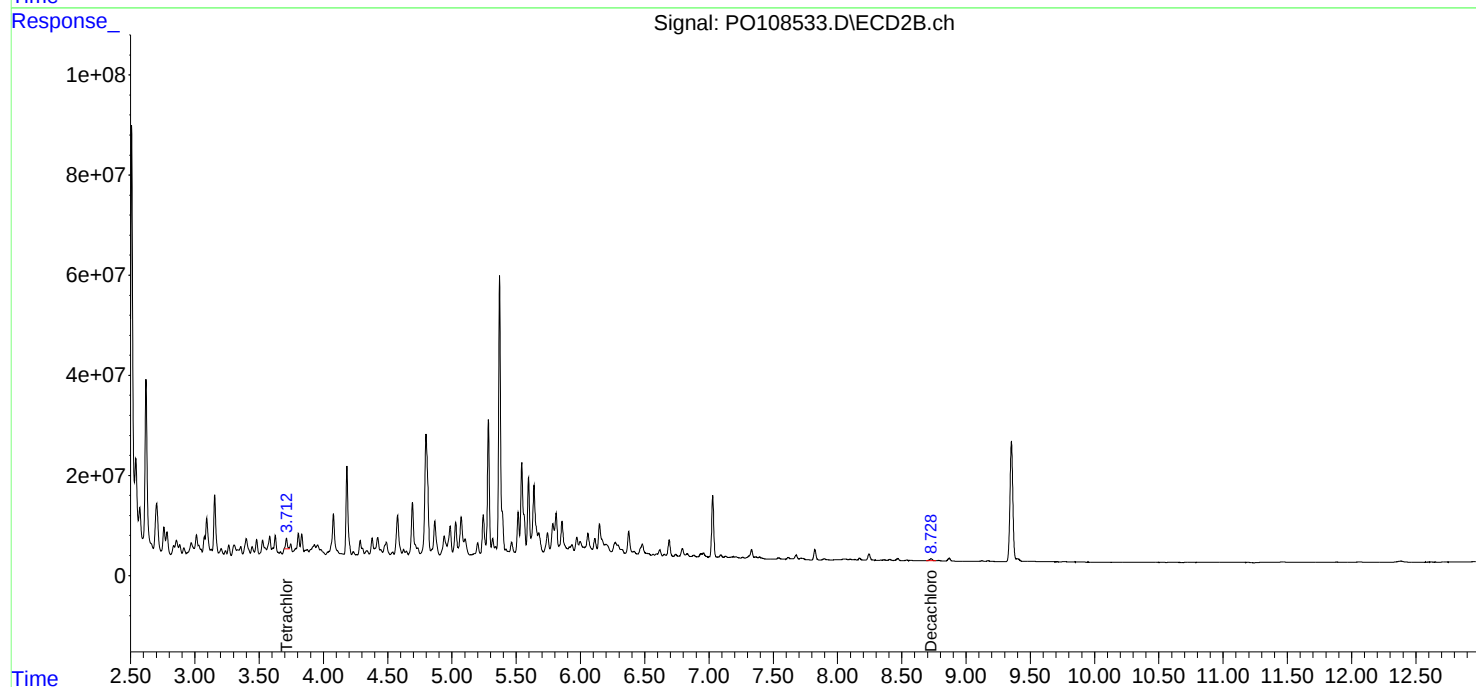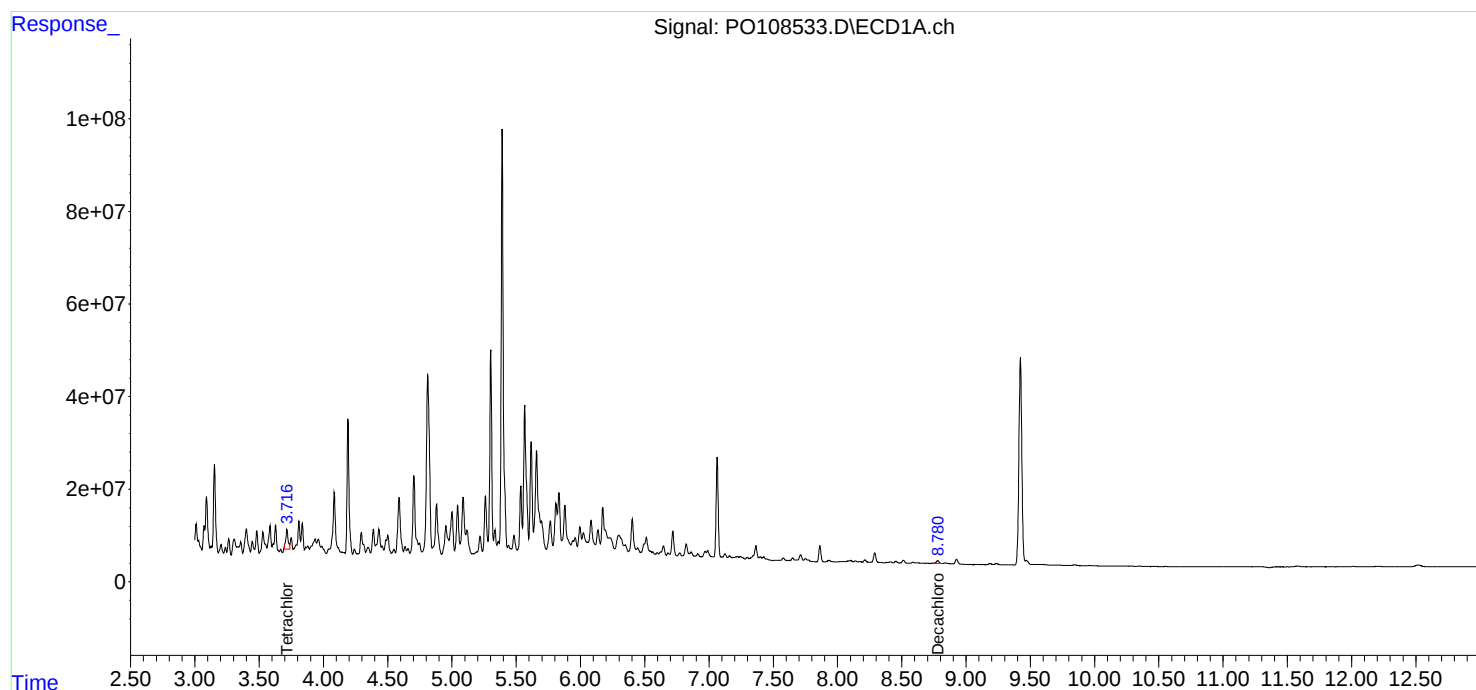

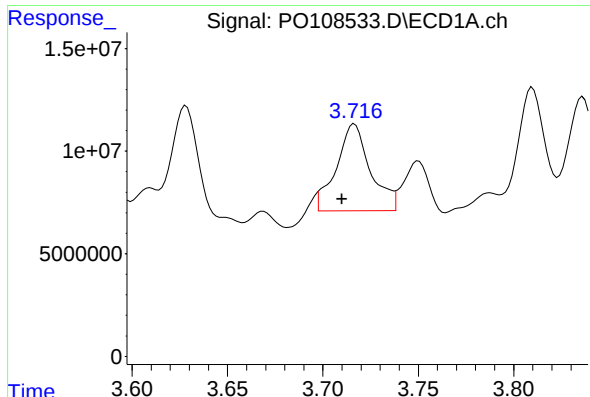

#1 Tetrachloro-m-xylene

R.T.: 3.716 min
Delta R.T.: 0.006 min
Response: 52410723
Conc: 6.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
1203RE

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/13/2024
Supervised By :Ankita Jodhani 12/13/2024

#1 Tetrachloro-m-xylene

R.T.: 3.712 min
Delta R.T.: 0.004 min
Response: 19817277
Conc: 3.91 ng/ml m

#2 Decachlorobiphenyl

R.T.: 8.780 min
Delta R.T.: -0.011 min
Response: 9392477
Conc: 1.29 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.728 min
Delta R.T.: -0.014 min
Response: 6495880
Conc: 1.68 ng/ml