

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0121225\
 Data File : P0115776.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Dec 2025 01:39
 Operator : YP/AJ
 Sample : Q3530-07
 Misc : AR1660 25PPB WATER LOD
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 13 03:48:38 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0120425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 05 02:11:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.333	3.636	141.3E6	85788058	18.197	17.604
2)	SA Decachlor...	9.905	8.615	100.2E6	74542088	19.042	17.335
Target Compounds							
3)	L1 AR-1016-1	5.472	4.711	5686137	5291538	22.867	28.639 #
4)	L1 AR-1016-2	5.494	4.729	8002787	6587200	21.013	24.922
5)	L1 AR-1016-3	5.555	4.903	4616522	5884330	21.594	38.882 #
6)	L1 AR-1016-4	5.650	4.939	3252185	1212907	18.212	10.762 #
7)	L1 AR-1016-5	5.941	5.158	10727048	12612335	61.148	86.185 #
8)	L2 AR-1221-1	4.529	3.847	6799936	278805	83.746	4.943 #
9)	L2 AR-1221-2	4.629	3.933	2779165	2140801	44.101	50.438
10)	L2 AR-1221-3	4.690	4.005	4262446	1960916	22.828	15.249 #
11)	L3 AR-1232-1	4.690	4.005	4262446	1960916	28.480	18.354 #
12)	L3 AR-1232-2	5.209	4.729	5406209	6587200	66.867	59.350
13)	L3 AR-1232-3	5.494	4.903	8002787	5884330	51.999	90.021 #
14)	L3 AR-1232-4	5.650	4.988	3252185	4714987	46.440	91.856 #
15)	L3 AR-1232-5	5.742	5.158	4420040	12612335	85.104	230.370 #
16)	L4 AR-1242-1	5.472	4.711	5686137	5291538	28.628	37.163 #
17)	L4 AR-1242-2	5.494	4.729	8002787	6587200	27.323	31.463
18)	L4 AR-1242-3	5.555	4.903	4616522	5884330	27.346	49.265 #
19)	L4 AR-1242-4	5.650	4.988	3252185	4714987	23.796	43.220 #
20)	L4 AR-1242-5	6.378	5.508	14568563	4995570	96.198	36.167 #
21)	L5 AR-1248-1	5.472	4.711	5686137	5291538	37.466	47.318 #
22)	L5 AR-1248-2	5.742	4.939	4420040	1212907	22.011	7.964 #
23)	L5 AR-1248-3	5.941	4.988	10727048	4714987	43.500	29.372 #
24)	L5 AR-1248-4	6.340	5.158	9692340	12612335	32.872	67.393 #
25)	L5 AR-1248-5	6.378	5.530	14568563	17473120	56.265	88.268 #
26)	L6 AR-1254-1	6.302	5.508	8240427	4995570	31.852	17.092 #
27)	L6 AR-1254-2	6.529	5.654	14374378	11615488	35.721	46.127 #
28)	L6 AR-1254-3	6.880	6.071	42022079	19144178	102.352	48.641 #
29)	L6 AR-1254-4	7.173	6.288	13824579	4529644	39.833	16.928 #
30)	L6 AR-1254-5	7.585	6.698	17768812	8009810	54.835	22.403 #
31)	L7 AR-1260-1	7.054	6.185	20915011	14610333	72.196	55.729
32)	L7 AR-1260-2	7.309	6.373	18923397	7893750	43.231	22.524 #
33)	L7 AR-1260-3	7.666	6.525	12578541	8876697	37.370	27.630 #
34)	L7 AR-1260-4	7.889	6.995	13142885	5951430	42.745	23.172 #
35)	L7 AR-1260-5	8.194	7.236	19890128	14731912	27.304	21.007
36)	L8 AR-1262-1	7.666	6.738	12578541	7393481	50.955	34.704 #
37)	L8 AR-1262-2	8.194	7.236	19890128	14731912	50.240	42.293
38)	L8 AR-1262-3	8.499	7.528	10113064	59981842	39.687	383.539 #
39)	L8 AR-1262-4	8.577	7.580	3063425	34027714	15.815	137.557 #
40)	L8 AR-1262-5	9.195	8.076	4136088	2632193	30.708	23.612
41)	L9 AR-1268-1	8.499	7.528	10113064	59981842	10.157	67.703 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121225\
 Data File : PO115776.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Dec 2025 01:39
 Operator : YP/AJ
 Sample : Q3530-07
 Misc : AR1660 25PPB WATER LOD
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 13 03:48:38 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 05 02:11:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.577	7.580	3063425	34027714	3.581	45.427 #
43) L9	AR-1268-3	8.812	7.800	263278	58884	0.354	0.092 #
44) L9	AR-1268-4	9.195	8.076	4136088	2632193	13.247	10.217
45) L9	AR-1268-5	9.586	8.362	2380785	1161347	1.093	0.689 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121225\
Data File : PO115776.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Dec 2025 01:39
Operator : YP/AJ
Sample : Q3530-07
Misc : AR1660 25PPB WATER LOD
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 13 03:48:38 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120425.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 05 02:11:05 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

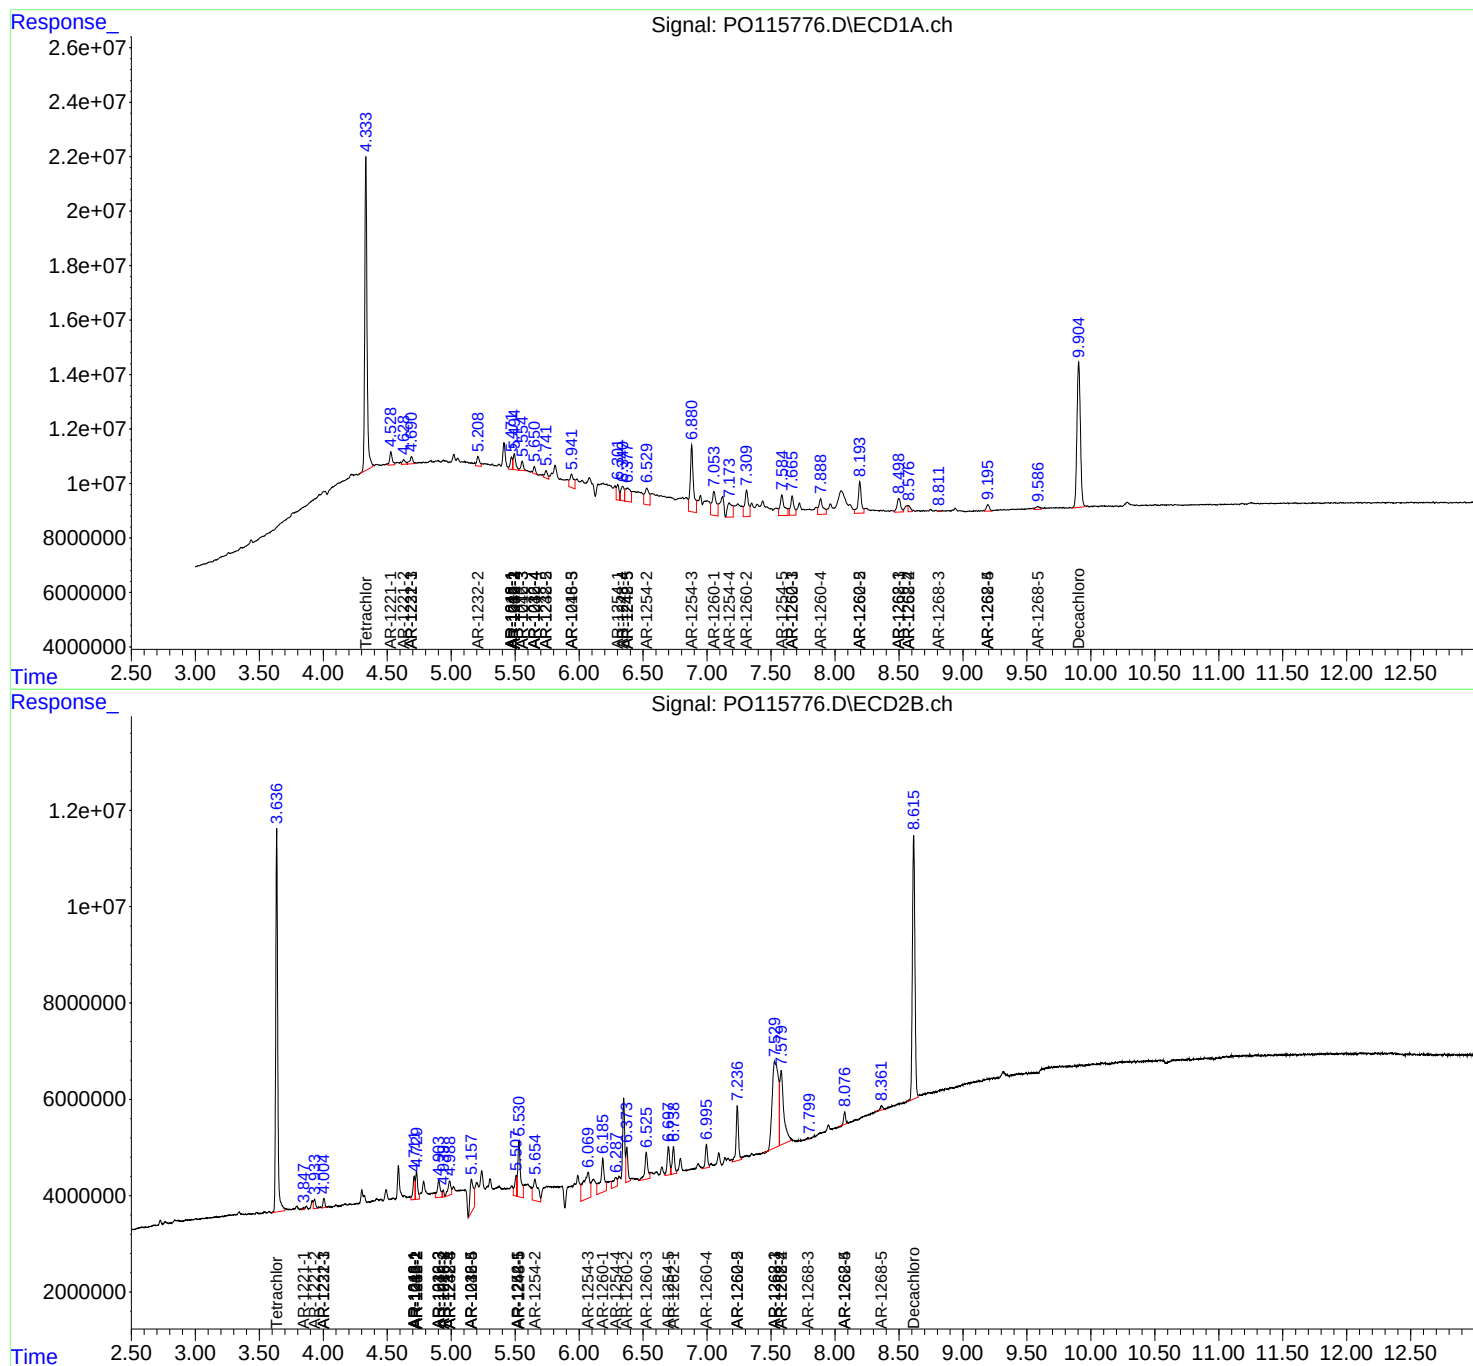


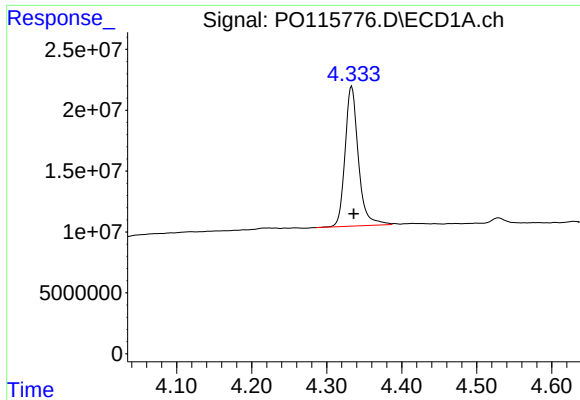

#1 Tetrachloro-m-xylene


R.T.: 4.333 min
Delta R.T.: -0.003 min
Response: 141340424
Conc: 18.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

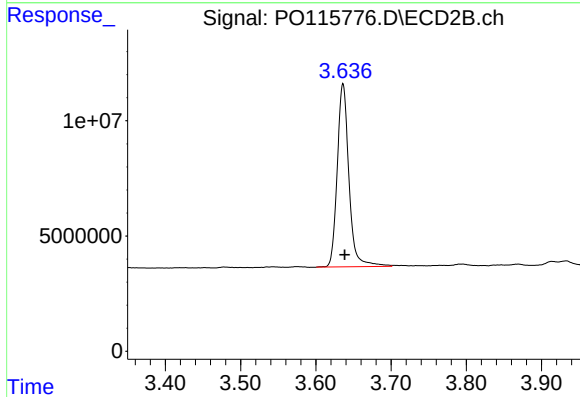


#1 Tetrachloro-m-xylene

R.T.: 3.636 min
Delta R.T.: -0.002 min
Response: 85788058
Conc: 17.60 ng/ml

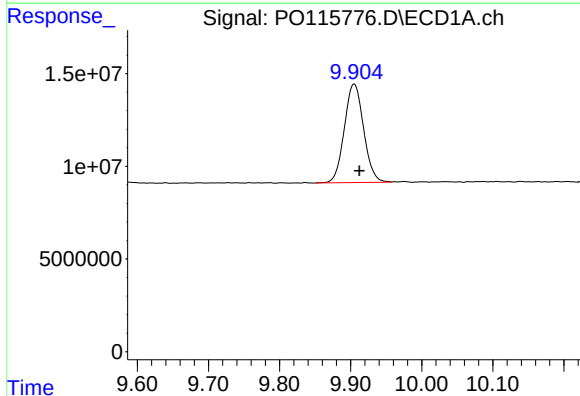


#2 Decachlorobiphenyl

R.T.: 9.905 min
Delta R.T.: -0.007 min
Response: 100181615
Conc: 19.04 ng/ml

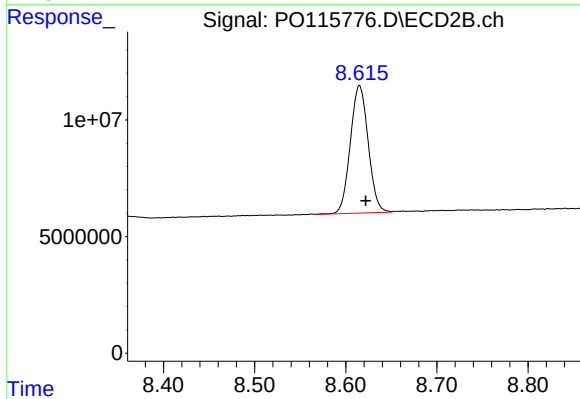

#2 Decachlorobiphenyl


R.T.: 8.615 min
Delta R.T.: -0.007 min
Response: 74542088
Conc: 17.33 ng/ml

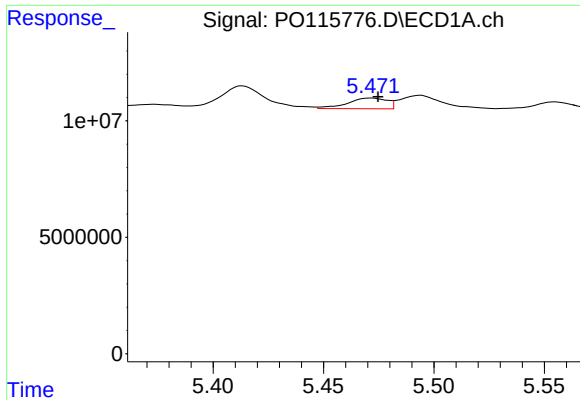

#3 AR-1016-1


R.T.: 5.472 min
Delta R.T.: -0.003 min
Response: 5686137
Conc: 22.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

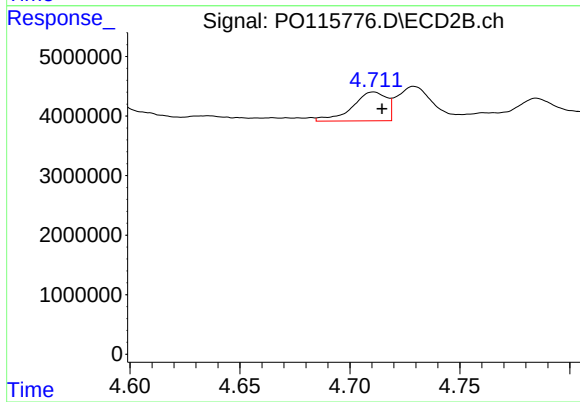


#3 AR-1016-1

R.T.: 4.711 min
Delta R.T.: -0.004 min
Response: 5291538
Conc: 28.64 ng/ml

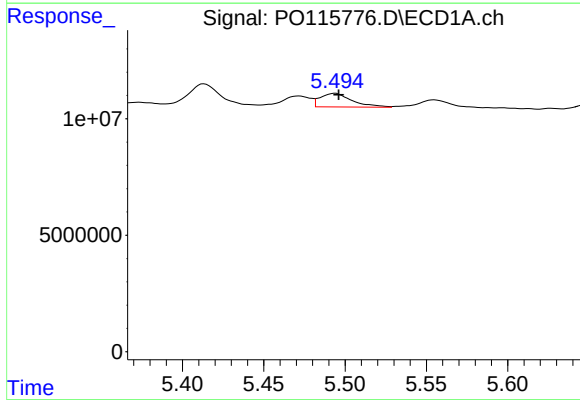


#4 AR-1016-2

R.T.: 5.494 min
Delta R.T.: -0.002 min
Response: 8002787
Conc: 21.01 ng/ml

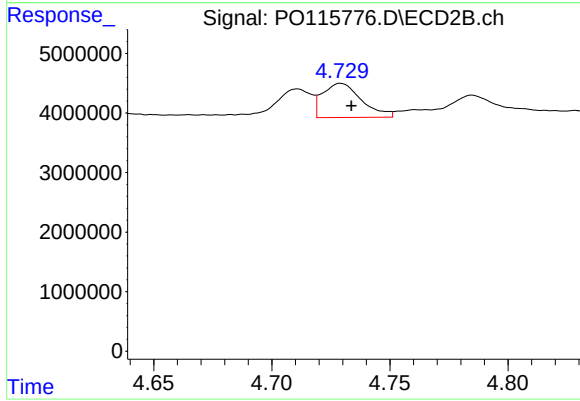

#4 AR-1016-2


R.T.: 4.729 min
Delta R.T.: -0.004 min
Response: 6587200
Conc: 24.92 ng/ml

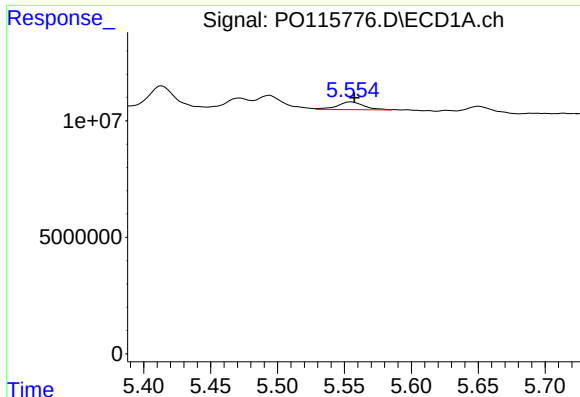

#5 AR-1016-3


R.T.: 5.555 min
Delta R.T.: -0.003 min
Response: 4616522
Conc: 21.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

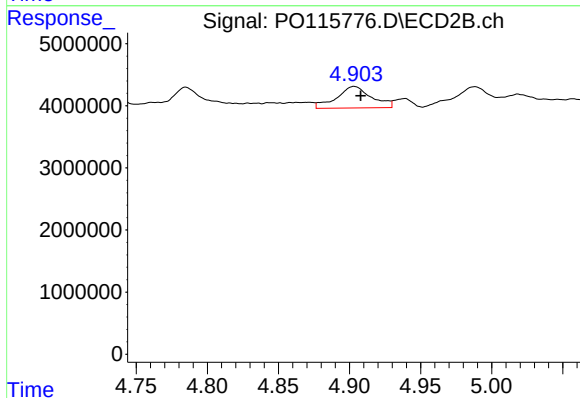


#5 AR-1016-3

R.T.: 4.903 min
Delta R.T.: -0.005 min
Response: 5884330
Conc: 38.88 ng/ml

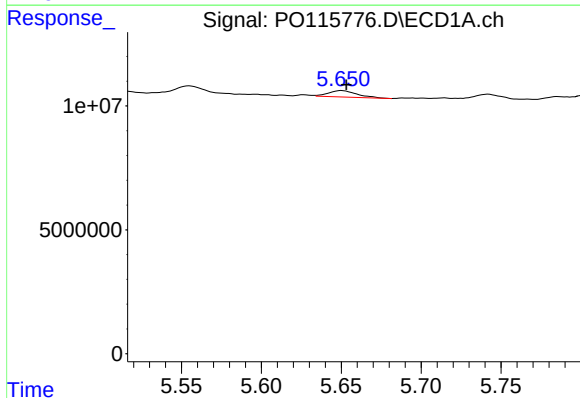


#6 AR-1016-4

R.T.: 5.650 min
Delta R.T.: -0.003 min
Response: 3252185
Conc: 18.21 ng/ml

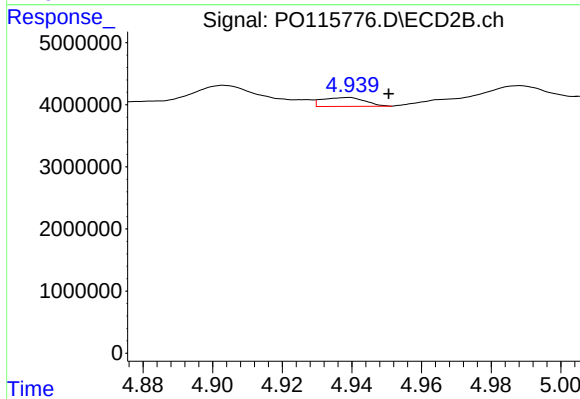

#6 AR-1016-4


R.T.: 4.939 min
Delta R.T.: -0.011 min
Response: 1212907
Conc: 10.76 ng/ml

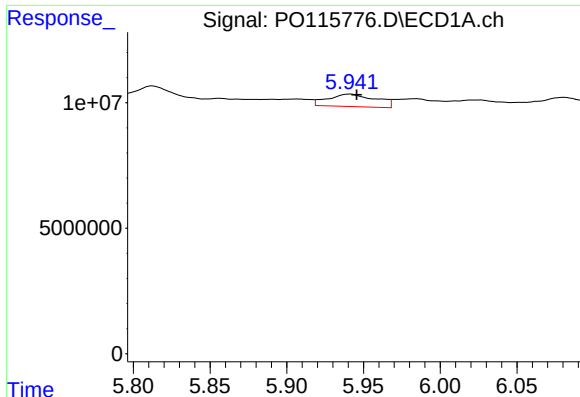

#7 AR-1016-5


R.T.: 5.941 min
Delta R.T.: -0.004 min
Response: 10727048
Conc: 61.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

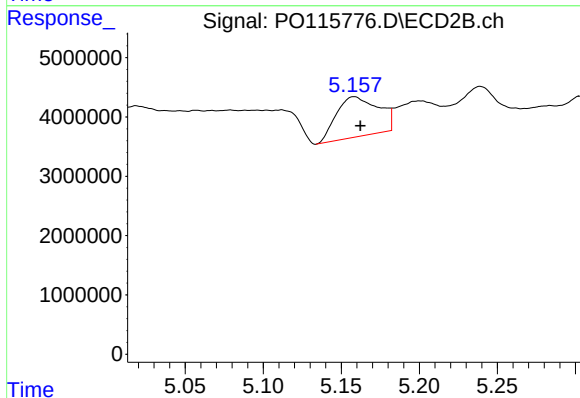


#7 AR-1016-5

R.T.: 5.158 min
Delta R.T.: -0.004 min
Response: 12612335
Conc: 86.18 ng/ml

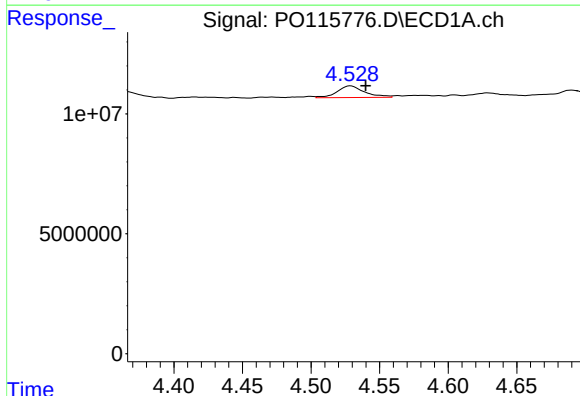


#8 AR-1221-1

R.T.: 4.529 min
Delta R.T.: -0.011 min
Response: 6799936
Conc: 83.75 ng/ml

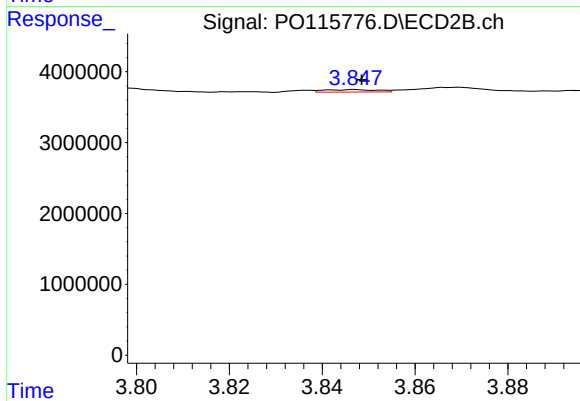

#8 AR-1221-1


R.T.: 3.847 min
Delta R.T.: -0.001 min
Response: 278805
Conc: 4.94 ng/ml

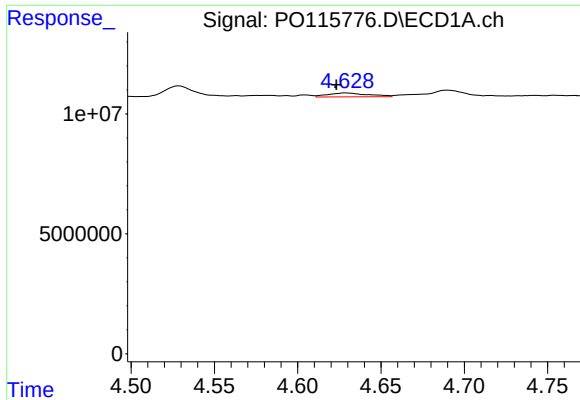

#9 AR-1221-2


R.T.: 4.629 min
Delta R.T.: 0.006 min
Response: 2779165
Conc: 44.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

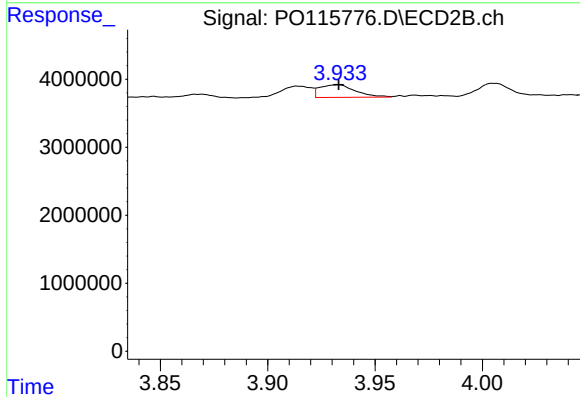


#9 AR-1221-2

R.T.: 3.933 min
Delta R.T.: 0.000 min
Response: 2140801
Conc: 50.44 ng/ml

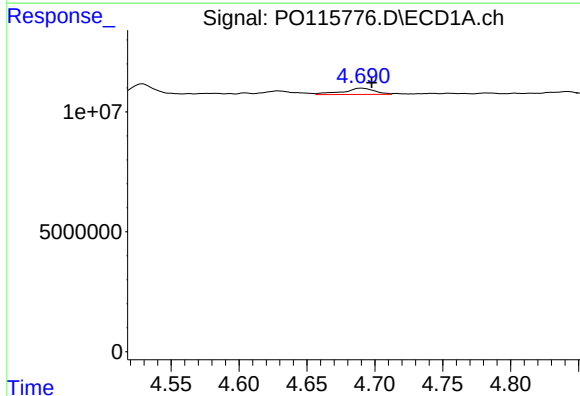


#10 AR-1221-3

R.T.: 4.690 min
Delta R.T.: -0.007 min
Response: 4262446
Conc: 22.83 ng/ml

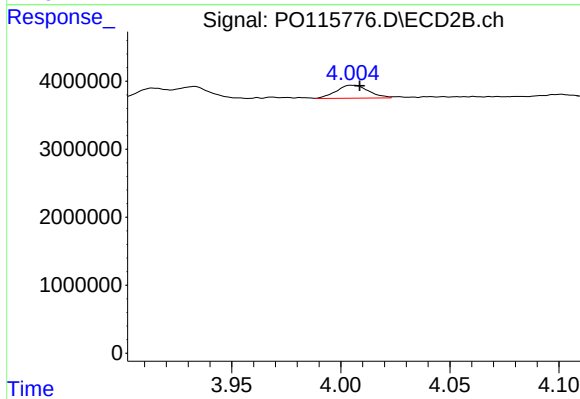

#10 AR-1221-3


R.T.: 4.005 min
Delta R.T.: -0.004 min
Response: 1960916
Conc: 15.25 ng/ml

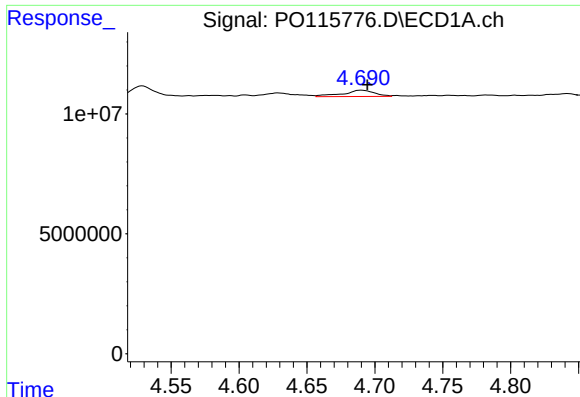

#11 AR-1232-1


R.T.: 4.690 min
Delta R.T.: -0.004 min
Response: 4262446
Conc: 28.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

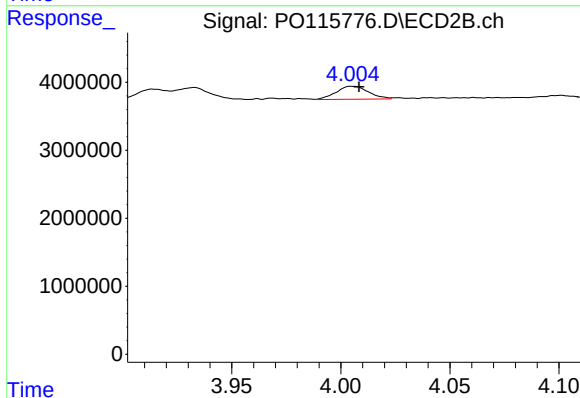


#11 AR-1232-1

R.T.: 4.005 min
Delta R.T.: -0.003 min
Response: 1960916
Conc: 18.35 ng/ml

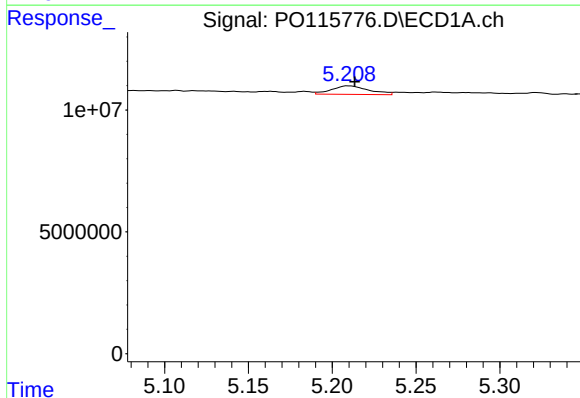


#12 AR-1232-2

R.T.: 5.209 min
Delta R.T.: -0.004 min
Response: 5406209
Conc: 66.87 ng/ml

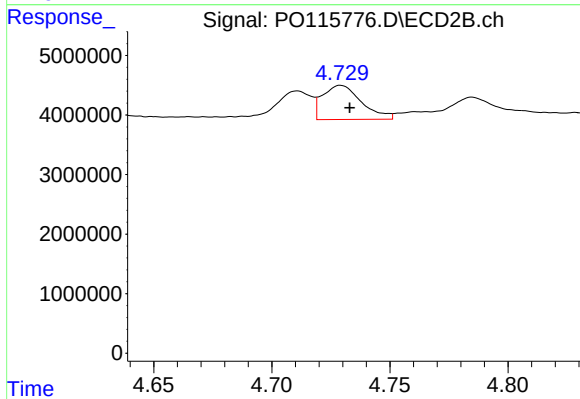

#12 AR-1232-2


R.T.: 4.729 min
Delta R.T.: -0.004 min
Response: 6587200
Conc: 59.35 ng/ml

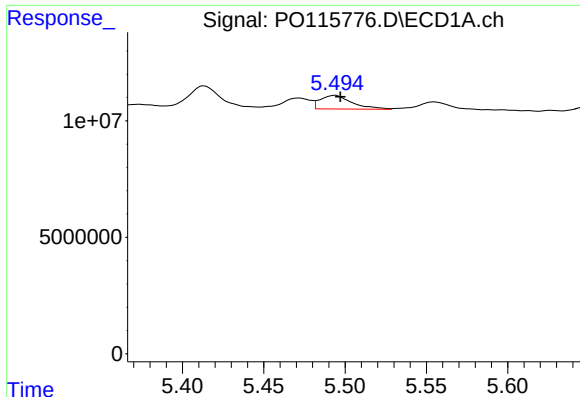

#13 AR-1232-3


R.T.: 5.494 min
Delta R.T.: -0.003 min
Response: 8002787
Conc: 52.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

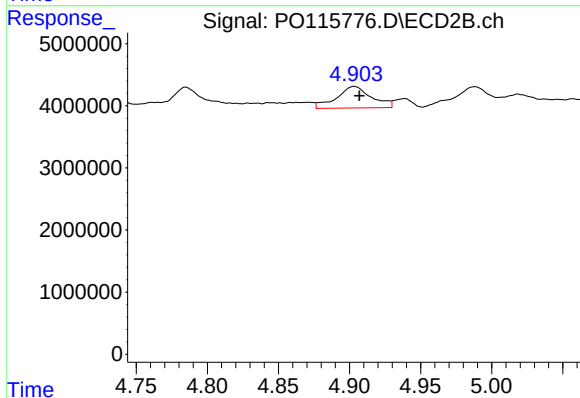


#13 AR-1232-3

R.T.: 4.903 min
Delta R.T.: -0.004 min
Response: 5884330
Conc: 90.02 ng/ml

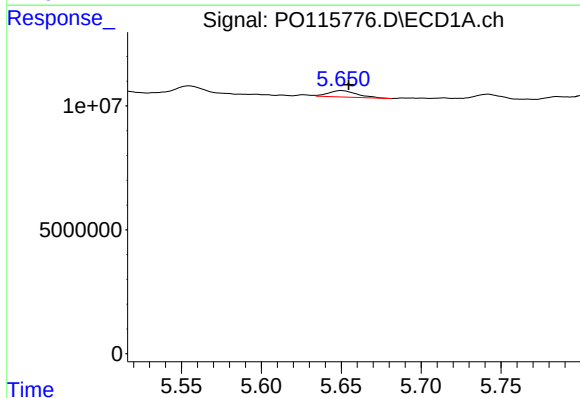


#14 AR-1232-4

R.T.: 5.650 min
Delta R.T.: -0.005 min
Response: 3252185
Conc: 46.44 ng/ml

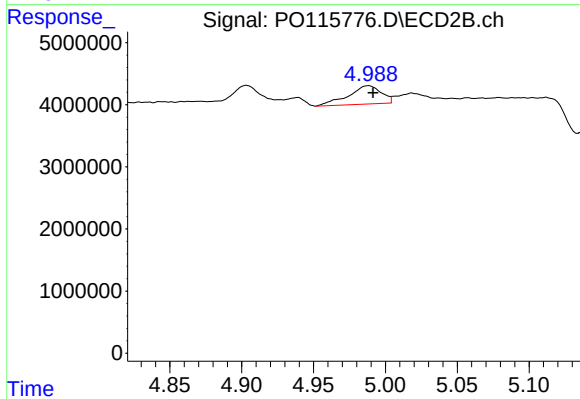

#14 AR-1232-4


R.T.: 4.988 min
Delta R.T.: -0.003 min
Response: 4714987
Conc: 91.86 ng/ml

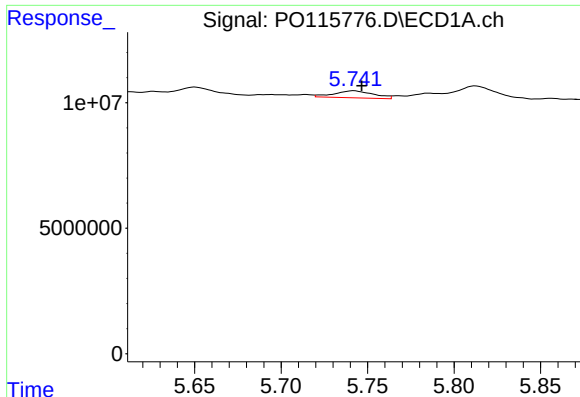

#15 AR-1232-5


R.T.: 5.742 min
Delta R.T.: -0.005 min
Response: 4420040
Conc: 85.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

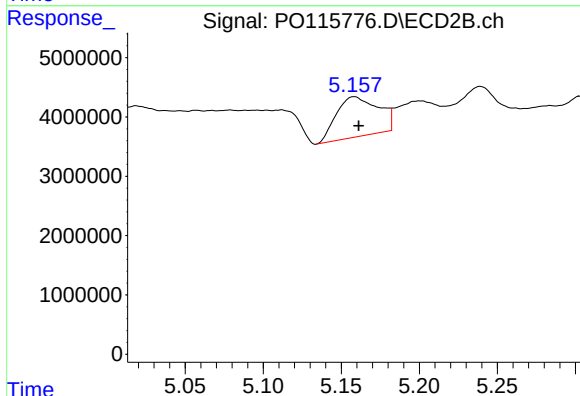


#15 AR-1232-5

R.T.: 5.158 min
Delta R.T.: -0.003 min
Response: 12612335
Conc: 230.37 ng/ml

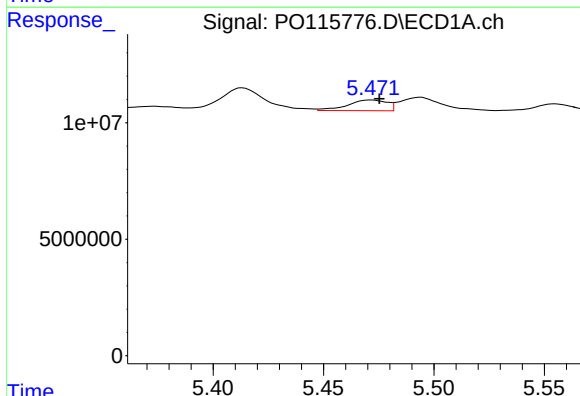


#16 AR-1242-1

R.T.: 5.472 min
Delta R.T.: -0.003 min
Response: 5686137
Conc: 28.63 ng/ml

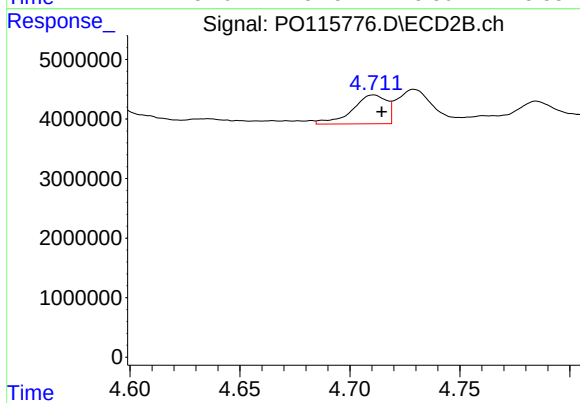

#16 AR-1242-1


R.T.: 4.711 min
Delta R.T.: -0.004 min
Response: 5291538
Conc: 37.16 ng/ml

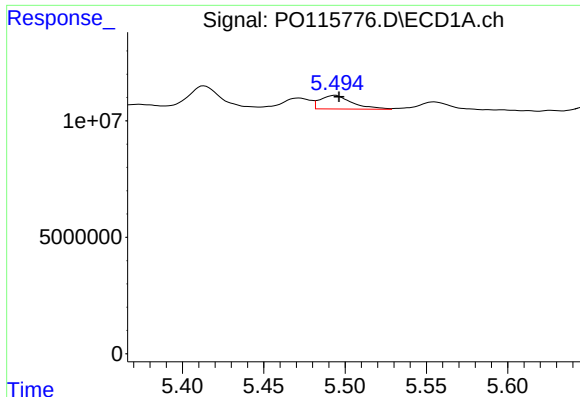

#17 AR-1242-2


R.T.: 5.494 min
Delta R.T.: -0.002 min
Response: 8002787
Conc: 27.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

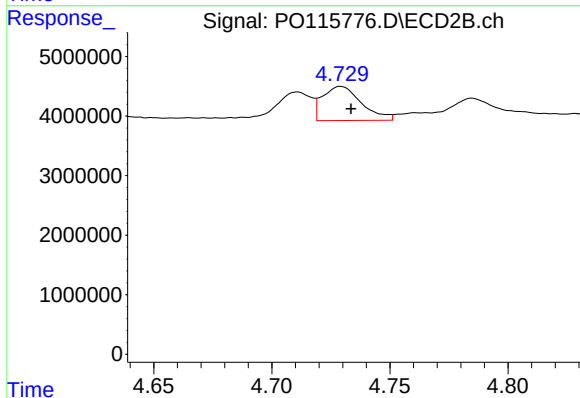


#17 AR-1242-2

R.T.: 4.729 min
Delta R.T.: -0.004 min
Response: 6587200
Conc: 31.46 ng/ml

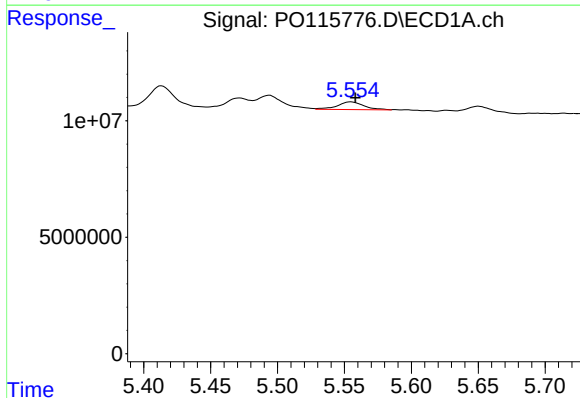


#18 AR-1242-3

R.T.: 5.555 min
Delta R.T.: -0.003 min
Response: 4616522
Conc: 27.35 ng/ml

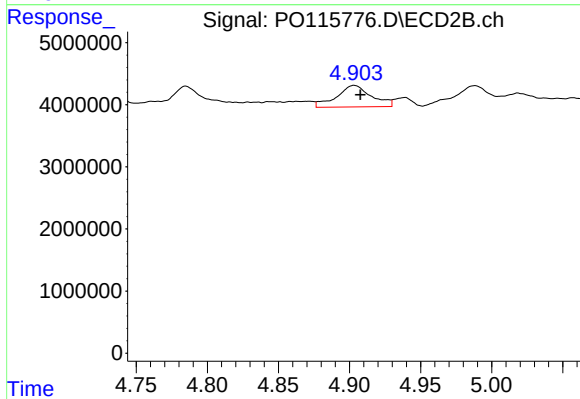

#18 AR-1242-3


R.T.: 4.903 min
Delta R.T.: -0.004 min
Response: 5884330
Conc: 49.27 ng/ml

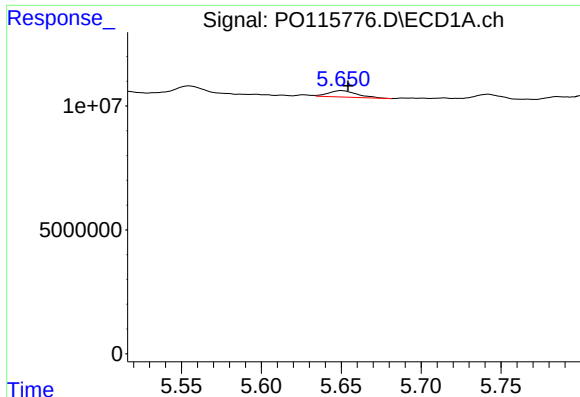

#19 AR-1242-4


R.T.: 5.650 min
Delta R.T.: -0.004 min
Response: 3252185
Conc: 23.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

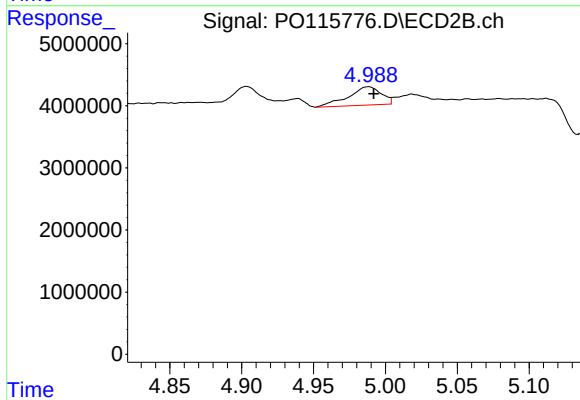


#19 AR-1242-4

R.T.: 4.988 min
Delta R.T.: -0.004 min
Response: 4714987
Conc: 43.22 ng/ml

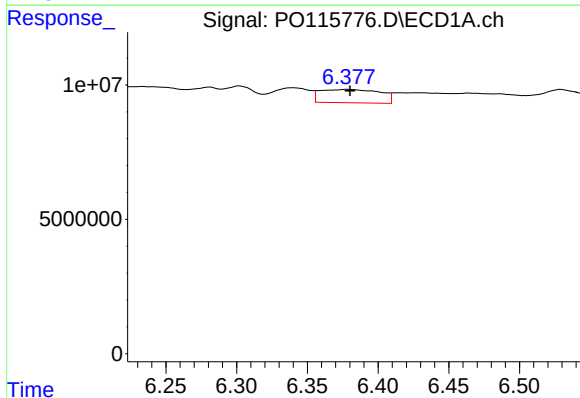


#20 AR-1242-5

R.T.: 6.378 min
Delta R.T.: -0.002 min
Response: 14568563
Conc: 96.20 ng/ml

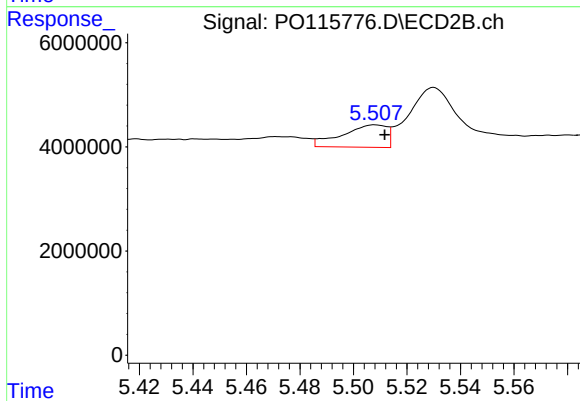

#20 AR-1242-5


R.T.: 5.508 min
Delta R.T.: -0.004 min
Response: 4995570
Conc: 36.17 ng/ml

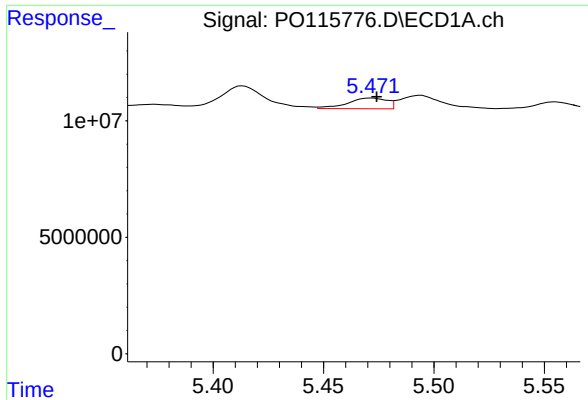

#21 AR-1248-1


R.T.: 5.472 min
Delta R.T.: -0.002 min
Response: 5686137
Conc: 37.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

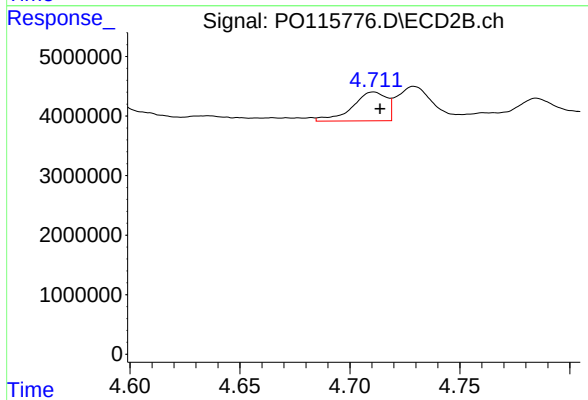


#21 AR-1248-1

R.T.: 4.711 min
Delta R.T.: -0.003 min
Response: 5291538
Conc: 47.32 ng/ml

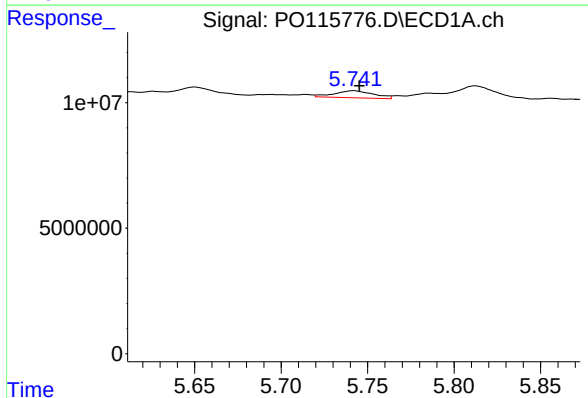


#22 AR-1248-2

R.T.: 5.742 min
Delta R.T.: -0.003 min
Response: 4420040
Conc: 22.01 ng/ml

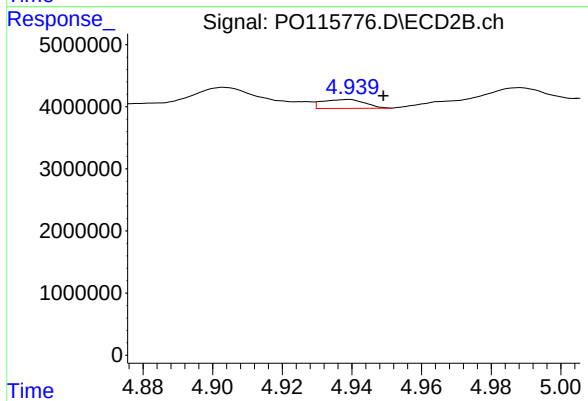

#22 AR-1248-2


R.T.: 4.939 min
Delta R.T.: -0.010 min
Response: 1212907
Conc: 7.96 ng/ml

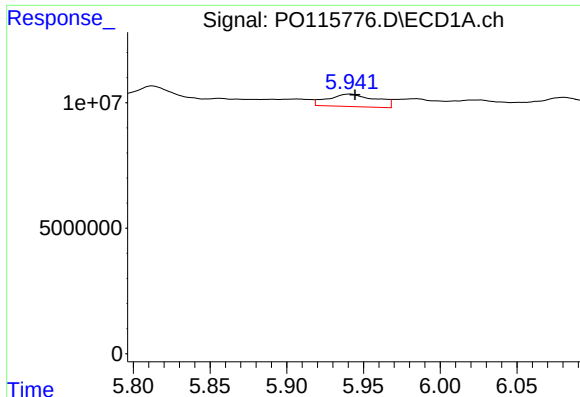

#23 AR-1248-3


R.T.: 5.941 min
Delta R.T.: -0.003 min
Response: 10727048
Conc: 43.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

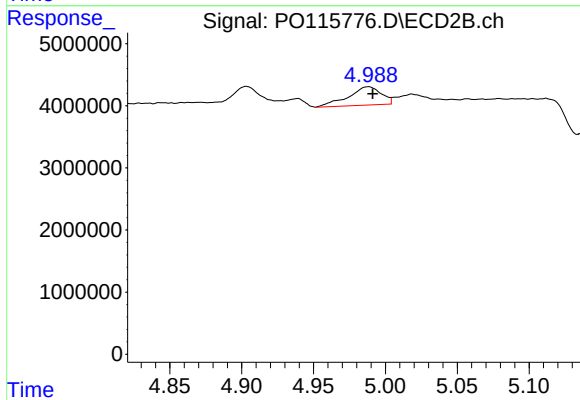


#23 AR-1248-3

R.T.: 4.988 min
Delta R.T.: -0.003 min
Response: 4714987
Conc: 29.37 ng/ml

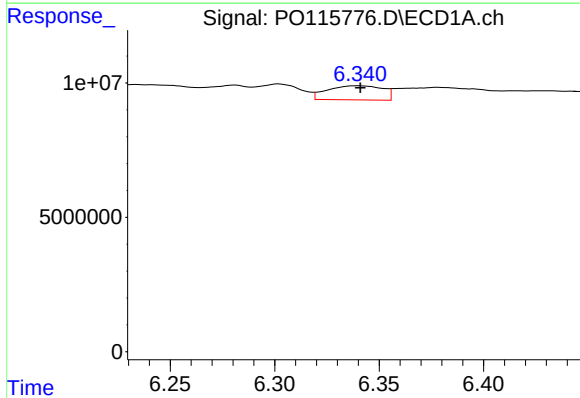


#24 AR-1248-4

R.T.: 6.340 min
Delta R.T.: 0.000 min
Response: 9692340
Conc: 32.87 ng/ml

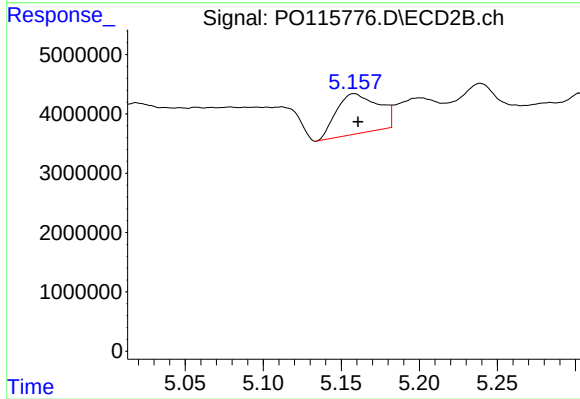

#24 AR-1248-4


R.T.: 5.158 min
Delta R.T.: -0.003 min
Response: 12612335
Conc: 67.39 ng/ml

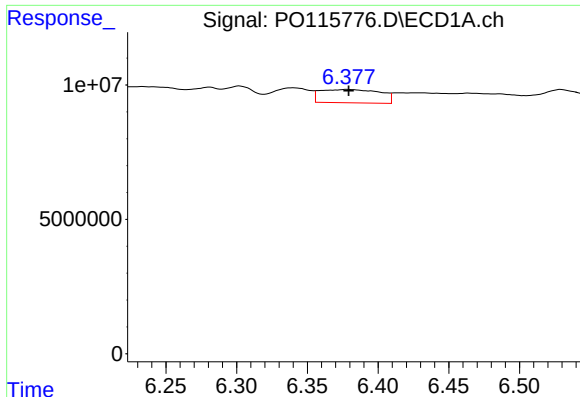

#25 AR-1248-5


R.T.: 6.378 min
Delta R.T.: -0.001 min
Response: 14568563
Conc: 56.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

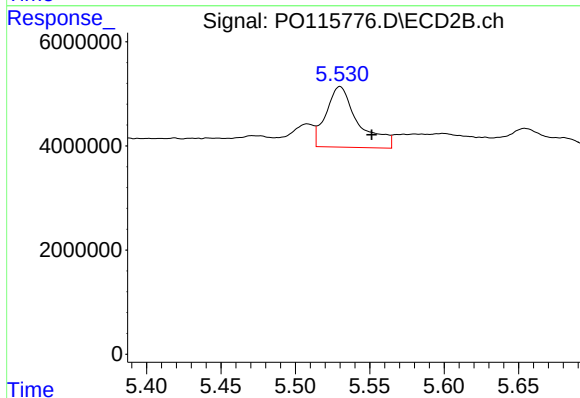


#25 AR-1248-5

R.T.: 5.530 min
Delta R.T.: -0.021 min
Response: 17473120
Conc: 88.27 ng/ml

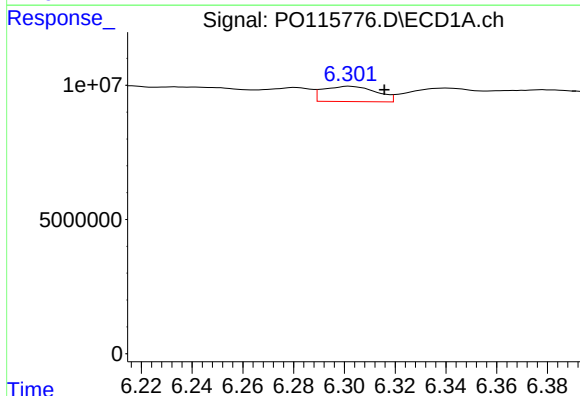


#26 AR-1254-1

R.T.: 6.302 min
Delta R.T.: -0.014 min
Response: 8240427
Conc: 31.85 ng/ml

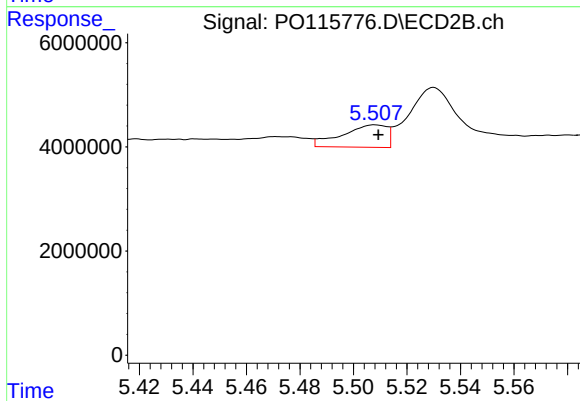

#26 AR-1254-1


R.T.: 5.508 min
Delta R.T.: -0.001 min
Response: 4995570
Conc: 17.09 ng/ml

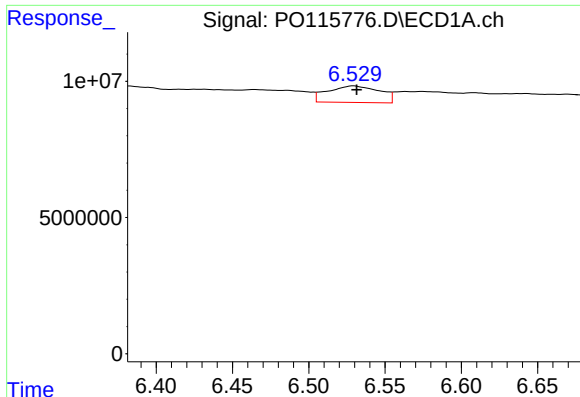

#27 AR-1254-2


R.T.: 6.529 min
Delta R.T.: -0.002 min
Response: 14374378
Conc: 35.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

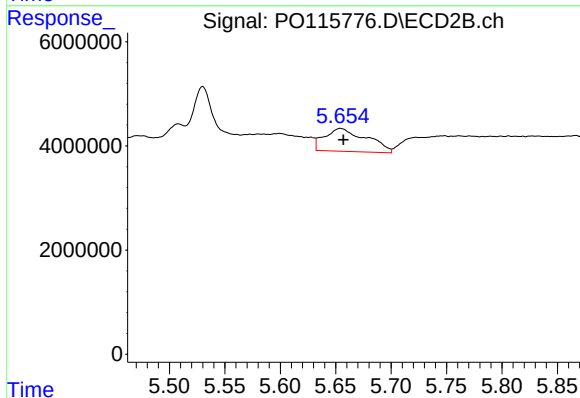


#27 AR-1254-2

R.T.: 5.654 min
Delta R.T.: -0.003 min
Response: 11615488
Conc: 46.13 ng/ml

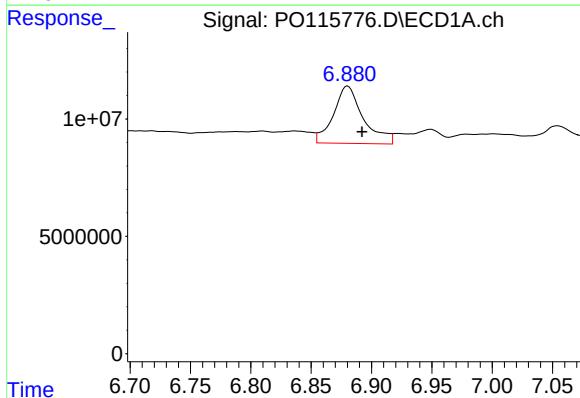


#28 AR-1254-3

R.T.: 6.880 min
Delta R.T.: -0.012 min
Response: 42022079
Conc: 102.35 ng/ml

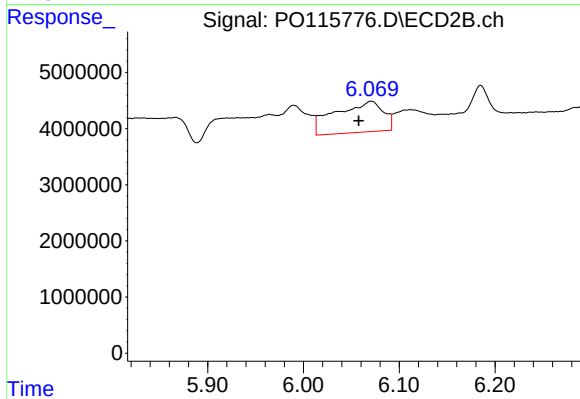

#28 AR-1254-3


R.T.: 6.071 min
Delta R.T.: 0.013 min
Response: 19144178
Conc: 48.64 ng/ml

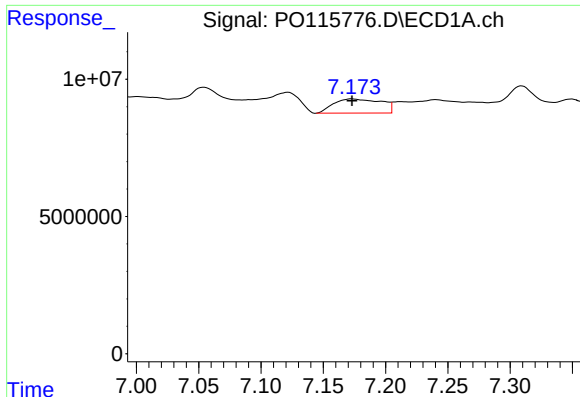

#29 AR-1254-4


R.T.: 7.173 min
Delta R.T.: 0.000 min
Response: 13824579
Conc: 39.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

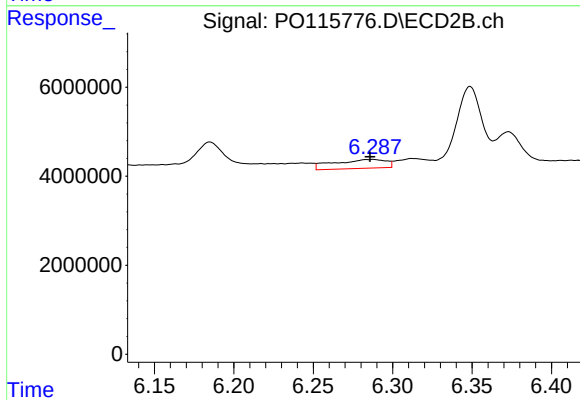


#29 AR-1254-4

R.T.: 6.288 min
Delta R.T.: 0.002 min
Response: 4529644
Conc: 16.93 ng/ml

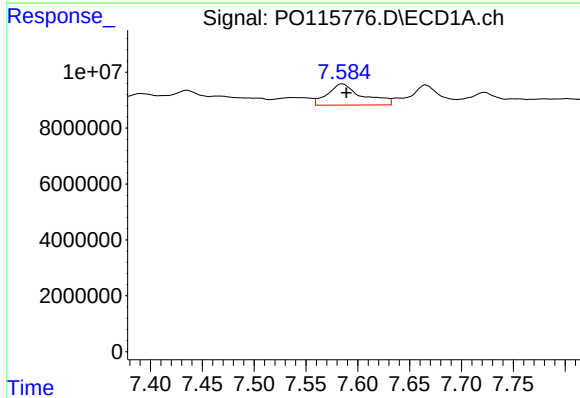


#30 AR-1254-5

R.T.: 7.585 min
Delta R.T.: -0.004 min
Response: 17768812
Conc: 54.83 ng/ml

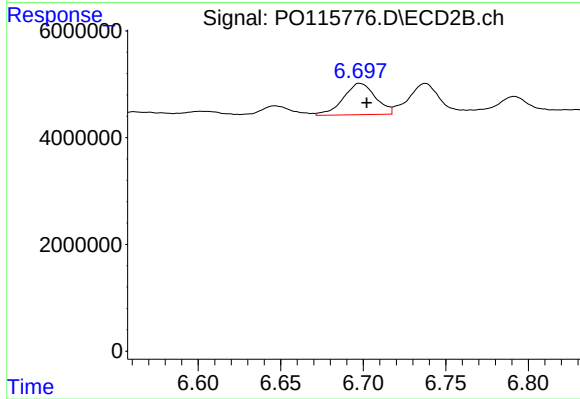

#30 AR-1254-5


R.T.: 6.698 min
Delta R.T.: -0.004 min
Response: 8009810
Conc: 22.40 ng/ml

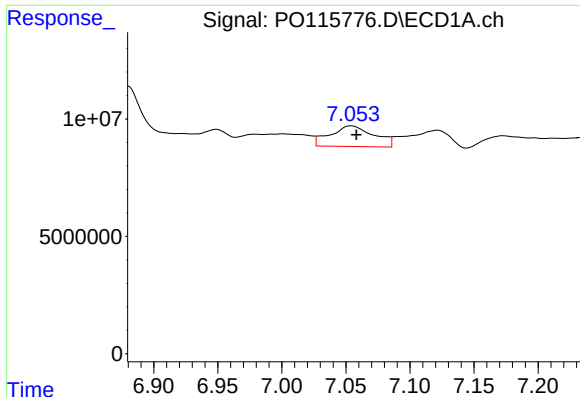

#31 AR-1260-1


R.T.: 7.054 min
Delta R.T.: -0.004 min
Response: 20915011
Conc: 72.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

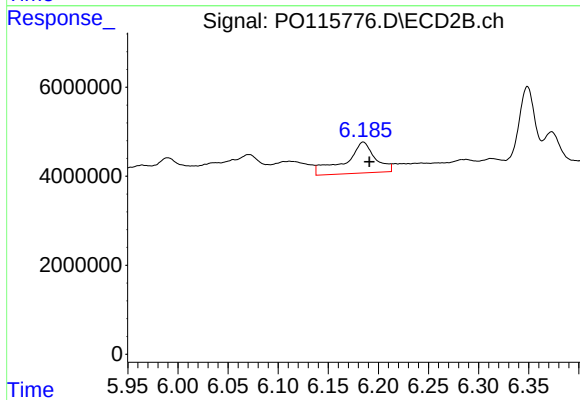


#31 AR-1260-1

R.T.: 6.185 min
Delta R.T.: -0.006 min
Response: 14610333
Conc: 55.73 ng/ml

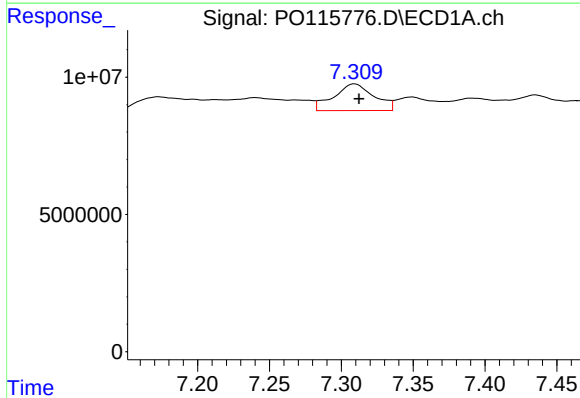


#32 AR-1260-2

R.T.: 7.309 min
Delta R.T.: -0.003 min
Response: 18923397
Conc: 43.23 ng/ml

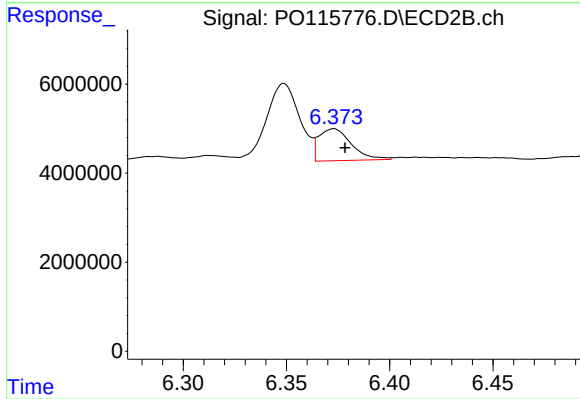

#32 AR-1260-2


R.T.: 6.373 min
Delta R.T.: -0.006 min
Response: 7893750
Conc: 22.52 ng/ml

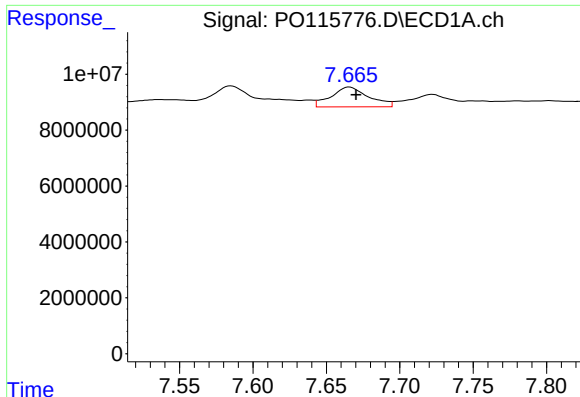

#33 AR-1260-3


R.T.: 7.666 min
Delta R.T.: -0.004 min
Response: 12578541
Conc: 37.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

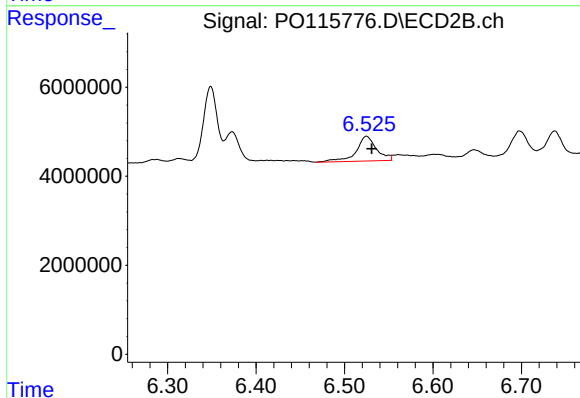


#33 AR-1260-3

R.T.: 6.525 min
Delta R.T.: -0.006 min
Response: 8876697
Conc: 27.63 ng/ml

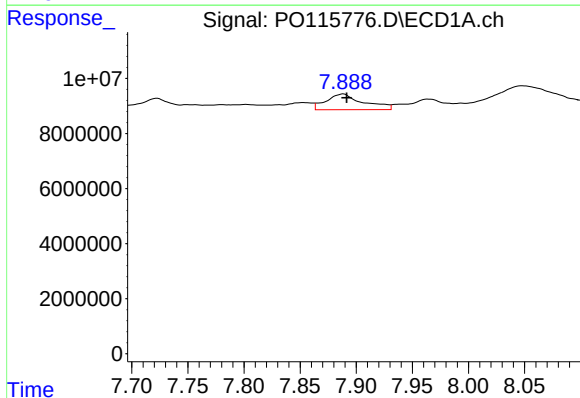


#34 AR-1260-4

R.T.: 7.889 min
Delta R.T.: -0.003 min
Response: 13142885
Conc: 42.75 ng/ml

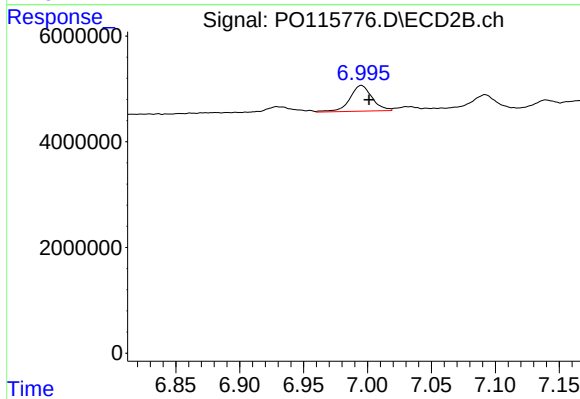

#34 AR-1260-4


R.T.: 6.995 min
Delta R.T.: -0.006 min
Response: 5951430
Conc: 23.17 ng/ml

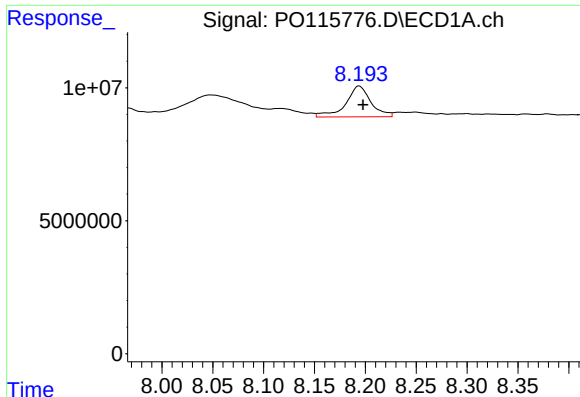

#35 AR-1260-5


R.T.: 8.194 min
Delta R.T.: -0.004 min
Response: 19890128
Conc: 27.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

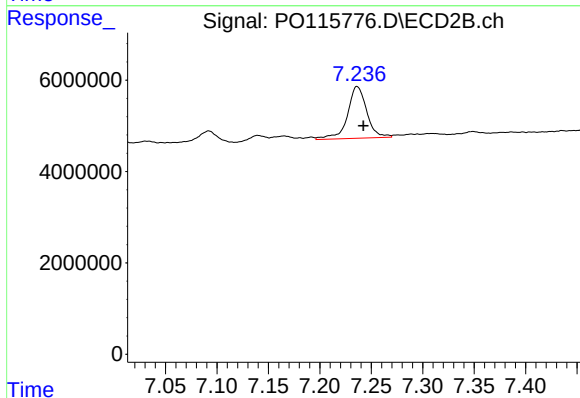


#35 AR-1260-5

R.T.: 7.236 min
Delta R.T.: -0.006 min
Response: 14731912
Conc: 21.01 ng/ml

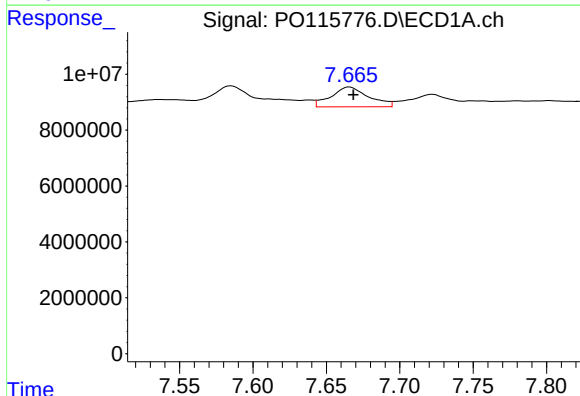


#36 AR-1262-1

R.T.: 7.666 min
Delta R.T.: -0.003 min
Response: 12578541
Conc: 50.95 ng/ml

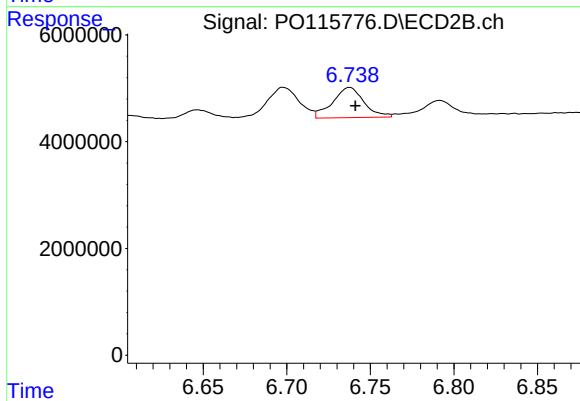

#36 AR-1262-1


R.T.: 6.738 min
Delta R.T.: -0.003 min
Response: 7393481
Conc: 34.70 ng/ml

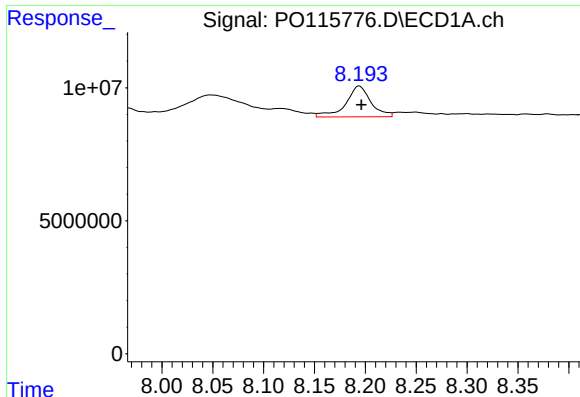

#37 AR-1262-2


R.T.: 8.194 min
Delta R.T.: -0.002 min
Response: 19890128
Conc: 50.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

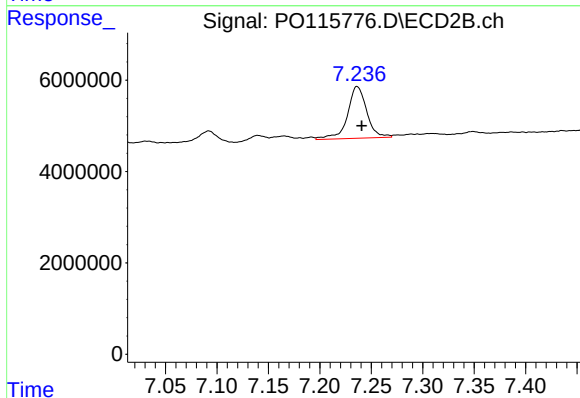


#37 AR-1262-2

R.T.: 7.236 min
Delta R.T.: -0.004 min
Response: 14731912
Conc: 42.29 ng/ml

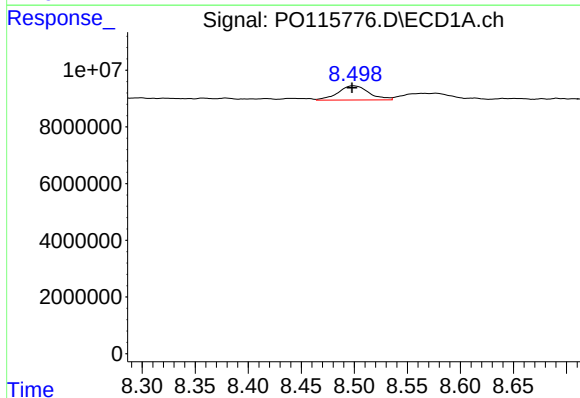


#38 AR-1262-3

R.T.: 8.499 min
Delta R.T.: 0.001 min
Response: 10113064
Conc: 39.69 ng/ml

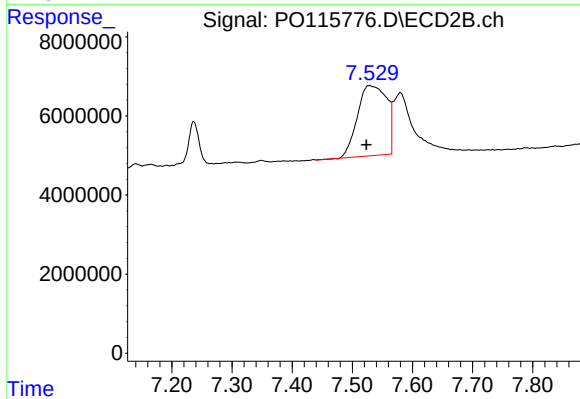

#38 AR-1262-3


R.T.: 7.528 min
Delta R.T.: 0.005 min
Response: 59981842
Conc: 383.54 ng/ml

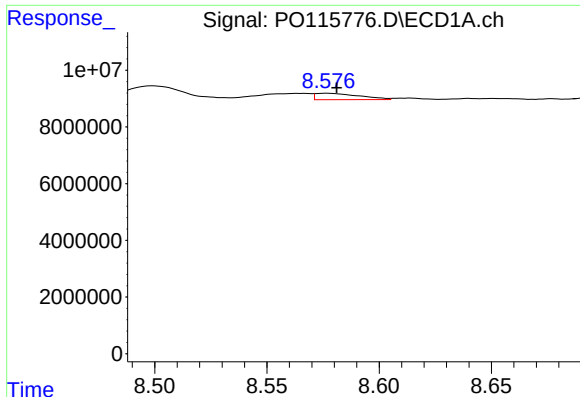

#39 AR-1262-4


R.T.: 8.577 min
Delta R.T.: -0.004 min
Response: 3063425
Conc: 15.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

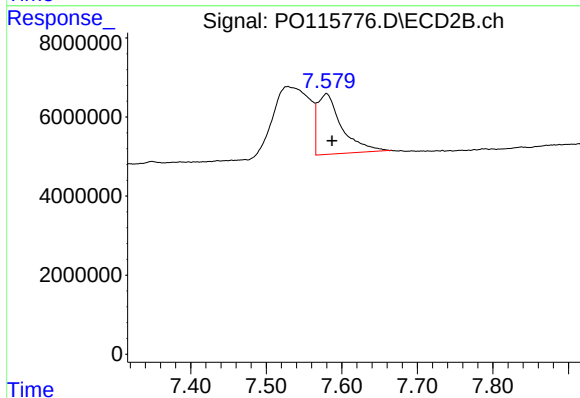


#39 AR-1262-4

R.T.: 7.580 min
Delta R.T.: -0.007 min
Response: 34027714
Conc: 137.56 ng/ml

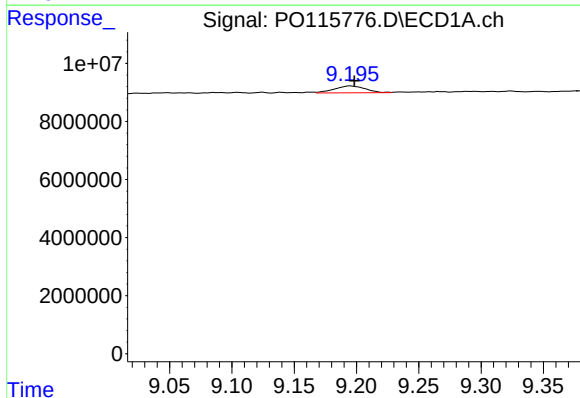


#40 AR-1262-5

R.T.: 9.195 min
Delta R.T.: -0.003 min
Response: 4136088
Conc: 30.71 ng/ml

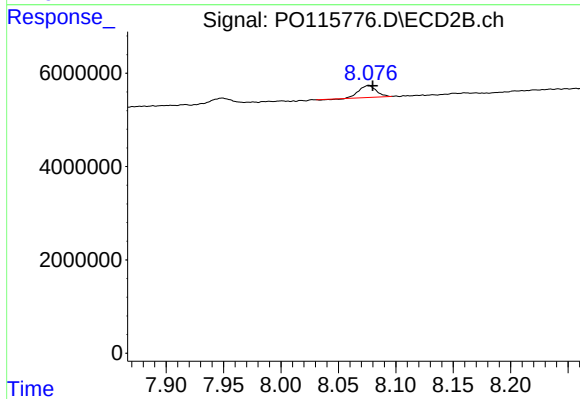

#40 AR-1262-5


R.T.: 8.076 min
Delta R.T.: -0.003 min
Response: 2632193
Conc: 23.61 ng/ml

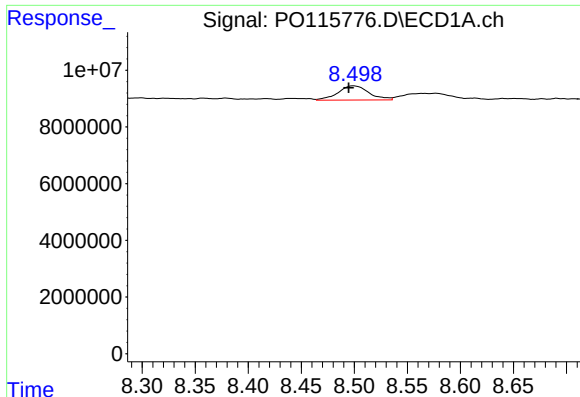

#41 AR-1268-1


R.T.: 8.499 min
Delta R.T.: 0.004 min
Response: 10113064
Conc: 10.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

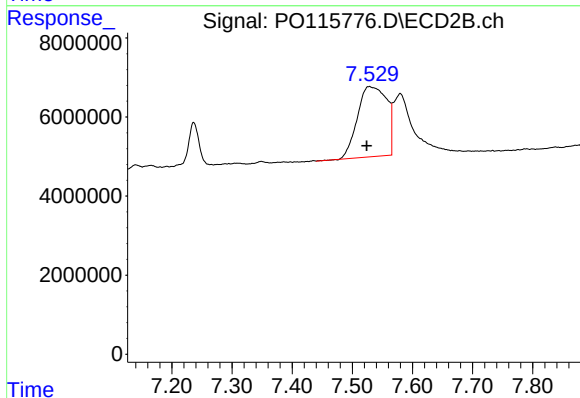


#41 AR-1268-1

R.T.: 7.528 min
Delta R.T.: 0.004 min
Response: 59981842
Conc: 67.70 ng/ml

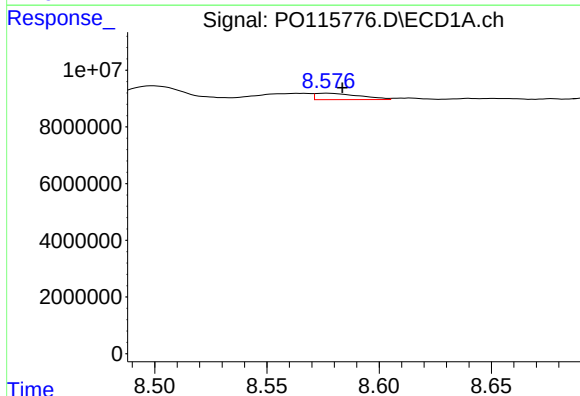


#42 AR-1268-2

R.T.: 8.577 min
Delta R.T.: -0.007 min
Response: 3063425
Conc: 3.58 ng/ml

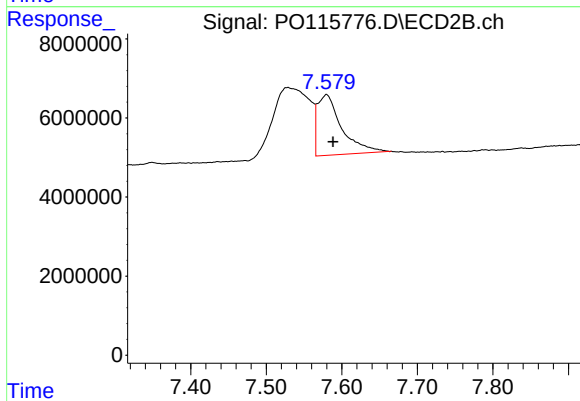

#42 AR-1268-2


R.T.: 7.580 min
Delta R.T.: -0.009 min
Response: 34027714
Conc: 45.43 ng/ml

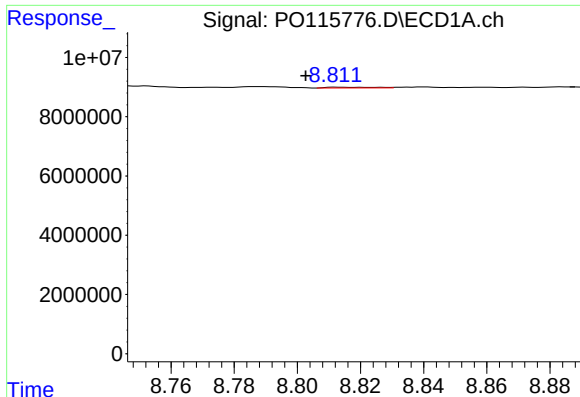

#43 AR-1268-3


R.T.: 8.812 min
Delta R.T.: 0.010 min
Response: 263278
Conc: 0.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

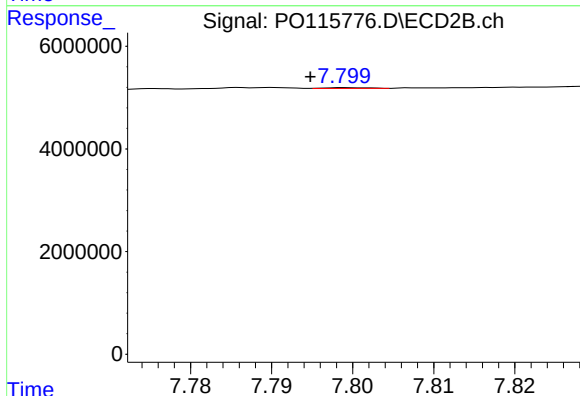


#43 AR-1268-3

R.T.: 7.800 min
Delta R.T.: 0.005 min
Response: 58884
Conc: 0.09 ng/ml

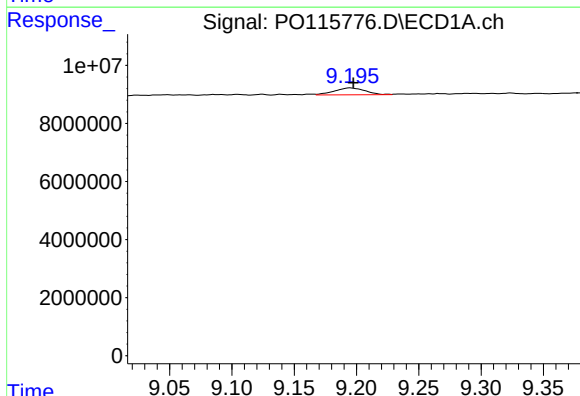


#44 AR-1268-4

R.T.: 9.195 min
Delta R.T.: -0.002 min
Response: 4136088
Conc: 13.25 ng/ml

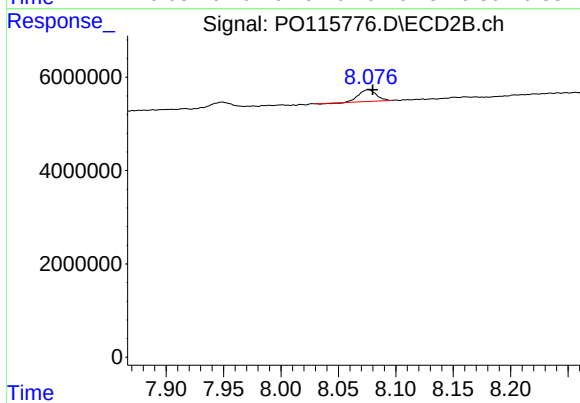

#44 AR-1268-4


R.T.: 8.076 min
Delta R.T.: -0.004 min
Response: 2632193
Conc: 10.22 ng/ml

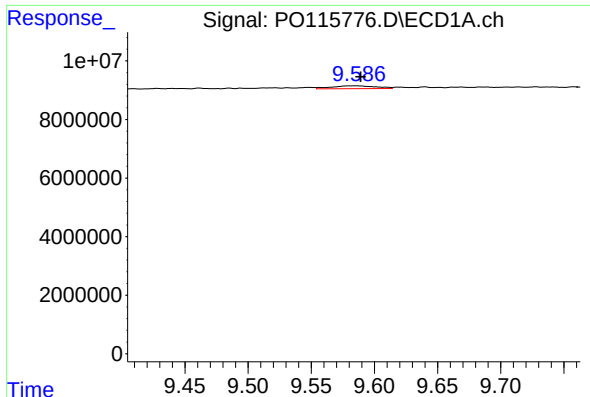

#45 AR-1268-5

R.T.: 9.586 min
Delta R.T.: -0.003 min
Response: 2380785
Conc: 1.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

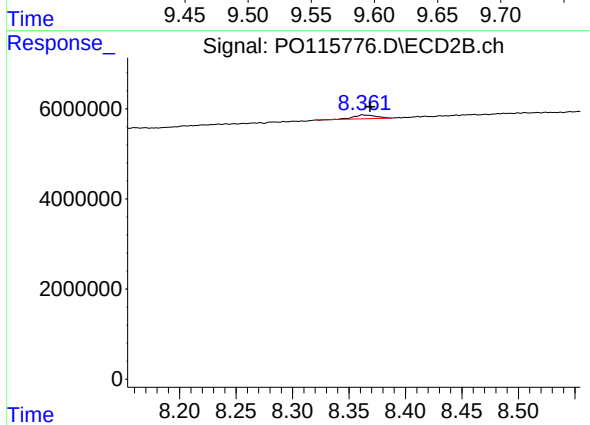

#45 AR-1268-5

R.T.: 8.362 min
Delta R.T.: -0.006 min
Response: 1161347
Conc: 0.69 ng/ml