

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO121225\
 Data File : PO115777.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Dec 2025 01:57
 Operator : YP/AJ
 Sample : Q3530-07
 Misc : AR1221 25PPB WATER LOD
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 13 03:49:23 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO120425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 05 02:11:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.334	3.637	153.8E6	94583254	19.804	19.408
2)	SA Decachlor...	9.908	8.616	108.6E6	81522027	20.647	18.958
Target Compounds							
3)	L1 AR-1016-1	5.468	4.716	755259	210371	3.037	1.139 #
4)	L1 AR-1016-2	5.497	4.733	846211	506841	2.222	1.918
5)	L1 AR-1016-3	5.551	4.903	705288	1321401	3.299	8.731 #
6)	L1 AR-1016-4	5.648	4.965	929524	267399	5.205	2.373 #
7)	L1 AR-1016-5	5.947	5.163	2870294	1951752	16.362	13.337
8)	L2 AR-1221-1	4.532	3.847	3395952	1324556	41.824	23.483 #
9)	L2 AR-1221-2	4.628	3.932	5150446	2543746	81.729	59.932 #
10)	L2 AR-1221-3	4.692	4.007	6085648	3205351	32.593	24.927
11)	L3 AR-1232-1	4.692	4.007	6085648	3205351	40.662	30.002 #
12)	L3 AR-1232-2	5.211	4.733	599251	506841	7.412	4.567 #
13)	L3 AR-1232-3	5.497	4.903	846211	1321401	5.498	20.215 #
14)	L3 AR-1232-4	5.648	4.992	929524	540273	13.273	10.525
15)	L3 AR-1232-5	5.752	5.163	175393	1951752	3.377	35.650 #
16)	L4 AR-1242-1	5.468	4.716	755259	210371	3.802	1.477 #
17)	L4 AR-1242-2	5.497	4.733	846211	506841	2.889	2.421
18)	L4 AR-1242-3	5.551	4.903	705288	1321401	4.178	11.063 #
19)	L4 AR-1242-4	5.648	4.992	929524	540273	6.801	4.952 #
20)	L4 AR-1242-5	6.375	5.503	1526780	450850	10.081	3.264 #
21)	L5 AR-1248-1	5.468	4.712	755259	611563	4.976	5.469
22)	L5 AR-1248-2	5.752	4.965	175393	267399	0.873	1.756 #
23)	L5 AR-1248-3	5.947	4.992	2870294	540273	11.640	3.366 #
24)	L5 AR-1248-4	6.337	5.163	1426957	1951752	4.840	10.429 #
25)	L5 AR-1248-5	6.375	5.551	1526780	478060	5.897	2.415 #
26)	L6 AR-1254-1	6.337	5.503	1426957	450850	5.516	1.543 #
27)	L6 AR-1254-2	6.527	5.657	2128538	1261158	5.290	5.008
28)	L6 AR-1254-3	6.881	6.055	12873243	977979	31.355	2.485 #
29)	L6 AR-1254-4	7.166	6.288	3075837	1078185	8.862	4.029 #
30)	L6 AR-1254-5	7.582	6.697	381137	126852	1.176	0.355 #
31)	L7 AR-1260-1	7.065	6.187	2719632	261936	9.388	0.999 #
32)	L7 AR-1260-2	7.333	6.378	3178970	280333	7.262	0.800 #
33)	L7 AR-1260-3	7.669	6.537	795923	310885	2.365	0.968 #
34)	L7 AR-1260-4	7.884	6.994	959889	113844	3.122	0.443 #
35)	L7 AR-1260-5	8.201	7.244	1298610	134521	1.783	0.192 #
36)	L8 AR-1262-1	7.669	6.739	795923	193633	3.224	0.909 #
37)	L8 AR-1262-2	8.201	7.244	1298610	134521	3.280	0.386 #
38)	L8 AR-1262-3	8.496	7.538	623144	21853095	2.445	139.734 #
39)	L8 AR-1262-4	8.581	7.624f	303409	181643	1.566	0.734 #
40)	L8 AR-1262-5	9.195	8.081	1135037	77493	8.427	0.695 #
41)	L9 AR-1268-1	8.496	7.538	623144	21853095	0.626	24.666 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121225\
Data File : PO115777.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Dec 2025 01:57
Operator : YP/AJ
Sample : Q3530-07
Misc : AR1221 25PPB WATER LOD
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 13 03:49:23 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120425.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 05 02:11:05 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.581	7.624	303409	181643	0.355	0.242 #
43)	L9 AR-1268-3	8.800	7.794	194382	261822	0.262	0.411 #
44)	L9 AR-1268-4	9.195	8.081	1135037	77493	3.635	0.301 #
45)	L9 AR-1268-5	9.589	8.368	1732212	572209	0.796	0.339 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121225\
Data File : PO115777.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Dec 2025 01:57
Operator : YP/AJ
Sample : Q3530-07
Misc : AR1221 25PPB WATER LOD
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 13 03:49:23 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120425.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 05 02:11:05 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

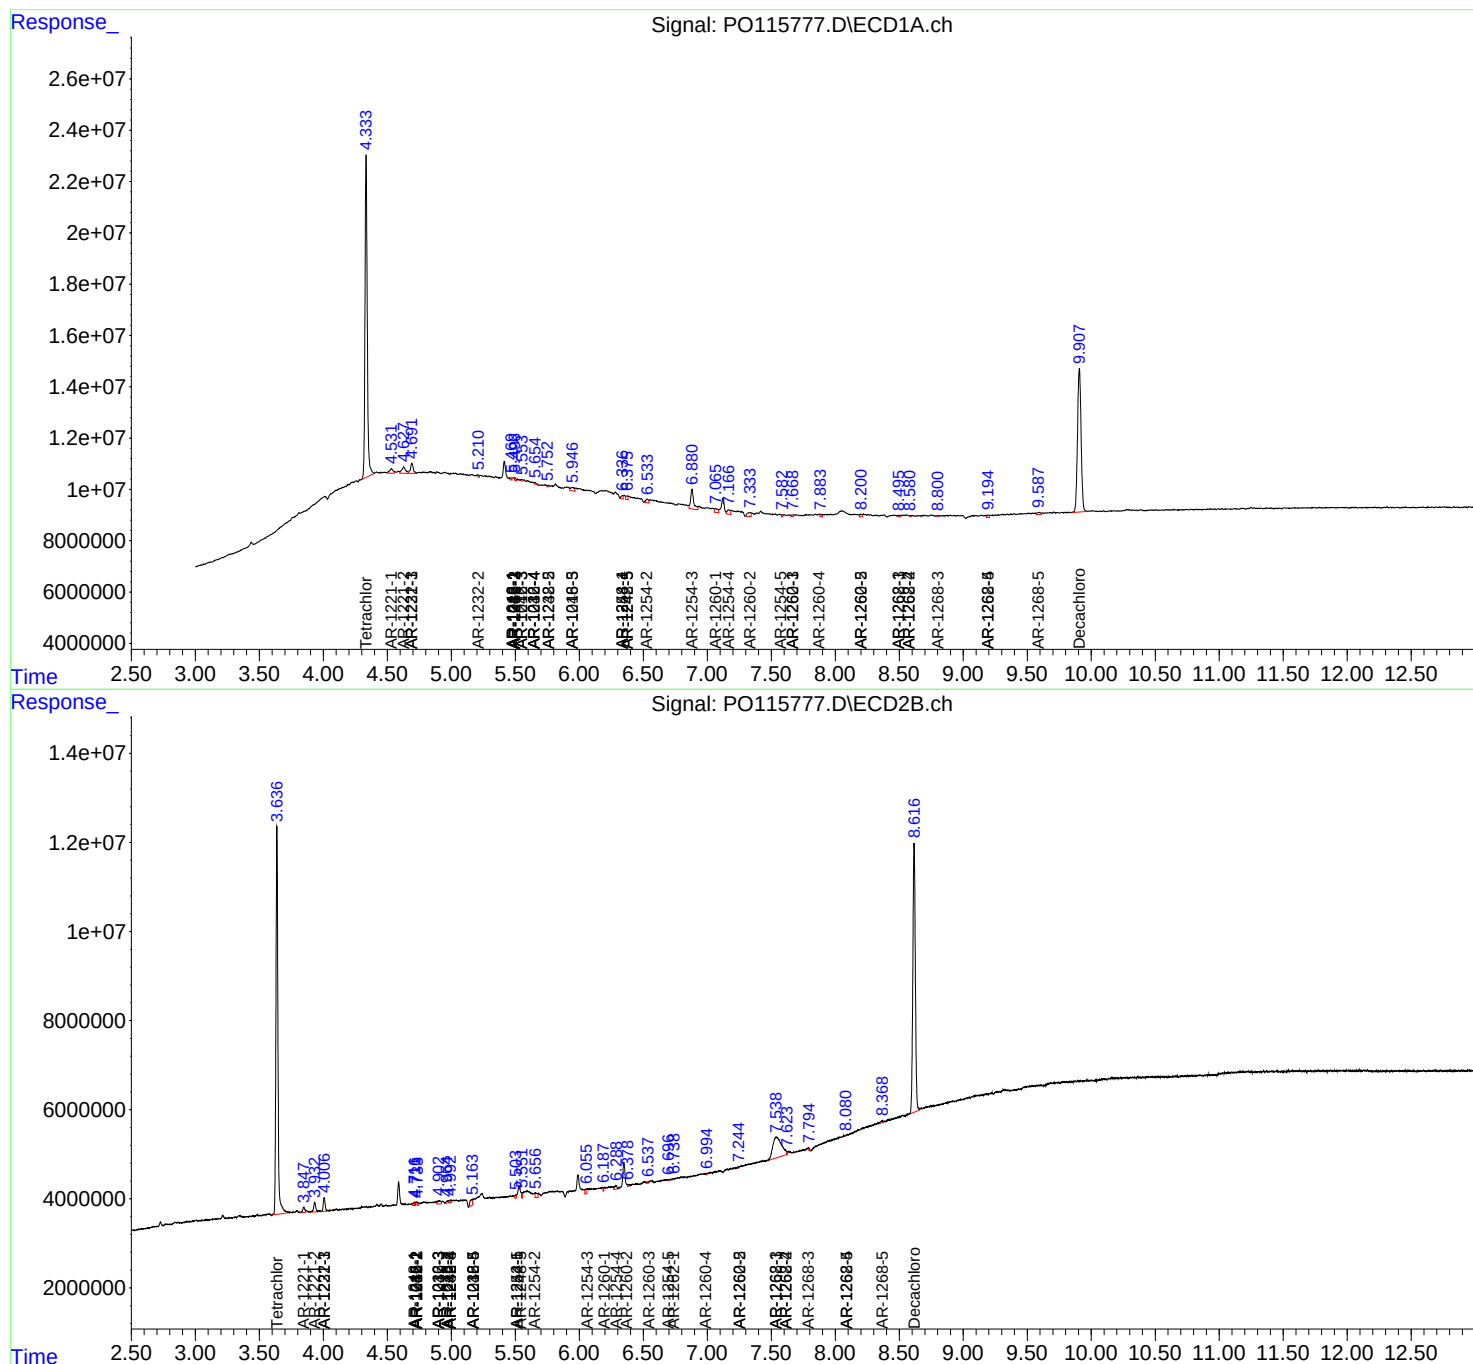


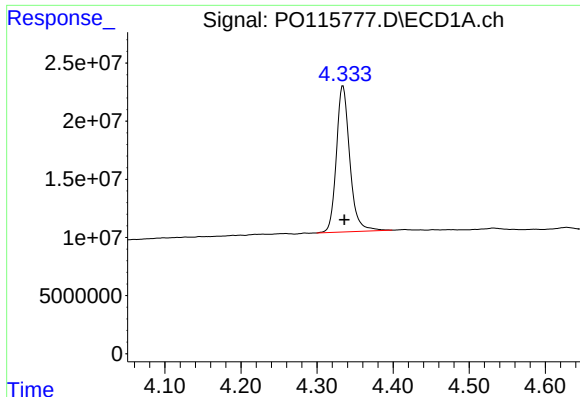

#1 Tetrachloro-m-xylene


R.T.: 4.334 min
Delta R.T.: -0.002 min
Response: 153822825
Conc: 19.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

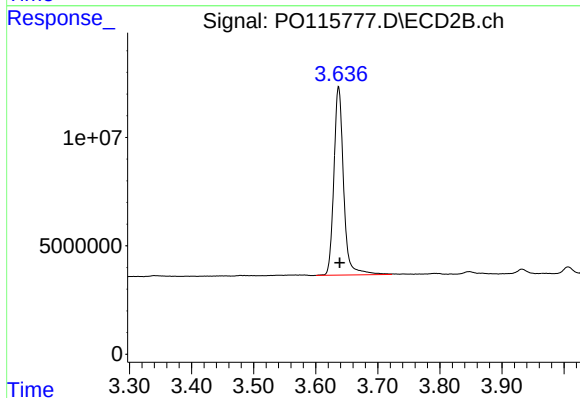


#1 Tetrachloro-m-xylene

R.T.: 3.637 min
Delta R.T.: -0.002 min
Response: 94583254
Conc: 19.41 ng/ml

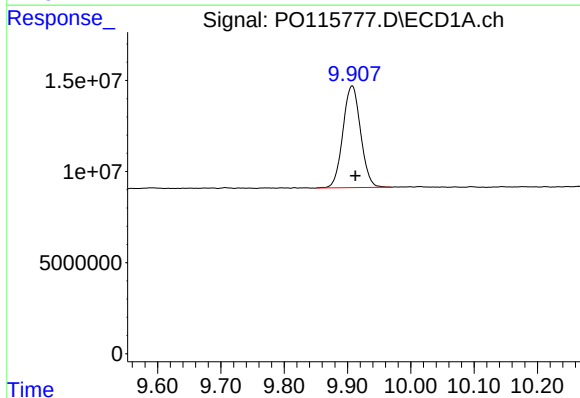


#2 Decachlorobiphenyl

R.T.: 9.908 min
Delta R.T.: -0.005 min
Response: 108623125
Conc: 20.65 ng/ml

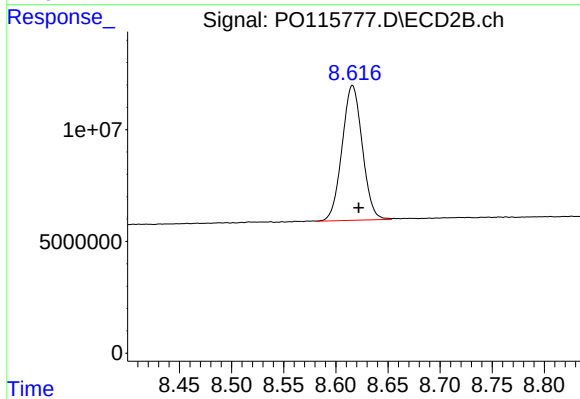

#2 Decachlorobiphenyl


R.T.: 8.616 min
Delta R.T.: -0.006 min
Response: 81522027
Conc: 18.96 ng/ml

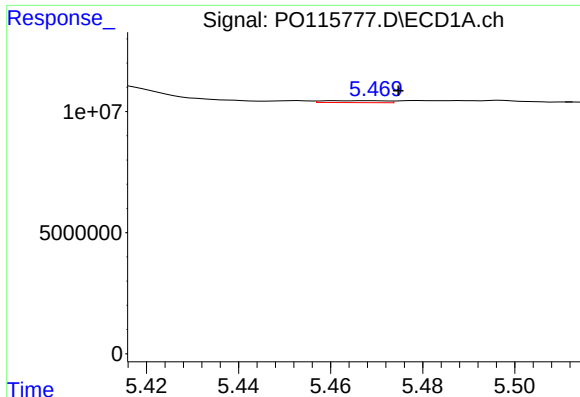

#3 AR-1016-1


R.T.: 5.468 min
Delta R.T.: -0.007 min
Response: 755259
Conc: 3.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

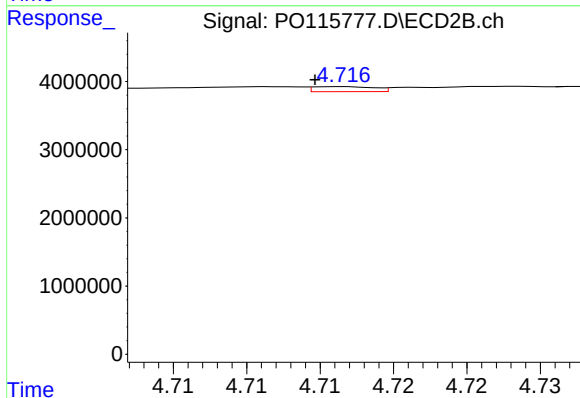


#3 AR-1016-1

R.T.: 4.716 min
Delta R.T.: 0.002 min
Response: 210371
Conc: 1.14 ng/ml

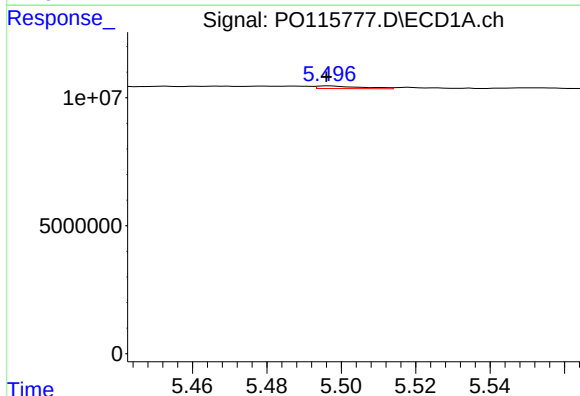


#4 AR-1016-2

R.T.: 5.497 min
Delta R.T.: 0.000 min
Response: 846211
Conc: 2.22 ng/ml

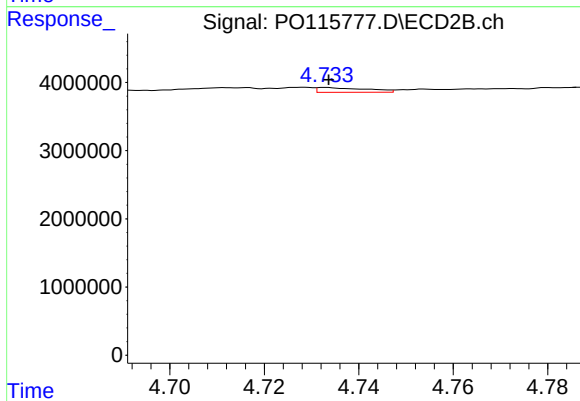

#4 AR-1016-2


R.T.: 4.733 min
Delta R.T.: 0.000 min
Response: 506841
Conc: 1.92 ng/ml

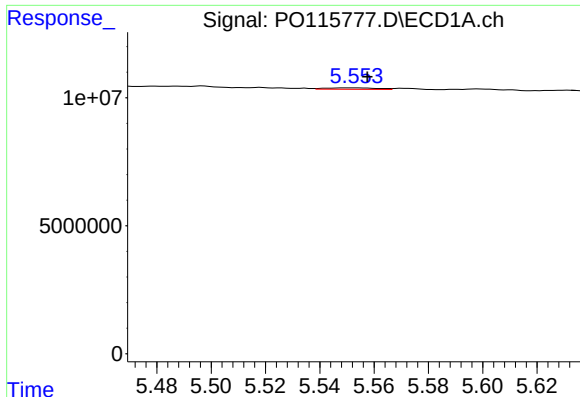

#5 AR-1016-3


R.T.: 5.551 min
Delta R.T.: -0.007 min
Response: 705288
Conc: 3.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

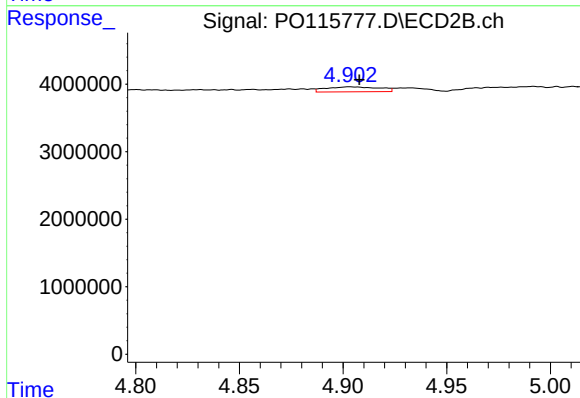


#5 AR-1016-3

R.T.: 4.903 min
Delta R.T.: -0.005 min
Response: 1321401
Conc: 8.73 ng/ml

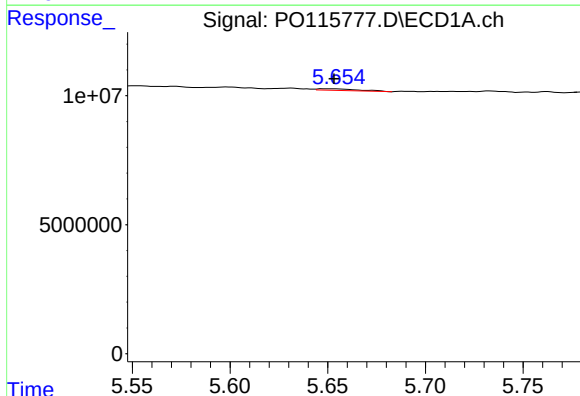


#6 AR-1016-4

R.T.: 5.648 min
Delta R.T.: -0.005 min
Response: 929524
Conc: 5.21 ng/ml

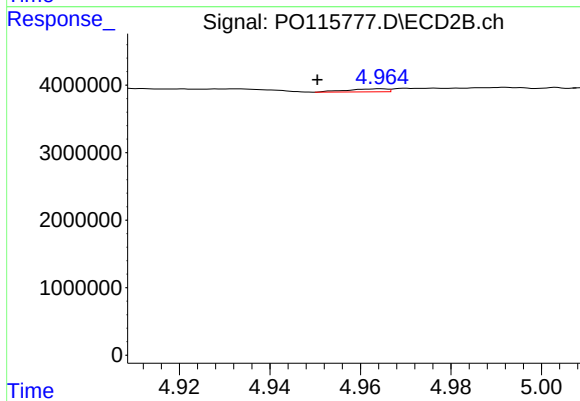

#6 AR-1016-4


R.T.: 4.965 min
Delta R.T.: 0.014 min
Response: 267399
Conc: 2.37 ng/ml

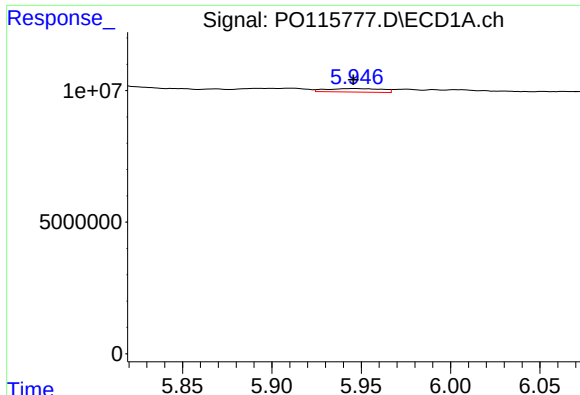

#7 AR-1016-5


R.T.: 5.947 min
Delta R.T.: 0.001 min
Response: 2870294
Conc: 16.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

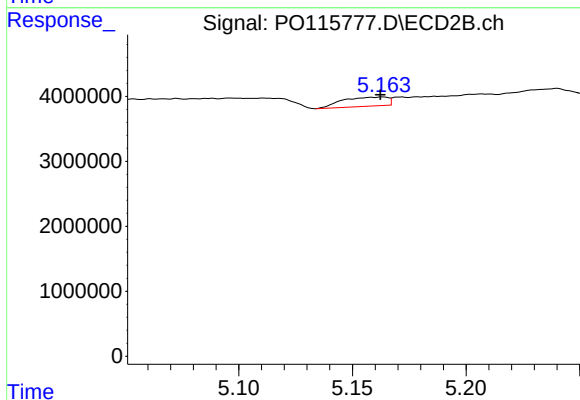


#7 AR-1016-5

R.T.: 5.163 min
Delta R.T.: 0.001 min
Response: 1951752
Conc: 13.34 ng/ml

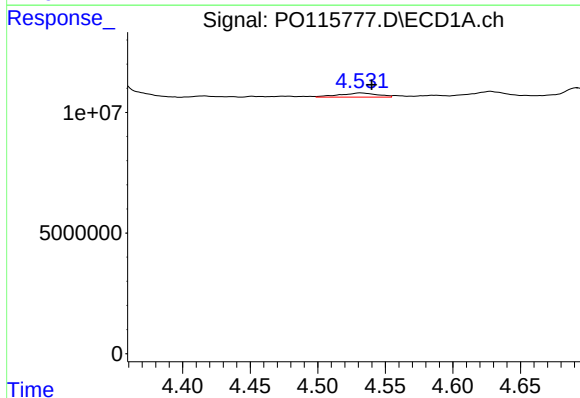


#8 AR-1221-1

R.T.: 4.532 min
Delta R.T.: -0.008 min
Response: 3395952
Conc: 41.82 ng/ml

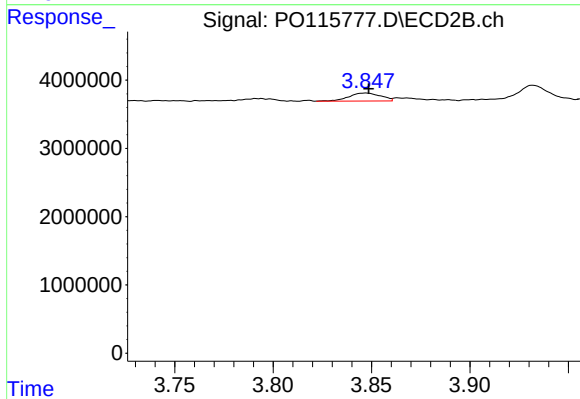

#8 AR-1221-1


R.T.: 3.847 min
Delta R.T.: -0.001 min
Response: 1324556
Conc: 23.48 ng/ml

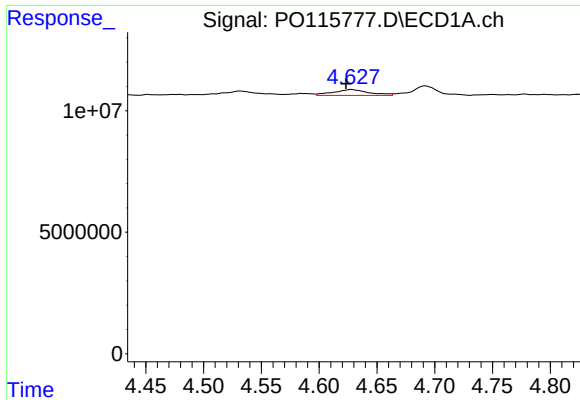

#9 AR-1221-2


R.T.: 4.628 min
Delta R.T.: 0.005 min
Response: 5150446
Conc: 81.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

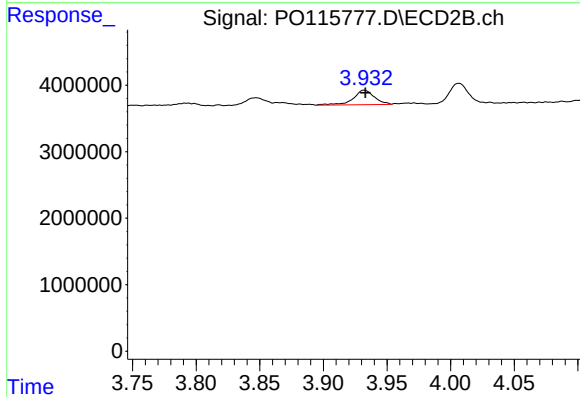


#9 AR-1221-2

R.T.: 3.932 min
Delta R.T.: -0.001 min
Response: 2543746
Conc: 59.93 ng/ml

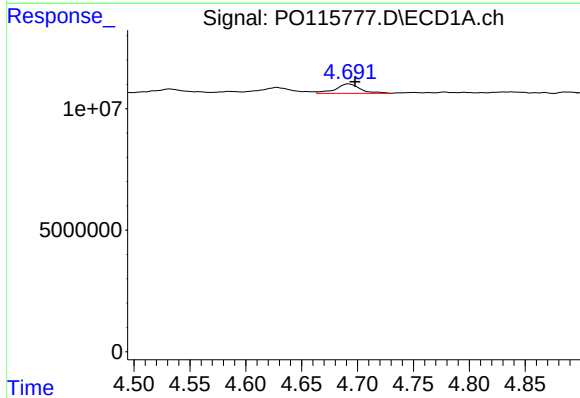


#10 AR-1221-3

R.T.: 4.692 min
Delta R.T.: -0.006 min
Response: 6085648
Conc: 32.59 ng/ml

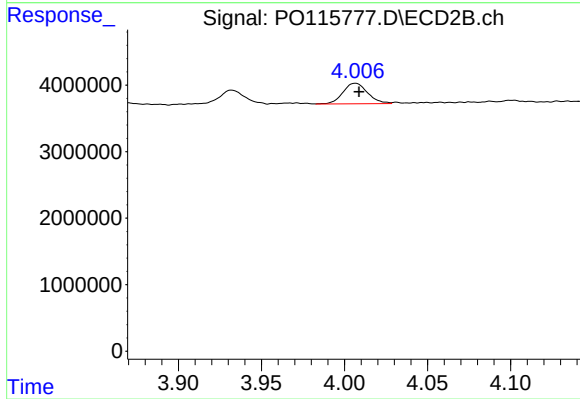

#10 AR-1221-3


R.T.: 4.007 min
Delta R.T.: -0.002 min
Response: 3205351
Conc: 24.93 ng/ml

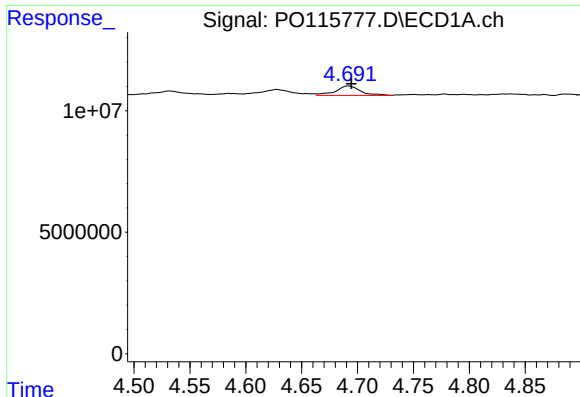

#11 AR-1232-1


R.T.: 4.692 min
Delta R.T.: -0.003 min
Response: 6085648
Conc: 40.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

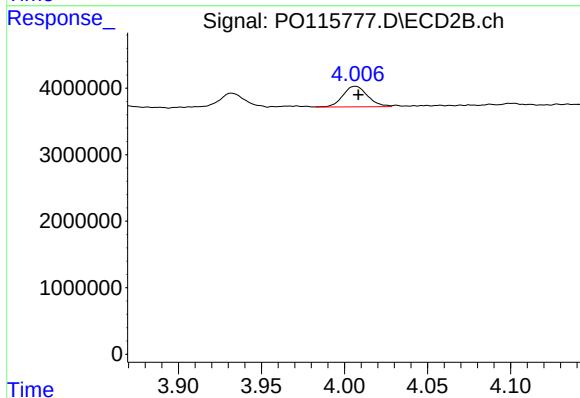


#11 AR-1232-1

R.T.: 4.007 min
Delta R.T.: -0.002 min
Response: 3205351
Conc: 30.00 ng/ml

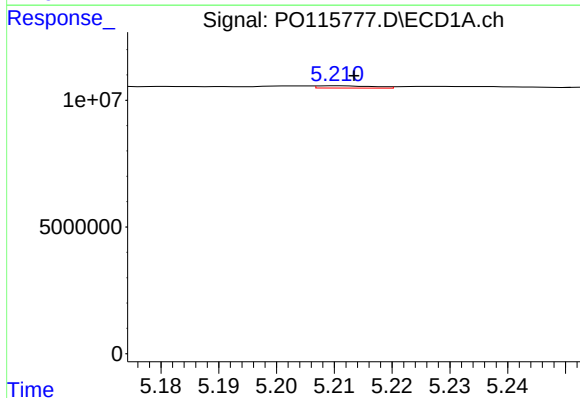


#12 AR-1232-2

R.T.: 5.211 min
Delta R.T.: -0.003 min
Response: 599251
Conc: 7.41 ng/ml

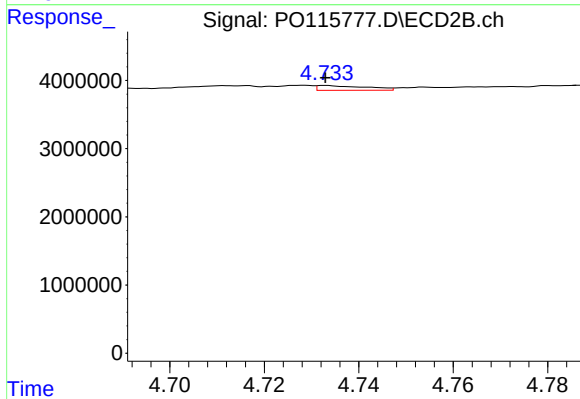

#12 AR-1232-2


R.T.: 4.733 min
Delta R.T.: 0.000 min
Response: 506841
Conc: 4.57 ng/ml

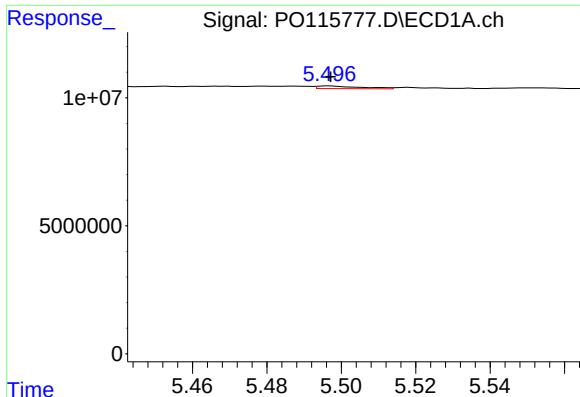

#13 AR-1232-3


R.T.: 5.497 min
Delta R.T.: 0.000 min
Response: 846211
Conc: 5.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

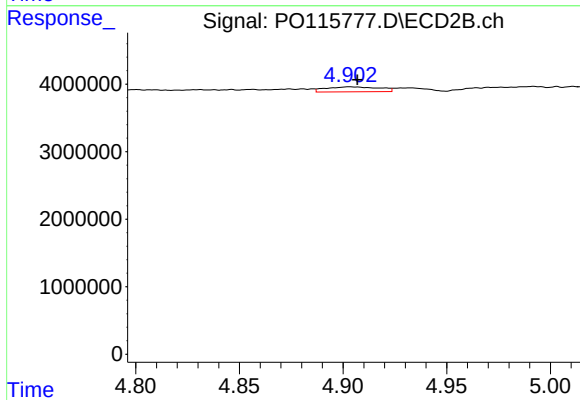


#13 AR-1232-3

R.T.: 4.903 min
Delta R.T.: -0.004 min
Response: 1321401
Conc: 20.22 ng/ml

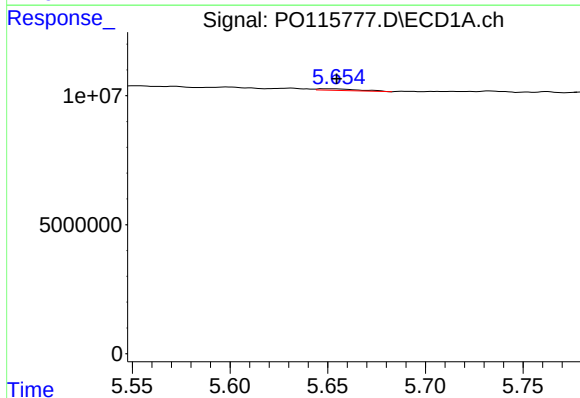


#14 AR-1232-4

R.T.: 5.648 min
Delta R.T.: -0.006 min
Response: 929524
Conc: 13.27 ng/ml

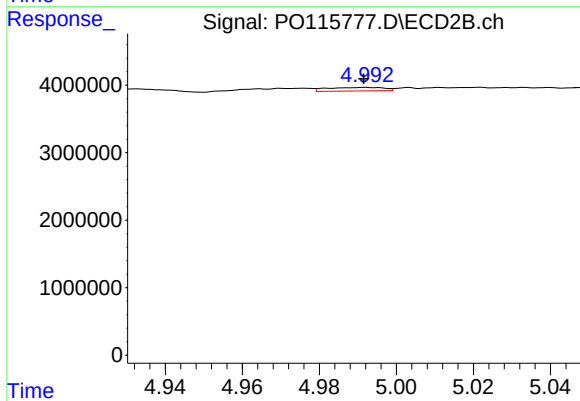

#14 AR-1232-4


R.T.: 4.992 min
Delta R.T.: 0.000 min
Response: 540273
Conc: 10.53 ng/ml

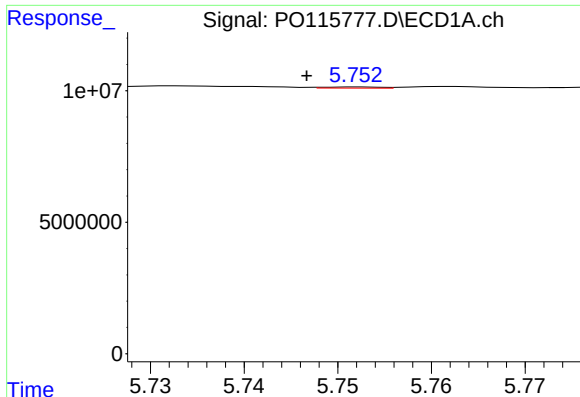

#15 AR-1232-5


R.T.: 5.752 min
Delta R.T.: 0.005 min
Response: 175393
Conc: 3.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

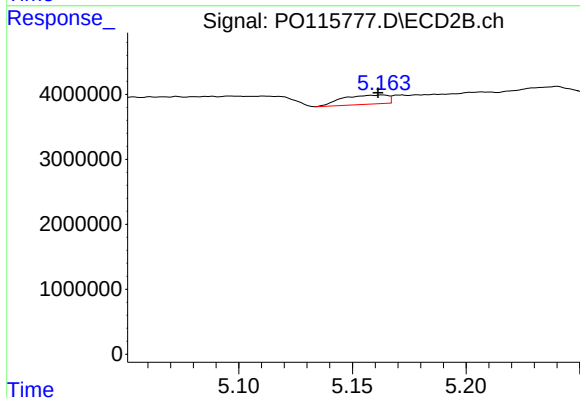


#15 AR-1232-5

R.T.: 5.163 min
Delta R.T.: 0.002 min
Response: 1951752
Conc: 35.65 ng/ml

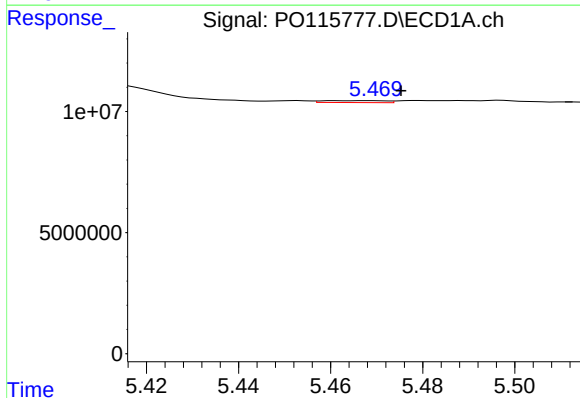


#16 AR-1242-1

R.T.: 5.468 min
Delta R.T.: -0.007 min
Response: 755259
Conc: 3.80 ng/ml

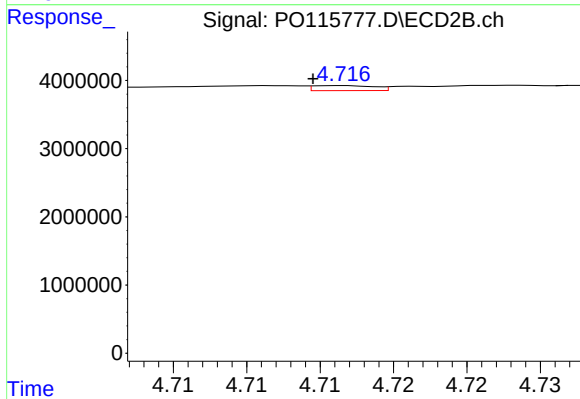

#16 AR-1242-1


R.T.: 4.716 min
Delta R.T.: 0.002 min
Response: 210371
Conc: 1.48 ng/ml

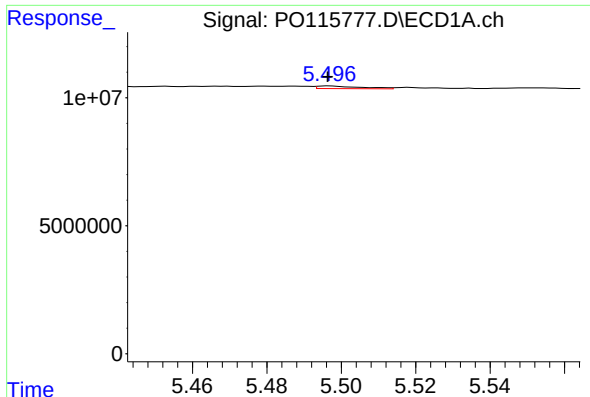

#17 AR-1242-2


R.T.: 5.497 min
Delta R.T.: 0.000 min
Response: 846211
Conc: 2.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

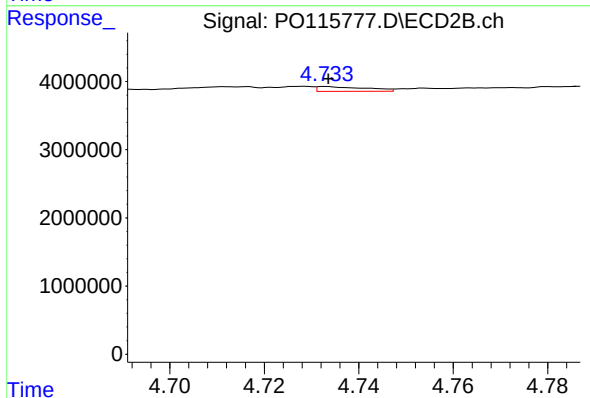


#17 AR-1242-2

R.T.: 4.733 min
Delta R.T.: 0.000 min
Response: 506841
Conc: 2.42 ng/ml

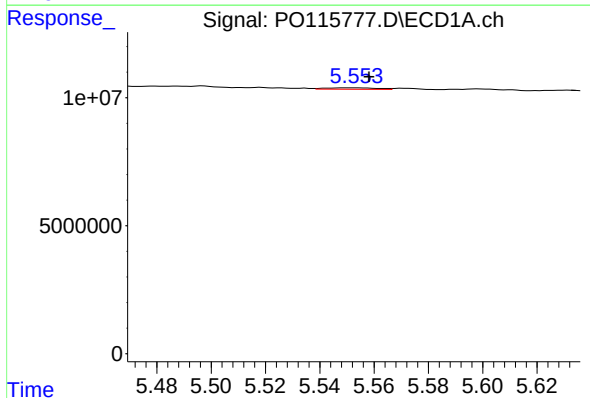


#18 AR-1242-3

R.T.: 5.551 min
Delta R.T.: -0.007 min
Response: 705288
Conc: 4.18 ng/ml

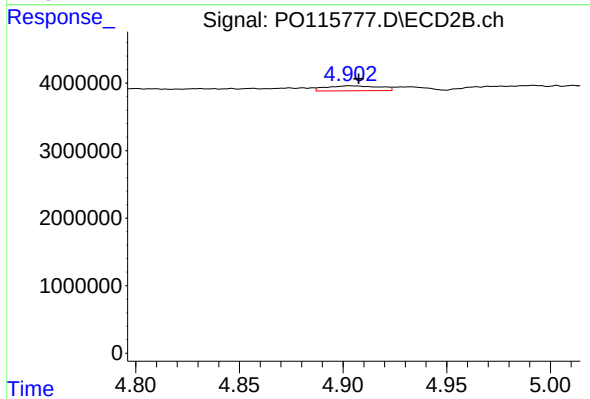

#18 AR-1242-3


R.T.: 4.903 min
Delta R.T.: -0.004 min
Response: 1321401
Conc: 11.06 ng/ml

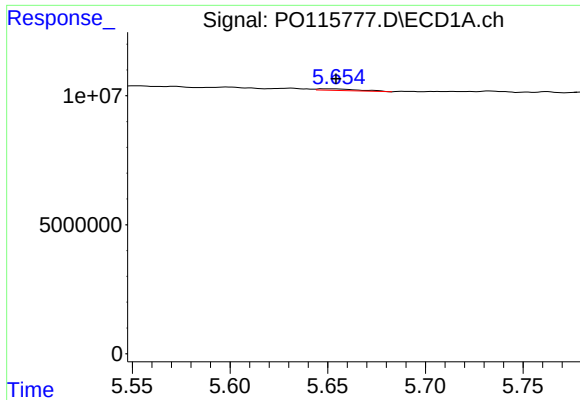

#19 AR-1242-4


R.T.: 5.648 min
Delta R.T.: -0.006 min
Response: 929524
Conc: 6.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

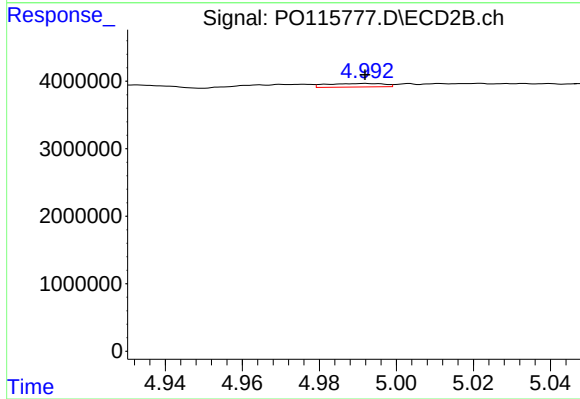


#19 AR-1242-4

R.T.: 4.992 min
Delta R.T.: 0.000 min
Response: 540273
Conc: 4.95 ng/ml

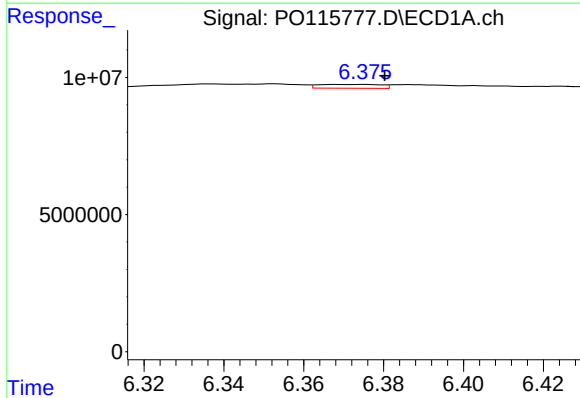


#20 AR-1242-5

R.T.: 6.375 min
Delta R.T.: -0.005 min
Response: 1526780
Conc: 10.08 ng/ml

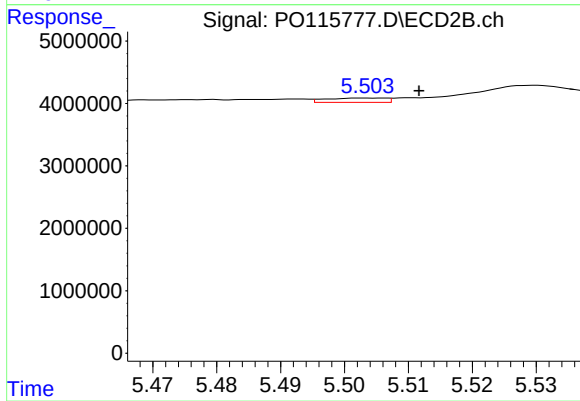

#20 AR-1242-5


R.T.: 5.503 min
Delta R.T.: -0.009 min
Response: 450850
Conc: 3.26 ng/ml

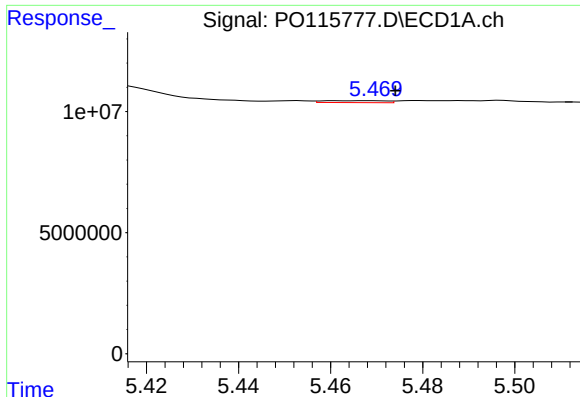

#21 AR-1248-1


R.T.: 5.468 min
Delta R.T.: -0.006 min
Response: 755259
Conc: 4.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

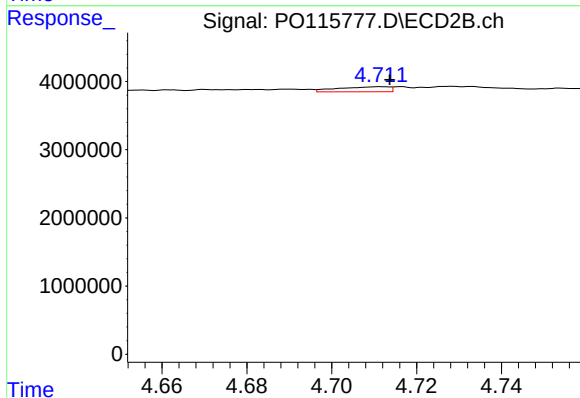


#21 AR-1248-1

R.T.: 4.712 min
Delta R.T.: -0.002 min
Response: 611563
Conc: 5.47 ng/ml

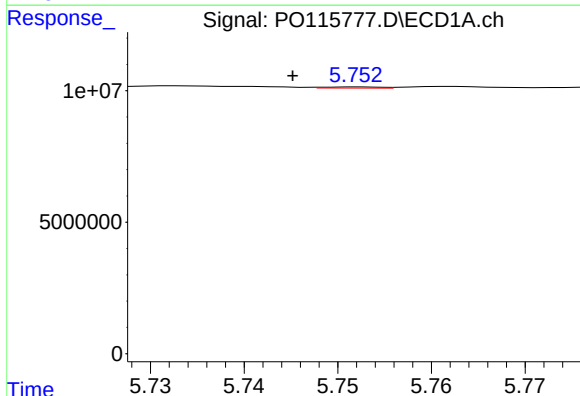


#22 AR-1248-2

R.T.: 5.752 min
Delta R.T.: 0.007 min
Response: 175393
Conc: 0.87 ng/ml

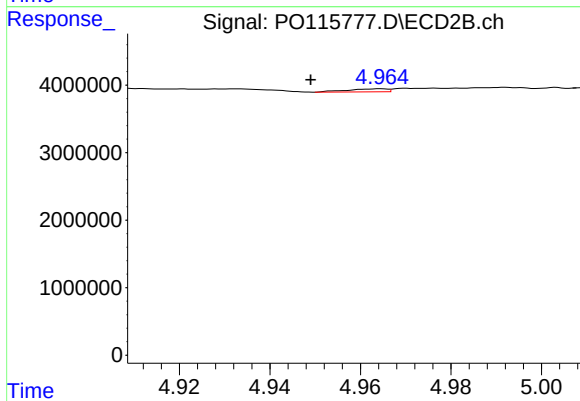

#22 AR-1248-2


R.T.: 4.965 min
Delta R.T.: 0.016 min
Response: 267399
Conc: 1.76 ng/ml

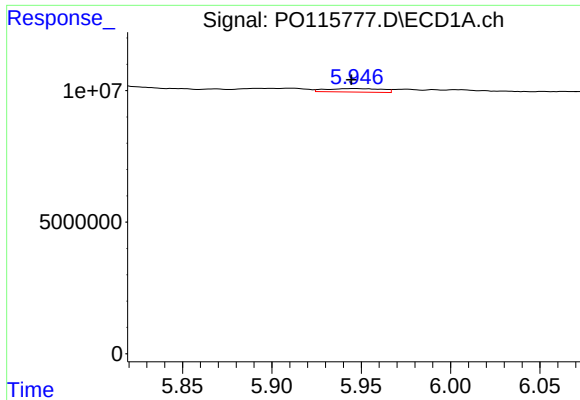

#23 AR-1248-3


R.T.: 5.947 min
Delta R.T.: 0.002 min
Response: 2870294
Conc: 11.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

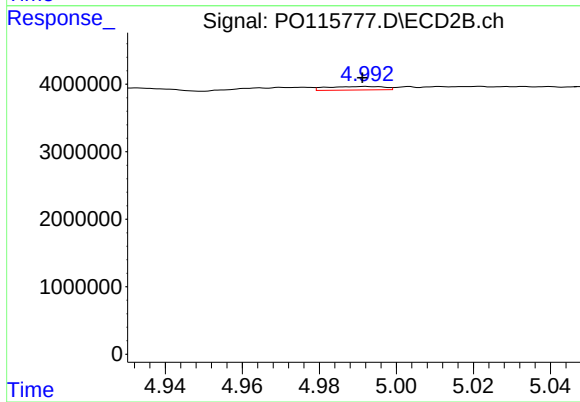


#23 AR-1248-3

R.T.: 4.992 min
Delta R.T.: 0.000 min
Response: 540273
Conc: 3.37 ng/ml

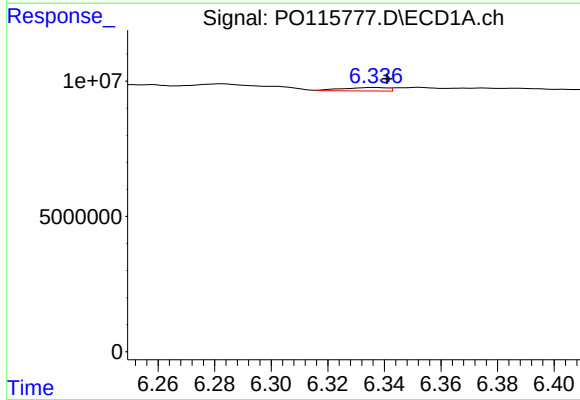


#24 AR-1248-4

R.T.: 6.337 min
Delta R.T.: -0.004 min
Response: 1426957
Conc: 4.84 ng/ml

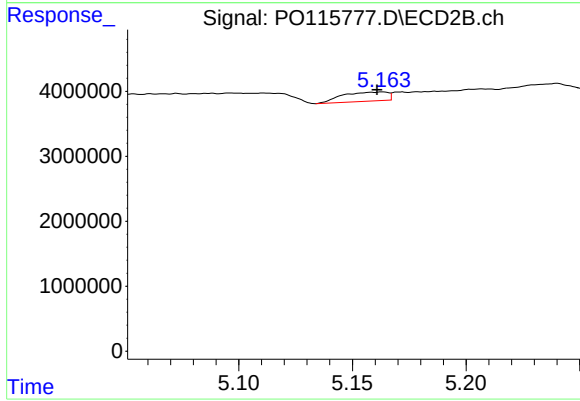

#24 AR-1248-4


R.T.: 5.163 min
Delta R.T.: 0.003 min
Response: 1951752
Conc: 10.43 ng/ml

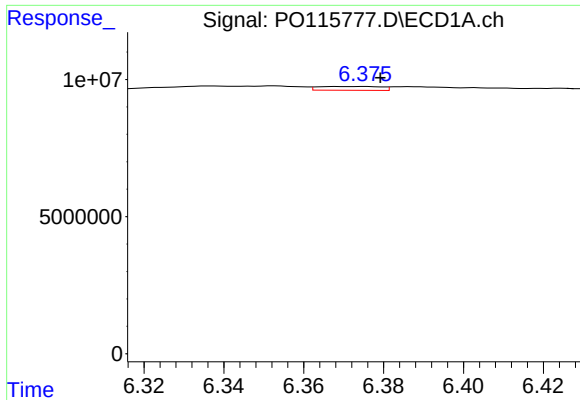

#25 AR-1248-5


R.T.: 6.375 min
Delta R.T.: -0.004 min
Response: 1526780
Conc: 5.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

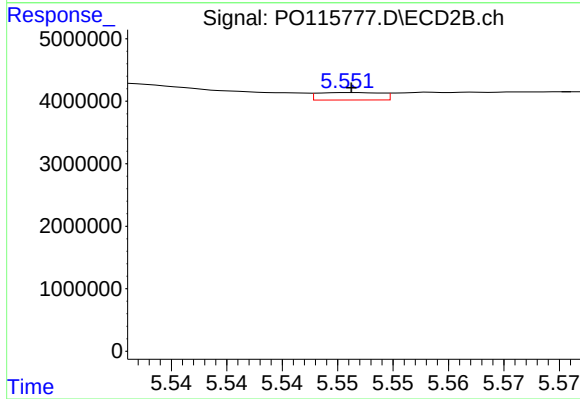


#25 AR-1248-5

R.T.: 5.551 min
Delta R.T.: 0.000 min
Response: 478060
Conc: 2.41 ng/ml

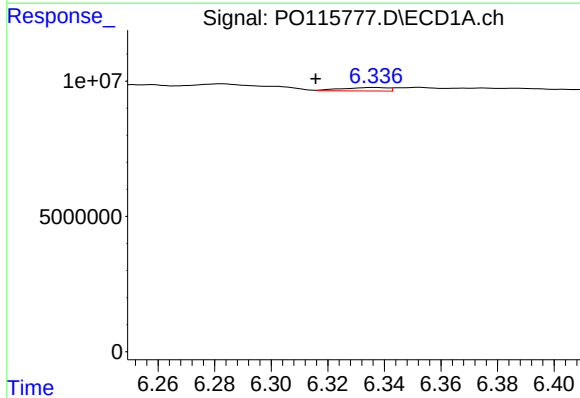


#26 AR-1254-1

R.T.: 6.337 min
Delta R.T.: 0.021 min
Response: 1426957
Conc: 5.52 ng/ml

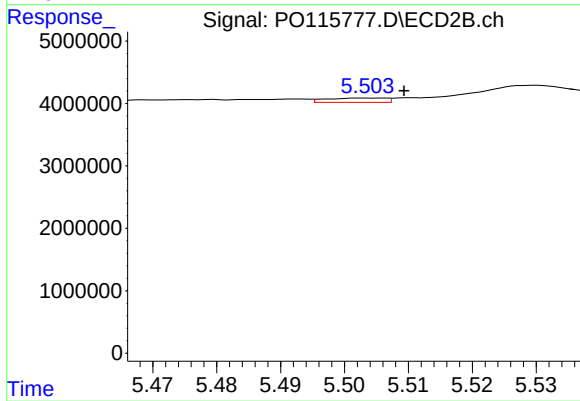

#26 AR-1254-1


R.T.: 5.503 min
Delta R.T.: -0.006 min
Response: 450850
Conc: 1.54 ng/ml

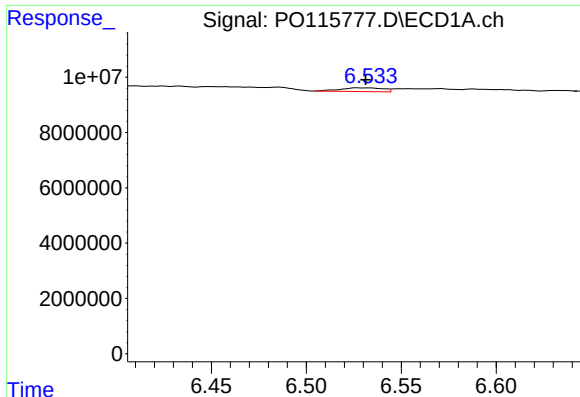

#27 AR-1254-2


R.T.: 6.527 min
Delta R.T.: -0.004 min
Response: 2128538
Conc: 5.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

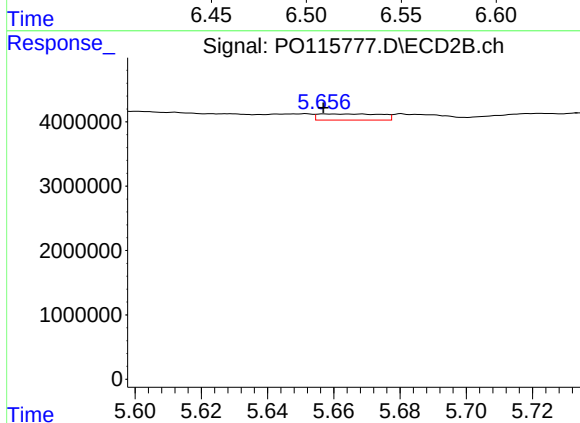


#27 AR-1254-2

R.T.: 5.657 min
Delta R.T.: 0.000 min
Response: 1261158
Conc: 5.01 ng/ml

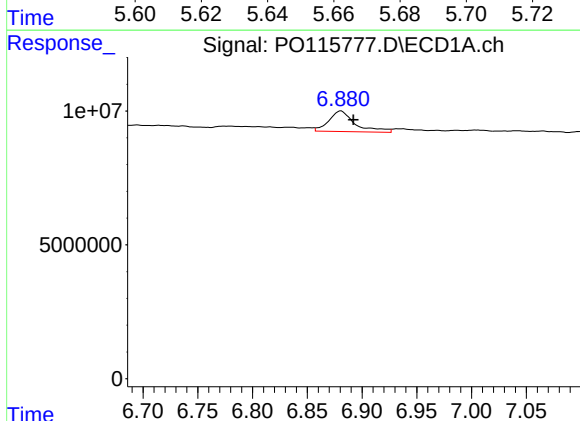


#28 AR-1254-3

R.T.: 6.881 min
Delta R.T.: -0.011 min
Response: 12873243
Conc: 31.35 ng/ml

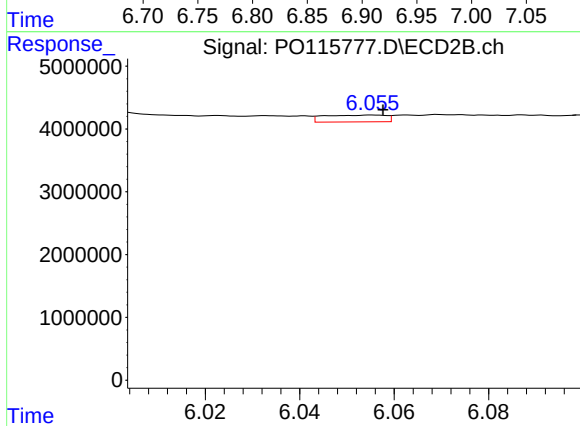

#28 AR-1254-3


R.T.: 6.055 min
Delta R.T.: -0.002 min
Response: 977979
Conc: 2.48 ng/ml

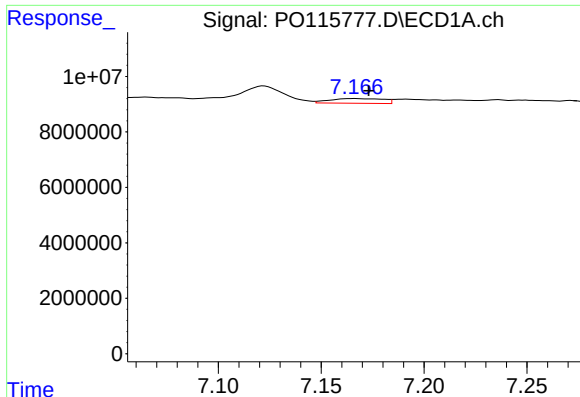

#29 AR-1254-4


R.T.: 7.166 min
Delta R.T.: -0.007 min
Response: 3075837
Conc: 8.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

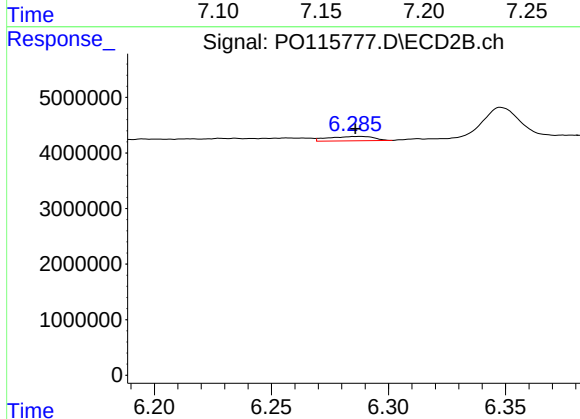


#29 AR-1254-4

R.T.: 6.288 min
Delta R.T.: 0.002 min
Response: 1078185
Conc: 4.03 ng/ml

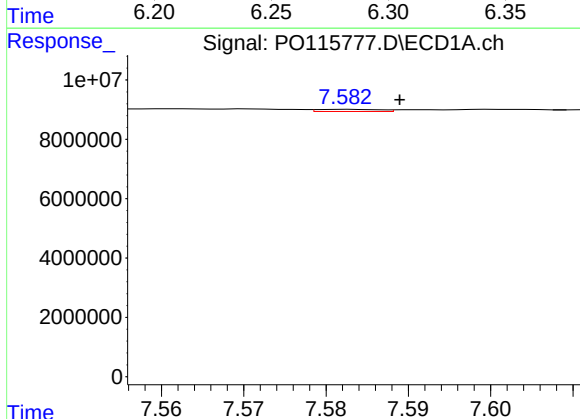


#30 AR-1254-5

R.T.: 7.582 min
Delta R.T.: -0.007 min
Response: 381137
Conc: 1.18 ng/ml

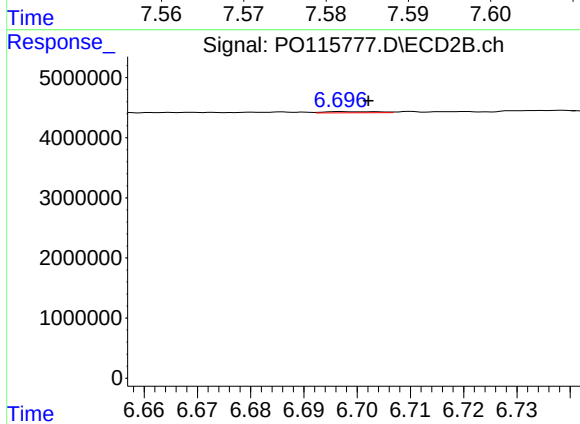

#30 AR-1254-5


R.T.: 6.697 min
Delta R.T.: -0.005 min
Response: 126852
Conc: 0.35 ng/ml

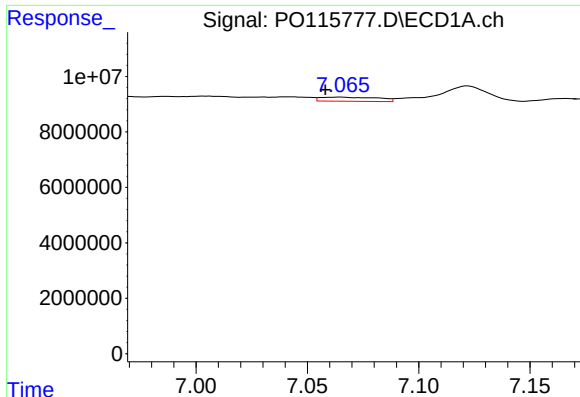

#31 AR-1260-1


R.T.: 7.065 min
Delta R.T.: 0.007 min
Response: 2719632
Conc: 9.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

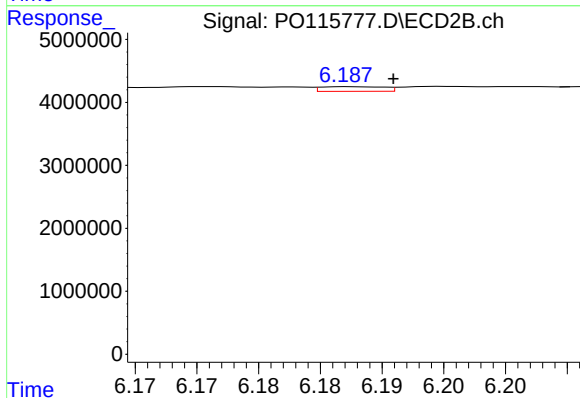


#31 AR-1260-1

R.T.: 6.187 min
Delta R.T.: -0.004 min
Response: 261936
Conc: 1.00 ng/ml

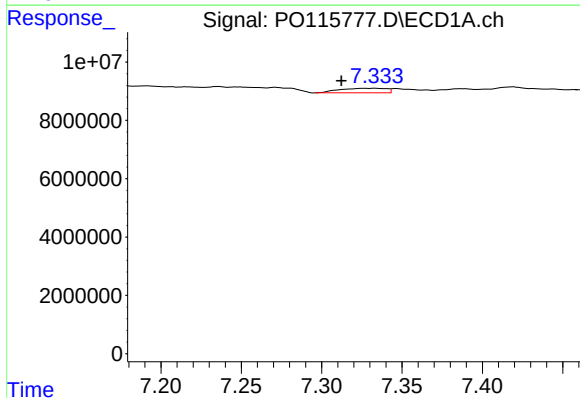


#32 AR-1260-2

R.T.: 7.333 min
Delta R.T.: 0.021 min
Response: 3178970
Conc: 7.26 ng/ml

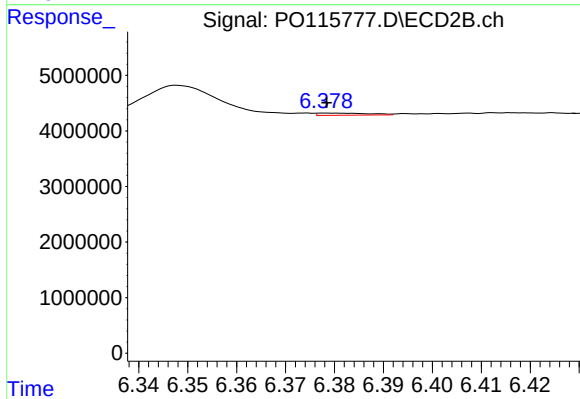

#32 AR-1260-2


R.T.: 6.378 min
Delta R.T.: 0.000 min
Response: 280333
Conc: 0.80 ng/ml

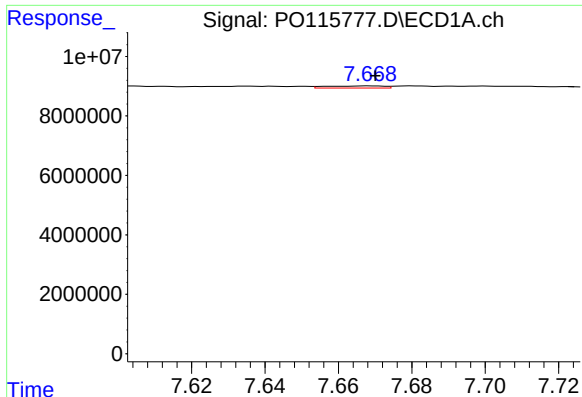

#33 AR-1260-3


R.T.: 7.669 min
Delta R.T.: -0.001 min
Response: 795923
Conc: 2.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

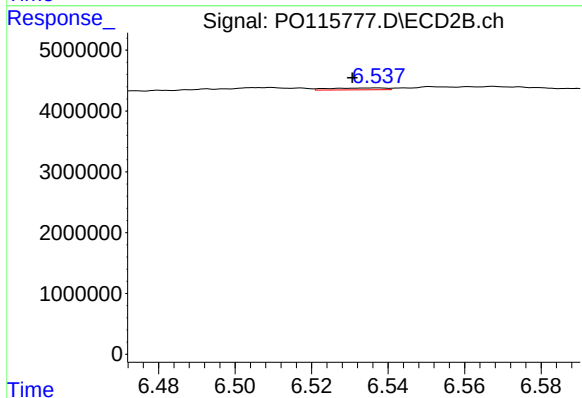


#33 AR-1260-3

R.T.: 6.537 min
Delta R.T.: 0.007 min
Response: 310885
Conc: 0.97 ng/ml

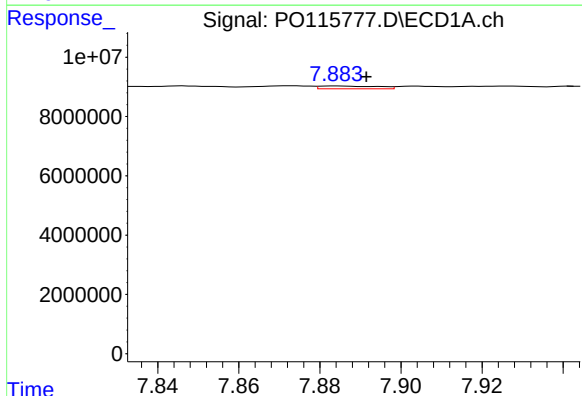


#34 AR-1260-4

R.T.: 7.884 min
Delta R.T.: -0.008 min
Response: 959889
Conc: 3.12 ng/ml

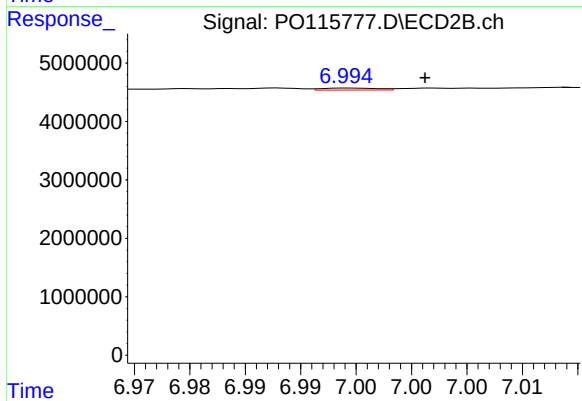

#34 AR-1260-4


R.T.: 6.994 min
Delta R.T.: -0.007 min
Response: 113844
Conc: 0.44 ng/ml

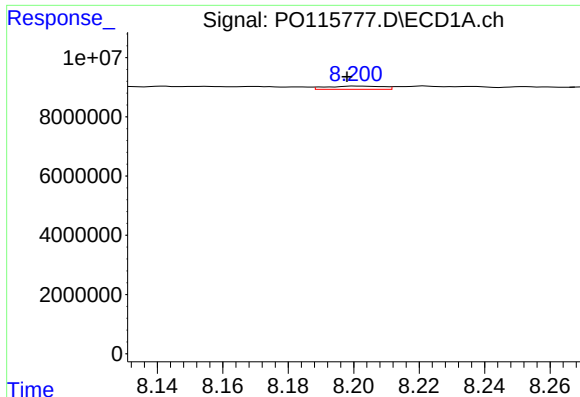

#35 AR-1260-5


R.T.: 8.201 min
Delta R.T.: 0.003 min
Response: 1298610
Conc: 1.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

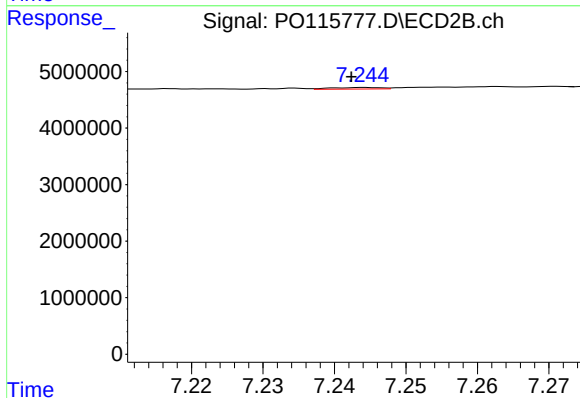


#35 AR-1260-5

R.T.: 7.244 min
Delta R.T.: 0.002 min
Response: 134521
Conc: 0.19 ng/ml

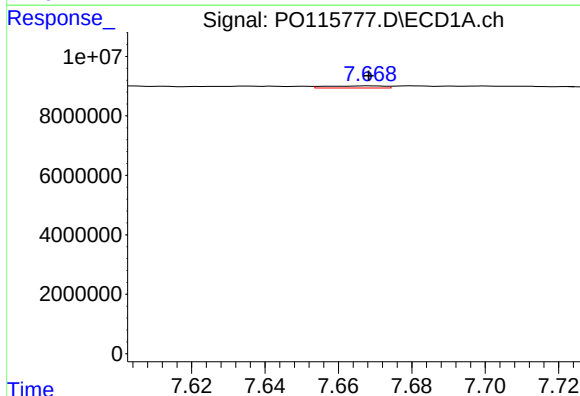


#36 AR-1262-1

R.T.: 7.669 min
Delta R.T.: 0.000 min
Response: 795923
Conc: 3.22 ng/ml

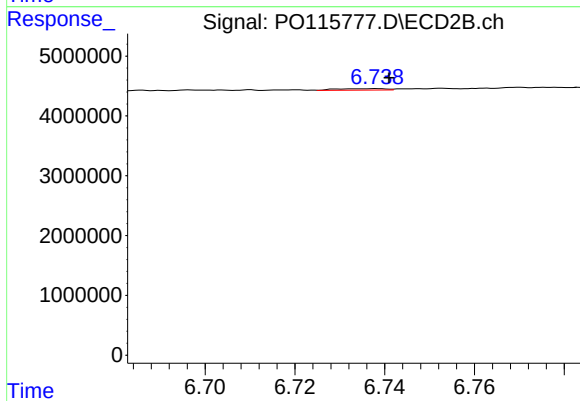

#36 AR-1262-1


R.T.: 6.739 min
Delta R.T.: -0.002 min
Response: 193633
Conc: 0.91 ng/ml

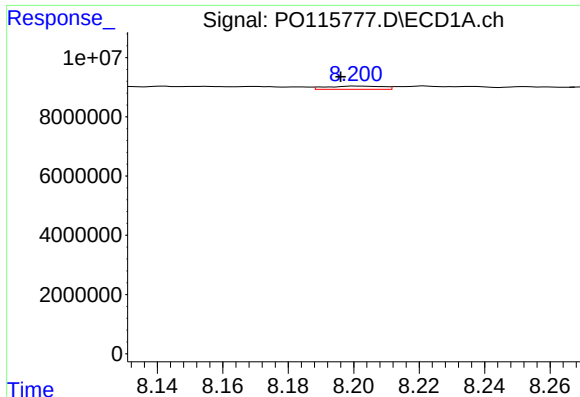

#37 AR-1262-2


R.T.: 8.201 min
Delta R.T.: 0.005 min
Response: 1298610
Conc: 3.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

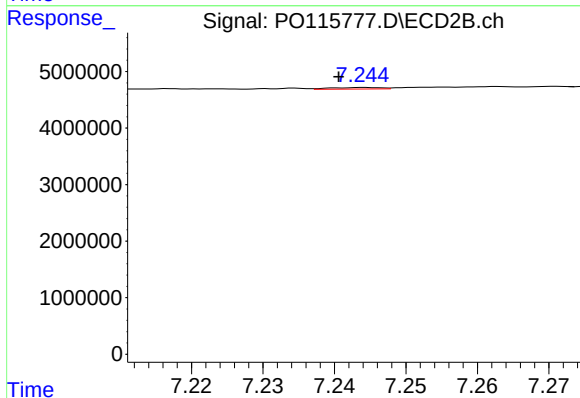


#37 AR-1262-2

R.T.: 7.244 min
Delta R.T.: 0.004 min
Response: 134521
Conc: 0.39 ng/ml

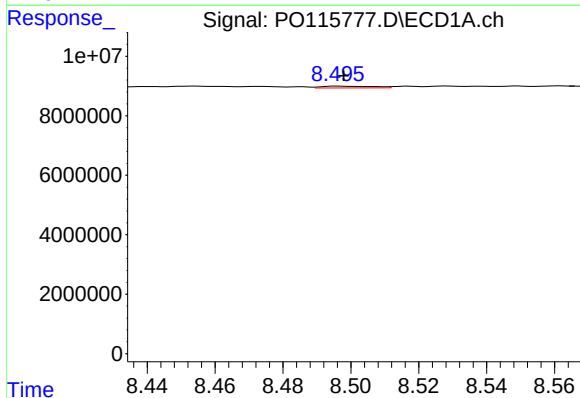


#38 AR-1262-3

R.T.: 8.496 min
Delta R.T.: -0.002 min
Response: 623144
Conc: 2.45 ng/ml

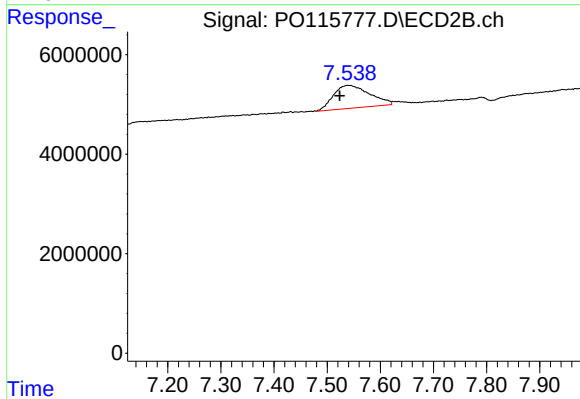

#38 AR-1262-3


R.T.: 7.538 min
Delta R.T.: 0.015 min
Response: 21853095
Conc: 139.73 ng/ml

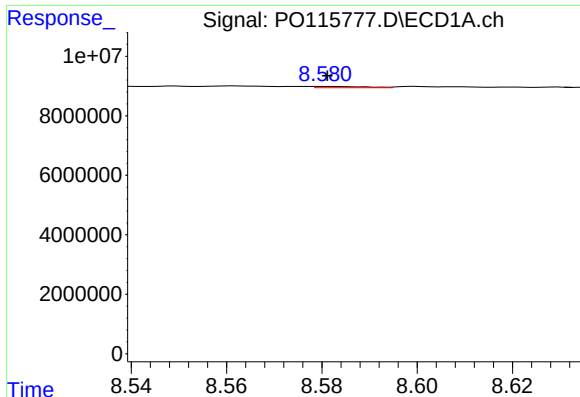

#39 AR-1262-4


R.T.: 8.581 min
Delta R.T.: 0.000 min
Response: 303409
Conc: 1.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

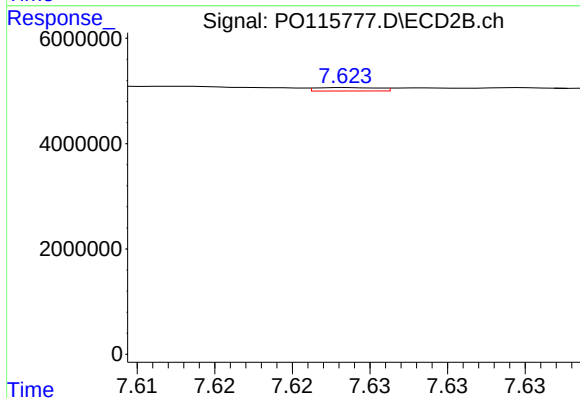


#39 AR-1262-4

R.T.: 7.624 min
Delta R.T.: 0.036 min
Response: 181643
Conc: 0.73 ng/ml

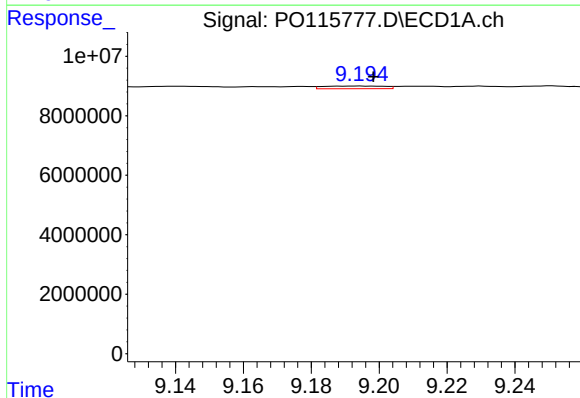


#40 AR-1262-5

R.T.: 9.195 min
Delta R.T.: -0.004 min
Response: 1135037
Conc: 8.43 ng/ml

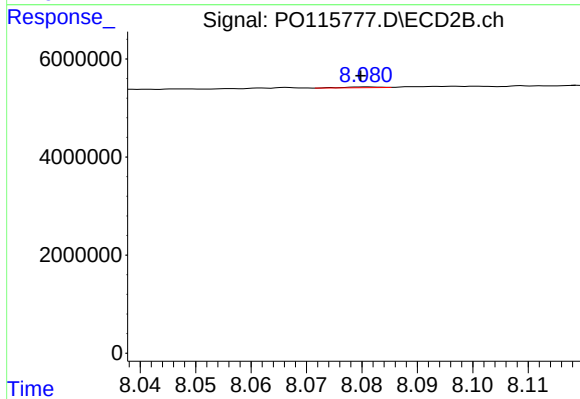

#40 AR-1262-5


R.T.: 8.081 min
Delta R.T.: 0.001 min
Response: 77493
Conc: 0.70 ng/ml

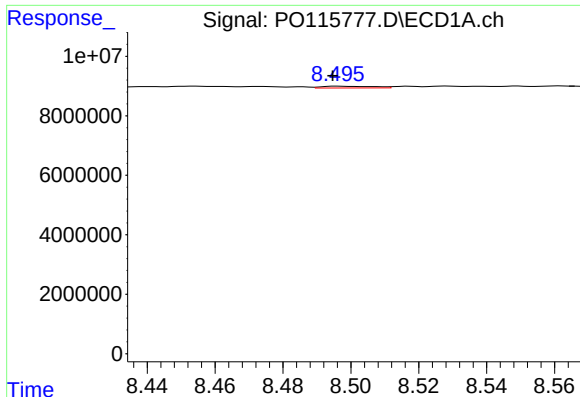

#41 AR-1268-1


R.T.: 8.496 min
Delta R.T.: 0.002 min
Response: 623144
Conc: 0.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

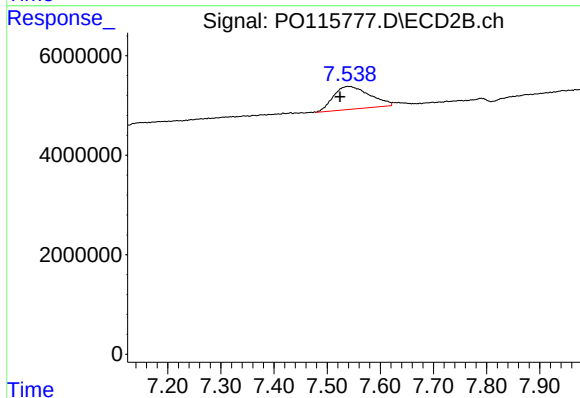


#41 AR-1268-1

R.T.: 7.538 min
Delta R.T.: 0.014 min
Response: 21853095
Conc: 24.67 ng/ml

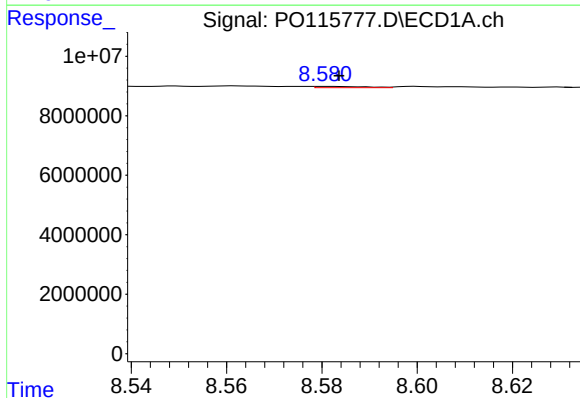


#42 AR-1268-2

R.T.: 8.581 min
Delta R.T.: -0.003 min
Response: 303409
Conc: 0.35 ng/ml

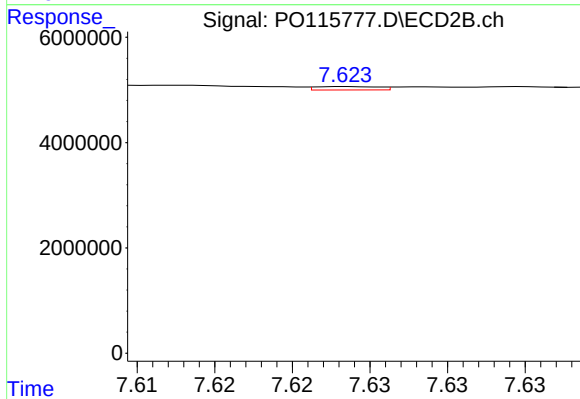

#42 AR-1268-2


R.T.: 7.624 min
Delta R.T.: 0.035 min
Response: 181643
Conc: 0.24 ng/ml

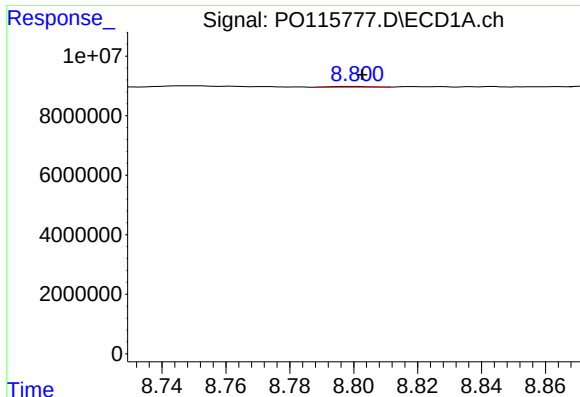

#43 AR-1268-3


R.T.: 8.800 min
Delta R.T.: -0.002 min
Response: 194382
Conc: 0.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

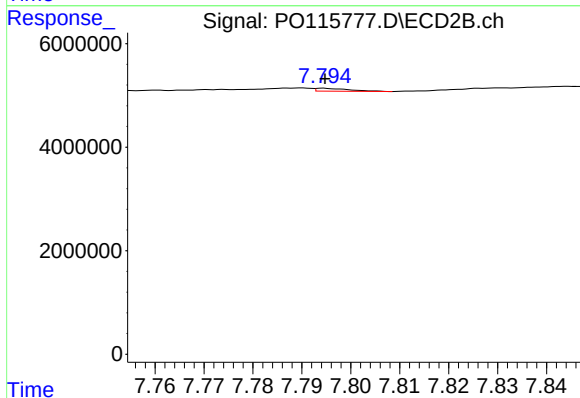


#43 AR-1268-3

R.T.: 7.794 min
Delta R.T.: 0.000 min
Response: 261822
Conc: 0.41 ng/ml

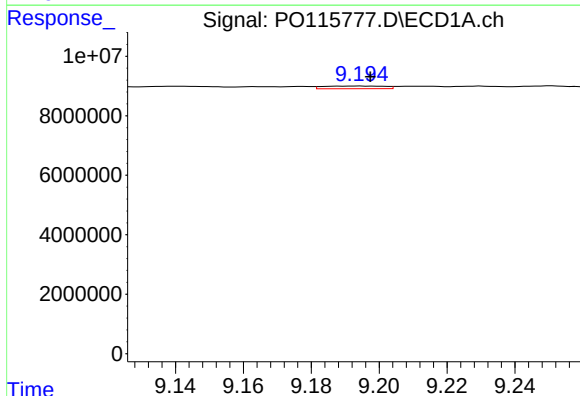


#44 AR-1268-4

R.T.: 9.195 min
Delta R.T.: -0.003 min
Response: 1135037
Conc: 3.64 ng/ml

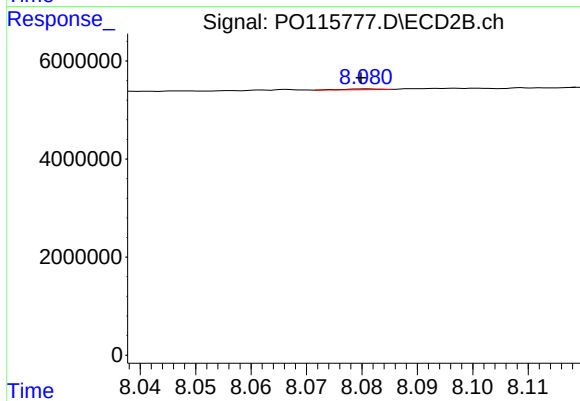

#44 AR-1268-4


R.T.: 8.081 min
Delta R.T.: 0.001 min
Response: 77493
Conc: 0.30 ng/ml

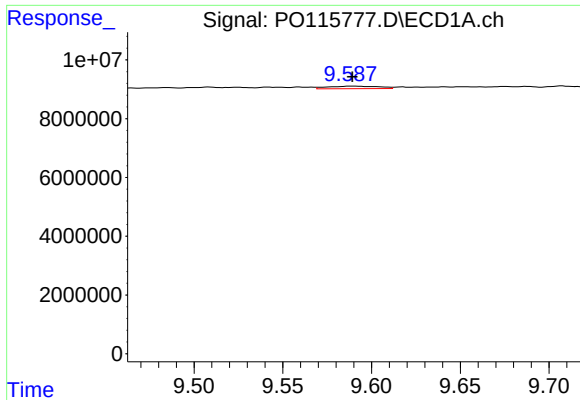

#45 AR-1268-5

R.T.: 9.589 min
Delta R.T.: 0.000 min
Response: 1732212
Conc: 0.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

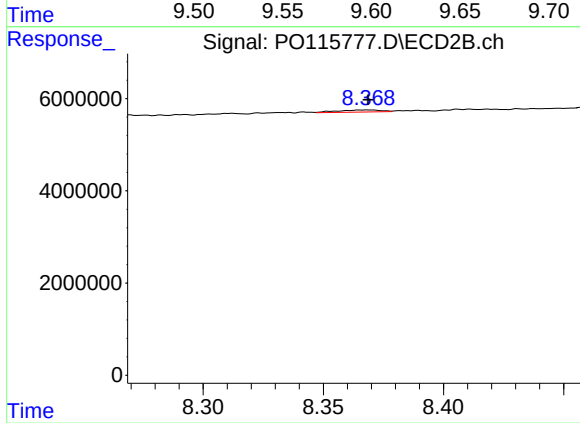

#45 AR-1268-5

R.T.: 8.368 min
Delta R.T.: 0.000 min
Response: 572209
Conc: 0.34 ng/ml