

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO121225\
 Data File : PO115778.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Dec 2025 02:15
 Operator : YP/AJ
 Sample : Q3530-07
 Misc : AR1232 25PPB WATER LOD
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 13 03:50:03 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO120425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 05 02:11:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.331	3.636	138.2E6	85337364	17.787	17.511
2)	SA Decachlor...	9.904	8.615	97868273	73663467	18.602	17.130
Target Compounds							
3)	L1 AR-1016-1	5.469	4.710	3270683	2272903	13.153	12.302
4)	L1 AR-1016-2	5.491	4.729	4699572	2923024	12.340	11.059
5)	L1 AR-1016-3	5.551	4.903	2362657	2171829	11.052	14.351 #
6)	L1 AR-1016-4	5.647	4.938	1254902	503158	7.027	4.464 #
7)	L1 AR-1016-5	5.940	5.159	3474845	6420482	19.808	43.873 #
8)	L2 AR-1221-1	4.540	3.846	1169846	857670	14.407	15.205
9)	L2 AR-1221-2	4.626	3.933	4099780	2454745	65.056	57.835
10)	L2 AR-1221-3	4.689	4.006	5310392	2556887	28.441	19.884 #
11)	L3 AR-1232-1	4.689	4.006	5310392	2556887	35.482	23.933 #
12)	L3 AR-1232-2	5.207	4.729	3917471	2923024	48.453	26.336 #
13)	L3 AR-1232-3	5.491	4.903	4699572	2171829	30.536	33.225
14)	L3 AR-1232-4	5.647	4.988	1254902	2035894	17.919	39.663 #
15)	L3 AR-1232-5	5.739	5.159	1950501	6420482	37.555	117.273 #
16)	L4 AR-1242-1	5.469	4.710	3270683	2272903	16.467	15.963
17)	L4 AR-1242-2	5.491	4.729	4699572	2923024	16.045	13.962
18)	L4 AR-1242-3	5.551	4.903	2362657	2171829	13.995	18.183 #
19)	L4 AR-1242-4	5.647	4.988	1254902	2035894	9.182	18.662 #
20)	L4 AR-1242-5	6.373	5.506	5955147	1957452	39.322	14.172 #
21)	L5 AR-1248-1	5.469	4.710	3270683	2272903	21.551	20.325
22)	L5 AR-1248-2	5.739	4.938	1950501	503158	9.713	3.304 #
23)	L5 AR-1248-3	5.940	4.988	3474845	2035894	14.091	12.683
24)	L5 AR-1248-4	6.338	5.159	4789306	6420482	16.243	34.307 #
25)	L5 AR-1248-5	6.373	5.529	5955147	10929516	22.999	55.212 #
26)	L6 AR-1254-1	6.303	5.506	5402673	1957452	20.883	6.697 #
27)	L6 AR-1254-2	6.526	5.654	3855929	2496722	9.582	9.915
28)	L6 AR-1254-3	6.878	6.056	20906107	5262076	50.920	13.370 #
29)	L6 AR-1254-4	7.164	6.290	3550515	2453886	10.230	9.171
30)	L6 AR-1254-5	7.574	6.697	244788	586854	0.755	1.641 #
31)	L7 AR-1260-1	7.054	6.199	1239197	1655611	4.278	6.315 #
32)	L7 AR-1260-2	7.323	6.389	1655819	116766	3.783	0.333 #
33)	L7 AR-1260-3	7.672	6.554	274791	1470323	0.816	4.577 #
34)	L7 AR-1260-4	7.897	7.001	368589	461685	1.199	1.798 #
35)	L7 AR-1260-5	8.211	7.238	525994	324682	0.722	0.463 #
36)	L8 AR-1262-1	7.672	6.740	274791	306913	1.113	1.441 #
37)	L8 AR-1262-2	8.211	7.238	525994	324682	1.329	0.932 #
38)	L8 AR-1262-3	8.499	7.538	279904	51746381	1.098	330.879 #
39)	L8 AR-1262-4	8.574	7.538f	262264	51746381	1.354	209.185 #
40)	L8 AR-1262-5	9.198	8.115f	264125	201866	1.961	1.811
41)	L9 AR-1268-1	8.499	7.538	279904	51746381	0.281	58.408 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121225\
 Data File : PO115778.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Dec 2025 02:15
 Operator : YP/AJ
 Sample : Q3530-07
 Misc : AR1232 25PPB WATER LOD
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 13 03:50:03 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 05 02:11:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.574	7.538f	262264	51746381	0.307	69.081 #
43) L9	AR-1268-3	8.797	7.793	46135	504446	0.062	0.792 #
44) L9	AR-1268-4	9.198	8.115	264125	201866	0.846	0.784
45) L9	AR-1268-5	9.588	8.363	1035732	166173	0.476	0.099 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO121225\
Data File : PO115778.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Dec 2025 02:15
Operator : YP/AJ
Sample : Q3530-07
Misc : AR1232 25PPB WATER LOD
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_0
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 13 03:50:03 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO120425.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 05 02:11:05 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

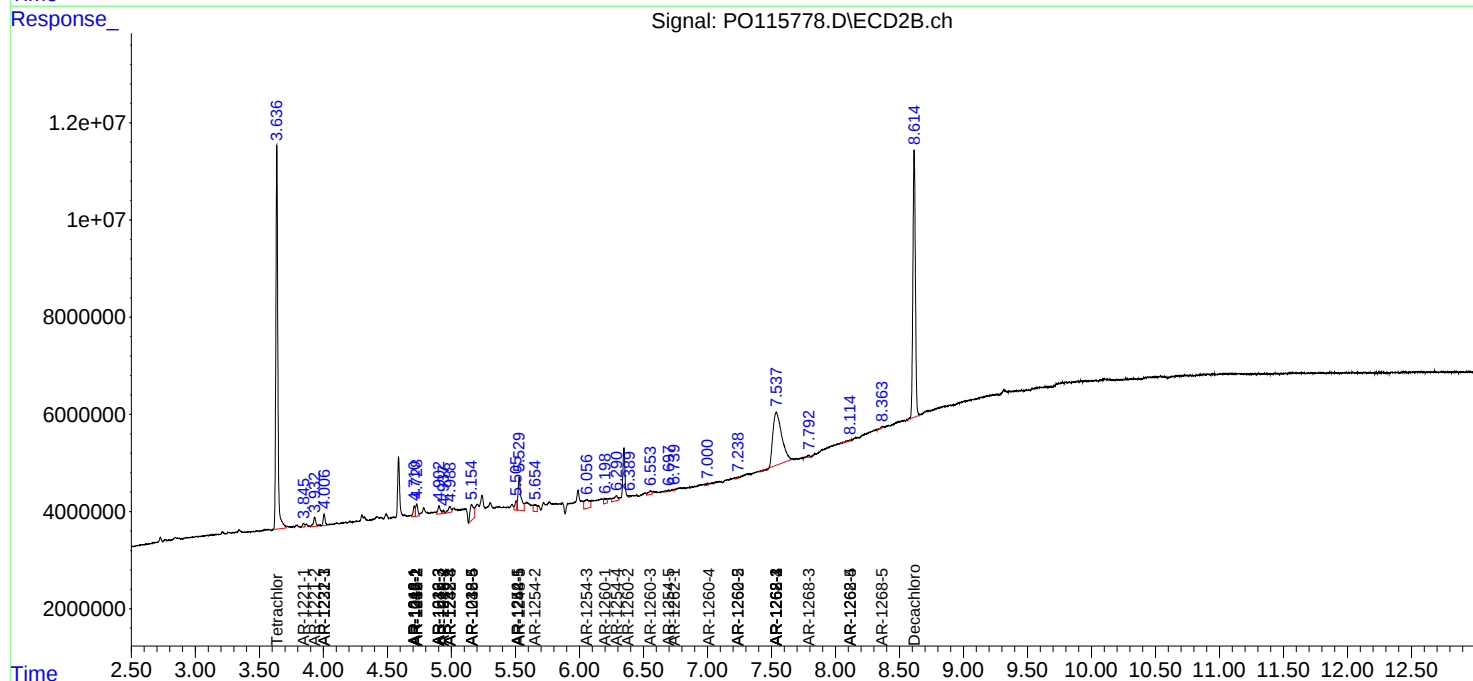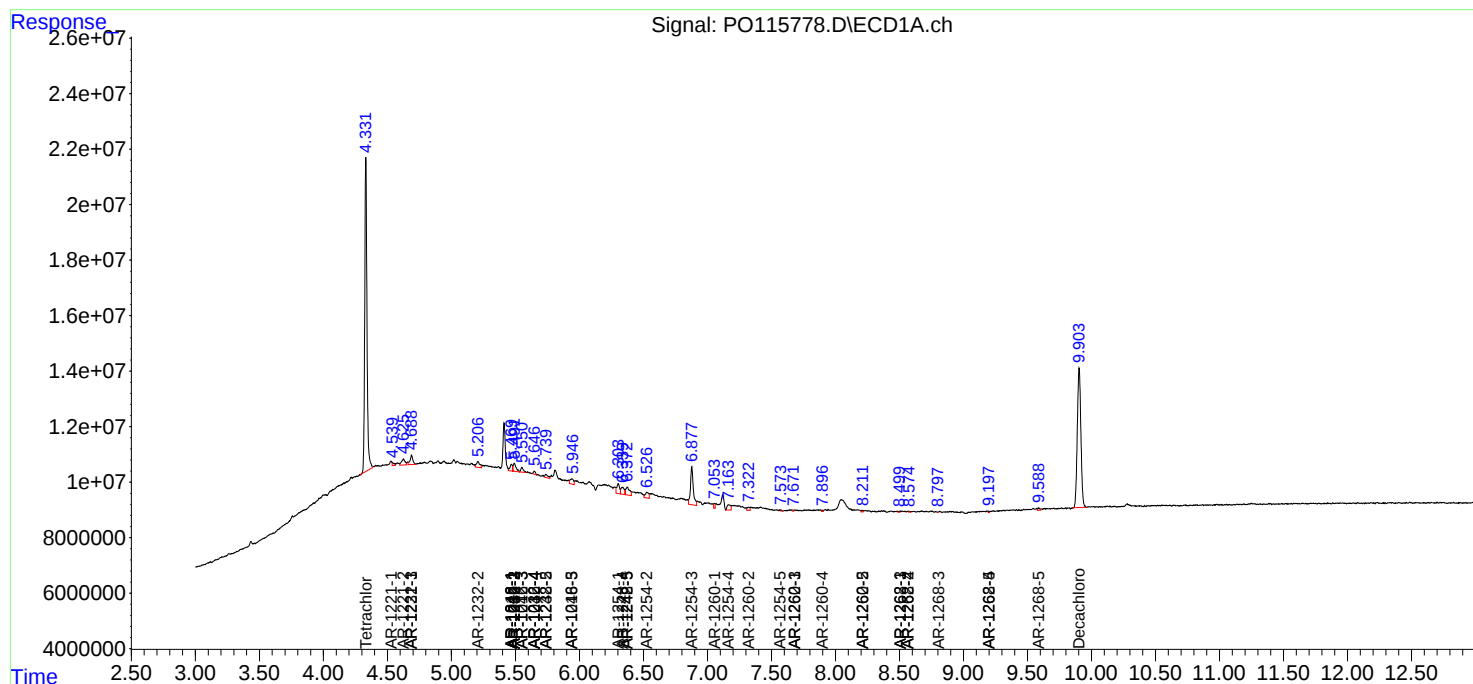


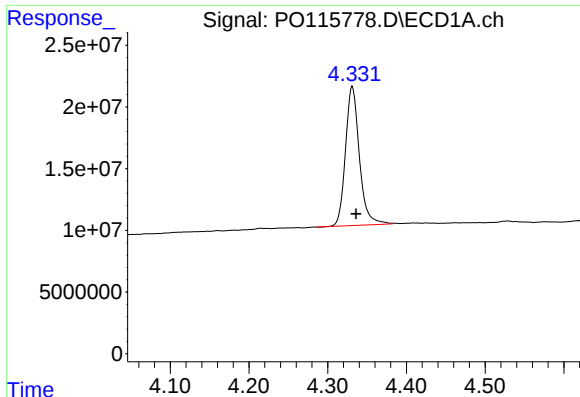

#1 Tetrachloro-m-xylene


R.T.: 4.331 min
Delta R.T.: -0.005 min
Response: 138152198
Conc: 17.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

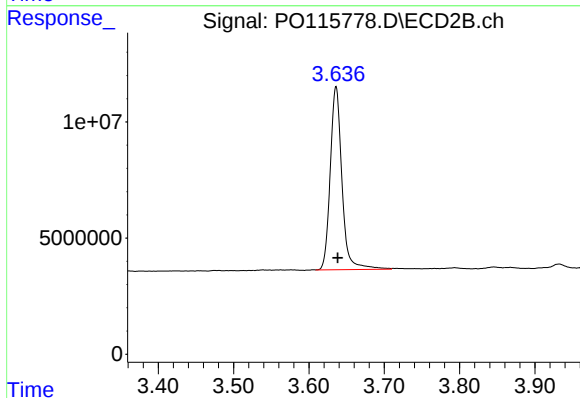


#1 Tetrachloro-m-xylene

R.T.: 3.636 min
Delta R.T.: -0.002 min
Response: 85337364
Conc: 17.51 ng/ml

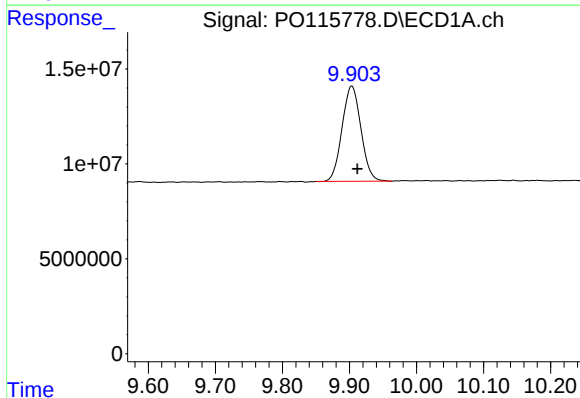


#2 Decachlorobiphenyl

R.T.: 9.904 min
Delta R.T.: -0.009 min
Response: 97868273
Conc: 18.60 ng/ml

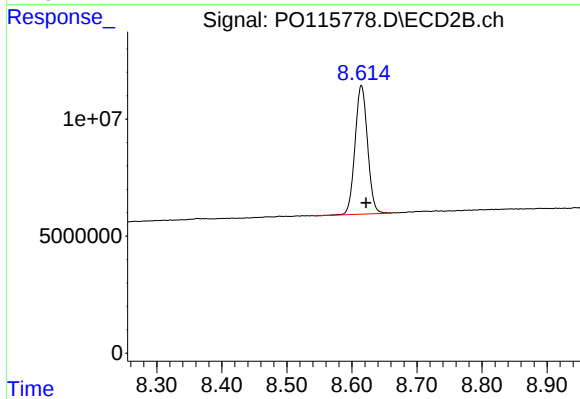

#2 Decachlorobiphenyl


R.T.: 8.615 min
Delta R.T.: -0.007 min
Response: 73663467
Conc: 17.13 ng/ml

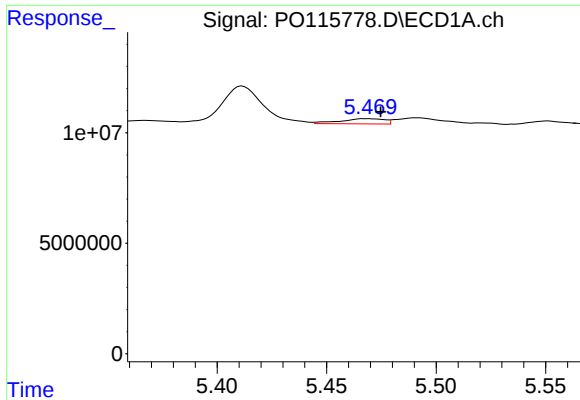

#3 AR-1016-1


R.T.: 5.469 min
Delta R.T.: -0.005 min
Response: 3270683
Conc: 13.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

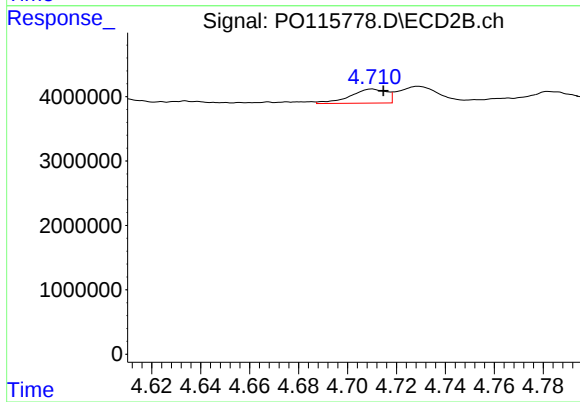


#3 AR-1016-1

R.T.: 4.710 min
Delta R.T.: -0.005 min
Response: 2272903
Conc: 12.30 ng/ml

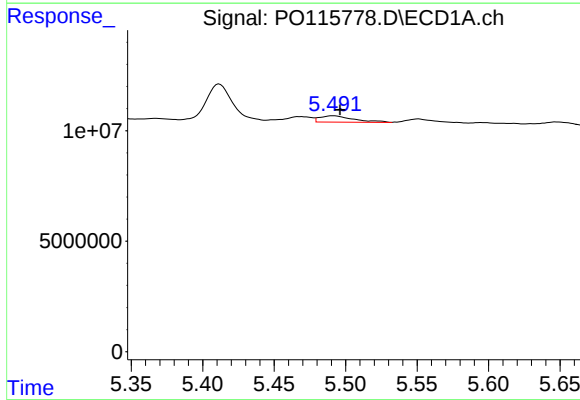


#4 AR-1016-2

R.T.: 5.491 min
Delta R.T.: -0.005 min
Response: 4699572
Conc: 12.34 ng/ml

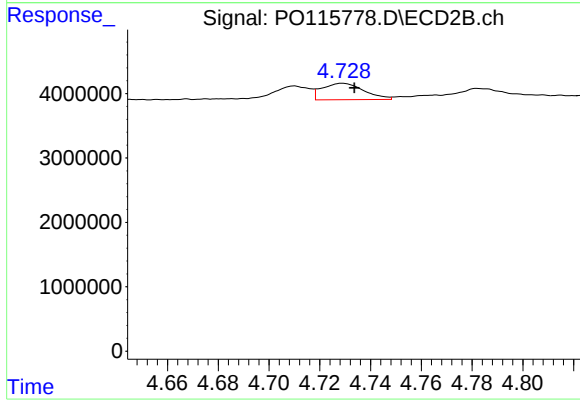

#4 AR-1016-2


R.T.: 4.729 min
Delta R.T.: -0.005 min
Response: 2923024
Conc: 11.06 ng/ml

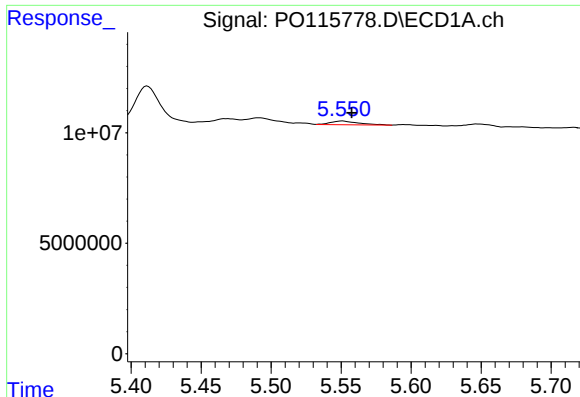

#5 AR-1016-3


R.T.: 5.551 min
Delta R.T.: -0.007 min
Response: 2362657
Conc: 11.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

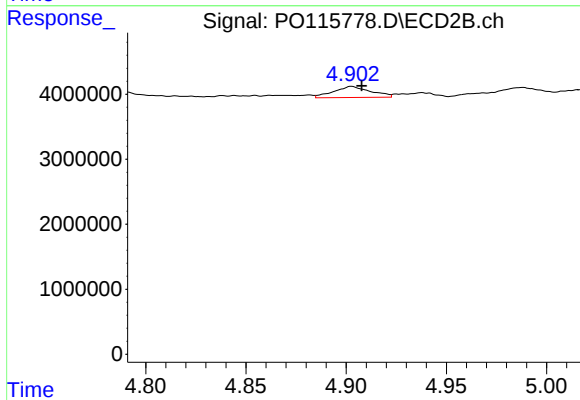


#5 AR-1016-3

R.T.: 4.903 min
Delta R.T.: -0.005 min
Response: 2171829
Conc: 14.35 ng/ml

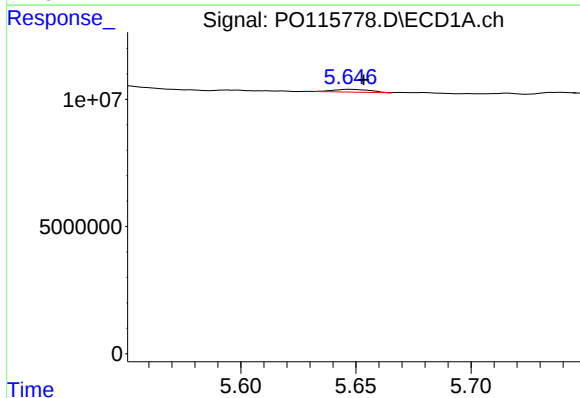


#6 AR-1016-4

R.T.: 5.647 min
Delta R.T.: -0.006 min
Response: 1254902
Conc: 7.03 ng/ml

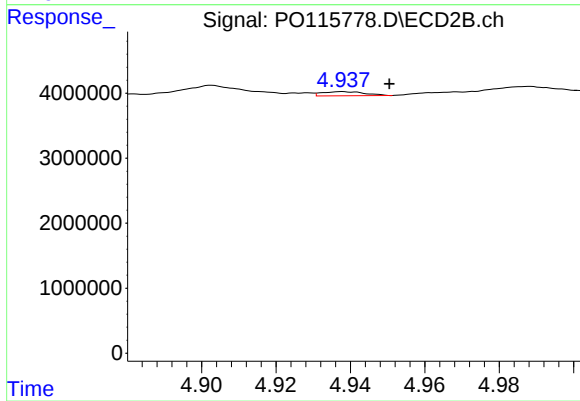

#6 AR-1016-4


R.T.: 4.938 min
Delta R.T.: -0.013 min
Response: 503158
Conc: 4.46 ng/ml

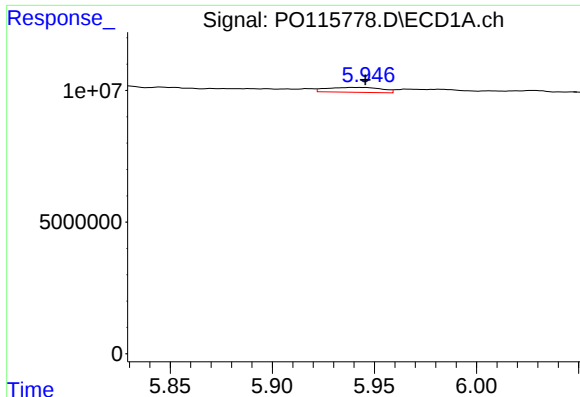

#7 AR-1016-5


R.T.: 5.940 min
Delta R.T.: -0.006 min
Response: 3474845
Conc: 19.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

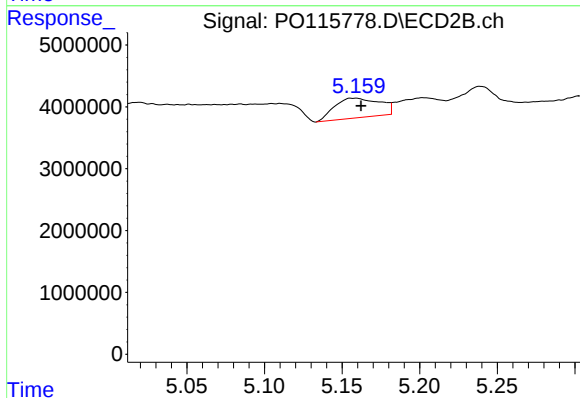


#7 AR-1016-5

R.T.: 5.159 min
Delta R.T.: -0.003 min
Response: 6420482
Conc: 43.87 ng/ml

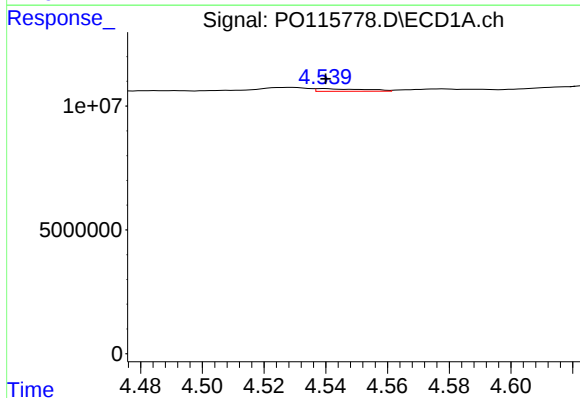


#8 AR-1221-1

R.T.: 4.540 min
Delta R.T.: 0.000 min
Response: 1169846
Conc: 14.41 ng/ml

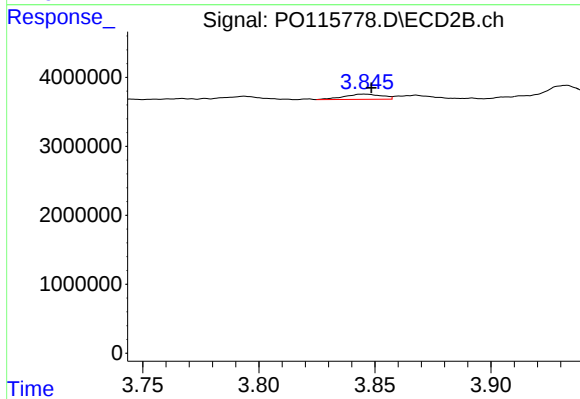

#8 AR-1221-1


R.T.: 3.846 min
Delta R.T.: -0.003 min
Response: 857670
Conc: 15.21 ng/ml

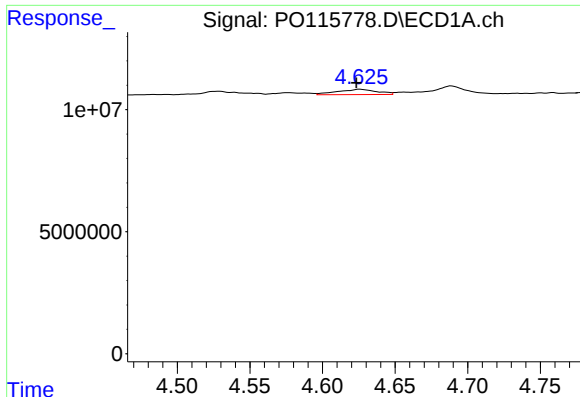

#9 AR-1221-2


R.T.: 4.626 min
Delta R.T.: 0.002 min
Response: 4099780
Conc: 65.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

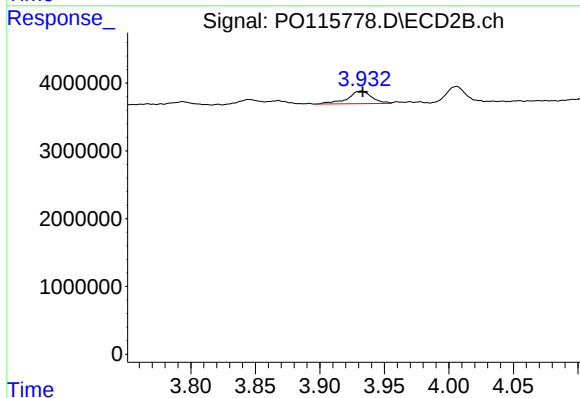


#9 AR-1221-2

R.T.: 3.933 min
Delta R.T.: 0.000 min
Response: 2454745
Conc: 57.84 ng/ml

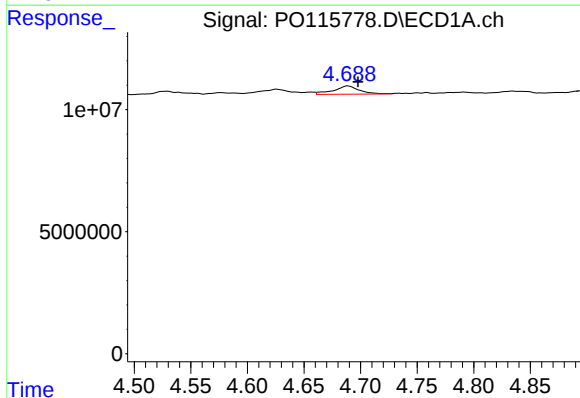


#10 AR-1221-3

R.T.: 4.689 min
Delta R.T.: -0.009 min
Response: 5310392
Conc: 28.44 ng/ml

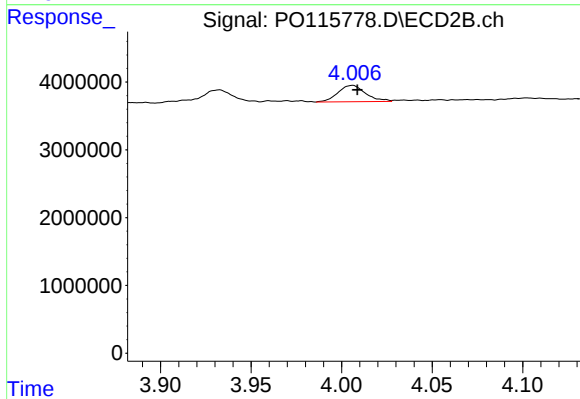

#10 AR-1221-3


R.T.: 4.006 min
Delta R.T.: -0.003 min
Response: 2556887
Conc: 19.88 ng/ml

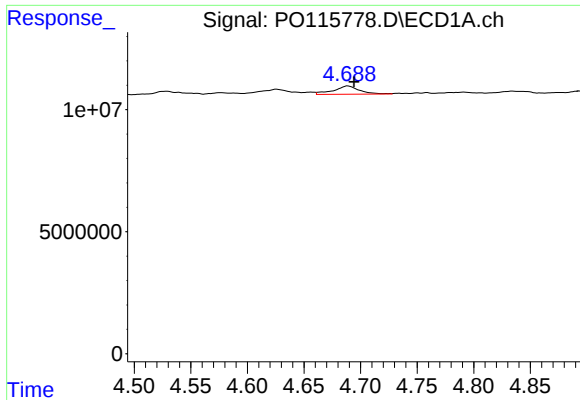

#11 AR-1232-1


R.T.: 4.689 min
Delta R.T.: -0.006 min
Response: 5310392
Conc: 35.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

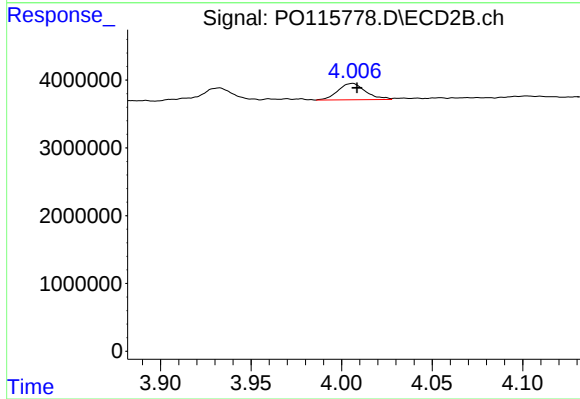


#11 AR-1232-1

R.T.: 4.006 min
Delta R.T.: -0.002 min
Response: 2556887
Conc: 23.93 ng/ml

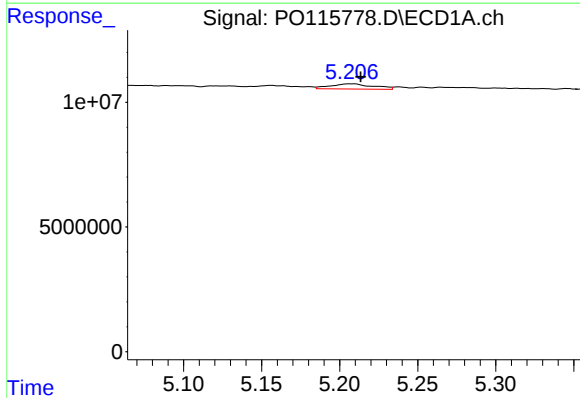


#12 AR-1232-2

R.T.: 5.207 min
Delta R.T.: -0.006 min
Response: 3917471
Conc: 48.45 ng/ml

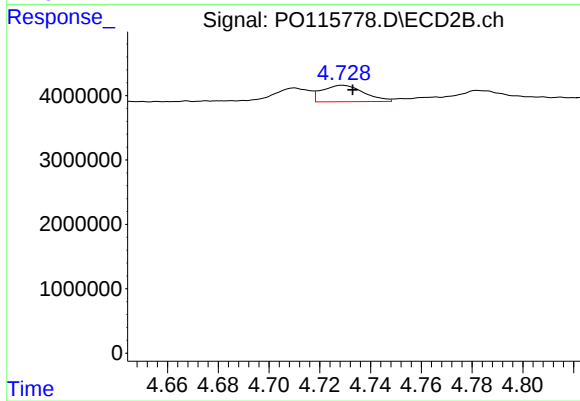

#12 AR-1232-2


R.T.: 4.729 min
Delta R.T.: -0.004 min
Response: 2923024
Conc: 26.34 ng/ml

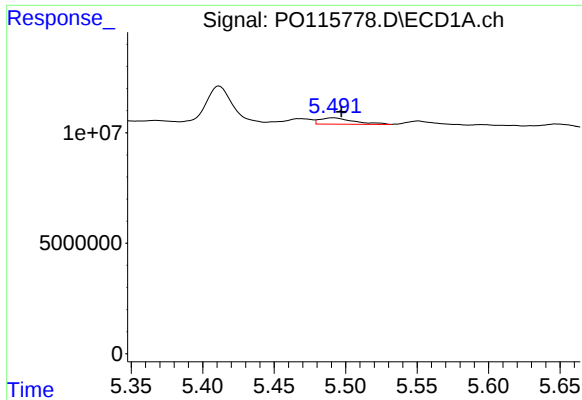

#13 AR-1232-3


R.T.: 5.491 min
Delta R.T.: -0.006 min
Response: 4699572
Conc: 30.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

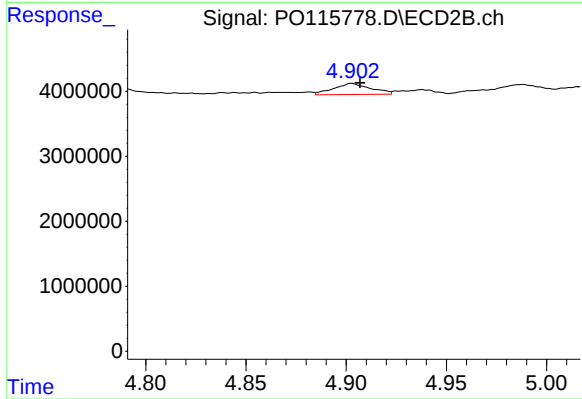


#13 AR-1232-3

R.T.: 4.903 min
Delta R.T.: -0.004 min
Response: 2171829
Conc: 33.23 ng/ml

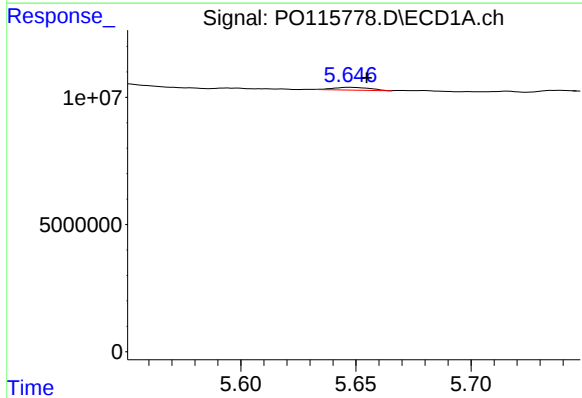


#14 AR-1232-4

R.T.: 5.647 min
Delta R.T.: -0.007 min
Response: 1254902
Conc: 17.92 ng/ml

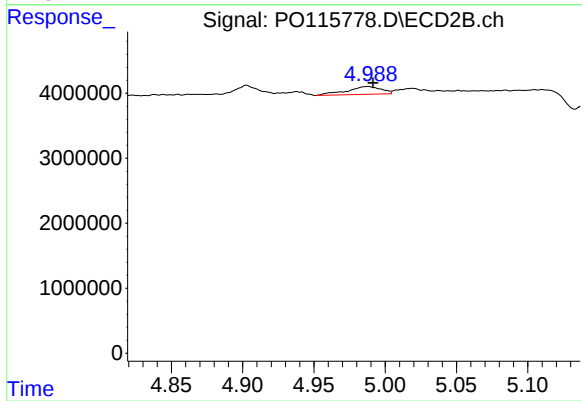

#14 AR-1232-4


R.T.: 4.988 min
Delta R.T.: -0.003 min
Response: 2035894
Conc: 39.66 ng/ml

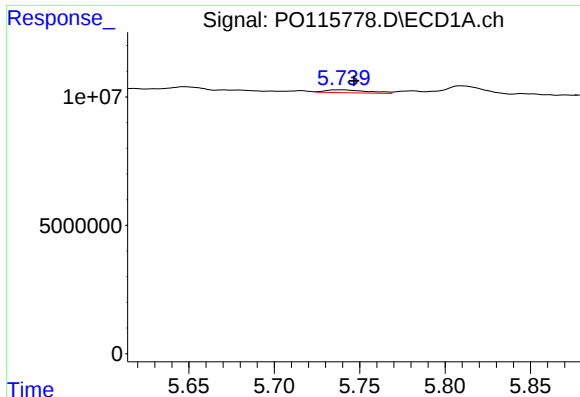

#15 AR-1232-5


R.T.: 5.739 min
Delta R.T.: -0.008 min
Response: 1950501
Conc: 37.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

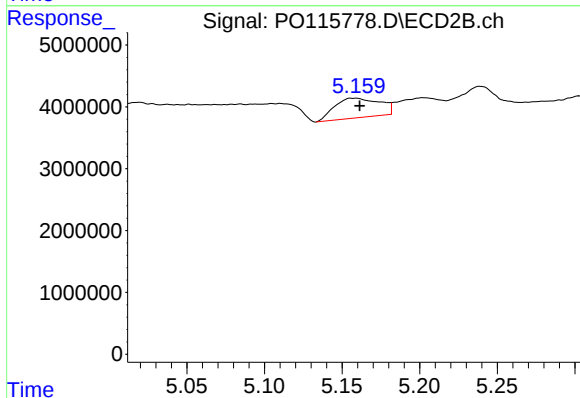


#15 AR-1232-5

R.T.: 5.159 min
Delta R.T.: -0.002 min
Response: 6420482
Conc: 117.27 ng/ml

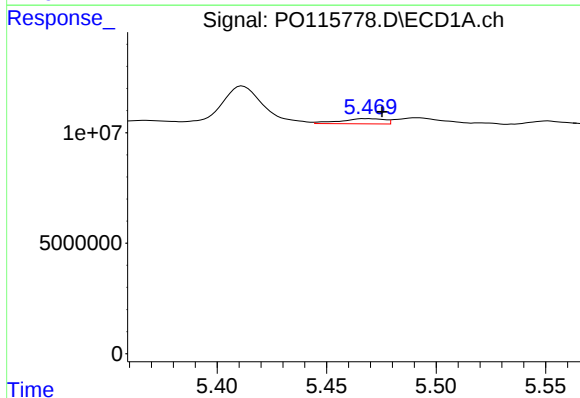


#16 AR-1242-1

R.T.: 5.469 min
Delta R.T.: -0.006 min
Response: 3270683
Conc: 16.47 ng/ml

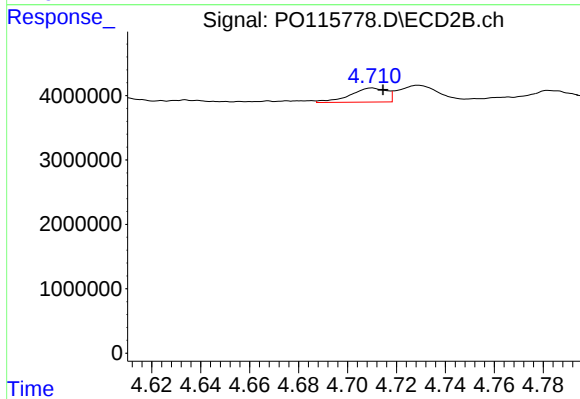

#16 AR-1242-1


R.T.: 4.710 min
Delta R.T.: -0.004 min
Response: 2272903
Conc: 15.96 ng/ml

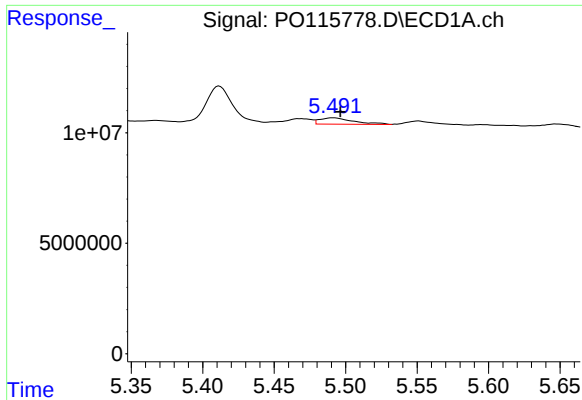

#17 AR-1242-2


R.T.: 5.491 min
Delta R.T.: -0.005 min
Response: 4699572
Conc: 16.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

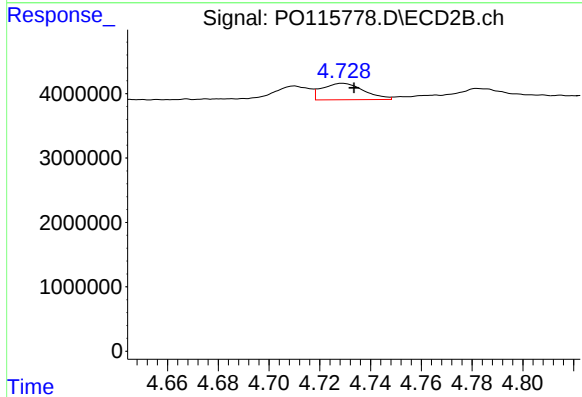


#17 AR-1242-2

R.T.: 4.729 min
Delta R.T.: -0.005 min
Response: 2923024
Conc: 13.96 ng/ml

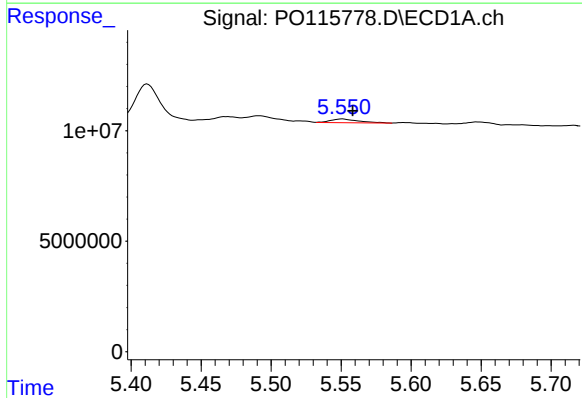


#18 AR-1242-3

R.T.: 5.551 min
Delta R.T.: -0.007 min
Response: 2362657
Conc: 14.00 ng/ml

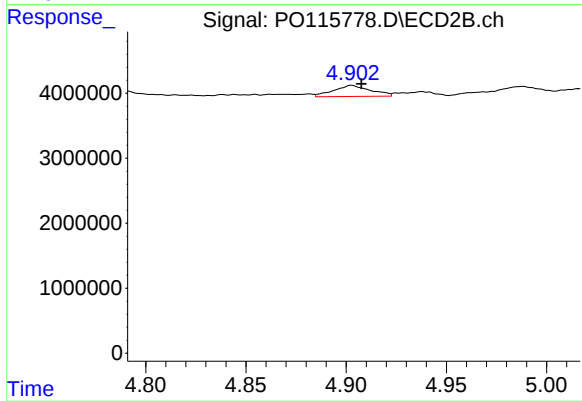

#18 AR-1242-3


R.T.: 4.903 min
Delta R.T.: -0.005 min
Response: 2171829
Conc: 18.18 ng/ml

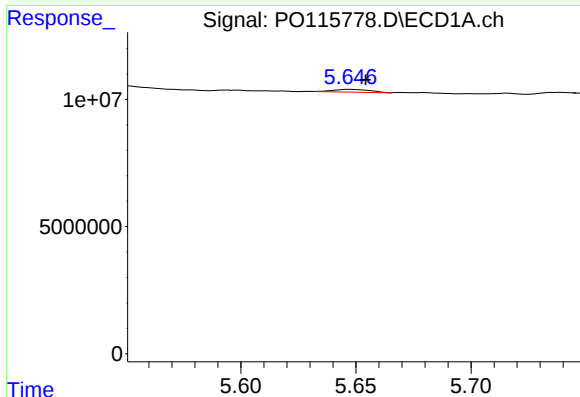

#19 AR-1242-4


R.T.: 5.647 min
Delta R.T.: -0.007 min
Response: 1254902
Conc: 9.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

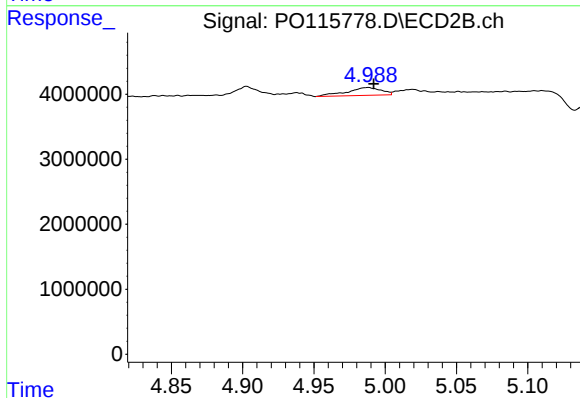


#19 AR-1242-4

R.T.: 4.988 min
Delta R.T.: -0.004 min
Response: 2035894
Conc: 18.66 ng/ml

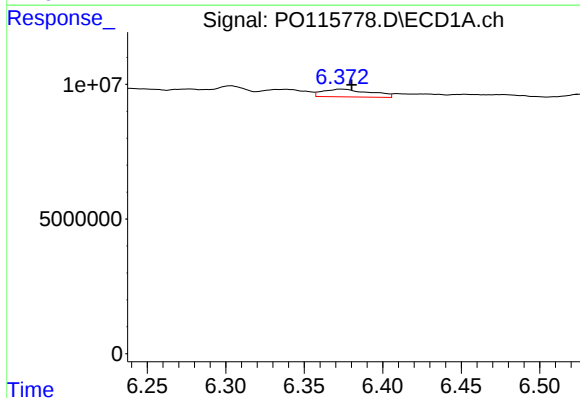


#20 AR-1242-5

R.T.: 6.373 min
Delta R.T.: -0.007 min
Response: 5955147
Conc: 39.32 ng/ml

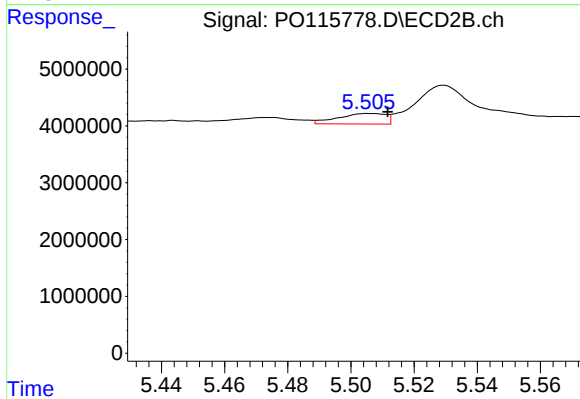

#20 AR-1242-5


R.T.: 5.506 min
Delta R.T.: -0.006 min
Response: 1957452
Conc: 14.17 ng/ml

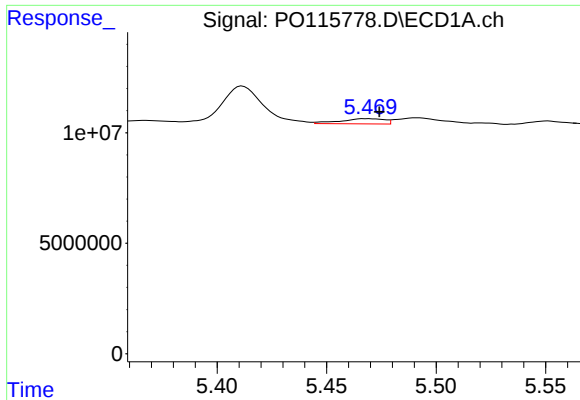

#21 AR-1248-1


R.T.: 5.469 min
Delta R.T.: -0.005 min
Response: 3270683
Conc: 21.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

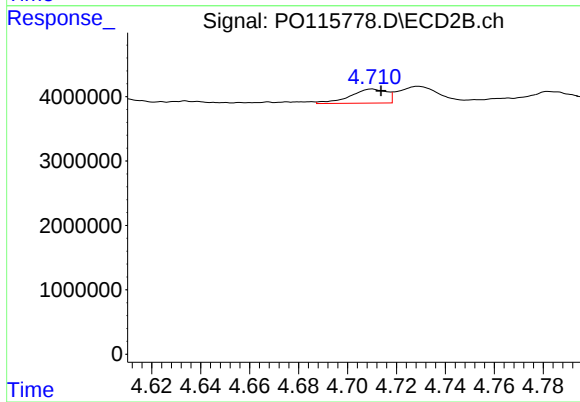


#21 AR-1248-1

R.T.: 4.710 min
Delta R.T.: -0.004 min
Response: 2272903
Conc: 20.32 ng/ml

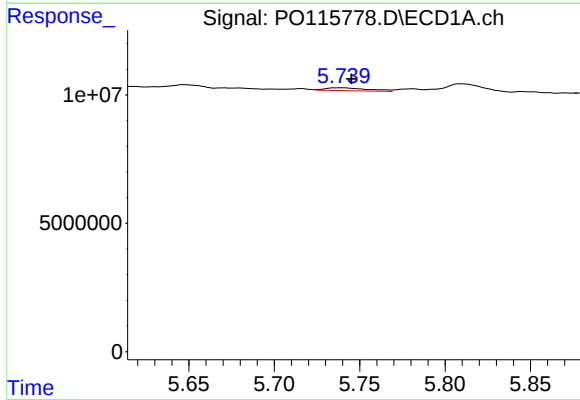


#22 AR-1248-2

R.T.: 5.739 min
Delta R.T.: -0.006 min
Response: 1950501
Conc: 9.71 ng/ml

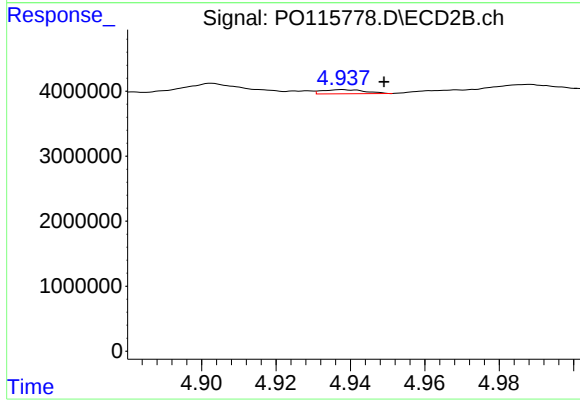

#22 AR-1248-2


R.T.: 4.938 min
Delta R.T.: -0.011 min
Response: 503158
Conc: 3.30 ng/ml

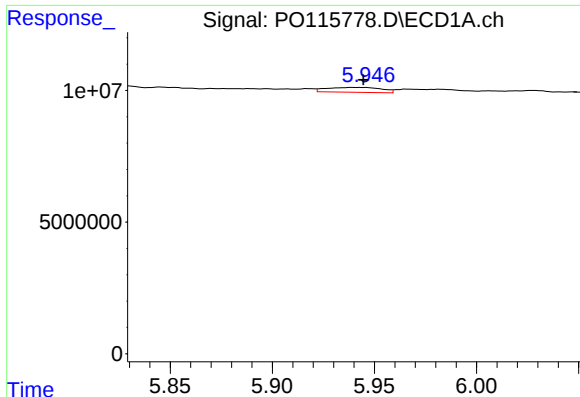

#23 AR-1248-3


R.T.: 5.940 min
Delta R.T.: -0.005 min
Response: 3474845
Conc: 14.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

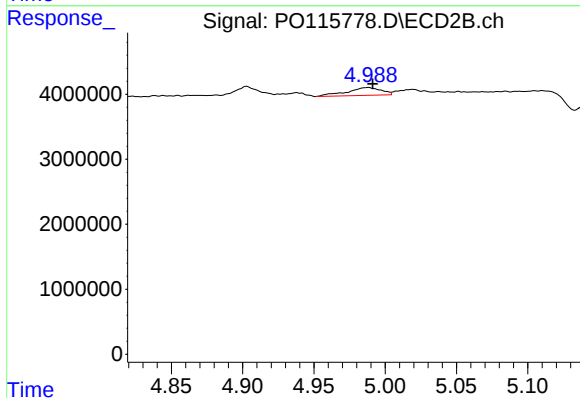


#23 AR-1248-3

R.T.: 4.988 min
Delta R.T.: -0.003 min
Response: 2035894
Conc: 12.68 ng/ml

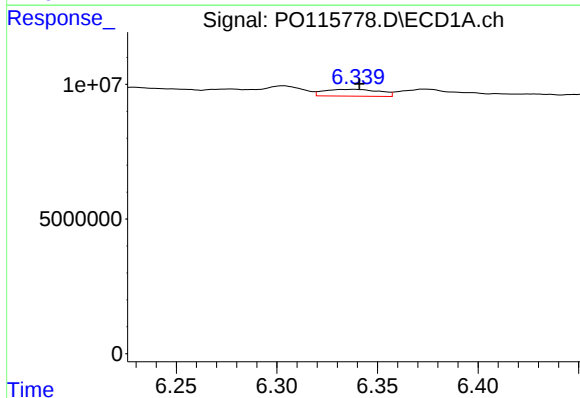


#24 AR-1248-4

R.T.: 6.338 min
Delta R.T.: -0.003 min
Response: 4789306
Conc: 16.24 ng/ml

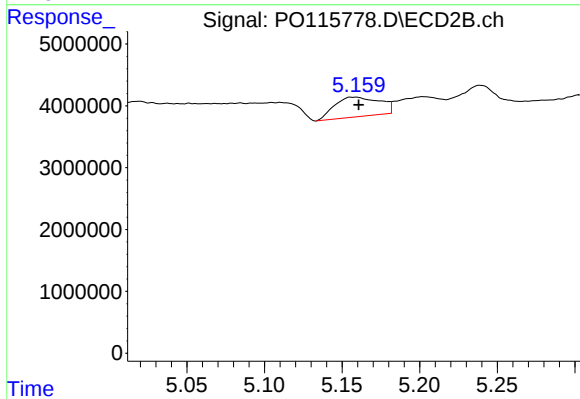

#24 AR-1248-4


R.T.: 5.159 min
Delta R.T.: -0.002 min
Response: 6420482
Conc: 34.31 ng/ml

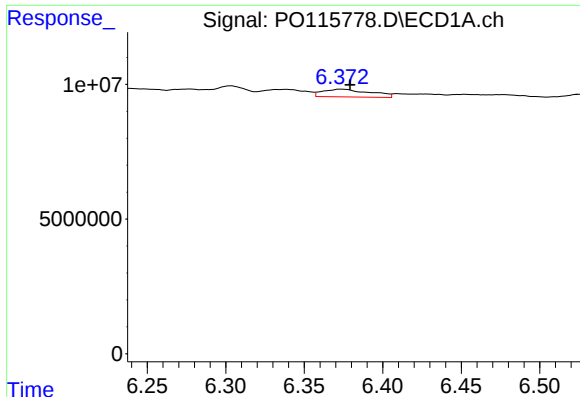

#25 AR-1248-5


R.T.: 6.373 min
Delta R.T.: -0.006 min
Response: 5955147
Conc: 23.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

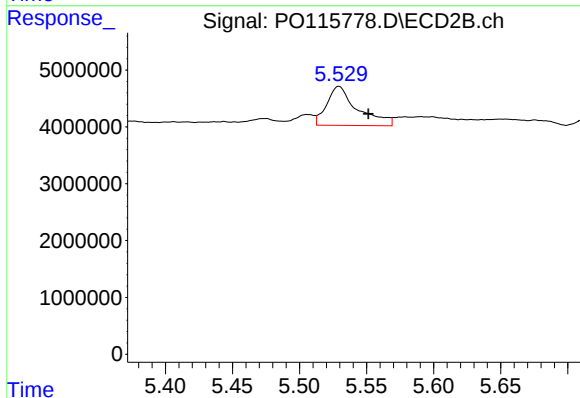


#25 AR-1248-5

R.T.: 5.529 min
Delta R.T.: -0.022 min
Response: 10929516
Conc: 55.21 ng/ml

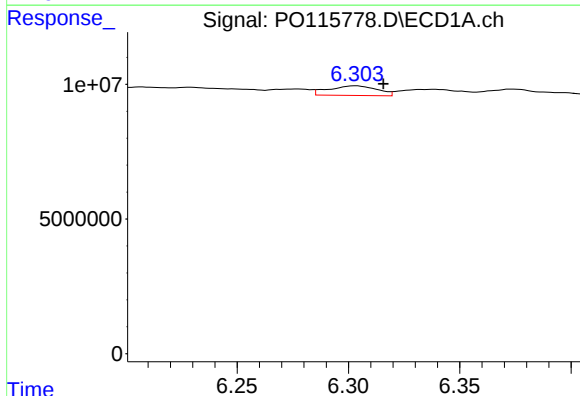


#26 AR-1254-1

R.T.: 6.303 min
Delta R.T.: -0.012 min
Response: 5402673
Conc: 20.88 ng/ml

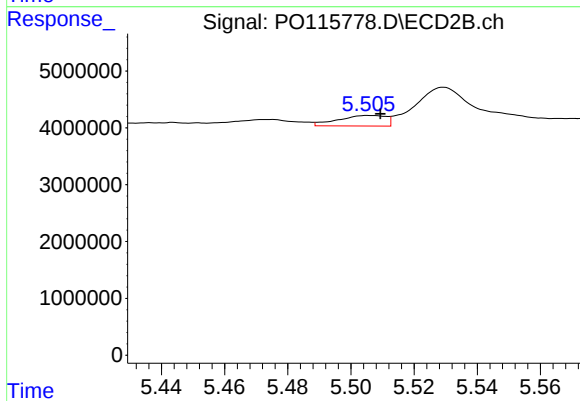

#26 AR-1254-1


R.T.: 5.506 min
Delta R.T.: -0.003 min
Response: 1957452
Conc: 6.70 ng/ml

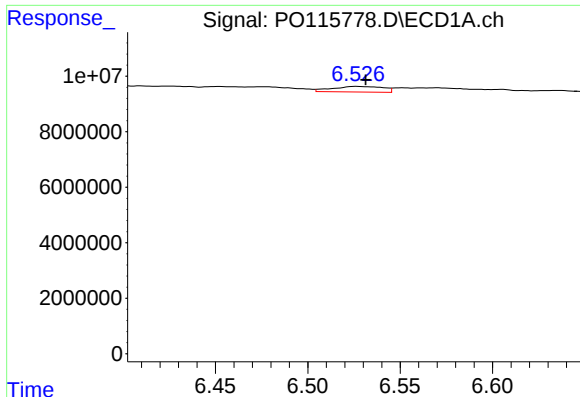

#27 AR-1254-2


R.T.: 6.526 min
Delta R.T.: -0.005 min
Response: 3855929
Conc: 9.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

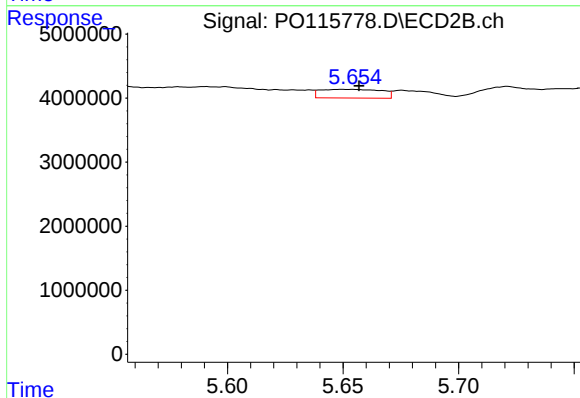


#27 AR-1254-2

R.T.: 5.654 min
Delta R.T.: -0.003 min
Response: 2496722
Conc: 9.91 ng/ml

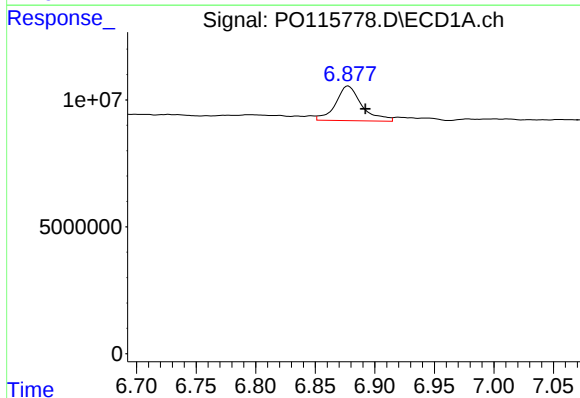


#28 AR-1254-3

R.T.: 6.878 min
Delta R.T.: -0.014 min
Response: 20906107
Conc: 50.92 ng/ml

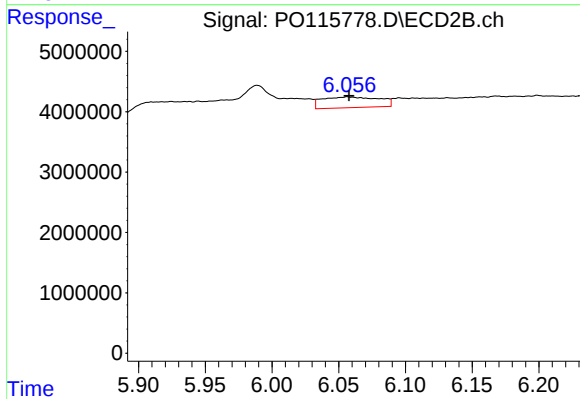

#28 AR-1254-3


R.T.: 6.056 min
Delta R.T.: -0.001 min
Response: 5262076
Conc: 13.37 ng/ml

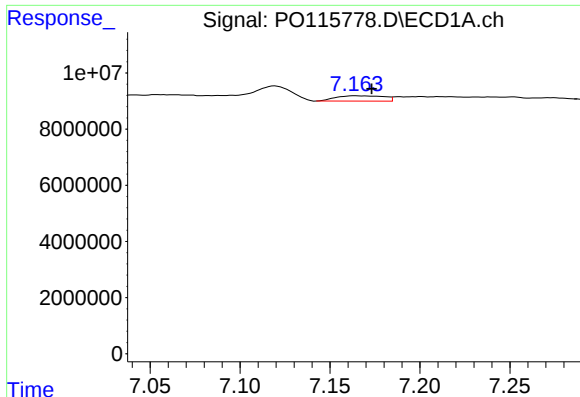

#29 AR-1254-4


R.T.: 7.164 min
Delta R.T.: -0.009 min
Response: 3550515
Conc: 10.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

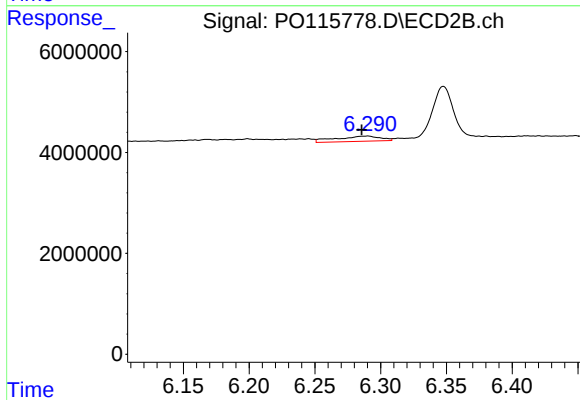


#29 AR-1254-4

R.T.: 6.290 min
Delta R.T.: 0.004 min
Response: 2453886
Conc: 9.17 ng/ml

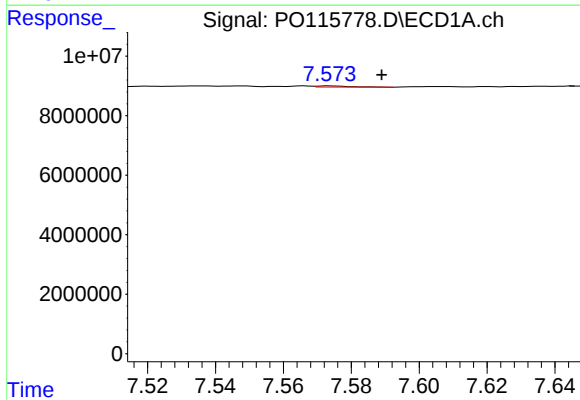


#30 AR-1254-5

R.T.: 7.574 min
Delta R.T.: -0.015 min
Response: 244788
Conc: 0.76 ng/ml

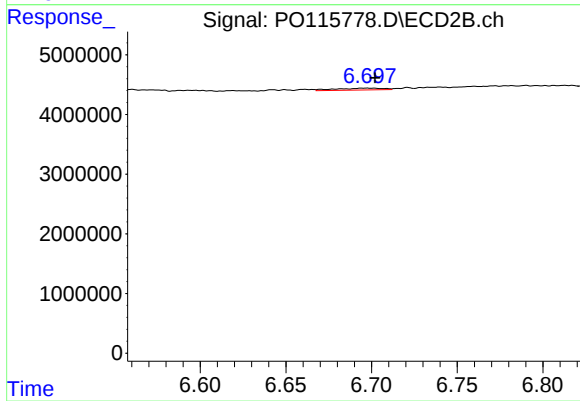

#30 AR-1254-5


R.T.: 6.697 min
Delta R.T.: -0.006 min
Response: 586854
Conc: 1.64 ng/ml

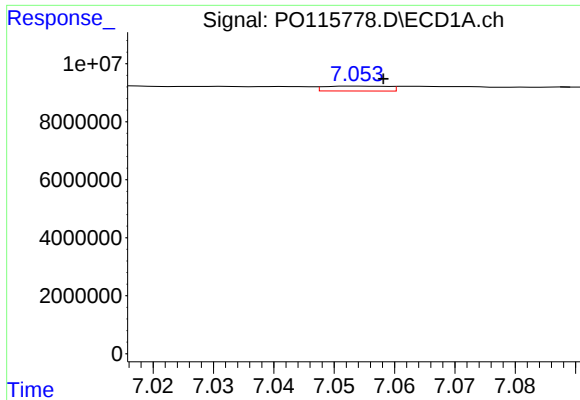

#31 AR-1260-1


R.T.: 7.054 min
Delta R.T.: -0.004 min
Response: 1239197
Conc: 4.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

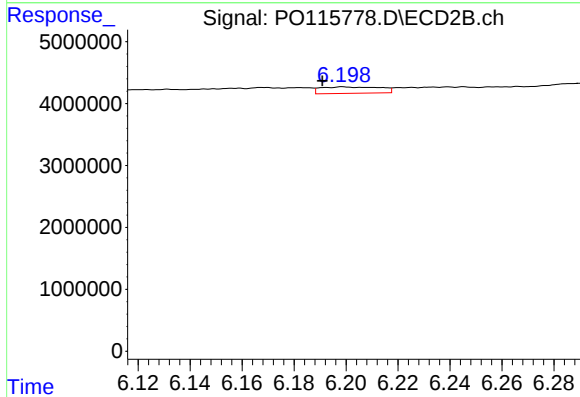


#31 AR-1260-1

R.T.: 6.199 min
Delta R.T.: 0.008 min
Response: 1655611
Conc: 6.32 ng/ml

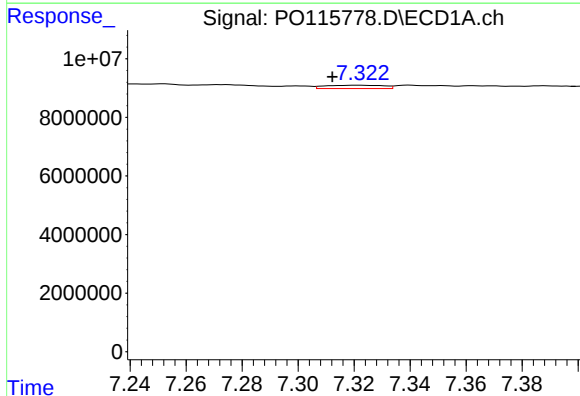


#32 AR-1260-2

R.T.: 7.323 min
Delta R.T.: 0.011 min
Response: 1655819
Conc: 3.78 ng/ml

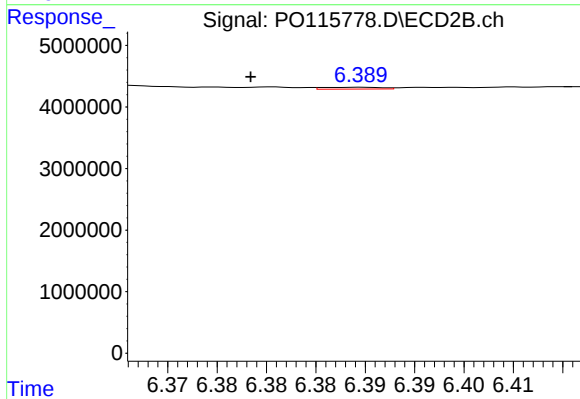

#32 AR-1260-2


R.T.: 6.389 min
Delta R.T.: 0.011 min
Response: 116766
Conc: 0.33 ng/ml

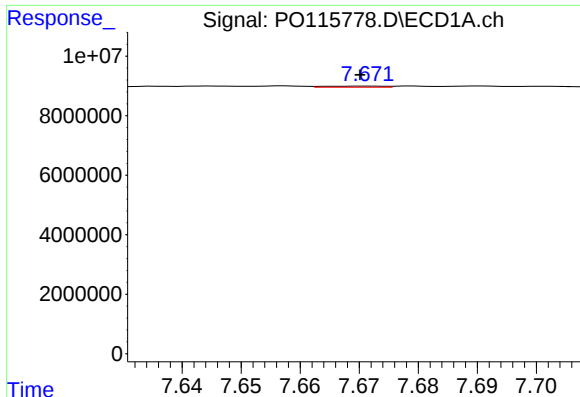

#33 AR-1260-3


R.T.: 7.672 min
Delta R.T.: 0.002 min
Response: 274791
Conc: 0.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

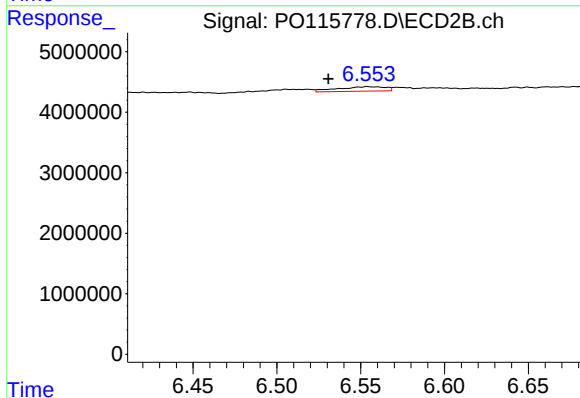


#33 AR-1260-3

R.T.: 6.554 min
Delta R.T.: 0.023 min
Response: 1470323
Conc: 4.58 ng/ml

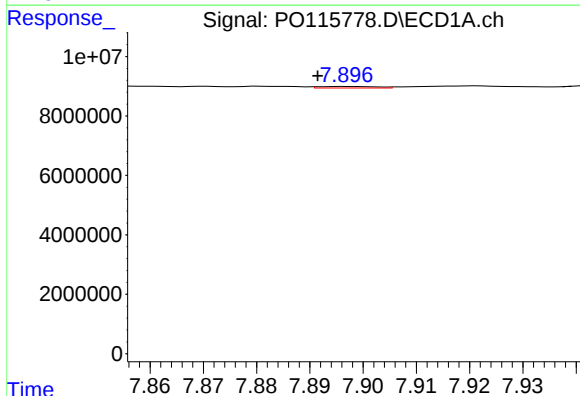


#34 AR-1260-4

R.T.: 7.897 min
Delta R.T.: 0.006 min
Response: 368589
Conc: 1.20 ng/ml

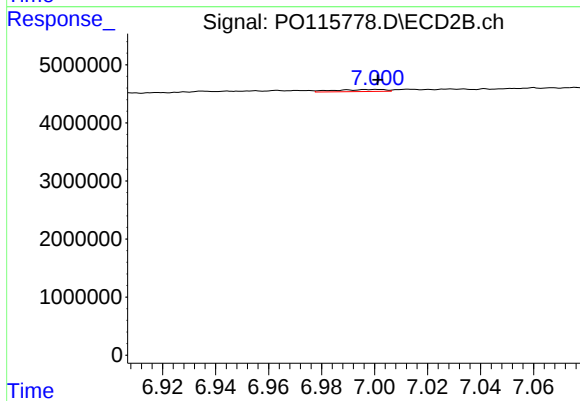

#34 AR-1260-4


R.T.: 7.001 min
Delta R.T.: 0.000 min
Response: 461685
Conc: 1.80 ng/ml

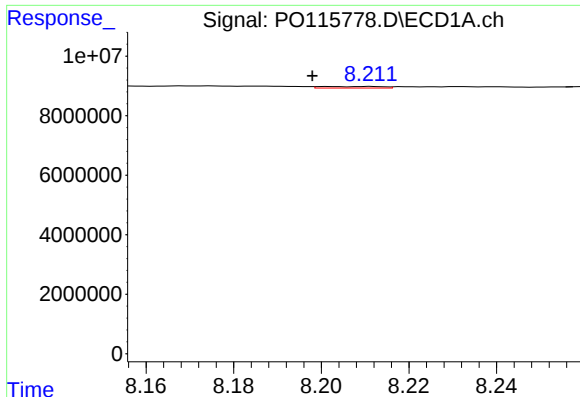

#35 AR-1260-5


R.T.: 8.211 min
Delta R.T.: 0.013 min
Response: 525994
Conc: 0.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

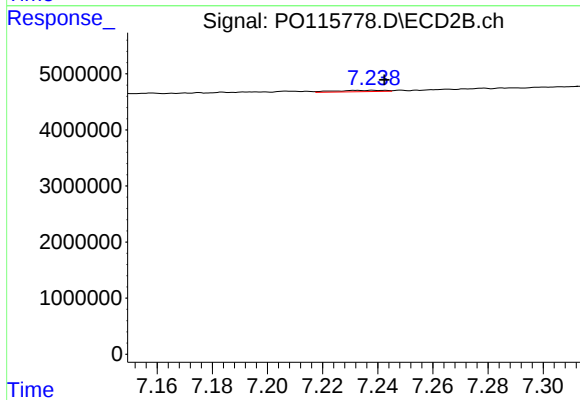


#35 AR-1260-5

R.T.: 7.238 min
Delta R.T.: -0.004 min
Response: 324682
Conc: 0.46 ng/ml

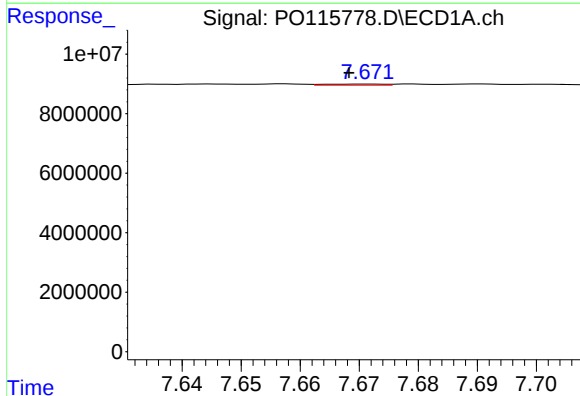


#36 AR-1262-1

R.T.: 7.672 min
Delta R.T.: 0.003 min
Response: 274791
Conc: 1.11 ng/ml

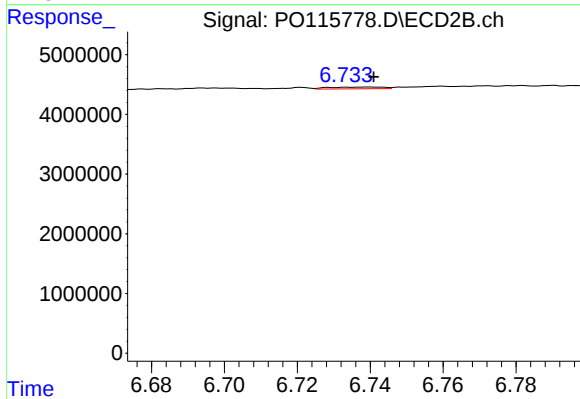

#36 AR-1262-1


R.T.: 6.740 min
Delta R.T.: -0.001 min
Response: 306913
Conc: 1.44 ng/ml

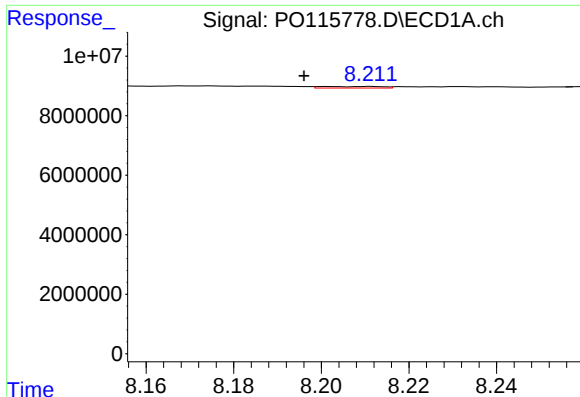

#37 AR-1262-2


R.T.: 8.211 min
Delta R.T.: 0.015 min
Response: 525994
Conc: 1.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

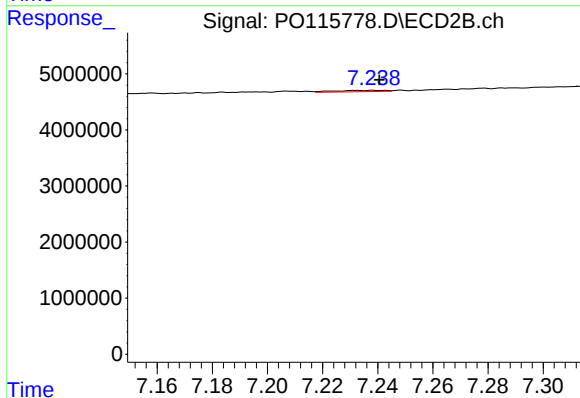


#37 AR-1262-2

R.T.: 7.238 min
Delta R.T.: -0.002 min
Response: 324682
Conc: 0.93 ng/ml

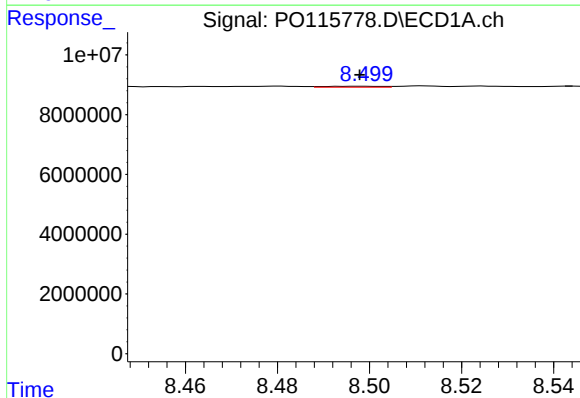


#38 AR-1262-3

R.T.: 8.499 min
Delta R.T.: 0.001 min
Response: 279904
Conc: 1.10 ng/ml

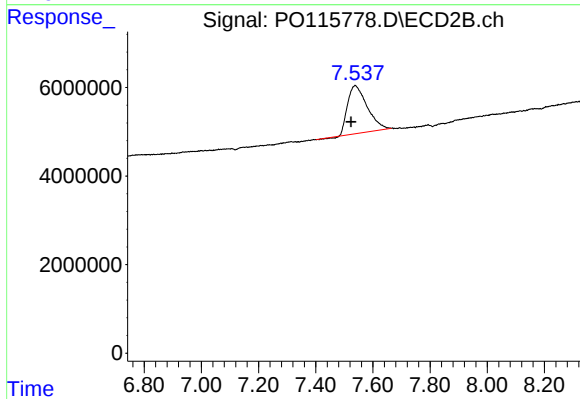

#38 AR-1262-3


R.T.: 7.538 min
Delta R.T.: 0.014 min
Response: 51746381
Conc: 330.88 ng/ml

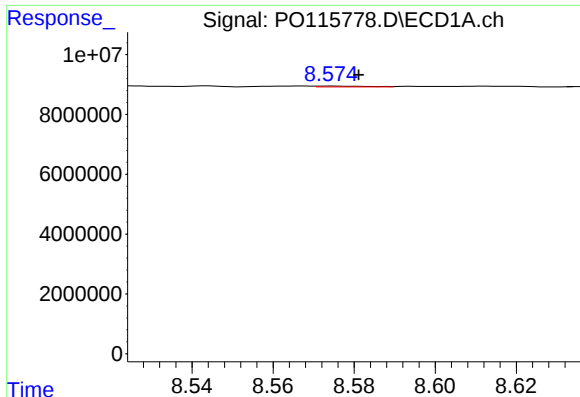

#39 AR-1262-4


R.T.: 8.574 min
Delta R.T.: -0.007 min
Response: 262264
Conc: 1.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

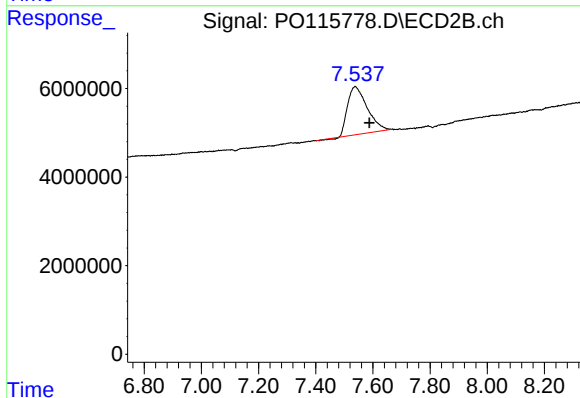


#39 AR-1262-4

R.T.: 7.538 min
Delta R.T.: -0.049 min
Response: 51746381
Conc: 209.18 ng/ml

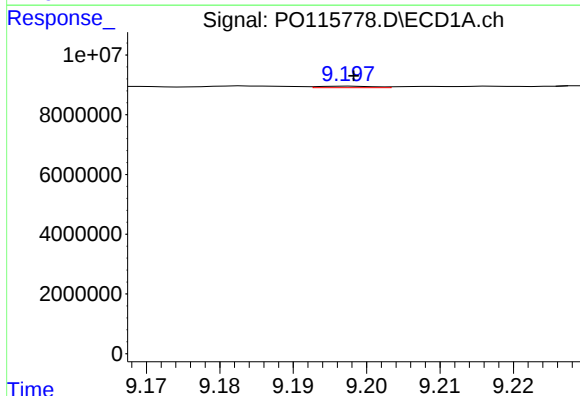


#40 AR-1262-5

R.T.: 9.198 min
Delta R.T.: 0.000 min
Response: 264125
Conc: 1.96 ng/ml

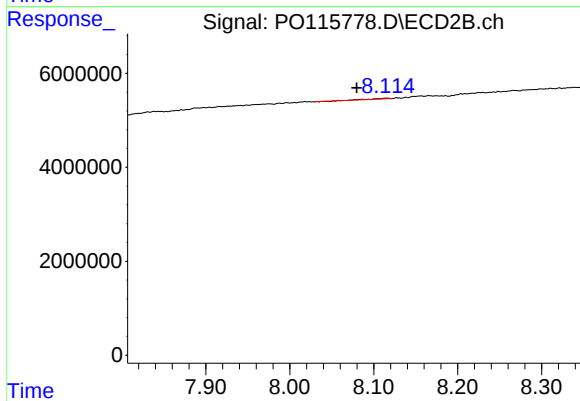

#40 AR-1262-5


R.T.: 8.115 min
Delta R.T.: 0.035 min
Response: 201866
Conc: 1.81 ng/ml

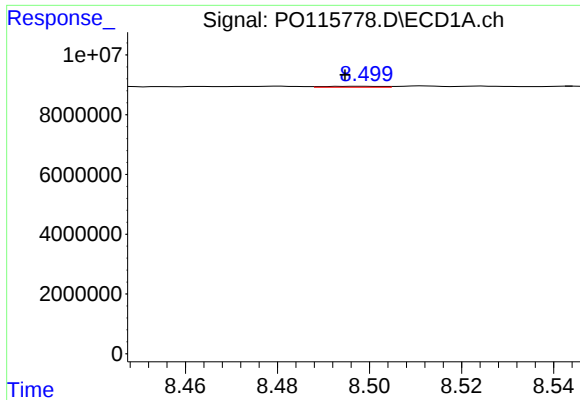

#41 AR-1268-1


R.T.: 8.499 min
Delta R.T.: 0.004 min
Response: 279904
Conc: 0.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

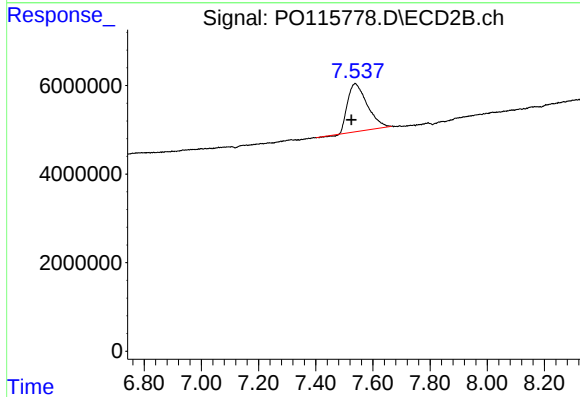


#41 AR-1268-1

R.T.: 7.538 min
Delta R.T.: 0.014 min
Response: 51746381
Conc: 58.41 ng/ml

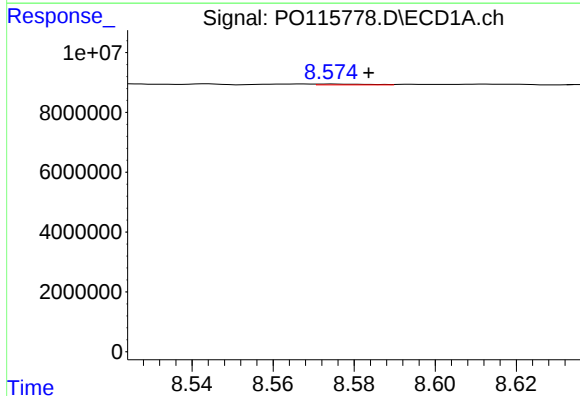


#42 AR-1268-2

R.T.: 8.574 min
Delta R.T.: -0.009 min
Response: 262264
Conc: 0.31 ng/ml

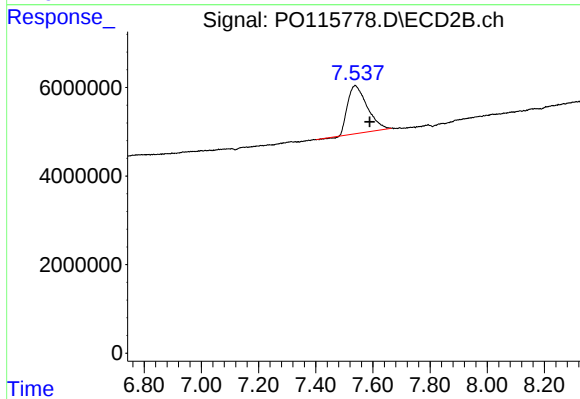

#42 AR-1268-2


R.T.: 7.538 min
Delta R.T.: -0.051 min
Response: 51746381
Conc: 69.08 ng/ml

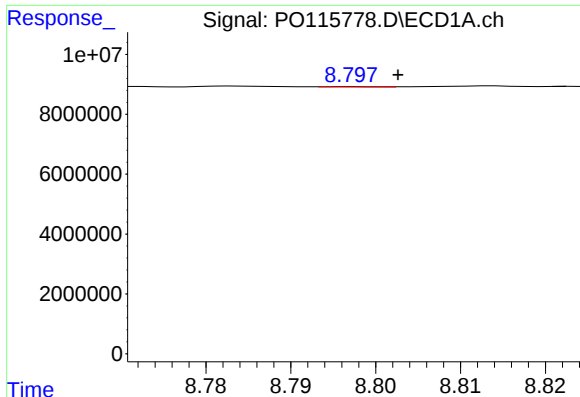

#43 AR-1268-3


R.T.: 8.797 min
Delta R.T.: -0.005 min
Response: 46135
Conc: 0.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

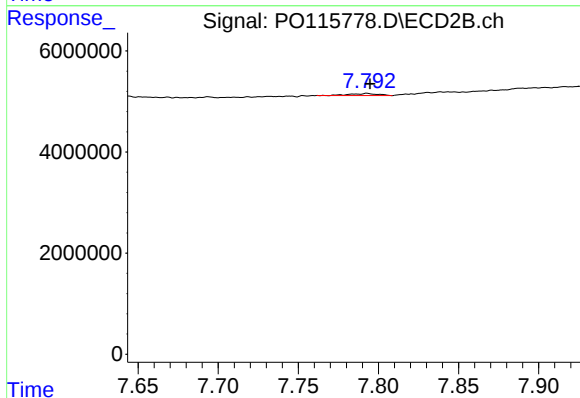


#43 AR-1268-3

R.T.: 7.793 min
Delta R.T.: -0.002 min
Response: 504446
Conc: 0.79 ng/ml

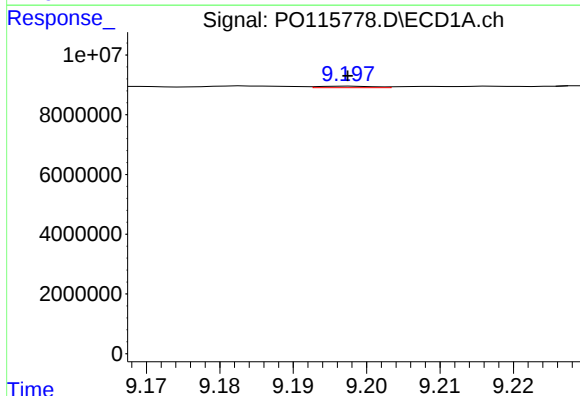


#44 AR-1268-4

R.T.: 9.198 min
Delta R.T.: 0.000 min
Response: 264125
Conc: 0.85 ng/ml

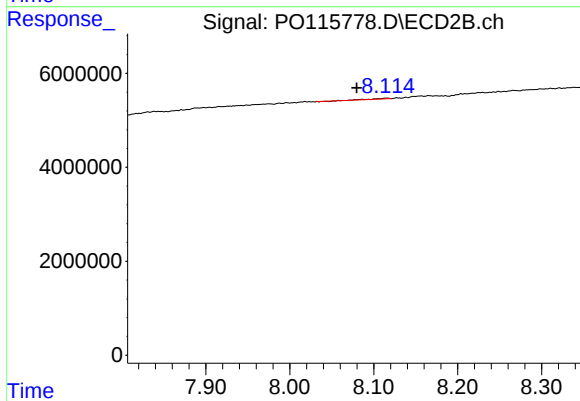

#44 AR-1268-4


R.T.: 8.115 min
Delta R.T.: 0.035 min
Response: 201866
Conc: 0.78 ng/ml

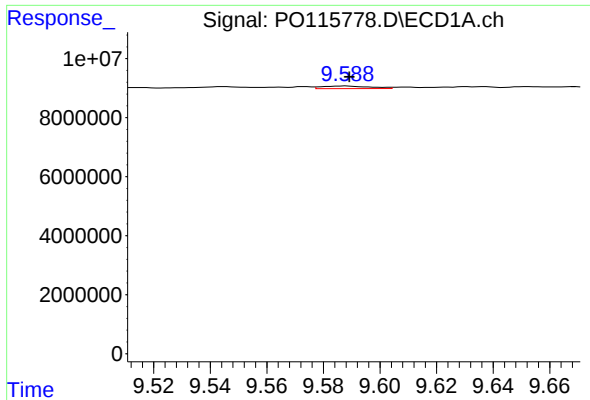

#45 AR-1268-5

R.T.: 9.588 min
Delta R.T.: -0.001 min
Response: 1035732
Conc: 0.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

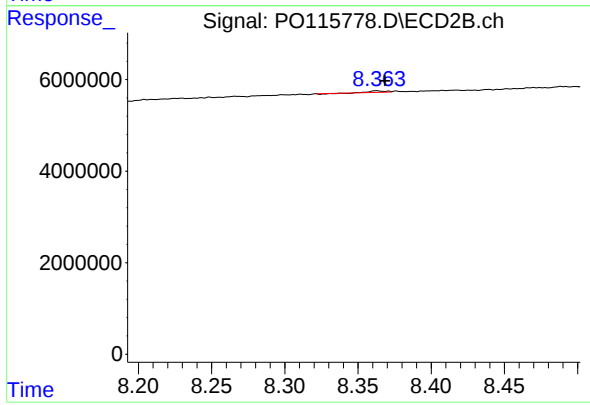

#45 AR-1268-5

R.T.: 8.363 min
Delta R.T.: -0.006 min
Response: 166173
Conc: 0.10 ng/ml