

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0121225\
 Data File : P0115779.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Dec 2025 02:33
 Operator : YP/AJ
 Sample : Q3530-07
 Misc : AR1242 25PPB WATER LOD
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 13 03:50:44 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0120425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 05 02:11:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.334	3.636	228.7E6	139.9E6	29.447	28.708
2)	SA Decachlor...	9.907	8.615	164.2E6	122.1E6	31.210	28.392
Target Compounds							
3)	L1 AR-1016-1	5.472	4.711	7620984	5965590	30.648	32.288
4)	L1 AR-1016-2	5.493	4.729	11190176	7942384	29.383	30.050
5)	L1 AR-1016-3	5.554	4.904	6260419	4619352	29.284	30.523
6)	L1 AR-1016-4	5.650	4.944	4244920	2101298	23.772	18.644
7)	L1 AR-1016-5	5.942	5.157	8607001	10226263	49.063	69.880 #
8)	L2 AR-1221-1	4.530	3.846	4451668	534275	54.826	9.472 #
9)	L2 AR-1221-2	4.628	3.933	4248026	3253137	67.409	76.646
10)	L2 AR-1221-3	4.692	4.005	5777833	2945363	30.944	22.905 #
11)	L3 AR-1232-1	4.692	4.005	5777833	2945363	38.605	27.569 #
12)	L3 AR-1232-2	5.210	4.729	6100439	7942384	75.453	71.560
13)	L3 AR-1232-3	5.493	4.904	11190176	4619352	72.709	70.669
14)	L3 AR-1232-4	5.650	4.988	4244920	4157799	60.615	81.001 #
15)	L3 AR-1232-5	5.742	5.157	4551611	10226263	87.637	186.787 #
16)	L4 AR-1242-1	5.472	4.711	7620984	5965590	38.369	41.897
17)	L4 AR-1242-2	5.493	4.729	11190176	7942384	38.206	37.936
18)	L4 AR-1242-3	5.554	4.904	6260419	4619352	37.084	38.674
19)	L4 AR-1242-4	5.650	4.988	4244920	4157799	31.060	38.113
20)	L4 AR-1242-5	6.376	5.507	11349314	6591448	74.941	47.721 #
21)	L5 AR-1248-1	5.472	4.711	7620984	5965590	50.215	53.346
22)	L5 AR-1248-2	5.742	4.944	4551611	2101298	22.666	13.798 #
23)	L5 AR-1248-3	5.942	4.988	8607001	4157799	34.903	25.901 #
24)	L5 AR-1248-4	6.339	5.157	9595552	10226263	32.543	54.643 #
25)	L5 AR-1248-5	6.376	5.546	11349314	6818374	43.832	34.444
26)	L6 AR-1254-1	6.307	5.507	5805293	6591448	22.439	22.552
27)	L6 AR-1254-2	6.532	5.654	8573165	7300559	21.305	28.992 #
28)	L6 AR-1254-3	6.880	6.055	26248811	5864009	63.933	14.899 #
29)	L6 AR-1254-4	7.169	6.286	5838515	4494082	16.823	16.795
30)	L6 AR-1254-5	7.599	6.699	575290	1197435	1.775	3.349 #
31)	L7 AR-1260-1	7.052	6.199	2302450	2693448	7.948	10.274 #
32)	L7 AR-1260-2	7.325	6.348	12552012	14004553	28.675	39.961 #
33)	L7 AR-1260-3	7.671	6.507	1554458	11506386	4.618	35.815 #
34)	L7 AR-1260-4	7.880	6.988	1482400	1033671	4.821	4.025
35)	L7 AR-1260-5	8.200	7.238	618803	1735411	0.849	2.475 #
36)	L8 AR-1262-1	7.671	6.733	1554458	2266948	6.297	10.641 #
37)	L8 AR-1262-2	8.200	7.238	618803	1735411	1.563	4.982 #
38)	L8 AR-1262-3	8.493	7.536	292048	60806908	1.146	388.815 #
39)	L8 AR-1262-4	8.581	7.536f	434294	60806908	2.242	245.812 #
40)	L8 AR-1262-5	9.194	8.077	767472	59715	5.698	0.536 #
41)	L9 AR-1268-1	8.493	7.536	292048	60806908	0.293	68.635 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121225\
 Data File : PO115779.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Dec 2025 02:33
 Operator : YP/AJ
 Sample : Q3530-07
 Misc : AR1242 25PPB WATER LOD
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 13 03:50:44 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 05 02:11:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.581	7.536f	434294	60806908	0.508	81.176 #
43) L9	AR-1268-3	8.800	7.790	359990	711490	0.485	1.117 #
44) L9	AR-1268-4	9.194	8.077	767472	59715	2.458	0.232 #
45) L9	AR-1268-5	9.587	8.368	1230938	941299	0.565	0.558


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121225\
Data File : PO115779.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Dec 2025 02:33
Operator : YP/AJ
Sample : Q3530-07
Misc : AR1242 25PPB WATER LOD
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 13 03:50:44 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120425.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 05 02:11:05 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

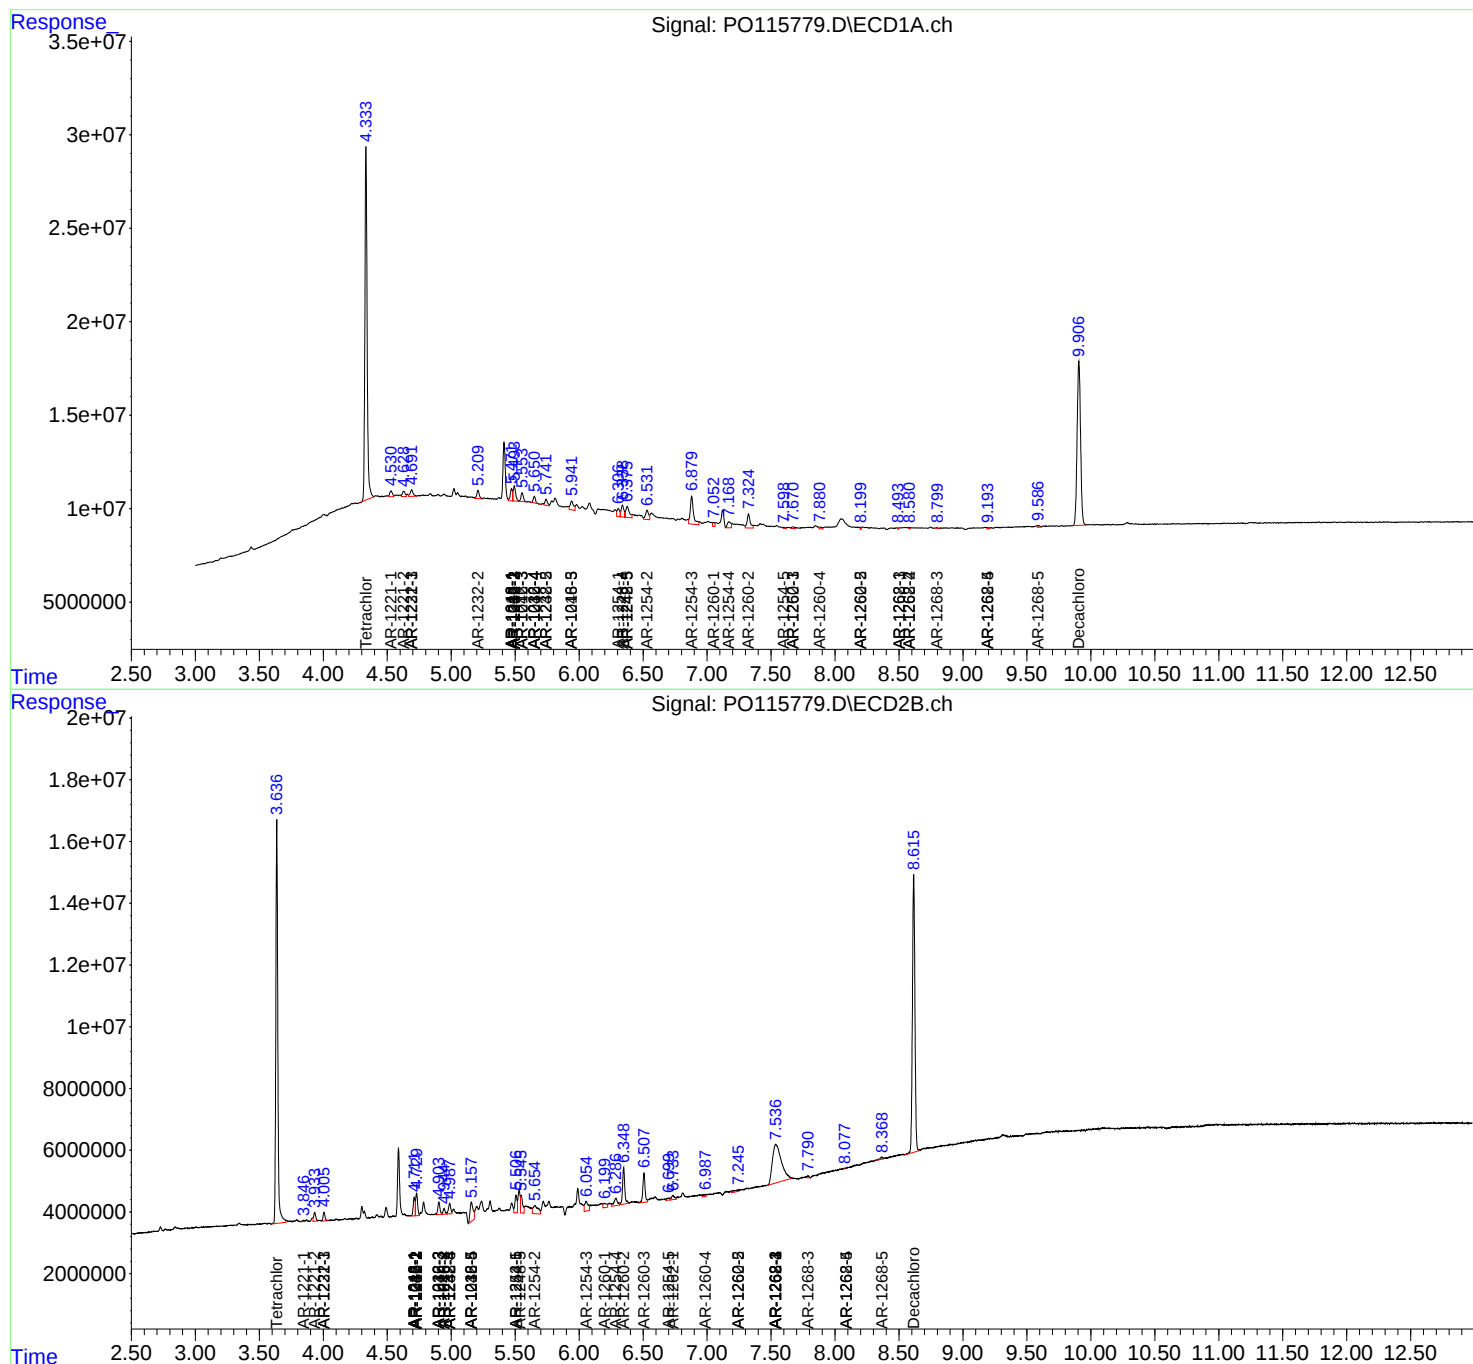


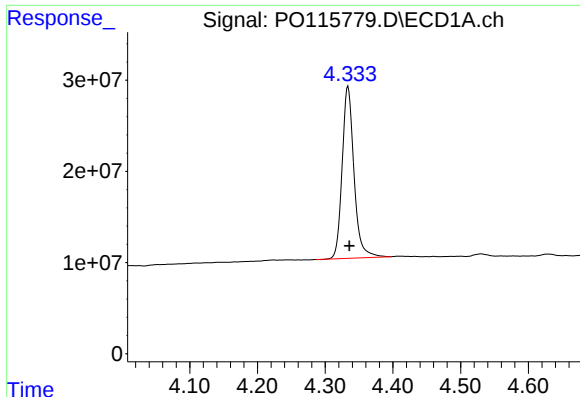

#1 Tetrachloro-m-xylene


R.T.: 4.334 min
Delta R.T.: -0.002 min
Response: 228718549
Conc: 29.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

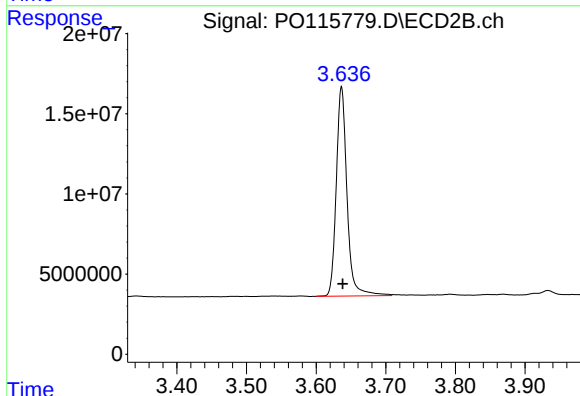


#1 Tetrachloro-m-xylene

R.T.: 3.636 min
Delta R.T.: -0.002 min
Response: 139902245
Conc: 28.71 ng/ml

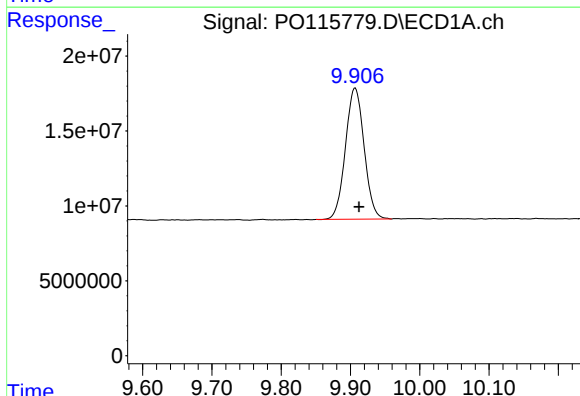


#2 Decachlorobiphenyl

R.T.: 9.907 min
Delta R.T.: -0.006 min
Response: 164195037
Conc: 31.21 ng/ml

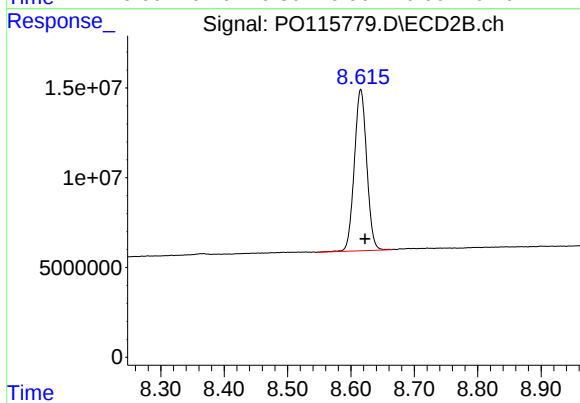

#2 Decachlorobiphenyl


R.T.: 8.615 min
Delta R.T.: -0.007 min
Response: 122090387
Conc: 28.39 ng/ml

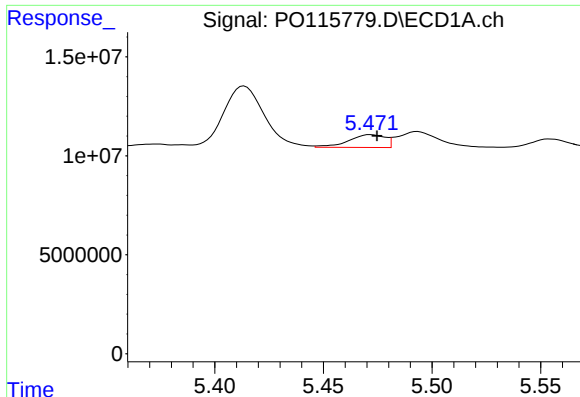

#3 AR-1016-1


R.T.: 5.472 min
Delta R.T.: -0.003 min
Response: 7620984
Conc: 30.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

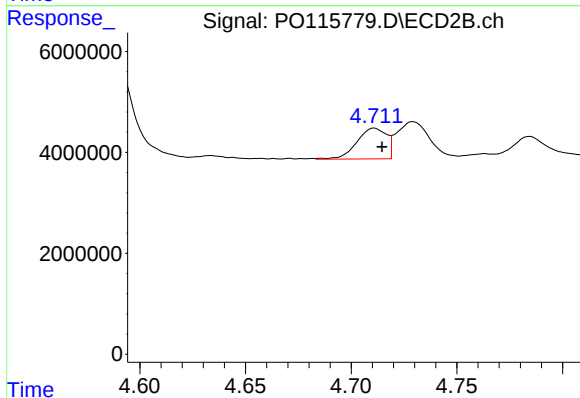


#3 AR-1016-1

R.T.: 4.711 min
Delta R.T.: -0.004 min
Response: 5965590
Conc: 32.29 ng/ml

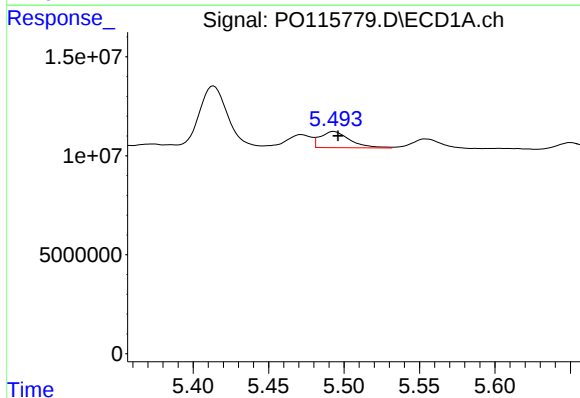


#4 AR-1016-2

R.T.: 5.493 min
Delta R.T.: -0.003 min
Response: 11190176
Conc: 29.38 ng/ml

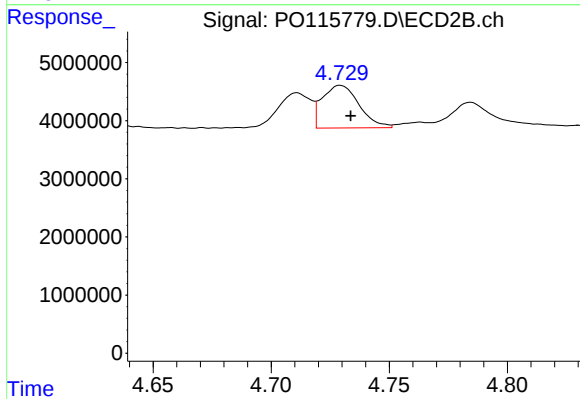

#4 AR-1016-2


R.T.: 4.729 min
Delta R.T.: -0.004 min
Response: 7942384
Conc: 30.05 ng/ml

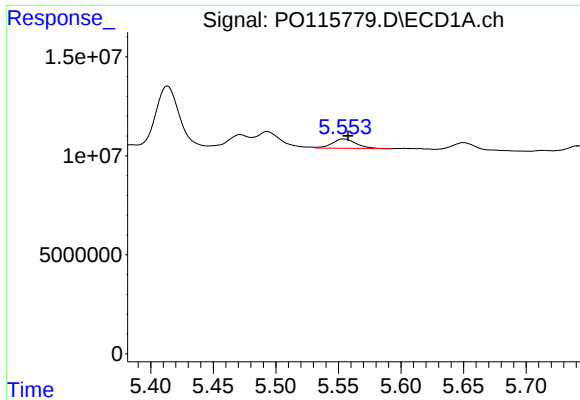

#5 AR-1016-3


R.T.: 5.554 min
Delta R.T.: -0.003 min
Response: 6260419
Conc: 29.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

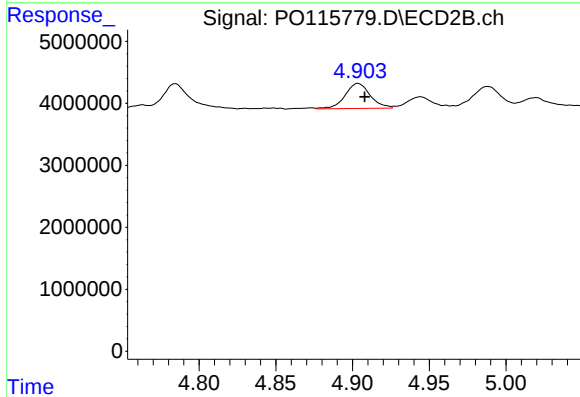


#5 AR-1016-3

R.T.: 4.904 min
Delta R.T.: -0.004 min
Response: 4619352
Conc: 30.52 ng/ml

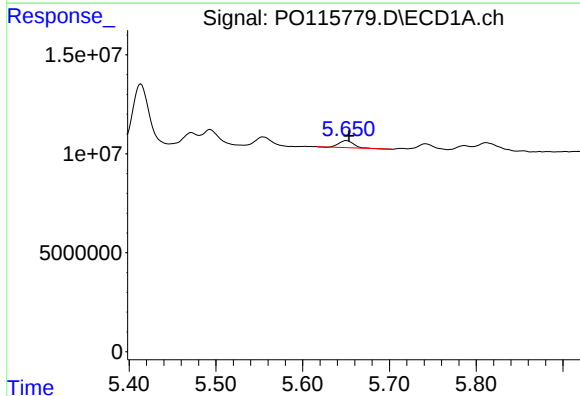


#6 AR-1016-4

R.T.: 5.650 min
Delta R.T.: -0.003 min
Response: 4244920
Conc: 23.77 ng/ml

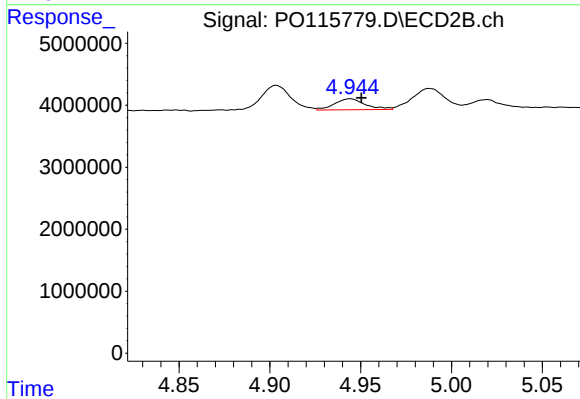

#6 AR-1016-4


R.T.: 4.944 min
Delta R.T.: -0.006 min
Response: 2101298
Conc: 18.64 ng/ml

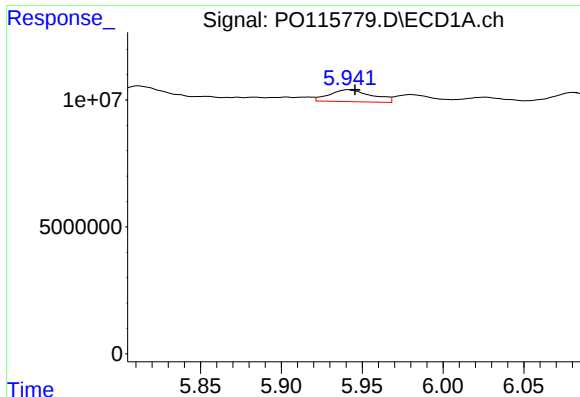

#7 AR-1016-5


R.T.: 5.942 min
Delta R.T.: -0.004 min
Response: 8607001
Conc: 49.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

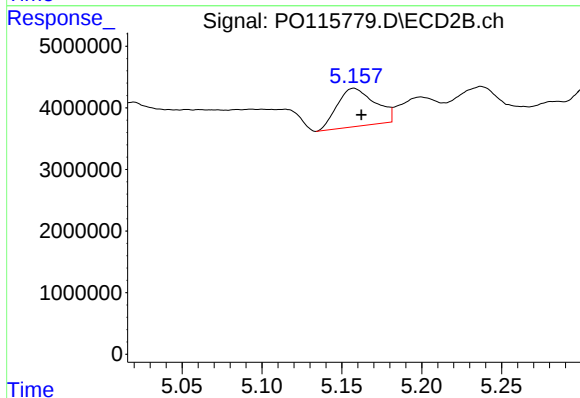


#7 AR-1016-5

R.T.: 5.157 min
Delta R.T.: -0.005 min
Response: 10226263
Conc: 69.88 ng/ml

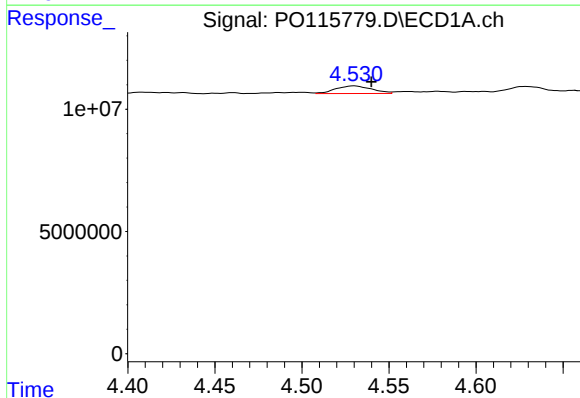


#8 AR-1221-1

R.T.: 4.530 min
Delta R.T.: -0.010 min
Response: 4451668
Conc: 54.83 ng/ml

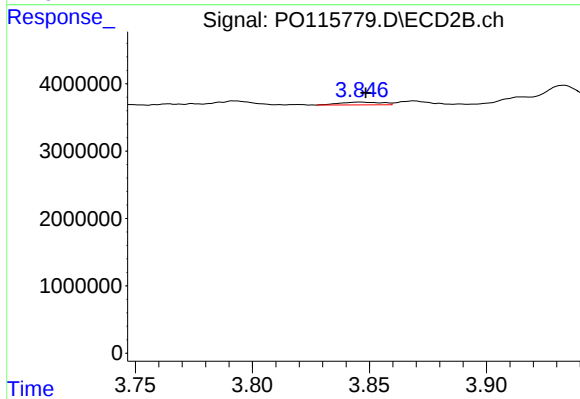

#8 AR-1221-1


R.T.: 3.846 min
Delta R.T.: -0.002 min
Response: 534275
Conc: 9.47 ng/ml

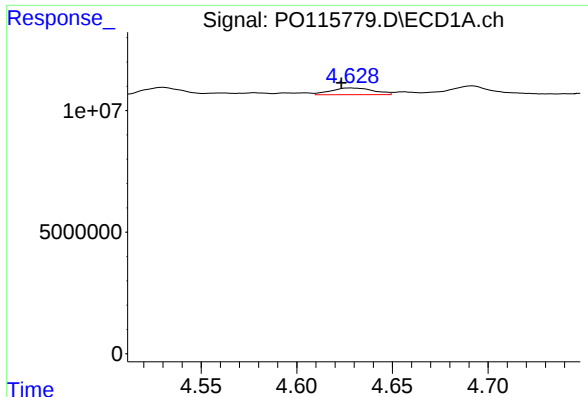

#9 AR-1221-2


R.T.: 4.628 min
Delta R.T.: 0.005 min
Response: 4248026
Conc: 67.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

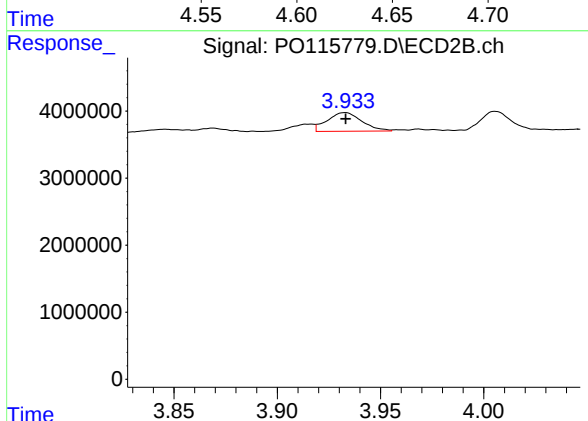


#9 AR-1221-2

R.T.: 3.933 min
Delta R.T.: 0.000 min
Response: 3253137
Conc: 76.65 ng/ml

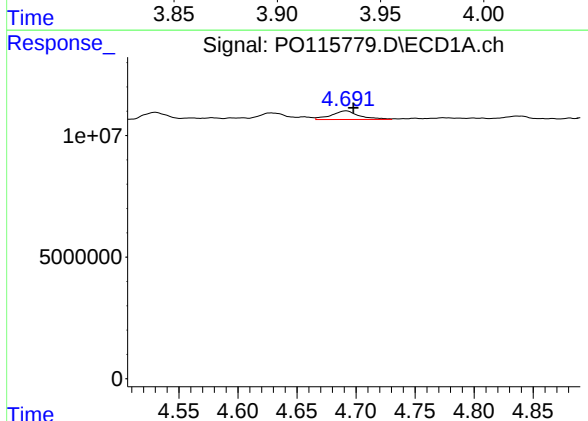


#10 AR-1221-3

R.T.: 4.692 min
Delta R.T.: -0.006 min
Response: 5777833
Conc: 30.94 ng/ml

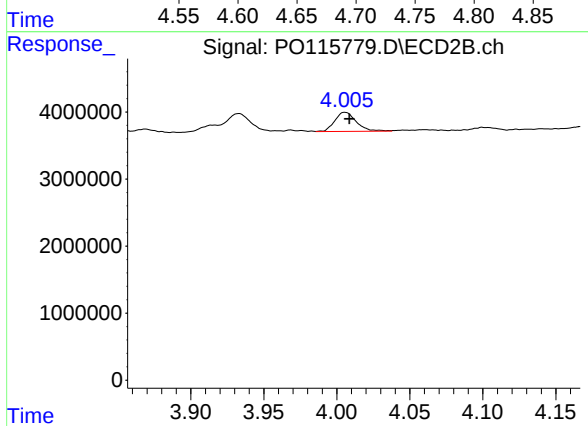

#10 AR-1221-3


R.T.: 4.005 min
Delta R.T.: -0.003 min
Response: 2945363
Conc: 22.90 ng/ml

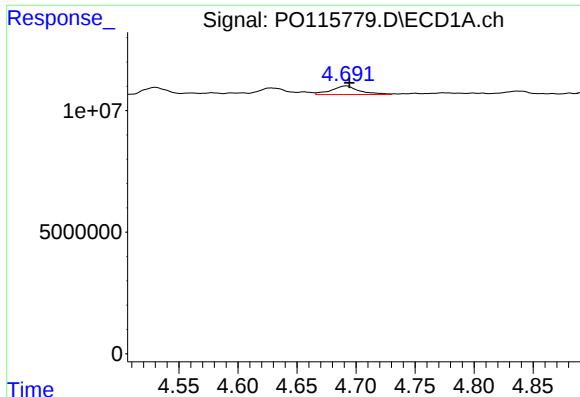

#11 AR-1232-1


R.T.: 4.692 min
Delta R.T.: -0.003 min
Response: 5777833
Conc: 38.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

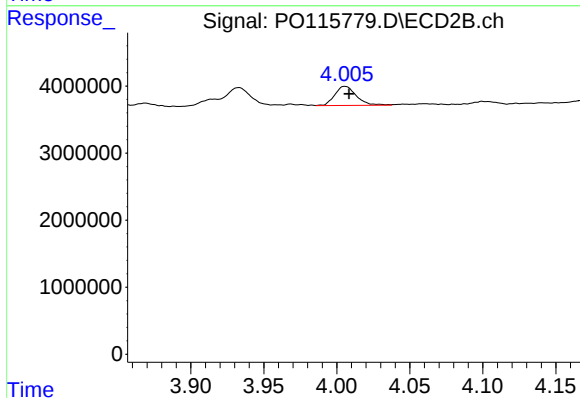


#11 AR-1232-1

R.T.: 4.005 min
Delta R.T.: -0.003 min
Response: 2945363
Conc: 27.57 ng/ml

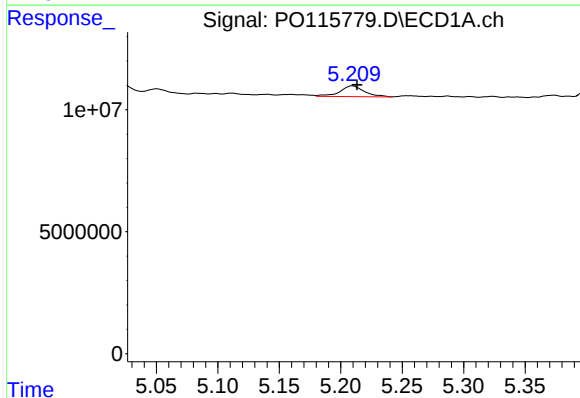


#12 AR-1232-2

R.T.: 5.210 min
Delta R.T.: -0.004 min
Response: 6100439
Conc: 75.45 ng/ml

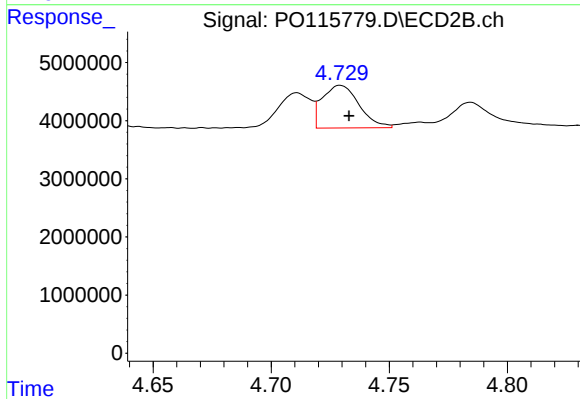

#12 AR-1232-2


R.T.: 4.729 min
Delta R.T.: -0.004 min
Response: 7942384
Conc: 71.56 ng/ml

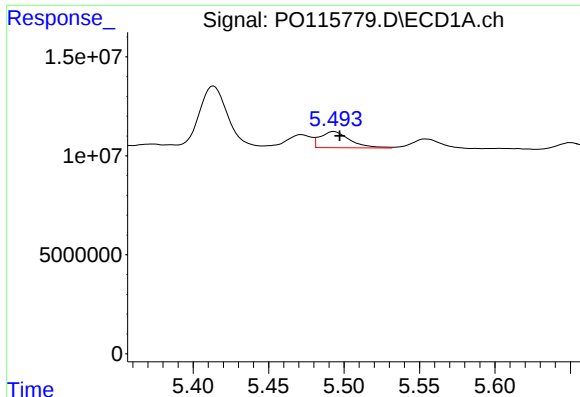

#13 AR-1232-3


R.T.: 5.493 min
Delta R.T.: -0.004 min
Response: 11190176
Conc: 72.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

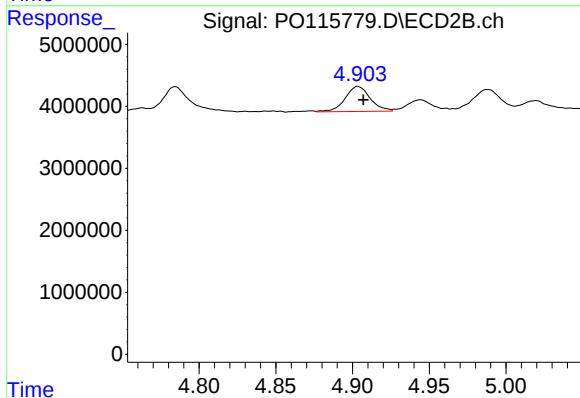


#13 AR-1232-3

R.T.: 4.904 min
Delta R.T.: -0.003 min
Response: 4619352
Conc: 70.67 ng/ml

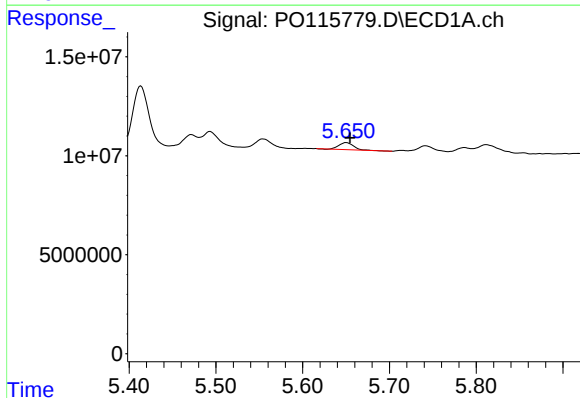


#14 AR-1232-4

R.T.: 5.650 min
Delta R.T.: -0.004 min
Response: 4244920
Conc: 60.62 ng/ml

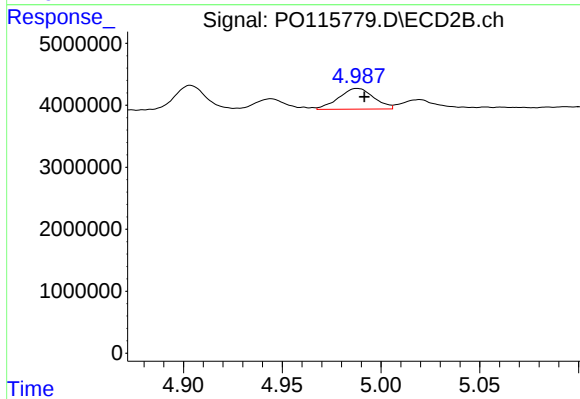

#14 AR-1232-4


R.T.: 4.988 min
Delta R.T.: -0.003 min
Response: 4157799
Conc: 81.00 ng/ml

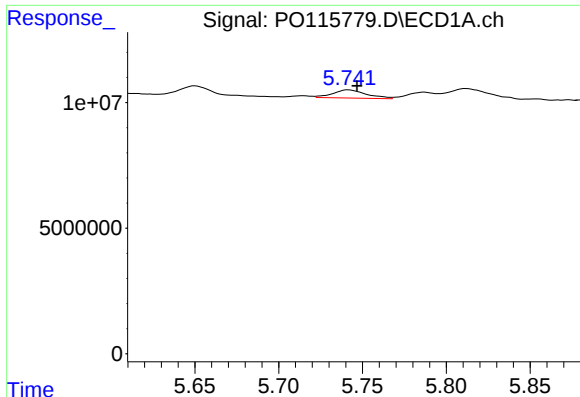

#15 AR-1232-5


R.T.: 5.742 min
Delta R.T.: -0.005 min
Response: 4551611
Conc: 87.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

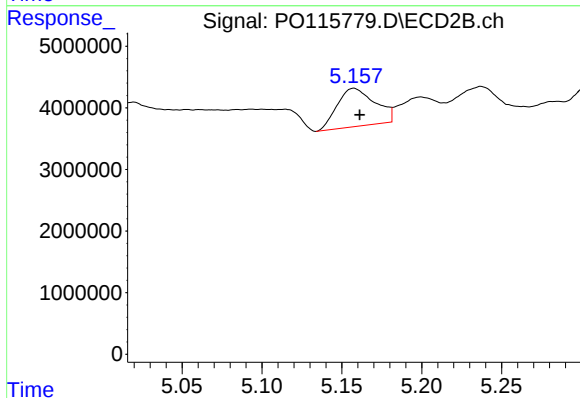


#15 AR-1232-5

R.T.: 5.157 min
Delta R.T.: -0.004 min
Response: 10226263
Conc: 186.79 ng/ml

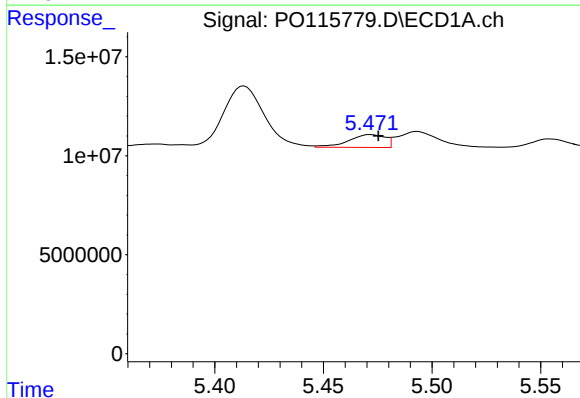


#16 AR-1242-1

R.T.: 5.472 min
Delta R.T.: -0.003 min
Response: 7620984
Conc: 38.37 ng/ml

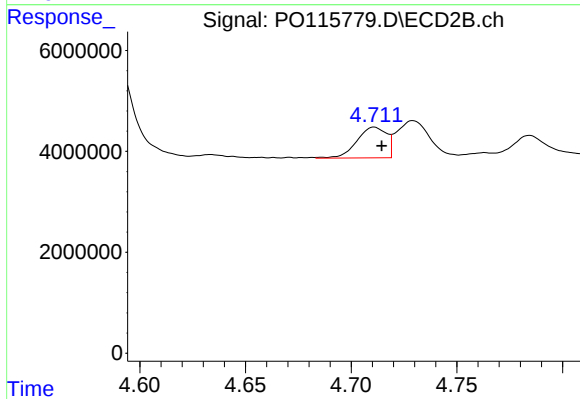

#16 AR-1242-1


R.T.: 4.711 min
Delta R.T.: -0.004 min
Response: 5965590
Conc: 41.90 ng/ml

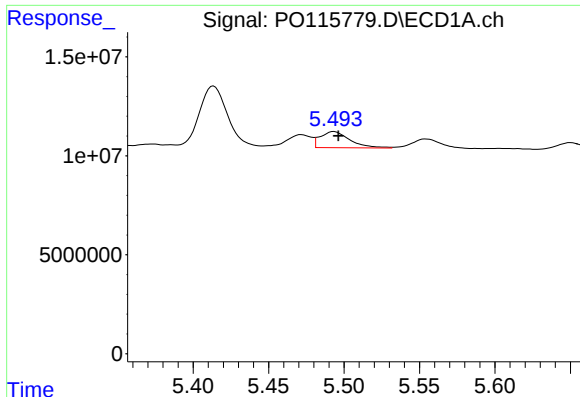

#17 AR-1242-2


R.T.: 5.493 min
Delta R.T.: -0.003 min
Response: 11190176
Conc: 38.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

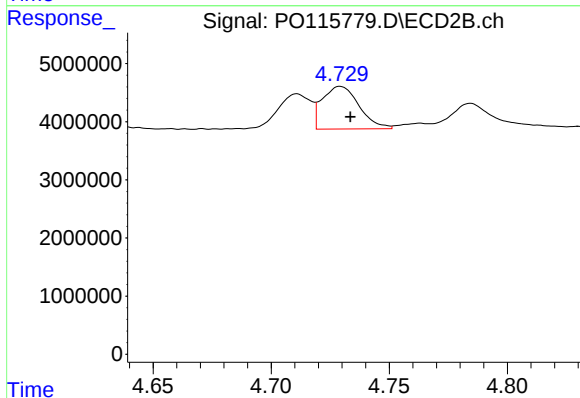


#17 AR-1242-2

R.T.: 4.729 min
Delta R.T.: -0.004 min
Response: 7942384
Conc: 37.94 ng/ml

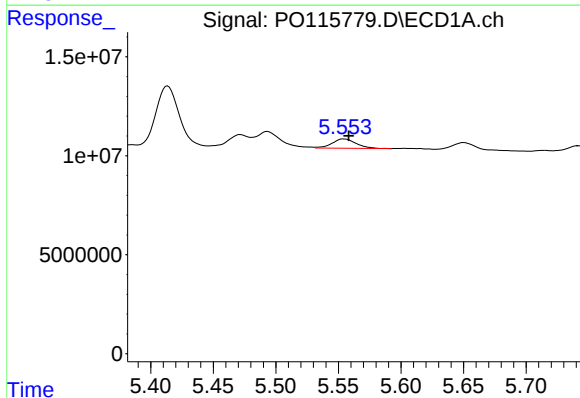


#18 AR-1242-3

R.T.: 5.554 min
Delta R.T.: -0.004 min
Response: 6260419
Conc: 37.08 ng/ml

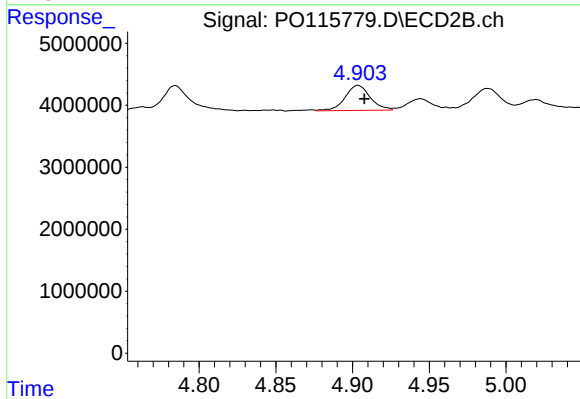

#18 AR-1242-3


R.T.: 4.904 min
Delta R.T.: -0.004 min
Response: 4619352
Conc: 38.67 ng/ml

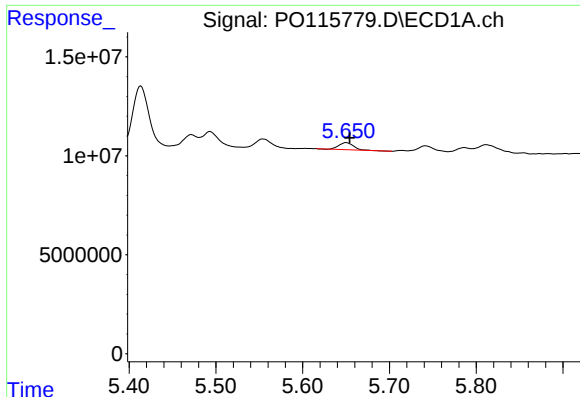

#19 AR-1242-4


R.T.: 5.650 min
Delta R.T.: -0.004 min
Response: 4244920
Conc: 31.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

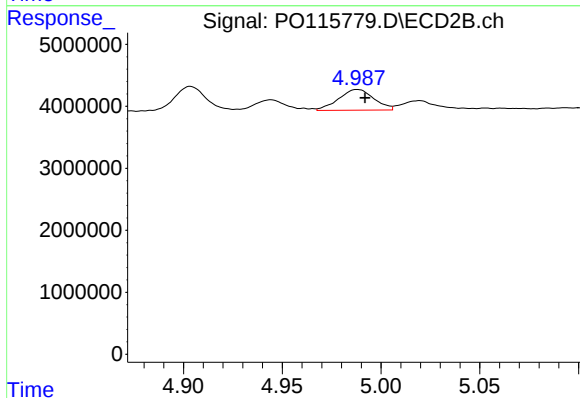


#19 AR-1242-4

R.T.: 4.988 min
Delta R.T.: -0.004 min
Response: 4157799
Conc: 38.11 ng/ml

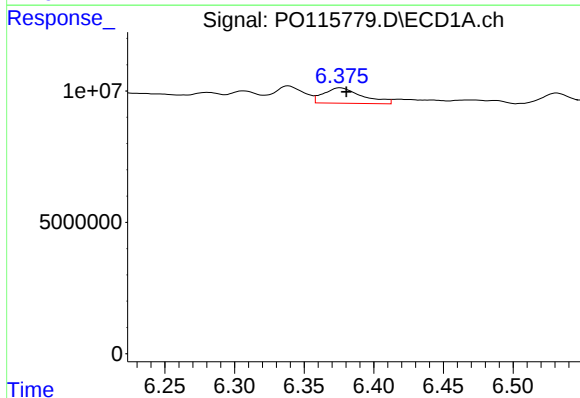


#20 AR-1242-5

R.T.: 6.376 min
Delta R.T.: -0.004 min
Response: 11349314
Conc: 74.94 ng/ml

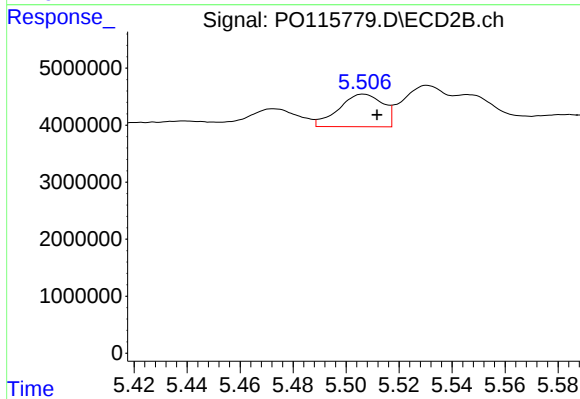

#20 AR-1242-5


R.T.: 5.507 min
Delta R.T.: -0.005 min
Response: 6591448
Conc: 47.72 ng/ml

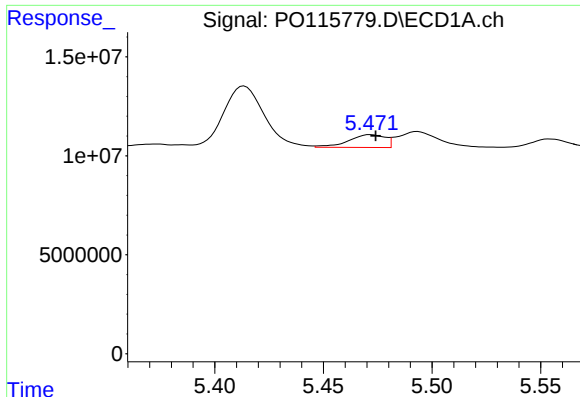

#21 AR-1248-1


R.T.: 5.472 min
Delta R.T.: -0.002 min
Response: 7620984
Conc: 50.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

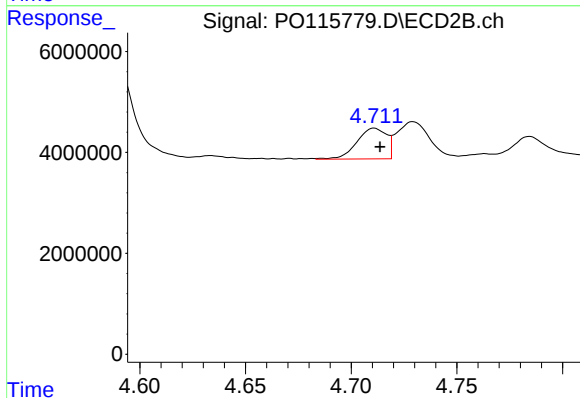


#21 AR-1248-1

R.T.: 4.711 min
Delta R.T.: -0.003 min
Response: 5965590
Conc: 53.35 ng/ml

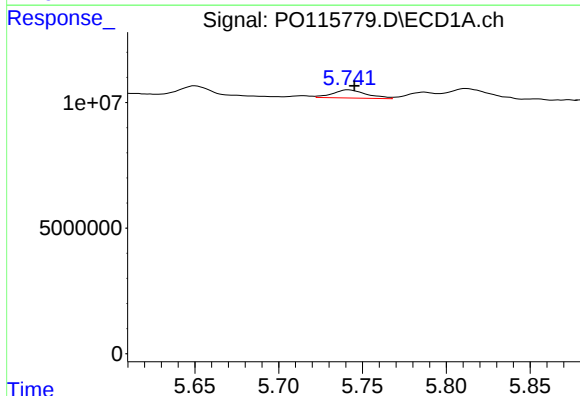


#22 AR-1248-2

R.T.: 5.742 min
Delta R.T.: -0.004 min
Response: 4551611
Conc: 22.67 ng/ml

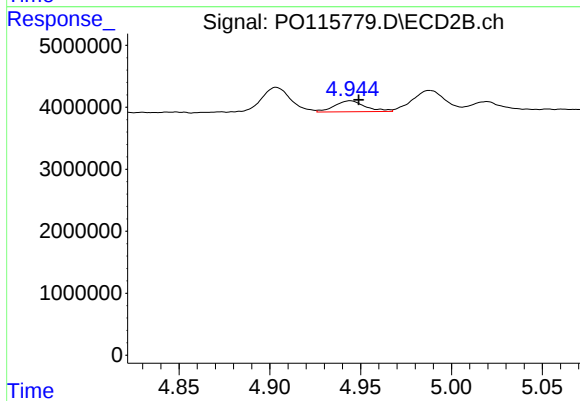

#22 AR-1248-2


R.T.: 4.944 min
Delta R.T.: -0.005 min
Response: 2101298
Conc: 13.80 ng/ml

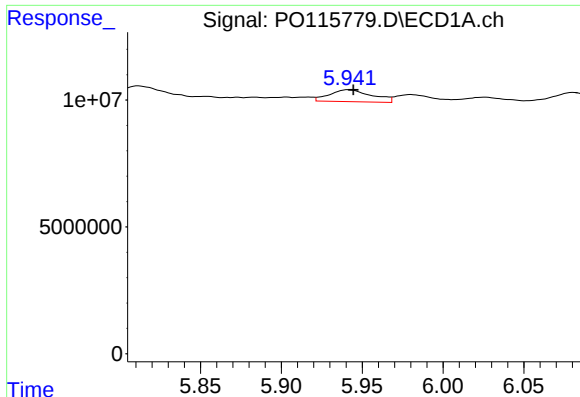

#23 AR-1248-3


R.T.: 5.942 min
Delta R.T.: -0.003 min
Response: 8607001
Conc: 34.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

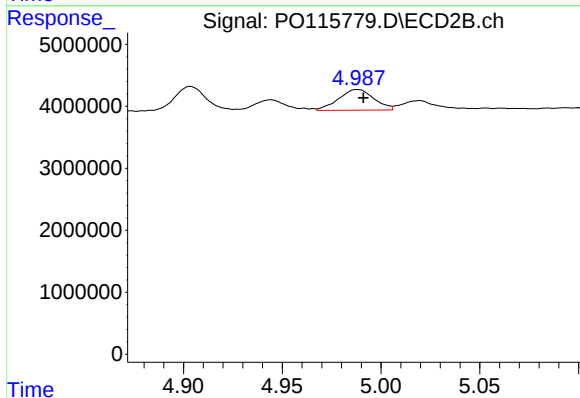


#23 AR-1248-3

R.T.: 4.988 min
Delta R.T.: -0.003 min
Response: 4157799
Conc: 25.90 ng/ml

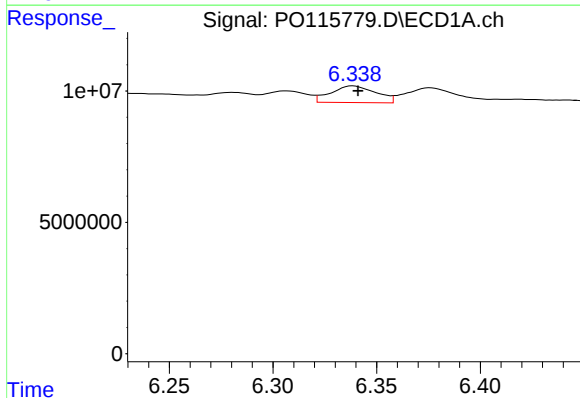


#24 AR-1248-4

R.T.: 6.339 min
Delta R.T.: -0.002 min
Response: 9595552
Conc: 32.54 ng/ml

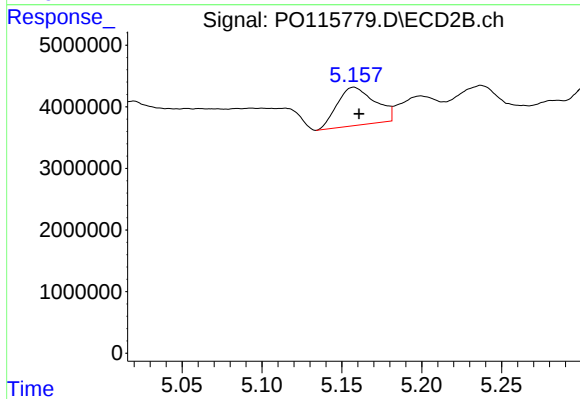

#24 AR-1248-4


R.T.: 5.157 min
Delta R.T.: -0.003 min
Response: 10226263
Conc: 54.64 ng/ml

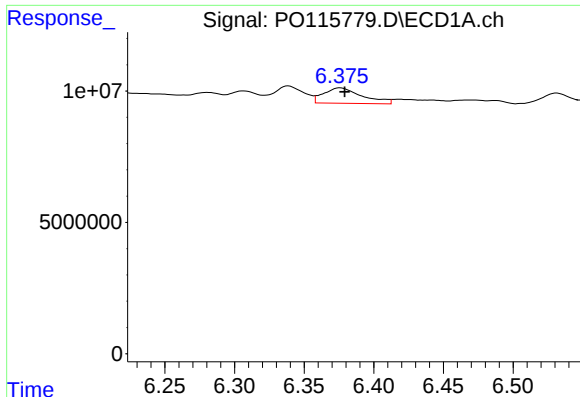

#25 AR-1248-5


R.T.: 6.376 min
Delta R.T.: -0.003 min
Response: 11349314
Conc: 43.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

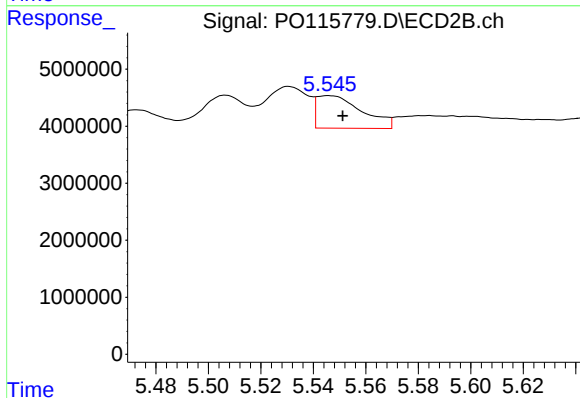


#25 AR-1248-5

R.T.: 5.546 min
Delta R.T.: -0.005 min
Response: 6818374
Conc: 34.44 ng/ml

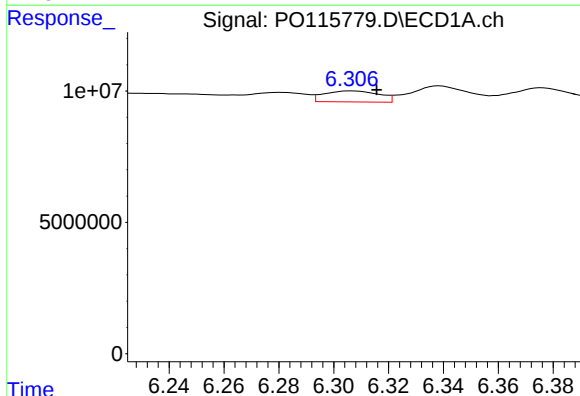


#26 AR-1254-1

R.T.: 6.307 min
Delta R.T.: -0.009 min
Response: 5805293
Conc: 22.44 ng/ml

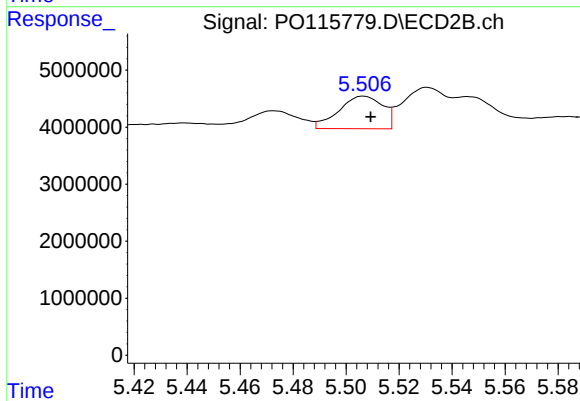

#26 AR-1254-1


R.T.: 5.507 min
Delta R.T.: -0.003 min
Response: 6591448
Conc: 22.55 ng/ml

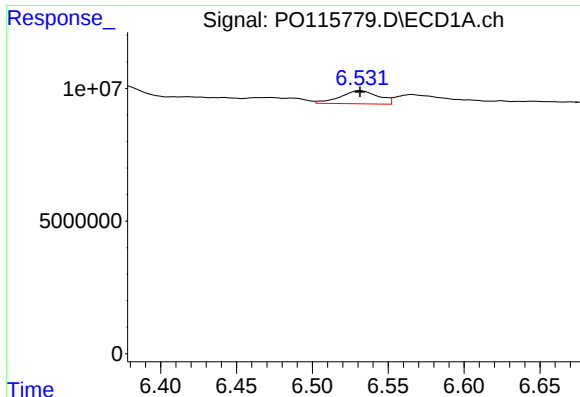

#27 AR-1254-2


R.T.: 6.532 min
Delta R.T.: 0.000 min
Response: 8573165
Conc: 21.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

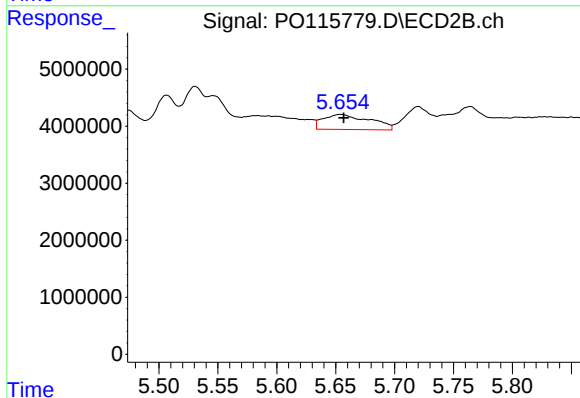


#27 AR-1254-2

R.T.: 5.654 min
Delta R.T.: -0.003 min
Response: 7300559
Conc: 28.99 ng/ml

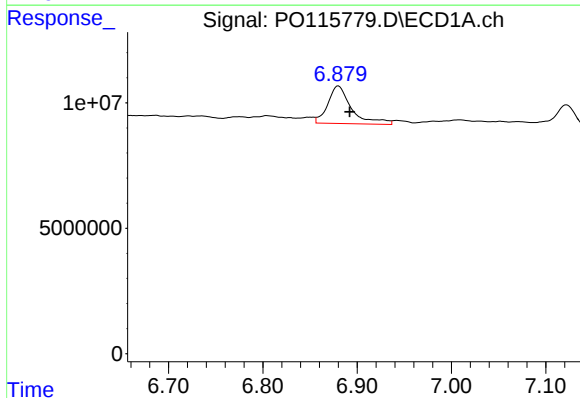


#28 AR-1254-3

R.T.: 6.880 min
Delta R.T.: -0.012 min
Response: 26248811
Conc: 63.93 ng/ml

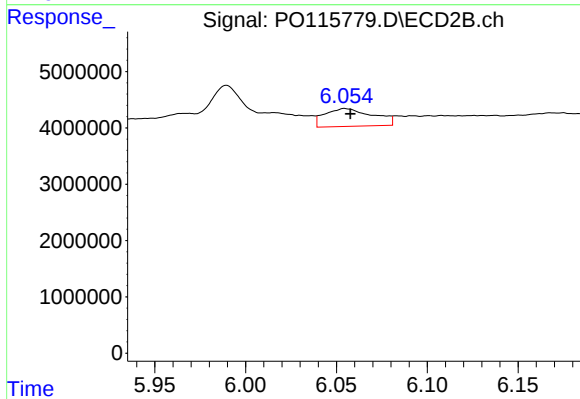

#28 AR-1254-3


R.T.: 6.055 min
Delta R.T.: -0.003 min
Response: 5864009
Conc: 14.90 ng/ml

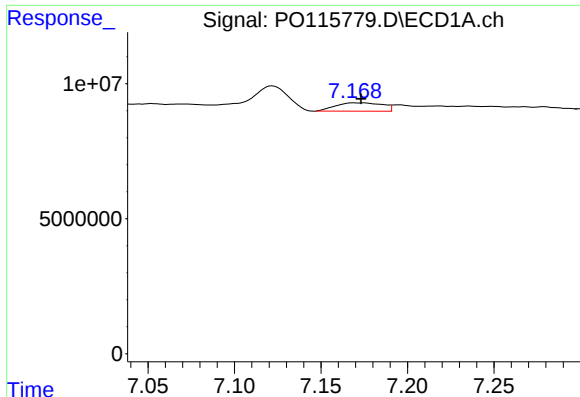

#29 AR-1254-4


R.T.: 7.169 min
Delta R.T.: -0.004 min
Response: 5838515
Conc: 16.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

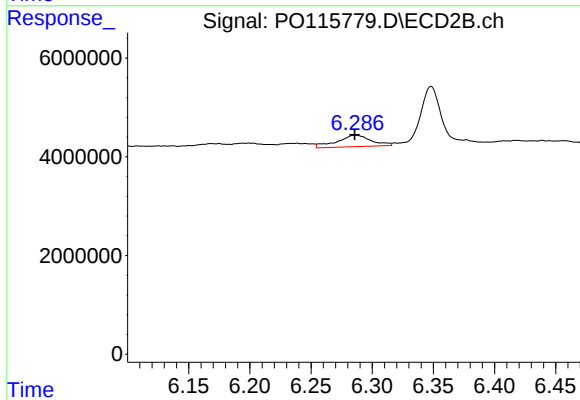


#29 AR-1254-4

R.T.: 6.286 min
Delta R.T.: 0.000 min
Response: 4494082
Conc: 16.80 ng/ml

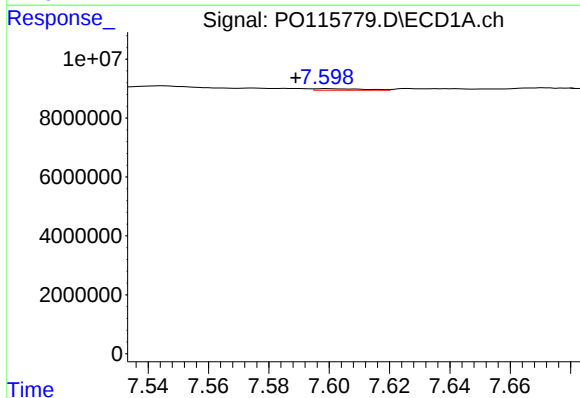


#30 AR-1254-5

R.T.: 7.599 min
Delta R.T.: 0.010 min
Response: 575290
Conc: 1.78 ng/ml

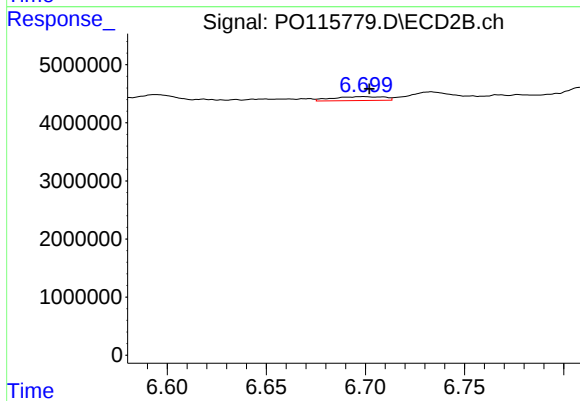

#30 AR-1254-5


R.T.: 6.699 min
Delta R.T.: -0.003 min
Response: 1197435
Conc: 3.35 ng/ml

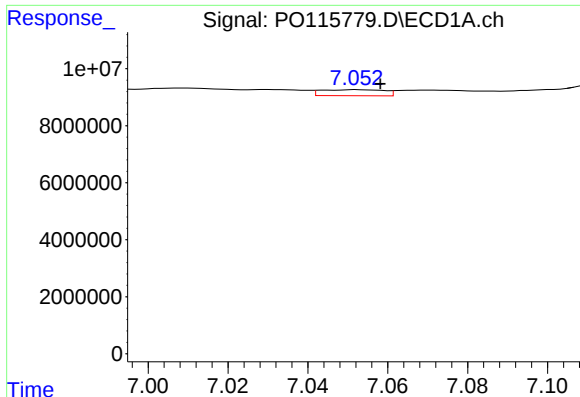

#31 AR-1260-1


R.T.: 7.052 min
Delta R.T.: -0.006 min
Response: 2302450
Conc: 7.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

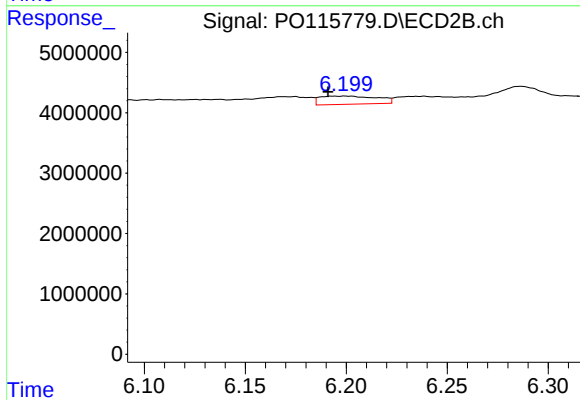


#31 AR-1260-1

R.T.: 6.199 min
Delta R.T.: 0.009 min
Response: 2693448
Conc: 10.27 ng/ml

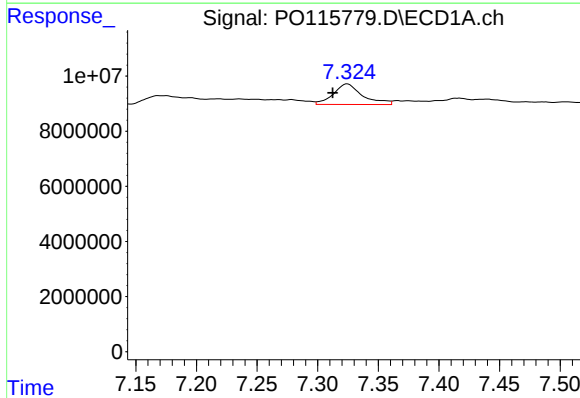


#32 AR-1260-2

R.T.: 7.325 min
Delta R.T.: 0.012 min
Response: 12552012
Conc: 28.68 ng/ml

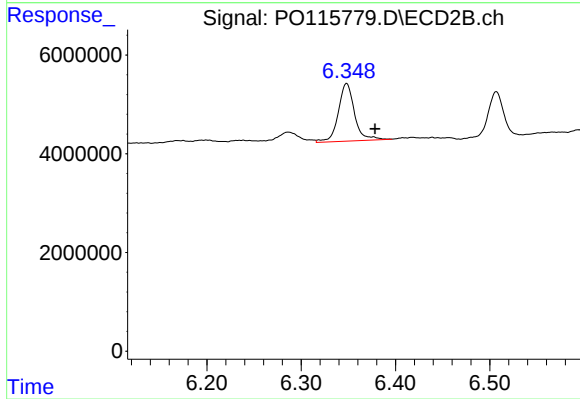

#32 AR-1260-2


R.T.: 6.348 min
Delta R.T.: -0.030 min
Response: 14004553
Conc: 39.96 ng/ml

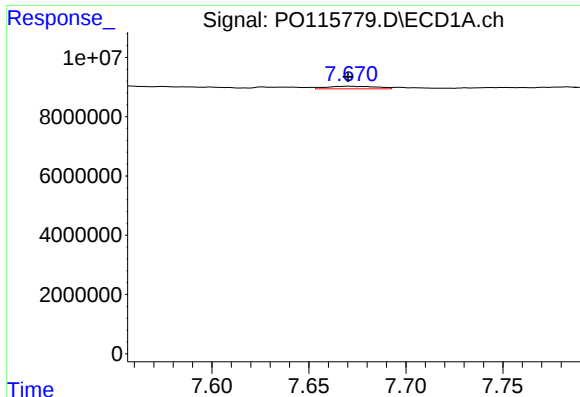

#33 AR-1260-3


R.T.: 7.671 min
Delta R.T.: 0.001 min
Response: 1554458
Conc: 4.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

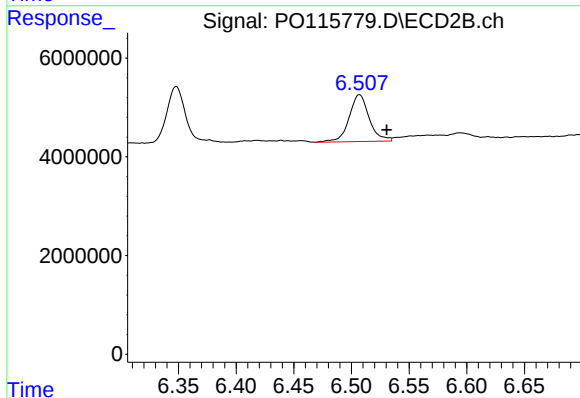


#33 AR-1260-3

R.T.: 6.507 min
Delta R.T.: -0.024 min
Response: 11506386
Conc: 35.82 ng/ml

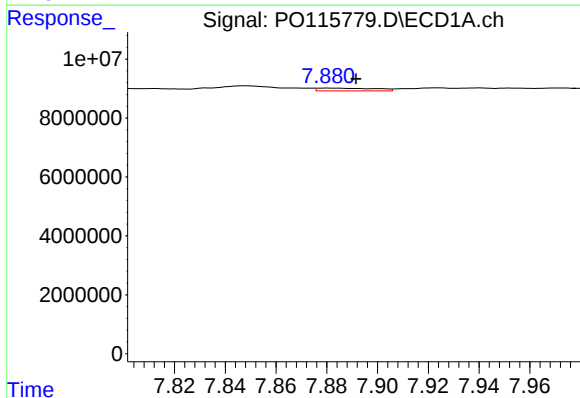


#34 AR-1260-4

R.T.: 7.880 min
Delta R.T.: -0.011 min
Response: 1482400
Conc: 4.82 ng/ml

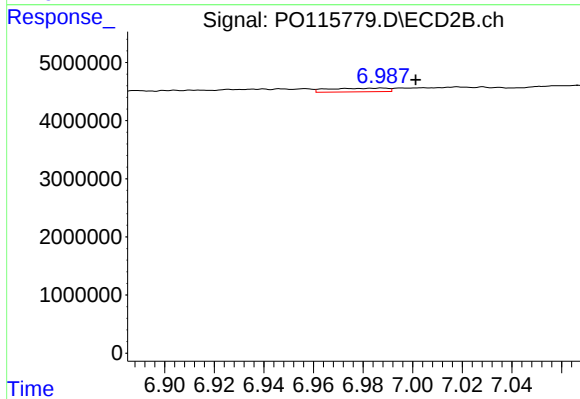

#34 AR-1260-4


R.T.: 6.988 min
Delta R.T.: -0.014 min
Response: 1033671
Conc: 4.02 ng/ml

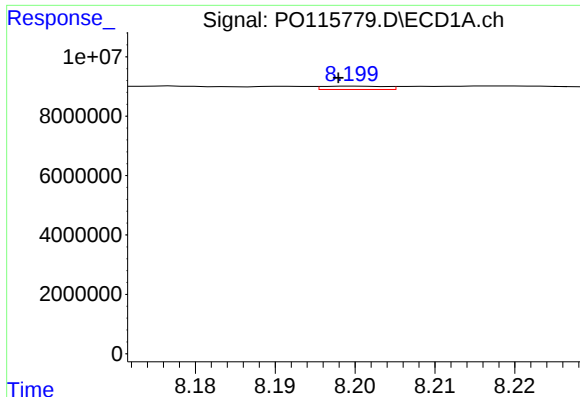

#35 AR-1260-5


R.T.: 8.200 min
Delta R.T.: 0.002 min
Response: 618803
Conc: 0.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

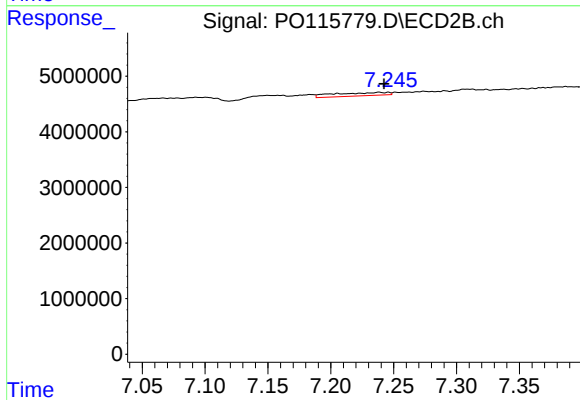


#35 AR-1260-5

R.T.: 7.238 min
Delta R.T.: -0.004 min
Response: 1735411
Conc: 2.47 ng/ml

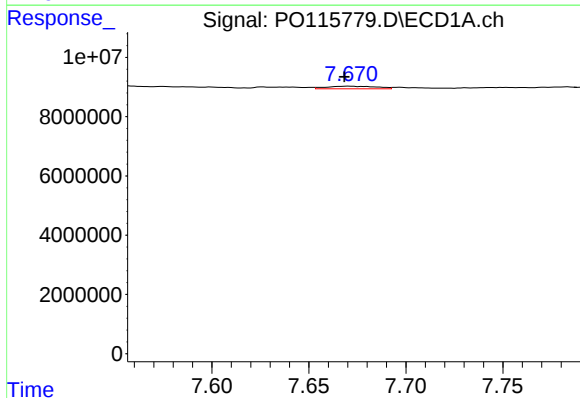


#36 AR-1262-1

R.T.: 7.671 min
Delta R.T.: 0.003 min
Response: 1554458
Conc: 6.30 ng/ml

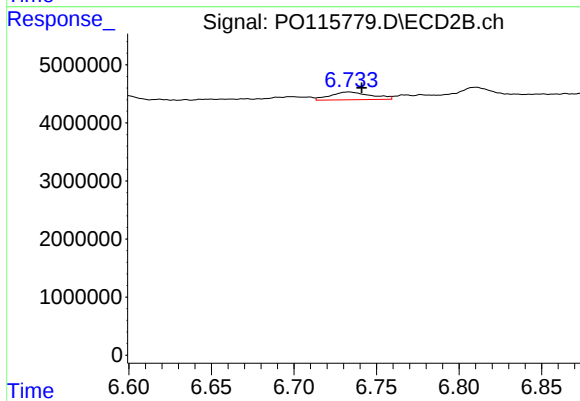

#36 AR-1262-1


R.T.: 6.733 min
Delta R.T.: -0.008 min
Response: 2266948
Conc: 10.64 ng/ml

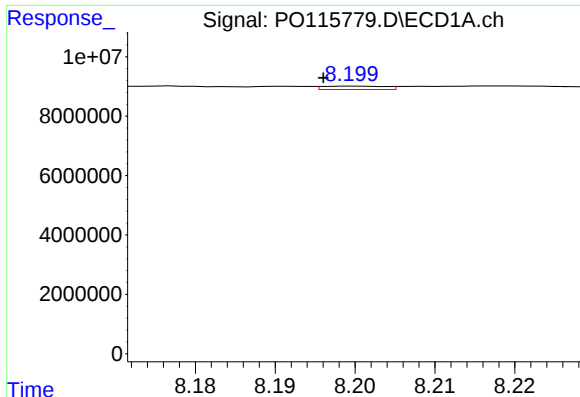

#37 AR-1262-2


R.T.: 8.200 min
Delta R.T.: 0.004 min
Response: 618803
Conc: 1.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

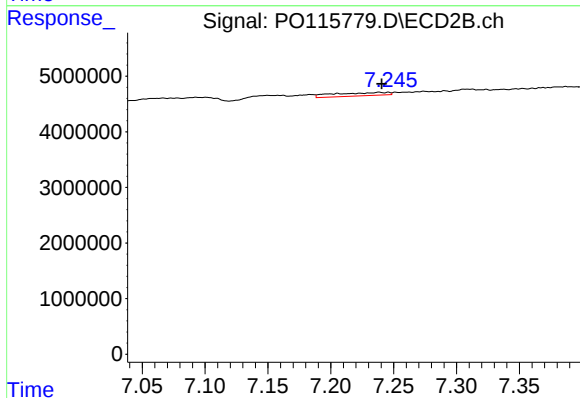


#37 AR-1262-2

R.T.: 7.238 min
Delta R.T.: -0.002 min
Response: 1735411
Conc: 4.98 ng/ml

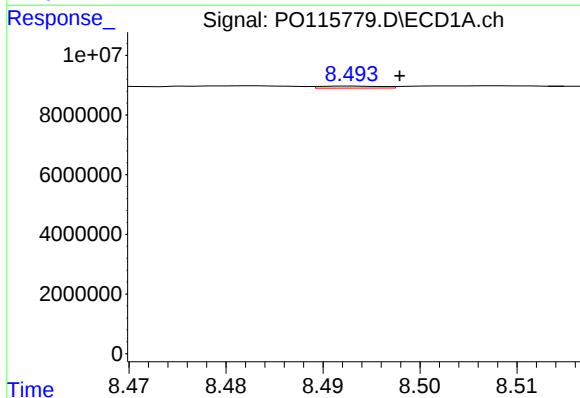


#38 AR-1262-3

R.T.: 8.493 min
Delta R.T.: -0.005 min
Response: 292048
Conc: 1.15 ng/ml

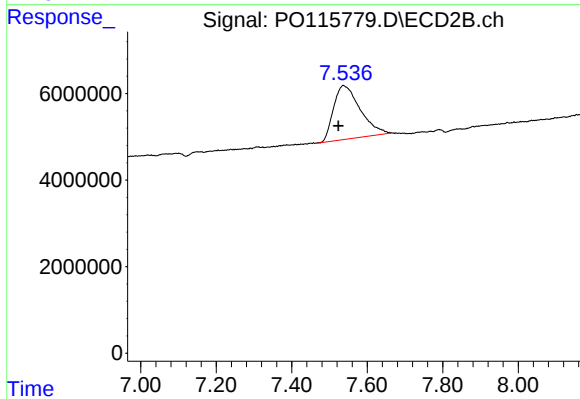

#38 AR-1262-3


R.T.: 7.536 min
Delta R.T.: 0.013 min
Response: 60806908
Conc: 388.81 ng/ml

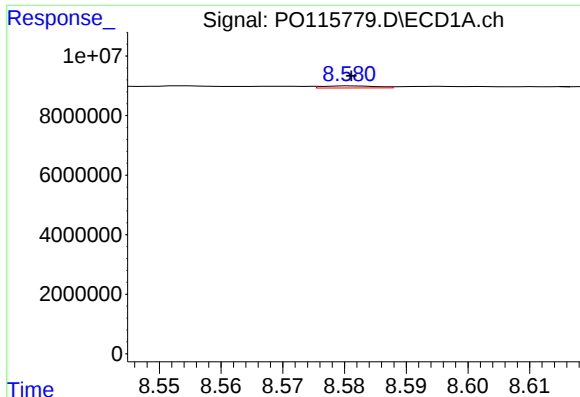

#39 AR-1262-4


R.T.: 8.581 min
Delta R.T.: 0.000 min
Response: 434294
Conc: 2.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

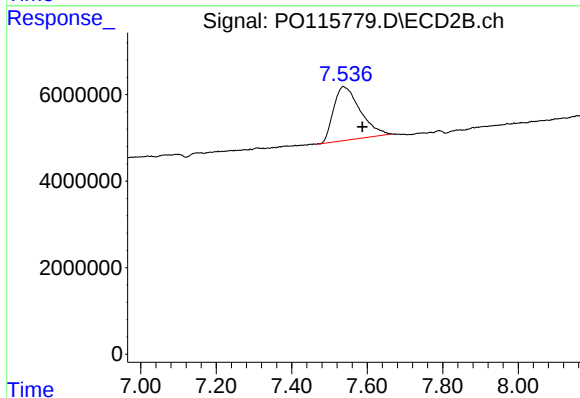


#39 AR-1262-4

R.T.: 7.536 min
Delta R.T.: -0.051 min
Response: 60806908
Conc: 245.81 ng/ml

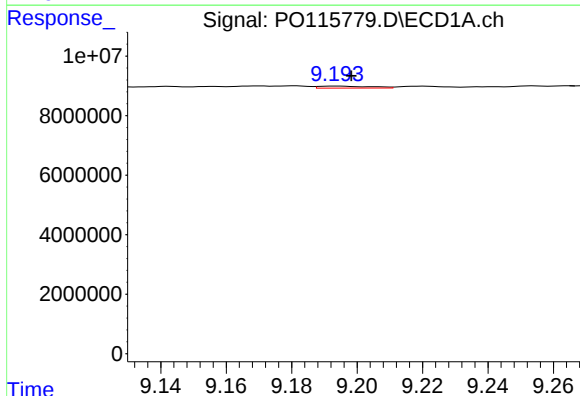


#40 AR-1262-5

R.T.: 9.194 min
Delta R.T.: -0.004 min
Response: 767472
Conc: 5.70 ng/ml

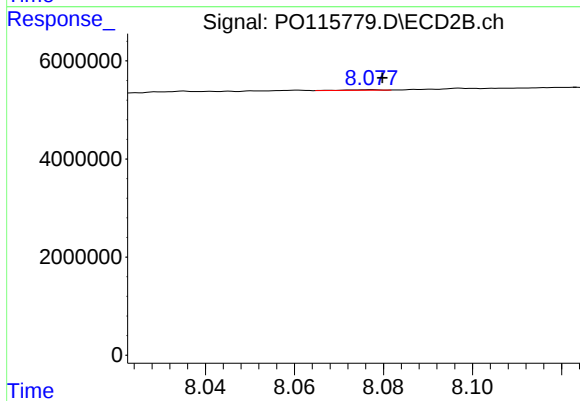

#40 AR-1262-5


R.T.: 8.077 min
Delta R.T.: -0.003 min
Response: 59715
Conc: 0.54 ng/ml

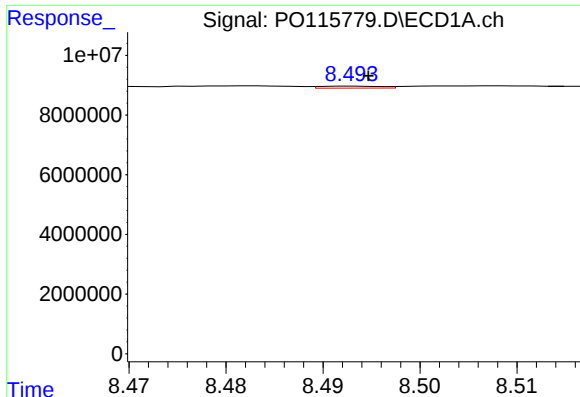

#41 AR-1268-1


R.T.: 8.493 min
Delta R.T.: -0.001 min
Response: 292048
Conc: 0.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

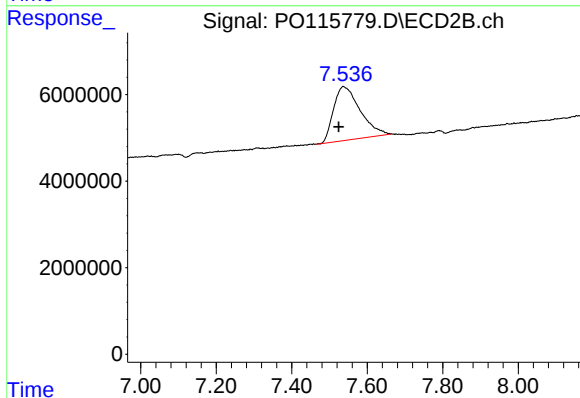


#41 AR-1268-1

R.T.: 7.536 min
Delta R.T.: 0.012 min
Response: 60806908
Conc: 68.63 ng/ml

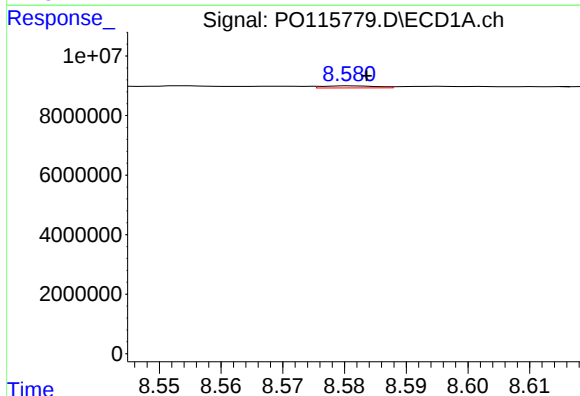


#42 AR-1268-2

R.T.: 8.581 min
Delta R.T.: -0.002 min
Response: 434294
Conc: 0.51 ng/ml

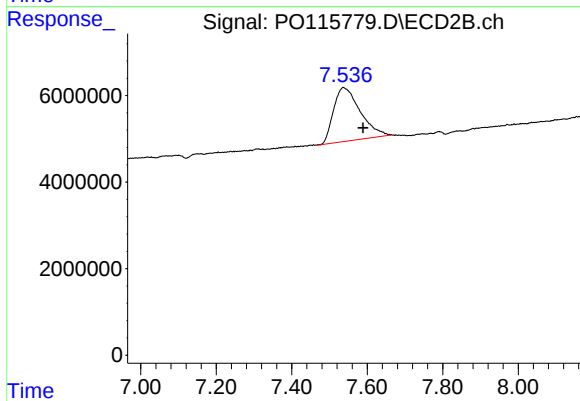

#42 AR-1268-2


R.T.: 7.536 min
Delta R.T.: -0.052 min
Response: 60806908
Conc: 81.18 ng/ml

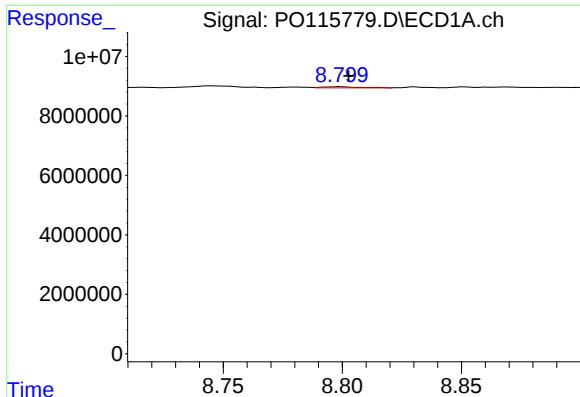

#43 AR-1268-3


R.T.: 8.800 min
Delta R.T.: -0.003 min
Response: 359990
Conc: 0.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

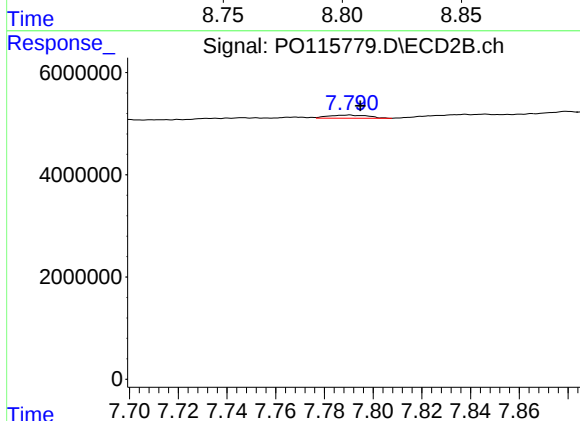


#43 AR-1268-3

R.T.: 7.790 min
Delta R.T.: -0.005 min
Response: 711490
Conc: 1.12 ng/ml

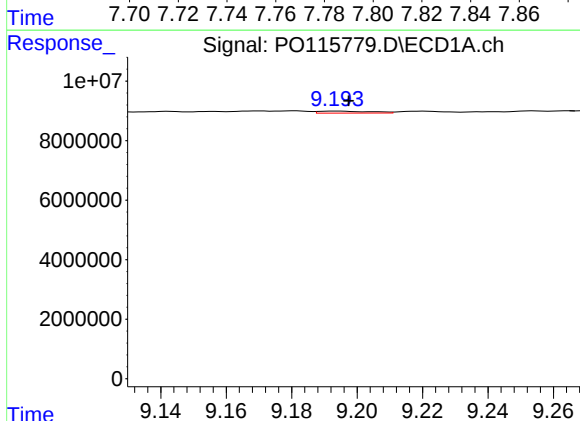


#44 AR-1268-4

R.T.: 9.194 min
Delta R.T.: -0.003 min
Response: 767472
Conc: 2.46 ng/ml

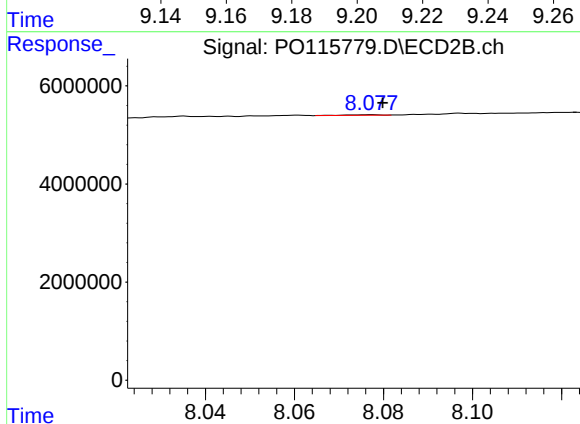

#44 AR-1268-4


R.T.: 8.077 min
Delta R.T.: -0.003 min
Response: 59715
Conc: 0.23 ng/ml

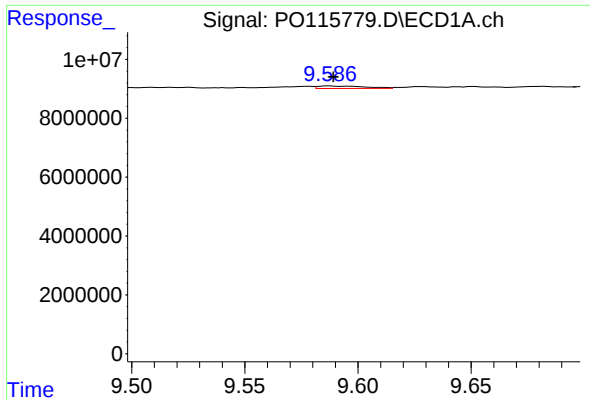

#45 AR-1268-5

R.T.: 9.587 min
Delta R.T.: -0.002 min
Response: 1230938
Conc: 0.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

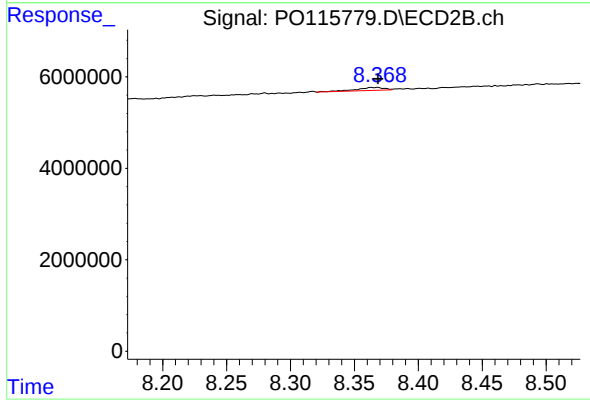

#45 AR-1268-5

R.T.: 8.368 min
Delta R.T.: 0.000 min
Response: 941299
Conc: 0.56 ng/ml