

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121225\
 Data File : PO115780.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Dec 2025 02:51
 Operator : YP/AJ
 Sample : Q3530-07
 Misc : AR1248 25PPB WATER LOD
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 13 03:51:24 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 05 02:11:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.333	3.636	148.8E6	90819492	19.160	18.636
2)	SA Decachlor...	9.904	8.614	105.8E6	79260857	20.103	18.432
Target Compounds							
3)	L1 AR-1016-1	5.471	4.711	4317885	2969023	17.364	16.069
4)	L1 AR-1016-2	5.494	4.729	5663678	3026494	14.871	11.451
5)	L1 AR-1016-3	5.554	4.905	2553060	2213357	11.942	14.625
6)	L1 AR-1016-4	5.648	4.946	1999330	3946559	11.196	35.017 #
7)	L1 AR-1016-5	5.942	5.157	7550493	5900302	43.041	40.319
8)	L2 AR-1221-1	4.528	3.839	5489706	68756	67.610	1.219 #
9)	L2 AR-1221-2	4.629	3.934	2709229	2134576	42.991	50.292
10)	L2 AR-1221-3	4.689	4.010	1017031	224598	5.447	1.747 #
11)	L3 AR-1232-1	4.689	4.010	1017031	224598	6.795	2.102 #
12)	L3 AR-1232-2	5.209	4.729	2939224	3026494	36.354	27.268
13)	L3 AR-1232-3	5.494	4.905	5663678	2213357	36.800	33.861
14)	L3 AR-1232-4	5.648	4.987	1999330	4192631	28.549	81.680 #
15)	L3 AR-1232-5	5.743	5.157	4917962	5900302	94.691	107.772
16)	L4 AR-1242-1	5.471	4.711	4317885	2969023	21.739	20.852
17)	L4 AR-1242-2	5.494	4.729	5663678	3026494	19.337	14.456 #
18)	L4 AR-1242-3	5.554	4.905	2553060	2213357	15.123	18.531
19)	L4 AR-1242-4	5.648	4.987	1999330	4192631	14.629	38.432 #
20)	L4 AR-1242-5	6.376	5.506	7943356	7219479	52.451	52.268
21)	L5 AR-1248-1	5.471	4.711	4317885	2969023	28.451	26.550
22)	L5 AR-1248-2	5.743	4.946	4917962	3946559	24.490	25.915
23)	L5 AR-1248-3	5.942	4.987	7550493	4192631	30.618	26.118
24)	L5 AR-1248-4	6.338	5.157	7835137	5900302	26.573	31.528
25)	L5 AR-1248-5	6.376	5.548	7943356	8092730	30.678	40.882 #
26)	L6 AR-1254-1	6.311	5.506	5928331	7219479	22.915	24.701
27)	L6 AR-1254-2	6.531	5.654	6977794	2327079	17.340	9.241 #
28)	L6 AR-1254-3	6.884	6.054	8541494	3242614	20.804	8.239 #
29)	L6 AR-1254-4	7.171	6.283	3163955	2664838	9.116	9.959
30)	L6 AR-1254-5	7.592	6.701	395392	746883	1.220	2.089 #
31)	L7 AR-1260-1	7.058	6.183	759509	97923	2.622	0.374 #
32)	L7 AR-1260-2	7.322	6.370	2813686	302771	6.428	0.864 #
33)	L7 AR-1260-3	7.668	6.507	582970	2885905	1.732	8.983 #
34)	L7 AR-1260-4	7.888	7.017	532352	730878	1.731	2.846 #
35)	L7 AR-1260-5	8.207	7.242	1696329	237324	2.329	0.338 #
36)	L8 AR-1262-1	7.668	6.737	582970	578035	2.362	2.713
37)	L8 AR-1262-2	8.207	7.242	1696329	237324	4.285	0.681 #
38)	L8 AR-1262-3	8.493	7.539	332732	13838370	1.306	88.486 #
39)	L8 AR-1262-4	8.580	7.619	278634	320337	1.438	1.295
40)	L8 AR-1262-5	9.195	8.074	694963	72551	5.160	0.651 #
41)	L9 AR-1268-1	8.493	7.539	332732	13838370	0.334	15.620 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121225\
 Data File : PO115780.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Dec 2025 02:51
 Operator : YP/AJ
 Sample : Q3530-07
 Misc : AR1248 25PPB WATER LOD
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 13 03:51:24 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 05 02:11:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.580	7.619	278634	320337	0.326	0.428 #
43) L9	AR-1268-3	8.801	7.779	52935	467034	0.071	0.734 #
44) L9	AR-1268-4	9.195	8.074	694963	72551	2.226	0.282 #
45) L9	AR-1268-5	9.587	8.362	1510891	365994	0.694	0.217 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121225\
Data File : PO115780.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Dec 2025 02:51
Operator : YP/AJ
Sample : Q3530-07
Misc : AR1248 25PPB WATER LOD
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 13 03:51:24 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120425.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 05 02:11:05 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

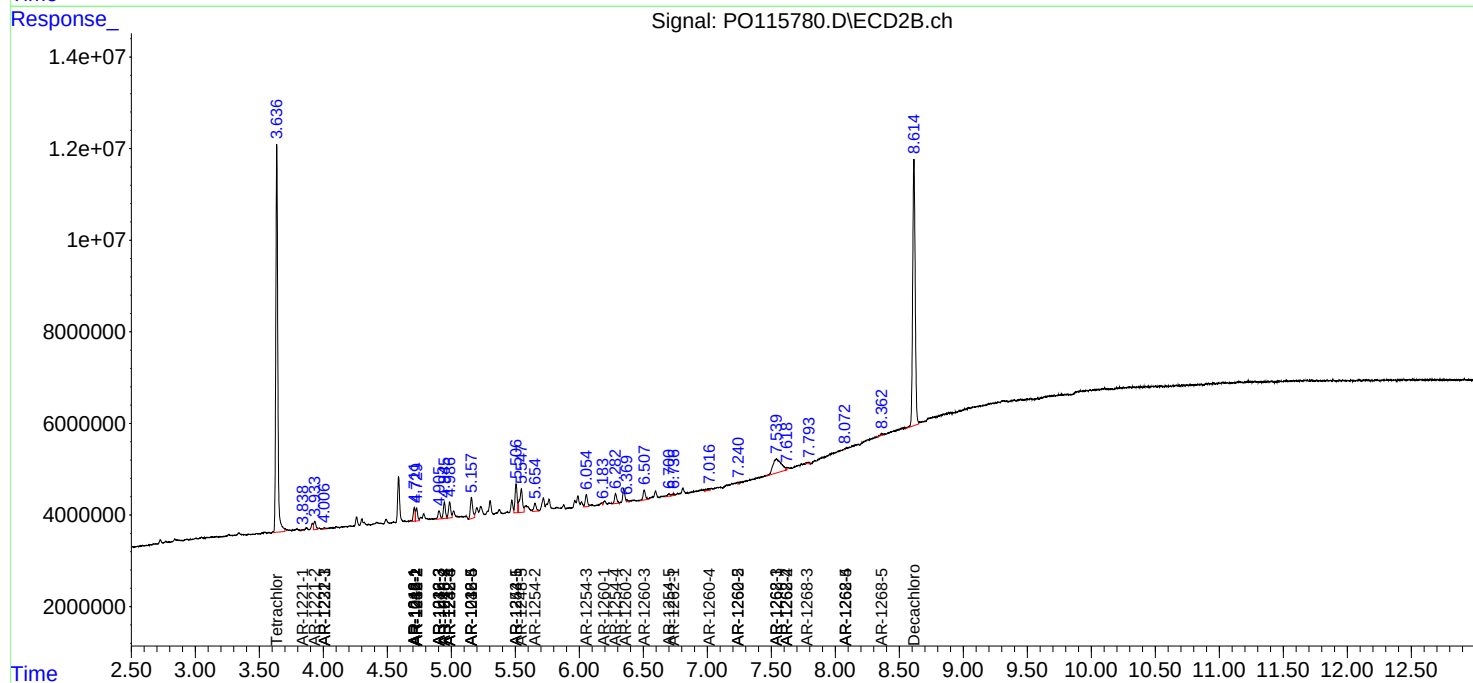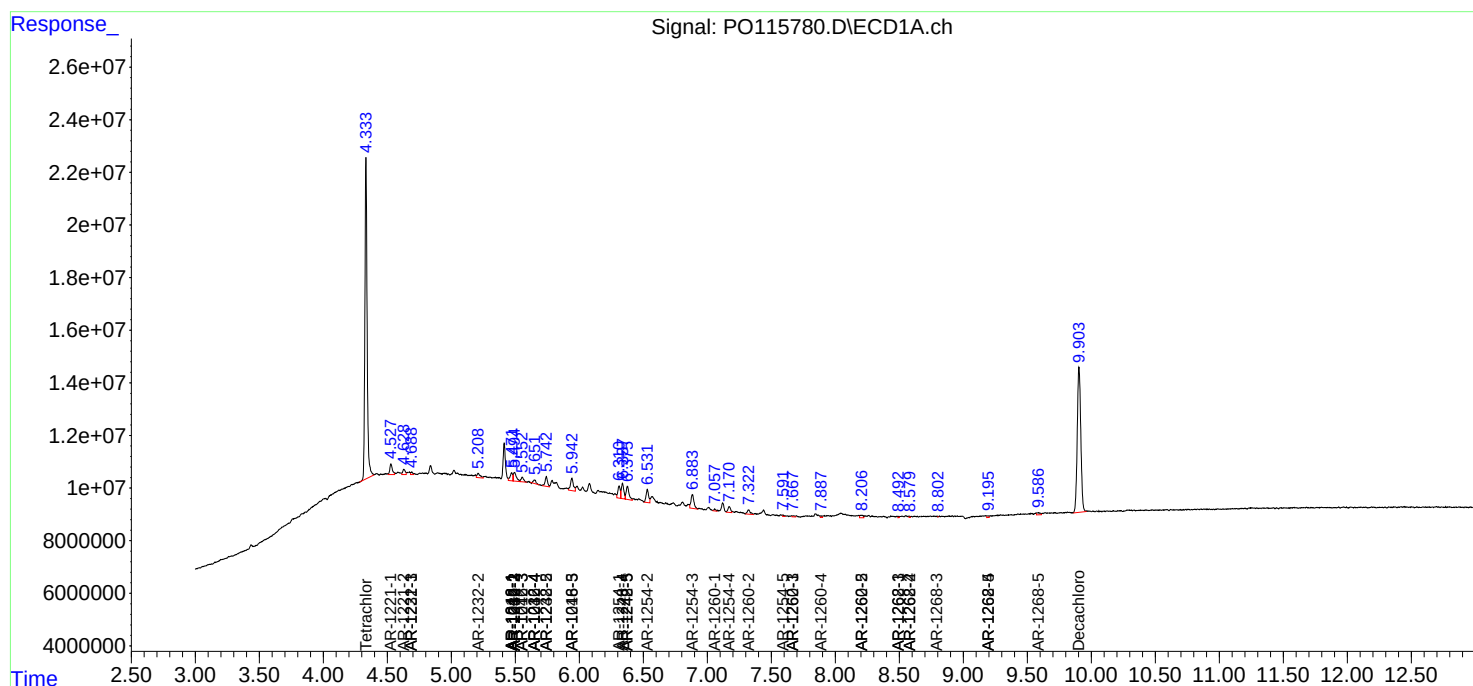


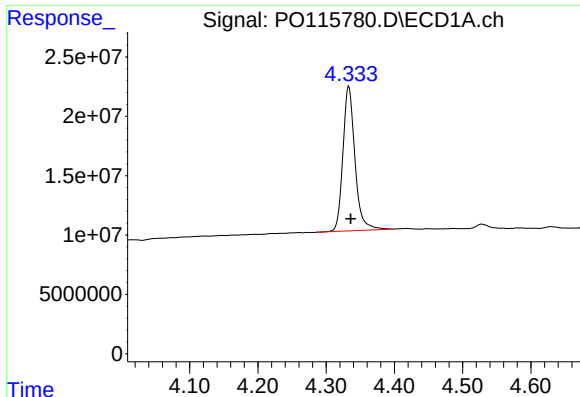

#1 Tetrachloro-m-xylene


R.T.: 4.333 min
Delta R.T.: -0.003 min
Response: 148817684
Conc: 19.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

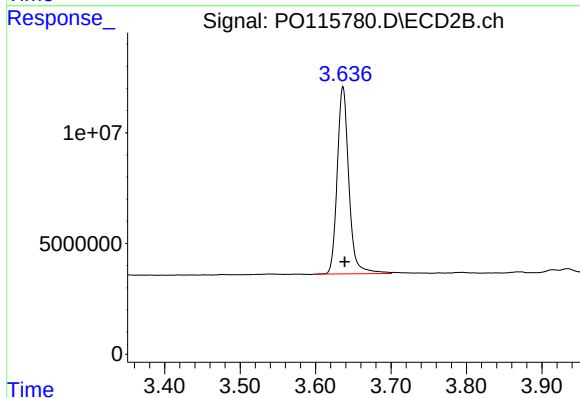


#1 Tetrachloro-m-xylene

R.T.: 3.636 min
Delta R.T.: -0.002 min
Response: 90819492
Conc: 18.64 ng/ml

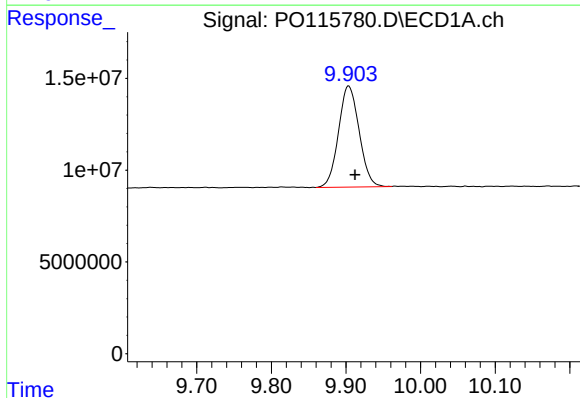


#2 Decachlorobiphenyl

R.T.: 9.904 min
Delta R.T.: -0.009 min
Response: 105764952
Conc: 20.10 ng/ml

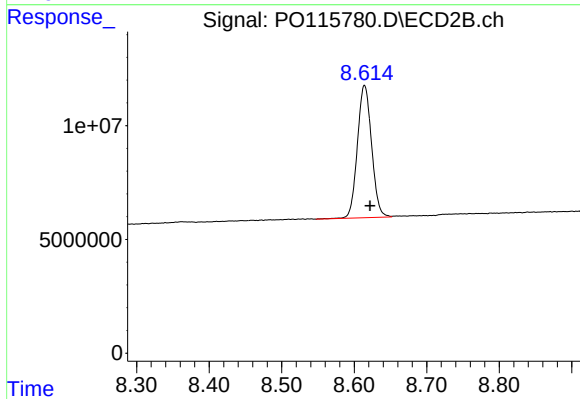

#2 Decachlorobiphenyl


R.T.: 8.614 min
Delta R.T.: -0.008 min
Response: 79260857
Conc: 18.43 ng/ml

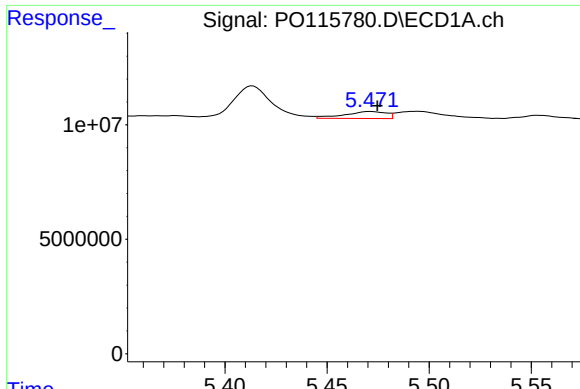

#3 AR-1016-1


R.T.: 5.471 min
Delta R.T.: -0.003 min
Response: 4317885
Conc: 17.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

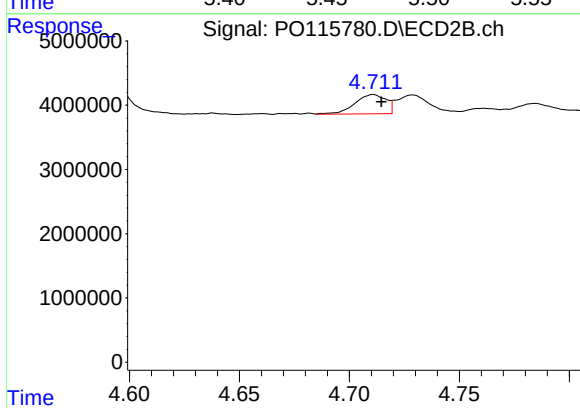


#3 AR-1016-1

R.T.: 4.711 min
Delta R.T.: -0.004 min
Response: 2969023
Conc: 16.07 ng/ml

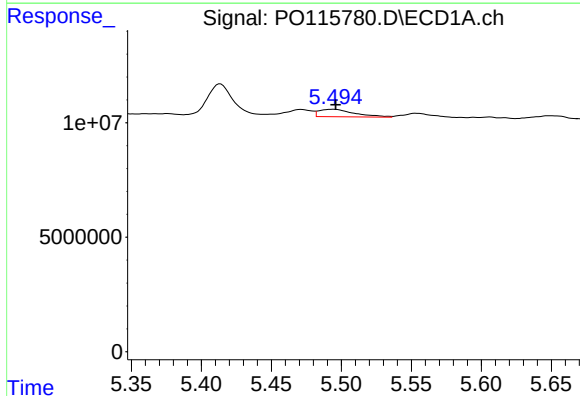


#4 AR-1016-2

R.T.: 5.494 min
Delta R.T.: -0.002 min
Response: 5663678
Conc: 14.87 ng/ml

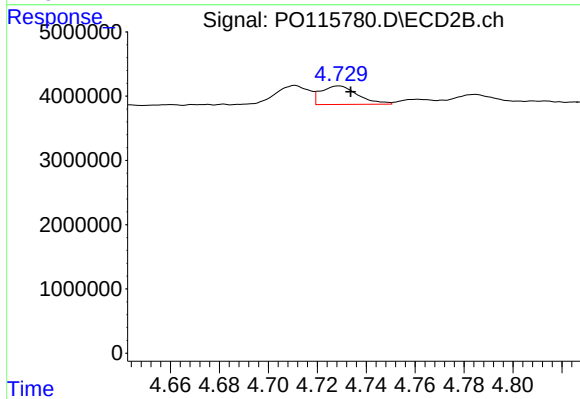

#4 AR-1016-2


R.T.: 4.729 min
Delta R.T.: -0.005 min
Response: 3026494
Conc: 11.45 ng/ml

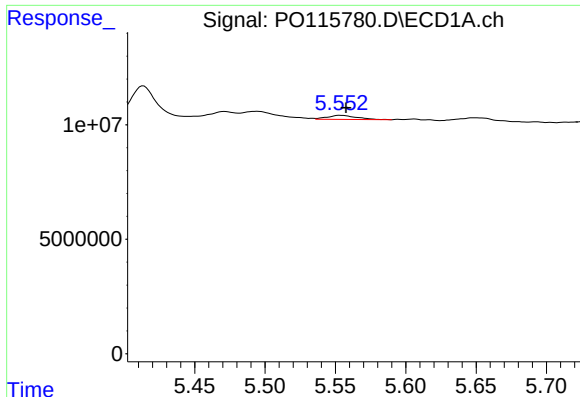

#5 AR-1016-3


R.T.: 5.554 min
Delta R.T.: -0.004 min
Response: 2553060
Conc: 11.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

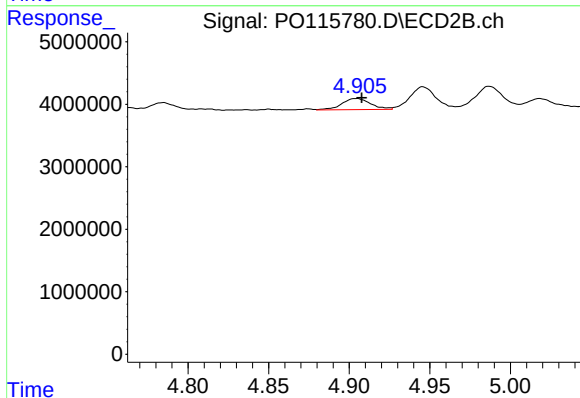


#5 AR-1016-3

R.T.: 4.905 min
Delta R.T.: -0.003 min
Response: 2213357
Conc: 14.63 ng/ml

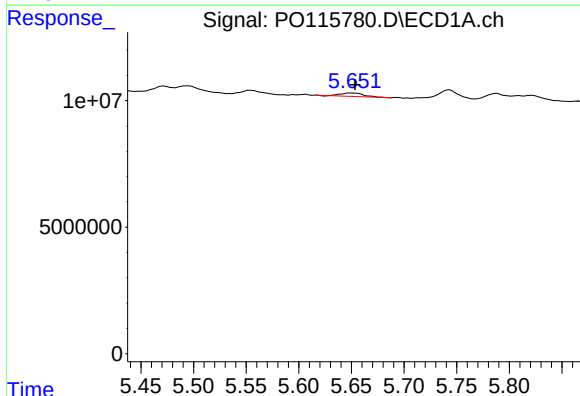


#6 AR-1016-4

R.T.: 5.648 min
Delta R.T.: -0.005 min
Response: 1999330
Conc: 11.20 ng/ml

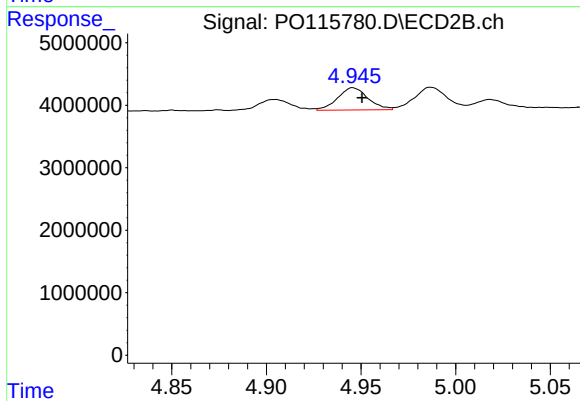

#6 AR-1016-4


R.T.: 4.946 min
Delta R.T.: -0.005 min
Response: 3946559
Conc: 35.02 ng/ml

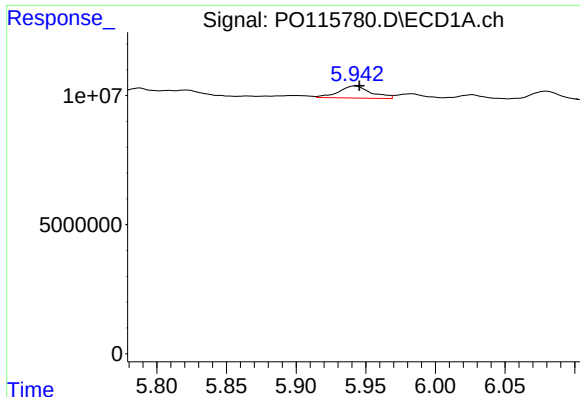

#7 AR-1016-5


R.T.: 5.942 min
Delta R.T.: -0.003 min
Response: 7550493
Conc: 43.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

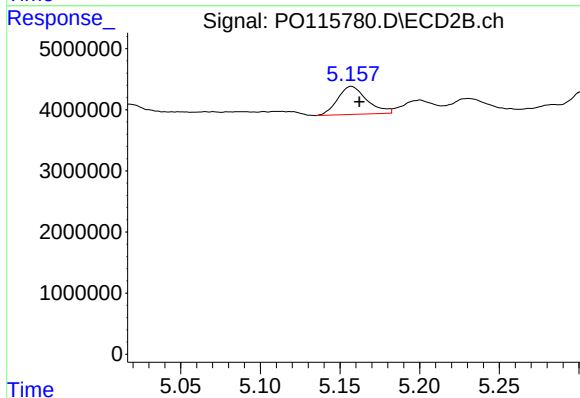


#7 AR-1016-5

R.T.: 5.157 min
Delta R.T.: -0.005 min
Response: 5900302
Conc: 40.32 ng/ml

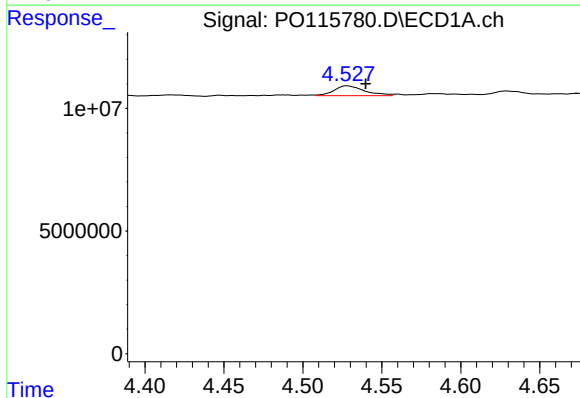


#8 AR-1221-1

R.T.: 4.528 min
Delta R.T.: -0.012 min
Response: 5489706
Conc: 67.61 ng/ml

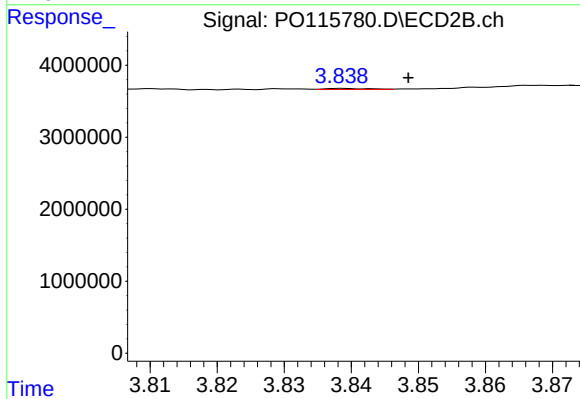

#8 AR-1221-1


R.T.: 3.839 min
Delta R.T.: -0.010 min
Response: 68756
Conc: 1.22 ng/ml

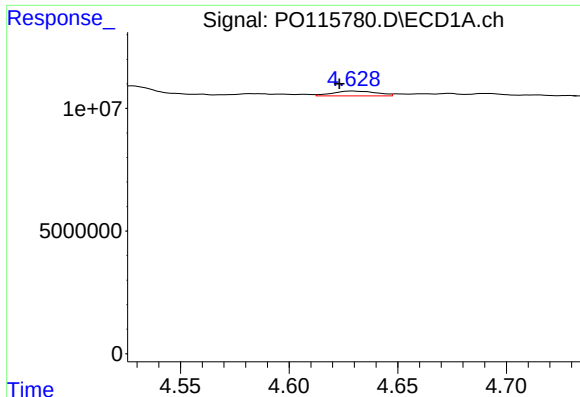

#9 AR-1221-2


R.T.: 4.629 min
Delta R.T.: 0.006 min
Response: 2709229
Conc: 42.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

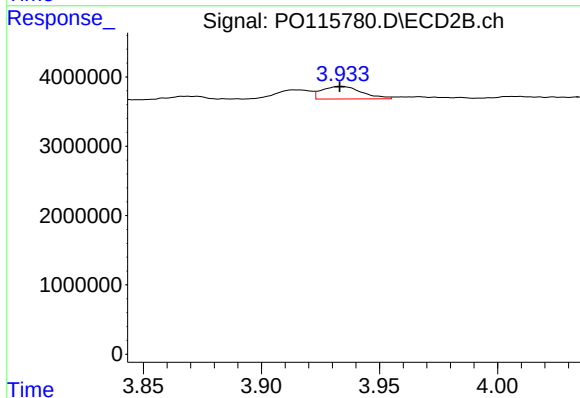


#9 AR-1221-2

R.T.: 3.934 min
Delta R.T.: 0.000 min
Response: 2134576
Conc: 50.29 ng/ml

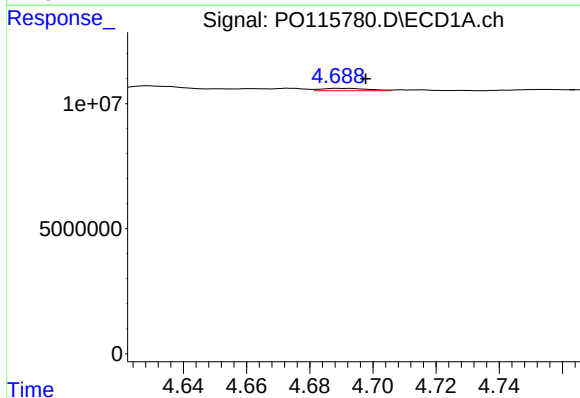


#10 AR-1221-3

R.T.: 4.689 min
Delta R.T.: -0.009 min
Response: 1017031
Conc: 5.45 ng/ml

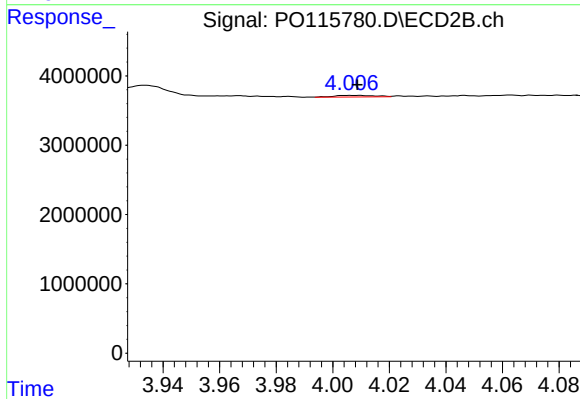

#10 AR-1221-3


R.T.: 4.010 min
Delta R.T.: 0.001 min
Response: 224598
Conc: 1.75 ng/ml

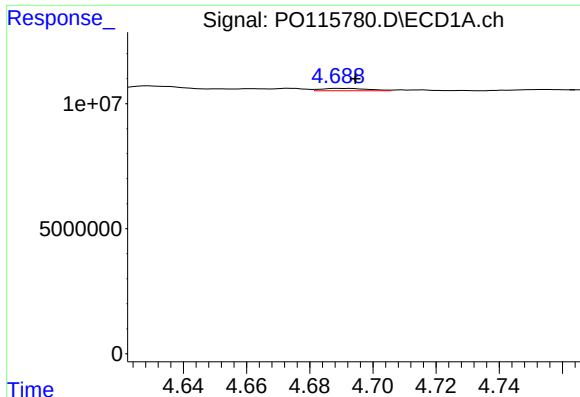

#11 AR-1232-1


R.T.: 4.689 min
Delta R.T.: -0.005 min
Response: 1017031
Conc: 6.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

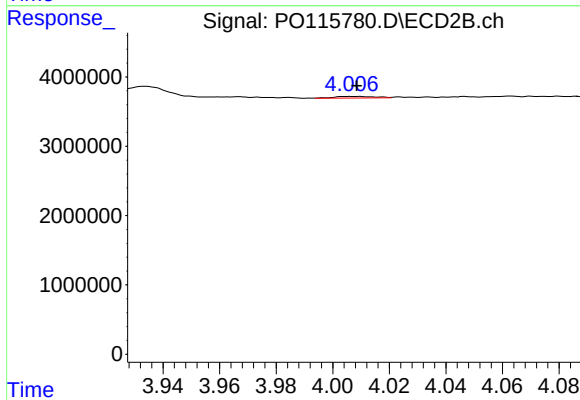


#11 AR-1232-1

R.T.: 4.010 min
Delta R.T.: 0.001 min
Response: 224598
Conc: 2.10 ng/ml

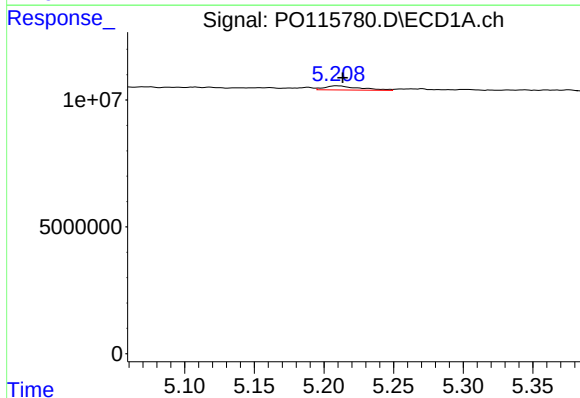


#12 AR-1232-2

R.T.: 5.209 min
Delta R.T.: -0.004 min
Response: 2939224
Conc: 36.35 ng/ml

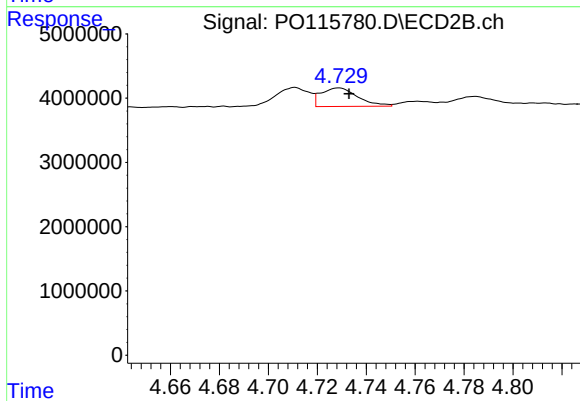

#12 AR-1232-2


R.T.: 4.729 min
Delta R.T.: -0.004 min
Response: 3026494
Conc: 27.27 ng/ml

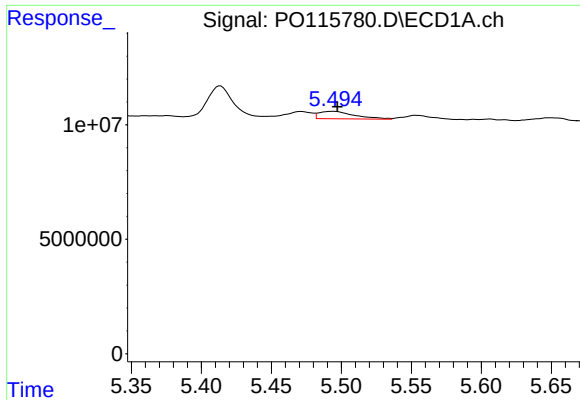

#13 AR-1232-3


R.T.: 5.494 min
Delta R.T.: -0.003 min
Response: 5663678
Conc: 36.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

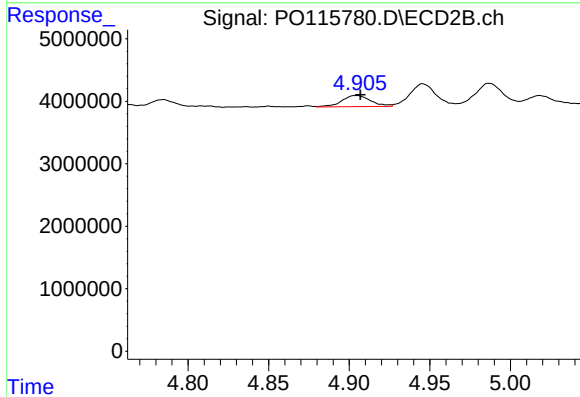


#13 AR-1232-3

R.T.: 4.905 min
Delta R.T.: -0.002 min
Response: 2213357
Conc: 33.86 ng/ml

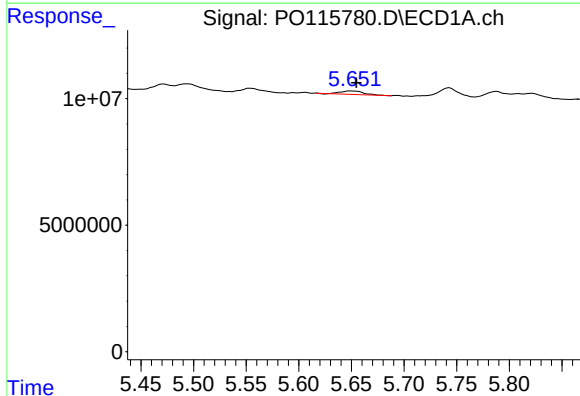


#14 AR-1232-4

R.T.: 5.648 min
Delta R.T.: -0.006 min
Response: 1999330
Conc: 28.55 ng/ml

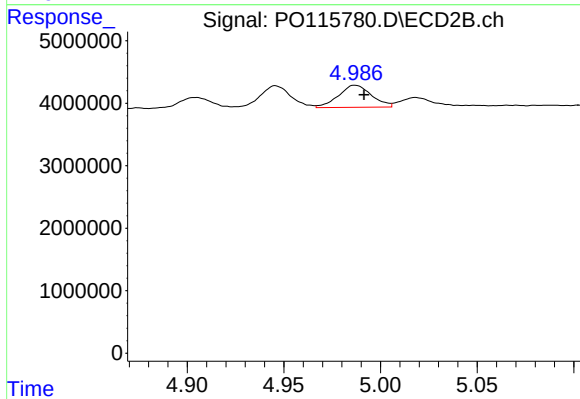

#14 AR-1232-4


R.T.: 4.987 min
Delta R.T.: -0.005 min
Response: 4192631
Conc: 81.68 ng/ml

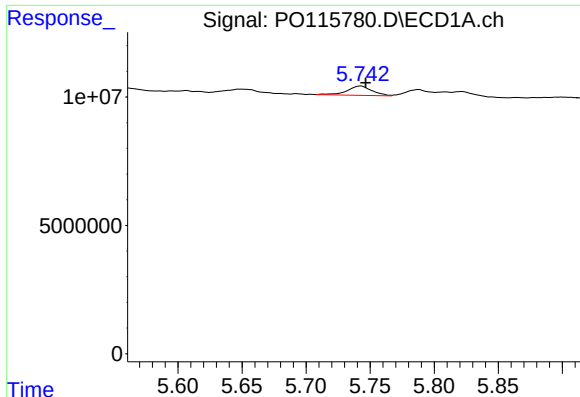

#15 AR-1232-5


R.T.: 5.743 min
Delta R.T.: -0.004 min
Response: 4917962
Conc: 94.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

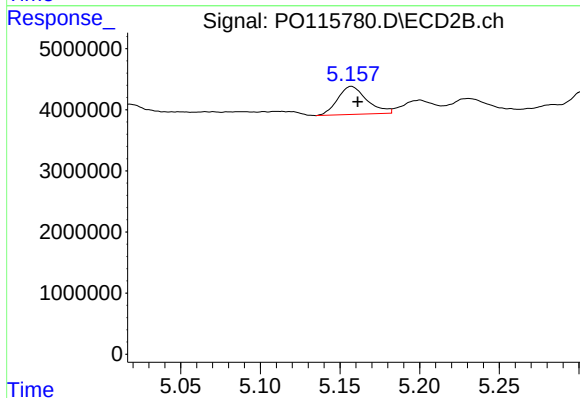


#15 AR-1232-5

R.T.: 5.157 min
Delta R.T.: -0.004 min
Response: 5900302
Conc: 107.77 ng/ml

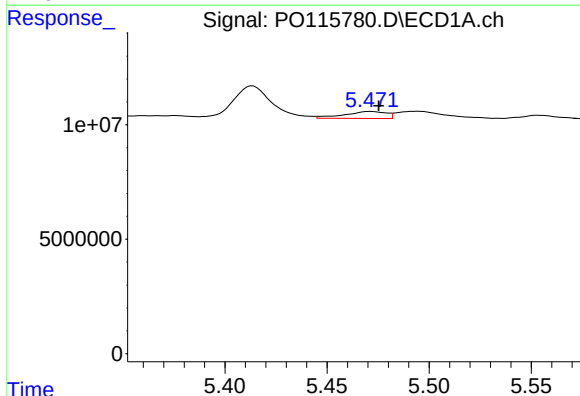


#16 AR-1242-1

R.T.: 5.471 min
Delta R.T.: -0.004 min
Response: 4317885
Conc: 21.74 ng/ml

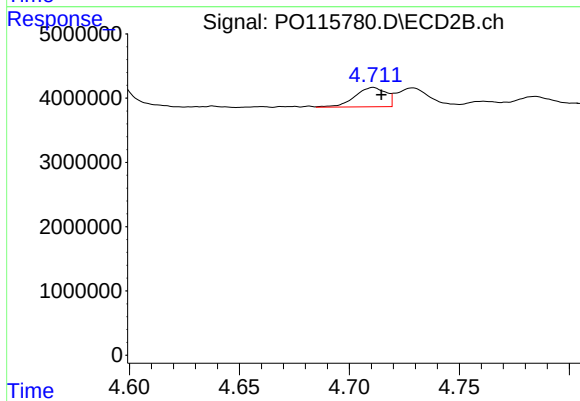

#16 AR-1242-1


R.T.: 4.711 min
Delta R.T.: -0.004 min
Response: 2969023
Conc: 20.85 ng/ml

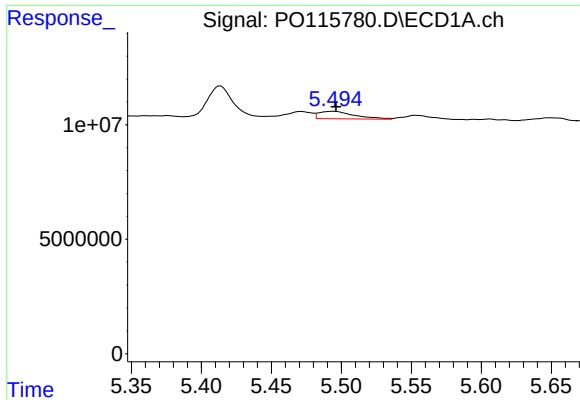

#17 AR-1242-2


R.T.: 5.494 min
Delta R.T.: -0.002 min
Response: 5663678
Conc: 19.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

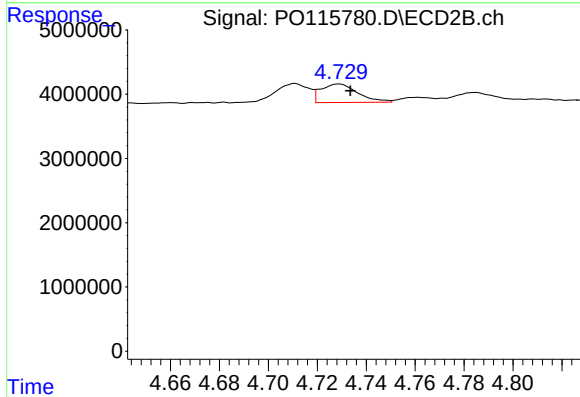


#17 AR-1242-2

R.T.: 4.729 min
Delta R.T.: -0.005 min
Response: 3026494
Conc: 14.46 ng/ml

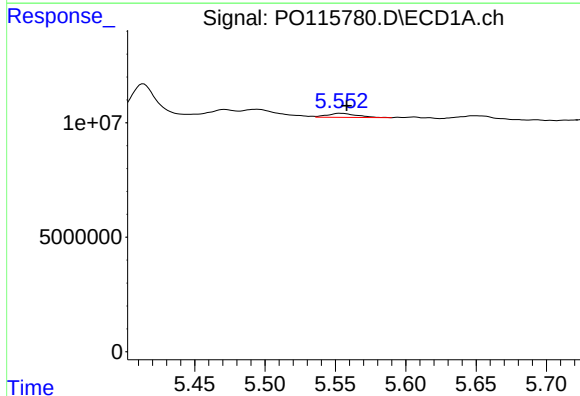


#18 AR-1242-3

R.T.: 5.554 min
Delta R.T.: -0.005 min
Response: 2553060
Conc: 15.12 ng/ml

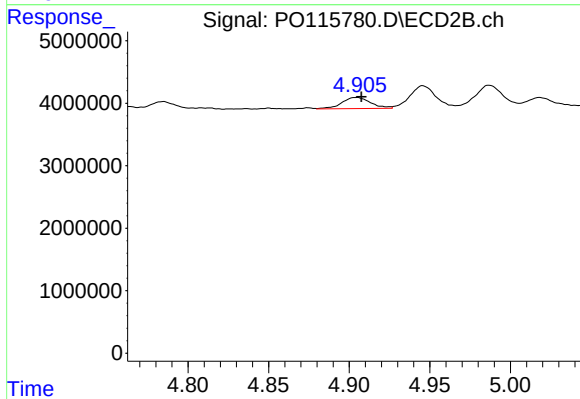

#18 AR-1242-3


R.T.: 4.905 min
Delta R.T.: -0.003 min
Response: 2213357
Conc: 18.53 ng/ml

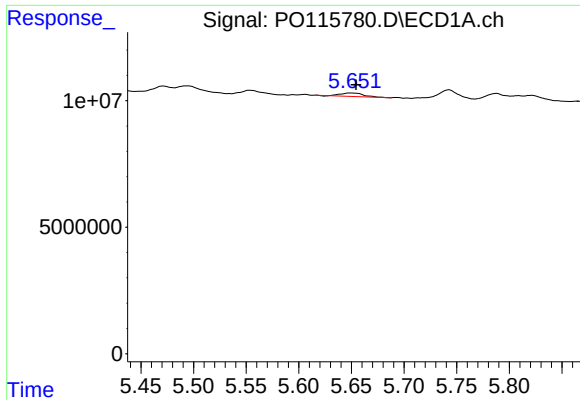

#19 AR-1242-4


R.T.: 5.648 min
Delta R.T.: -0.006 min
Response: 1999330
Conc: 14.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

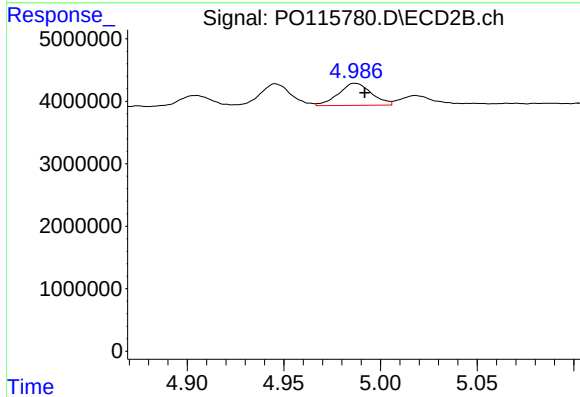


#19 AR-1242-4

R.T.: 4.987 min
Delta R.T.: -0.005 min
Response: 4192631
Conc: 38.43 ng/ml

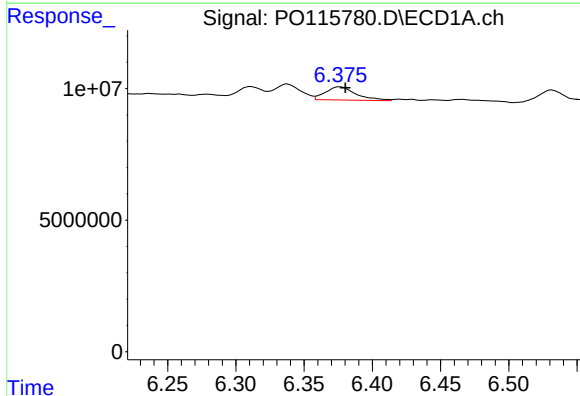


#20 AR-1242-5

R.T.: 6.376 min
Delta R.T.: -0.004 min
Response: 7943356
Conc: 52.45 ng/ml

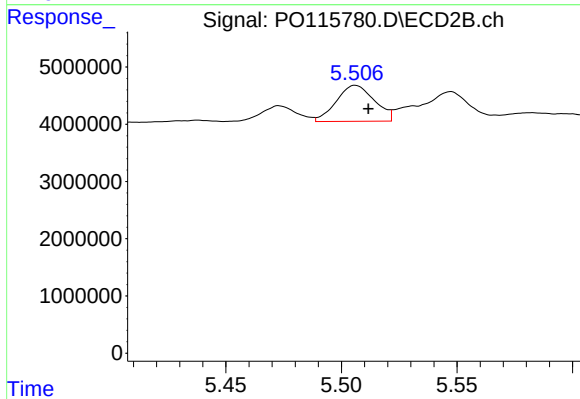

#20 AR-1242-5


R.T.: 5.506 min
Delta R.T.: -0.006 min
Response: 7219479
Conc: 52.27 ng/ml

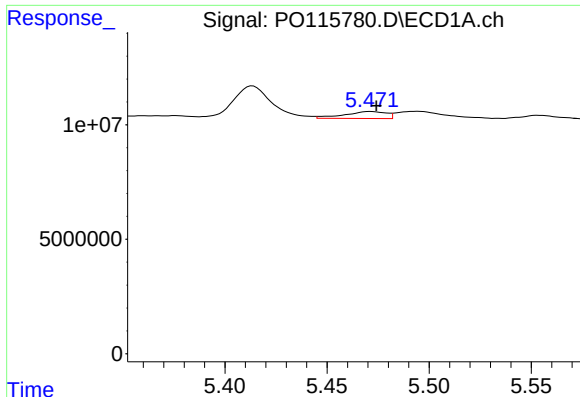

#21 AR-1248-1


R.T.: 5.471 min
Delta R.T.: -0.003 min
Response: 4317885
Conc: 28.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

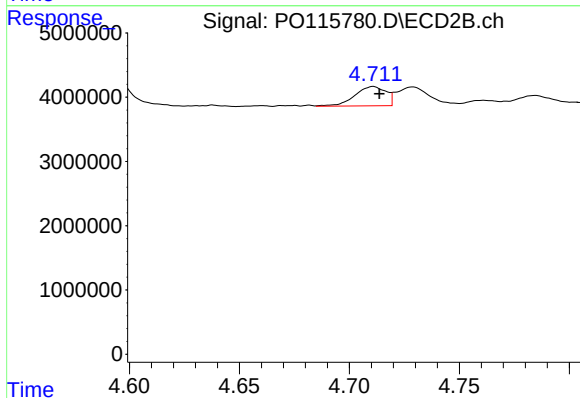


#21 AR-1248-1

R.T.: 4.711 min
Delta R.T.: -0.003 min
Response: 2969023
Conc: 26.55 ng/ml

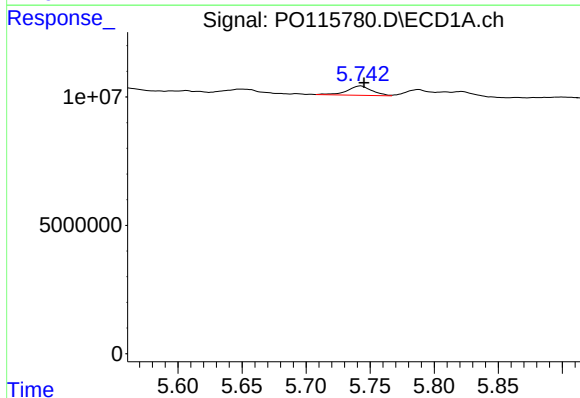


#22 AR-1248-2

R.T.: 5.743 min
Delta R.T.: -0.002 min
Response: 4917962
Conc: 24.49 ng/ml

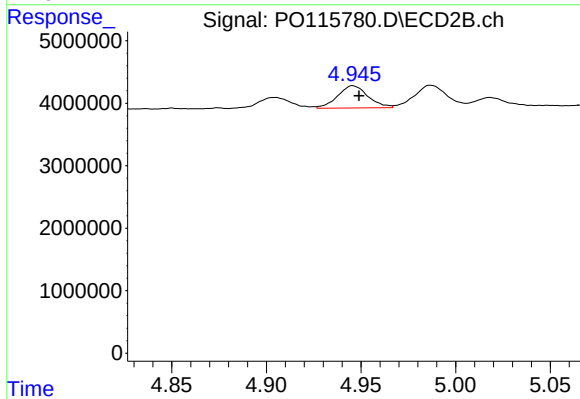

#22 AR-1248-2


R.T.: 4.946 min
Delta R.T.: -0.003 min
Response: 3946559
Conc: 25.91 ng/ml

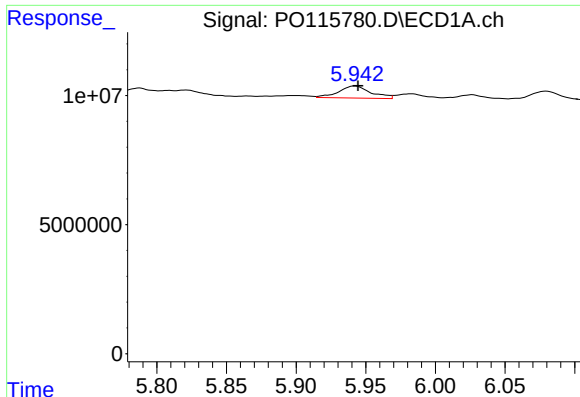

#23 AR-1248-3


R.T.: 5.942 min
Delta R.T.: -0.002 min
Response: 7550493
Conc: 30.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

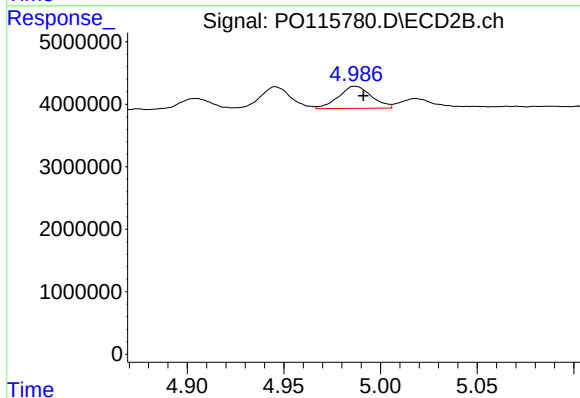


#23 AR-1248-3

R.T.: 4.987 min
Delta R.T.: -0.004 min
Response: 4192631
Conc: 26.12 ng/ml

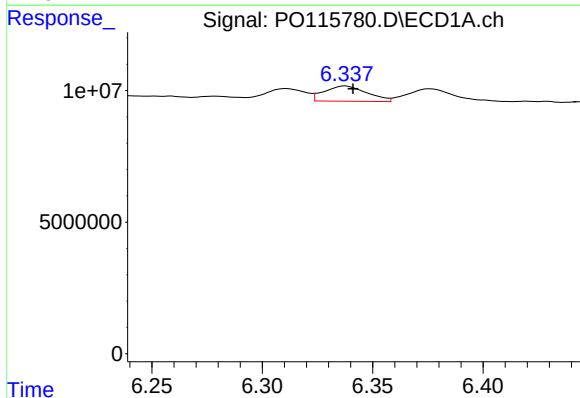


#24 AR-1248-4

R.T.: 6.338 min
Delta R.T.: -0.003 min
Response: 7835137
Conc: 26.57 ng/ml

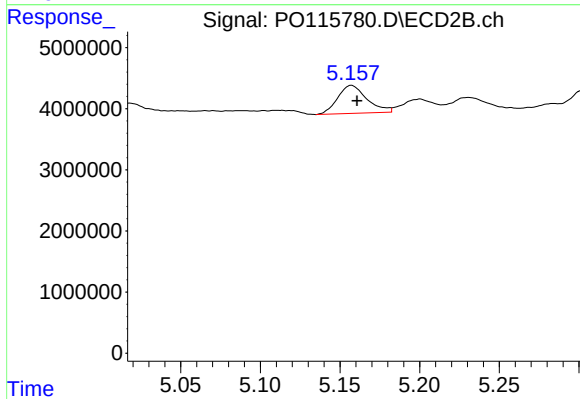

#24 AR-1248-4


R.T.: 5.157 min
Delta R.T.: -0.004 min
Response: 5900302
Conc: 31.53 ng/ml

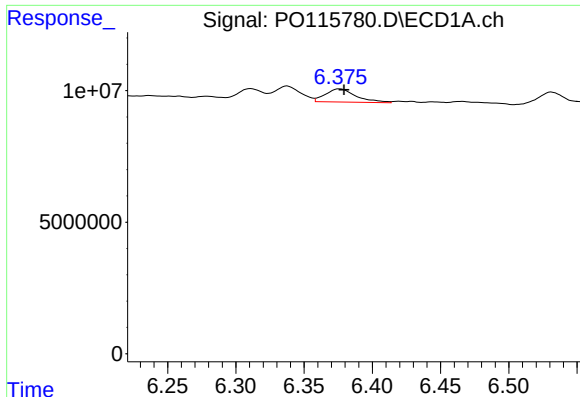

#25 AR-1248-5


R.T.: 6.376 min
Delta R.T.: -0.003 min
Response: 7943356
Conc: 30.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

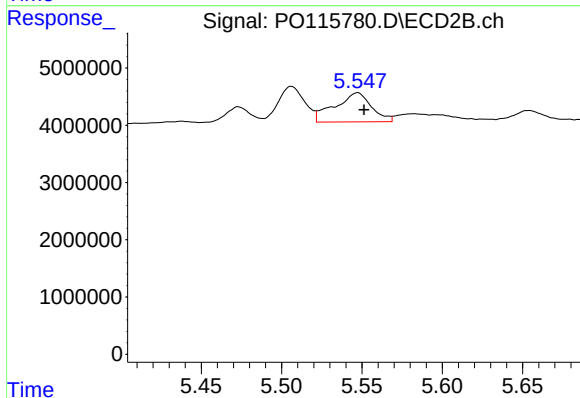


#25 AR-1248-5

R.T.: 5.548 min
Delta R.T.: -0.004 min
Response: 8092730
Conc: 40.88 ng/ml

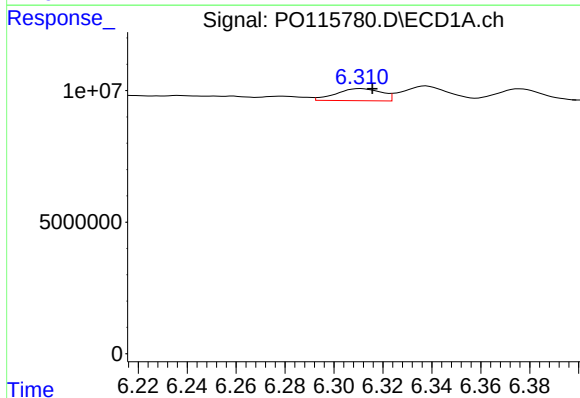


#26 AR-1254-1

R.T.: 6.311 min
Delta R.T.: -0.005 min
Response: 5928331
Conc: 22.91 ng/ml

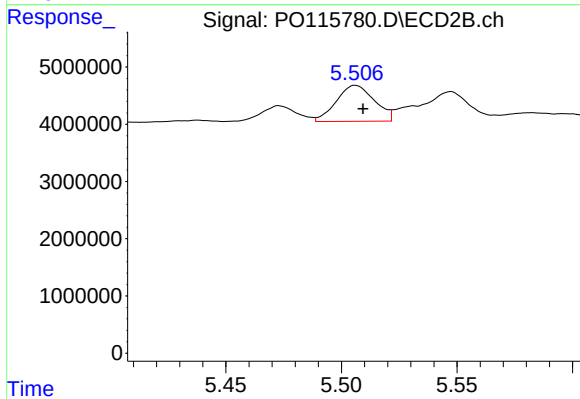

#26 AR-1254-1


R.T.: 5.506 min
Delta R.T.: -0.003 min
Response: 7219479
Conc: 24.70 ng/ml

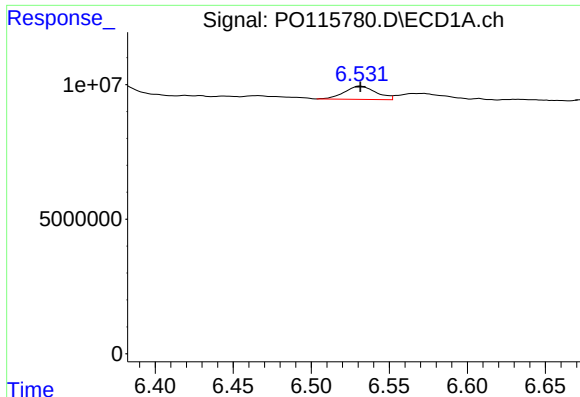

#27 AR-1254-2


R.T.: 6.531 min
Delta R.T.: 0.000 min
Response: 6977794
Conc: 17.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

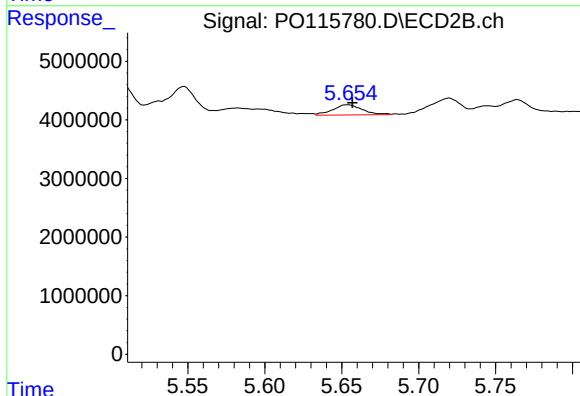


#27 AR-1254-2

R.T.: 5.654 min
Delta R.T.: -0.003 min
Response: 2327079
Conc: 9.24 ng/ml

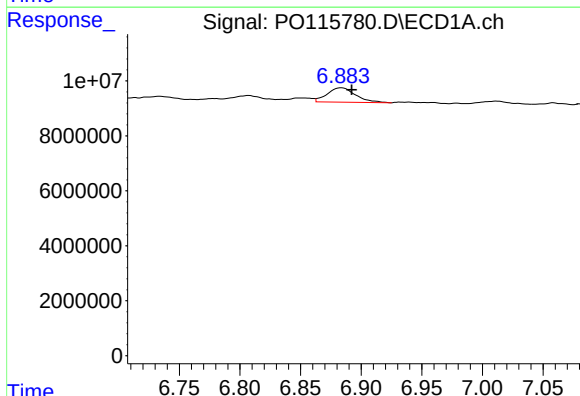


#28 AR-1254-3

R.T.: 6.884 min
Delta R.T.: -0.009 min
Response: 8541494
Conc: 20.80 ng/ml

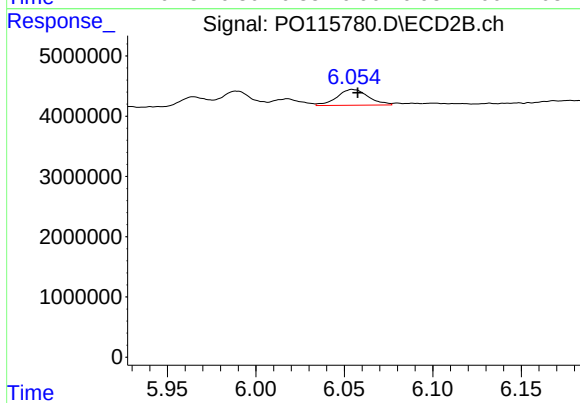

#28 AR-1254-3


R.T.: 6.054 min
Delta R.T.: -0.003 min
Response: 3242614
Conc: 8.24 ng/ml

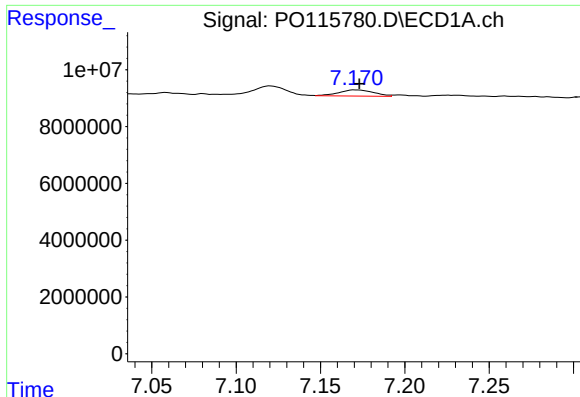

#29 AR-1254-4


R.T.: 7.171 min
Delta R.T.: -0.002 min
Response: 3163955
Conc: 9.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

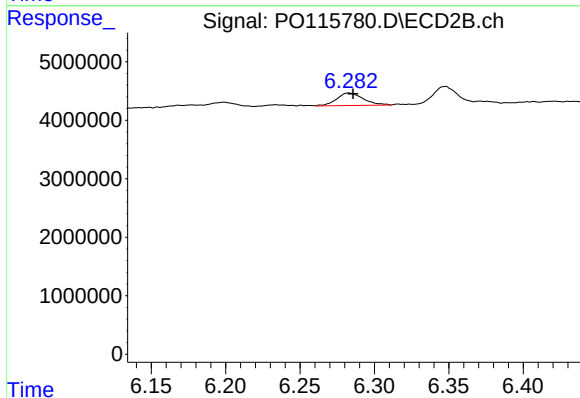


#29 AR-1254-4

R.T.: 6.283 min
Delta R.T.: -0.003 min
Response: 2664838
Conc: 9.96 ng/ml

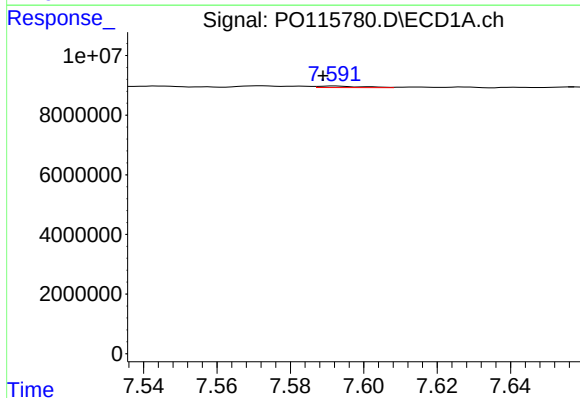


#30 AR-1254-5

R.T.: 7.592 min
Delta R.T.: 0.003 min
Response: 395392
Conc: 1.22 ng/ml

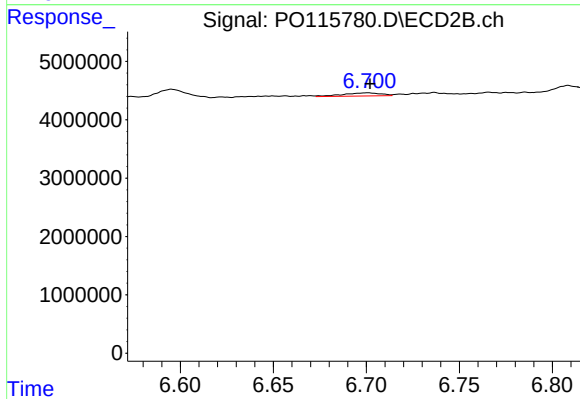

#30 AR-1254-5


R.T.: 6.701 min
Delta R.T.: -0.001 min
Response: 746883
Conc: 2.09 ng/ml

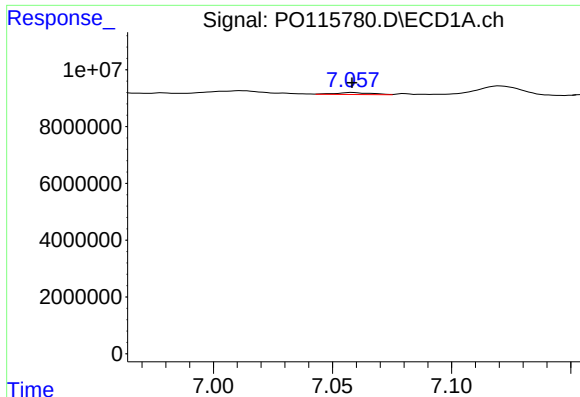

#31 AR-1260-1


R.T.: 7.058 min
Delta R.T.: 0.000 min
Response: 759509
Conc: 2.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

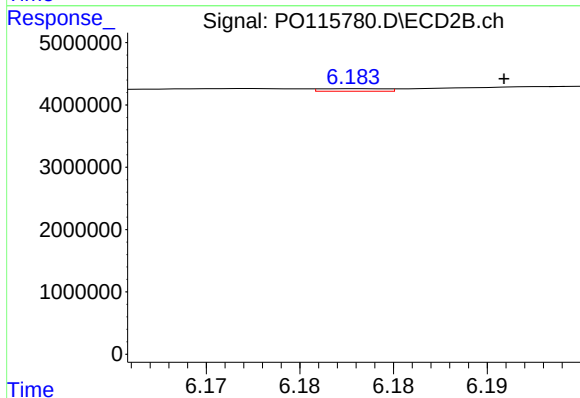


#31 AR-1260-1

R.T.: 6.183 min
Delta R.T.: -0.008 min
Response: 97923
Conc: 0.37 ng/ml

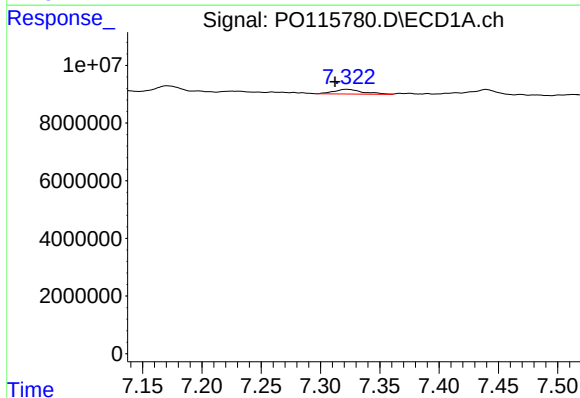


#32 AR-1260-2

R.T.: 7.322 min
Delta R.T.: 0.010 min
Response: 2813686
Conc: 6.43 ng/ml

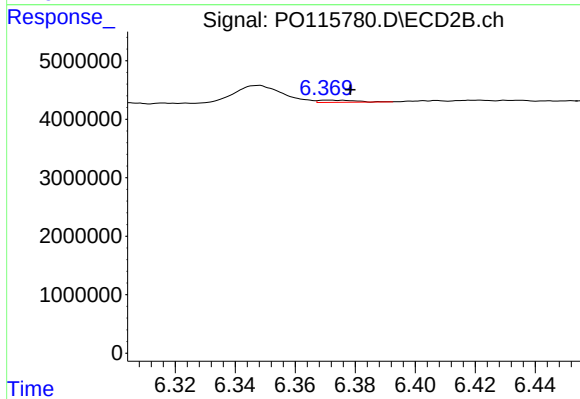

#32 AR-1260-2


R.T.: 6.370 min
Delta R.T.: -0.008 min
Response: 302771
Conc: 0.86 ng/ml

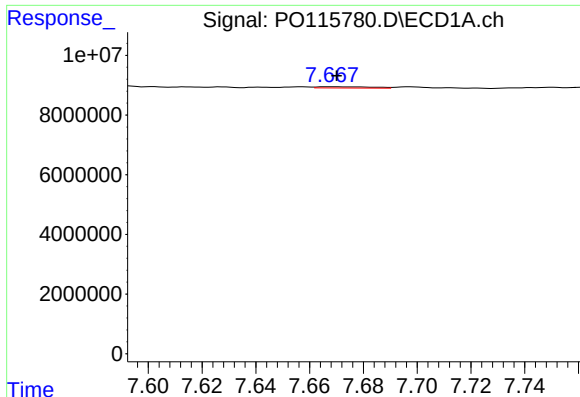

#33 AR-1260-3


R.T.: 7.668 min
Delta R.T.: -0.002 min
Response: 582970
Conc: 1.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

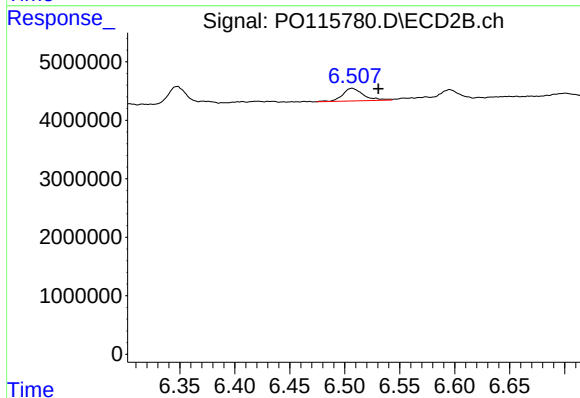


#33 AR-1260-3

R.T.: 6.507 min
Delta R.T.: -0.024 min
Response: 2885905
Conc: 8.98 ng/ml

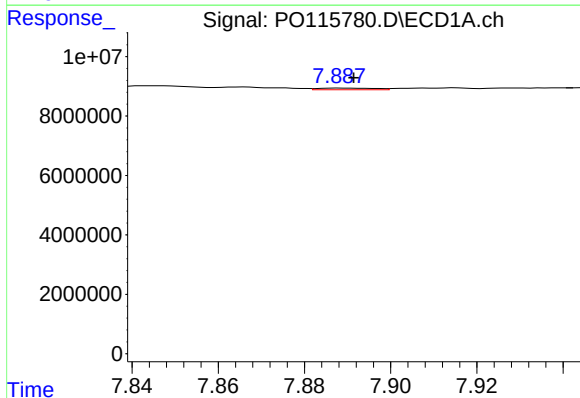


#34 AR-1260-4

R.T.: 7.888 min
Delta R.T.: -0.003 min
Response: 532352
Conc: 1.73 ng/ml

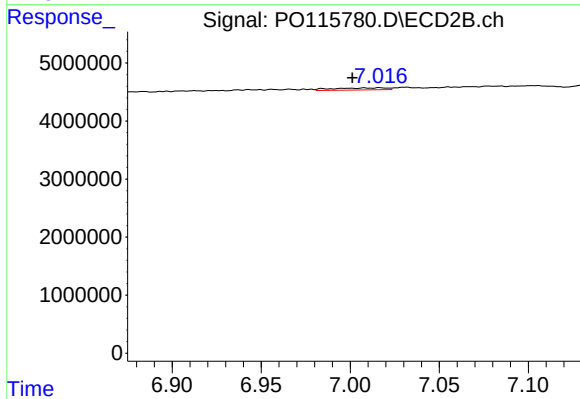

#34 AR-1260-4


R.T.: 7.017 min
Delta R.T.: 0.015 min
Response: 730878
Conc: 2.85 ng/ml

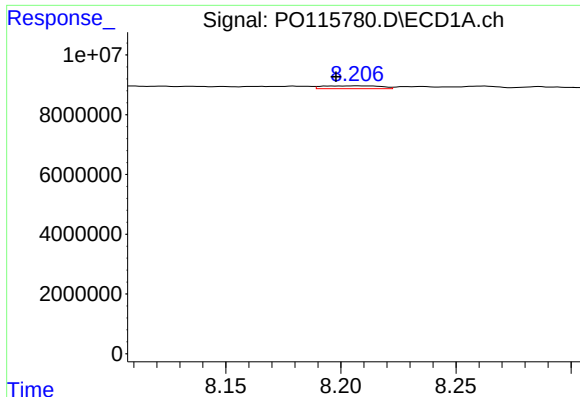

#35 AR-1260-5


R.T.: 8.207 min
Delta R.T.: 0.009 min
Response: 1696329
Conc: 2.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

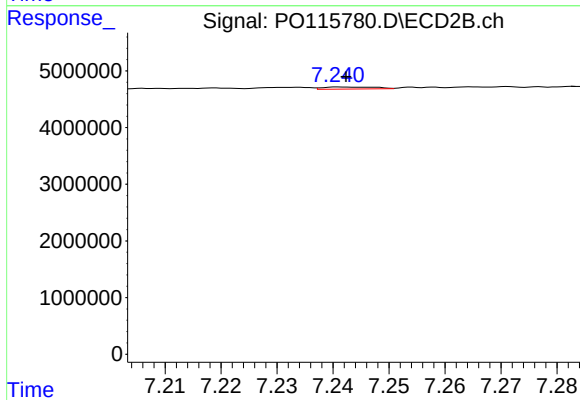


#35 AR-1260-5

R.T.: 7.242 min
Delta R.T.: 0.000 min
Response: 237324
Conc: 0.34 ng/ml

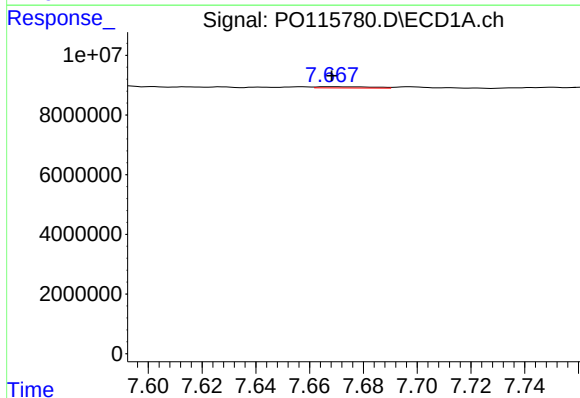


#36 AR-1262-1

R.T.: 7.668 min
Delta R.T.: 0.000 min
Response: 582970
Conc: 2.36 ng/ml

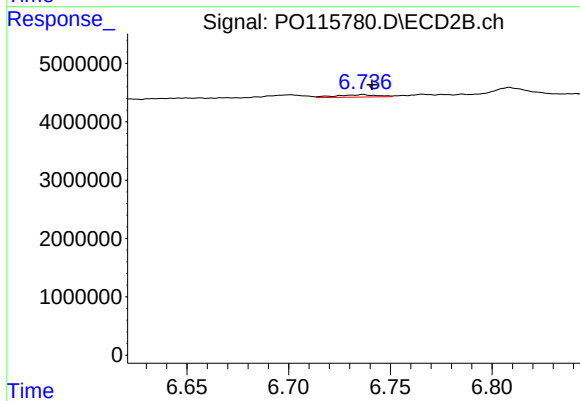

#36 AR-1262-1


R.T.: 6.737 min
Delta R.T.: -0.004 min
Response: 578035
Conc: 2.71 ng/ml

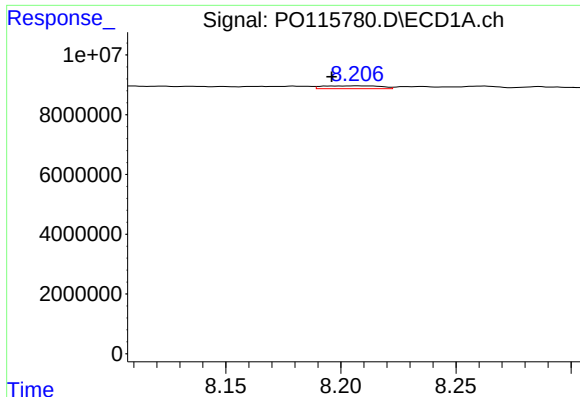

#37 AR-1262-2


R.T.: 8.207 min
Delta R.T.: 0.011 min
Response: 1696329
Conc: 4.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

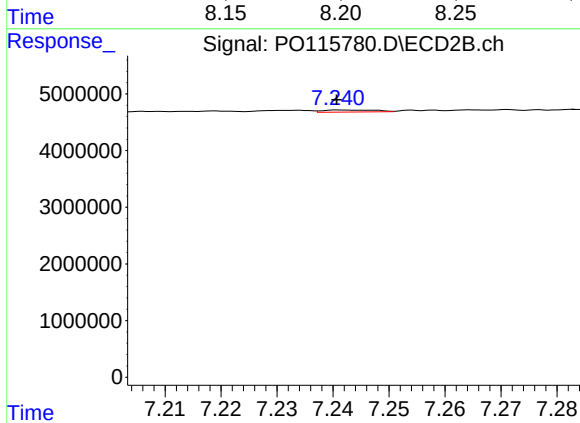


#37 AR-1262-2

R.T.: 7.242 min
Delta R.T.: 0.001 min
Response: 237324
Conc: 0.68 ng/ml

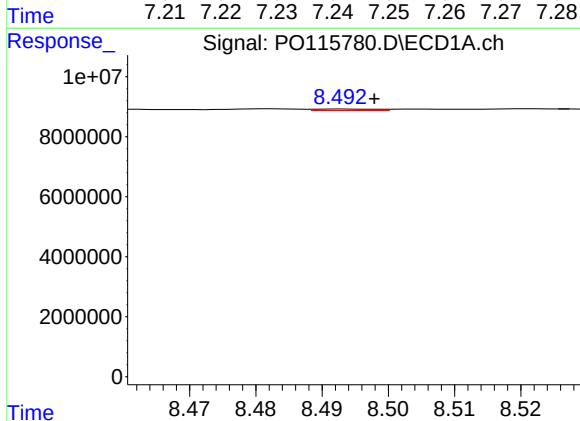


#38 AR-1262-3

R.T.: 8.493 min
Delta R.T.: -0.005 min
Response: 332732
Conc: 1.31 ng/ml

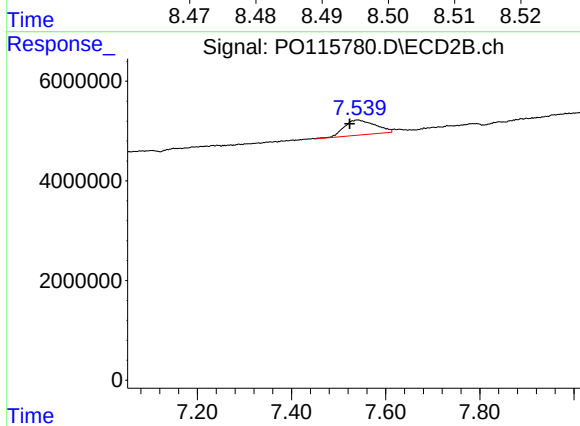

#38 AR-1262-3


R.T.: 7.539 min
Delta R.T.: 0.016 min
Response: 13838370
Conc: 88.49 ng/ml

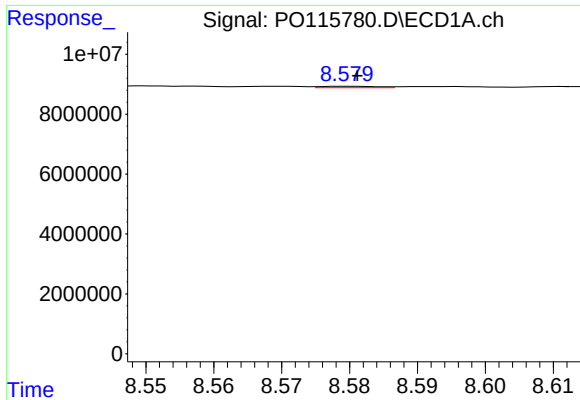

#39 AR-1262-4


R.T.: 8.580 min
Delta R.T.: -0.001 min
Response: 278634
Conc: 1.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

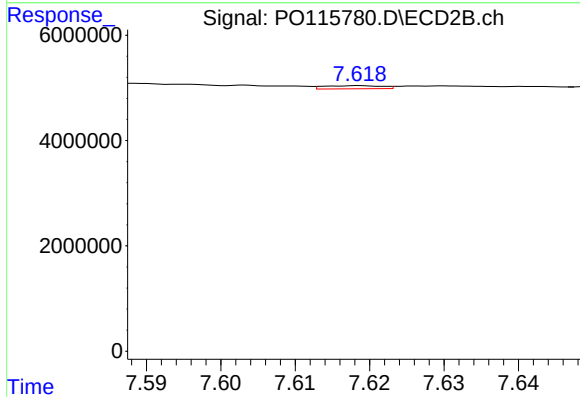


#39 AR-1262-4

R.T.: 7.619 min
Delta R.T.: 0.031 min
Response: 320337
Conc: 1.29 ng/ml

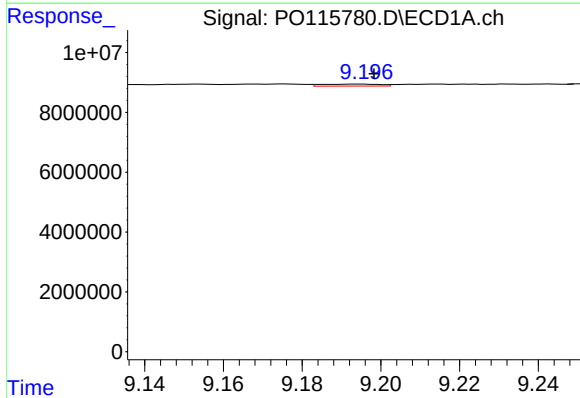


#40 AR-1262-5

R.T.: 9.195 min
Delta R.T.: -0.004 min
Response: 694963
Conc: 5.16 ng/ml

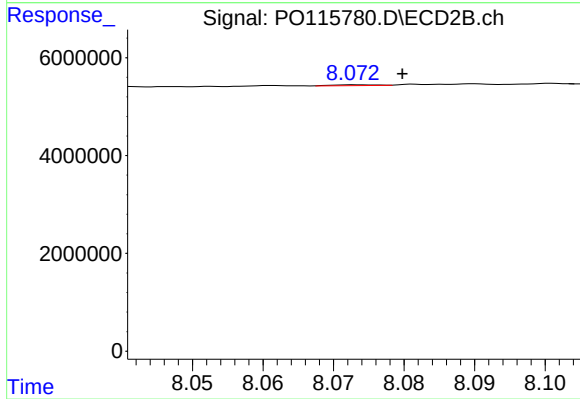

#40 AR-1262-5


R.T.: 8.074 min
Delta R.T.: -0.006 min
Response: 72551
Conc: 0.65 ng/ml

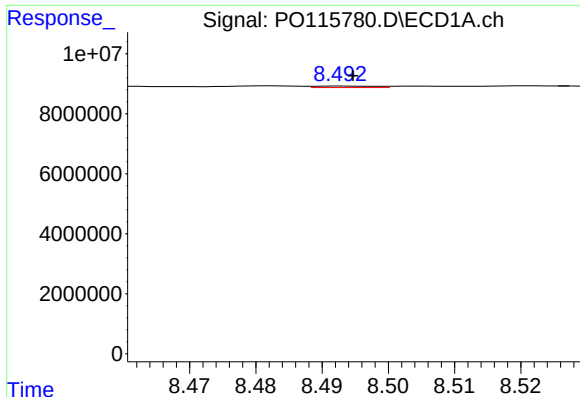

#41 AR-1268-1


R.T.: 8.493 min
Delta R.T.: -0.002 min
Response: 332732
Conc: 0.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

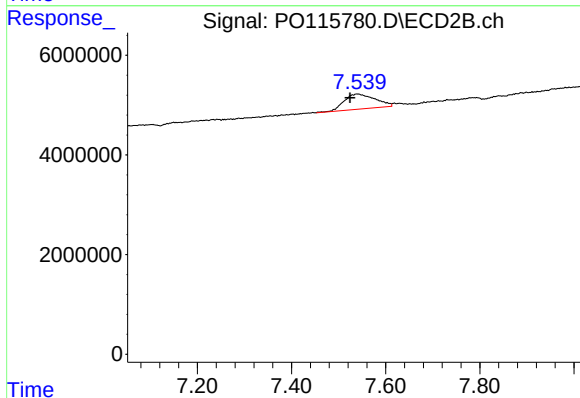


#41 AR-1268-1

R.T.: 7.539 min
Delta R.T.: 0.015 min
Response: 13838370
Conc: 15.62 ng/ml

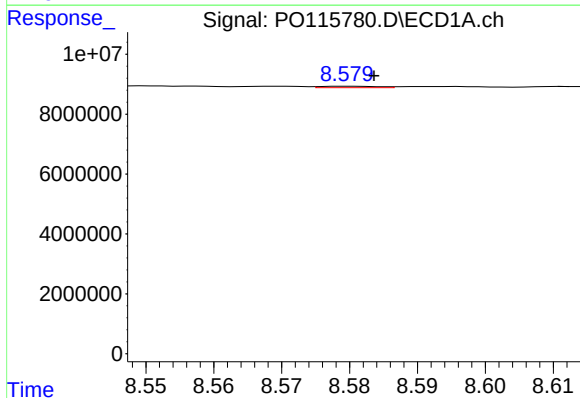


#42 AR-1268-2

R.T.: 8.580 min
Delta R.T.: -0.004 min
Response: 278634
Conc: 0.33 ng/ml

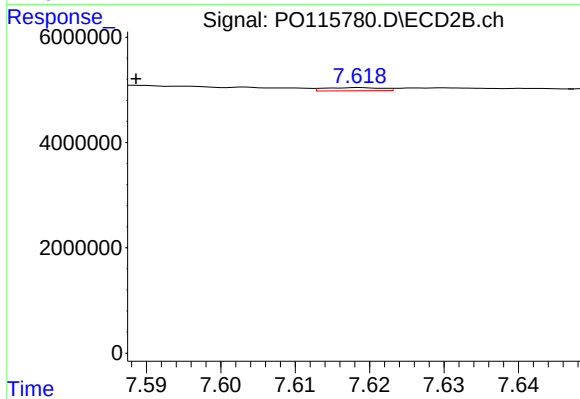

#42 AR-1268-2


R.T.: 7.619 min
Delta R.T.: 0.030 min
Response: 320337
Conc: 0.43 ng/ml

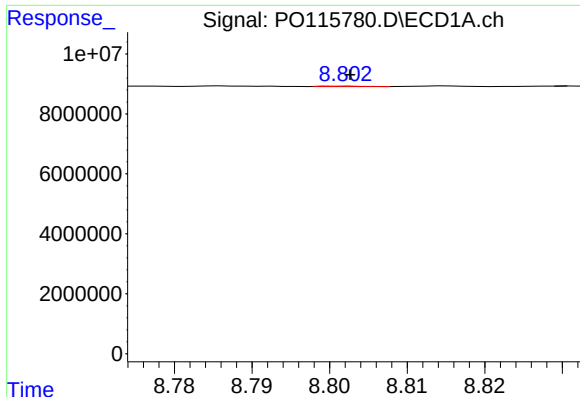

#43 AR-1268-3


R.T.: 8.801 min
Delta R.T.: -0.001 min
Response: 52935
Conc: 0.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

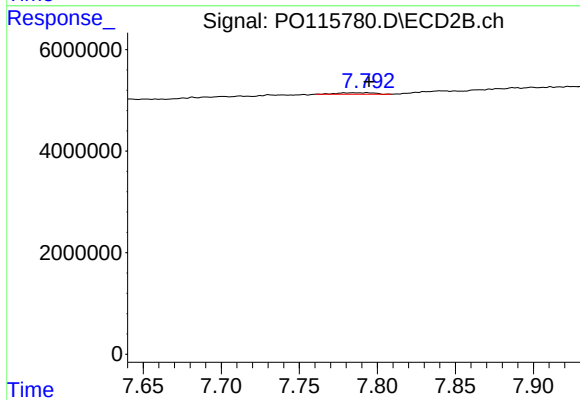


#43 AR-1268-3

R.T.: 7.779 min
Delta R.T.: -0.016 min
Response: 467034
Conc: 0.73 ng/ml

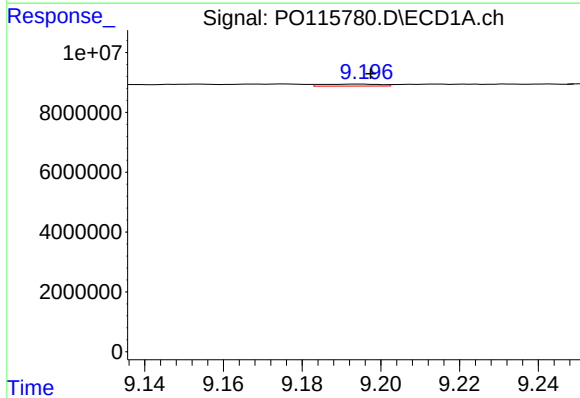


#44 AR-1268-4

R.T.: 9.195 min
Delta R.T.: -0.003 min
Response: 694963
Conc: 2.23 ng/ml

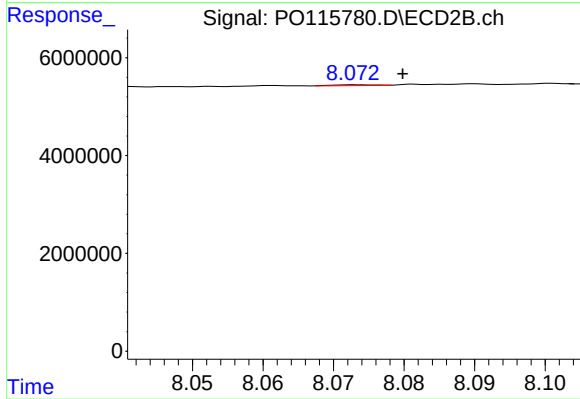

#44 AR-1268-4


R.T.: 8.074 min
Delta R.T.: -0.006 min
Response: 72551
Conc: 0.28 ng/ml

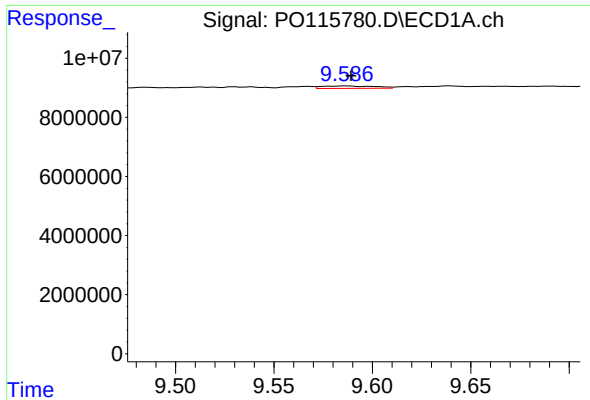

#45 AR-1268-5

R.T.: 9.587 min
Delta R.T.: -0.003 min
Response: 1510891
Conc: 0.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

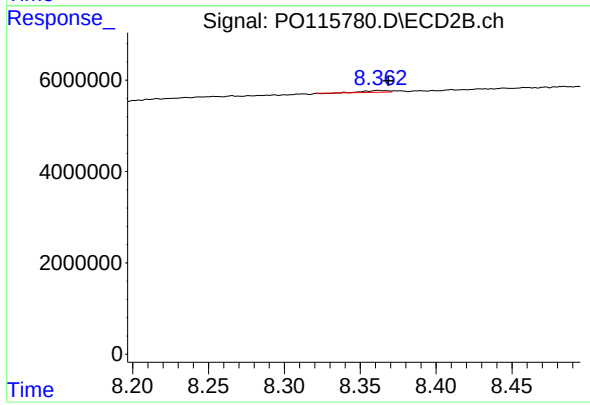

#45 AR-1268-5

R.T.: 8.362 min
Delta R.T.: -0.006 min
Response: 365994
Conc: 0.22 ng/ml