

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO121225\
 Data File : PO115781.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Dec 2025 03:10
 Operator : YP/AJ
 Sample : Q3530-07
 Misc : AR1254 25PPB WATER LOD
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 00:56:31 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO120425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 05 02:11:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.334	3.637	174.8E6	106.2E6	22.500	21.790
2)	SA Decachlor...	9.906	8.615	123.2E6	93431455	23.414	21.727
Target Compounds							
3)	L1 AR-1016-1	5.478	4.717	533725	485010	2.146	2.625
4)	L1 AR-1016-2	5.490	4.739	828359	96088	2.175	0.364 #
5)	L1 AR-1016-3	5.555	4.907	825683	254864	3.862	1.684 #
6)	L1 AR-1016-4	5.651	4.945	23846	3354936	0.134	29.768 #
7)	L1 AR-1016-5	5.942	5.157	3526856	3602012	20.104	24.614
8)	L2 AR-1221-1	4.530	3.868	7681252	770787	94.600	13.665 #
9)	L2 AR-1221-2	4.630	3.934	3546737	2618464	56.281	61.693
10)	L2 AR-1221-3	4.695	4.004	1905784	48968	10.207	0.381 #
11)	L3 AR-1232-1	4.695	4.004	1905784	48968	12.734	0.458 #
12)	L3 AR-1232-2	5.222	4.739	816605	96088	10.100	0.866 #
13)	L3 AR-1232-3	5.503	4.907	1056155	254864	6.862	3.899 #
14)	L3 AR-1232-4	5.651	4.987	23846	1239123	0.341	24.140 #
15)	L3 AR-1232-5	5.742	5.157	4657352	3602012	89.673	65.792 #
16)	L4 AR-1242-1	5.478	4.717	533725	485010	2.687	3.406 #
17)	L4 AR-1242-2	5.490	4.739	828359	96088	2.828	0.459 #
18)	L4 AR-1242-3	5.555	4.907	825683	254864	4.891	2.134 #
19)	L4 AR-1242-4	5.651	4.987	23846	1239123	0.174	11.359 #
20)	L4 AR-1242-5	6.380	5.507	3636333	8077735	24.011	58.481 #
21)	L5 AR-1248-1	5.478	4.717	533725	485010	3.517	4.337
22)	L5 AR-1248-2	5.742	4.945	4657352	3354936	23.192	22.030
23)	L5 AR-1248-3	5.942	4.987	3526856	1239123	14.302	7.719 #
24)	L5 AR-1248-4	6.339	5.157	5202938	3602012	17.646	19.247
25)	L5 AR-1248-5	6.380	5.529	3636333	5518171	14.044	27.876 #
26)	L6 AR-1254-1	6.312	5.507	8597395	8077735	33.231	27.638
27)	L6 AR-1254-2	6.530	5.654	11255010	7370095	27.969	29.268
28)	L6 AR-1254-3	6.886	6.054	19651379	10575036	47.864	26.869 #
29)	L6 AR-1254-4	7.172	6.283	10710500	6967927	30.860	26.041
30)	L6 AR-1254-5	7.588	6.698	7828768	7781511	24.160	21.765
31)	L7 AR-1260-1	7.055	6.184	5242230	5056451	18.095	19.287
32)	L7 AR-1260-2	7.308	6.372	5249970	4472167	11.994	12.761
33)	L7 AR-1260-3	7.663	6.523	504070	5320686	1.498	16.561 #
34)	L7 AR-1260-4	7.870	6.998	3851616	386247	12.527	1.504 #
35)	L7 AR-1260-5	8.194	7.238	2134315	1188429	2.930	1.695 #
36)	L8 AR-1262-1	7.663	6.754	504070	125911	2.042	0.591 #
37)	L8 AR-1262-2	8.194	7.238	2134315	1188429	5.391	3.412 #
38)	L8 AR-1262-3	8.504	7.535	1496252	9846623	5.872	62.962 #
39)	L8 AR-1262-4	8.593	7.573	475607	7286089	2.455	29.454 #
40)	L8 AR-1262-5	9.202	8.083	1477656	186416	10.971	1.672 #
41)	L9 AR-1268-1	8.504	7.535	1496252	9846623	1.503	11.114 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO121225\
 Data File : PO115781.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Dec 2025 03:10
 Operator : YP/AJ
 Sample : Q3530-07
 Misc : AR1254 25PPB WATER LOD
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 00:56:31 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO120425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 05 02:11:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.593	7.573	475607	7286089	0.556	9.727 #
43) L9	AR-1268-3	8.803	7.789	157662	1070286	0.212	1.681 #
44) L9	AR-1268-4	9.202	8.083	1477656	186416	4.733	0.724 #
45) L9	AR-1268-5	9.588	8.368	1535328	613238	0.705	0.364 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121225\
Data File : PO115781.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Dec 2025 03:10
Operator : YP/AJ
Sample : Q3530-07
Misc : AR1254 25PPB WATER LOD
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 00:56:31 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120425.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 05 02:11:05 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

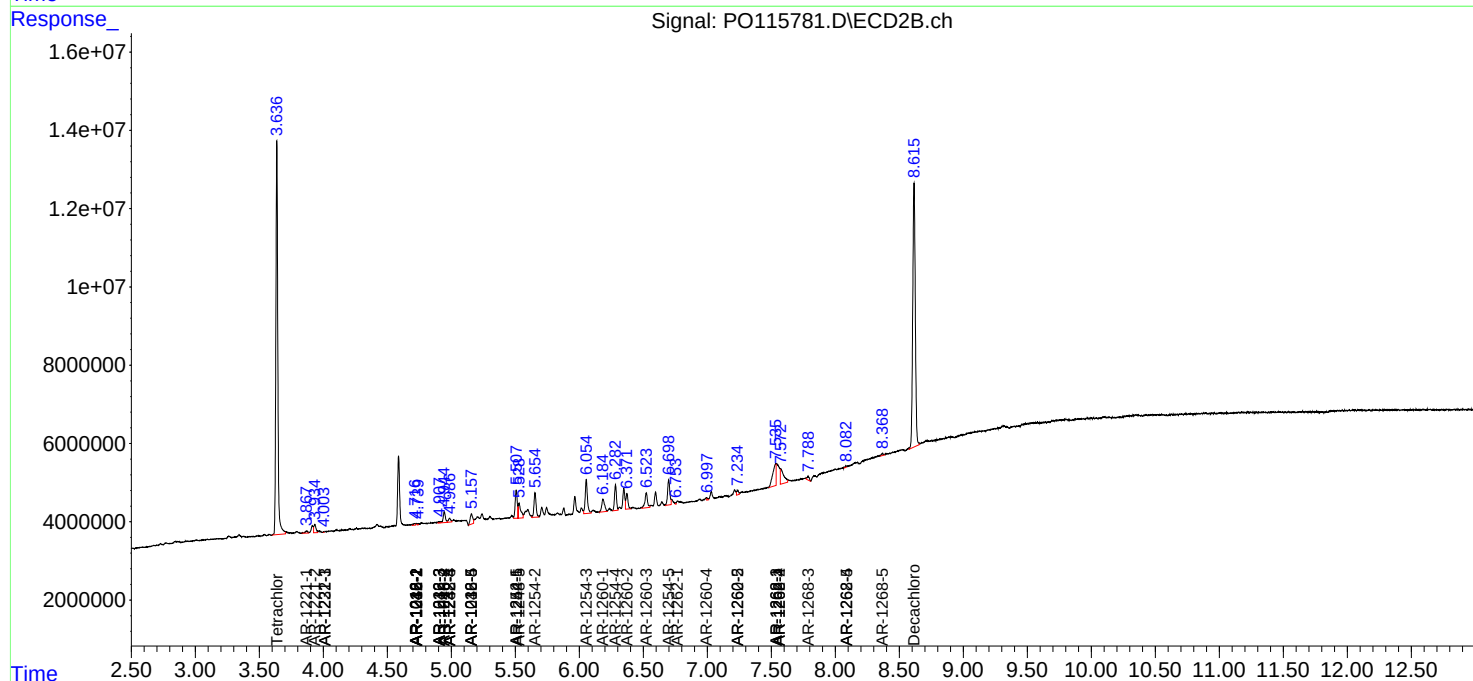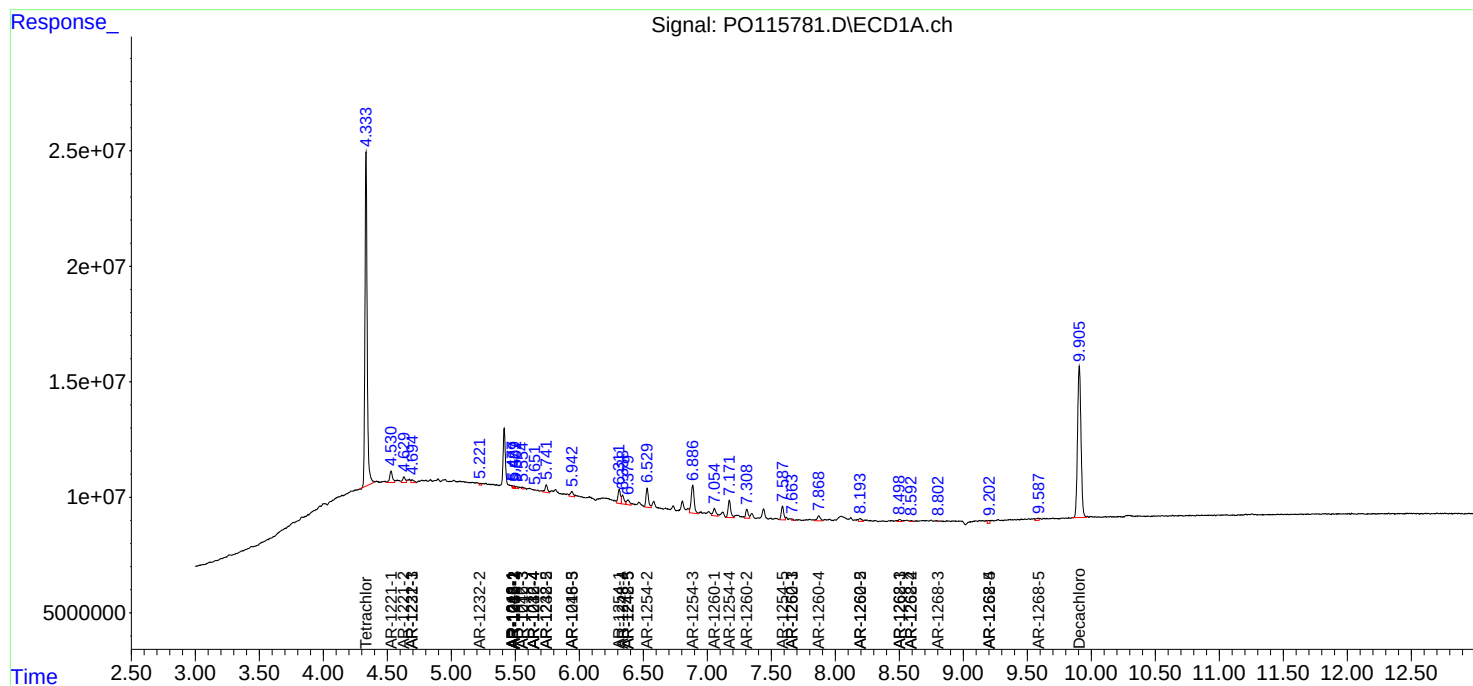


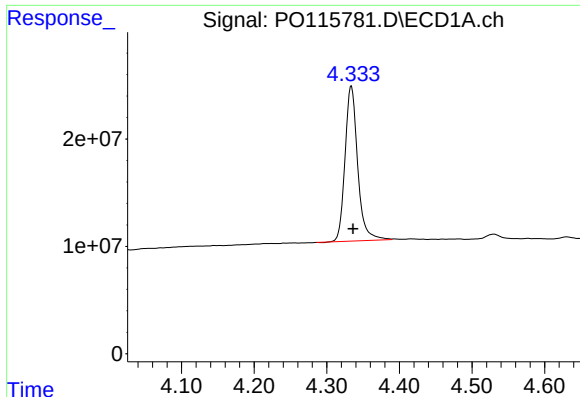

#1 Tetrachloro-m-xylene


R.T.: 4.334 min
Delta R.T.: -0.002 min
Response: 174761101
Conc: 22.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

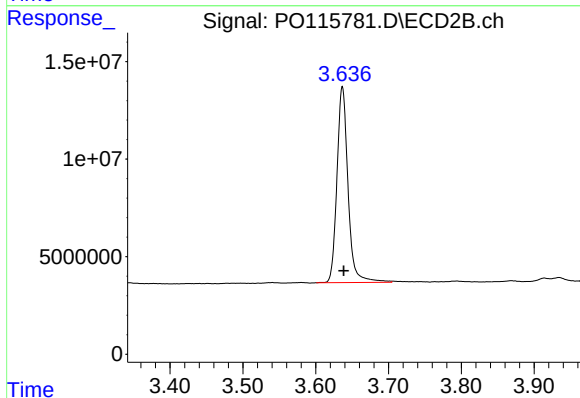


#1 Tetrachloro-m-xylene

R.T.: 3.637 min
Delta R.T.: -0.002 min
Response: 106190145
Conc: 21.79 ng/ml

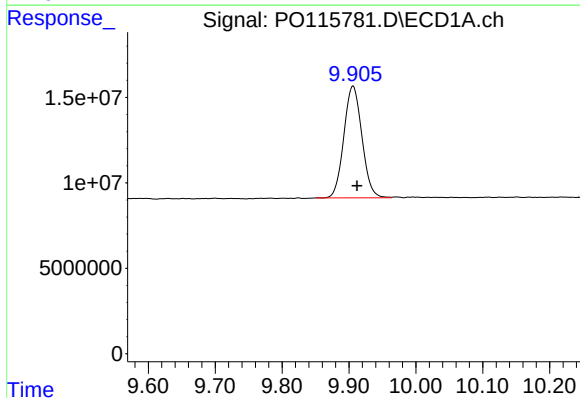


#2 Decachlorobiphenyl

R.T.: 9.906 min
Delta R.T.: -0.006 min
Response: 123183472
Conc: 23.41 ng/ml

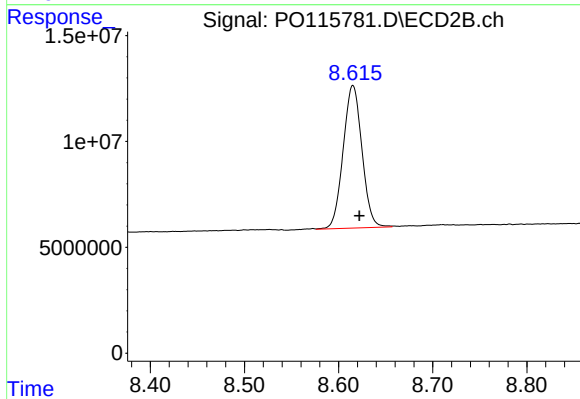

#2 Decachlorobiphenyl


R.T.: 8.615 min
Delta R.T.: -0.007 min
Response: 93431455
Conc: 21.73 ng/ml

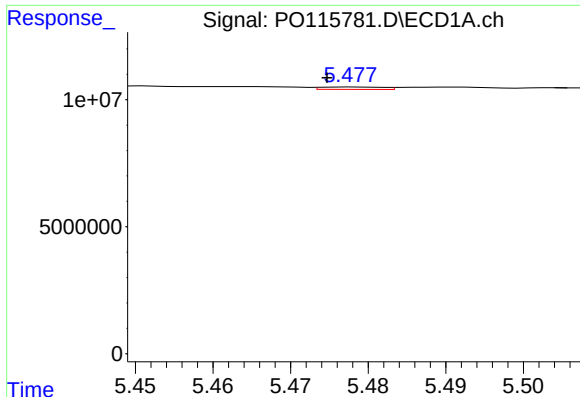

#3 AR-1016-1


R.T.: 5.478 min
Delta R.T.: 0.003 min
Response: 533725
Conc: 2.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

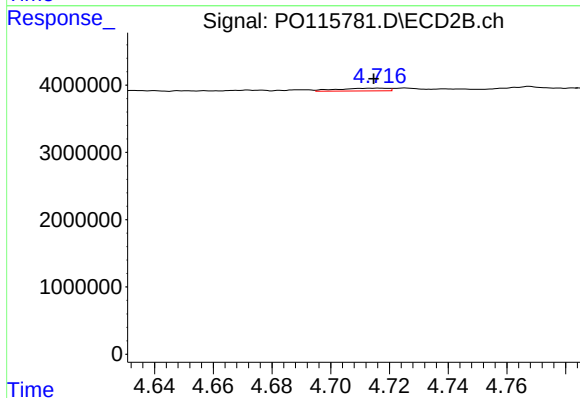


#3 AR-1016-1

R.T.: 4.717 min
Delta R.T.: 0.002 min
Response: 485010
Conc: 2.63 ng/ml

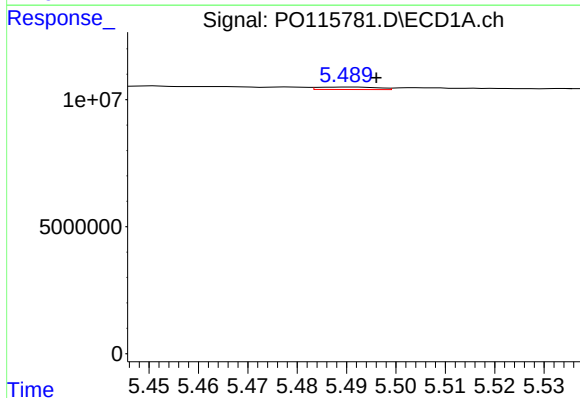


#4 AR-1016-2

R.T.: 5.490 min
Delta R.T.: -0.006 min
Response: 828359
Conc: 2.18 ng/ml

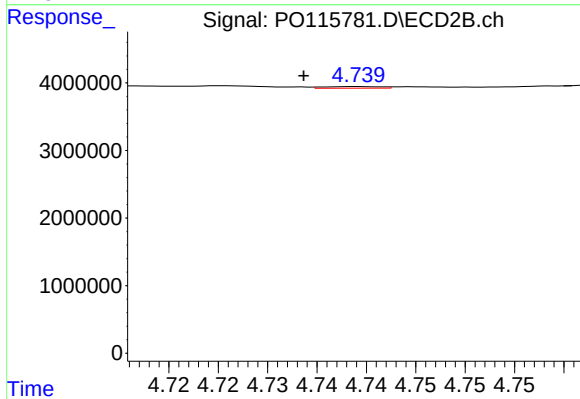

#4 AR-1016-2


R.T.: 4.739 min
Delta R.T.: 0.005 min
Response: 96088
Conc: 0.36 ng/ml

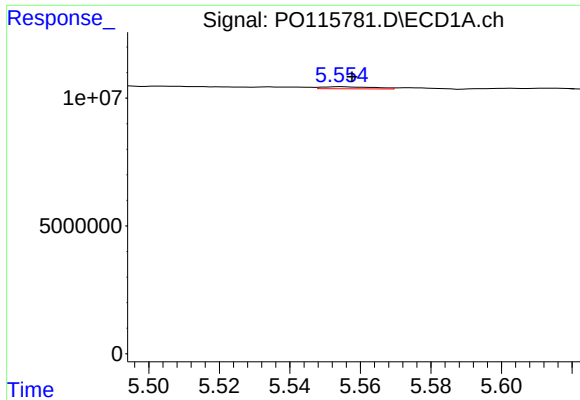

#5 AR-1016-3


R.T.: 5.555 min
Delta R.T.: -0.003 min
Response: 825683
Conc: 3.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

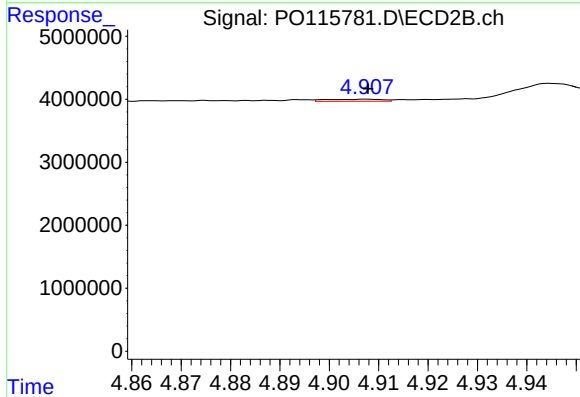


#5 AR-1016-3

R.T.: 4.907 min
Delta R.T.: 0.000 min
Response: 254864
Conc: 1.68 ng/ml

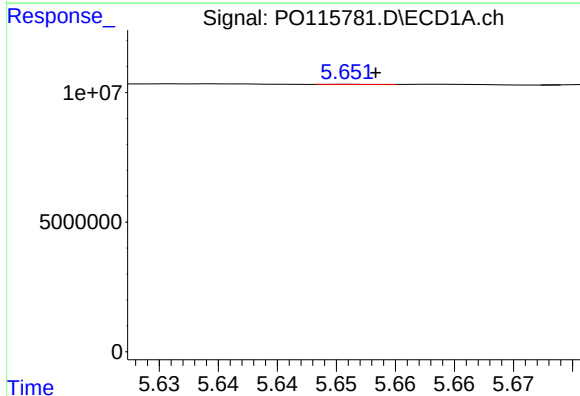


#6 AR-1016-4

R.T.: 5.651 min
Delta R.T.: -0.002 min
Response: 23846
Conc: 0.13 ng/ml

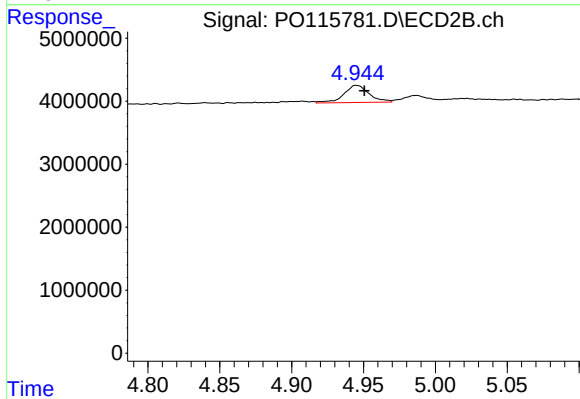

#6 AR-1016-4


R.T.: 4.945 min
Delta R.T.: -0.006 min
Response: 3354936
Conc: 29.77 ng/ml

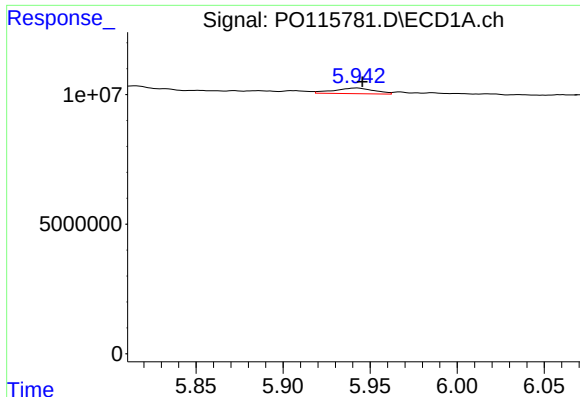

#7 AR-1016-5


R.T.: 5.942 min
Delta R.T.: -0.003 min
Response: 3526856
Conc: 20.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

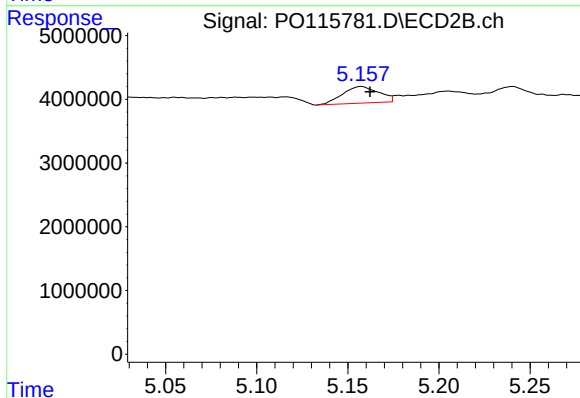


#7 AR-1016-5

R.T.: 5.157 min
Delta R.T.: -0.005 min
Response: 3602012
Conc: 24.61 ng/ml

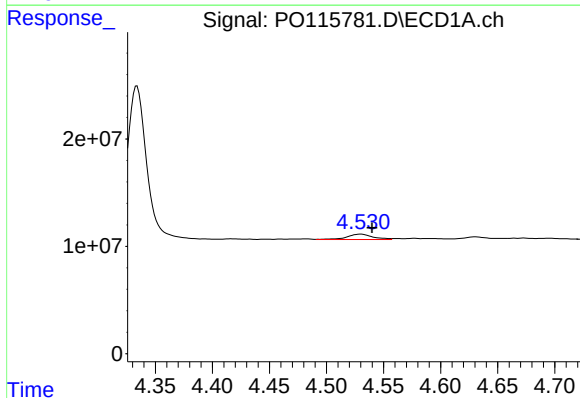


#8 AR-1221-1

R.T.: 4.530 min
Delta R.T.: -0.010 min
Response: 7681252
Conc: 94.60 ng/ml

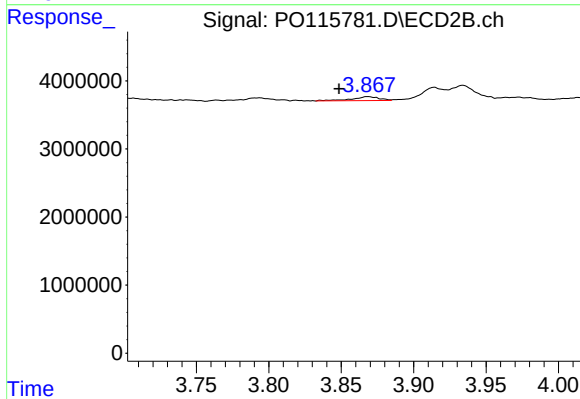

#8 AR-1221-1


R.T.: 3.868 min
Delta R.T.: 0.020 min
Response: 770787
Conc: 13.66 ng/ml

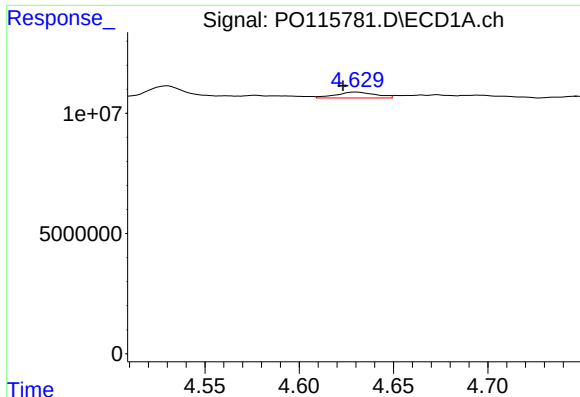

#9 AR-1221-2


R.T.: 4.630 min
Delta R.T.: 0.007 min
Response: 3546737
Conc: 56.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

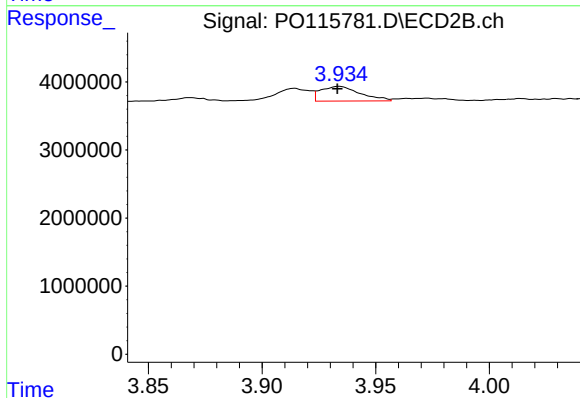


#9 AR-1221-2

R.T.: 3.934 min
Delta R.T.: 0.000 min
Response: 2618464
Conc: 61.69 ng/ml

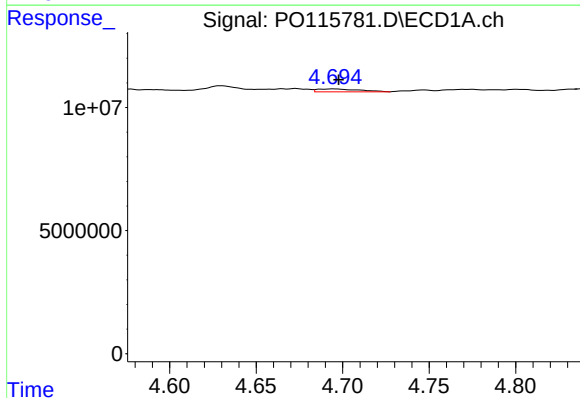


#10 AR-1221-3

R.T.: 4.695 min
Delta R.T.: -0.003 min
Response: 1905784
Conc: 10.21 ng/ml

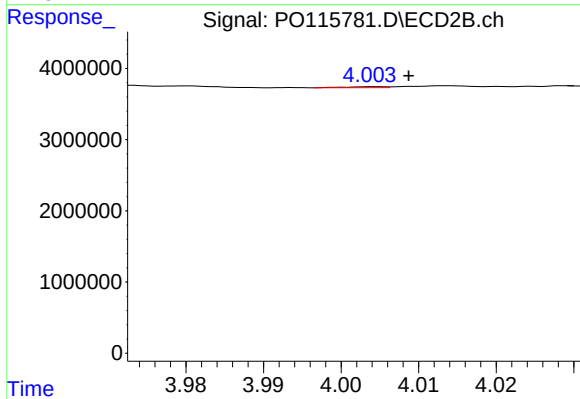

#10 AR-1221-3


R.T.: 4.004 min
Delta R.T.: -0.004 min
Response: 48968
Conc: 0.38 ng/ml

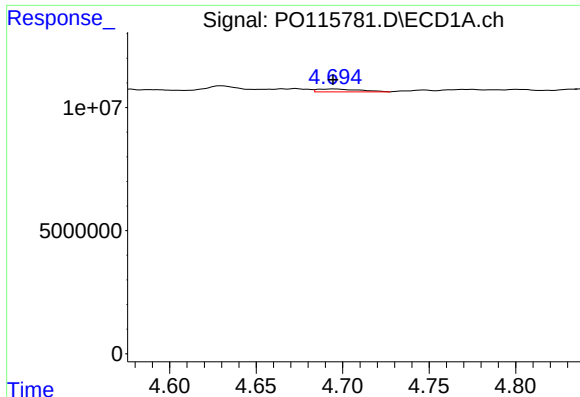

#11 AR-1232-1


R.T.: 4.695 min
Delta R.T.: 0.000 min
Response: 1905784
Conc: 12.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

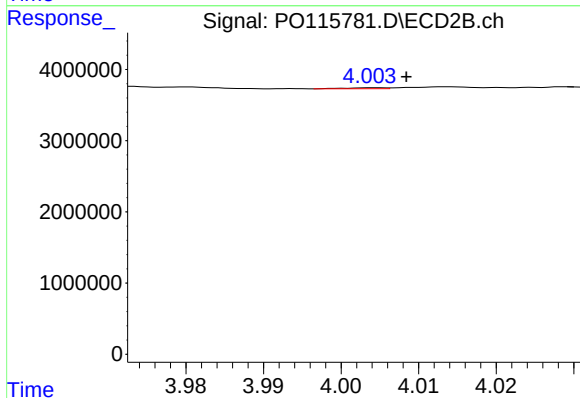


#11 AR-1232-1

R.T.: 4.004 min
Delta R.T.: -0.004 min
Response: 48968
Conc: 0.46 ng/ml

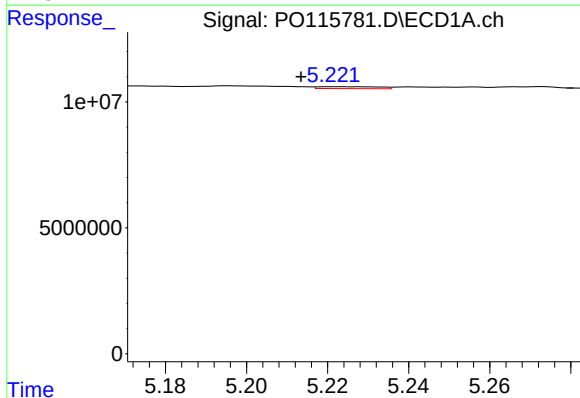


#12 AR-1232-2

R.T.: 5.222 min
Delta R.T.: 0.008 min
Response: 816605
Conc: 10.10 ng/ml

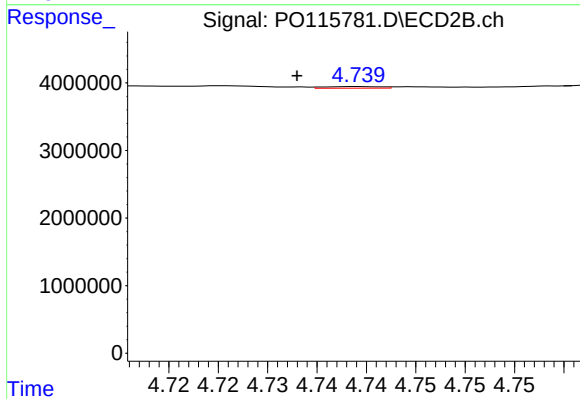

#12 AR-1232-2


R.T.: 4.739 min
Delta R.T.: 0.006 min
Response: 96088
Conc: 0.87 ng/ml

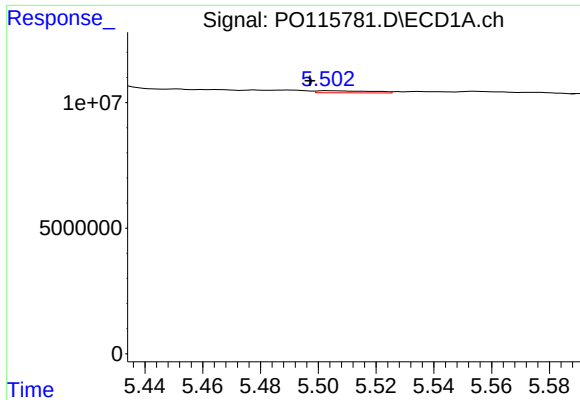

#13 AR-1232-3


R.T.: 5.503 min
Delta R.T.: 0.006 min
Response: 1056155
Conc: 6.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

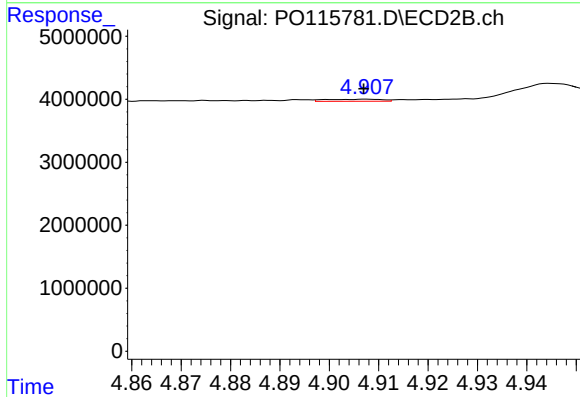


#13 AR-1232-3

R.T.: 4.907 min
Delta R.T.: 0.000 min
Response: 254864
Conc: 3.90 ng/ml

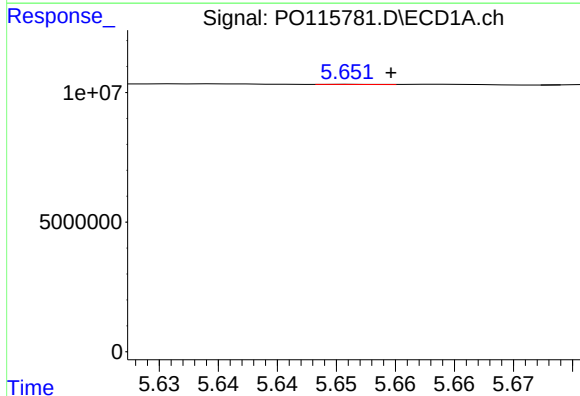


#14 AR-1232-4

R.T.: 5.651 min
Delta R.T.: -0.003 min
Response: 23846
Conc: 0.34 ng/ml

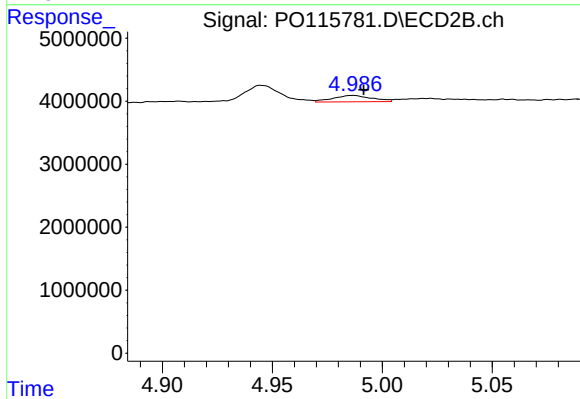

#14 AR-1232-4


R.T.: 4.987 min
Delta R.T.: -0.005 min
Response: 1239123
Conc: 24.14 ng/ml

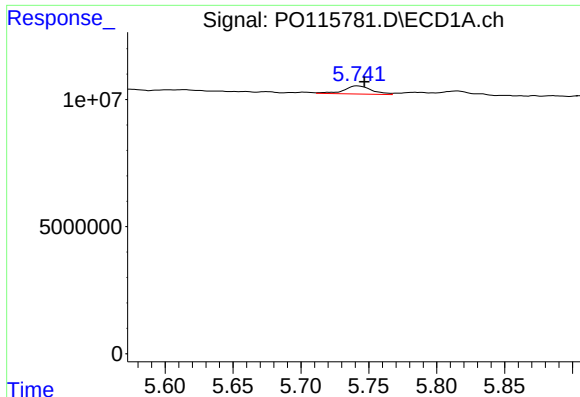

#15 AR-1232-5


R.T.: 5.742 min
Delta R.T.: -0.005 min
Response: 4657352
Conc: 89.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

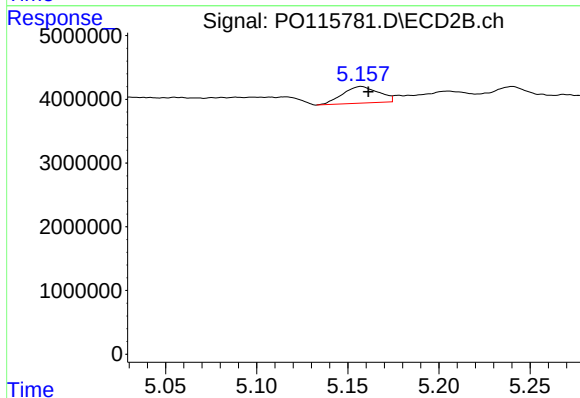


#15 AR-1232-5

R.T.: 5.157 min
Delta R.T.: -0.004 min
Response: 3602012
Conc: 65.79 ng/ml

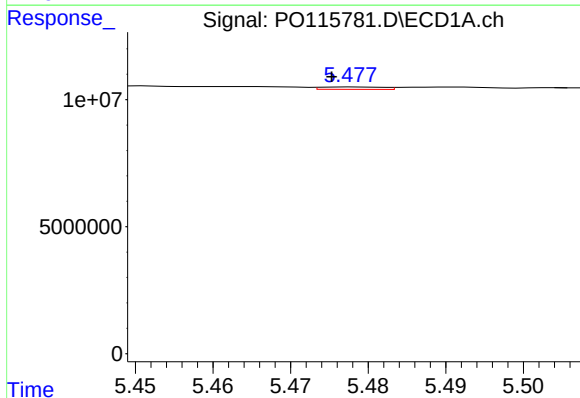


#16 AR-1242-1

R.T.: 5.478 min
Delta R.T.: 0.003 min
Response: 533725
Conc: 2.69 ng/ml

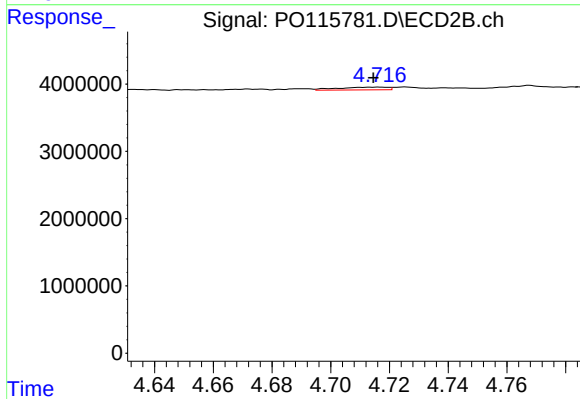

#16 AR-1242-1


R.T.: 4.717 min
Delta R.T.: 0.002 min
Response: 485010
Conc: 3.41 ng/ml

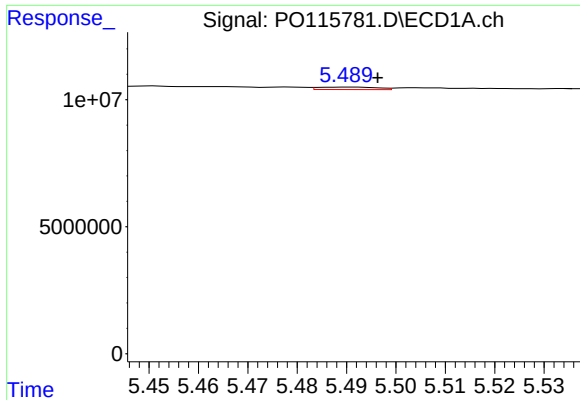

#17 AR-1242-2


R.T.: 5.490 min
Delta R.T.: -0.006 min
Response: 828359
Conc: 2.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

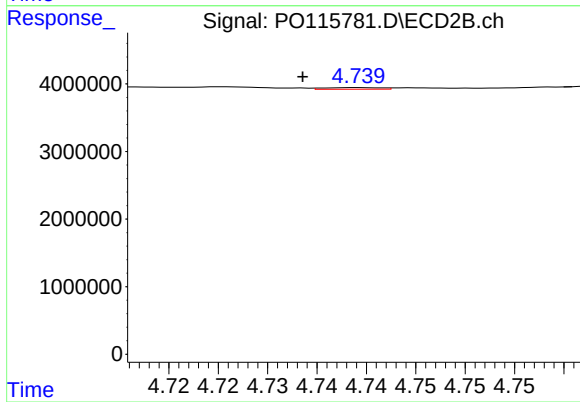


#17 AR-1242-2

R.T.: 4.739 min
Delta R.T.: 0.006 min
Response: 96088
Conc: 0.46 ng/ml

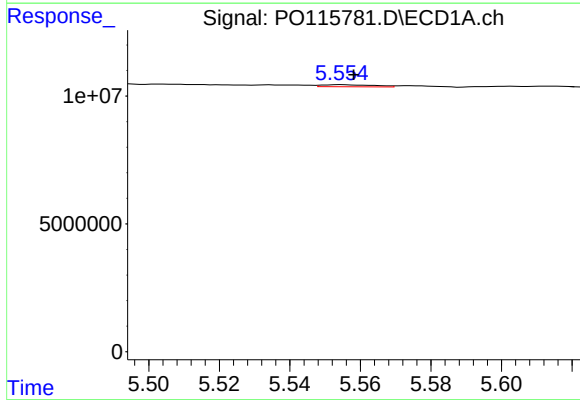


#18 AR-1242-3

R.T.: 5.555 min
Delta R.T.: -0.004 min
Response: 825683
Conc: 4.89 ng/ml

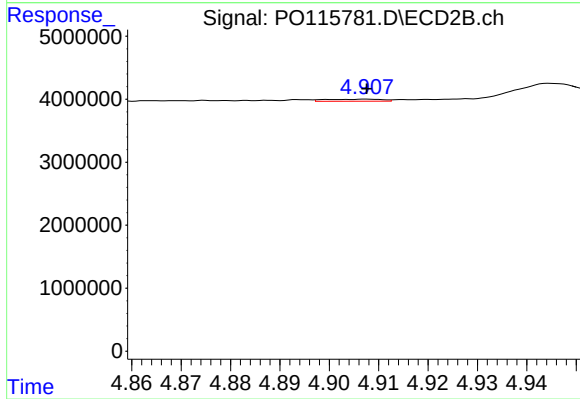

#18 AR-1242-3


R.T.: 4.907 min
Delta R.T.: 0.000 min
Response: 254864
Conc: 2.13 ng/ml

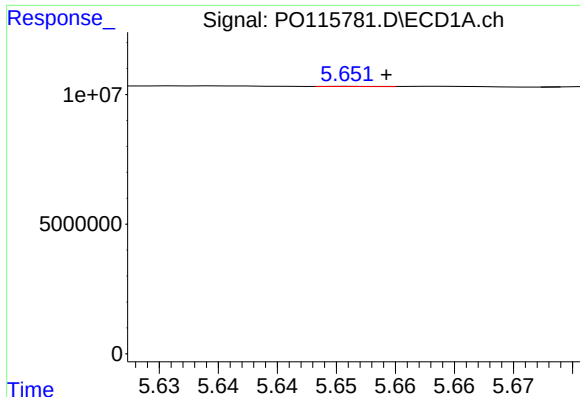

#19 AR-1242-4


R.T.: 5.651 min
Delta R.T.: -0.003 min
Response: 23846
Conc: 0.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

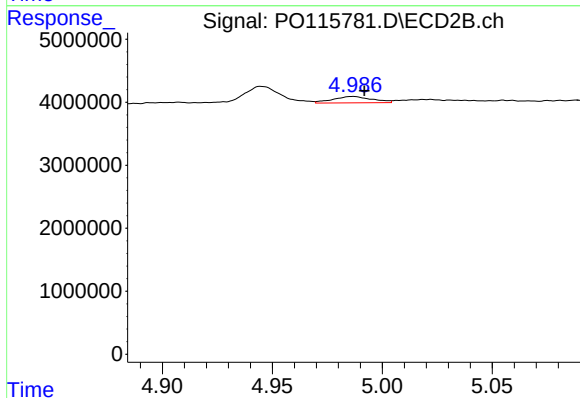


#19 AR-1242-4

R.T.: 4.987 min
Delta R.T.: -0.005 min
Response: 1239123
Conc: 11.36 ng/ml

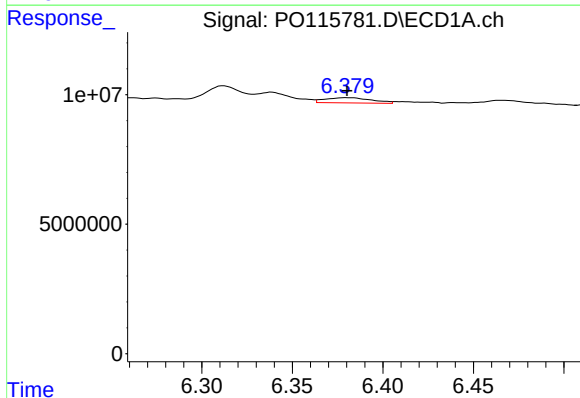


#20 AR-1242-5

R.T.: 6.380 min
Delta R.T.: 0.000 min
Response: 3636333
Conc: 24.01 ng/ml

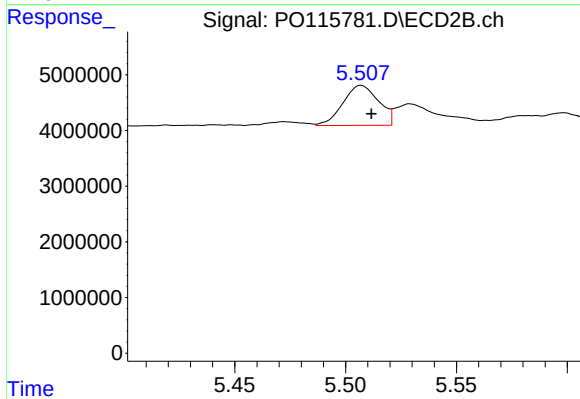

#20 AR-1242-5


R.T.: 5.507 min
Delta R.T.: -0.005 min
Response: 8077735
Conc: 58.48 ng/ml

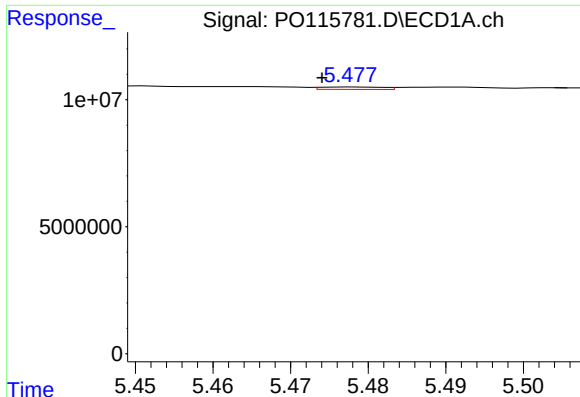

#21 AR-1248-1


R.T.: 5.478 min
Delta R.T.: 0.004 min
Response: 533725
Conc: 3.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

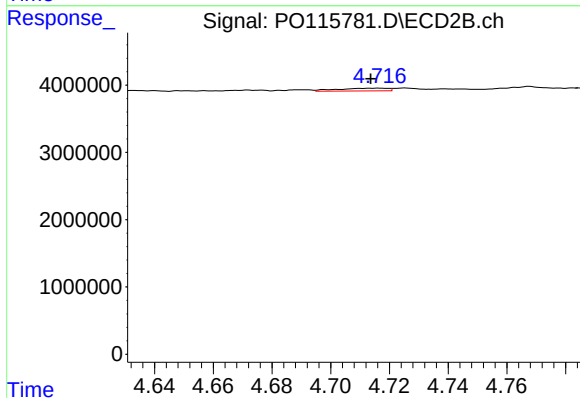


#21 AR-1248-1

R.T.: 4.717 min
Delta R.T.: 0.003 min
Response: 485010
Conc: 4.34 ng/ml

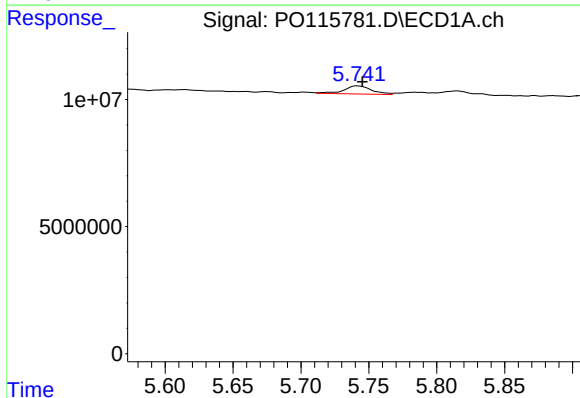


#22 AR-1248-2

R.T.: 5.742 min
Delta R.T.: -0.004 min
Response: 4657352
Conc: 23.19 ng/ml

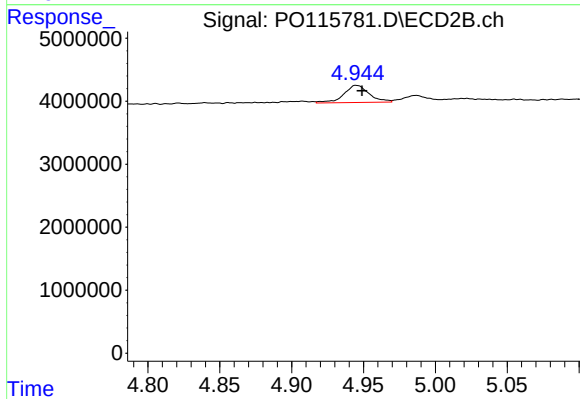

#22 AR-1248-2


R.T.: 4.945 min
Delta R.T.: -0.004 min
Response: 3354936
Conc: 22.03 ng/ml

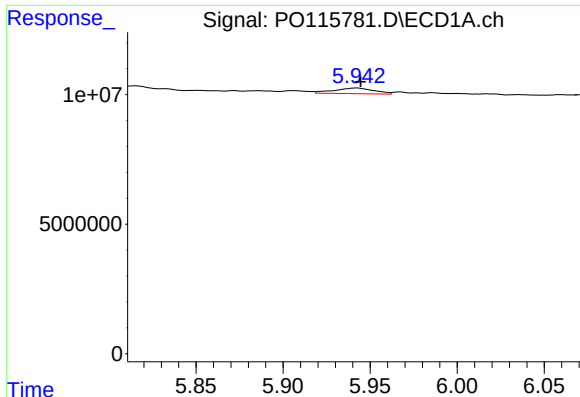

#23 AR-1248-3


R.T.: 5.942 min
Delta R.T.: -0.002 min
Response: 3526856
Conc: 14.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

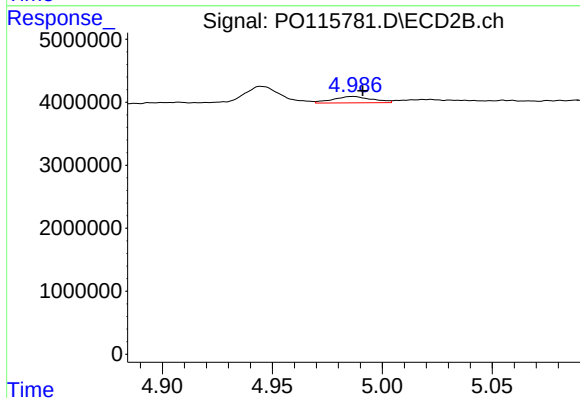


#23 AR-1248-3

R.T.: 4.987 min
Delta R.T.: -0.005 min
Response: 1239123
Conc: 7.72 ng/ml

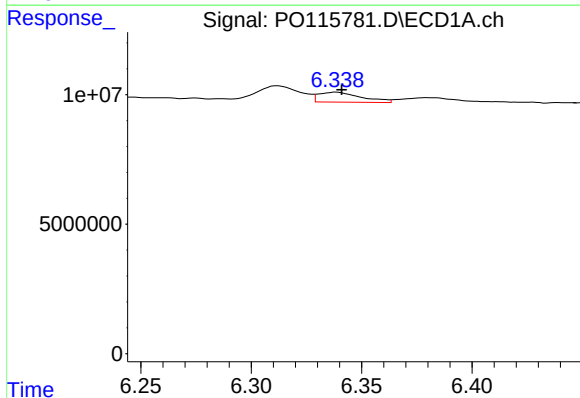


#24 AR-1248-4

R.T.: 6.339 min
Delta R.T.: -0.002 min
Response: 5202938
Conc: 17.65 ng/ml

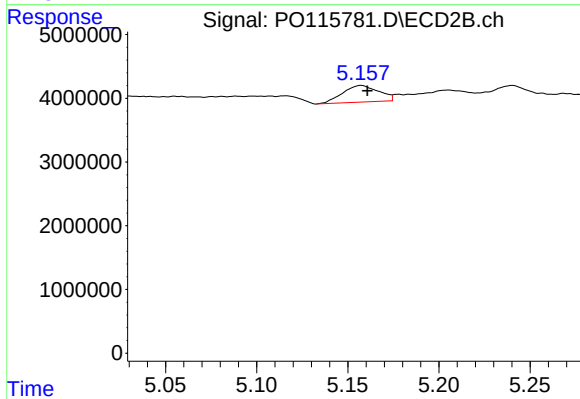

#24 AR-1248-4


R.T.: 5.157 min
Delta R.T.: -0.003 min
Response: 3602012
Conc: 19.25 ng/ml

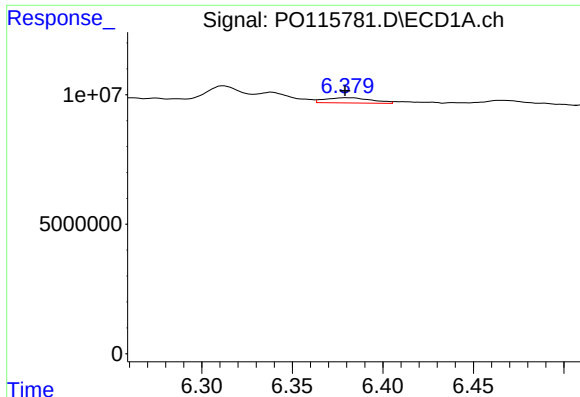

#25 AR-1248-5


R.T.: 6.380 min
Delta R.T.: 0.000 min
Response: 3636333
Conc: 14.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

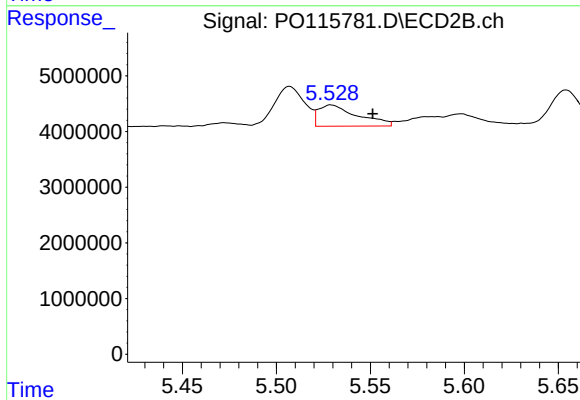


#25 AR-1248-5

R.T.: 5.529 min
Delta R.T.: -0.022 min
Response: 5518171
Conc: 27.88 ng/ml

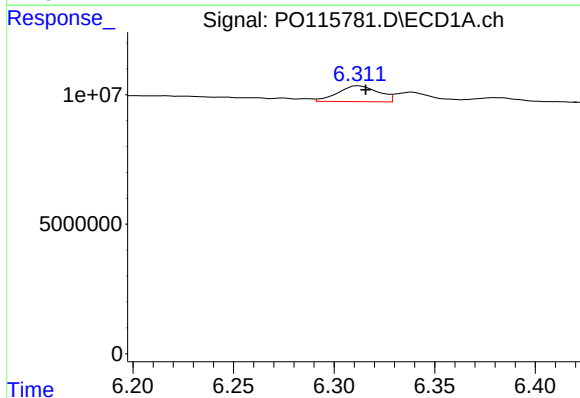


#26 AR-1254-1

R.T.: 6.312 min
Delta R.T.: -0.004 min
Response: 8597395
Conc: 33.23 ng/ml

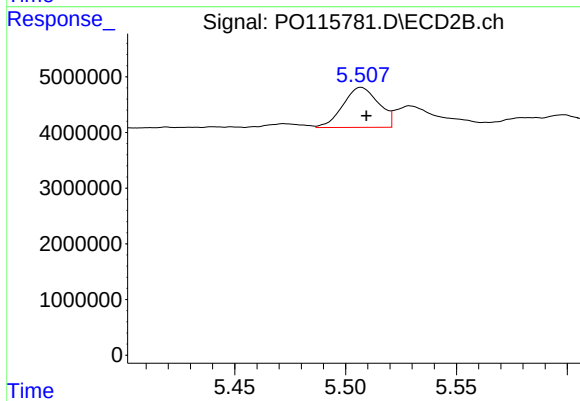

#26 AR-1254-1


R.T.: 5.507 min
Delta R.T.: -0.002 min
Response: 8077735
Conc: 27.64 ng/ml

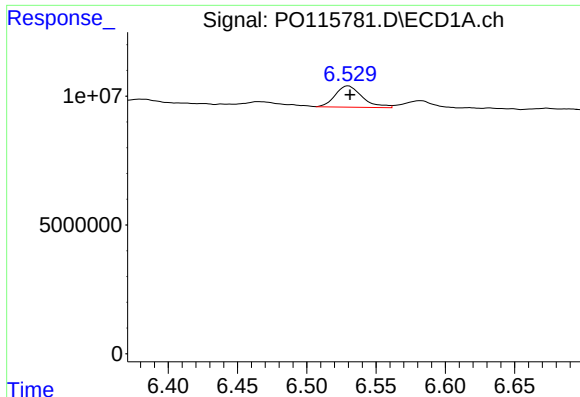

#27 AR-1254-2


R.T.: 6.530 min
Delta R.T.: -0.001 min
Response: 11255010
Conc: 27.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

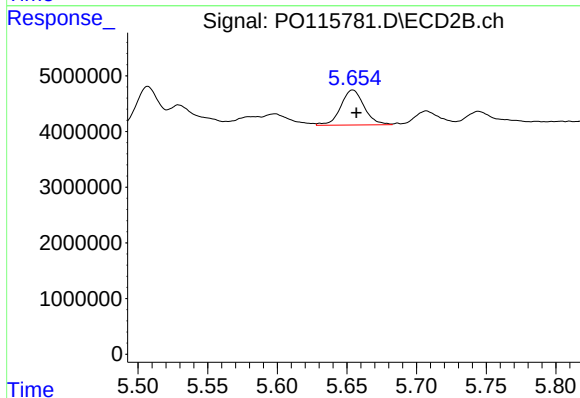


#27 AR-1254-2

R.T.: 5.654 min
Delta R.T.: -0.003 min
Response: 7370095
Conc: 29.27 ng/ml

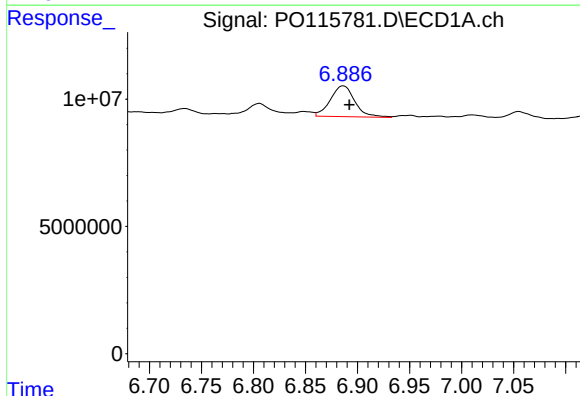


#28 AR-1254-3

R.T.: 6.886 min
Delta R.T.: -0.006 min
Response: 19651379
Conc: 47.86 ng/ml

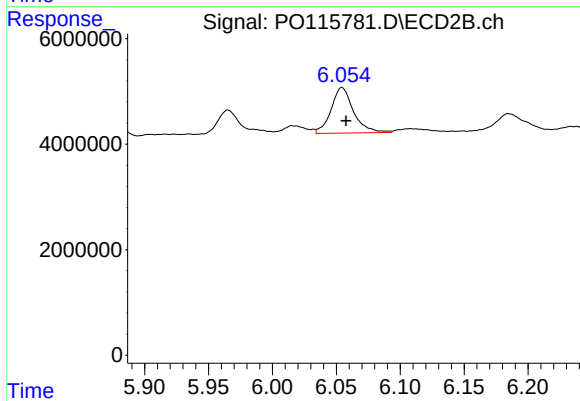

#28 AR-1254-3


R.T.: 6.054 min
Delta R.T.: -0.003 min
Response: 10575036
Conc: 26.87 ng/ml

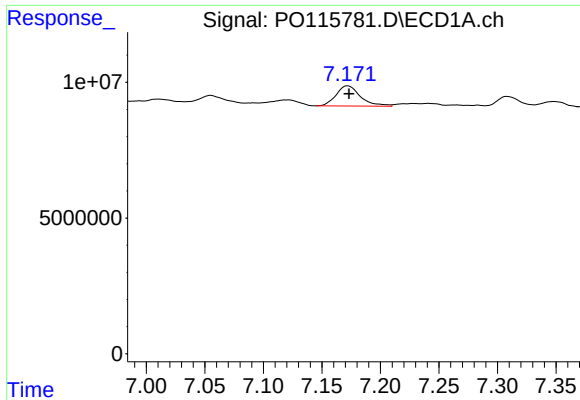

#29 AR-1254-4


R.T.: 7.172 min
Delta R.T.: -0.001 min
Response: 10710500
Conc: 30.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

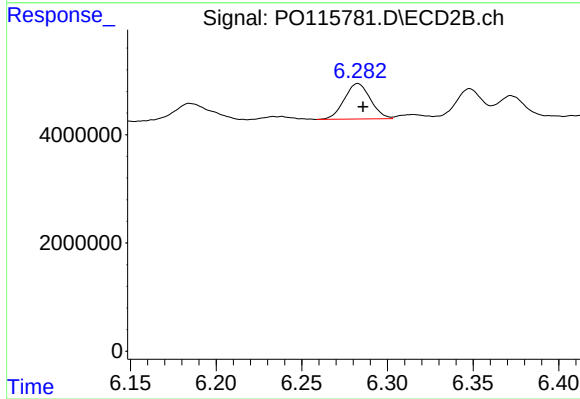


#29 AR-1254-4

R.T.: 6.283 min
Delta R.T.: -0.003 min
Response: 6967927
Conc: 26.04 ng/ml

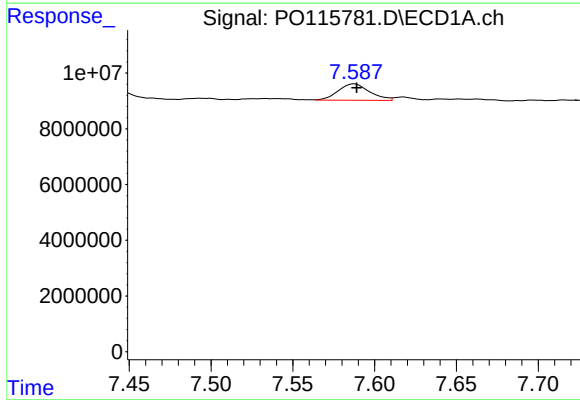


#30 AR-1254-5

R.T.: 7.588 min
Delta R.T.: -0.001 min
Response: 7828768
Conc: 24.16 ng/ml

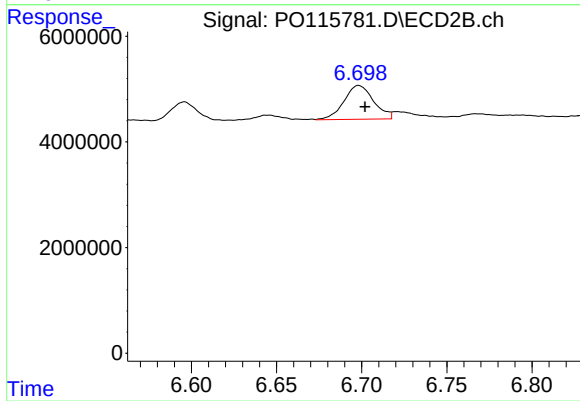

#30 AR-1254-5


R.T.: 6.698 min
Delta R.T.: -0.004 min
Response: 7781511
Conc: 21.76 ng/ml

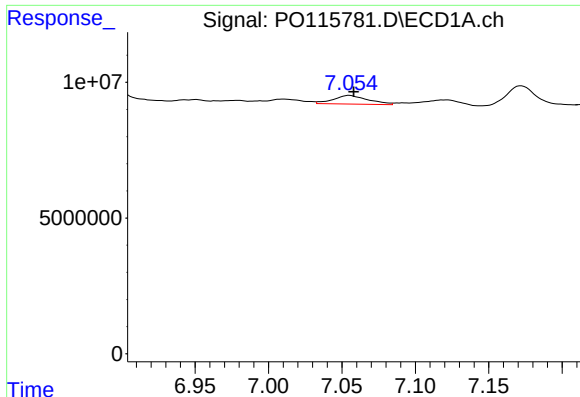

#31 AR-1260-1


R.T.: 7.055 min
Delta R.T.: -0.003 min
Response: 5242230
Conc: 18.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

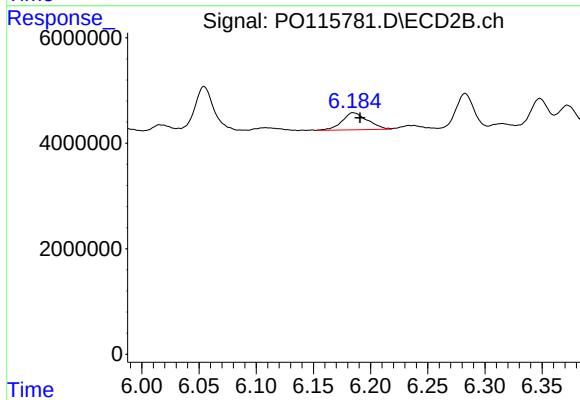


#31 AR-1260-1

R.T.: 6.184 min
Delta R.T.: -0.006 min
Response: 5056451
Conc: 19.29 ng/ml

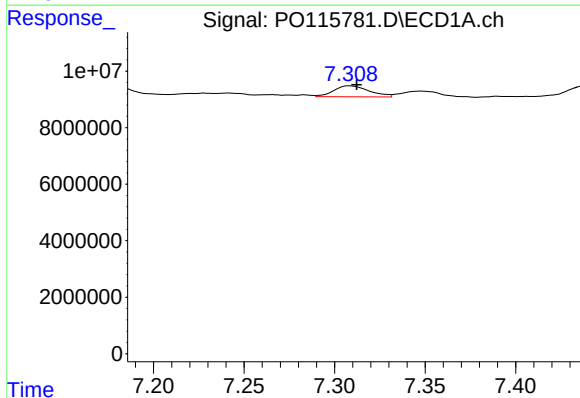


#32 AR-1260-2

R.T.: 7.308 min
Delta R.T.: -0.004 min
Response: 5249970
Conc: 11.99 ng/ml

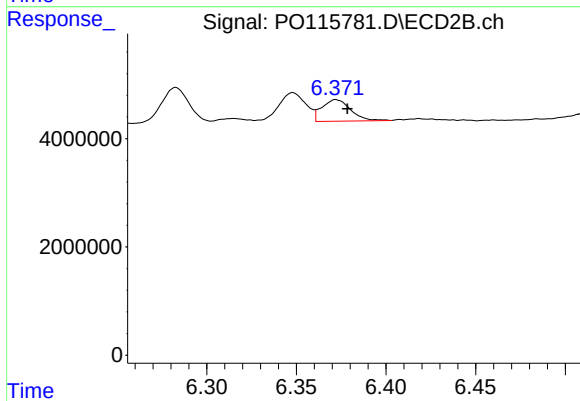

#32 AR-1260-2


R.T.: 6.372 min
Delta R.T.: -0.006 min
Response: 4472167
Conc: 12.76 ng/ml

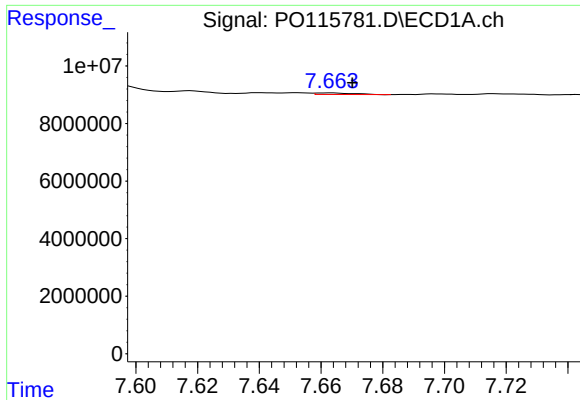

#33 AR-1260-3


R.T.: 7.663 min
Delta R.T.: -0.007 min
Response: 504070
Conc: 1.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

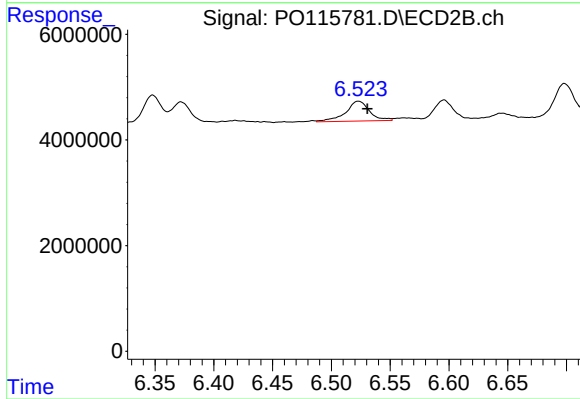


#33 AR-1260-3

R.T.: 6.523 min
Delta R.T.: -0.008 min
Response: 5320686
Conc: 16.56 ng/ml

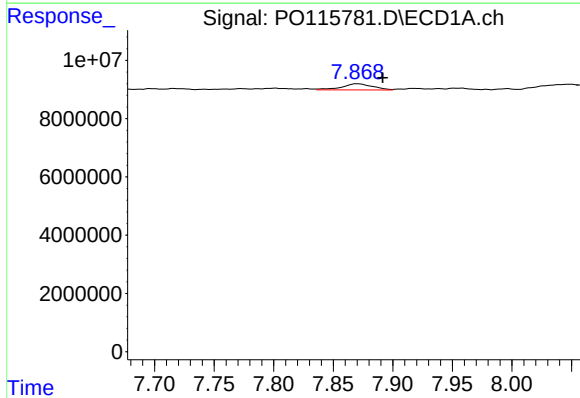


#34 AR-1260-4

R.T.: 7.870 min
Delta R.T.: -0.021 min
Response: 3851616
Conc: 12.53 ng/ml

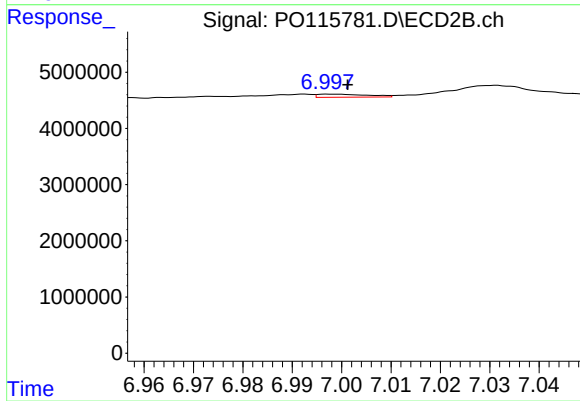

#34 AR-1260-4


R.T.: 6.998 min
Delta R.T.: -0.004 min
Response: 386247
Conc: 1.50 ng/ml

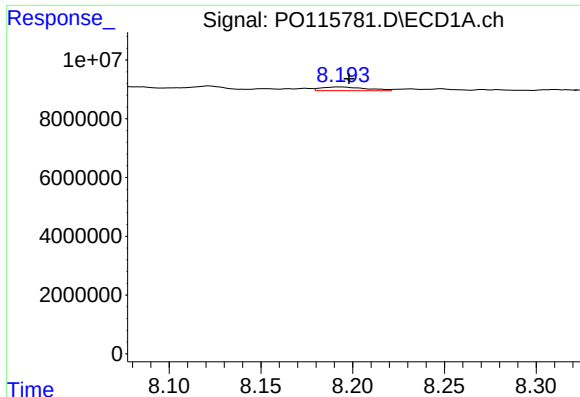

#35 AR-1260-5


R.T.: 8.194 min
Delta R.T.: -0.004 min
Response: 2134315
Conc: 2.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

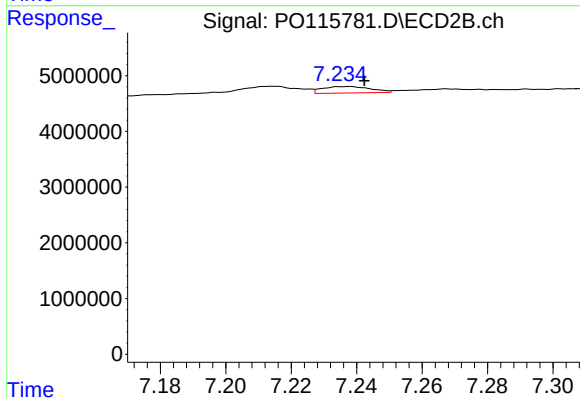


#35 AR-1260-5

R.T.: 7.238 min
Delta R.T.: -0.004 min
Response: 1188429
Conc: 1.69 ng/ml

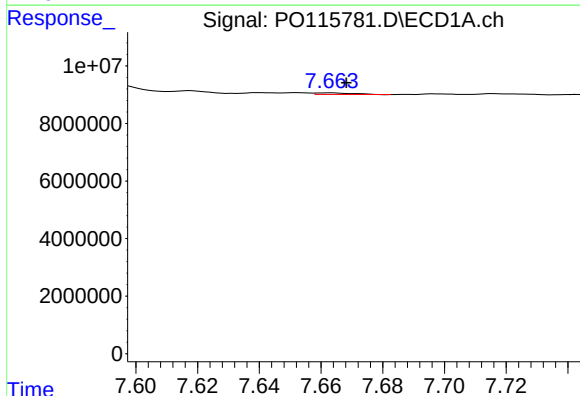


#36 AR-1262-1

R.T.: 7.663 min
Delta R.T.: -0.005 min
Response: 504070
Conc: 2.04 ng/ml

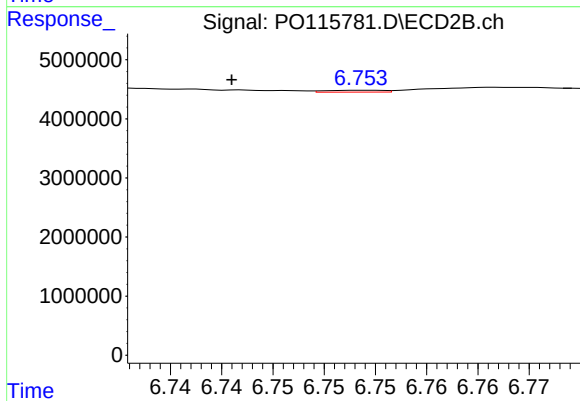

#36 AR-1262-1


R.T.: 6.754 min
Delta R.T.: 0.013 min
Response: 125911
Conc: 0.59 ng/ml

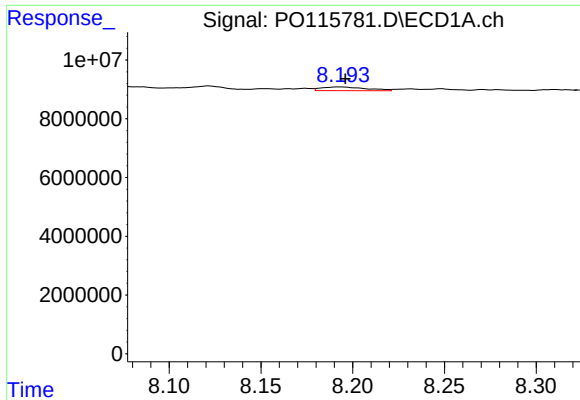

#37 AR-1262-2


R.T.: 8.194 min
Delta R.T.: -0.002 min
Response: 2134315
Conc: 5.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

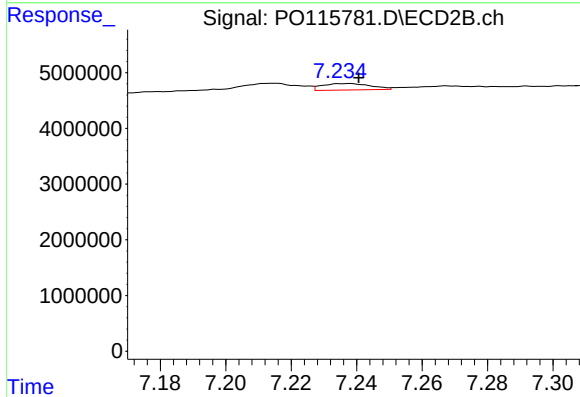


#37 AR-1262-2

R.T.: 7.238 min
Delta R.T.: -0.003 min
Response: 1188429
Conc: 3.41 ng/ml

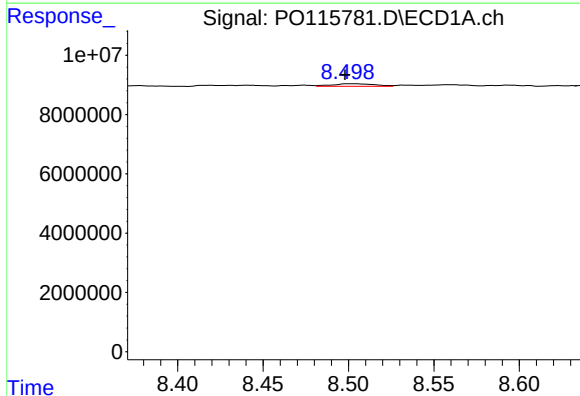


#38 AR-1262-3

R.T.: 8.504 min
Delta R.T.: 0.006 min
Response: 1496252
Conc: 5.87 ng/ml

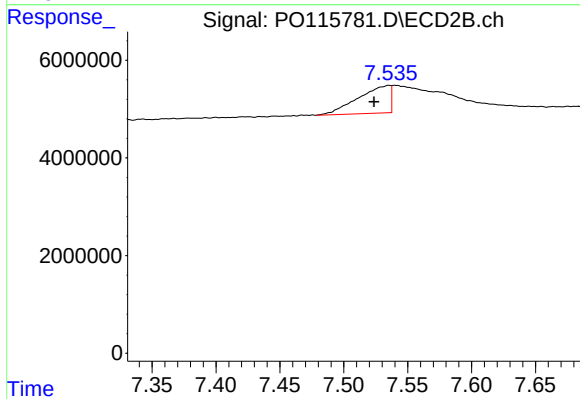

#38 AR-1262-3


R.T.: 7.535 min
Delta R.T.: 0.012 min
Response: 9846623
Conc: 62.96 ng/ml

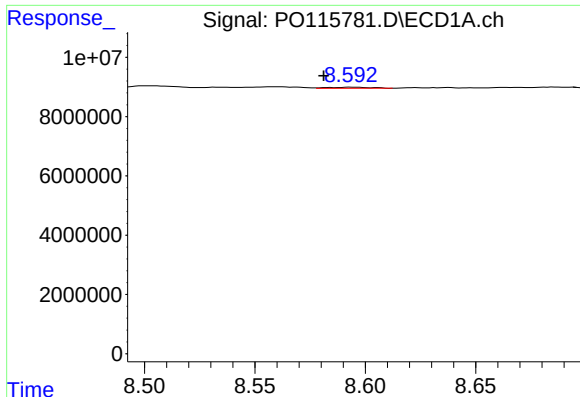

#39 AR-1262-4


R.T.: 8.593 min
Delta R.T.: 0.012 min
Response: 475607
Conc: 2.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

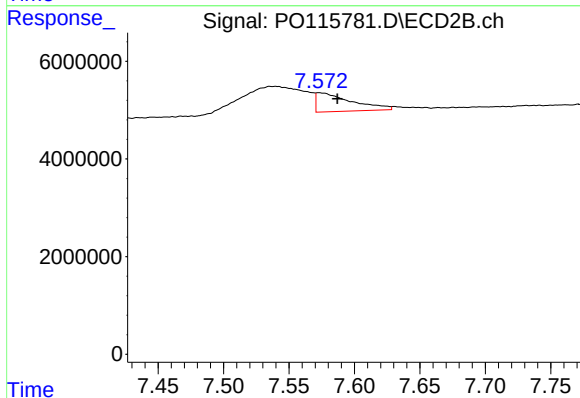


#39 AR-1262-4

R.T.: 7.573 min
Delta R.T.: -0.014 min
Response: 7286089
Conc: 29.45 ng/ml

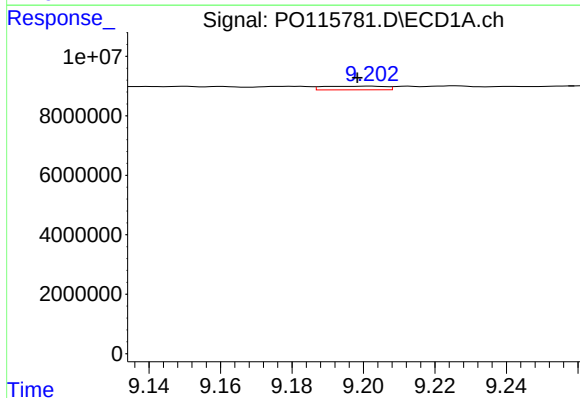


#40 AR-1262-5

R.T.: 9.202 min
Delta R.T.: 0.004 min
Response: 1477656
Conc: 10.97 ng/ml

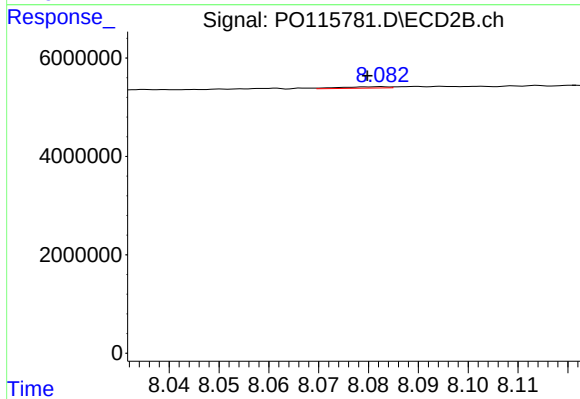

#40 AR-1262-5


R.T.: 8.083 min
Delta R.T.: 0.003 min
Response: 186416
Conc: 1.67 ng/ml

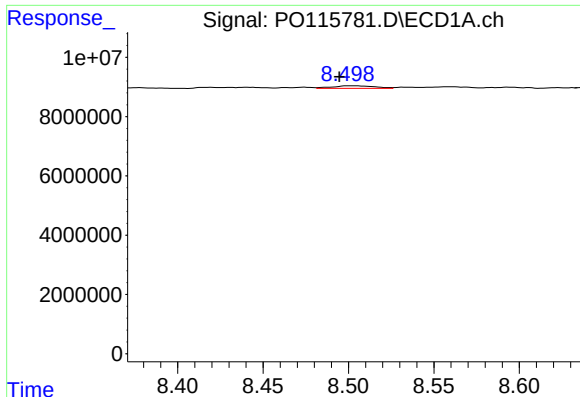

#41 AR-1268-1


R.T.: 8.504 min
Delta R.T.: 0.009 min
Response: 1496252
Conc: 1.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

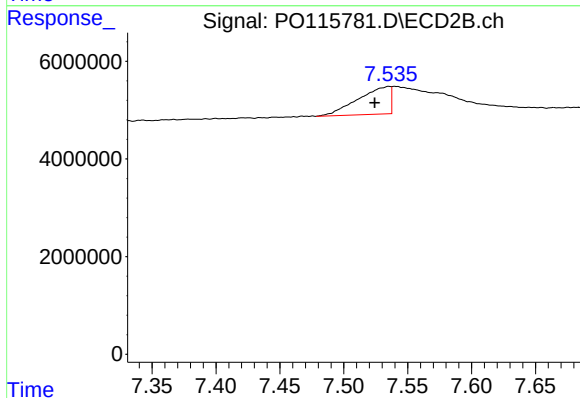


#41 AR-1268-1

R.T.: 7.535 min
Delta R.T.: 0.011 min
Response: 9846623
Conc: 11.11 ng/ml

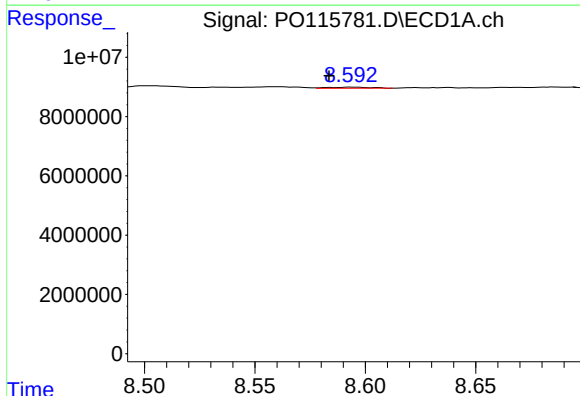


#42 AR-1268-2

R.T.: 8.593 min
Delta R.T.: 0.010 min
Response: 475607
Conc: 0.56 ng/ml

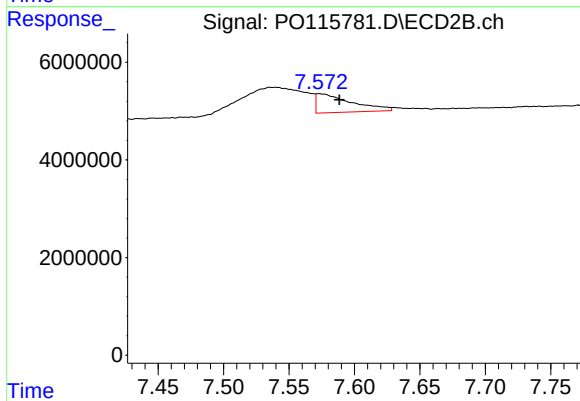

#42 AR-1268-2


R.T.: 7.573 min
Delta R.T.: -0.016 min
Response: 7286089
Conc: 9.73 ng/ml

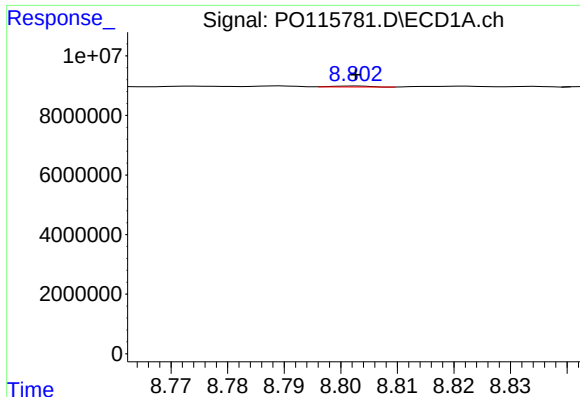

#43 AR-1268-3


R.T.: 8.803 min
Delta R.T.: 0.000 min
Response: 157662
Conc: 0.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

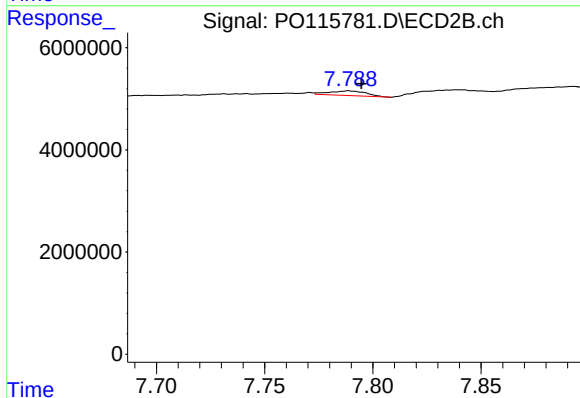


#43 AR-1268-3

R.T.: 7.789 min
Delta R.T.: -0.006 min
Response: 1070286
Conc: 1.68 ng/ml

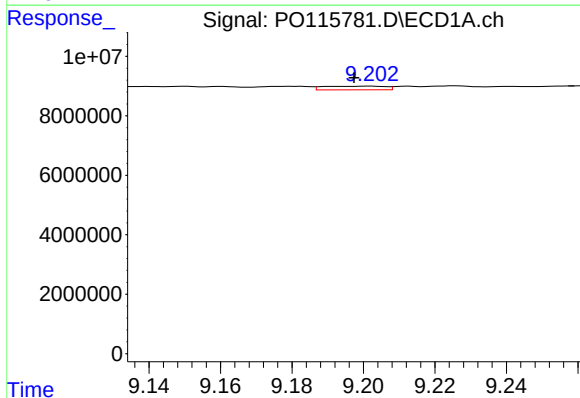


#44 AR-1268-4

R.T.: 9.202 min
Delta R.T.: 0.004 min
Response: 1477656
Conc: 4.73 ng/ml

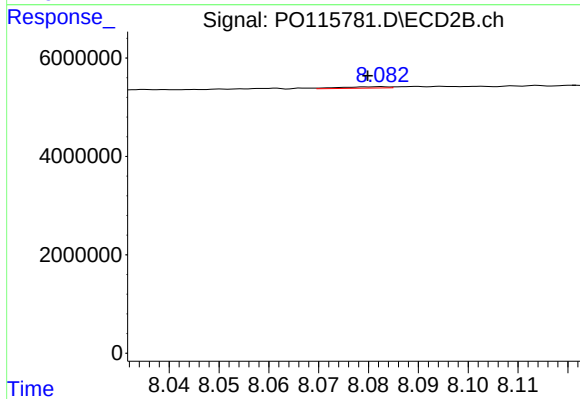

#44 AR-1268-4


R.T.: 8.083 min
Delta R.T.: 0.003 min
Response: 186416
Conc: 0.72 ng/ml

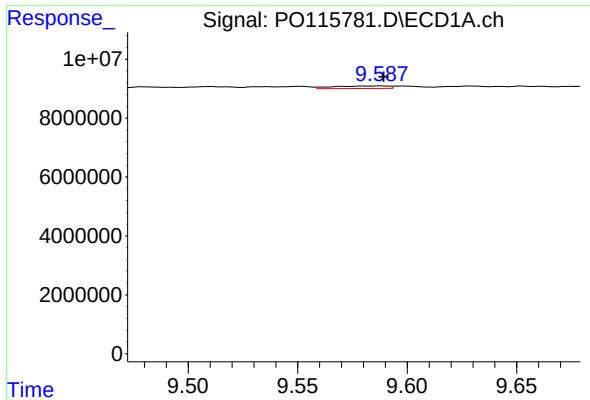

#45 AR-1268-5

R.T.: 9.588 min
Delta R.T.: -0.001 min
Response: 1535328
Conc: 0.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

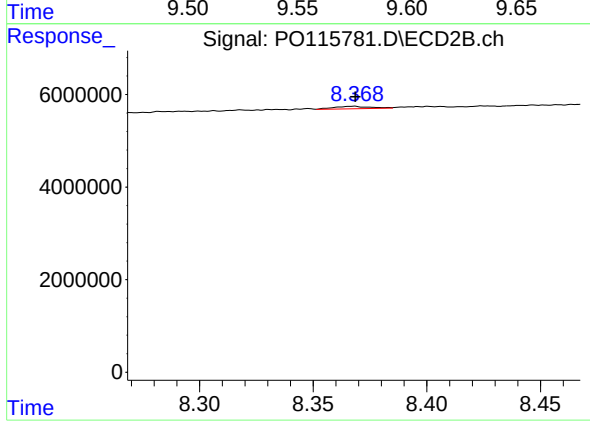

#45 AR-1268-5

R.T.: 8.368 min
Delta R.T.: 0.000 min
Response: 613238
Conc: 0.36 ng/ml