

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121225\
 Data File : PO115782.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Dec 2025 03:28
 Operator : YP/AJ
 Sample : Q3530-07
 Misc : AR1262 25PPB WATER LOD
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 00:57:13 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 05 02:11:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.334	3.636	314.6E6	192.9E6	40.504	39.587
2)	SA Decachlor...	9.907	8.615	217.6E6	160.5E6	41.359	37.330
Target Compounds							
3)	L1 AR-1016-1	5.451	4.709	2579148	8459693	10.372	45.786 #
4)	L1 AR-1016-2	5.500	4.709	3263960	8459693	8.570	32.007 #
5)	L1 AR-1016-3	5.556	4.903	3135158	11596725	14.665	76.628 #
6)	L1 AR-1016-4	5.640	4.987f	329879	6795853	1.847	60.298 #
7)	L1 AR-1016-5	5.943	5.207f	14228548	20577997	81.108	140.617 #
8)	L2 AR-1221-1	4.531	3.869	7124642	1393096	87.745	24.698 #
9)	L2 AR-1221-2	4.631	3.932	4798794	6093114	76.149	143.557 #
10)	L2 AR-1221-3	4.689	4.011	1654998	730403	8.864	5.680 #
11)	L3 AR-1232-1	4.689	4.011	1654998	730403	11.058	6.837 #
12)	L3 AR-1232-2	5.212	4.709	752337	8459693	9.305	76.220 #
13)	L3 AR-1232-3	5.500	4.903	3263960	11596725	21.208	177.411 #
14)	L3 AR-1232-4	5.667	4.987	153503	6795853	2.192	132.395 #
15)	L3 AR-1232-5	5.748	5.207f	2950855	20577997	56.816	375.867 #
16)	L4 AR-1242-1	5.451	4.709	2579148	8459693	12.985	59.413 #
17)	L4 AR-1242-2	5.500	4.709	3263960	8459693	11.144	40.407 #
18)	L4 AR-1242-3	5.556	4.903	3135158	11596725	18.571	97.091 #
19)	L4 AR-1242-4	5.667	4.987	153503	6795853	1.123	62.295 #
20)	L4 AR-1242-5	6.376	5.530	17616827	24565931	116.326	177.853 #
21)	L5 AR-1248-1	5.451	4.709	2579148	8459693	16.994	75.648 #
22)	L5 AR-1248-2	5.748	4.987f	2950855	6795853	14.694	44.625 #
23)	L5 AR-1248-3	5.943	4.987	14228548	6795853	57.699	42.335 #
24)	L5 AR-1248-4	6.341	5.207f	6594496	20577997	22.365	109.957 #
25)	L5 AR-1248-5	6.376	5.530	17616827	24565931	68.038	124.098 #
26)	L6 AR-1254-1	6.298	5.530	7424368	24565931	28.697	84.052 #
27)	L6 AR-1254-2	6.531	5.654	20455137	13442588	50.832	53.383
28)	L6 AR-1254-3	6.881	6.071	34736075	16092572	84.605	40.888 #
29)	L6 AR-1254-4	7.172	6.289	15999268	4500569	46.099	16.820 #
30)	L6 AR-1254-5	7.584	6.698	20766577	9057099	64.086	25.333 #
31)	L7 AR-1260-1	7.056	6.186	27336178	21518356	94.360	82.078
32)	L7 AR-1260-2	7.310	6.373	27486077	14920255	62.792	42.574 #
33)	L7 AR-1260-3	7.667	6.528	30637482	13047937	91.022	40.614 #
34)	L7 AR-1260-4	7.889	6.996	25648290	15371783	83.417	59.851 #
35)	L7 AR-1260-5	8.194	7.237	42827889	32437843	58.791	46.255
36)	L8 AR-1262-1	7.667	6.738	30637482	20308956	124.110	95.328
37)	L8 AR-1262-2	8.194	7.237	42827889	32437843	108.179	93.125
38)	L8 AR-1262-3	8.496	7.521	24545606	32402055	96.324	207.187 #
39)	L8 AR-1262-4	8.579	7.583	19351404	33571167	99.901	135.712 #
40)	L8 AR-1262-5	9.196	8.076	14985830	9665522	111.261	86.706
41)	L9 AR-1268-1	8.496	7.521	24545606	32402055	24.651	36.573 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121225\
 Data File : PO115782.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Dec 2025 03:28
 Operator : YP/AJ
 Sample : Q3530-07
 Misc : AR1262 25PPB WATER LOD
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 00:57:13 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 05 02:11:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.579	7.583	19351404	33571167	22.623	44.817 #
43) L9	AR-1268-3	8.802	7.792	1632002	1595832	2.197	2.506
44) L9	AR-1268-4	9.196	8.076	14985830	9665522	47.995	37.518
45) L9	AR-1268-5	9.586	8.364	6755918	4098586	3.103	2.431



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121225\
Data File : PO115782.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Dec 2025 03:28
Operator : YP/AJ
Sample : Q3530-07
Misc : AR1262 25PPB WATER LOD
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 00:57:13 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120425.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 05 02:11:05 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

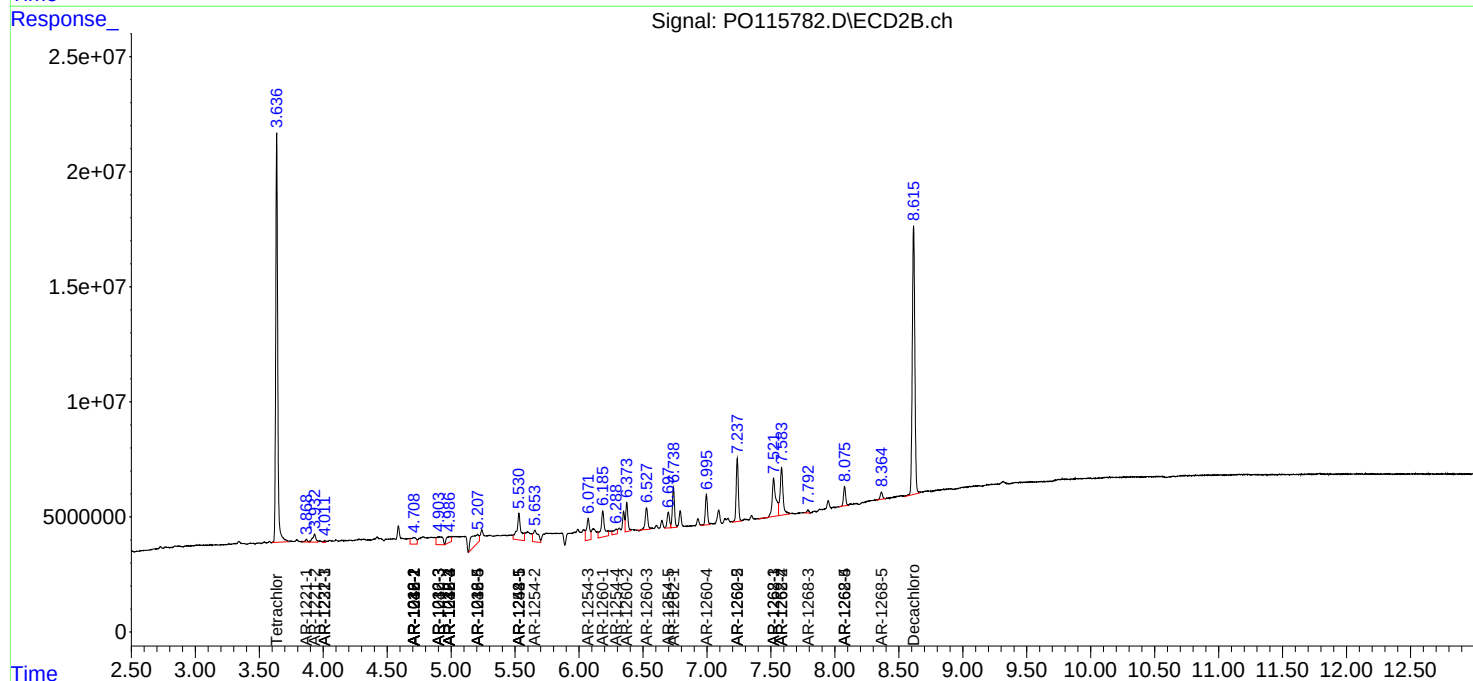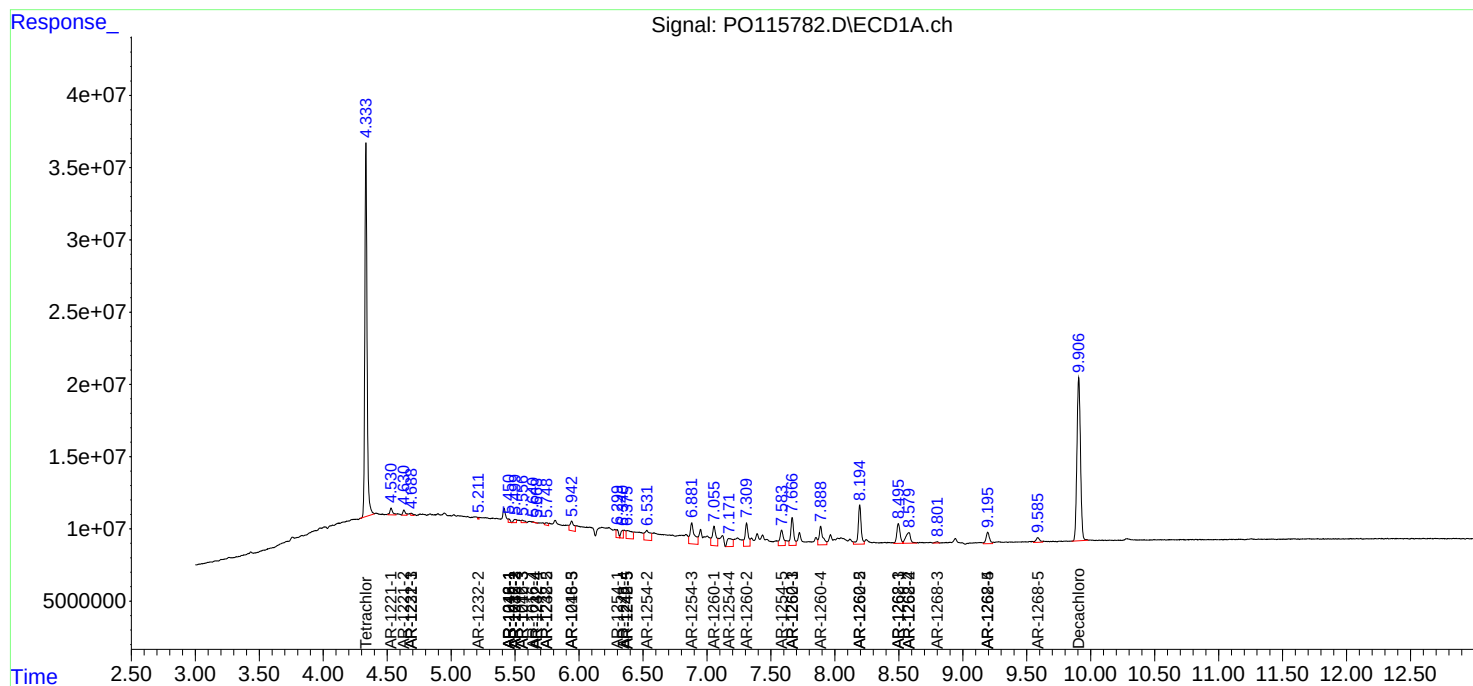


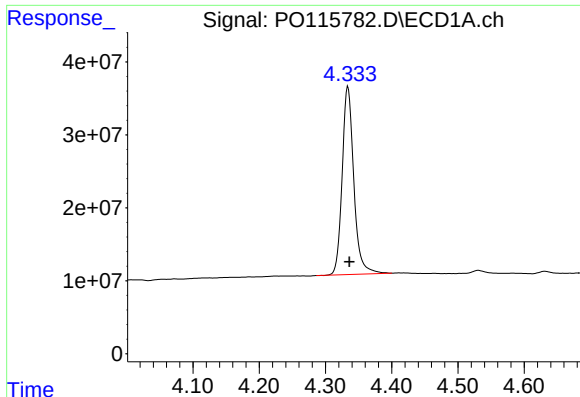

#1 Tetrachloro-m-xylene


R.T.: 4.334 min
Delta R.T.: -0.002 min
Response: 314601650
Conc: 40.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

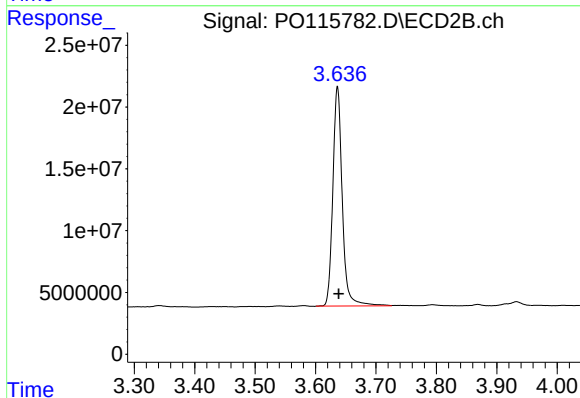


#1 Tetrachloro-m-xylene

R.T.: 3.636 min
Delta R.T.: -0.002 min
Response: 192920597
Conc: 39.59 ng/ml

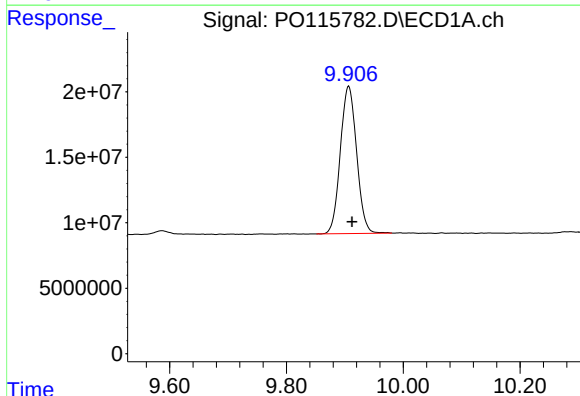


#2 Decachlorobiphenyl

R.T.: 9.907 min
Delta R.T.: -0.006 min
Response: 217591692
Conc: 41.36 ng/ml

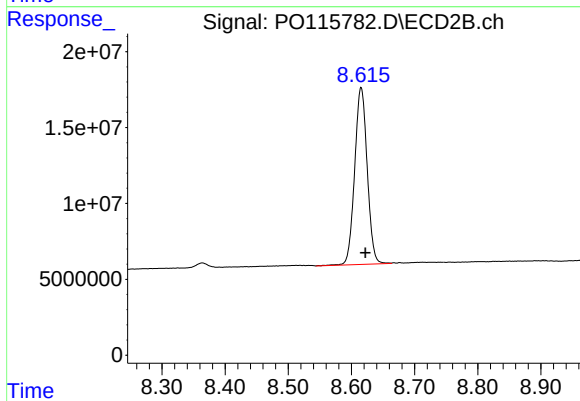

#2 Decachlorobiphenyl


R.T.: 8.615 min
Delta R.T.: -0.007 min
Response: 160529078
Conc: 37.33 ng/ml

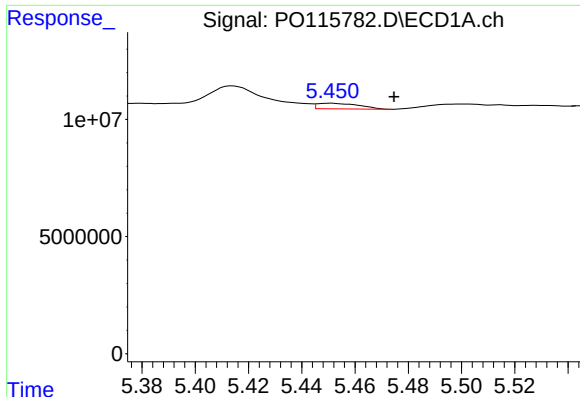

#3 AR-1016-1


R.T.: 5.451 min
Delta R.T.: -0.024 min
Response: 2579148
Conc: 10.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

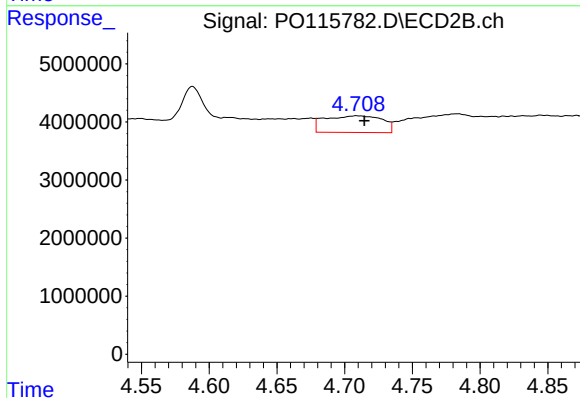


#3 AR-1016-1

R.T.: 4.709 min
Delta R.T.: -0.006 min
Response: 8459693
Conc: 45.79 ng/ml

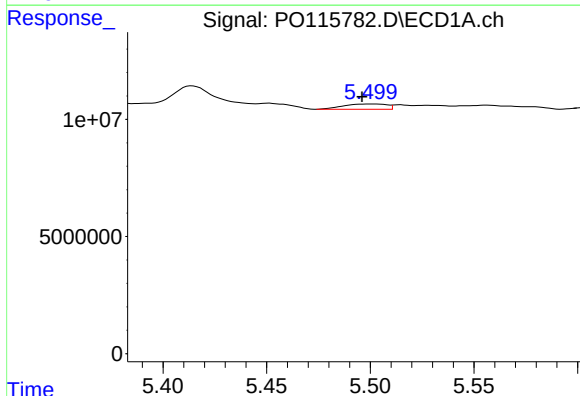


#4 AR-1016-2

R.T.: 5.500 min
Delta R.T.: 0.004 min
Response: 3263960
Conc: 8.57 ng/ml

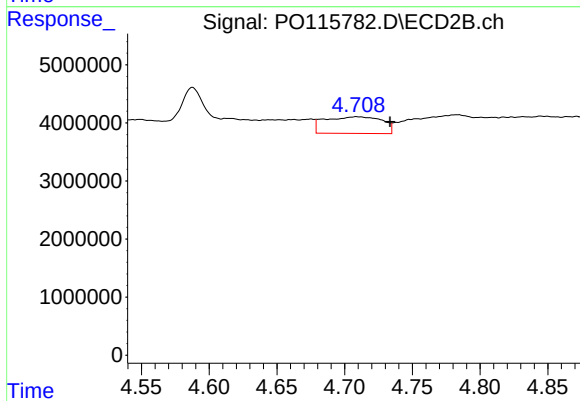

#4 AR-1016-2


R.T.: 4.709 min
Delta R.T.: -0.025 min
Response: 8459693
Conc: 32.01 ng/ml

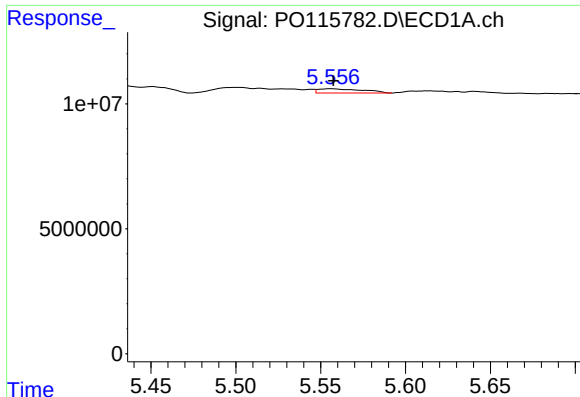

#5 AR-1016-3


R.T.: 5.556 min
Delta R.T.: -0.001 min
Response: 3135158
Conc: 14.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

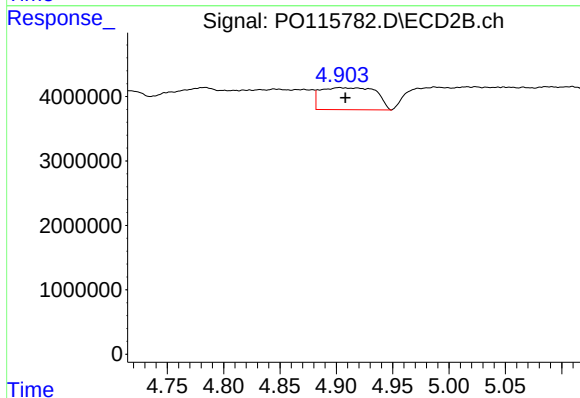


#5 AR-1016-3

R.T.: 4.903 min
Delta R.T.: -0.005 min
Response: 11596725
Conc: 76.63 ng/ml

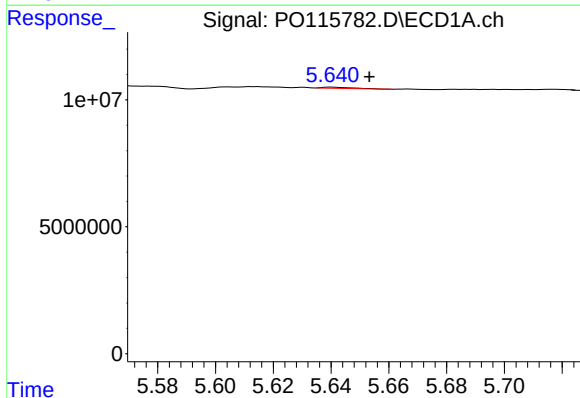


#6 AR-1016-4

R.T.: 5.640 min
Delta R.T.: -0.013 min
Response: 329879
Conc: 1.85 ng/ml

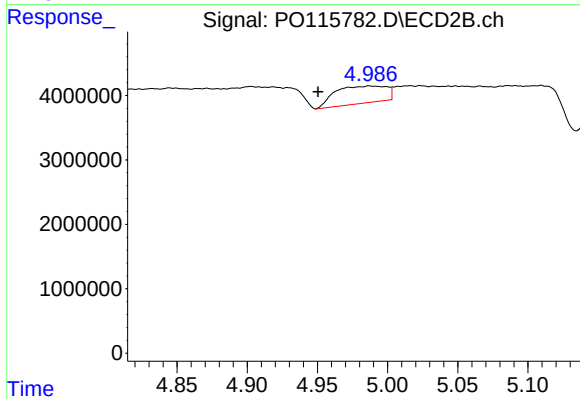

#6 AR-1016-4


R.T.: 4.987 min
Delta R.T.: 0.037 min
Response: 6795853
Conc: 60.30 ng/ml

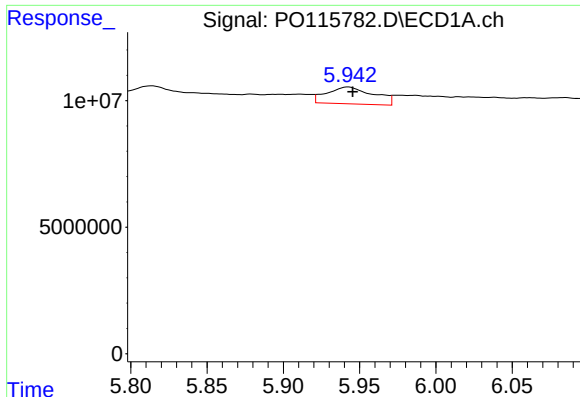

#7 AR-1016-5


R.T.: 5.943 min
Delta R.T.: -0.003 min
Response: 14228548
Conc: 81.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

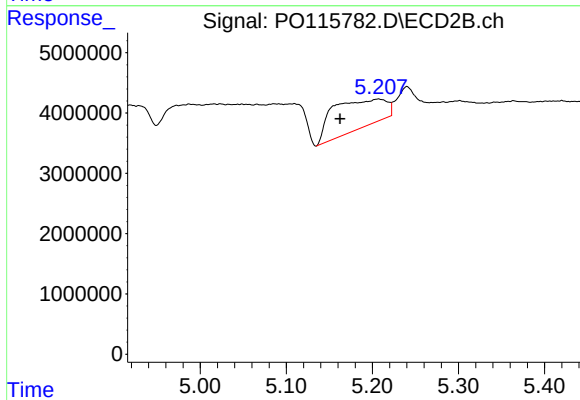


#7 AR-1016-5

R.T.: 5.207 min
Delta R.T.: 0.045 min
Response: 20577997
Conc: 140.62 ng/ml

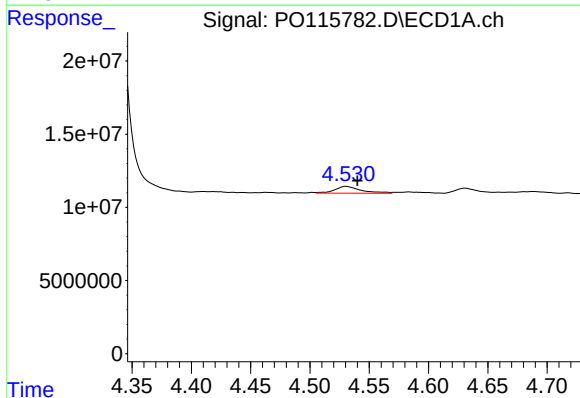


#8 AR-1221-1

R.T.: 4.531 min
Delta R.T.: -0.009 min
Response: 7124642
Conc: 87.75 ng/ml

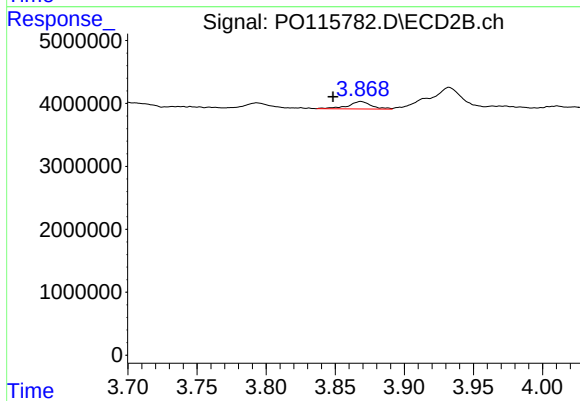

#8 AR-1221-1


R.T.: 3.869 min
Delta R.T.: 0.020 min
Response: 1393096
Conc: 24.70 ng/ml

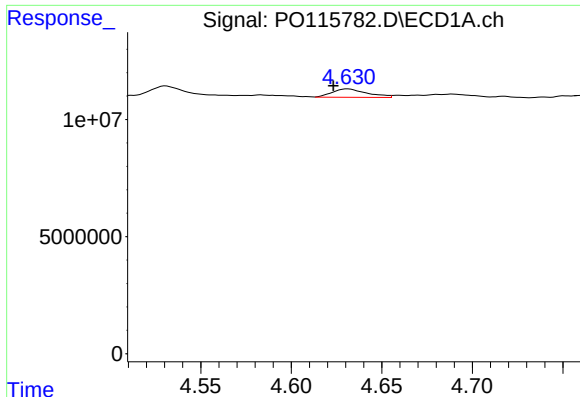

#9 AR-1221-2


R.T.: 4.631 min
Delta R.T.: 0.008 min
Response: 4798794
Conc: 76.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

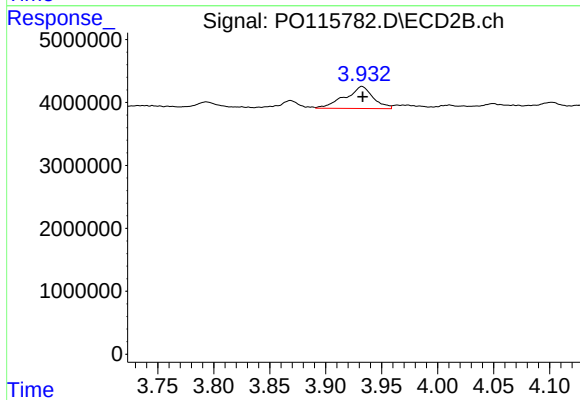


#9 AR-1221-2

R.T.: 3.932 min
Delta R.T.: 0.000 min
Response: 6093114
Conc: 143.56 ng/ml

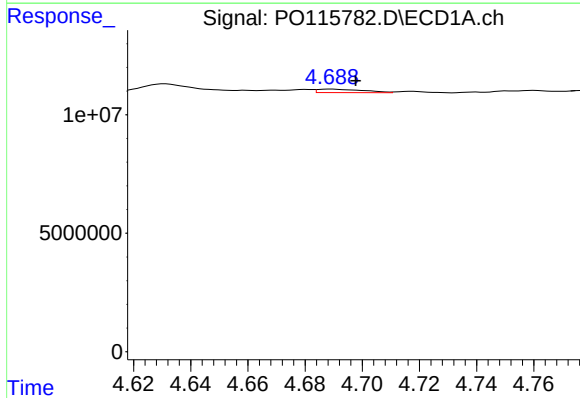


#10 AR-1221-3

R.T.: 4.689 min
Delta R.T.: -0.009 min
Response: 1654998
Conc: 8.86 ng/ml

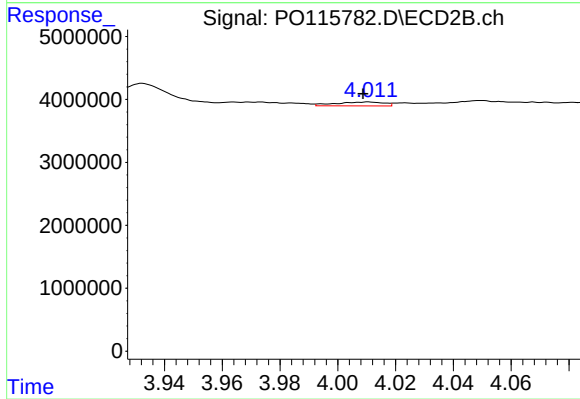

#10 AR-1221-3


R.T.: 4.011 min
Delta R.T.: 0.002 min
Response: 730403
Conc: 5.68 ng/ml

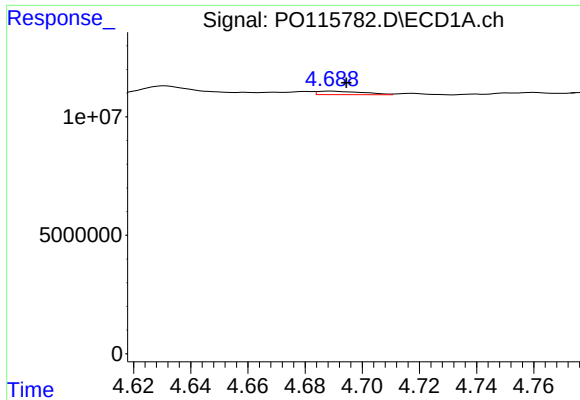

#11 AR-1232-1


R.T.: 4.689 min
Delta R.T.: -0.005 min
Response: 1654998
Conc: 11.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

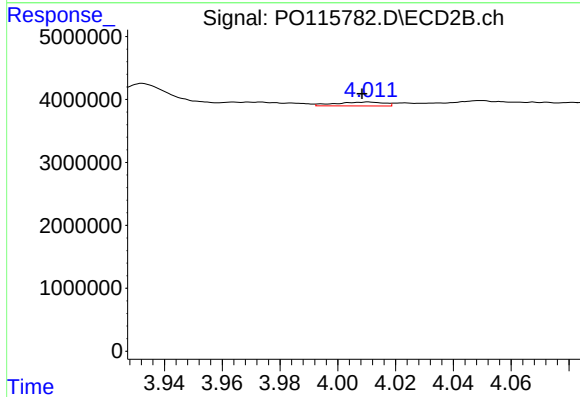


#11 AR-1232-1

R.T.: 4.011 min
Delta R.T.: 0.002 min
Response: 730403
Conc: 6.84 ng/ml

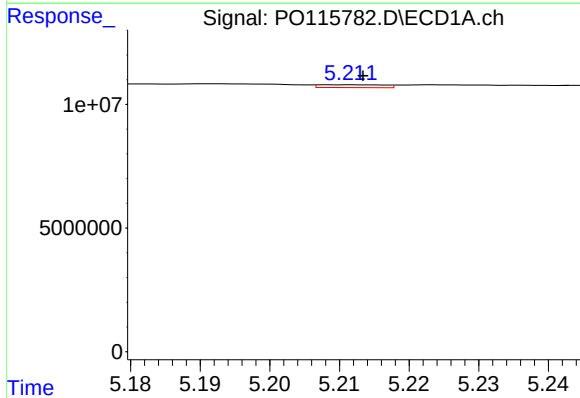


#12 AR-1232-2

R.T.: 5.212 min
Delta R.T.: -0.002 min
Response: 752337
Conc: 9.31 ng/ml

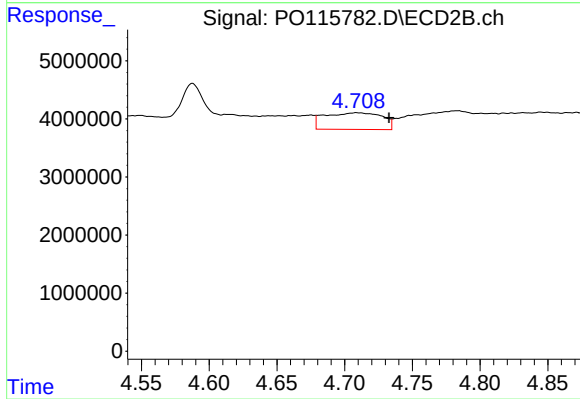

#12 AR-1232-2


R.T.: 4.709 min
Delta R.T.: -0.024 min
Response: 8459693
Conc: 76.22 ng/ml

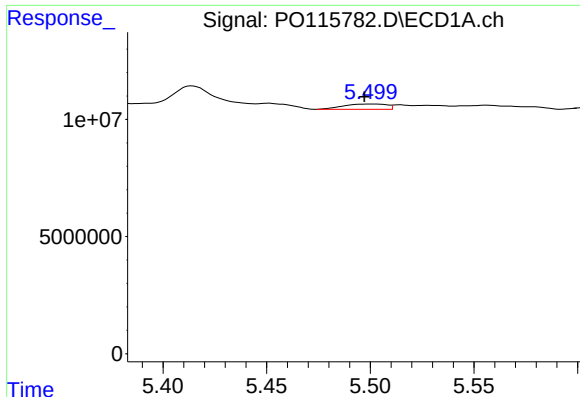

#13 AR-1232-3


R.T.: 5.500 min
Delta R.T.: 0.003 min
Response: 3263960
Conc: 21.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

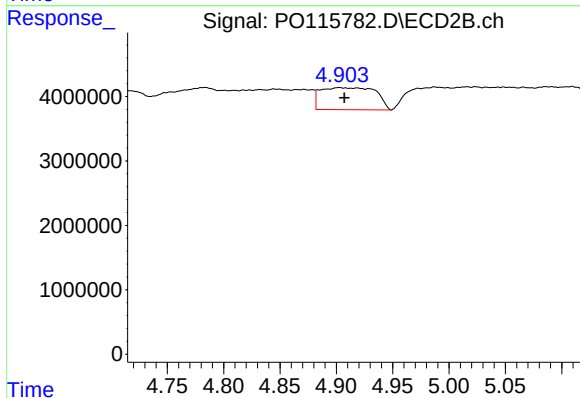


#13 AR-1232-3

R.T.: 4.903 min
Delta R.T.: -0.004 min
Response: 11596725
Conc: 177.41 ng/ml

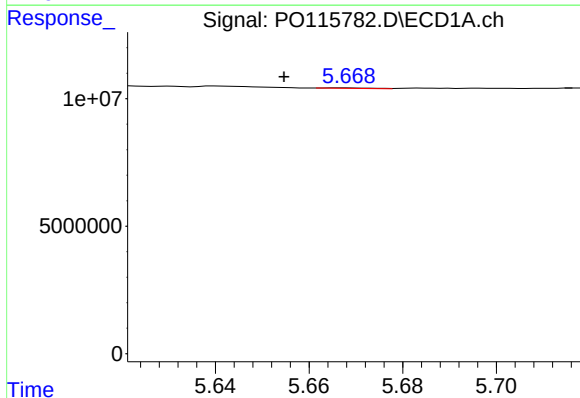


#14 AR-1232-4

R.T.: 5.667 min
Delta R.T.: 0.012 min
Response: 153503
Conc: 2.19 ng/ml

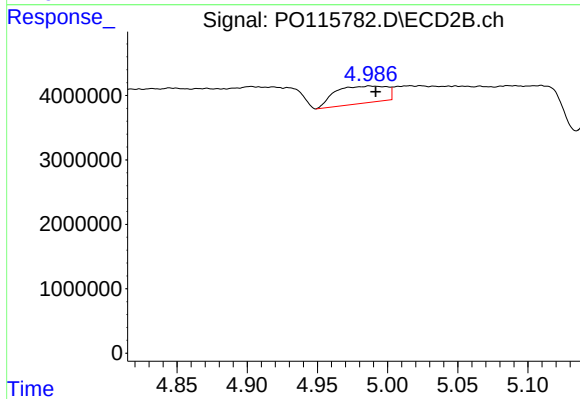

#14 AR-1232-4


R.T.: 4.987 min
Delta R.T.: -0.004 min
Response: 6795853
Conc: 132.39 ng/ml

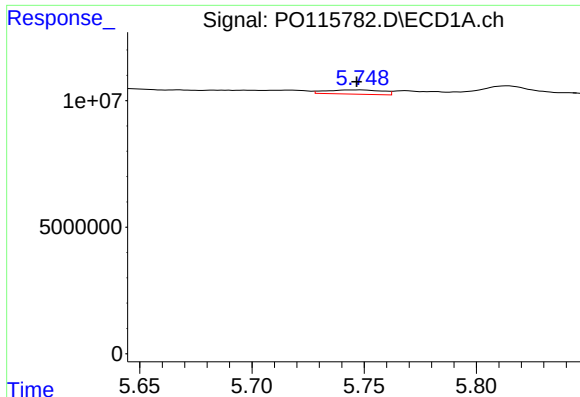

#15 AR-1232-5


R.T.: 5.748 min
Delta R.T.: 0.001 min
Response: 2950855
Conc: 56.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

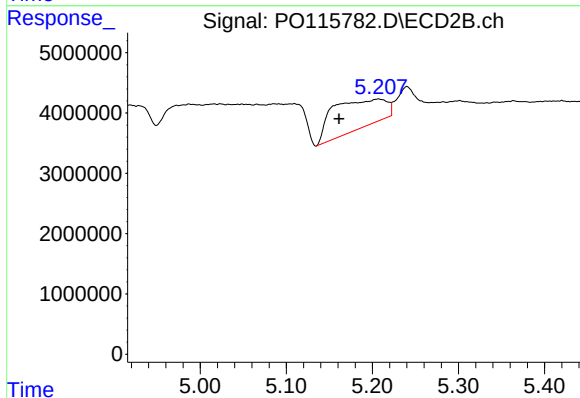


#15 AR-1232-5

R.T.: 5.207 min
Delta R.T.: 0.046 min
Response: 20577997
Conc: 375.87 ng/ml

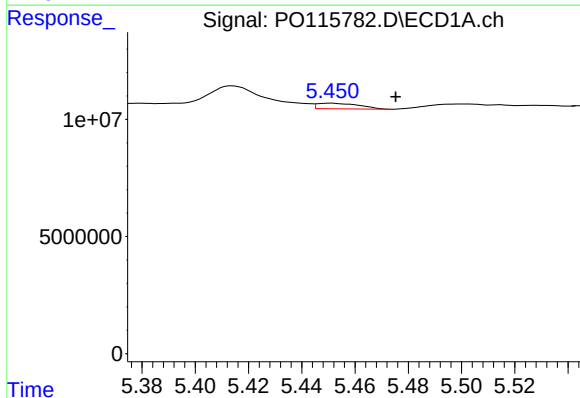


#16 AR-1242-1

R.T.: 5.451 min
Delta R.T.: -0.024 min
Response: 2579148
Conc: 12.99 ng/ml

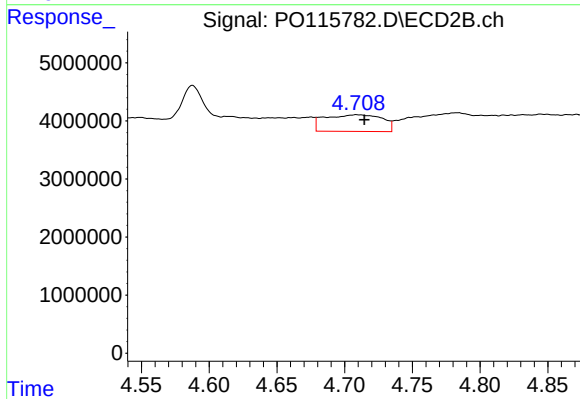

#16 AR-1242-1


R.T.: 4.709 min
Delta R.T.: -0.006 min
Response: 8459693
Conc: 59.41 ng/ml

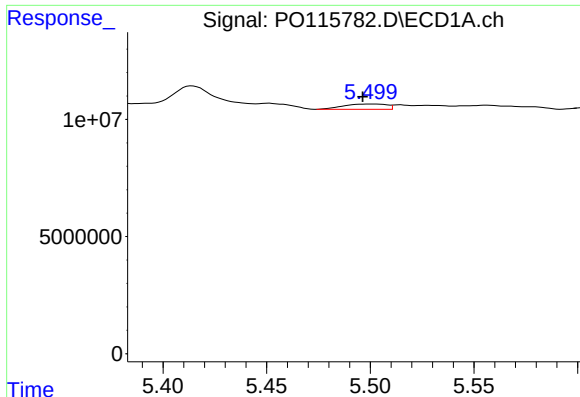

#17 AR-1242-2


R.T.: 5.500 min
Delta R.T.: 0.003 min
Response: 3263960
Conc: 11.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

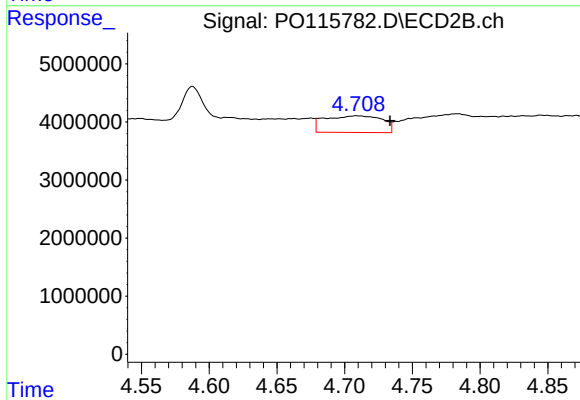


#17 AR-1242-2

R.T.: 4.709 min
Delta R.T.: -0.025 min
Response: 8459693
Conc: 40.41 ng/ml

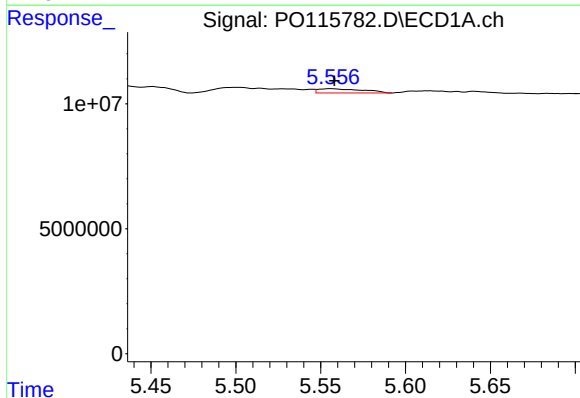


#18 AR-1242-3

R.T.: 5.556 min
Delta R.T.: -0.002 min
Response: 3135158
Conc: 18.57 ng/ml

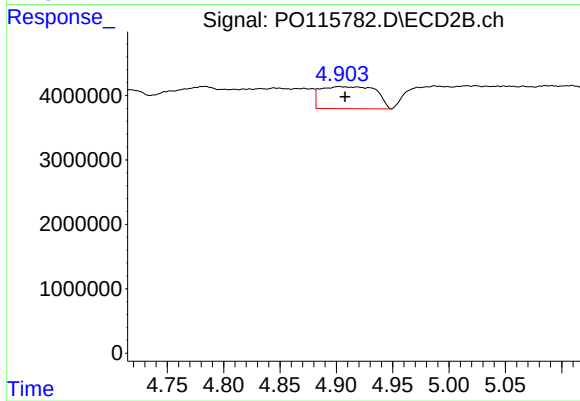

#18 AR-1242-3


R.T.: 4.903 min
Delta R.T.: -0.005 min
Response: 11596725
Conc: 97.09 ng/ml

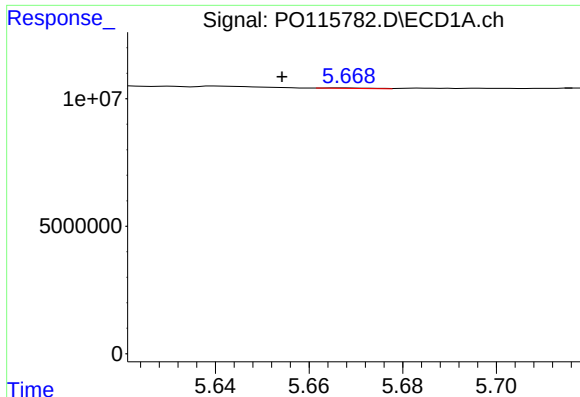

#19 AR-1242-4


R.T.: 5.667 min
Delta R.T.: 0.013 min
Response: 153503
Conc: 1.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

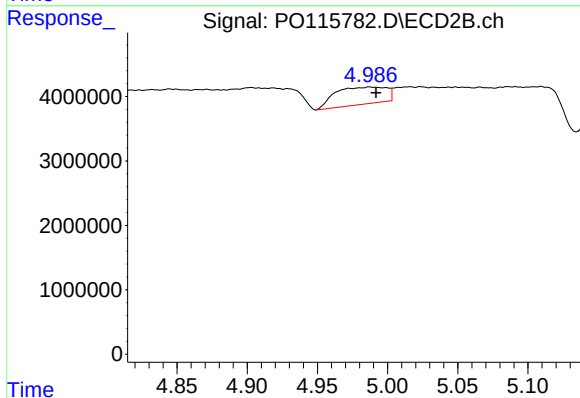


#19 AR-1242-4

R.T.: 4.987 min
Delta R.T.: -0.005 min
Response: 6795853
Conc: 62.29 ng/ml

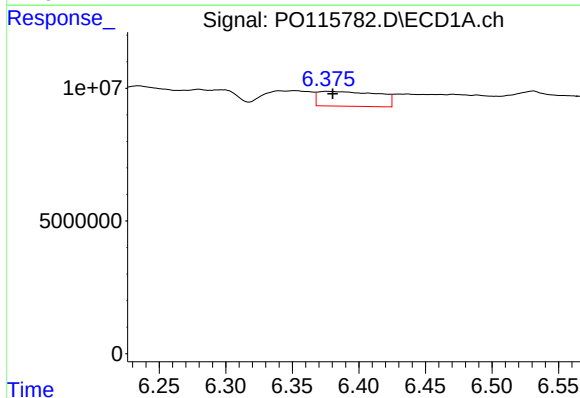


#20 AR-1242-5

R.T.: 6.376 min
Delta R.T.: -0.004 min
Response: 17616827
Conc: 116.33 ng/ml

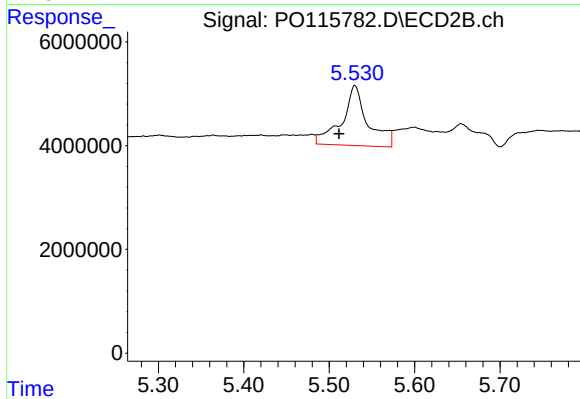

#20 AR-1242-5


R.T.: 5.530 min
Delta R.T.: 0.018 min
Response: 24565931
Conc: 177.85 ng/ml

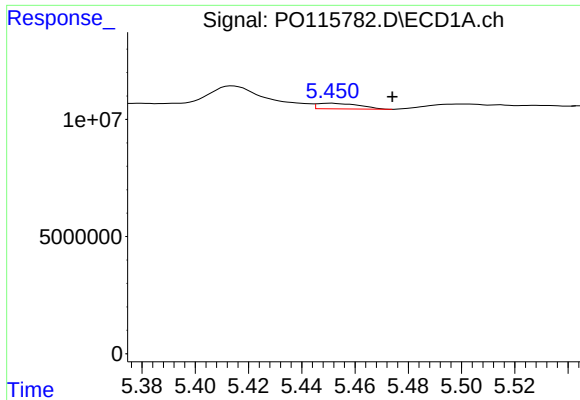

#21 AR-1248-1


R.T.: 5.451 min
Delta R.T.: -0.023 min
Response: 2579148
Conc: 16.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

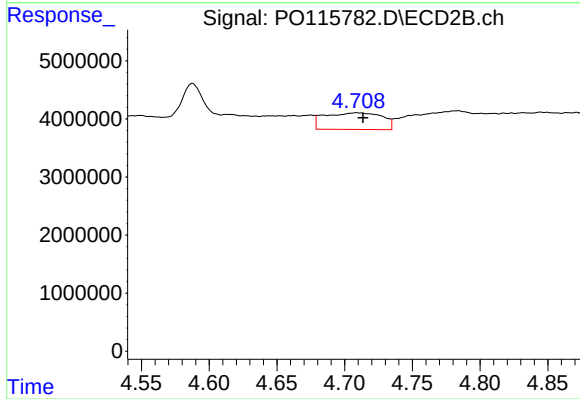


#21 AR-1248-1

R.T.: 4.709 min
Delta R.T.: -0.005 min
Response: 8459693
Conc: 75.65 ng/ml

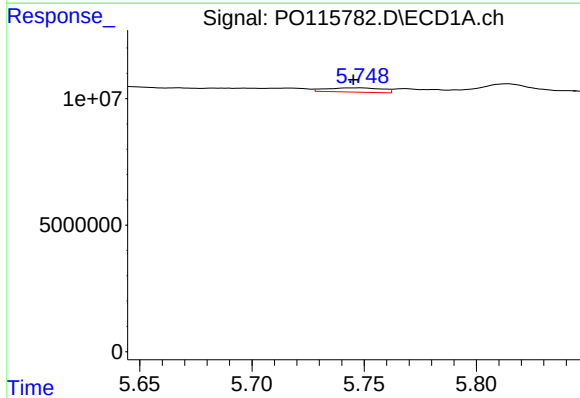


#22 AR-1248-2

R.T.: 5.748 min
Delta R.T.: 0.003 min
Response: 2950855
Conc: 14.69 ng/ml

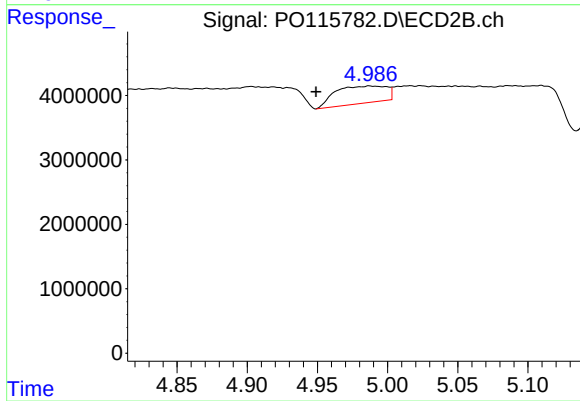

#22 AR-1248-2


R.T.: 4.987 min
Delta R.T.: 0.038 min
Response: 6795853
Conc: 44.62 ng/ml

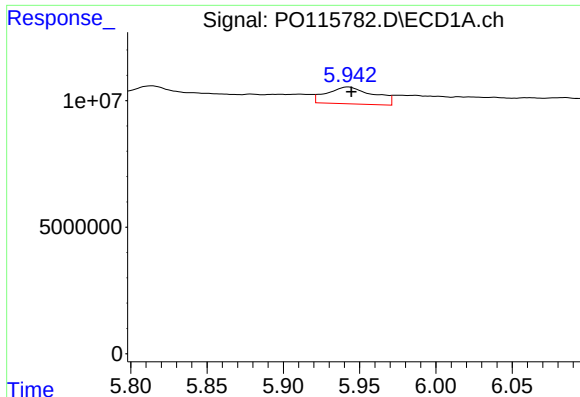

#23 AR-1248-3


R.T.: 5.943 min
Delta R.T.: -0.002 min
Response: 14228548
Conc: 57.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

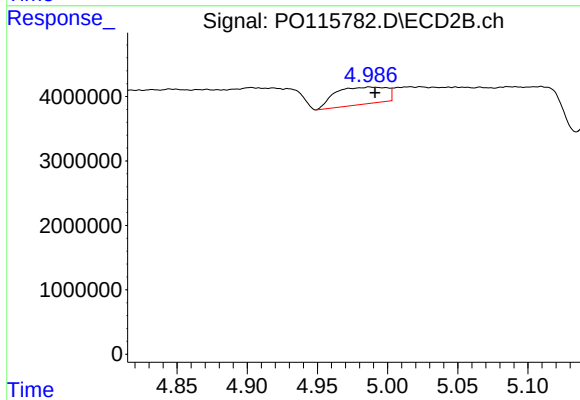


#23 AR-1248-3

R.T.: 4.987 min
Delta R.T.: -0.004 min
Response: 6795853
Conc: 42.33 ng/ml

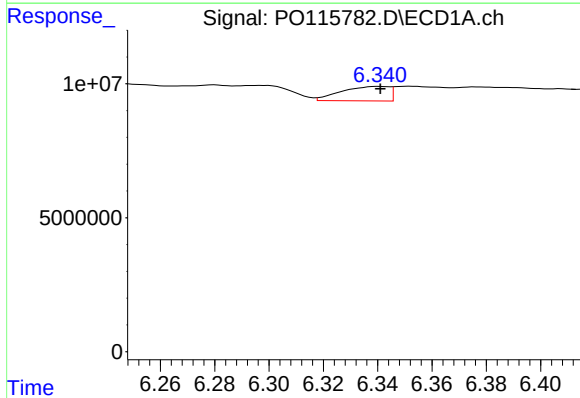


#24 AR-1248-4

R.T.: 6.341 min
Delta R.T.: 0.000 min
Response: 6594496
Conc: 22.37 ng/ml

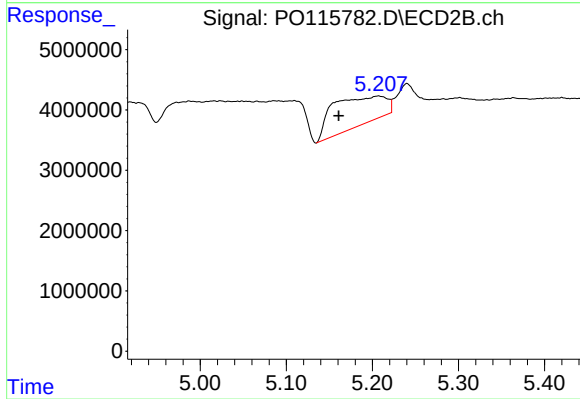

#24 AR-1248-4


R.T.: 5.207 min
Delta R.T.: 0.046 min
Response: 20577997
Conc: 109.96 ng/ml

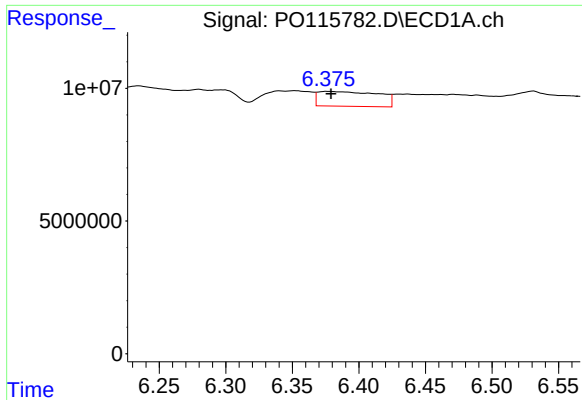

#25 AR-1248-5


R.T.: 6.376 min
Delta R.T.: -0.003 min
Response: 17616827
Conc: 68.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

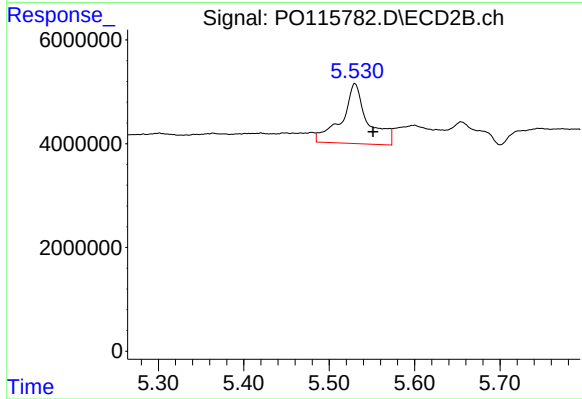


#25 AR-1248-5

R.T.: 5.530 min
Delta R.T.: -0.021 min
Response: 24565931
Conc: 124.10 ng/ml

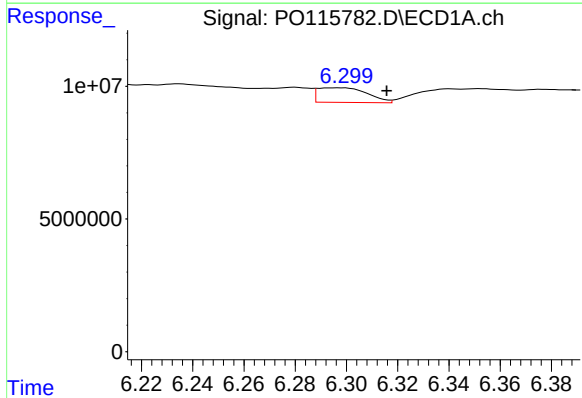


#26 AR-1254-1

R.T.: 6.298 min
Delta R.T.: -0.018 min
Response: 7424368
Conc: 28.70 ng/ml

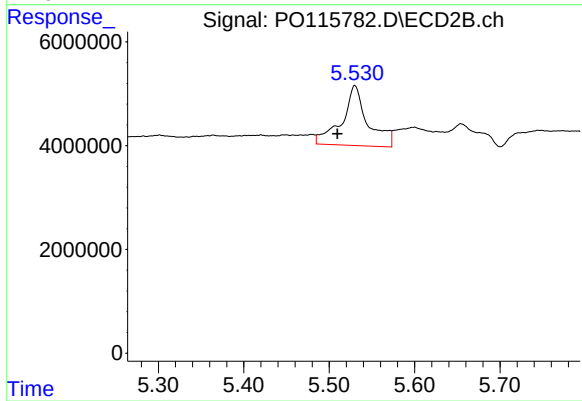

#26 AR-1254-1


R.T.: 5.530 min
Delta R.T.: 0.021 min
Response: 24565931
Conc: 84.05 ng/ml

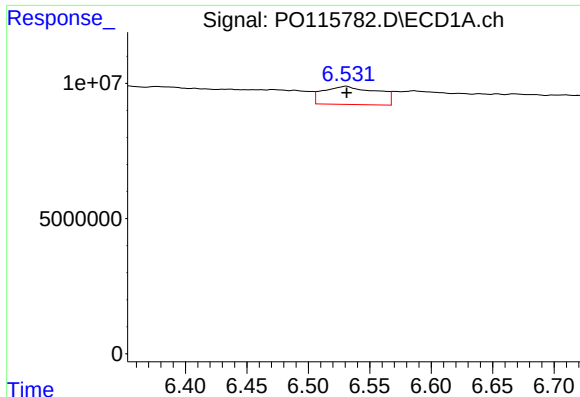

#27 AR-1254-2


R.T.: 6.531 min
Delta R.T.: 0.000 min
Response: 20455137
Conc: 50.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

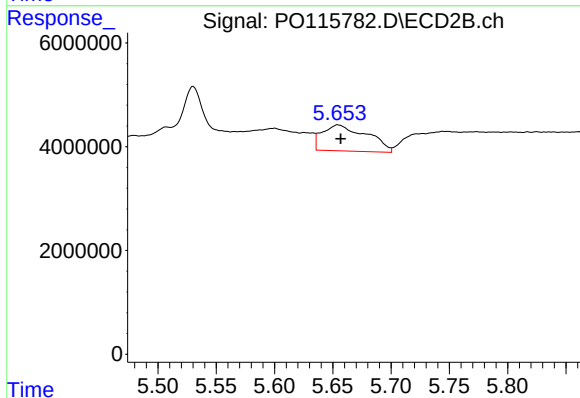


#27 AR-1254-2

R.T.: 5.654 min
Delta R.T.: -0.002 min
Response: 13442588
Conc: 53.38 ng/ml

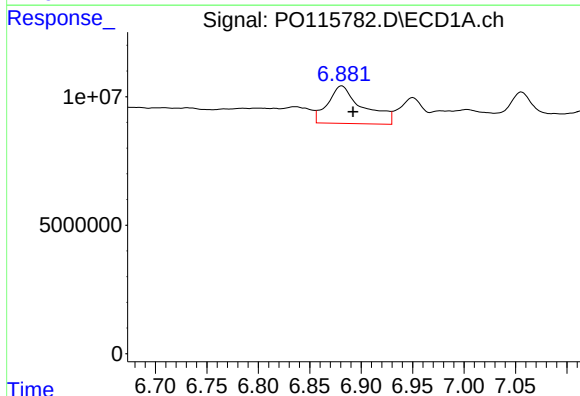


#28 AR-1254-3

R.T.: 6.881 min
Delta R.T.: -0.011 min
Response: 34736075
Conc: 84.61 ng/ml

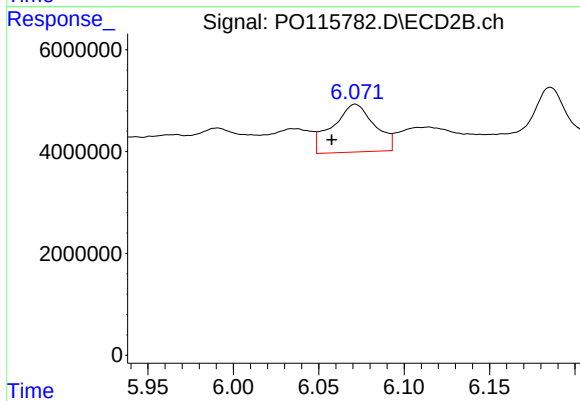

#28 AR-1254-3


R.T.: 6.071 min
Delta R.T.: 0.014 min
Response: 16092572
Conc: 40.89 ng/ml

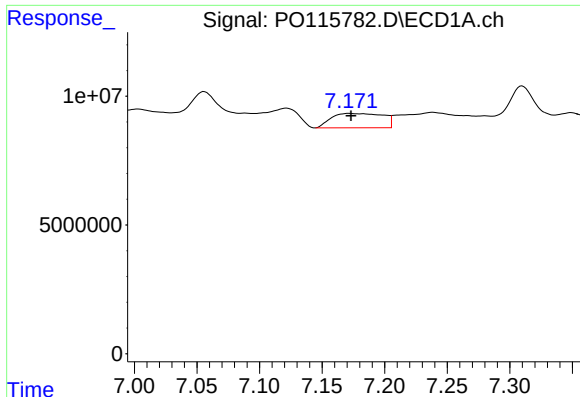

#29 AR-1254-4


R.T.: 7.172 min
Delta R.T.: -0.001 min
Response: 15999268
Conc: 46.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

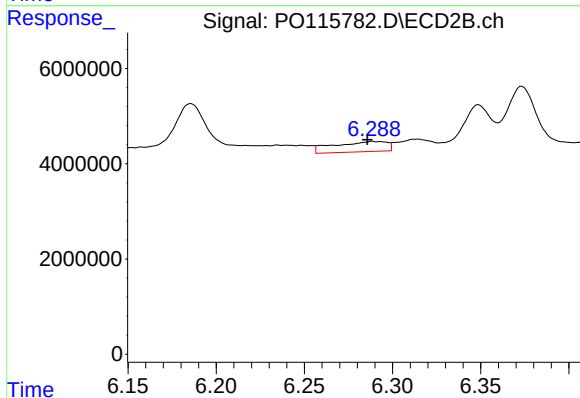


#29 AR-1254-4

R.T.: 6.289 min
Delta R.T.: 0.003 min
Response: 4500569
Conc: 16.82 ng/ml

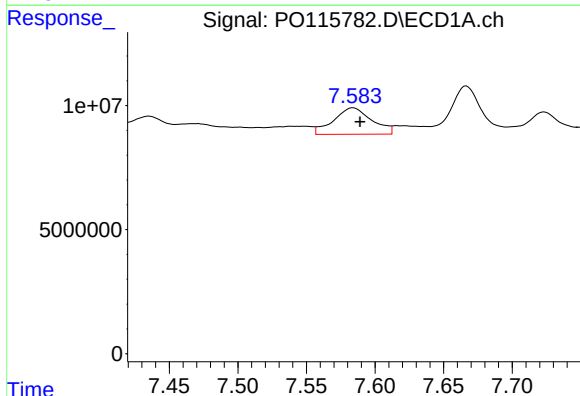


#30 AR-1254-5

R.T.: 7.584 min
Delta R.T.: -0.005 min
Response: 20766577
Conc: 64.09 ng/ml

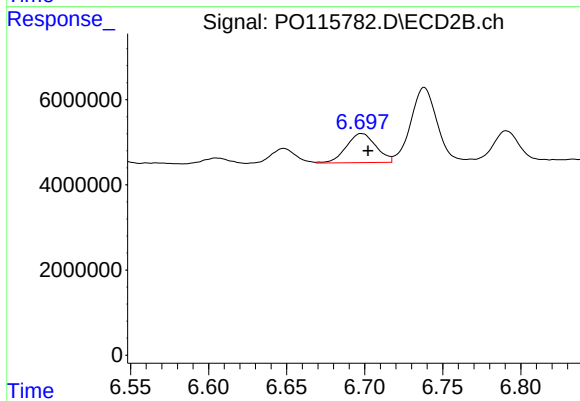

#30 AR-1254-5


R.T.: 6.698 min
Delta R.T.: -0.004 min
Response: 9057099
Conc: 25.33 ng/ml

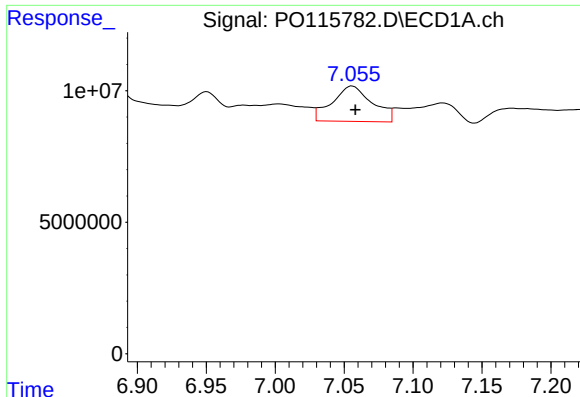

#31 AR-1260-1


R.T.: 7.056 min
Delta R.T.: -0.002 min
Response: 27336178
Conc: 94.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

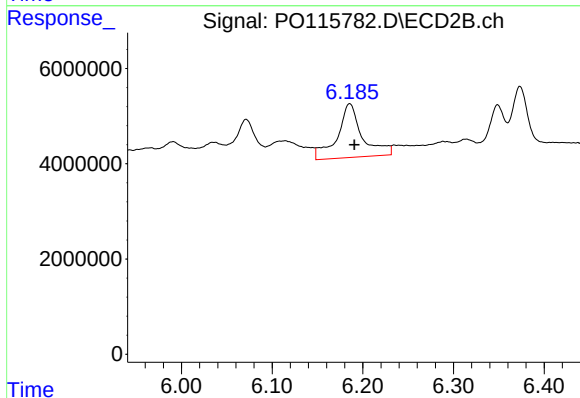


#31 AR-1260-1

R.T.: 6.186 min
Delta R.T.: -0.005 min
Response: 21518356
Conc: 82.08 ng/ml

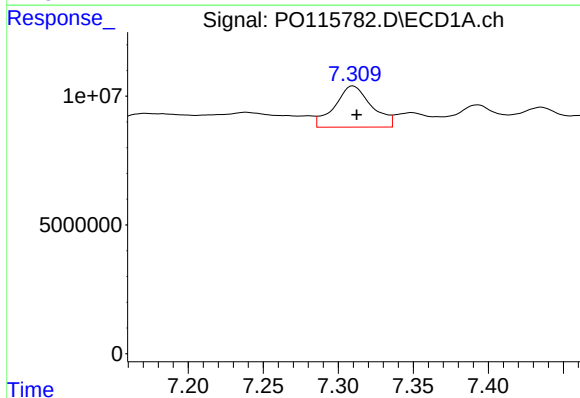


#32 AR-1260-2

R.T.: 7.310 min
Delta R.T.: -0.002 min
Response: 27486077
Conc: 62.79 ng/ml

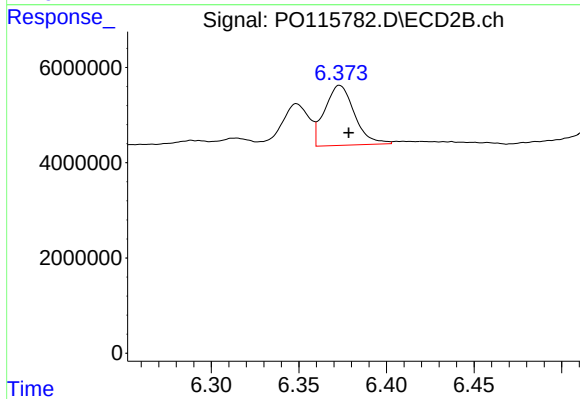

#32 AR-1260-2


R.T.: 6.373 min
Delta R.T.: -0.005 min
Response: 14920255
Conc: 42.57 ng/ml

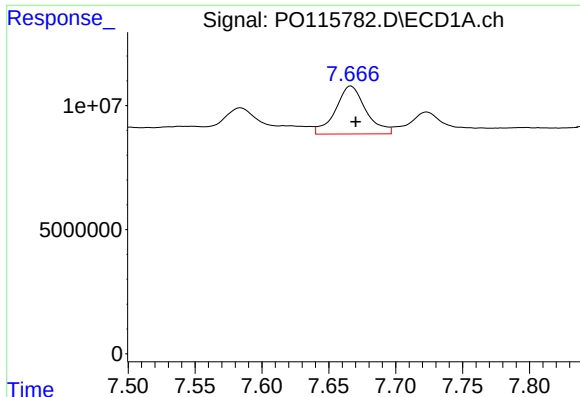

#33 AR-1260-3


R.T.: 7.667 min
Delta R.T.: -0.004 min
Response: 30637482
Conc: 91.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

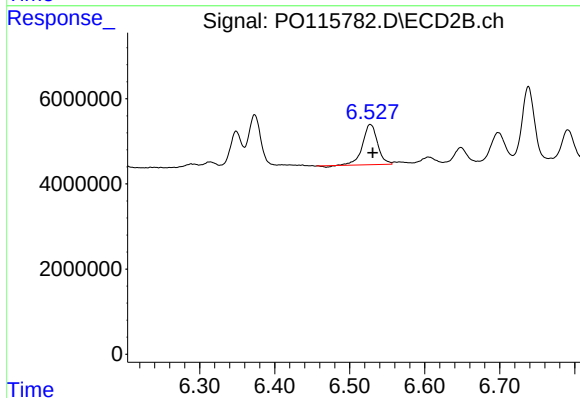


#33 AR-1260-3

R.T.: 6.528 min
Delta R.T.: -0.003 min
Response: 13047937
Conc: 40.61 ng/ml

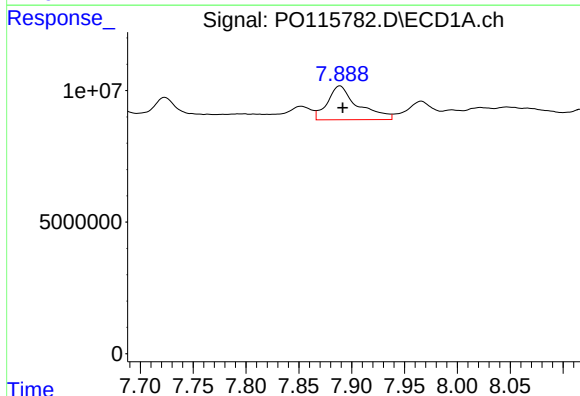


#34 AR-1260-4

R.T.: 7.889 min
Delta R.T.: -0.002 min
Response: 25648290
Conc: 83.42 ng/ml

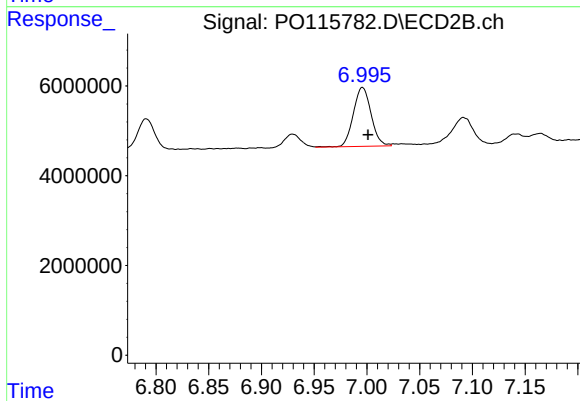

#34 AR-1260-4


R.T.: 6.996 min
Delta R.T.: -0.005 min
Response: 15371783
Conc: 59.85 ng/ml

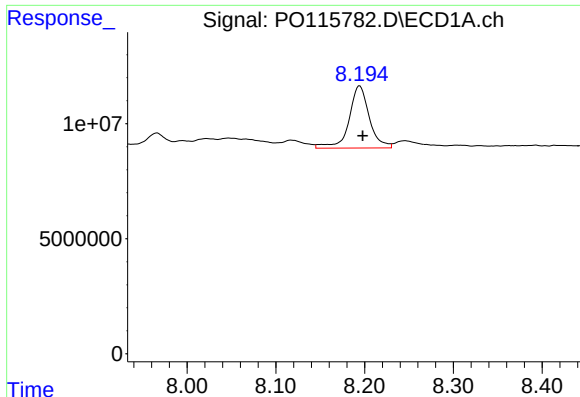

#35 AR-1260-5


R.T.: 8.194 min
Delta R.T.: -0.004 min
Response: 42827889
Conc: 58.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

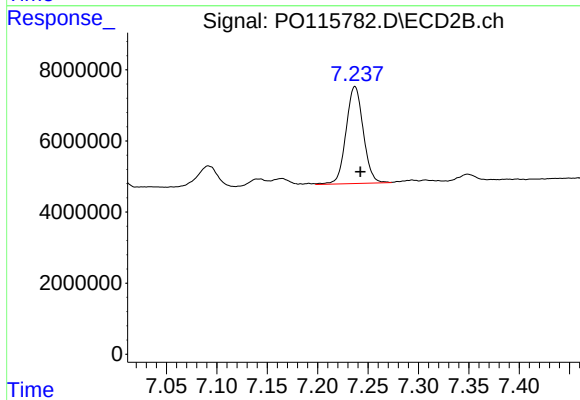


#35 AR-1260-5

R.T.: 7.237 min
Delta R.T.: -0.005 min
Response: 32437843
Conc: 46.26 ng/ml

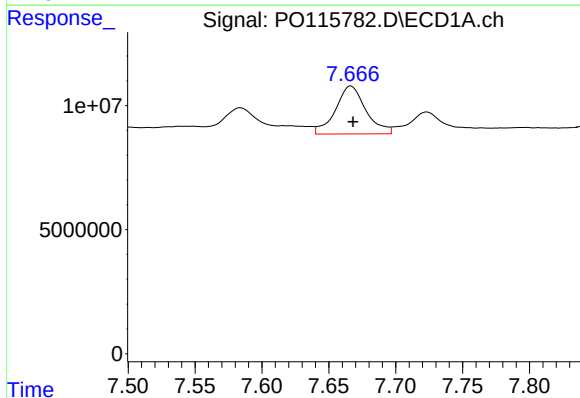


#36 AR-1262-1

R.T.: 7.667 min
Delta R.T.: -0.002 min
Response: 30637482
Conc: 124.11 ng/ml

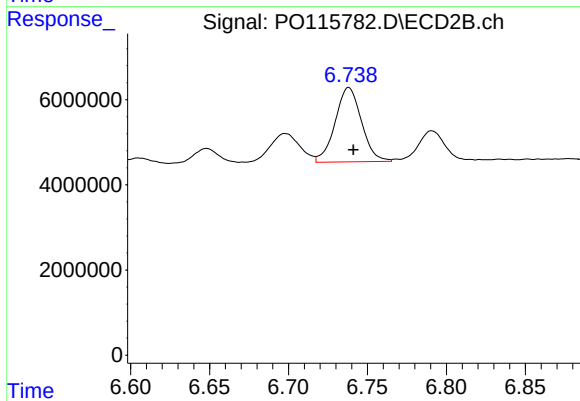

#36 AR-1262-1


R.T.: 6.738 min
Delta R.T.: -0.003 min
Response: 20308956
Conc: 95.33 ng/ml

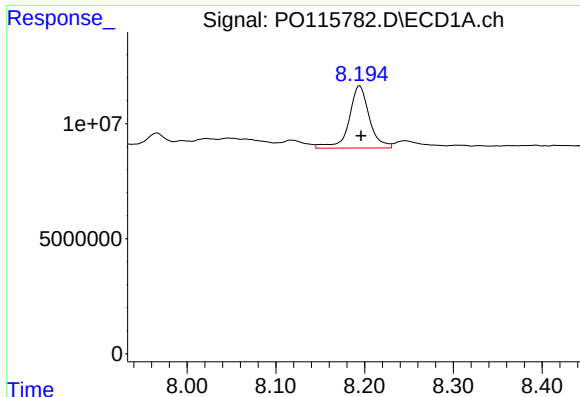

#37 AR-1262-2


R.T.: 8.194 min
Delta R.T.: -0.002 min
Response: 42827889
Conc: 108.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

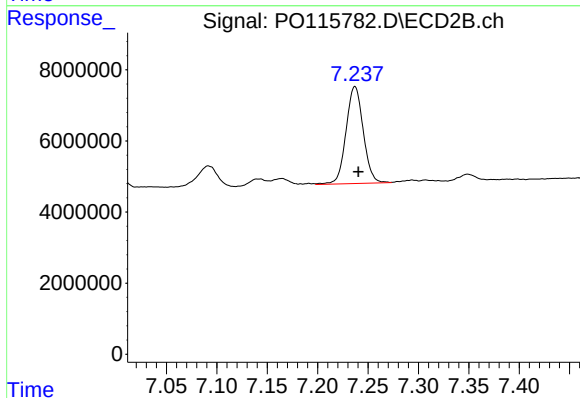


#37 AR-1262-2

R.T.: 7.237 min
Delta R.T.: -0.004 min
Response: 32437843
Conc: 93.12 ng/ml

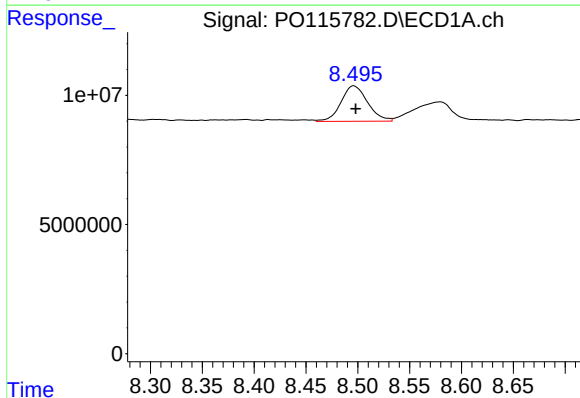


#38 AR-1262-3

R.T.: 8.496 min
Delta R.T.: -0.002 min
Response: 24545606
Conc: 96.32 ng/ml

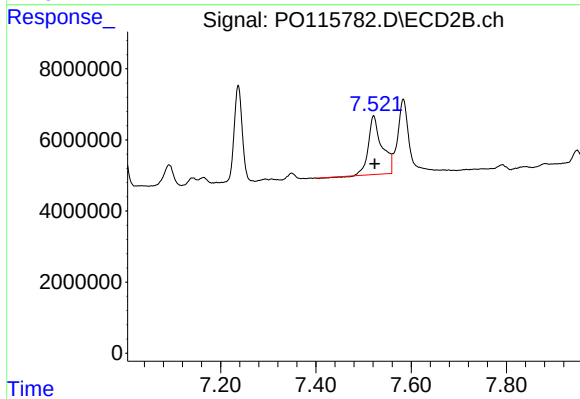

#38 AR-1262-3


R.T.: 7.521 min
Delta R.T.: -0.003 min
Response: 32402055
Conc: 207.19 ng/ml

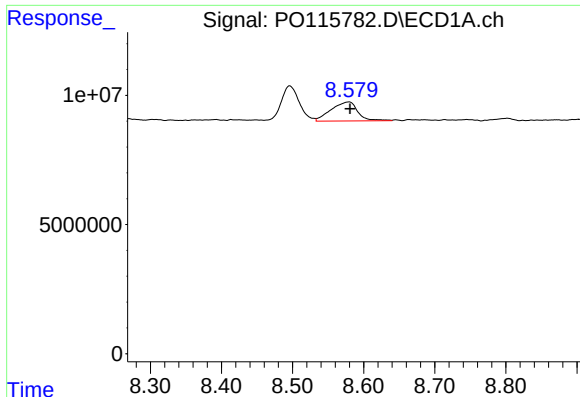

#39 AR-1262-4


R.T.: 8.579 min
Delta R.T.: -0.002 min
Response: 19351404
Conc: 99.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

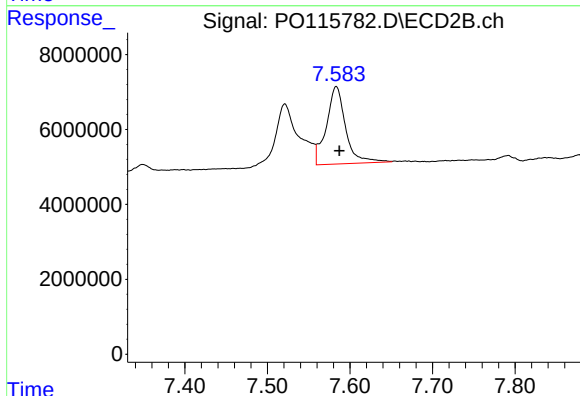


#39 AR-1262-4

R.T.: 7.583 min
Delta R.T.: -0.004 min
Response: 33571167
Conc: 135.71 ng/ml

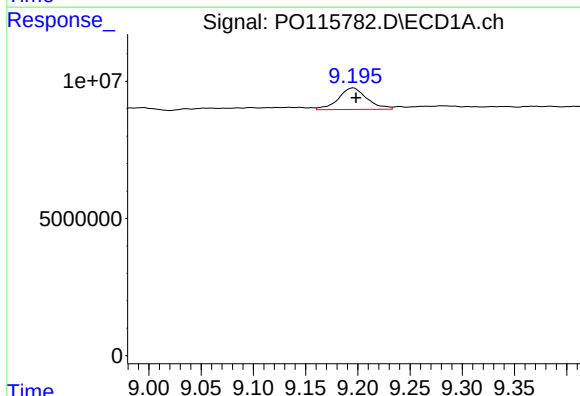


#40 AR-1262-5

R.T.: 9.196 min
Delta R.T.: -0.003 min
Response: 14985830
Conc: 111.26 ng/ml

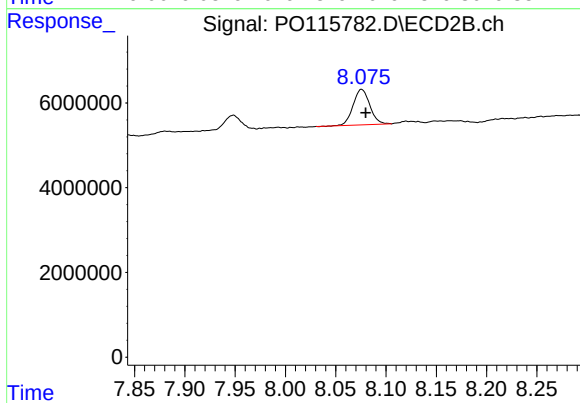

#40 AR-1262-5


R.T.: 8.076 min
Delta R.T.: -0.004 min
Response: 9665522
Conc: 86.71 ng/ml

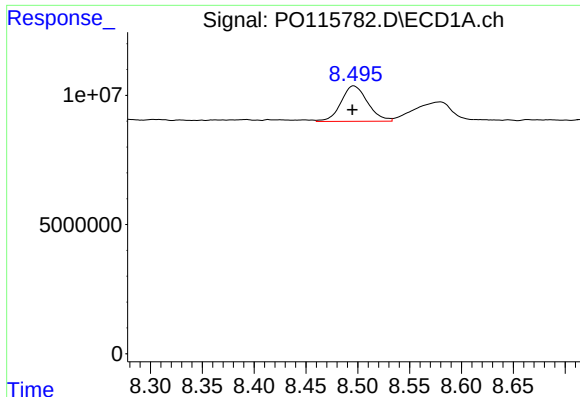

#41 AR-1268-1


R.T.: 8.496 min
Delta R.T.: 0.001 min
Response: 24545606
Conc: 24.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

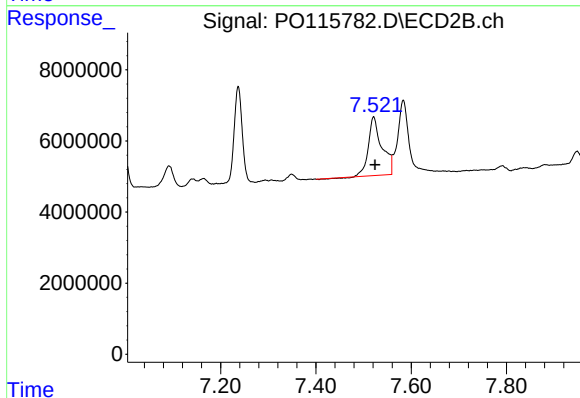


#41 AR-1268-1

R.T.: 7.521 min
Delta R.T.: -0.003 min
Response: 32402055
Conc: 36.57 ng/ml

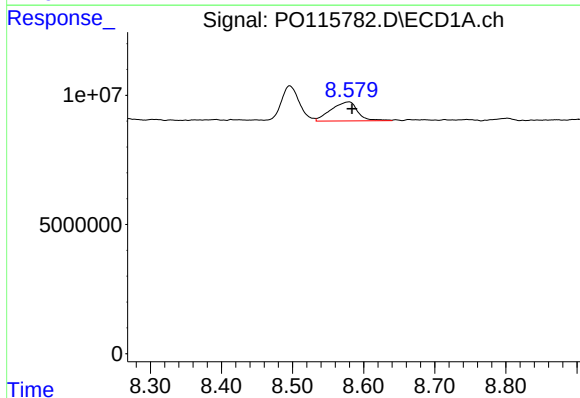


#42 AR-1268-2

R.T.: 8.579 min
Delta R.T.: -0.004 min
Response: 19351404
Conc: 22.62 ng/ml

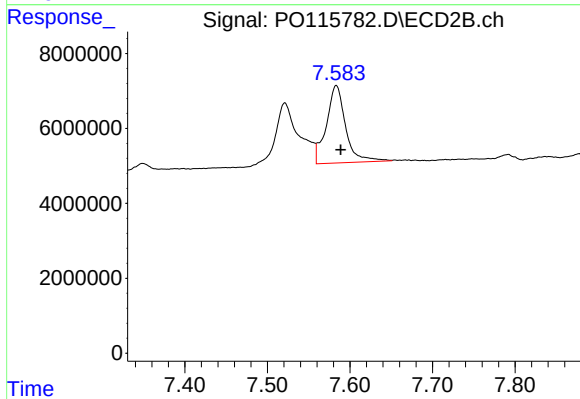

#42 AR-1268-2


R.T.: 7.583 min
Delta R.T.: -0.005 min
Response: 33571167
Conc: 44.82 ng/ml

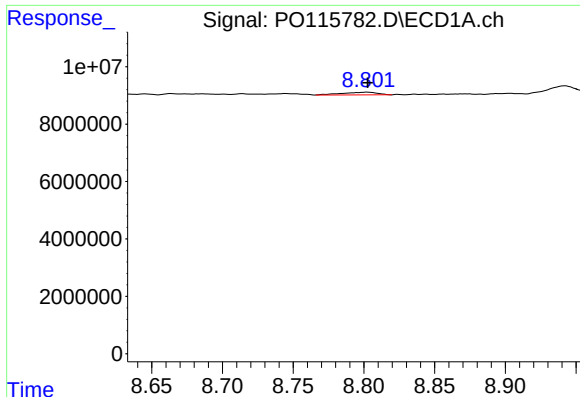

#43 AR-1268-3


R.T.: 8.802 min
Delta R.T.: 0.000 min
Response: 1632002
Conc: 2.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

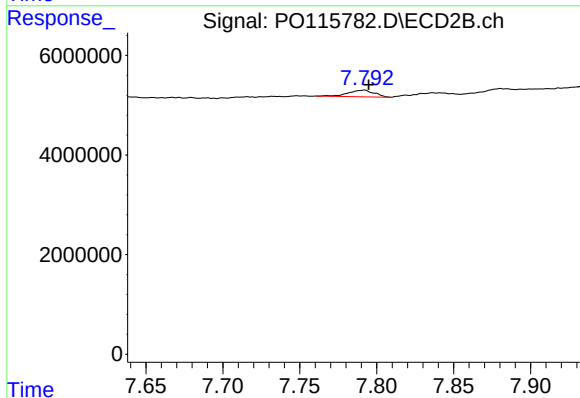


#43 AR-1268-3

R.T.: 7.792 min
Delta R.T.: -0.003 min
Response: 1595832
Conc: 2.51 ng/ml

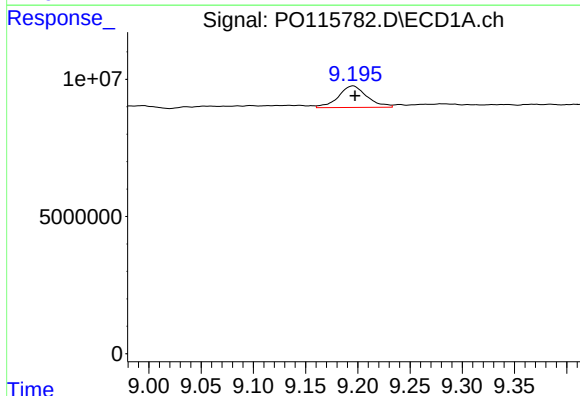


#44 AR-1268-4

R.T.: 9.196 min
Delta R.T.: -0.002 min
Response: 14985830
Conc: 48.00 ng/ml

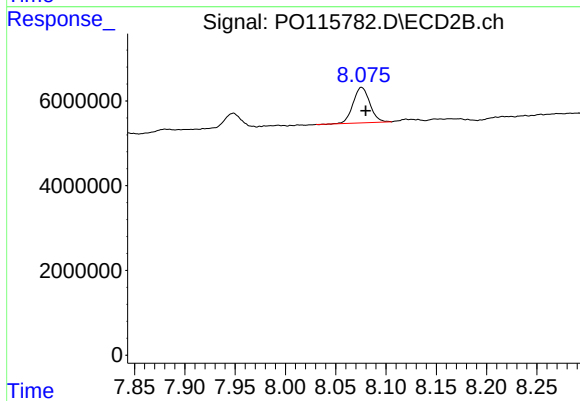

#44 AR-1268-4


R.T.: 8.076 min
Delta R.T.: -0.004 min
Response: 9665522
Conc: 37.52 ng/ml

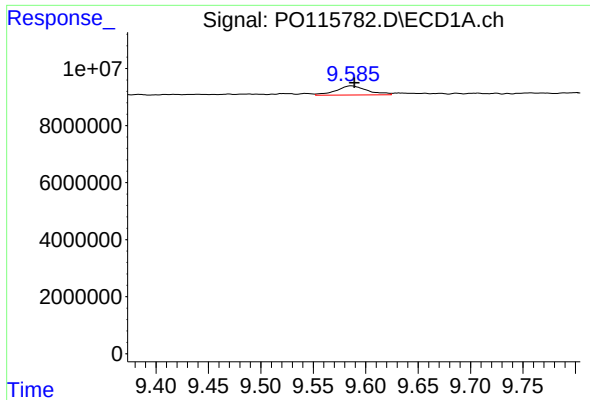

#45 AR-1268-5

R.T.: 9.586 min
Delta R.T.: -0.003 min
Response: 6755918
Conc: 3.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

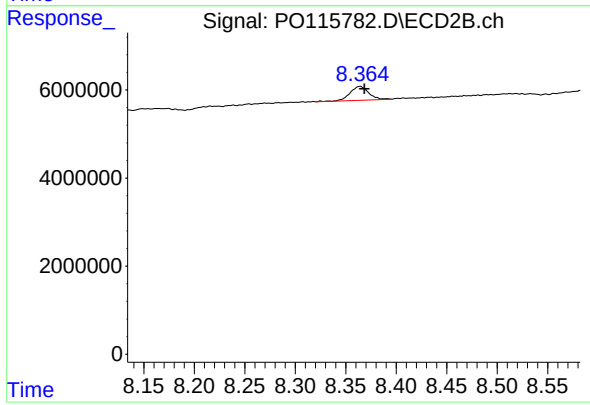

#45 AR-1268-5

R.T.: 8.364 min
Delta R.T.: -0.005 min
Response: 4098586
Conc: 2.43 ng/ml