

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121225\
 Data File : PO115800.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Dec 2025 12:36
 Operator : YP/AJ
 Sample : Q3530-07
 Misc : AR1248 40PPB WATER LOD
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 02:18:28 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 05 02:11:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.333	3.636	170.5E6	104.8E6	21.947	21.514
2)	SA Decachlor...	9.907	8.616	122.6E6	91179089	23.303	21.203
Target Compounds							
3)	L1 AR-1016-1	5.472	4.710	6233765	4894351	25.069	26.490
4)	L1 AR-1016-2	5.493	4.728	8251414	4734813	21.666	17.914
5)	L1 AR-1016-3	5.555	4.905	4383394	3256282	20.504	21.517
6)	L1 AR-1016-4	5.650	4.945	3587220	5844263	20.088	51.855 #
7)	L1 AR-1016-5	5.941	5.157	10903501	11159157	62.154	76.254
8)	L2 AR-1221-1	4.528	3.844	3534912	50910	43.535	0.903 #
9)	L2 AR-1221-2	4.629	3.932	3336301	1997885	52.941	47.071
10)	L2 AR-1221-3	4.692	4.006	1714591	357061	9.183	2.777 #
11)	L3 AR-1232-1	4.692	4.006	1714591	357061	11.456	3.342 #
12)	L3 AR-1232-2	5.208	4.728	4007250	4734813	49.564	42.660
13)	L3 AR-1232-3	5.493	4.905	8251414	3256282	53.614	49.816
14)	L3 AR-1232-4	5.650	4.987	3587220	6657225	51.224	129.694 #
15)	L3 AR-1232-5	5.742	5.157	8437107	11159157	162.448	203.827 #
16)	L4 AR-1242-1	5.472	4.710	6233765	4894351	31.385	34.373
17)	L4 AR-1242-2	5.493	4.728	8251414	4734813	28.172	22.615
18)	L4 AR-1242-3	5.555	4.905	4383394	3256282	25.966	27.262
19)	L4 AR-1242-4	5.650	4.987	3587220	6657225	26.248	61.024 #
20)	L4 AR-1242-5	6.377	5.507	14098484	12050597	93.094	87.244
21)	L5 AR-1248-1	5.472	4.710	6233765	4894351	41.075	43.766
22)	L5 AR-1248-2	5.742	4.945	8437107	5844263	42.014	38.376
23)	L5 AR-1248-3	5.941	4.987	10903501	6657225	44.215	41.471
24)	L5 AR-1248-4	6.339	5.157	12778187	11159157	43.337	59.628 #
25)	L5 AR-1248-5	6.377	5.547	14098484	9897470	54.450	49.999
26)	L6 AR-1254-1	6.311	5.507	10384915	12050597	40.141	41.231
27)	L6 AR-1254-2	6.531	5.655	11422618	5210390	28.386	20.692 #
28)	L6 AR-1254-3	6.883	6.055	20886791	6504313	50.873	16.526 #
29)	L6 AR-1254-4	7.174	6.283	7910365	4045695	22.792	15.120 #
30)	L6 AR-1254-5	7.590	6.701	1016144	1411143	3.136	3.947 #
31)	L7 AR-1260-1	7.058	6.199	3678147	2539936	12.696	9.688
32)	L7 AR-1260-2	7.312	6.349	684304	9419685	1.563	26.879 #
33)	L7 AR-1260-3	7.681	6.525	239662	1502034	0.712	4.675 #
34)	L7 AR-1260-4	7.893	6.990	529250	284223	1.721	1.107 #
35)	L7 AR-1260-5	8.193	7.239	1419757	1089548	1.949	1.554
36)	L8 AR-1262-1	7.681	6.738	239662	485844	0.971	2.281 #
37)	L8 AR-1262-2	8.193	7.239	1419757	1089548	3.586	3.128
38)	L8 AR-1262-3	8.498	7.536	964471	54060905	3.785	345.679 #
39)	L8 AR-1262-4	8.585	7.536f	176976	54060905	0.914	218.541 #
40)	L8 AR-1262-5	9.191	8.055	606731	80804	4.505	0.725 #
41)	L9 AR-1268-1	8.498	7.536	964471	54060905	0.969	61.020 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121225\
 Data File : PO115800.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Dec 2025 12:36
 Operator : YP/AJ
 Sample : Q3530-07
 Misc : AR1248 40PPB WATER LOD
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 02:18:28 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 05 02:11:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.585	7.536f	176976	54060905	0.207	72.171 #
43) L9	AR-1268-3	8.804	7.793	190434	410908	0.256	0.645 #
44) L9	AR-1268-4	9.191	8.055	606731	80804	1.943	0.314 #
45) L9	AR-1268-5	9.588	8.371	1163782	185454	0.534	0.110 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO121225\
Data File : PO115800.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Dec 2025 12:36
Operator : YP/AJ
Sample : Q3530-07
Misc : AR1248 40PPB WATER LOD
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_0
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 02:18:28 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO120425.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 05 02:11:05 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

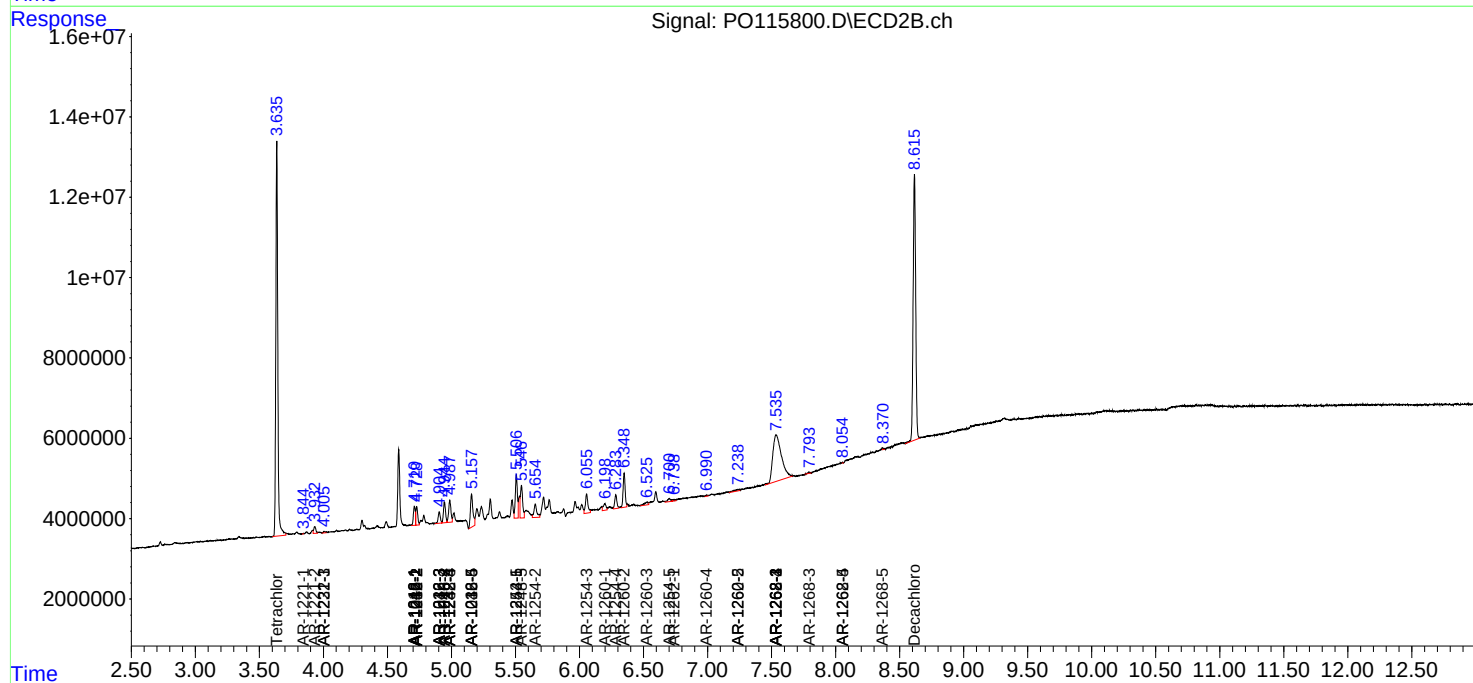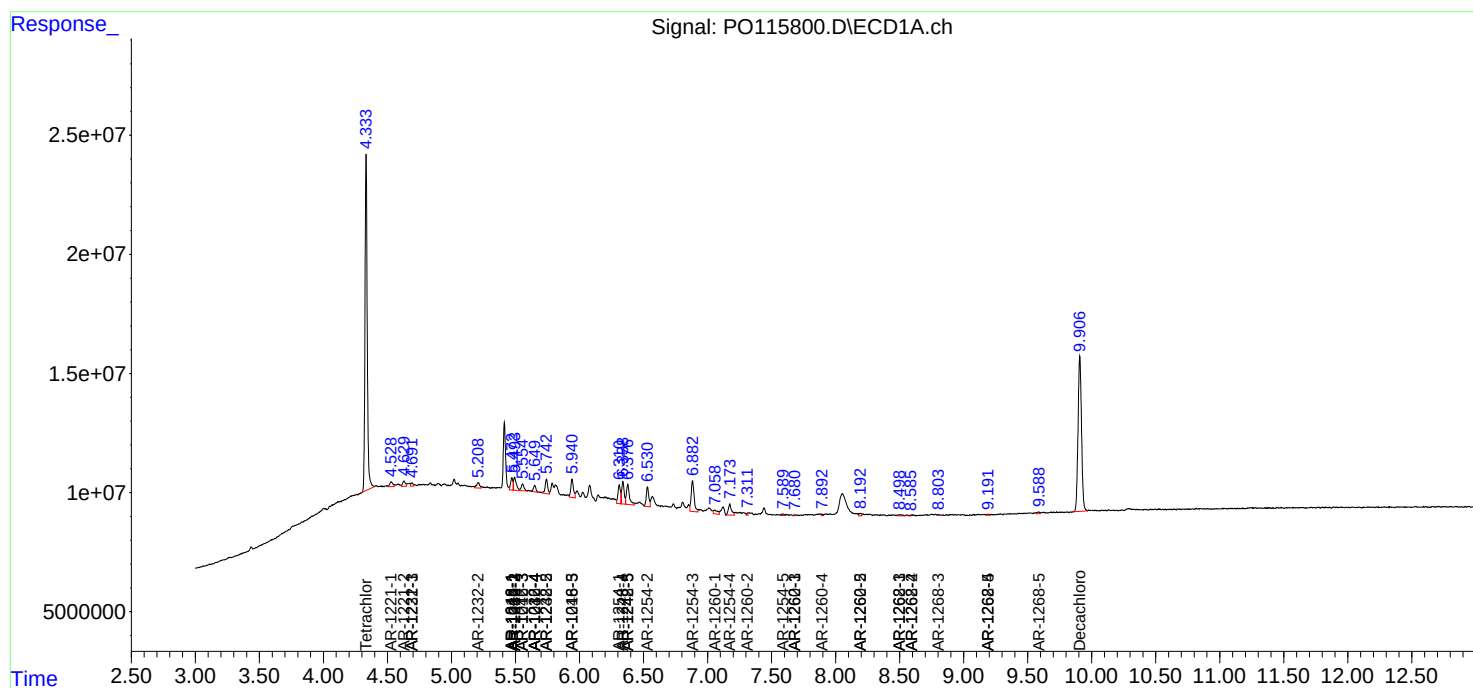


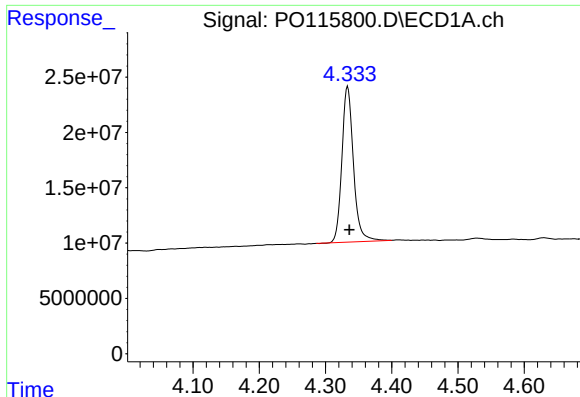

#1 Tetrachloro-m-xylene


R.T.: 4.333 min
Delta R.T.: -0.003 min
Response: 170468155
Conc: 21.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

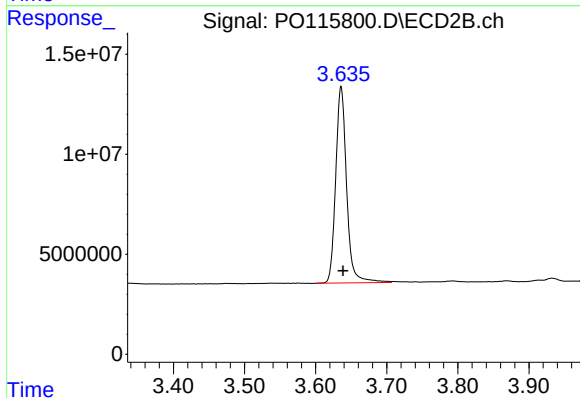


#1 Tetrachloro-m-xylene

R.T.: 3.636 min
Delta R.T.: -0.003 min
Response: 104844985
Conc: 21.51 ng/ml

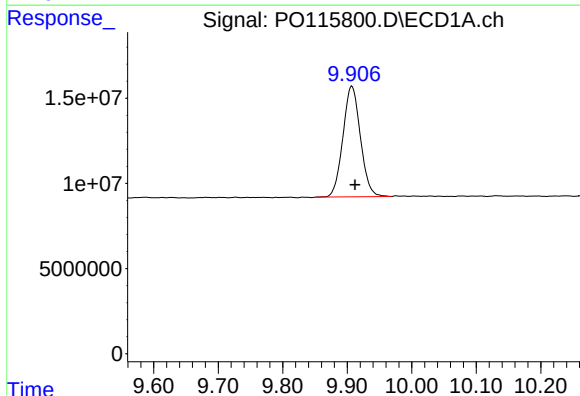


#2 Decachlorobiphenyl

R.T.: 9.907 min
Delta R.T.: -0.005 min
Response: 122599242
Conc: 23.30 ng/ml

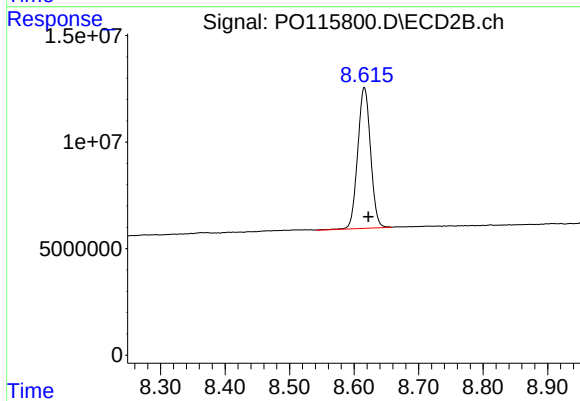

#2 Decachlorobiphenyl


R.T.: 8.616 min
Delta R.T.: -0.006 min
Response: 91179089
Conc: 21.20 ng/ml

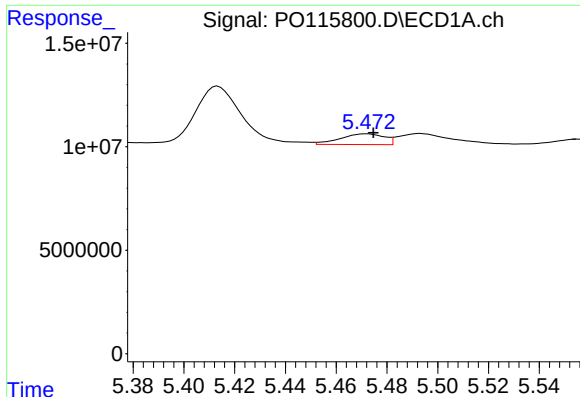

#3 AR-1016-1


R.T.: 5.472 min
Delta R.T.: -0.002 min
Response: 6233765
Conc: 25.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

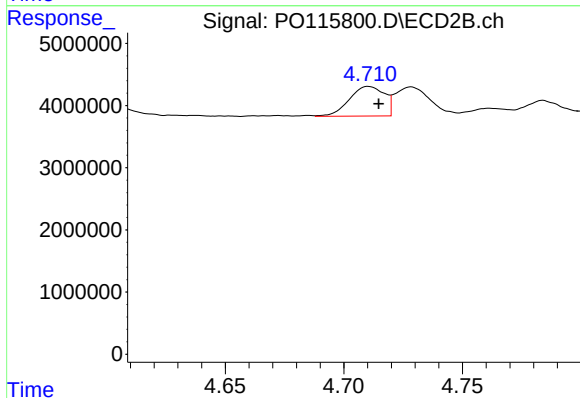


#3 AR-1016-1

R.T.: 4.710 min
Delta R.T.: -0.004 min
Response: 4894351
Conc: 26.49 ng/ml

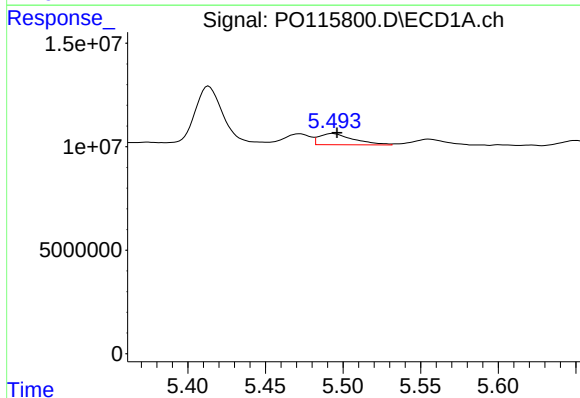


#4 AR-1016-2

R.T.: 5.493 min
Delta R.T.: -0.003 min
Response: 8251414
Conc: 21.67 ng/ml

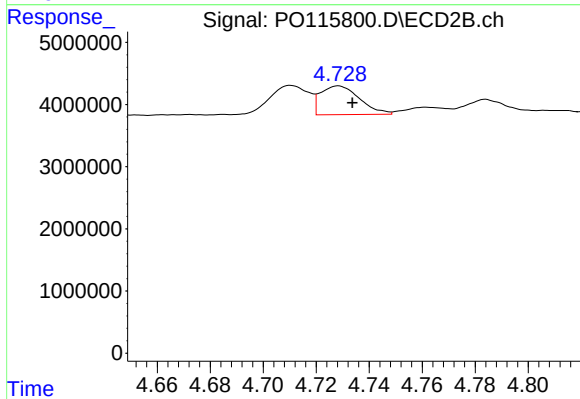

#4 AR-1016-2


R.T.: 4.728 min
Delta R.T.: -0.005 min
Response: 4734813
Conc: 17.91 ng/ml

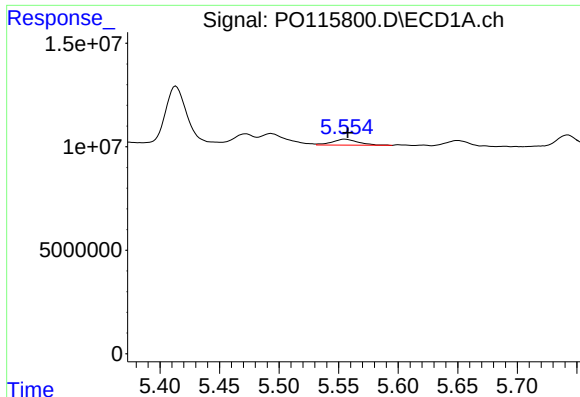

#5 AR-1016-3


R.T.: 5.555 min
Delta R.T.: -0.003 min
Response: 4383394
Conc: 20.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

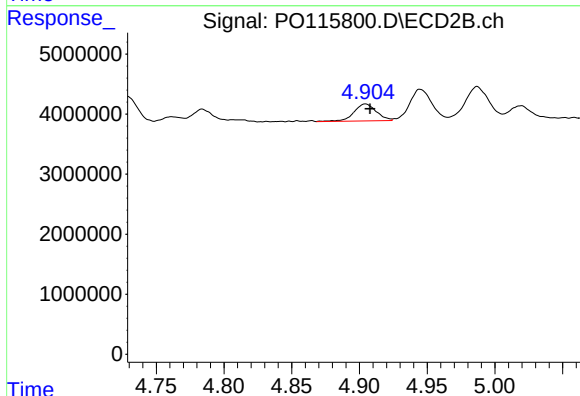


#5 AR-1016-3

R.T.: 4.905 min
Delta R.T.: -0.003 min
Response: 3256282
Conc: 21.52 ng/ml

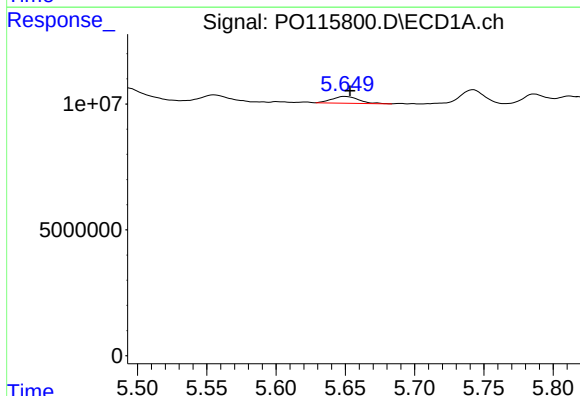


#6 AR-1016-4

R.T.: 5.650 min
Delta R.T.: -0.004 min
Response: 3587220
Conc: 20.09 ng/ml

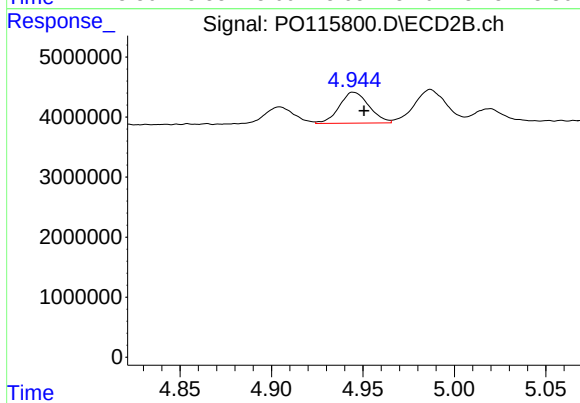

#6 AR-1016-4


R.T.: 4.945 min
Delta R.T.: -0.006 min
Response: 5844263
Conc: 51.85 ng/ml

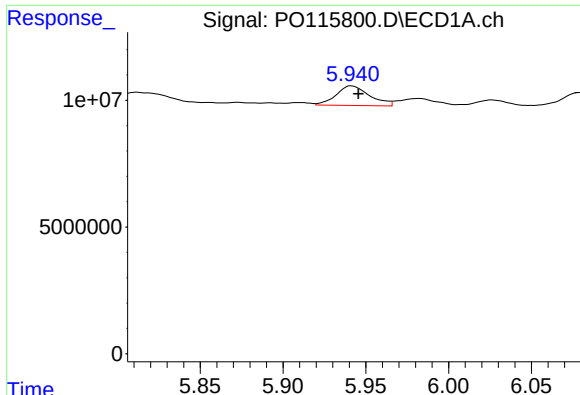

#7 AR-1016-5


R.T.: 5.941 min
Delta R.T.: -0.004 min
Response: 10903501
Conc: 62.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

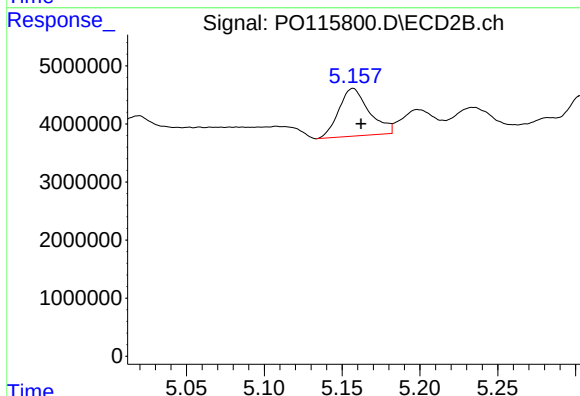


#7 AR-1016-5

R.T.: 5.157 min
Delta R.T.: -0.005 min
Response: 11159157
Conc: 76.25 ng/ml

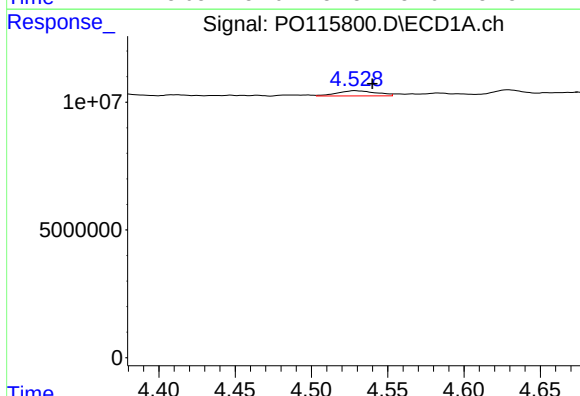


#8 AR-1221-1

R.T.: 4.528 min
Delta R.T.: -0.012 min
Response: 3534912
Conc: 43.54 ng/ml

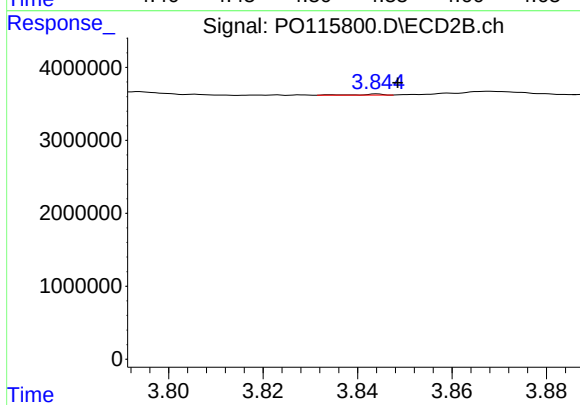

#8 AR-1221-1


R.T.: 3.844 min
Delta R.T.: -0.004 min
Response: 50910
Conc: 0.90 ng/ml

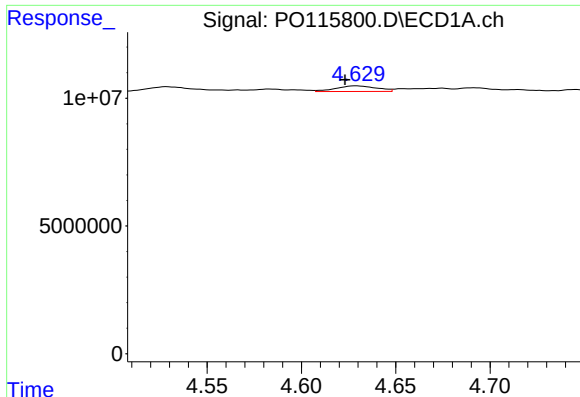

#9 AR-1221-2


R.T.: 4.629 min
Delta R.T.: 0.006 min
Response: 3336301
Conc: 52.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

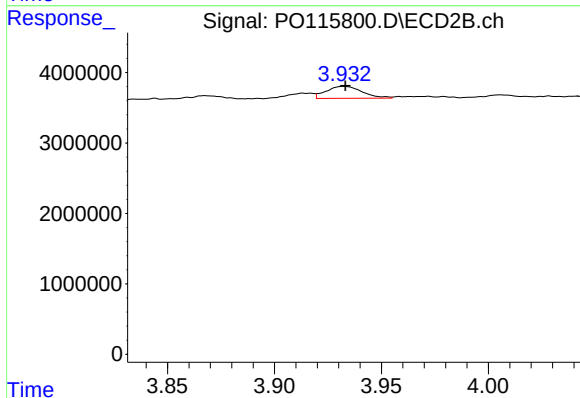


#9 AR-1221-2

R.T.: 3.932 min
Delta R.T.: 0.000 min
Response: 1997885
Conc: 47.07 ng/ml

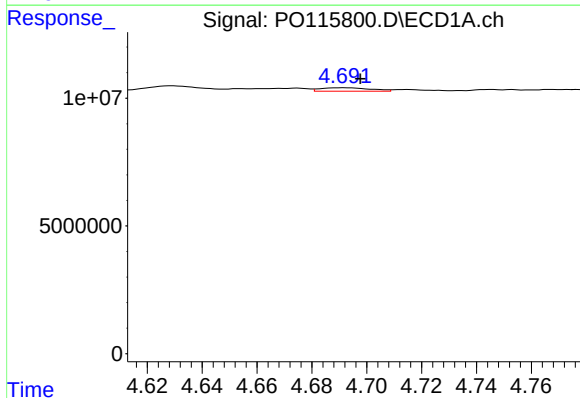


#10 AR-1221-3

R.T.: 4.692 min
Delta R.T.: -0.006 min
Response: 1714591
Conc: 9.18 ng/ml

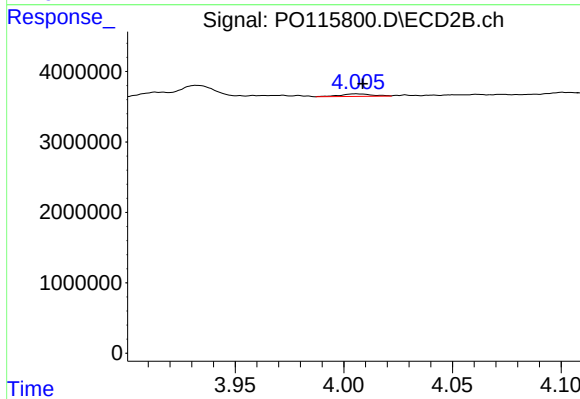

#10 AR-1221-3


R.T.: 4.006 min
Delta R.T.: -0.003 min
Response: 357061
Conc: 2.78 ng/ml

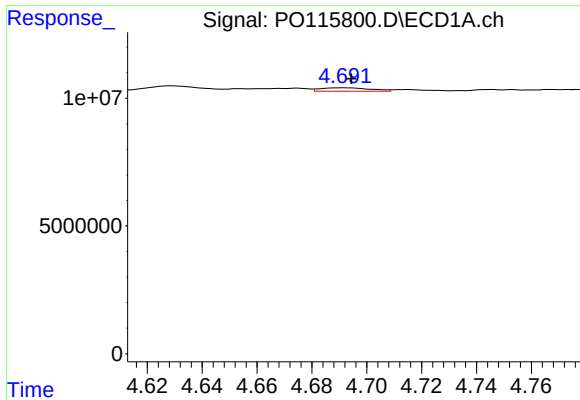

#11 AR-1232-1


R.T.: 4.692 min
Delta R.T.: -0.003 min
Response: 1714591
Conc: 11.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

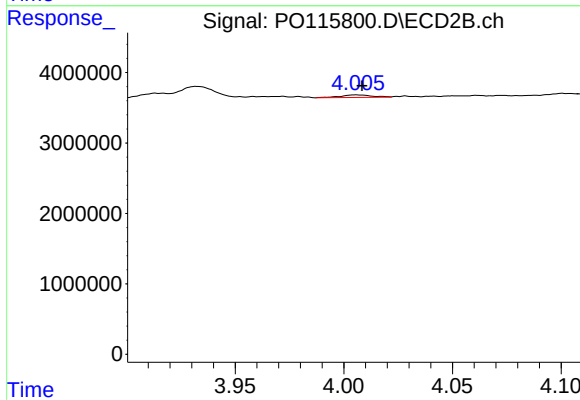


#11 AR-1232-1

R.T.: 4.006 min
Delta R.T.: -0.003 min
Response: 357061
Conc: 3.34 ng/ml

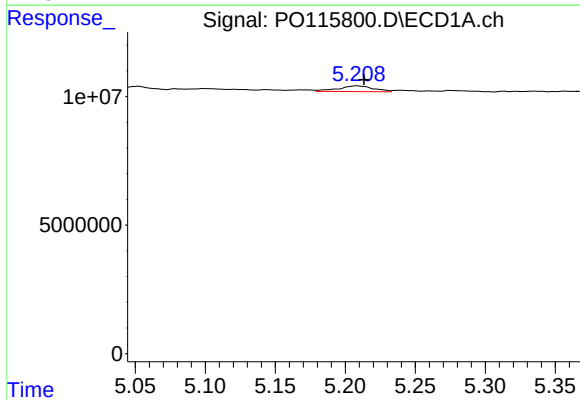


#12 AR-1232-2

R.T.: 5.208 min
Delta R.T.: -0.005 min
Response: 4007250
Conc: 49.56 ng/ml

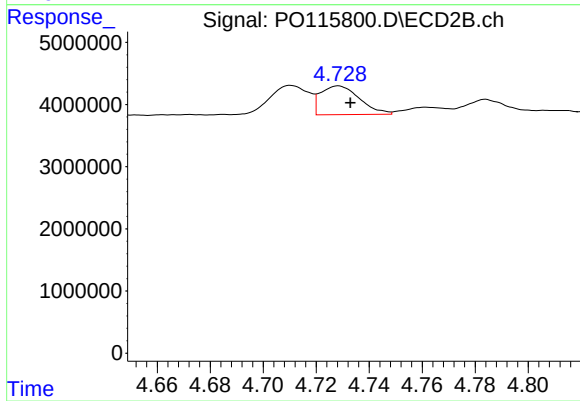

#12 AR-1232-2


R.T.: 4.728 min
Delta R.T.: -0.005 min
Response: 4734813
Conc: 42.66 ng/ml

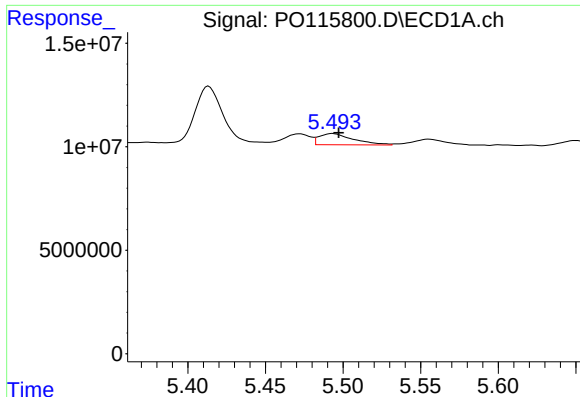

#13 AR-1232-3


R.T.: 5.493 min
Delta R.T.: -0.004 min
Response: 8251414
Conc: 53.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

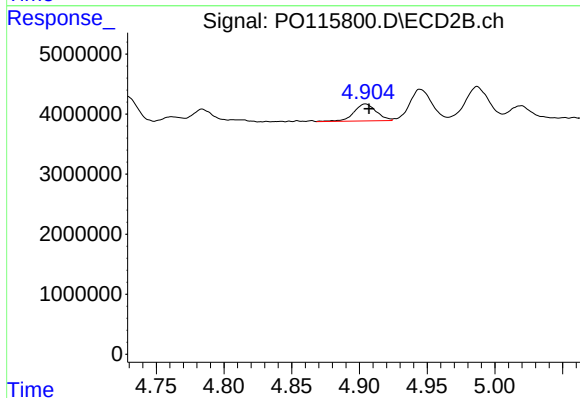


#13 AR-1232-3

R.T.: 4.905 min
Delta R.T.: -0.002 min
Response: 3256282
Conc: 49.82 ng/ml

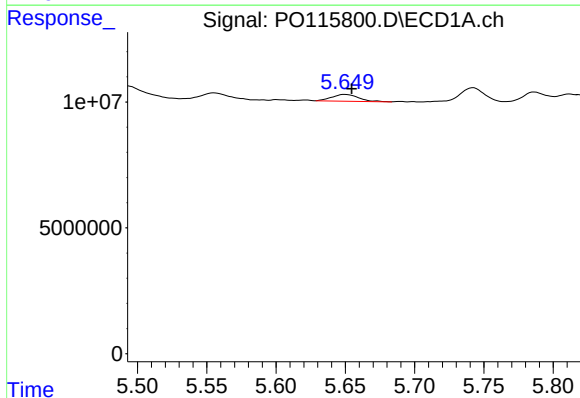


#14 AR-1232-4

R.T.: 5.650 min
Delta R.T.: -0.005 min
Response: 3587220
Conc: 51.22 ng/ml

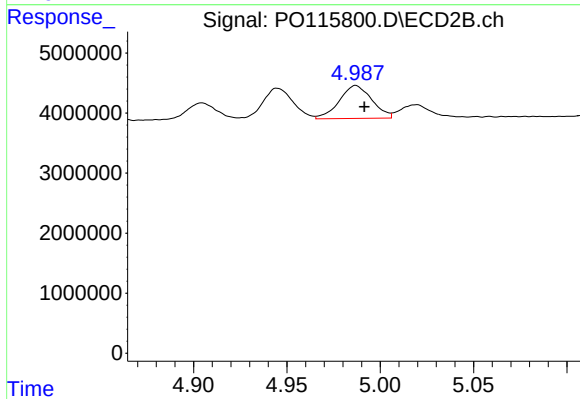

#14 AR-1232-4


R.T.: 4.987 min
Delta R.T.: -0.005 min
Response: 6657225
Conc: 129.69 ng/ml

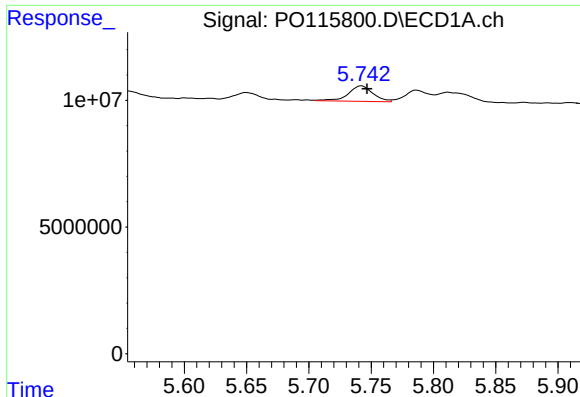

#15 AR-1232-5


R.T.: 5.742 min
Delta R.T.: -0.004 min
Response: 8437107
Conc: 162.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

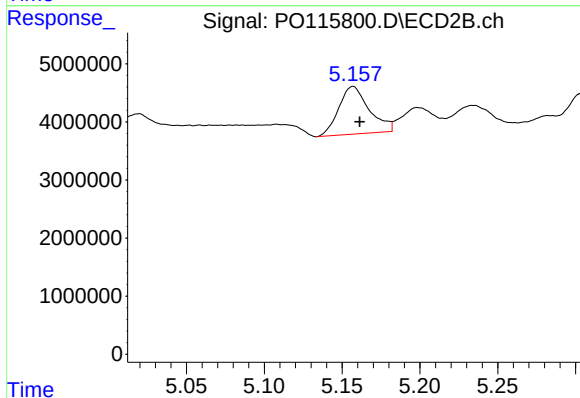


#15 AR-1232-5

R.T.: 5.157 min
Delta R.T.: -0.004 min
Response: 11159157
Conc: 203.83 ng/ml

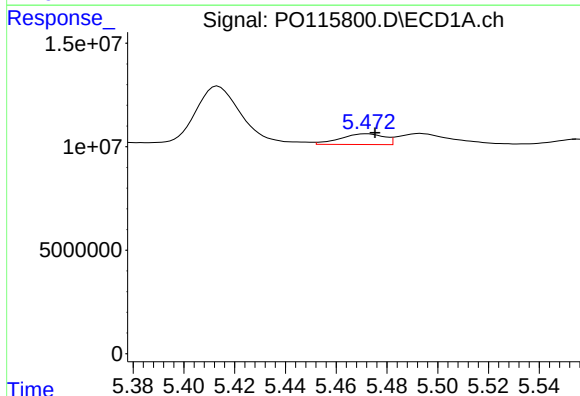


#16 AR-1242-1

R.T.: 5.472 min
Delta R.T.: -0.003 min
Response: 6233765
Conc: 31.38 ng/ml

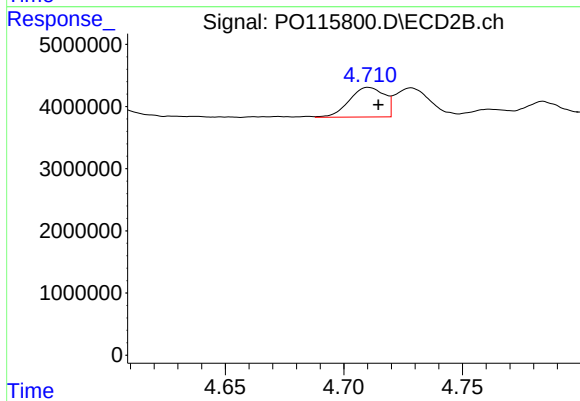

#16 AR-1242-1


R.T.: 4.710 min
Delta R.T.: -0.004 min
Response: 4894351
Conc: 34.37 ng/ml

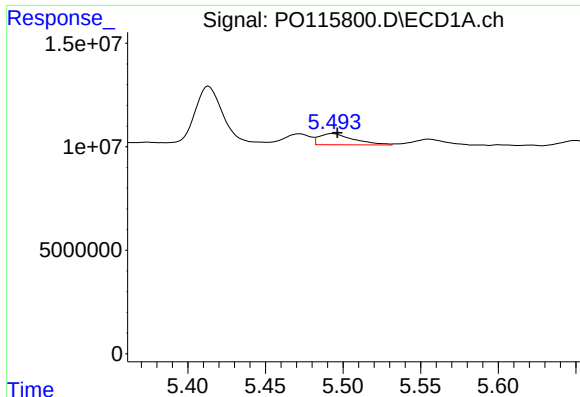

#17 AR-1242-2


R.T.: 5.493 min
Delta R.T.: -0.003 min
Response: 8251414
Conc: 28.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

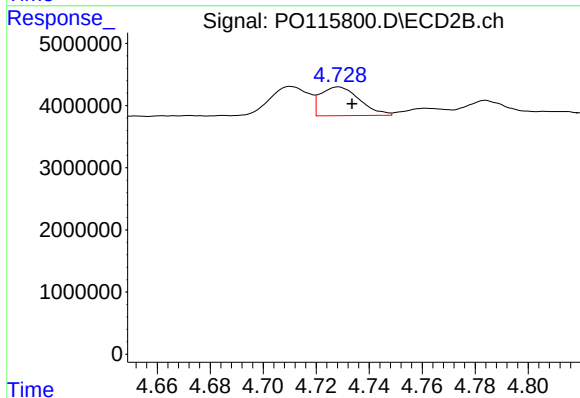


#17 AR-1242-2

R.T.: 4.728 min
Delta R.T.: -0.005 min
Response: 4734813
Conc: 22.62 ng/ml

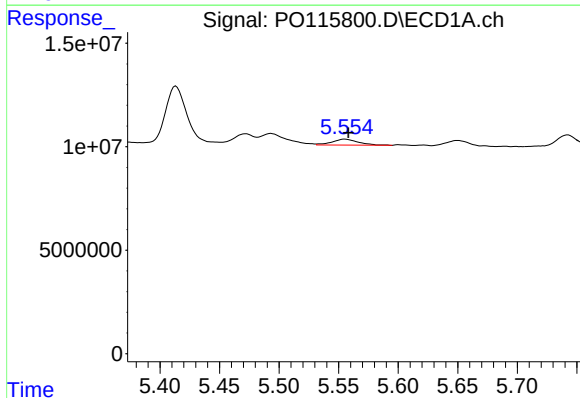


#18 AR-1242-3

R.T.: 5.555 min
Delta R.T.: -0.003 min
Response: 4383394
Conc: 25.97 ng/ml

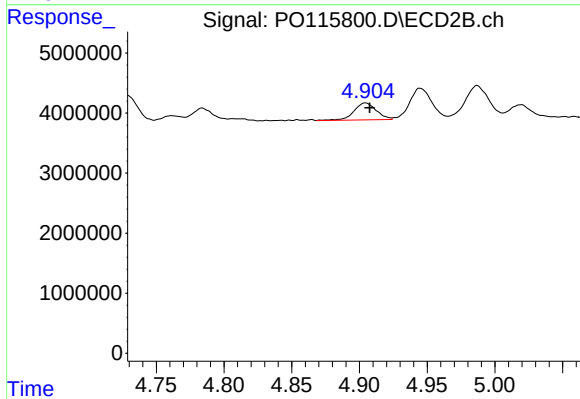

#18 AR-1242-3


R.T.: 4.905 min
Delta R.T.: -0.003 min
Response: 3256282
Conc: 27.26 ng/ml

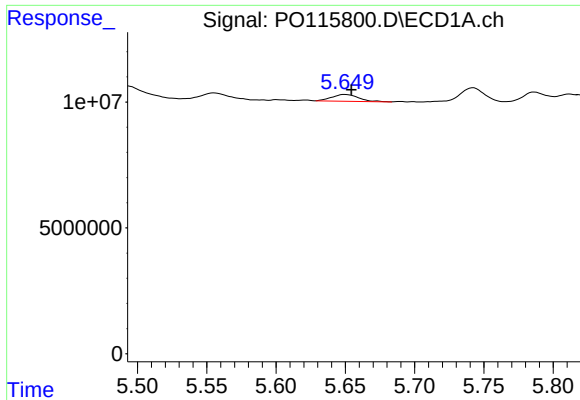

#19 AR-1242-4


R.T.: 5.650 min
Delta R.T.: -0.004 min
Response: 3587220
Conc: 26.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

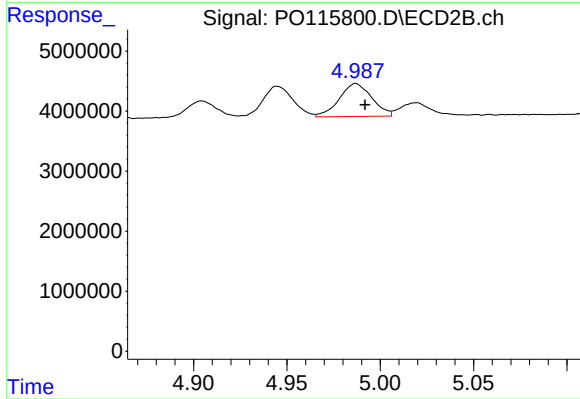


#19 AR-1242-4

R.T.: 4.987 min
Delta R.T.: -0.005 min
Response: 6657225
Conc: 61.02 ng/ml

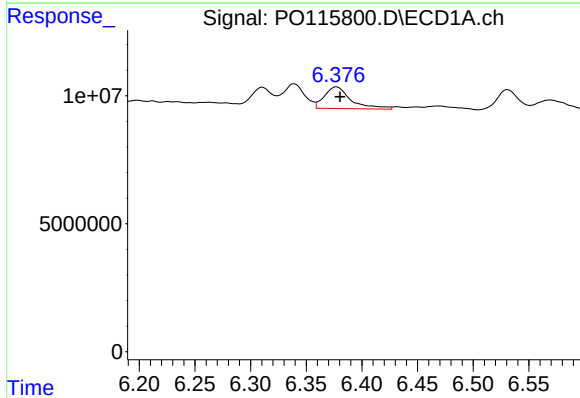


#20 AR-1242-5

R.T.: 6.377 min
Delta R.T.: -0.003 min
Response: 14098484
Conc: 93.09 ng/ml

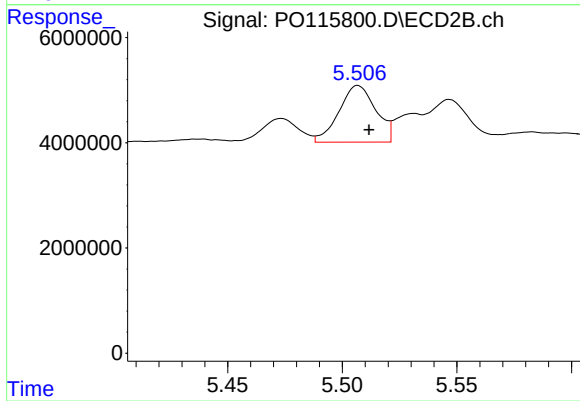

#20 AR-1242-5


R.T.: 5.507 min
Delta R.T.: -0.005 min
Response: 12050597
Conc: 87.24 ng/ml

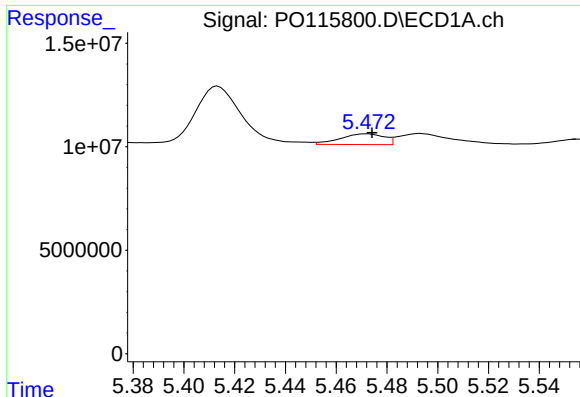

#21 AR-1248-1


R.T.: 5.472 min
Delta R.T.: -0.002 min
Response: 6233765
Conc: 41.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

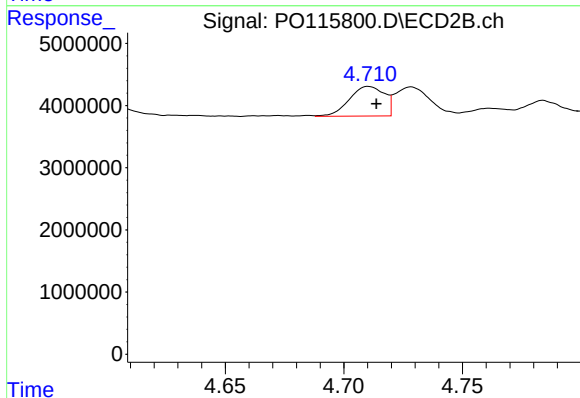


#21 AR-1248-1

R.T.: 4.710 min
Delta R.T.: -0.003 min
Response: 4894351
Conc: 43.77 ng/ml

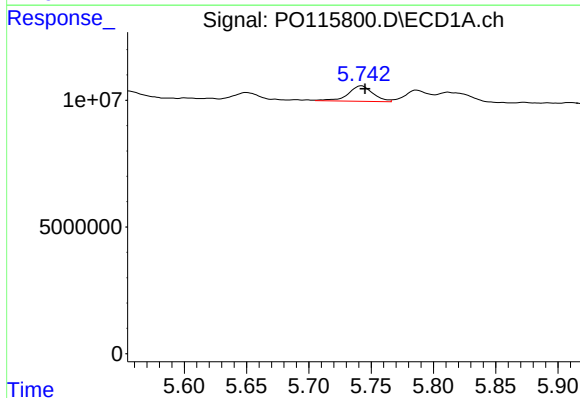


#22 AR-1248-2

R.T.: 5.742 min
Delta R.T.: -0.003 min
Response: 8437107
Conc: 42.01 ng/ml

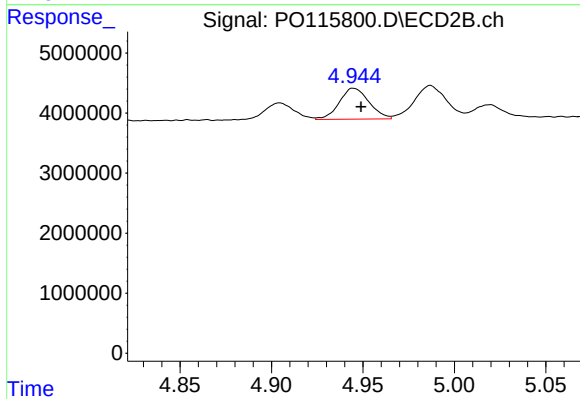

#22 AR-1248-2


R.T.: 4.945 min
Delta R.T.: -0.004 min
Response: 5844263
Conc: 38.38 ng/ml

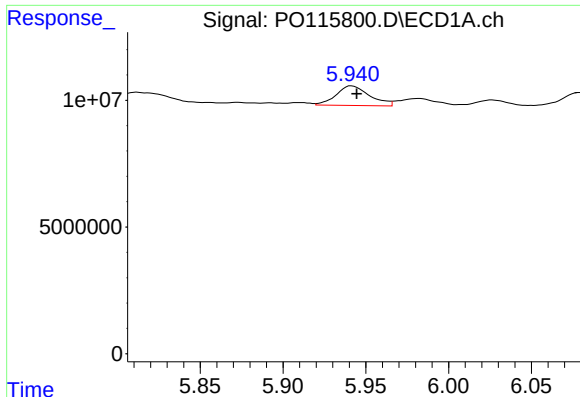

#23 AR-1248-3


R.T.: 5.941 min
Delta R.T.: -0.003 min
Response: 10903501
Conc: 44.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

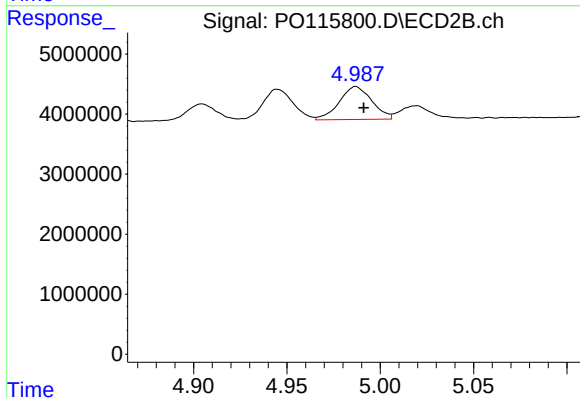


#23 AR-1248-3

R.T.: 4.987 min
Delta R.T.: -0.004 min
Response: 6657225
Conc: 41.47 ng/ml

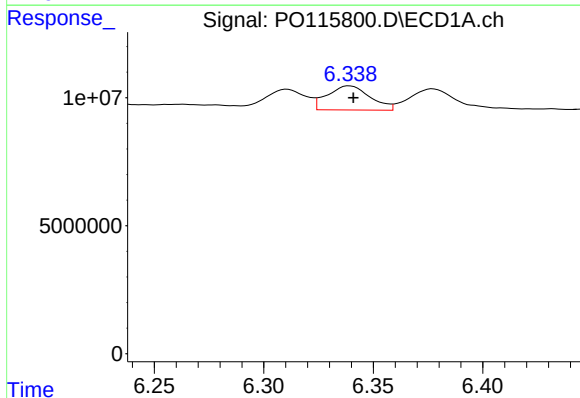


#24 AR-1248-4

R.T.: 6.339 min
Delta R.T.: -0.002 min
Response: 12778187
Conc: 43.34 ng/ml

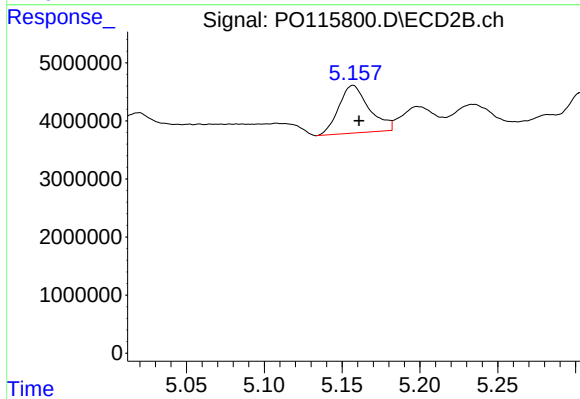

#24 AR-1248-4


R.T.: 5.157 min
Delta R.T.: -0.004 min
Response: 11159157
Conc: 59.63 ng/ml

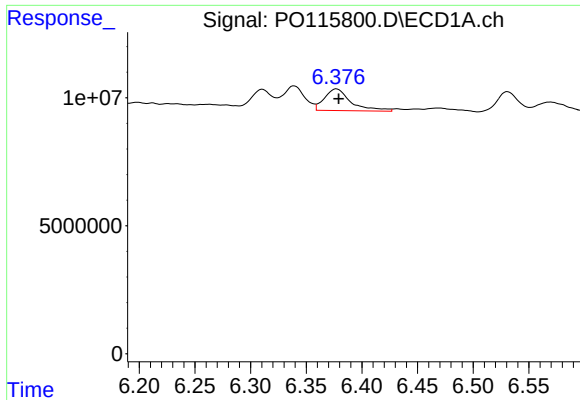

#25 AR-1248-5


R.T.: 6.377 min
Delta R.T.: -0.002 min
Response: 14098484
Conc: 54.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

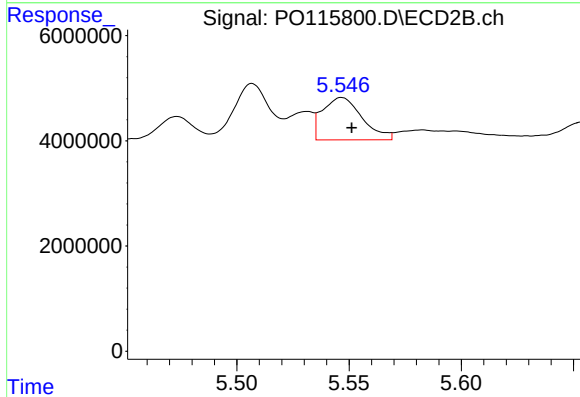


#25 AR-1248-5

R.T.: 5.547 min
Delta R.T.: -0.005 min
Response: 9897470
Conc: 50.00 ng/ml

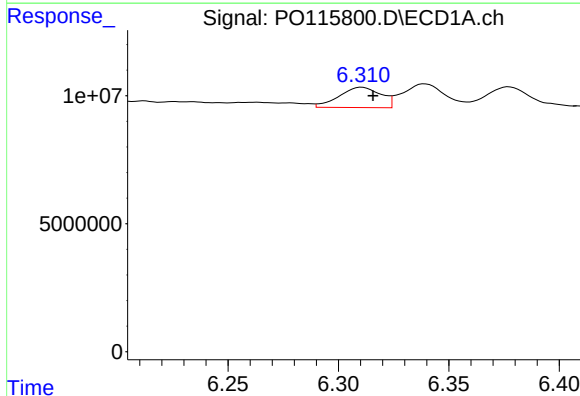


#26 AR-1254-1

R.T.: 6.311 min
Delta R.T.: -0.005 min
Response: 10384915
Conc: 40.14 ng/ml

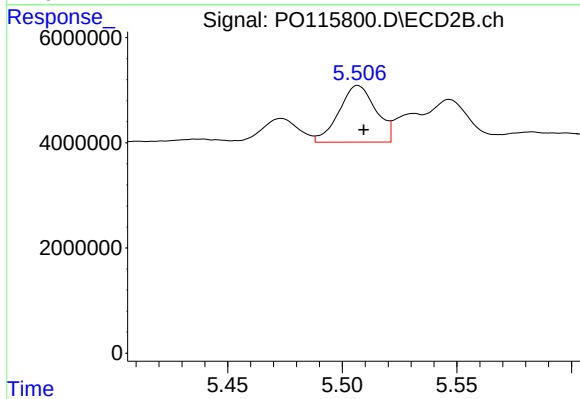

#26 AR-1254-1


R.T.: 5.507 min
Delta R.T.: -0.003 min
Response: 12050597
Conc: 41.23 ng/ml

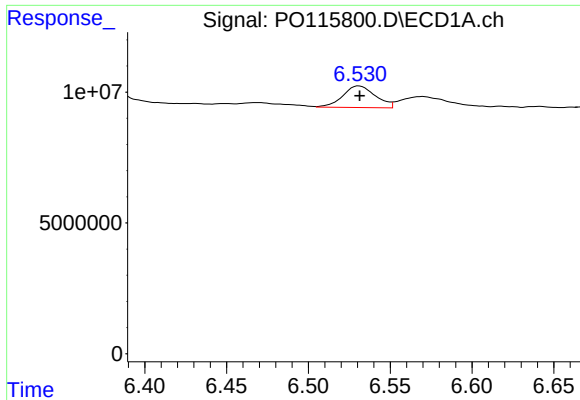

#27 AR-1254-2


R.T.: 6.531 min
Delta R.T.: 0.000 min
Response: 11422618
Conc: 28.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

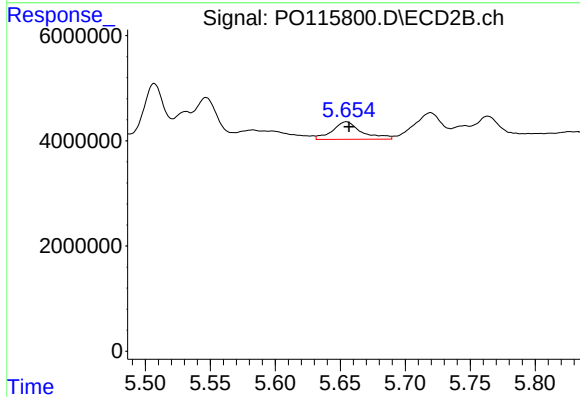


#27 AR-1254-2

R.T.: 5.655 min
Delta R.T.: -0.002 min
Response: 5210390
Conc: 20.69 ng/ml

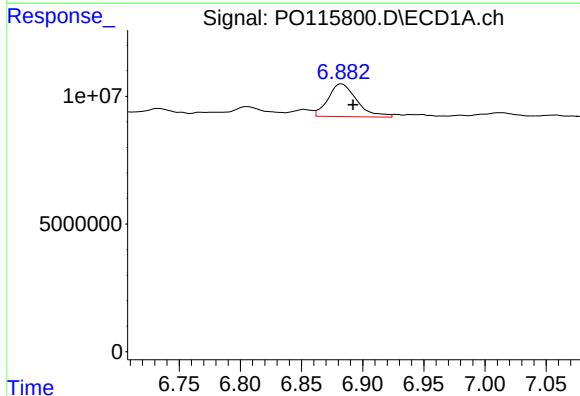


#28 AR-1254-3

R.T.: 6.883 min
Delta R.T.: -0.009 min
Response: 20886791
Conc: 50.87 ng/ml

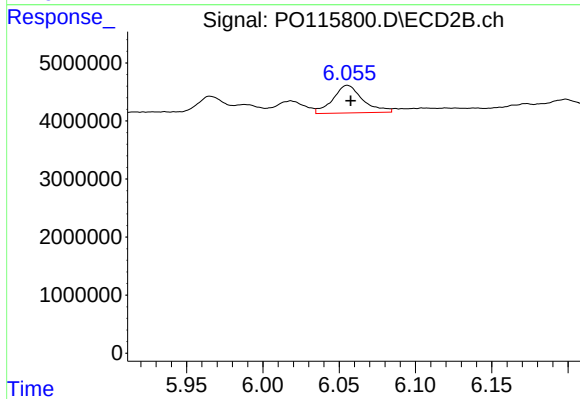

#28 AR-1254-3


R.T.: 6.055 min
Delta R.T.: -0.002 min
Response: 6504313
Conc: 16.53 ng/ml

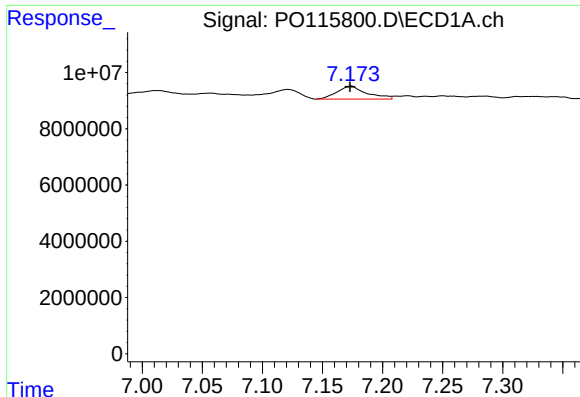

#29 AR-1254-4


R.T.: 7.174 min
Delta R.T.: 0.000 min
Response: 7910365
Conc: 22.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

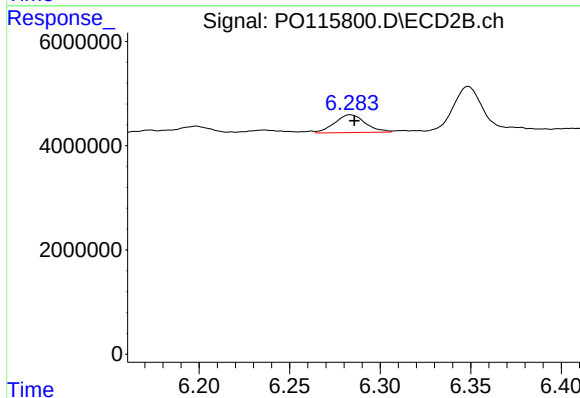


#29 AR-1254-4

R.T.: 6.283 min
Delta R.T.: -0.003 min
Response: 4045695
Conc: 15.12 ng/ml

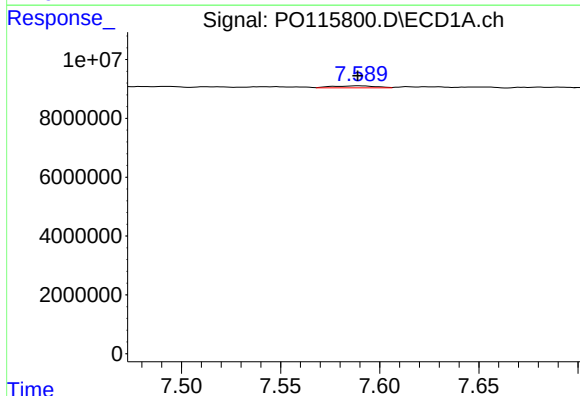


#30 AR-1254-5

R.T.: 7.590 min
Delta R.T.: 0.000 min
Response: 1016144
Conc: 3.14 ng/ml

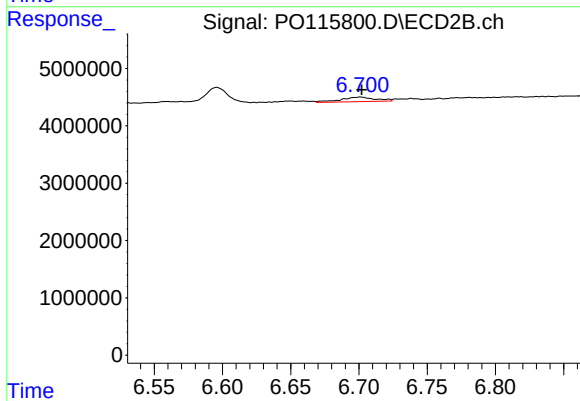

#30 AR-1254-5


R.T.: 6.701 min
Delta R.T.: -0.001 min
Response: 1411143
Conc: 3.95 ng/ml

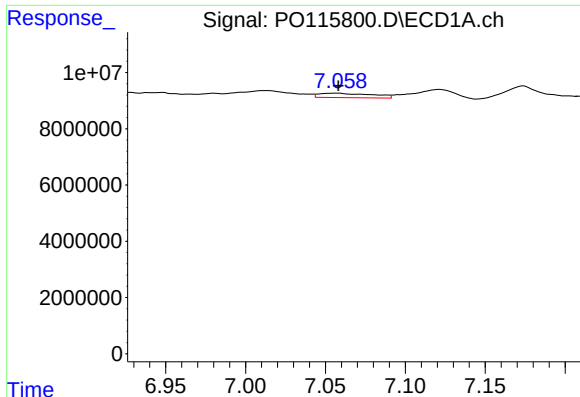

#31 AR-1260-1


R.T.: 7.058 min
Delta R.T.: 0.000 min
Response: 3678147
Conc: 12.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

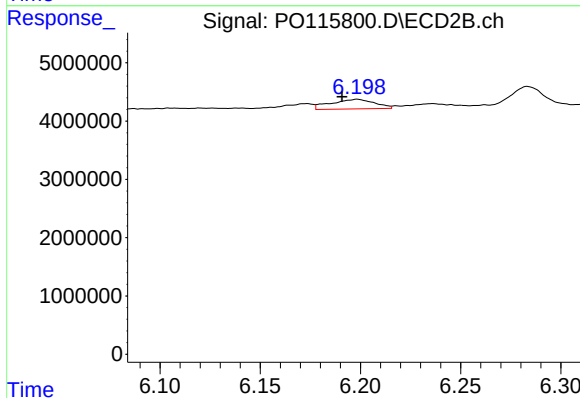


#31 AR-1260-1

R.T.: 6.199 min
Delta R.T.: 0.008 min
Response: 2539936
Conc: 9.69 ng/ml

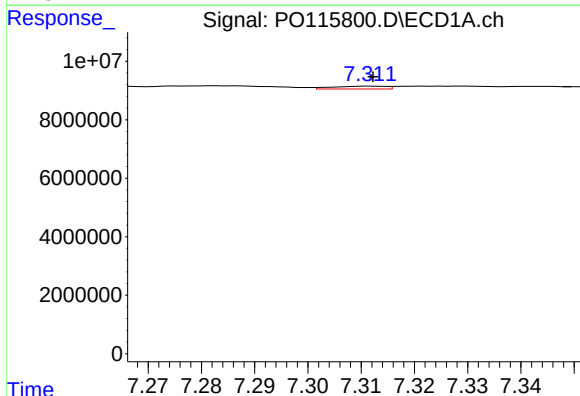


#32 AR-1260-2

R.T.: 7.312 min
Delta R.T.: 0.000 min
Response: 684304
Conc: 1.56 ng/ml

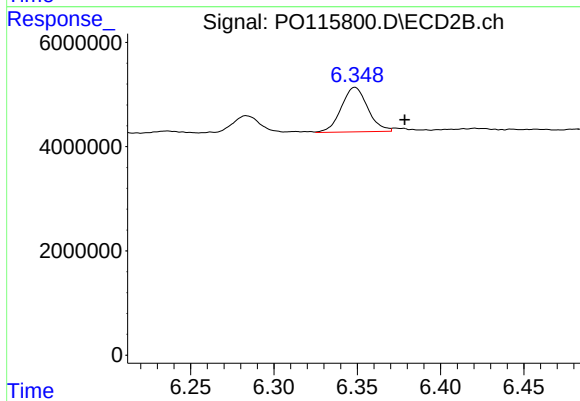

#32 AR-1260-2


R.T.: 6.349 min
Delta R.T.: -0.030 min
Response: 9419685
Conc: 26.88 ng/ml

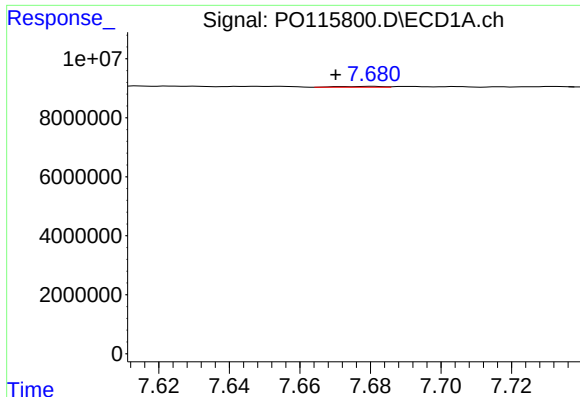

#33 AR-1260-3


R.T.: 7.681 min
Delta R.T.: 0.011 min
Response: 239662
Conc: 0.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

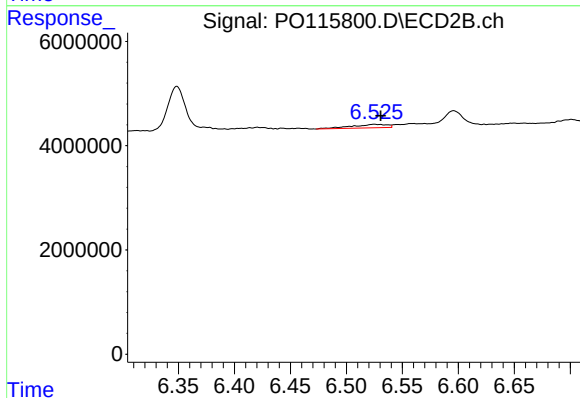


#33 AR-1260-3

R.T.: 6.525 min
Delta R.T.: -0.006 min
Response: 1502034
Conc: 4.68 ng/ml

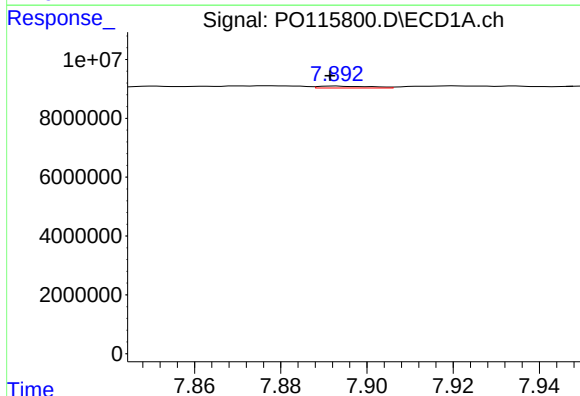


#34 AR-1260-4

R.T.: 7.893 min
Delta R.T.: 0.001 min
Response: 529250
Conc: 1.72 ng/ml

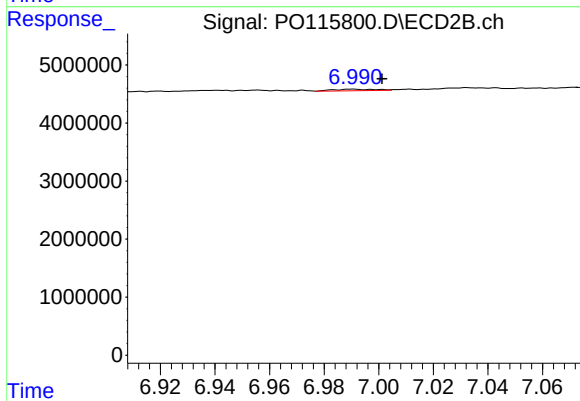

#34 AR-1260-4


R.T.: 6.990 min
Delta R.T.: -0.011 min
Response: 284223
Conc: 1.11 ng/ml

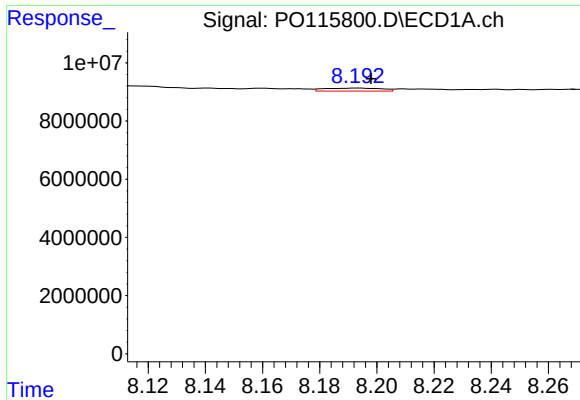

#35 AR-1260-5


R.T.: 8.193 min
Delta R.T.: -0.005 min
Response: 1419757
Conc: 1.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

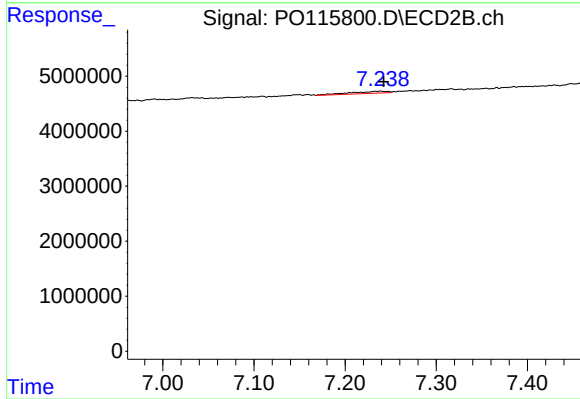


#35 AR-1260-5

R.T.: 7.239 min
Delta R.T.: -0.003 min
Response: 1089548
Conc: 1.55 ng/ml

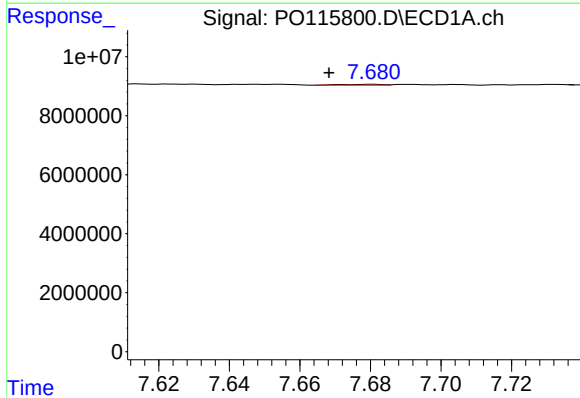


#36 AR-1262-1

R.T.: 7.681 min
Delta R.T.: 0.012 min
Response: 239662
Conc: 0.97 ng/ml

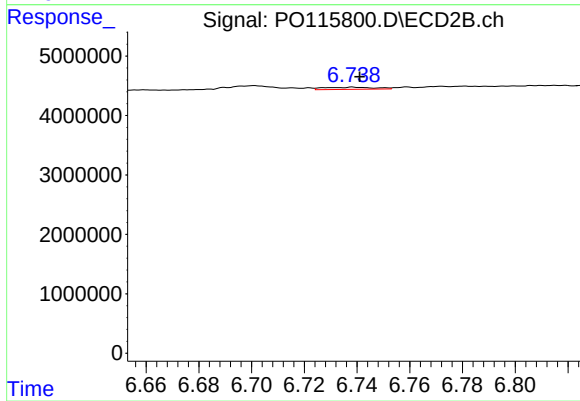

#36 AR-1262-1


R.T.: 6.738 min
Delta R.T.: -0.003 min
Response: 485844
Conc: 2.28 ng/ml

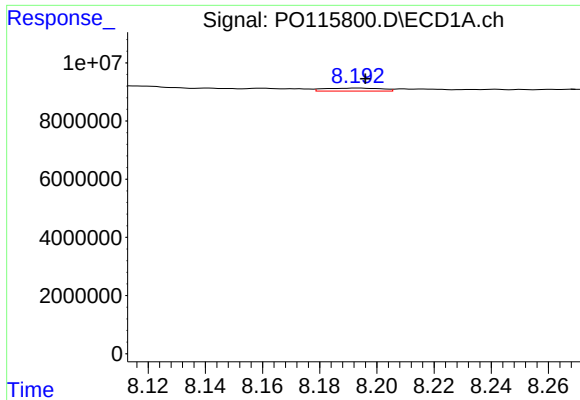

#37 AR-1262-2


R.T.: 8.193 min
Delta R.T.: -0.003 min
Response: 1419757
Conc: 3.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

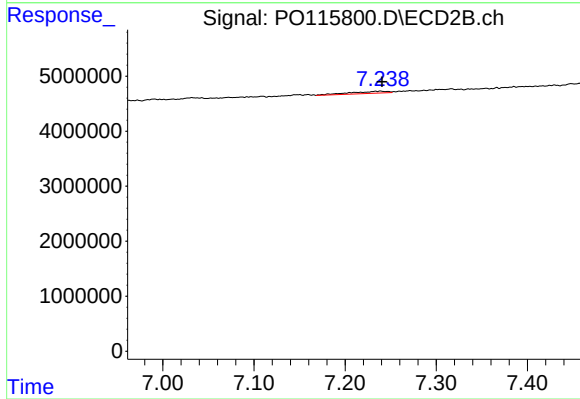


#37 AR-1262-2

R.T.: 7.239 min
Delta R.T.: -0.002 min
Response: 1089548
Conc: 3.13 ng/ml

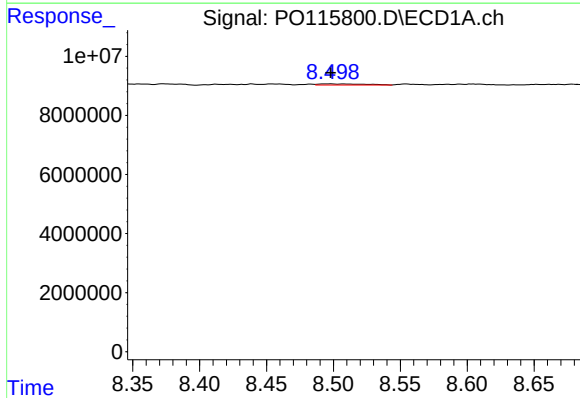


#38 AR-1262-3

R.T.: 8.498 min
Delta R.T.: 0.000 min
Response: 964471
Conc: 3.78 ng/ml

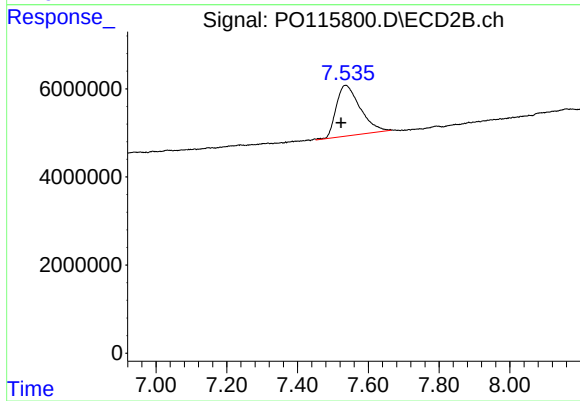

#38 AR-1262-3


R.T.: 7.536 min
Delta R.T.: 0.012 min
Response: 54060905
Conc: 345.68 ng/ml

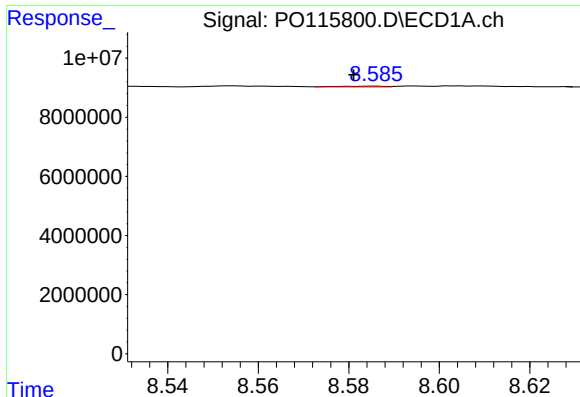

#39 AR-1262-4


R.T.: 8.585 min
Delta R.T.: 0.004 min
Response: 176976
Conc: 0.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

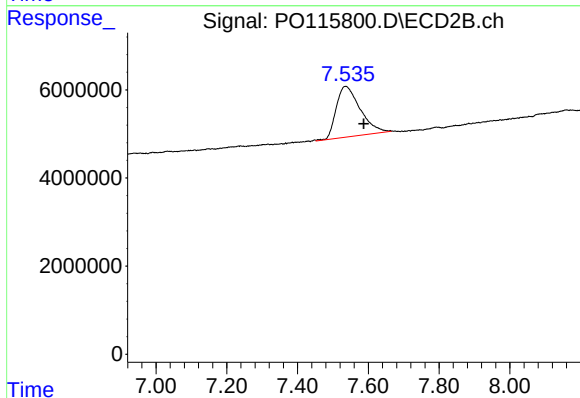


#39 AR-1262-4

R.T.: 7.536 min
Delta R.T.: -0.051 min
Response: 54060905
Conc: 218.54 ng/ml

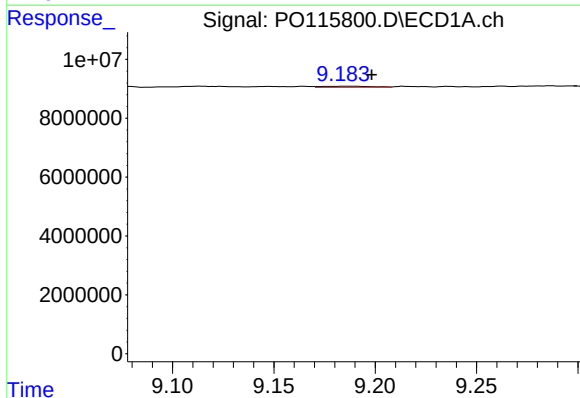


#40 AR-1262-5

R.T.: 9.191 min
Delta R.T.: -0.007 min
Response: 606731
Conc: 4.50 ng/ml

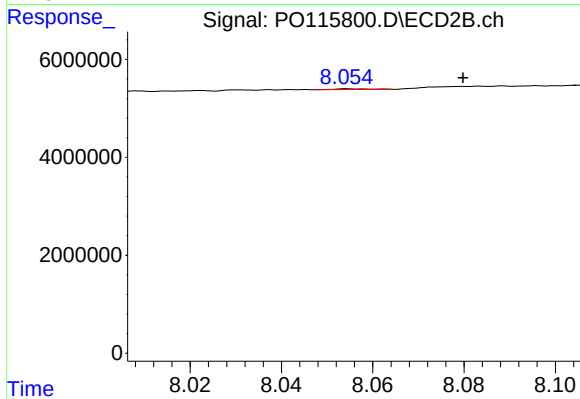

#40 AR-1262-5


R.T.: 8.055 min
Delta R.T.: -0.025 min
Response: 80804
Conc: 0.72 ng/ml

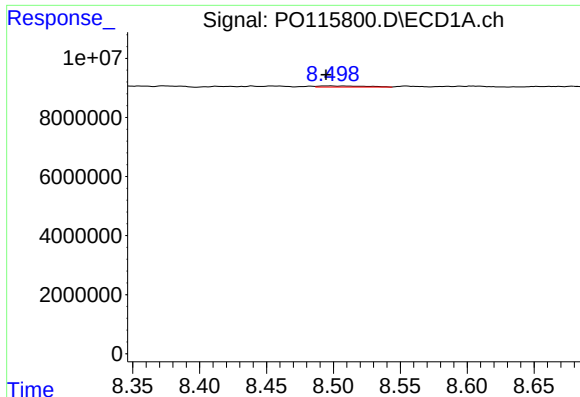

#41 AR-1268-1


R.T.: 8.498 min
Delta R.T.: 0.003 min
Response: 964471
Conc: 0.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

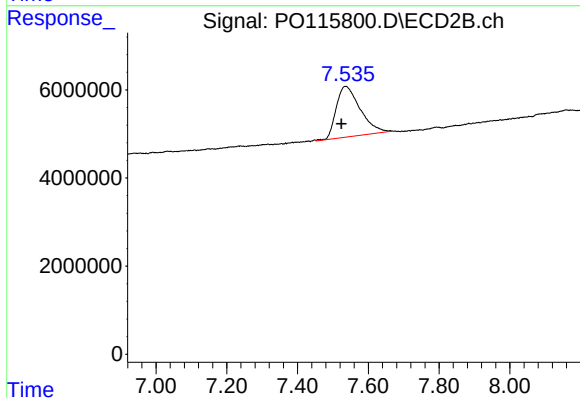


#41 AR-1268-1

R.T.: 7.536 min
Delta R.T.: 0.012 min
Response: 54060905
Conc: 61.02 ng/ml

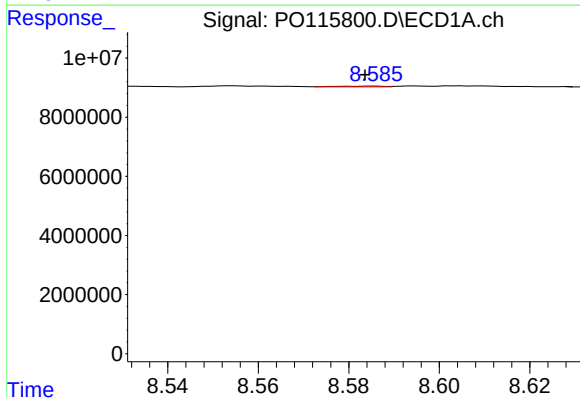


#42 AR-1268-2

R.T.: 8.585 min
Delta R.T.: 0.002 min
Response: 176976
Conc: 0.21 ng/ml

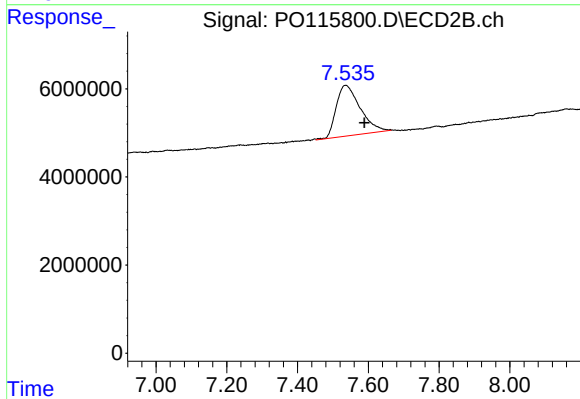

#42 AR-1268-2


R.T.: 7.536 min
Delta R.T.: -0.053 min
Response: 54060905
Conc: 72.17 ng/ml

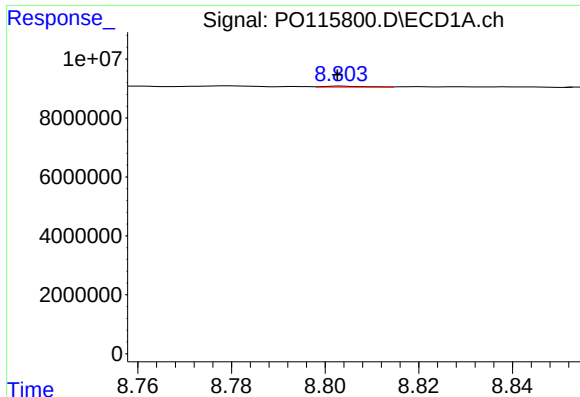

#43 AR-1268-3


R.T.: 8.804 min
Delta R.T.: 0.000 min
Response: 190434
Conc: 0.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

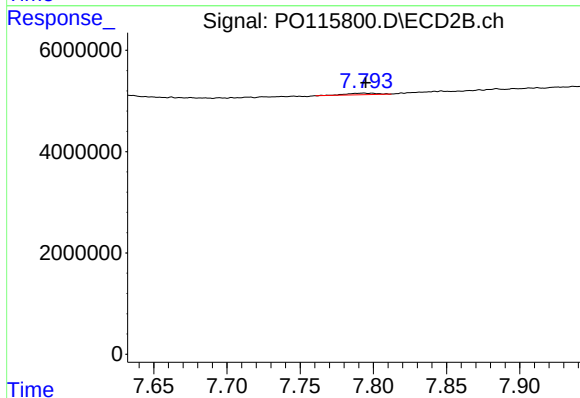


#43 AR-1268-3

R.T.: 7.793 min
Delta R.T.: -0.002 min
Response: 410908
Conc: 0.65 ng/ml

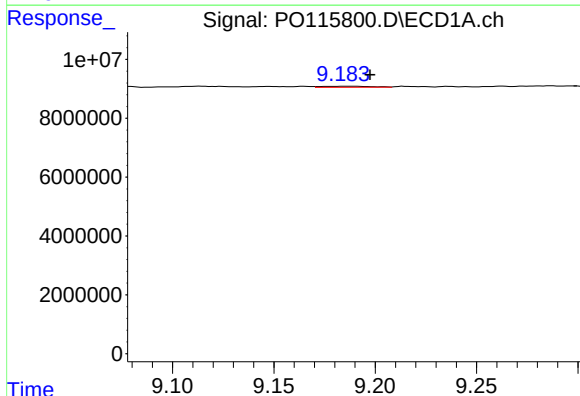


#44 AR-1268-4

R.T.: 9.191 min
Delta R.T.: -0.007 min
Response: 606731
Conc: 1.94 ng/ml

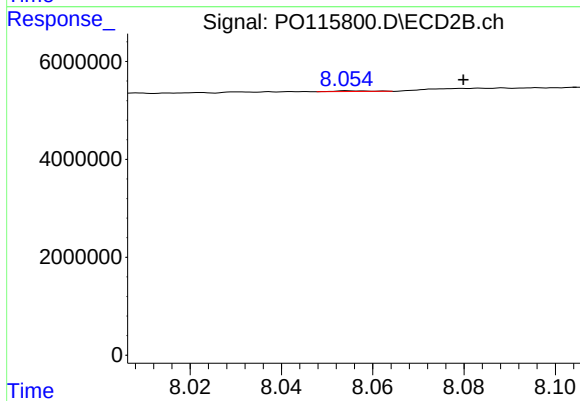

#44 AR-1268-4


R.T.: 8.055 min
Delta R.T.: -0.025 min
Response: 80804
Conc: 0.31 ng/ml

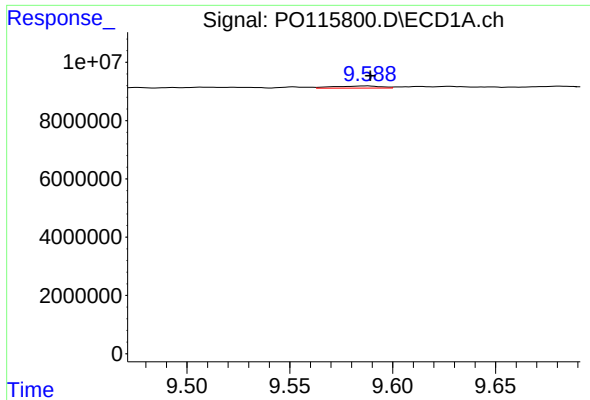

#45 AR-1268-5

R.T.: 9.588 min
Delta R.T.: -0.001 min
Response: 1163782
Conc: 0.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

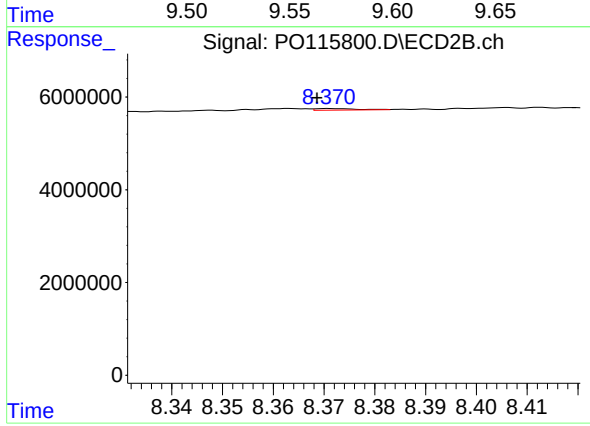

#45 AR-1268-5

R.T.: 8.371 min
Delta R.T.: 0.003 min
Response: 185454
Conc: 0.11 ng/ml