

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO121225\
 Data File : PO115801.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Dec 2025 12:54
 Operator : YP/AJ
 Sample : Q3530-07
 Misc : AR1254 40PPB WATER LOD
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 02:19:04 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO120425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 05 02:11:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.334	3.636	172.7E6	105.2E6	22.232	21.579
2)	SA Decachlor...	9.907	8.616	123.3E6	93874084	23.429	21.830
Target Compounds							
3)	L1 AR-1016-1	5.476	4.716	405523	574406	1.631	3.109 #
4)	L1 AR-1016-2	5.487	4.739	748802	44646	1.966	0.169 #
5)	L1 AR-1016-3	5.550	4.905	845475	328628	3.955	2.171 #
6)	L1 AR-1016-4	5.653	4.946	157428	5056347	0.882	44.864 #
7)	L1 AR-1016-5	5.943	5.157	5053933	4560613	28.809	31.164
8)	L2 AR-1221-1	4.547	3.843	387004	65922	4.766	1.169 #
9)	L2 AR-1221-2	4.631	3.932	3835648	2019017	60.865	47.569
10)	L2 AR-1221-3	4.698	4.012	306487	102692	1.641	0.799 #
11)	L3 AR-1232-1	4.698	4.012	306487	102692	2.048	0.961 #
12)	L3 AR-1232-2	5.213	4.739	286753	44646	3.547	0.402 #
13)	L3 AR-1232-3	5.487	4.905	748802	328628	4.865	5.027
14)	L3 AR-1232-4	5.653	4.987	157428	1610487	2.248	31.375 #
15)	L3 AR-1232-5	5.743	5.157	5976711	4560613	115.076	83.302 #
16)	L4 AR-1242-1	5.476	4.716	405523	574406	2.042	4.034 #
17)	L4 AR-1242-2	5.487	4.739	748802	44646	2.557	0.213 #
18)	L4 AR-1242-3	5.550	4.905	845475	328628	5.008	2.751 #
19)	L4 AR-1242-4	5.653	4.987	157428	1610487	1.152	14.763 #
20)	L4 AR-1242-5	6.381	5.507	5230339	12516666	34.536	90.618 #
21)	L5 AR-1248-1	5.476	4.716	405523	574406	2.672	5.136 #
22)	L5 AR-1248-2	5.743	4.946	5976711	5056347	29.762	33.202
23)	L5 AR-1248-3	5.943	4.987	5053933	1610487	20.495	10.033 #
24)	L5 AR-1248-4	6.338	5.157	6436863	4560613	21.831	24.369
25)	L5 AR-1248-5	6.381	5.545	5230339	1828068	20.200	9.235 #
26)	L6 AR-1254-1	6.314	5.507	12068587	12516666	46.649	42.825
27)	L6 AR-1254-2	6.531	5.654	16457695	10894788	40.898	43.265
28)	L6 AR-1254-3	6.889	6.055	26270768	16136446	63.987	40.999 #
29)	L6 AR-1254-4	7.173	6.283	14840182	11043898	42.759	41.274
30)	L6 AR-1254-5	7.588	6.699	11767468	14518638	36.315	40.609
31)	L7 AR-1260-1	7.056	6.186	7380517	7708414	25.476	29.402
32)	L7 AR-1260-2	7.310	6.373	7700851	6797048	17.593	19.395
33)	L7 AR-1260-3	7.665	6.524	602190	7197771	1.789	22.404 #
34)	L7 AR-1260-4	7.873	6.999	5367088	1008076	17.456	3.925 #
35)	L7 AR-1260-5	8.194	7.236	2871525	1959279	3.942	2.794 #
36)	L8 AR-1262-1	7.665	6.768	602190	1305221	2.439	6.127 #
37)	L8 AR-1262-2	8.194	7.236	2871525	1959279	7.253	5.625
38)	L8 AR-1262-3	8.507	7.535	1996864	34777460	7.836	222.376 #
39)	L8 AR-1262-4	8.591	7.535f	329786	34777460	1.703	140.588 #
40)	L8 AR-1262-5	9.199	8.015f	2363237	295143	17.546	2.648 #
41)	L9 AR-1268-1	8.507	7.535	1996864	34777460	2.005	39.254 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO121225\
Data File : PO115801.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Dec 2025 12:54
Operator : YP/AJ
Sample : Q3530-07
Misc : AR1254 40PPB WATER LOD
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_0
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 02:19:04 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO120425.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 05 02:11:05 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.591	7.535f	329786	34777460	0.386	46.427 #
43)	L9 AR-1268-3	8.806	7.789	144286	799793	0.194	1.256 #
44)	L9 AR-1268-4	9.199	8.015f	2363237	295143	7.569	1.146 #
45)	L9 AR-1268-5	9.589	8.362	1287976	662414	0.592	0.393 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121225\
Data File : PO115801.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Dec 2025 12:54
Operator : YP/AJ
Sample : Q3530-07
Misc : AR1254 40PPB WATER LOD
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 02:19:04 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120425.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 05 02:11:05 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

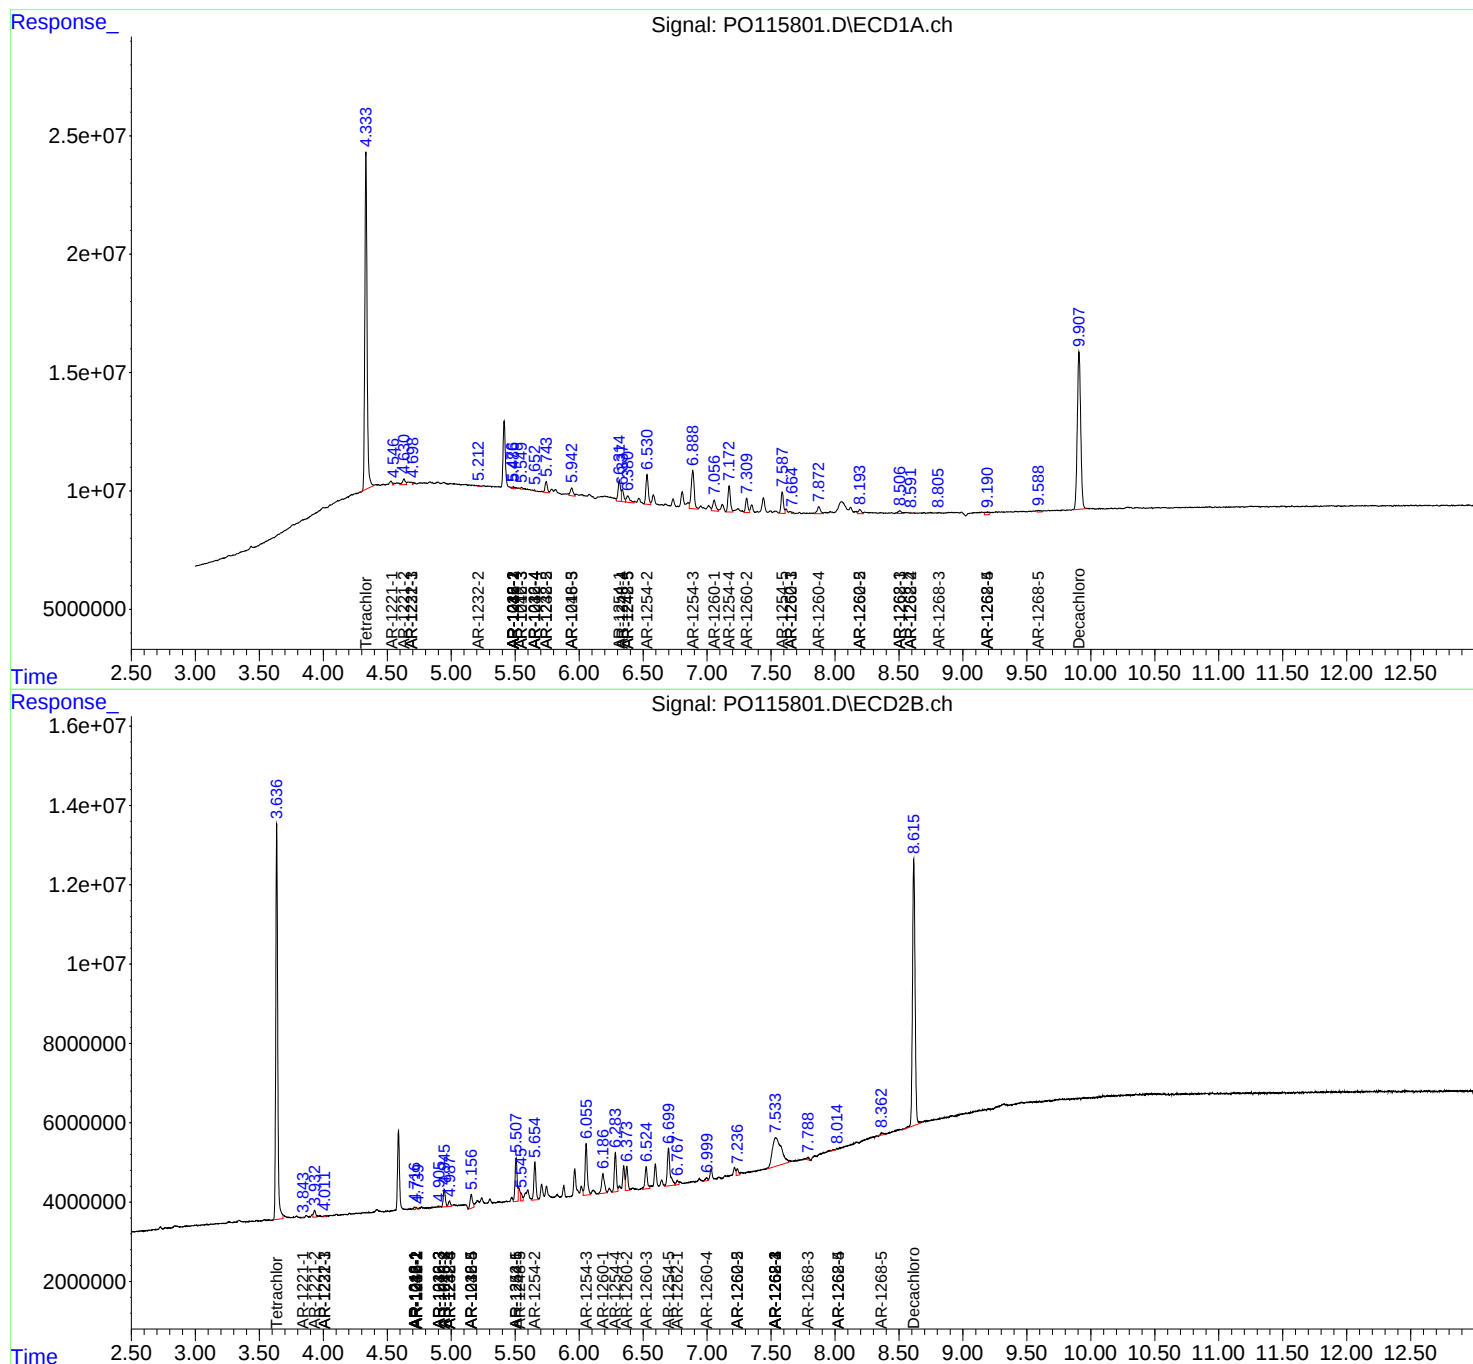


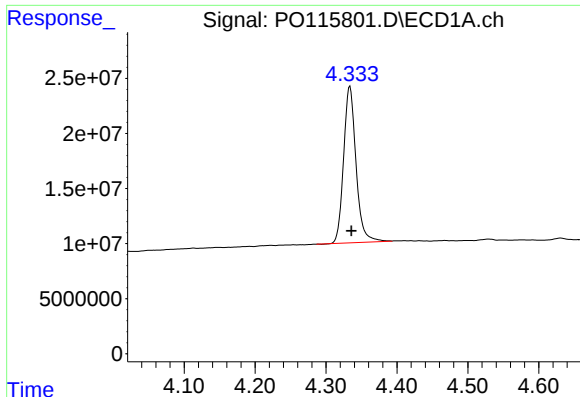

#1 Tetrachloro-m-xylene


R.T.: 4.334 min
Delta R.T.: -0.002 min
Response: 172681561
Conc: 22.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

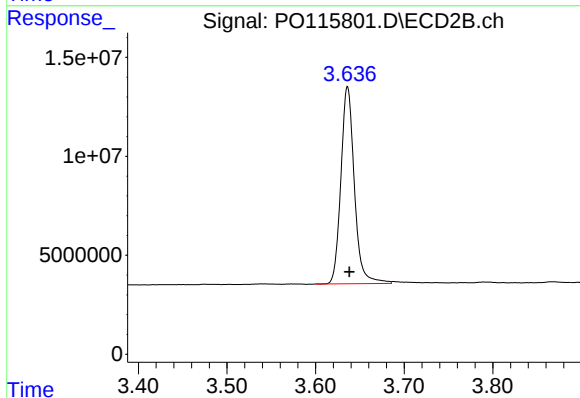


#1 Tetrachloro-m-xylene

R.T.: 3.636 min
Delta R.T.: -0.002 min
Response: 105163716
Conc: 21.58 ng/ml

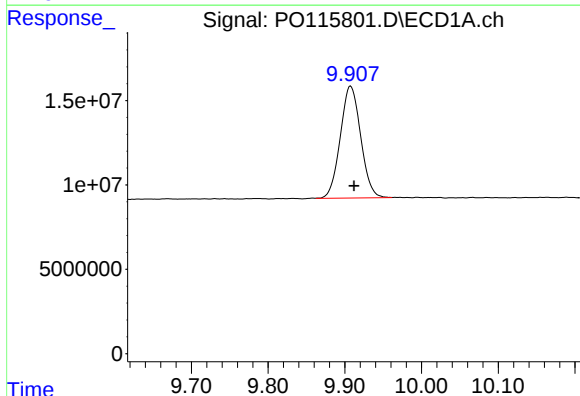


#2 Decachlorobiphenyl

R.T.: 9.907 min
Delta R.T.: -0.005 min
Response: 123260463
Conc: 23.43 ng/ml

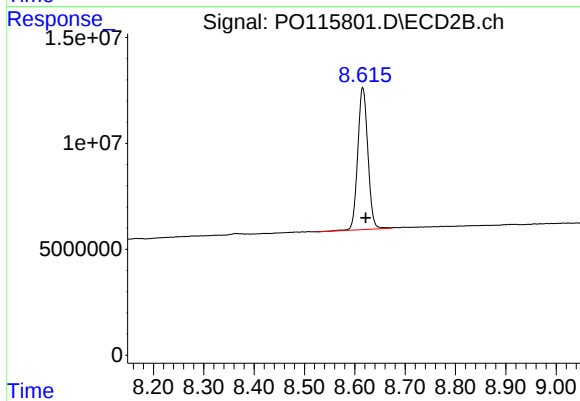

#2 Decachlorobiphenyl


R.T.: 8.616 min
Delta R.T.: -0.006 min
Response: 93874084
Conc: 21.83 ng/ml

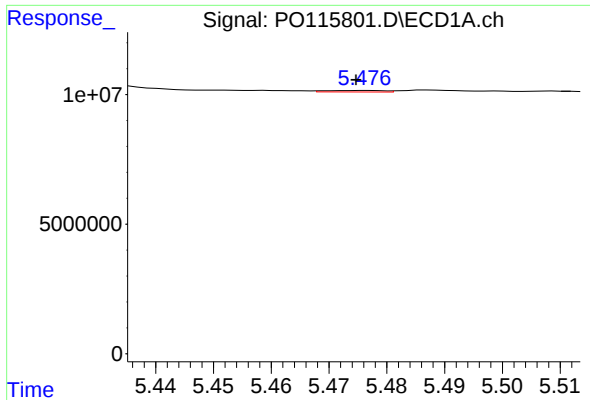

#3 AR-1016-1


R.T.: 5.476 min
Delta R.T.: 0.002 min
Response: 405523
Conc: 1.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

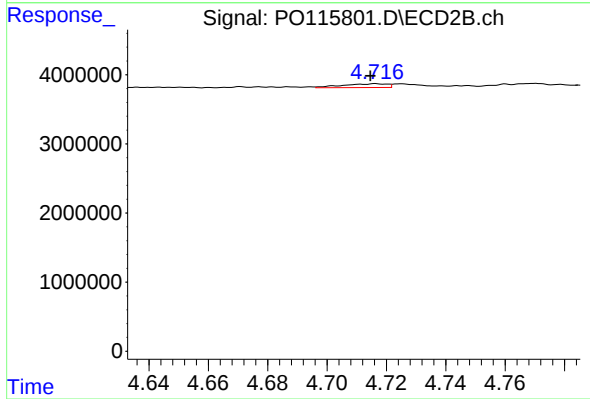


#3 AR-1016-1

R.T.: 4.716 min
Delta R.T.: 0.002 min
Response: 574406
Conc: 3.11 ng/ml

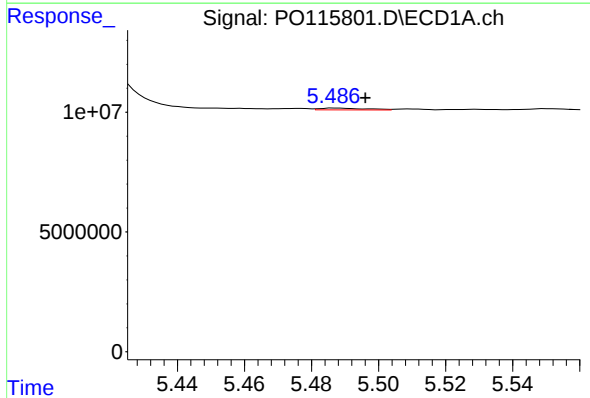


#4 AR-1016-2

R.T.: 5.487 min
Delta R.T.: -0.009 min
Response: 748802
Conc: 1.97 ng/ml

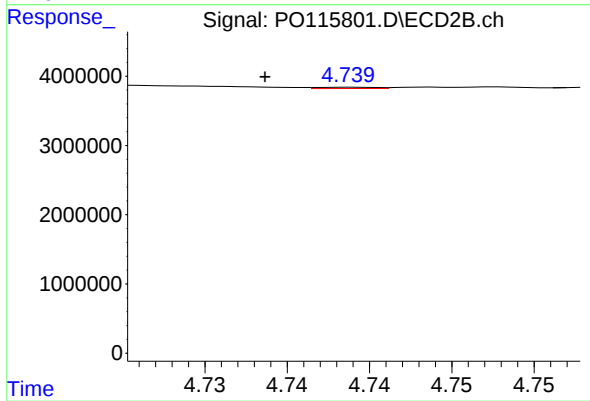

#4 AR-1016-2


R.T.: 4.739 min
Delta R.T.: 0.005 min
Response: 44646
Conc: 0.17 ng/ml

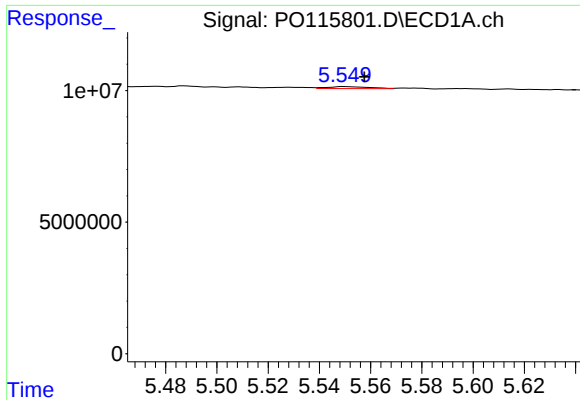

#5 AR-1016-3


R.T.: 5.550 min
Delta R.T.: -0.008 min
Response: 845475
Conc: 3.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

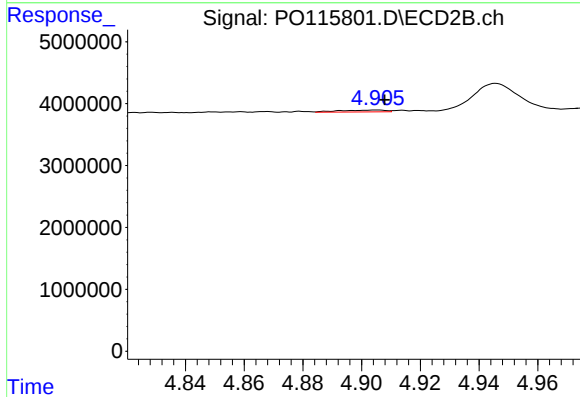


#5 AR-1016-3

R.T.: 4.905 min
Delta R.T.: -0.003 min
Response: 328628
Conc: 2.17 ng/ml

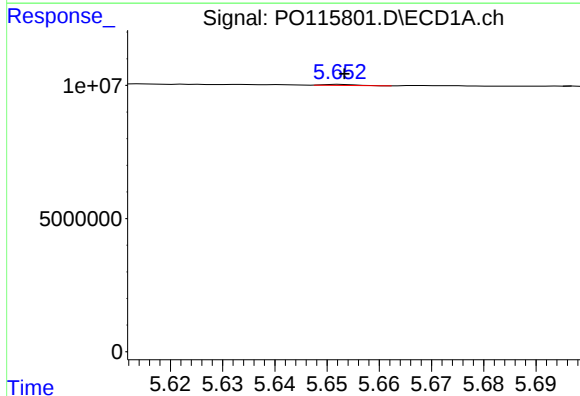


#6 AR-1016-4

R.T.: 5.653 min
Delta R.T.: 0.000 min
Response: 157428
Conc: 0.88 ng/ml

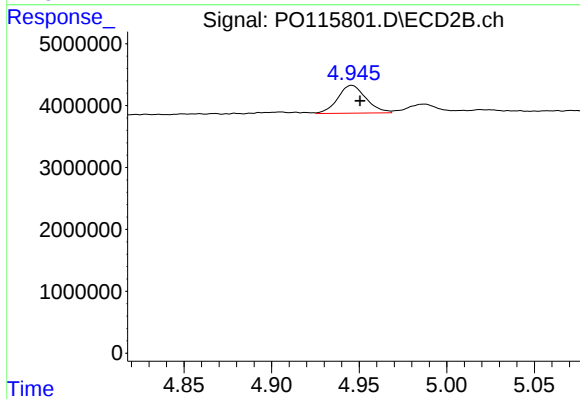

#6 AR-1016-4


R.T.: 4.946 min
Delta R.T.: -0.005 min
Response: 5056347
Conc: 44.86 ng/ml

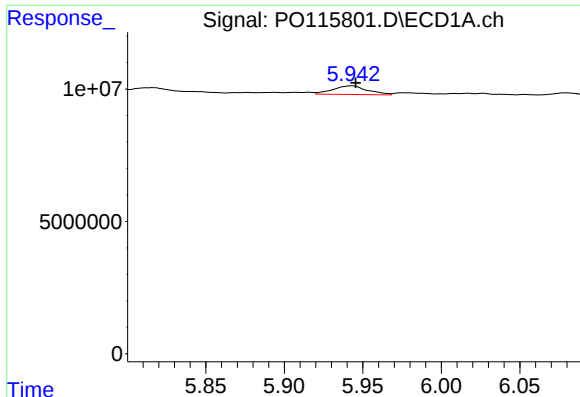

#7 AR-1016-5


R.T.: 5.943 min
Delta R.T.: -0.002 min
Response: 5053933
Conc: 28.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

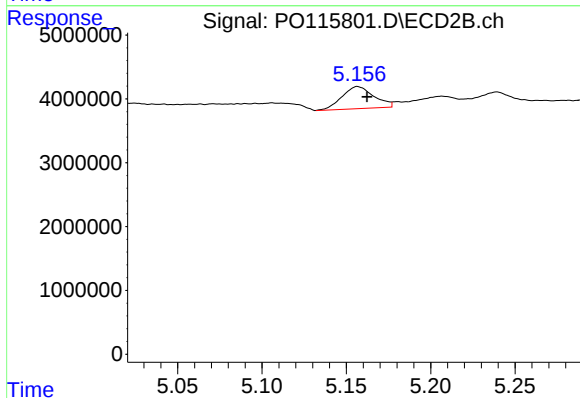


#7 AR-1016-5

R.T.: 5.157 min
Delta R.T.: -0.006 min
Response: 4560613
Conc: 31.16 ng/ml

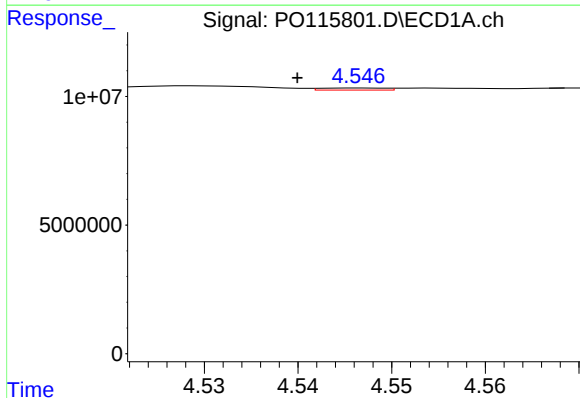


#8 AR-1221-1

R.T.: 4.547 min
Delta R.T.: 0.007 min
Response: 387004
Conc: 4.77 ng/ml

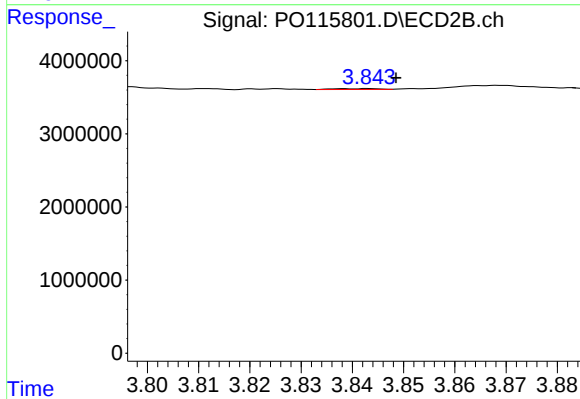

#8 AR-1221-1


R.T.: 3.843 min
Delta R.T.: -0.005 min
Response: 65922
Conc: 1.17 ng/ml

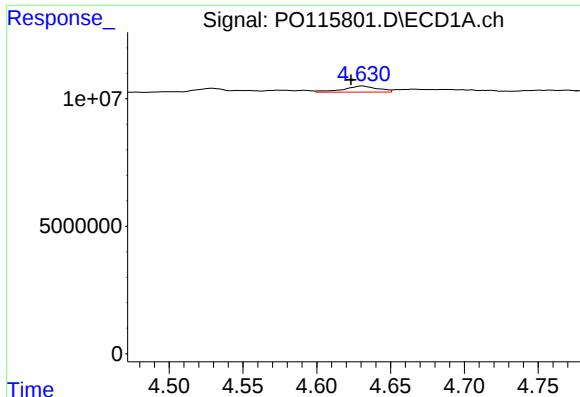

#9 AR-1221-2


R.T.: 4.631 min
Delta R.T.: 0.008 min
Response: 3835648
Conc: 60.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

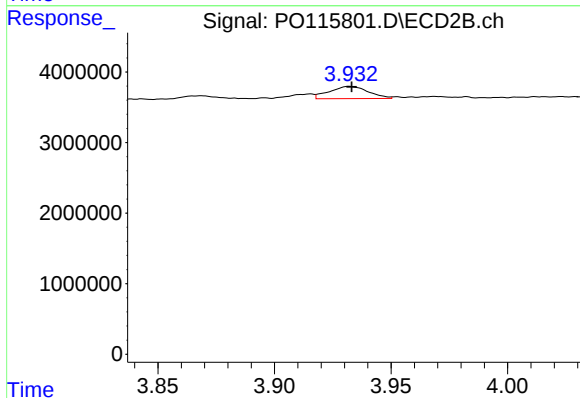


#9 AR-1221-2

R.T.: 3.932 min
Delta R.T.: -0.001 min
Response: 2019017
Conc: 47.57 ng/ml

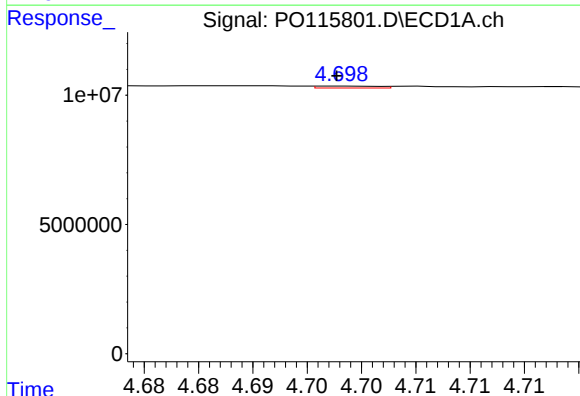


#10 AR-1221-3

R.T.: 4.698 min
Delta R.T.: 0.000 min
Response: 306487
Conc: 1.64 ng/ml

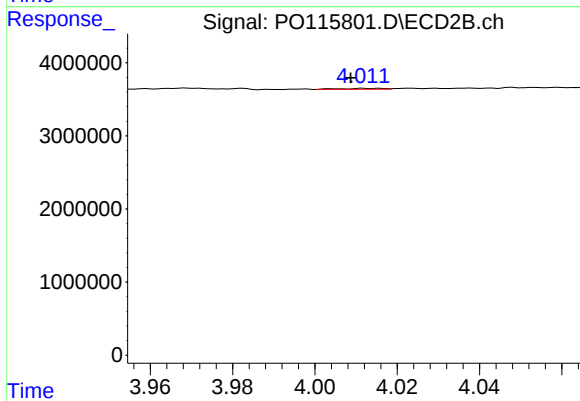

#10 AR-1221-3


R.T.: 4.012 min
Delta R.T.: 0.003 min
Response: 102692
Conc: 0.80 ng/ml

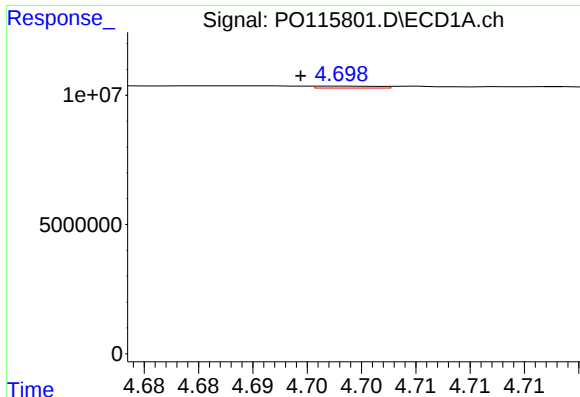

#11 AR-1232-1


R.T.: 4.698 min
Delta R.T.: 0.004 min
Response: 306487
Conc: 2.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

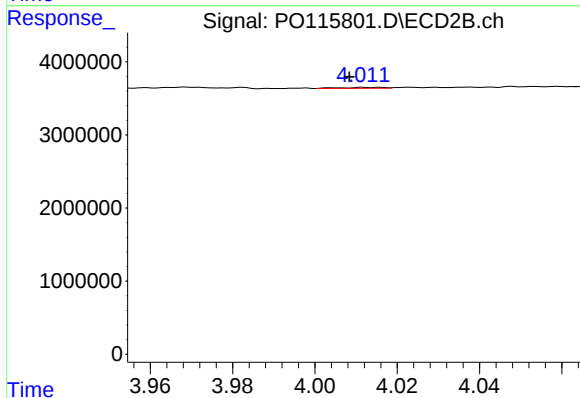


#11 AR-1232-1

R.T.: 4.012 min
Delta R.T.: 0.003 min
Response: 102692
Conc: 0.96 ng/ml

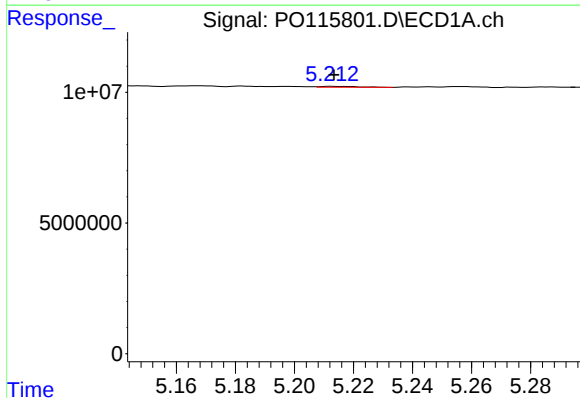


#12 AR-1232-2

R.T.: 5.213 min
Delta R.T.: 0.000 min
Response: 286753
Conc: 3.55 ng/ml

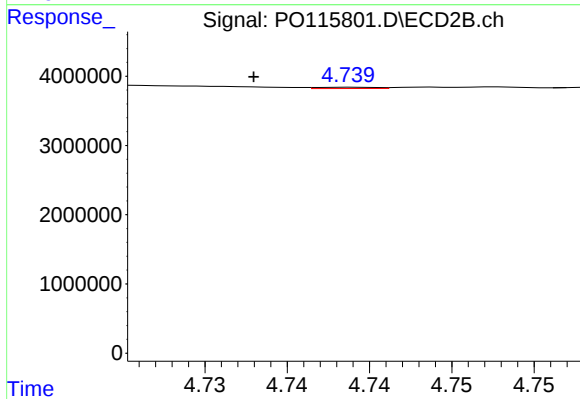

#12 AR-1232-2


R.T.: 4.739 min
Delta R.T.: 0.006 min
Response: 44646
Conc: 0.40 ng/ml

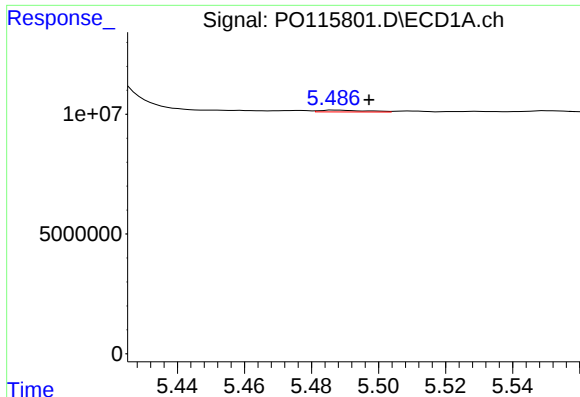

#13 AR-1232-3


R.T.: 5.487 min
Delta R.T.: -0.010 min
Response: 748802
Conc: 4.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

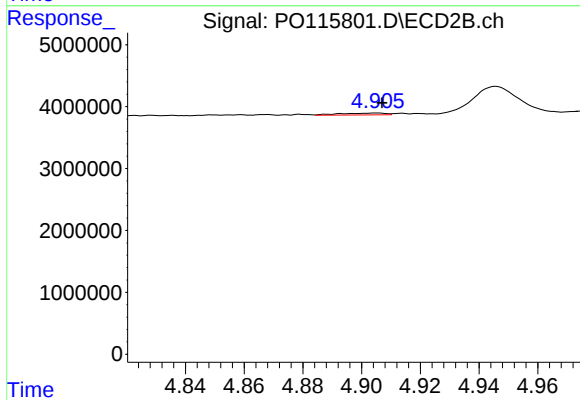


#13 AR-1232-3

R.T.: 4.905 min
Delta R.T.: -0.002 min
Response: 328628
Conc: 5.03 ng/ml

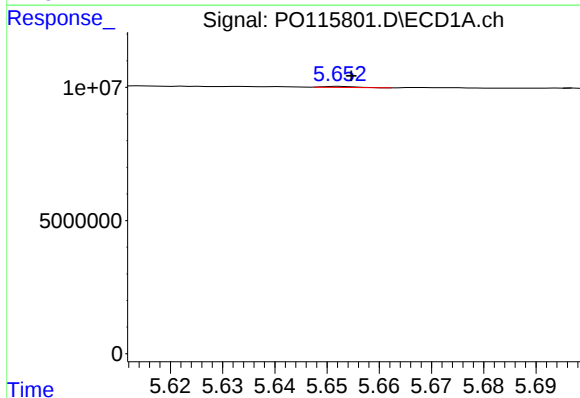


#14 AR-1232-4

R.T.: 5.653 min
Delta R.T.: -0.002 min
Response: 157428
Conc: 2.25 ng/ml

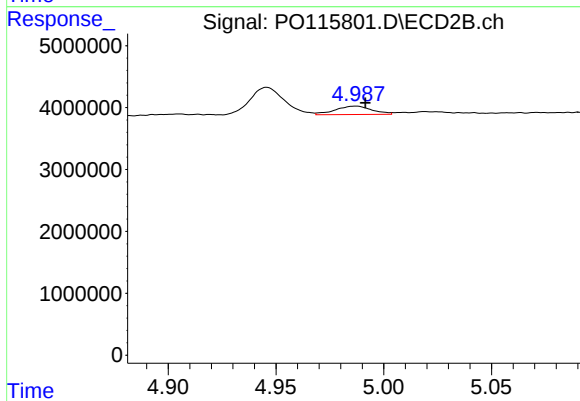

#14 AR-1232-4


R.T.: 4.987 min
Delta R.T.: -0.004 min
Response: 1610487
Conc: 31.38 ng/ml

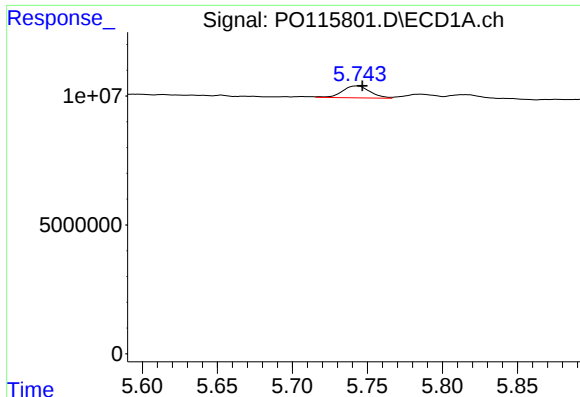

#15 AR-1232-5


R.T.: 5.743 min
Delta R.T.: -0.003 min
Response: 5976711
Conc: 115.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

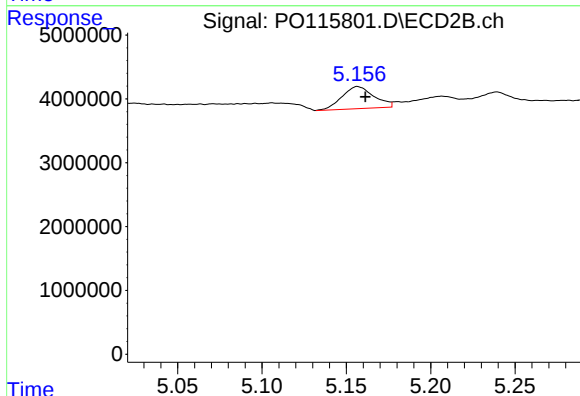


#15 AR-1232-5

R.T.: 5.157 min
Delta R.T.: -0.005 min
Response: 4560613
Conc: 83.30 ng/ml

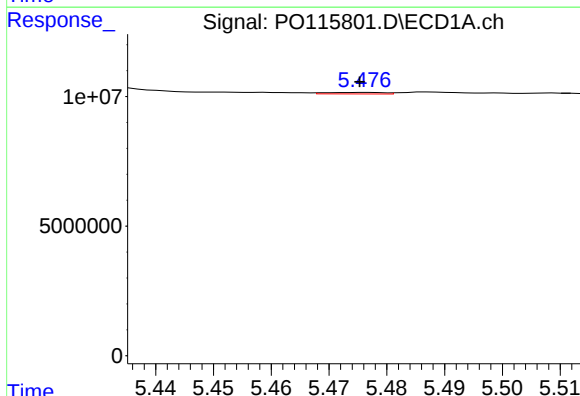


#16 AR-1242-1

R.T.: 5.476 min
Delta R.T.: 0.001 min
Response: 405523
Conc: 2.04 ng/ml

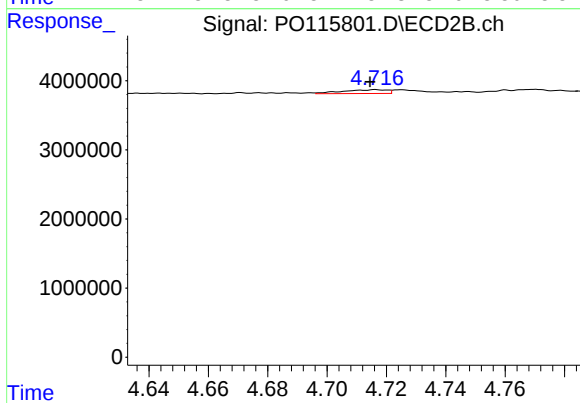

#16 AR-1242-1


R.T.: 4.716 min
Delta R.T.: 0.002 min
Response: 574406
Conc: 4.03 ng/ml

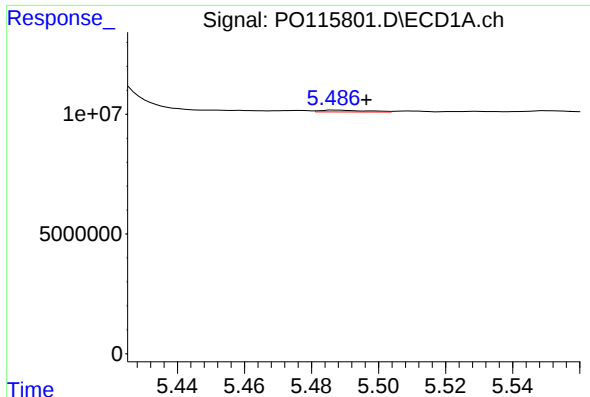

#17 AR-1242-2


R.T.: 5.487 min
Delta R.T.: -0.009 min
Response: 748802
Conc: 2.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

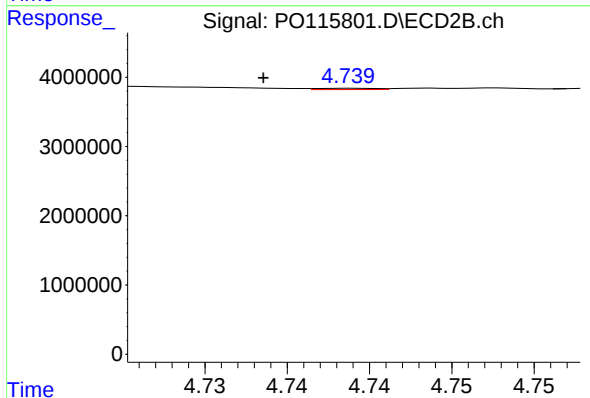


#17 AR-1242-2

R.T.: 4.739 min
Delta R.T.: 0.005 min
Response: 44646
Conc: 0.21 ng/ml

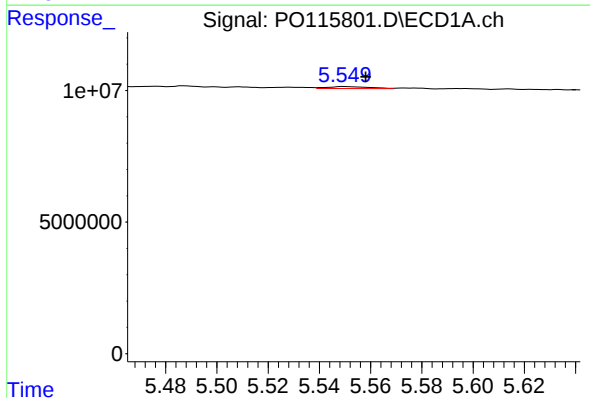


#18 AR-1242-3

R.T.: 5.550 min
Delta R.T.: -0.008 min
Response: 845475
Conc: 5.01 ng/ml

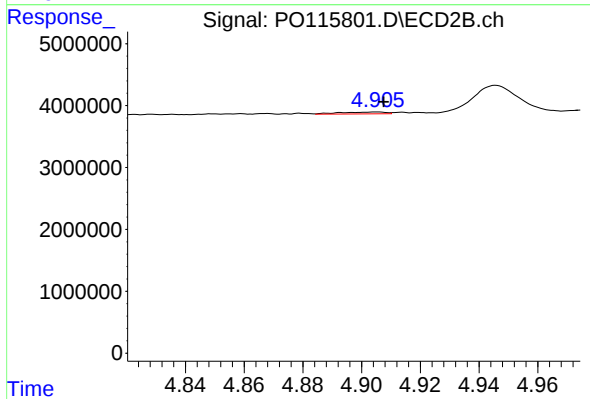

#18 AR-1242-3


R.T.: 4.905 min
Delta R.T.: -0.002 min
Response: 328628
Conc: 2.75 ng/ml

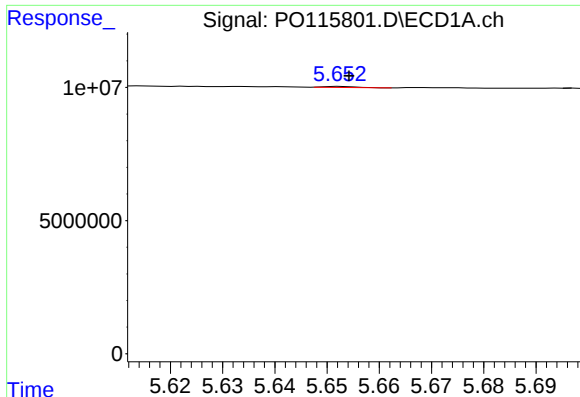

#19 AR-1242-4


R.T.: 5.653 min
Delta R.T.: -0.002 min
Response: 157428
Conc: 1.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

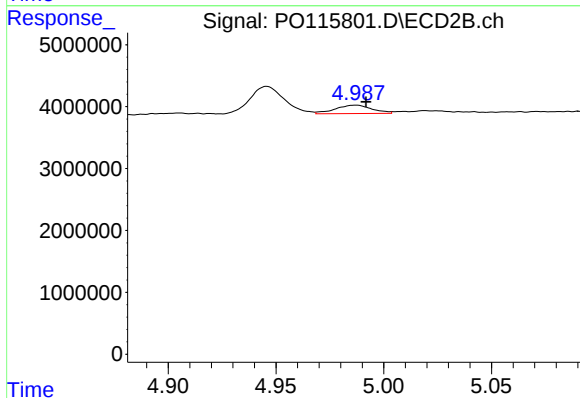


#19 AR-1242-4

R.T.: 4.987 min
Delta R.T.: -0.004 min
Response: 1610487
Conc: 14.76 ng/ml

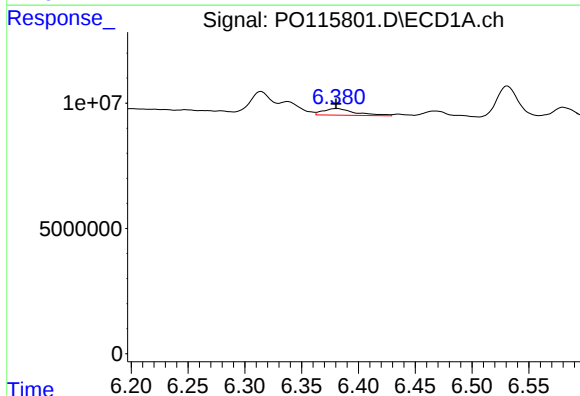


#20 AR-1242-5

R.T.: 6.381 min
Delta R.T.: 0.000 min
Response: 5230339
Conc: 34.54 ng/ml

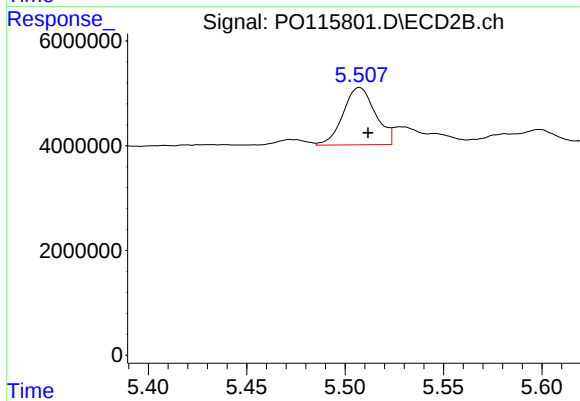

#20 AR-1242-5


R.T.: 5.507 min
Delta R.T.: -0.004 min
Response: 12516666
Conc: 90.62 ng/ml

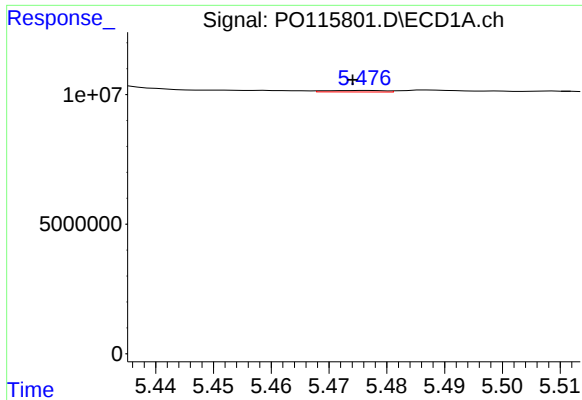

#21 AR-1248-1


R.T.: 5.476 min
Delta R.T.: 0.002 min
Response: 405523
Conc: 2.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

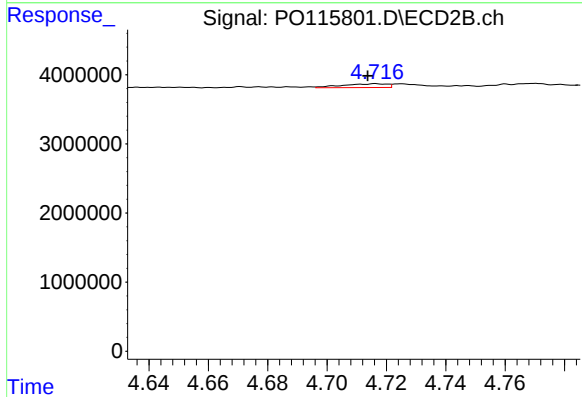


#21 AR-1248-1

R.T.: 4.716 min
Delta R.T.: 0.003 min
Response: 574406
Conc: 5.14 ng/ml

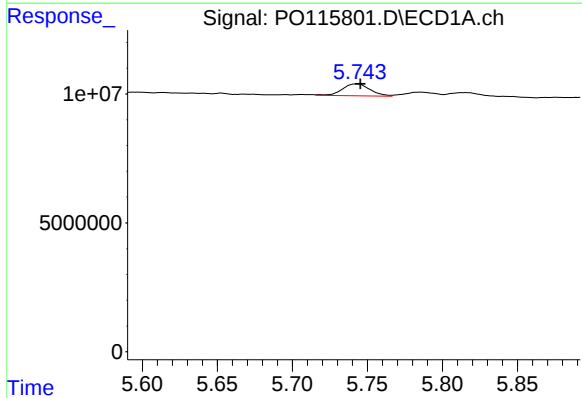


#22 AR-1248-2

R.T.: 5.743 min
Delta R.T.: -0.002 min
Response: 5976711
Conc: 29.76 ng/ml

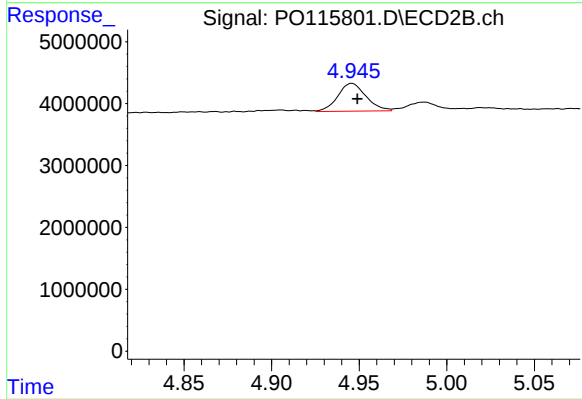

#22 AR-1248-2


R.T.: 4.946 min
Delta R.T.: -0.003 min
Response: 5056347
Conc: 33.20 ng/ml

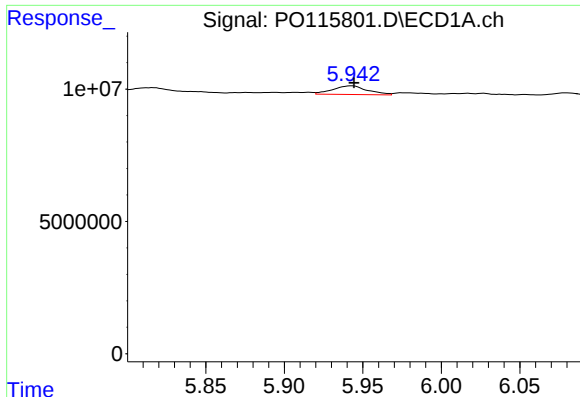

#23 AR-1248-3


R.T.: 5.943 min
Delta R.T.: -0.001 min
Response: 5053933
Conc: 20.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

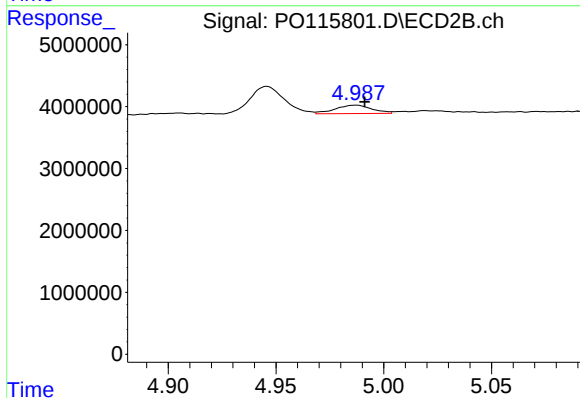


#23 AR-1248-3

R.T.: 4.987 min
Delta R.T.: -0.004 min
Response: 1610487
Conc: 10.03 ng/ml

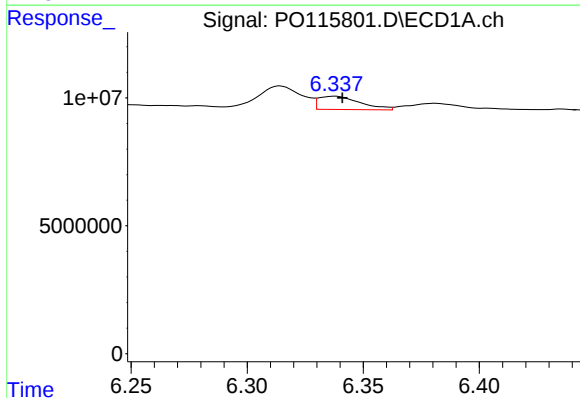


#24 AR-1248-4

R.T.: 6.338 min
Delta R.T.: -0.003 min
Response: 6436863
Conc: 21.83 ng/ml

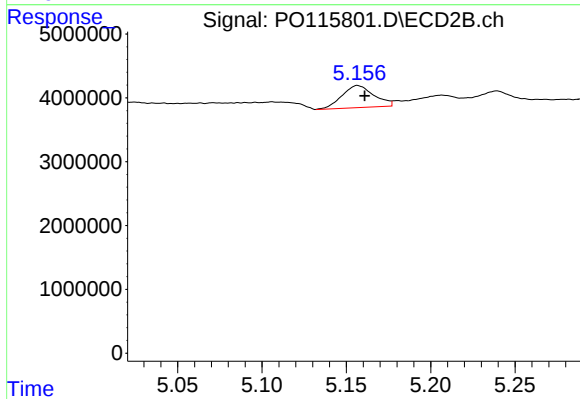

#24 AR-1248-4


R.T.: 5.157 min
Delta R.T.: -0.004 min
Response: 4560613
Conc: 24.37 ng/ml

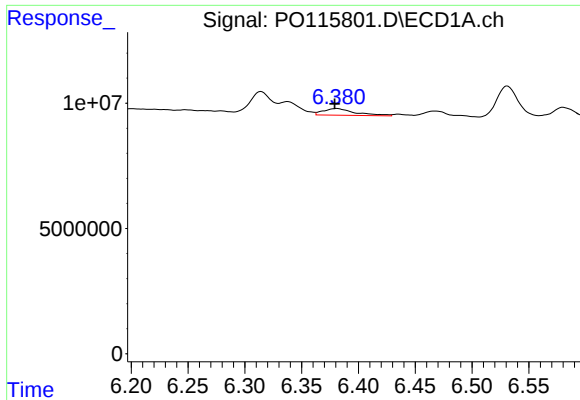

#25 AR-1248-5


R.T.: 6.381 min
Delta R.T.: 0.002 min
Response: 5230339
Conc: 20.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

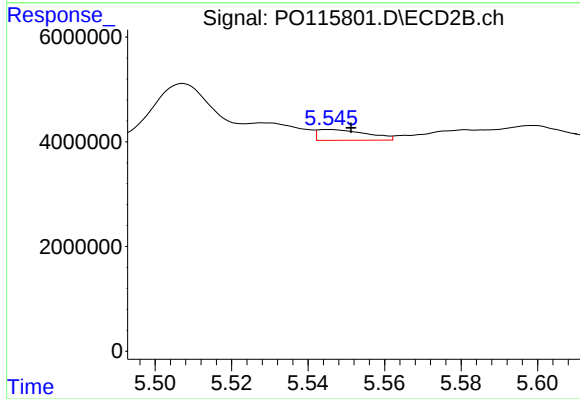


#25 AR-1248-5

R.T.: 5.545 min
Delta R.T.: -0.006 min
Response: 1828068
Conc: 9.23 ng/ml

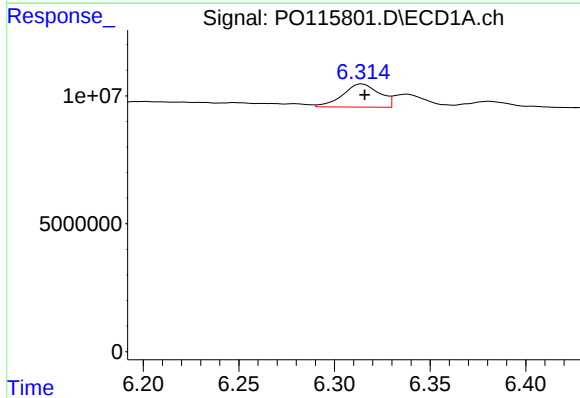


#26 AR-1254-1

R.T.: 6.314 min
Delta R.T.: -0.001 min
Response: 12068587
Conc: 46.65 ng/ml

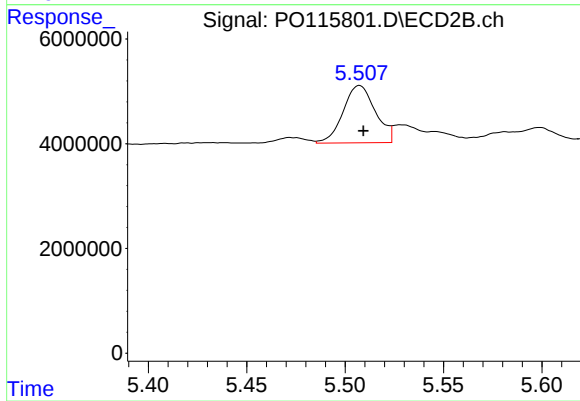

#26 AR-1254-1


R.T.: 5.507 min
Delta R.T.: -0.002 min
Response: 12516666
Conc: 42.83 ng/ml

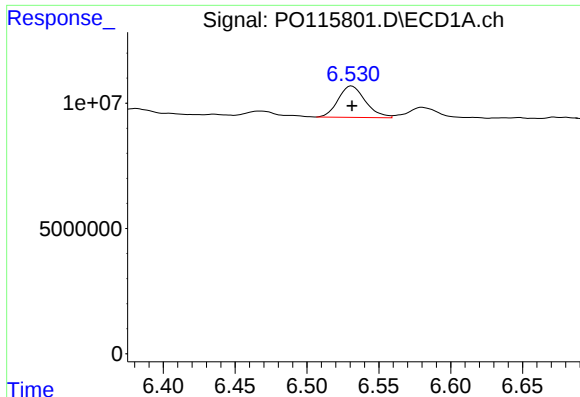

#27 AR-1254-2


R.T.: 6.531 min
Delta R.T.: 0.000 min
Response: 16457695
Conc: 40.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

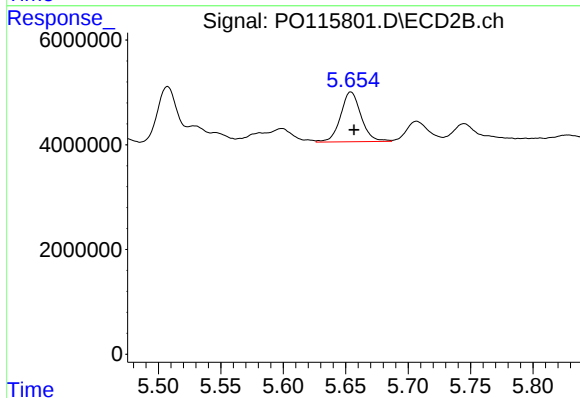


#27 AR-1254-2

R.T.: 5.654 min
Delta R.T.: -0.003 min
Response: 10894788
Conc: 43.27 ng/ml

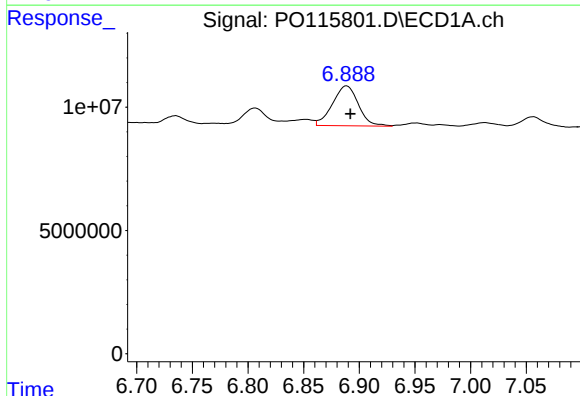


#28 AR-1254-3

R.T.: 6.889 min
Delta R.T.: -0.003 min
Response: 26270768
Conc: 63.99 ng/ml

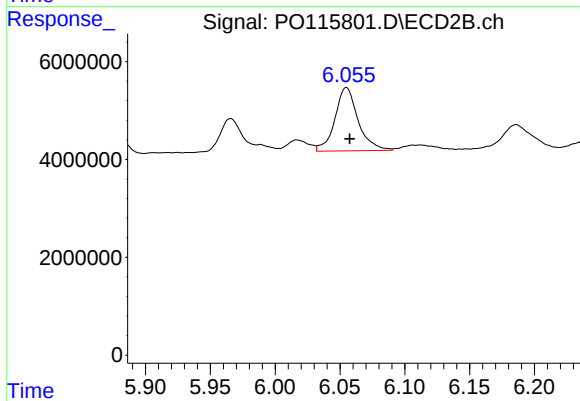

#28 AR-1254-3


R.T.: 6.055 min
Delta R.T.: -0.003 min
Response: 16136446
Conc: 41.00 ng/ml

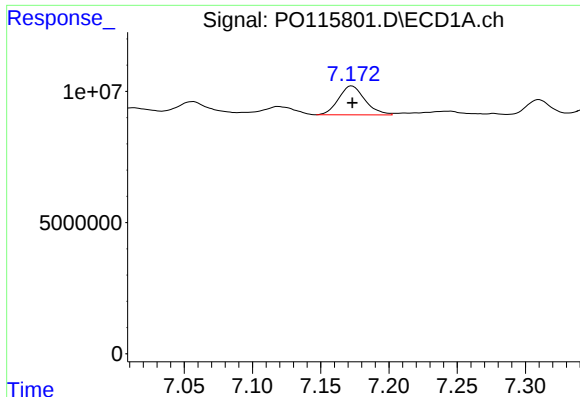

#29 AR-1254-4


R.T.: 7.173 min
Delta R.T.: 0.000 min
Response: 14840182
Conc: 42.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

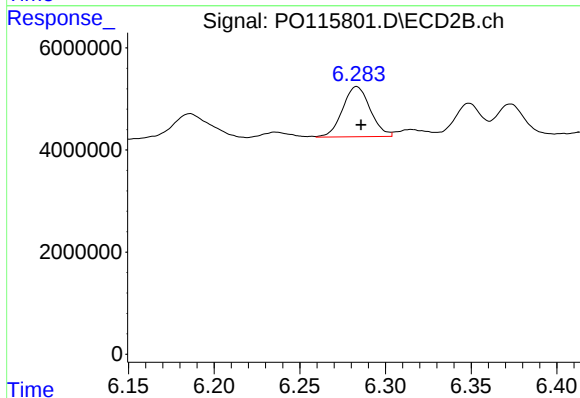


#29 AR-1254-4

R.T.: 6.283 min
Delta R.T.: -0.003 min
Response: 11043898
Conc: 41.27 ng/ml

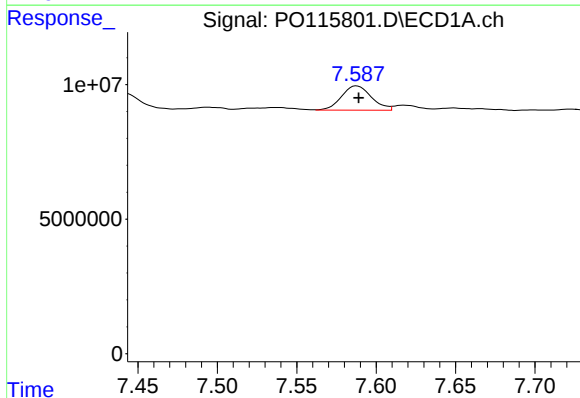


#30 AR-1254-5

R.T.: 7.588 min
Delta R.T.: -0.001 min
Response: 11767468
Conc: 36.31 ng/ml

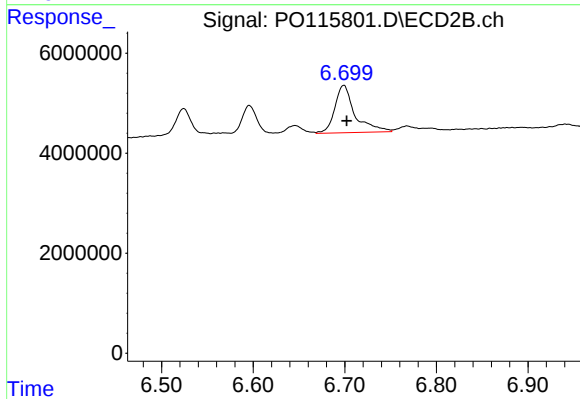

#30 AR-1254-5


R.T.: 6.699 min
Delta R.T.: -0.003 min
Response: 14518638
Conc: 40.61 ng/ml

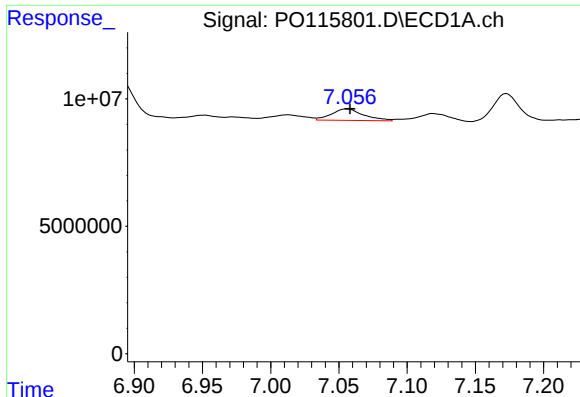

#31 AR-1260-1


R.T.: 7.056 min
Delta R.T.: -0.002 min
Response: 7380517
Conc: 25.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

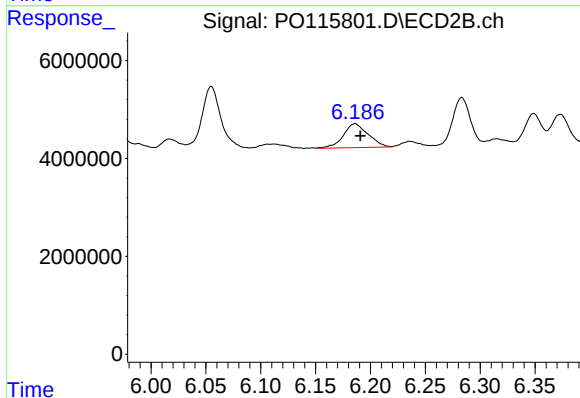


#31 AR-1260-1

R.T.: 6.186 min
Delta R.T.: -0.005 min
Response: 7708414
Conc: 29.40 ng/ml

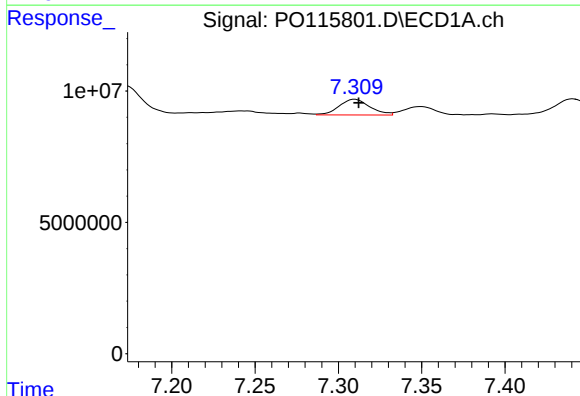


#32 AR-1260-2

R.T.: 7.310 min
Delta R.T.: -0.002 min
Response: 7700851
Conc: 17.59 ng/ml

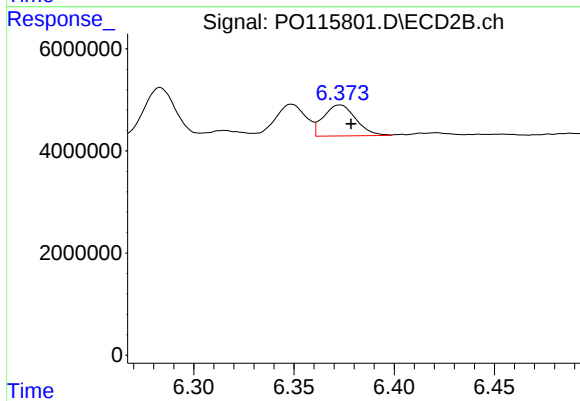

#32 AR-1260-2


R.T.: 6.373 min
Delta R.T.: -0.005 min
Response: 6797048
Conc: 19.40 ng/ml

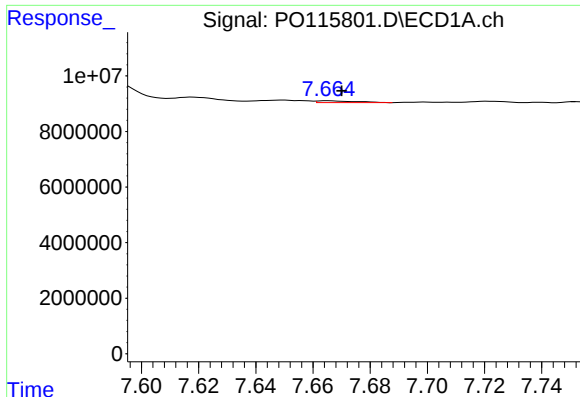

#33 AR-1260-3


R.T.: 7.665 min
Delta R.T.: -0.005 min
Response: 602190
Conc: 1.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

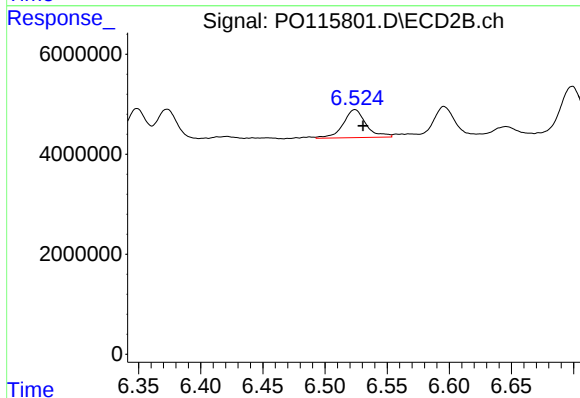


#33 AR-1260-3

R.T.: 6.524 min
Delta R.T.: -0.006 min
Response: 7197771
Conc: 22.40 ng/ml

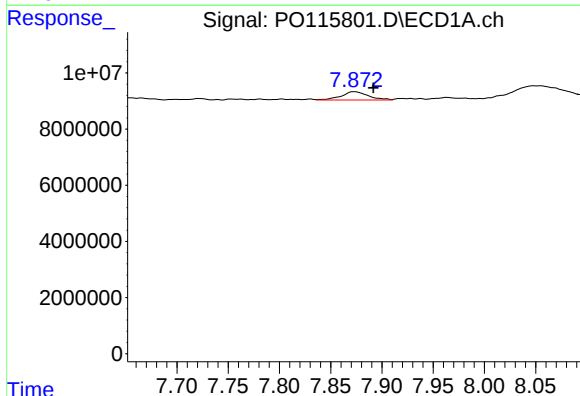


#34 AR-1260-4

R.T.: 7.873 min
Delta R.T.: -0.019 min
Response: 5367088
Conc: 17.46 ng/ml

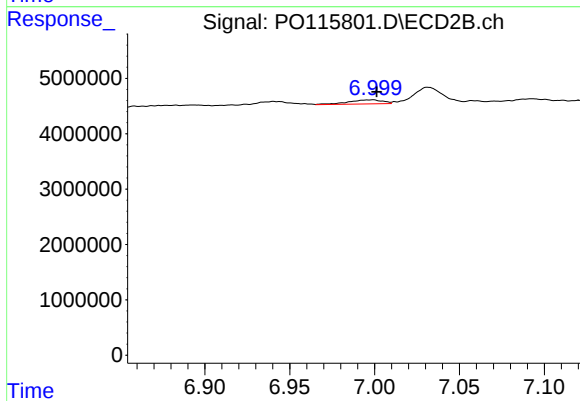

#34 AR-1260-4


R.T.: 6.999 min
Delta R.T.: -0.003 min
Response: 1008076
Conc: 3.92 ng/ml

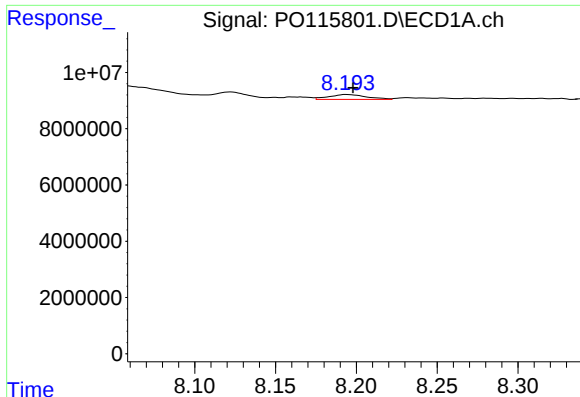

#35 AR-1260-5


R.T.: 8.194 min
Delta R.T.: -0.004 min
Response: 2871525
Conc: 3.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

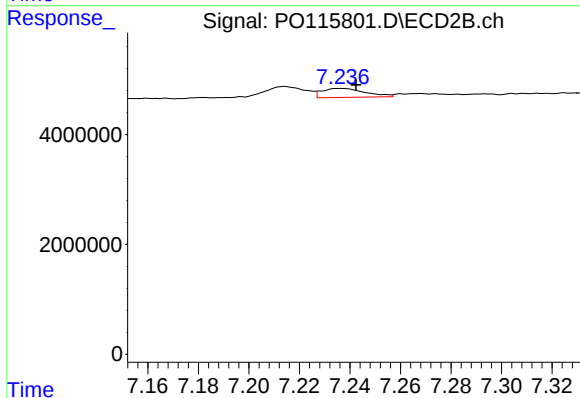


#35 AR-1260-5

R.T.: 7.236 min
Delta R.T.: -0.006 min
Response: 1959279
Conc: 2.79 ng/ml

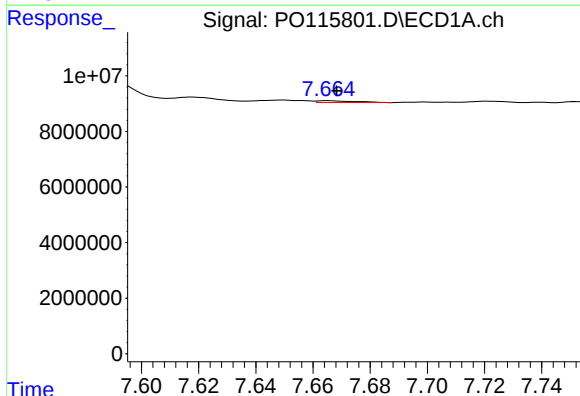


#36 AR-1262-1

R.T.: 7.665 min
Delta R.T.: -0.003 min
Response: 602190
Conc: 2.44 ng/ml

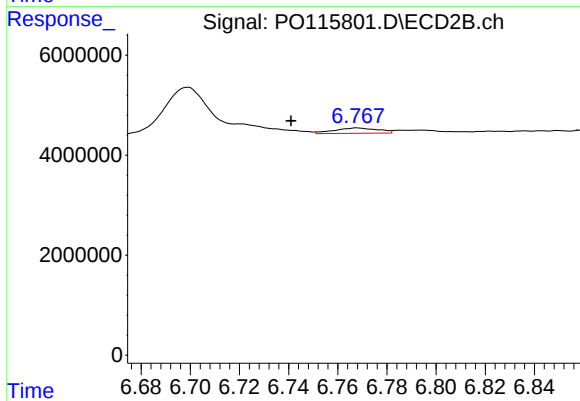

#36 AR-1262-1


R.T.: 6.768 min
Delta R.T.: 0.027 min
Response: 1305221
Conc: 6.13 ng/ml

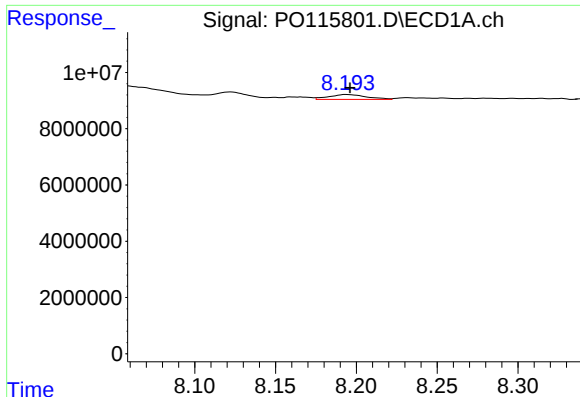

#37 AR-1262-2


R.T.: 8.194 min
Delta R.T.: -0.002 min
Response: 2871525
Conc: 7.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

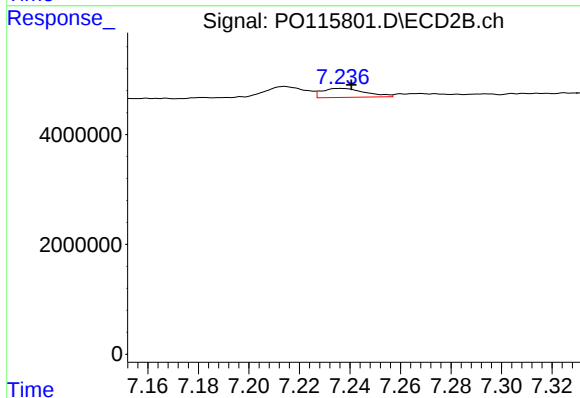


#37 AR-1262-2

R.T.: 7.236 min
Delta R.T.: -0.004 min
Response: 1959279
Conc: 5.62 ng/ml

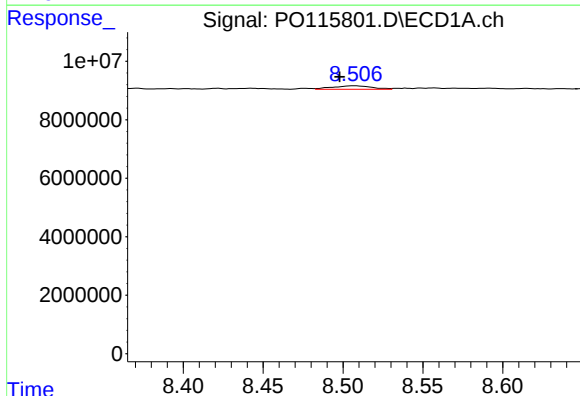


#38 AR-1262-3

R.T.: 8.507 min
Delta R.T.: 0.009 min
Response: 1996864
Conc: 7.84 ng/ml

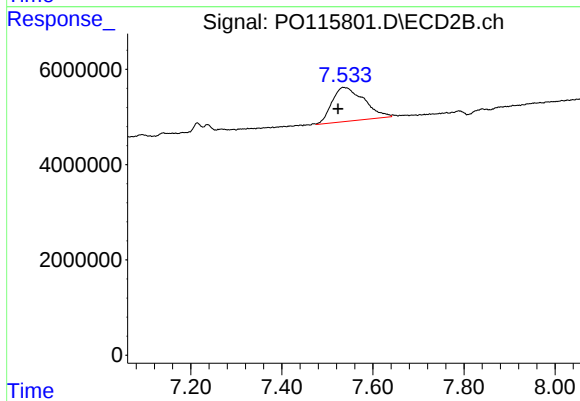

#38 AR-1262-3


R.T.: 7.535 min
Delta R.T.: 0.011 min
Response: 34777460
Conc: 222.38 ng/ml

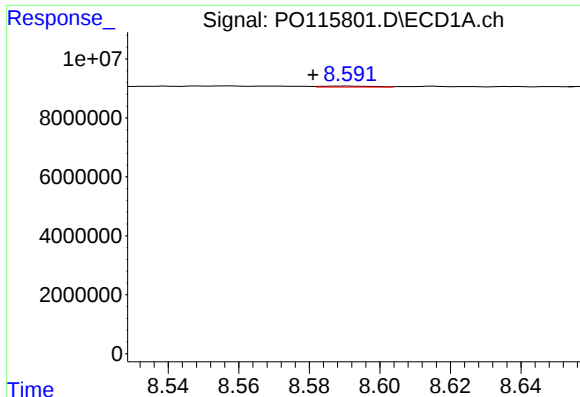

#39 AR-1262-4


R.T.: 8.591 min
Delta R.T.: 0.010 min
Response: 329786
Conc: 1.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

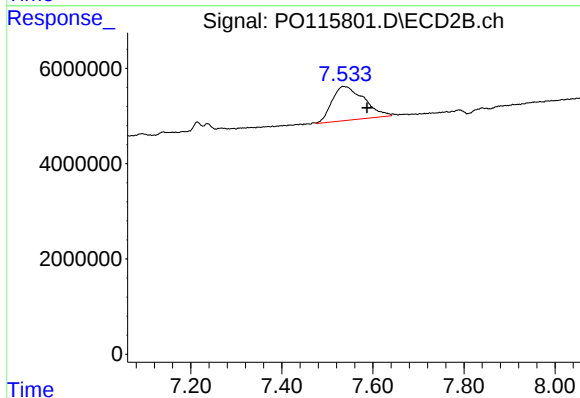


#39 AR-1262-4

R.T.: 7.535 min
Delta R.T.: -0.052 min
Response: 34777460
Conc: 140.59 ng/ml

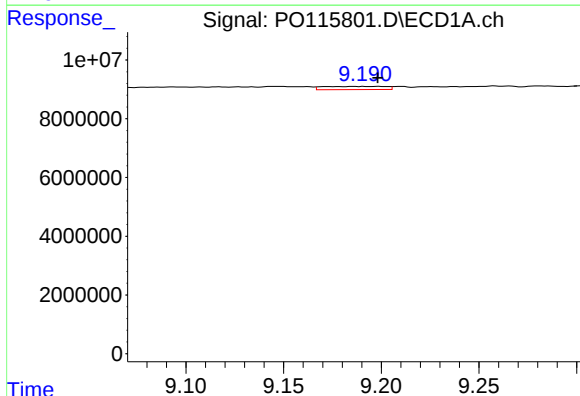


#40 AR-1262-5

R.T.: 9.199 min
Delta R.T.: 0.000 min
Response: 2363237
Conc: 17.55 ng/ml

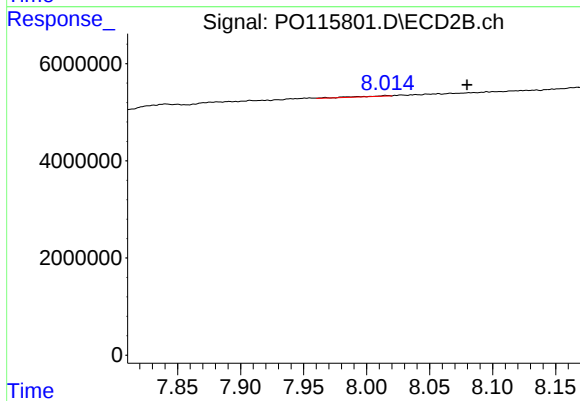

#40 AR-1262-5


R.T.: 8.015 min
Delta R.T.: -0.064 min
Response: 295143
Conc: 2.65 ng/ml

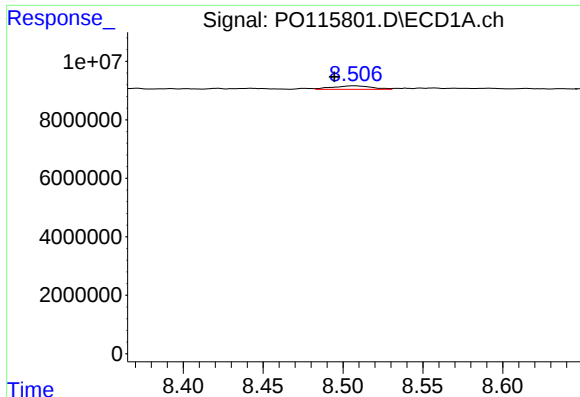

#41 AR-1268-1


R.T.: 8.507 min
Delta R.T.: 0.012 min
Response: 1996864
Conc: 2.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

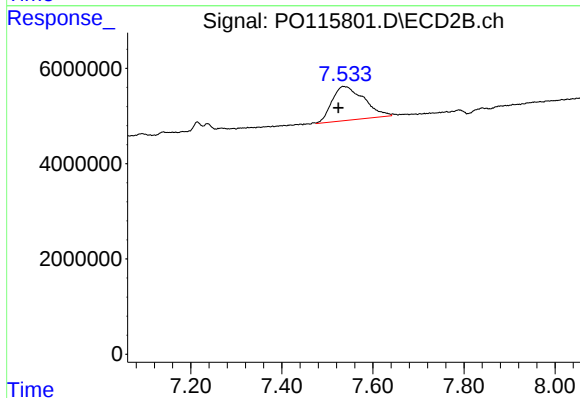


#41 AR-1268-1

R.T.: 7.535 min
Delta R.T.: 0.010 min
Response: 34777460
Conc: 39.25 ng/ml

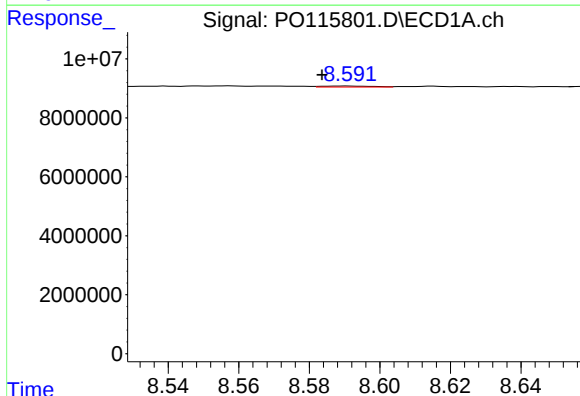


#42 AR-1268-2

R.T.: 8.591 min
Delta R.T.: 0.008 min
Response: 329786
Conc: 0.39 ng/ml

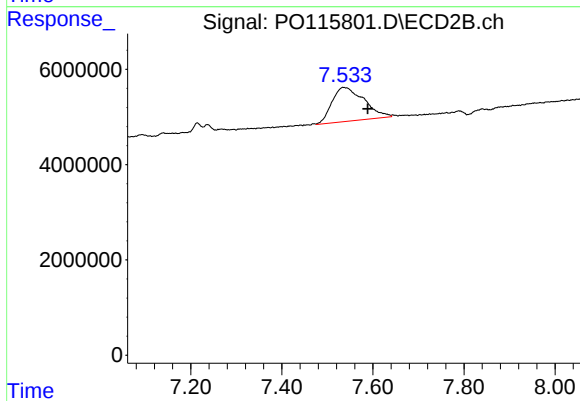

#42 AR-1268-2


R.T.: 7.535 min
Delta R.T.: -0.054 min
Response: 34777460
Conc: 46.43 ng/ml

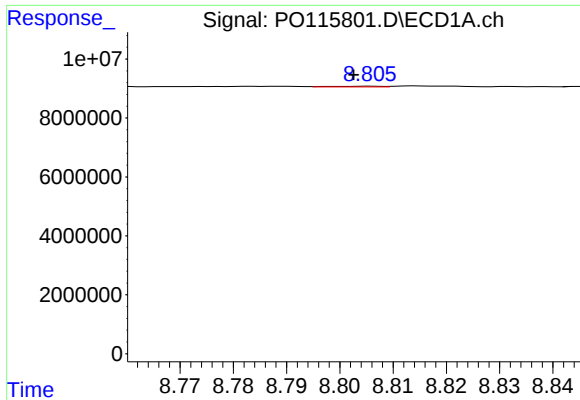

#43 AR-1268-3


R.T.: 8.806 min
Delta R.T.: 0.003 min
Response: 144286
Conc: 0.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

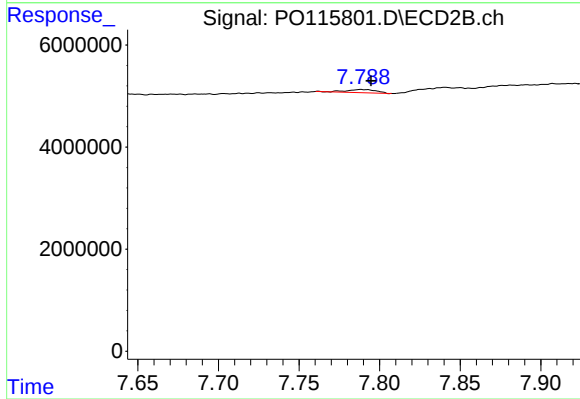


#43 AR-1268-3

R.T.: 7.789 min
Delta R.T.: -0.006 min
Response: 799793
Conc: 1.26 ng/ml

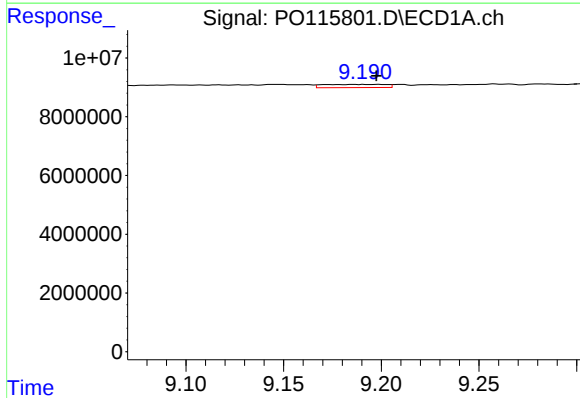


#44 AR-1268-4

R.T.: 9.199 min
Delta R.T.: 0.001 min
Response: 2363237
Conc: 7.57 ng/ml

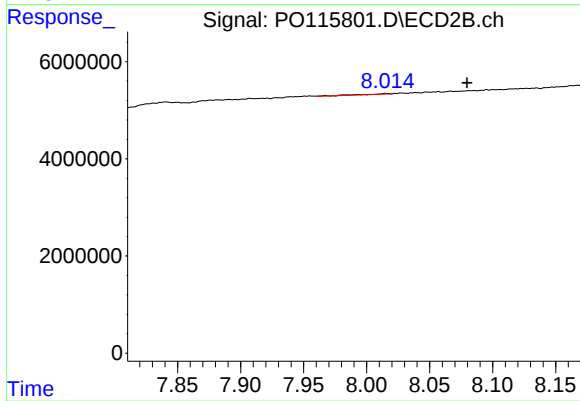

#44 AR-1268-4


R.T.: 8.015 min
Delta R.T.: -0.065 min
Response: 295143
Conc: 1.15 ng/ml

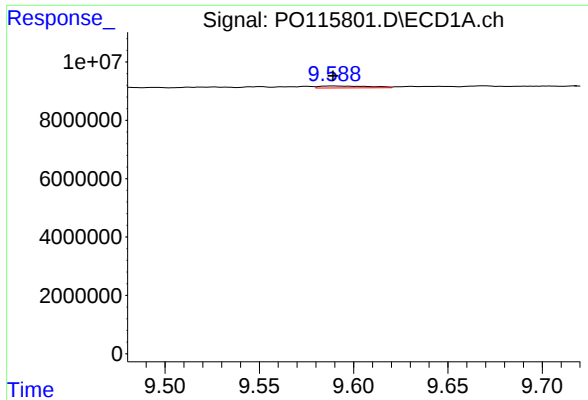

#45 AR-1268-5

R.T.: 9.589 min
Delta R.T.: 0.000 min
Response: 1287976
Conc: 0.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

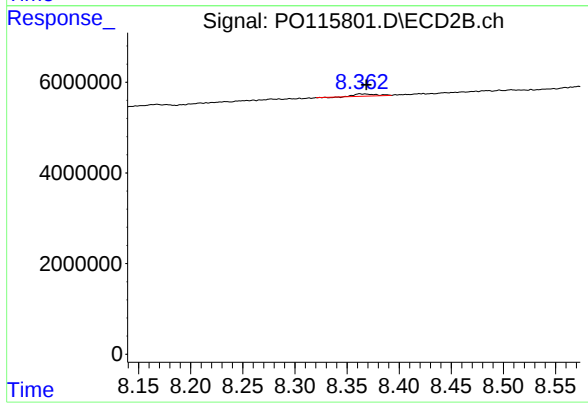

#45 AR-1268-5

R.T.: 8.362 min
Delta R.T.: -0.006 min
Response: 662414
Conc: 0.39 ng/ml