

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO121225\
 Data File : PO115841.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Dec 2025 09:24
 Operator : YP/AJ
 Sample : Q3530-09
 Misc : AR1221 25PPB WATER MDL
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 MDL-WATER-03-QT4-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 02:41:51 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO120425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 05 02:11:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.332	3.634	183.5E6	112.4E6	23.619	23.068
2)	SA Decachlor...	9.907	8.615	125.6E6	93870760	23.871	21.829
Target Compounds							
3)	L1 AR-1016-1	5.476	4.709	877597	4014929	3.529	21.730 #
4)	L1 AR-1016-2	5.497	4.727	669908	4986392	1.759	18.866 #
5)	L1 AR-1016-3	5.557	4.904	926751	7468498	4.335	49.350 #
6)	L1 AR-1016-4	5.639	4.904f	189540	7468498	1.061	66.266 #
7)	L1 AR-1016-5	5.949	5.205f	2391599	18071361	13.633	123.488 #
8)	L2 AR-1221-1	4.537	3.845	1980788	2152389	24.395	38.159 #
9)	L2 AR-1221-2	4.628	3.930	3976810	3298300	63.105	77.710
10)	L2 AR-1221-3	4.691	4.004	8185088	4491002	43.837	34.924
11)	L3 AR-1232-1	4.691	4.004	8185088	4491002	54.690	42.036
12)	L3 AR-1232-2	5.204	4.727	1199284	4986392	14.833	44.927 #
13)	L3 AR-1232-3	5.497	4.904	669908	7468498	4.353	114.256 #
14)	L3 AR-1232-4	5.639	5.021	189540	6906808	2.707	134.557 #
15)	L3 AR-1232-5	5.750	5.205f	53848	18071361	1.037	330.082 #
16)	L4 AR-1242-1	5.476	4.709	877597	4014929	4.418	28.197 #
17)	L4 AR-1242-2	5.497	4.727	669908	4986392	2.287	23.817 #
18)	L4 AR-1242-3	5.557	4.904	926751	7468498	5.490	62.528 #
19)	L4 AR-1242-4	5.639	5.021	189540	6906808	1.387	63.312 #
20)	L4 AR-1242-5	6.376	5.528	4491919	18832070	29.661	136.341 #
21)	L5 AR-1248-1	5.476	4.709	877597	4014929	5.783	35.902 #
22)	L5 AR-1248-2	5.750	4.904f	53848	7468498	0.268	49.041 #
23)	L5 AR-1248-3	5.942	5.021	1669310	6906808	6.769	43.026 #
24)	L5 AR-1248-4	6.359	5.205f	8495403	18071361	28.812	96.563 #
25)	L5 AR-1248-5	6.376	5.570	4491919	2674374	17.348	13.510
26)	L6 AR-1254-1	6.301	5.528	4488718	18832070	17.350	64.434 #
27)	L6 AR-1254-2	6.535	5.645	11302690	5478680	28.088	21.757
28)	L6 AR-1254-3	6.880	6.064	47897157	6374213	116.661	16.195 #
29)	L6 AR-1254-4	7.178	6.284	7999499	2140835	23.049	8.001 #
30)	L6 AR-1254-5	7.607	6.706	3324882	625899	10.261	1.751 #
31)	L7 AR-1260-1	7.058	6.195	4703184	2557475	16.235	9.755 #
32)	L7 AR-1260-2	7.322	6.404	3554708	667907	8.121	1.906 #
33)	L7 AR-1260-3	7.676	6.507	2416076	205050	7.178	0.638 #
34)	L7 AR-1260-4	7.883	7.019	2165716	1615139	7.044	6.289
35)	L7 AR-1260-5	8.197	7.234	1468274	676711	2.016	0.965 #
36)	L8 AR-1262-1	7.662	6.738	2949124	599086	11.947	2.812 #
37)	L8 AR-1262-2	8.197	7.234	1468274	676711	3.709	1.943 #
38)	L8 AR-1262-3	8.493	7.532	691286	100.1E6	2.713	639.963 #
39)	L8 AR-1262-4	8.577	7.532f	881327	100.1E6	4.550	404.590 #
40)	L8 AR-1262-5	9.186	8.071	1135933	123656	8.434	1.109 #
41)	L9 AR-1268-1	8.493	7.532	691286	100.1E6	0.694	112.968 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121225\
 Data File : PO115841.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Dec 2025 09:24
 Operator : YP/AJ
 Sample : Q3530-09
 Misc : AR1221 25PPB WATER MDL
 ALS Vial : 20 Sample Multiplier: 1


Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT4-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 02:41:51 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 05 02:11:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.577	7.532f	881327	100.1E6	1.030	133.611 #
43) L9	AR-1268-3	8.806	7.789	834768	943006	1.124	1.481 #
44) L9	AR-1268-4	9.186	8.071	1135933	123656	3.638	0.480 #
45) L9	AR-1268-5	9.597	8.366	1261442	705769	0.579	0.419 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

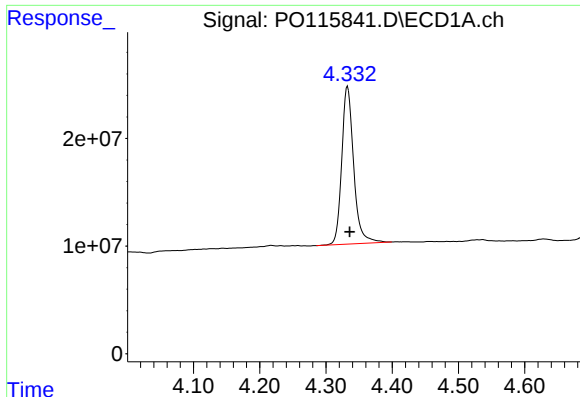

#1 Tetrachloro-m-xylene


R.T.: 4.332 min
Delta R.T.: -0.004 min
Response: 183450985
Conc: 23.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

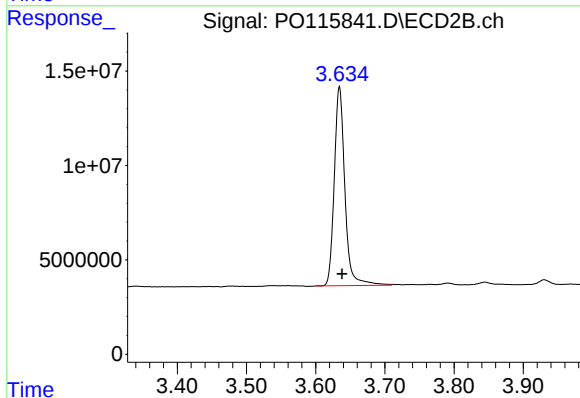


#1 Tetrachloro-m-xylene

R.T.: 3.634 min
Delta R.T.: -0.004 min
Response: 112418835
Conc: 23.07 ng/ml

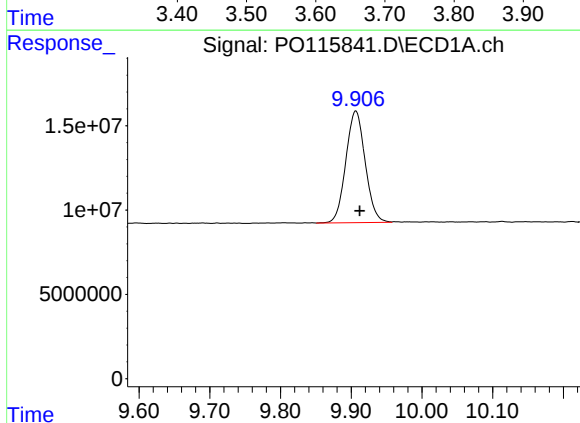


#2 Decachlorobiphenyl

R.T.: 9.907 min
Delta R.T.: -0.006 min
Response: 125588282
Conc: 23.87 ng/ml

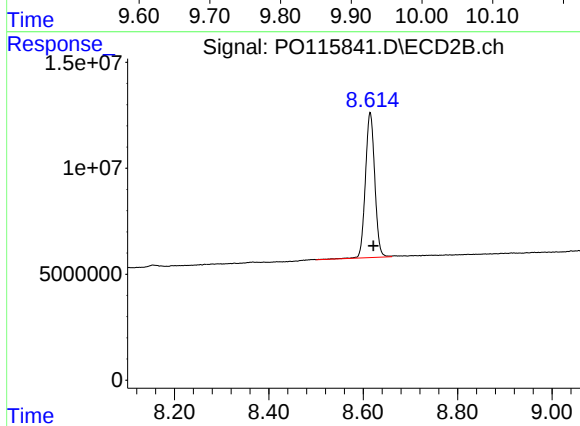

#2 Decachlorobiphenyl


R.T.: 8.615 min
Delta R.T.: -0.007 min
Response: 93870760
Conc: 21.83 ng/ml

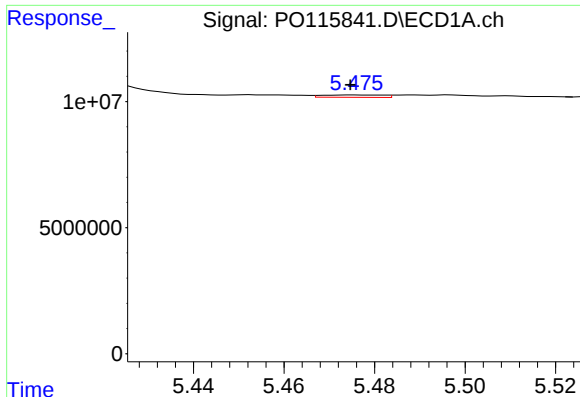

#3 AR-1016-1


R.T.: 5.476 min
Delta R.T.: 0.000 min
Response: 877597
Conc: 3.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

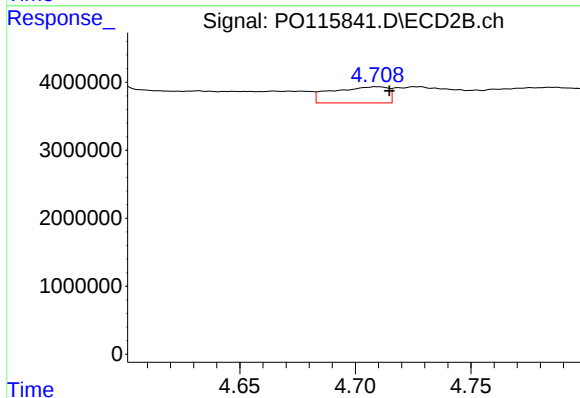


#3 AR-1016-1

R.T.: 4.709 min
Delta R.T.: -0.005 min
Response: 4014929
Conc: 21.73 ng/ml

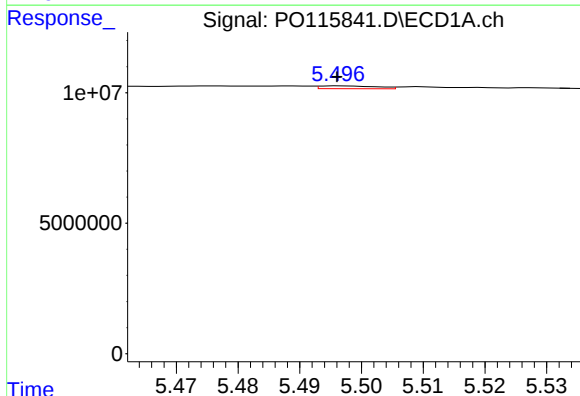


#4 AR-1016-2

R.T.: 5.497 min
Delta R.T.: 0.000 min
Response: 669908
Conc: 1.76 ng/ml

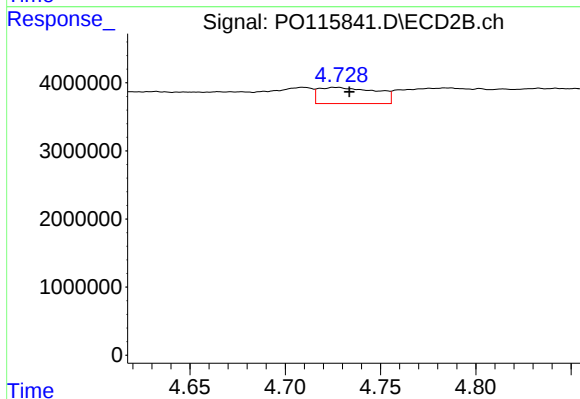

#4 AR-1016-2


R.T.: 4.727 min
Delta R.T.: -0.007 min
Response: 4986392
Conc: 18.87 ng/ml

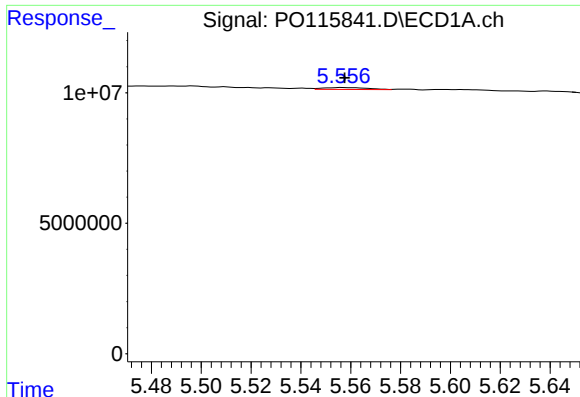

#5 AR-1016-3


R.T.: 5.557 min
Delta R.T.: 0.000 min
Response: 926751
Conc: 4.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

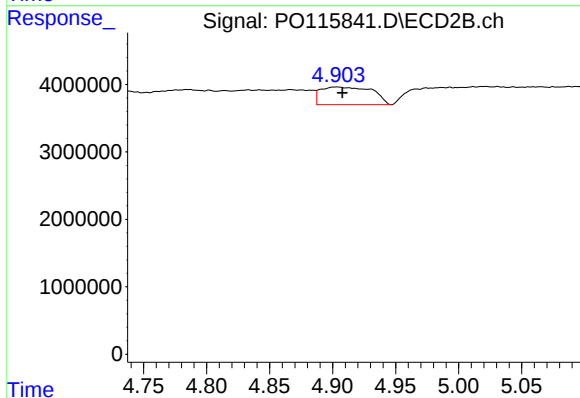


#5 AR-1016-3

R.T.: 4.904 min
Delta R.T.: -0.004 min
Response: 7468498
Conc: 49.35 ng/ml

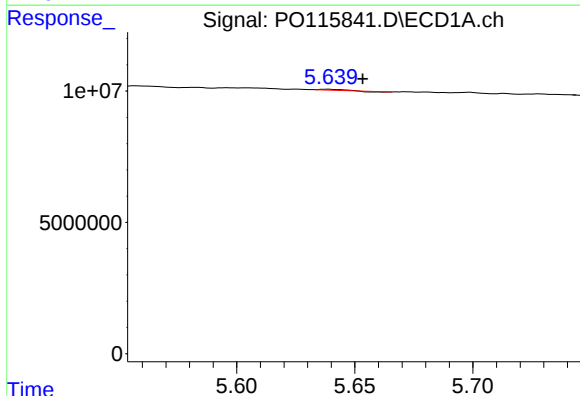


#6 AR-1016-4

R.T.: 5.639 min
Delta R.T.: -0.014 min
Response: 189540
Conc: 1.06 ng/ml

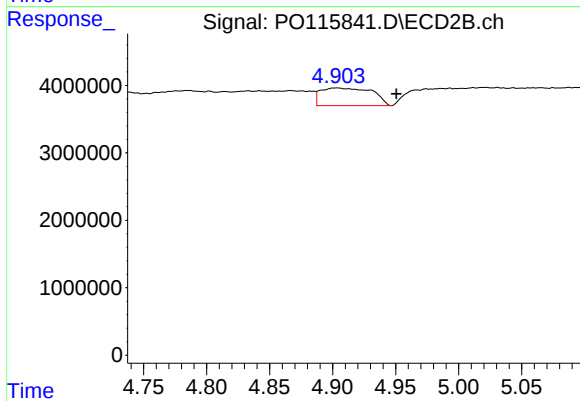

#6 AR-1016-4


R.T.: 4.904 min
Delta R.T.: -0.047 min
Response: 7468498
Conc: 66.27 ng/ml

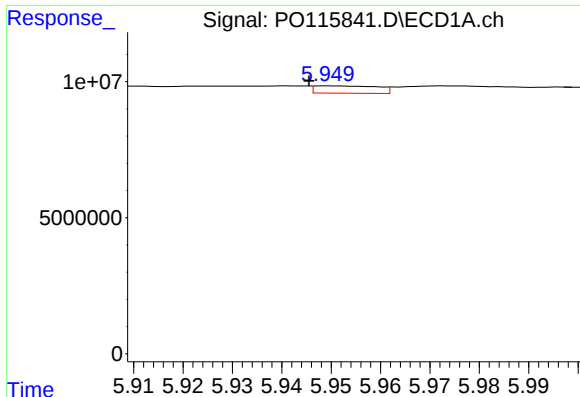

#7 AR-1016-5


R.T.: 5.949 min
Delta R.T.: 0.004 min
Response: 2391599
Conc: 13.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

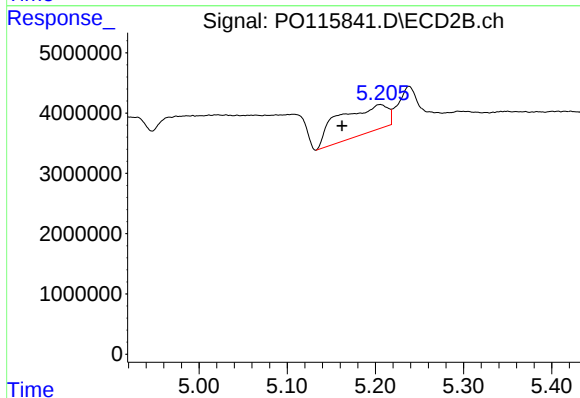


#7 AR-1016-5

R.T.: 5.205 min
Delta R.T.: 0.043 min
Response: 18071361
Conc: 123.49 ng/ml

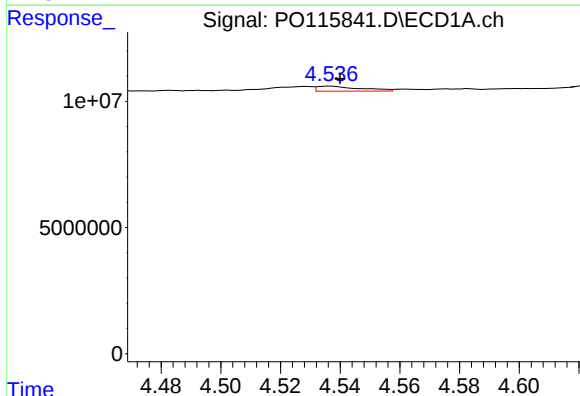


#8 AR-1221-1

R.T.: 4.537 min
Delta R.T.: -0.003 min
Response: 1980788
Conc: 24.39 ng/ml

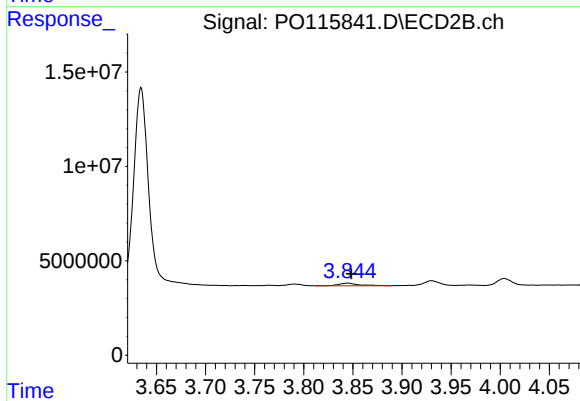

#8 AR-1221-1


R.T.: 3.845 min
Delta R.T.: -0.004 min
Response: 2152389
Conc: 38.16 ng/ml

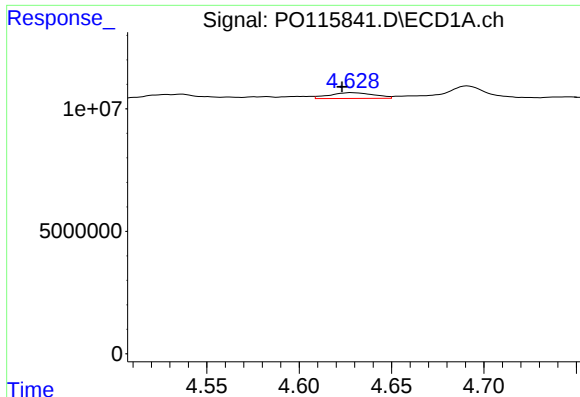

#9 AR-1221-2


R.T.: 4.628 min
Delta R.T.: 0.005 min
Response: 3976810
Conc: 63.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

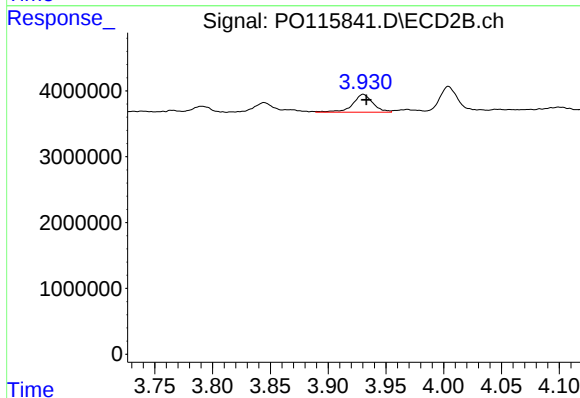


#9 AR-1221-2

R.T.: 3.930 min
Delta R.T.: -0.003 min
Response: 3298300
Conc: 77.71 ng/ml

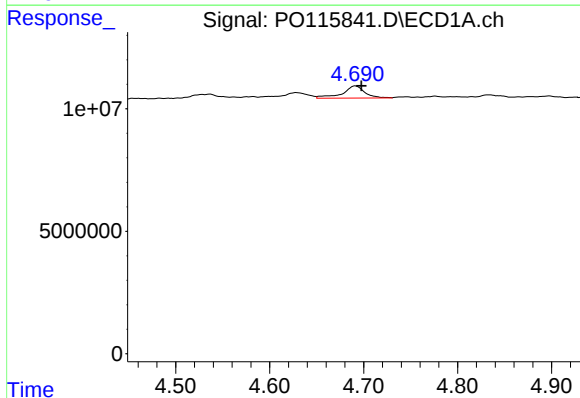


#10 AR-1221-3

R.T.: 4.691 min
Delta R.T.: -0.007 min
Response: 8185088
Conc: 43.84 ng/ml

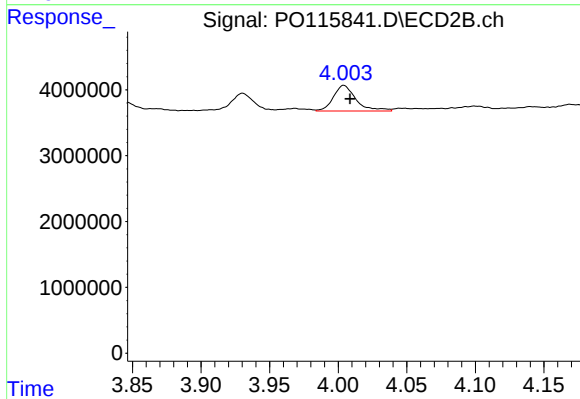

#10 AR-1221-3


R.T.: 4.004 min
Delta R.T.: -0.005 min
Response: 4491002
Conc: 34.92 ng/ml

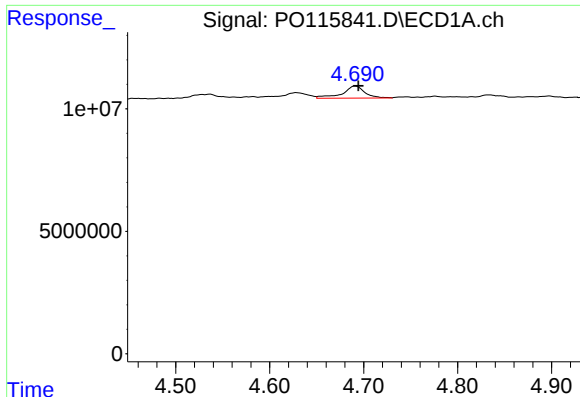

#11 AR-1232-1


R.T.: 4.691 min
Delta R.T.: -0.003 min
Response: 8185088
Conc: 54.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

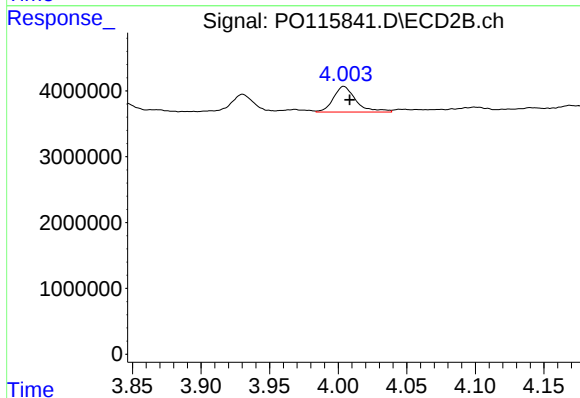


#11 AR-1232-1

R.T.: 4.004 min
Delta R.T.: -0.004 min
Response: 4491002
Conc: 42.04 ng/ml

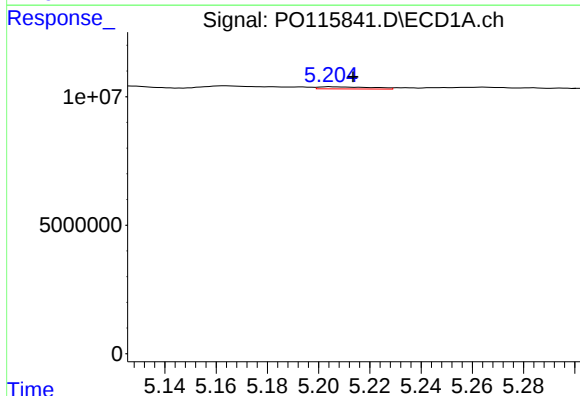


#12 AR-1232-2

R.T.: 5.204 min
Delta R.T.: -0.009 min
Response: 1199284
Conc: 14.83 ng/ml

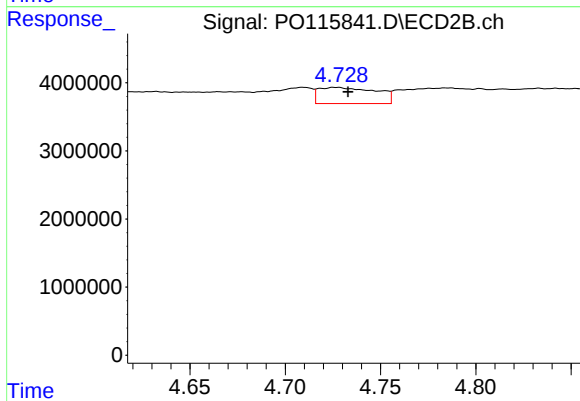

#12 AR-1232-2


R.T.: 4.727 min
Delta R.T.: -0.006 min
Response: 4986392
Conc: 44.93 ng/ml

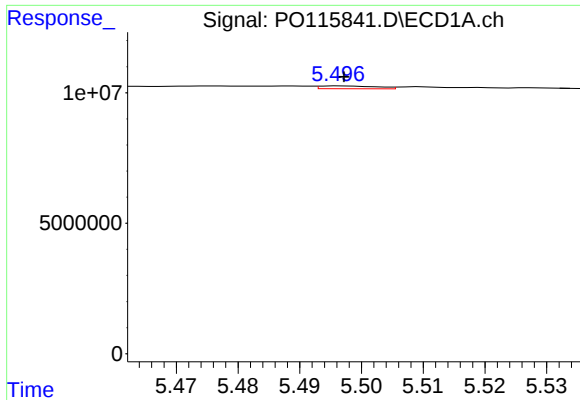

#13 AR-1232-3


R.T.: 5.497 min
Delta R.T.: 0.000 min
Response: 669908
Conc: 4.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

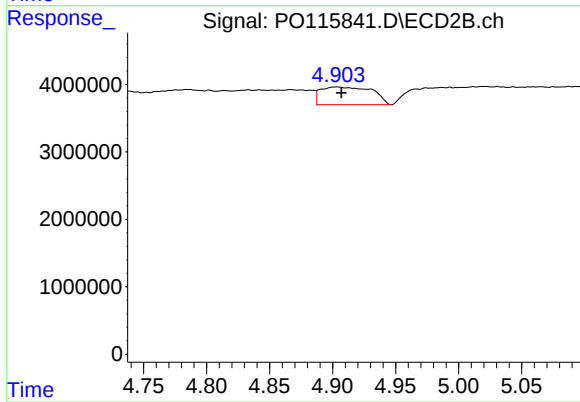


#13 AR-1232-3

R.T.: 4.904 min
Delta R.T.: -0.003 min
Response: 7468498
Conc: 114.26 ng/ml

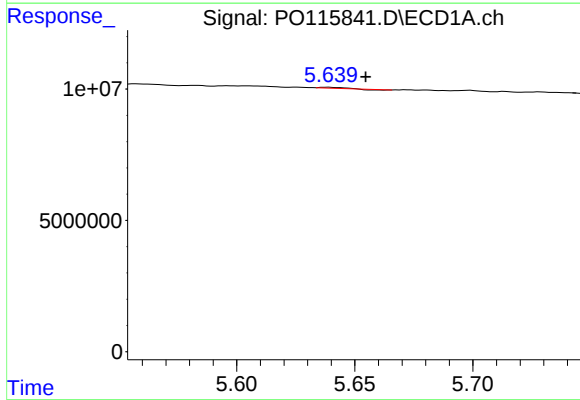


#14 AR-1232-4

R.T.: 5.639 min
Delta R.T.: -0.016 min
Response: 189540
Conc: 2.71 ng/ml

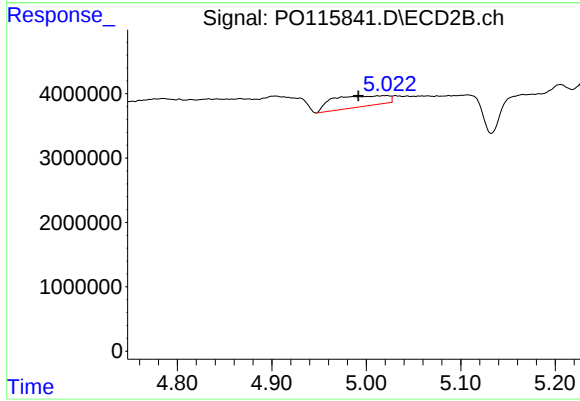

#14 AR-1232-4


R.T.: 5.021 min
Delta R.T.: 0.030 min
Response: 6906808
Conc: 134.56 ng/ml

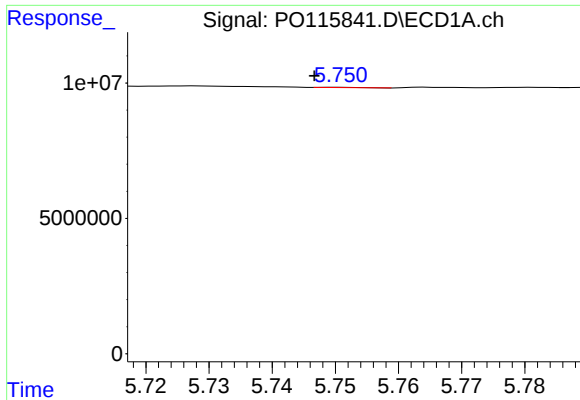

#15 AR-1232-5


R.T.: 5.750 min
Delta R.T.: 0.004 min
Response: 53848
Conc: 1.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

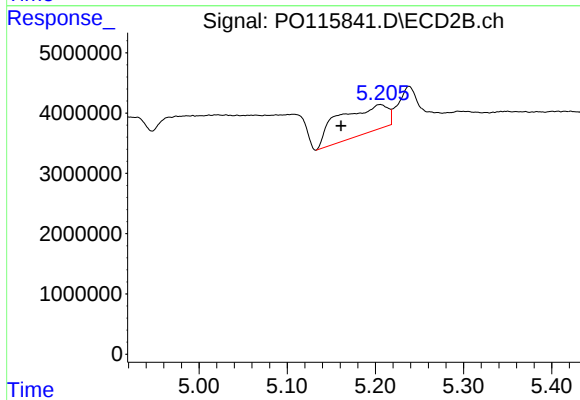


#15 AR-1232-5

R.T.: 5.205 min
Delta R.T.: 0.044 min
Response: 18071361
Conc: 330.08 ng/ml

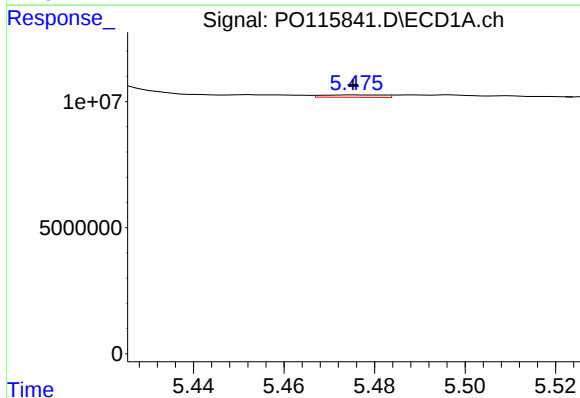


#16 AR-1242-1

R.T.: 5.476 min
Delta R.T.: 0.000 min
Response: 877597
Conc: 4.42 ng/ml

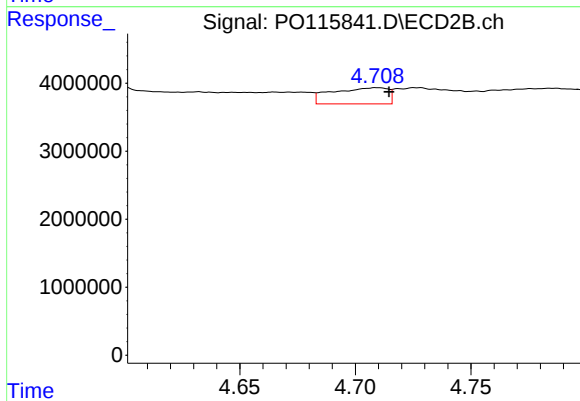

#16 AR-1242-1


R.T.: 4.709 min
Delta R.T.: -0.005 min
Response: 4014929
Conc: 28.20 ng/ml

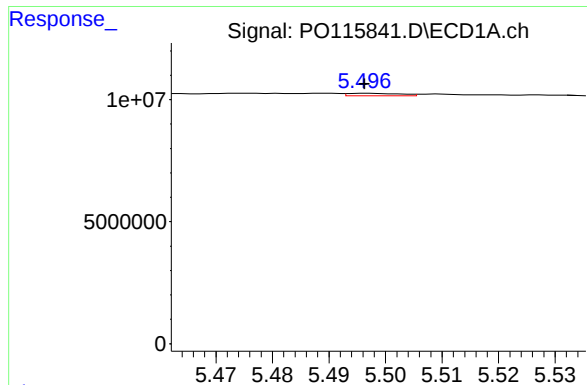

#17 AR-1242-2


R.T.: 5.497 min
Delta R.T.: 0.000 min
Response: 669908
Conc: 2.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

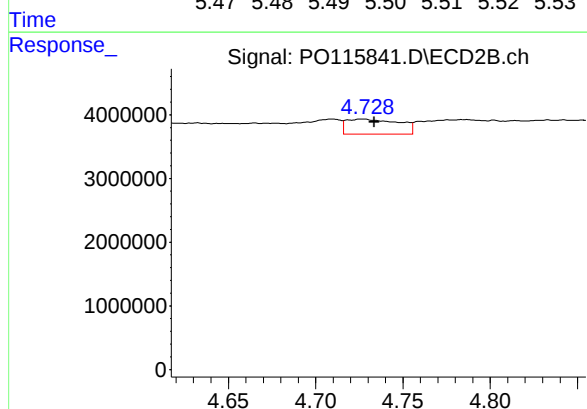


#17 AR-1242-2

R.T.: 4.727 min
Delta R.T.: -0.007 min
Response: 4986392
Conc: 23.82 ng/ml

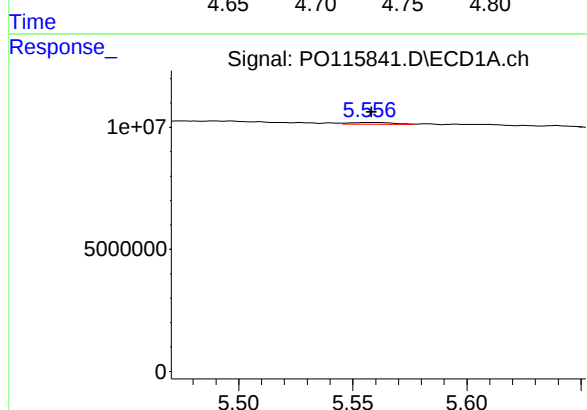


#18 AR-1242-3

R.T.: 5.557 min
Delta R.T.: -0.001 min
Response: 926751
Conc: 5.49 ng/ml

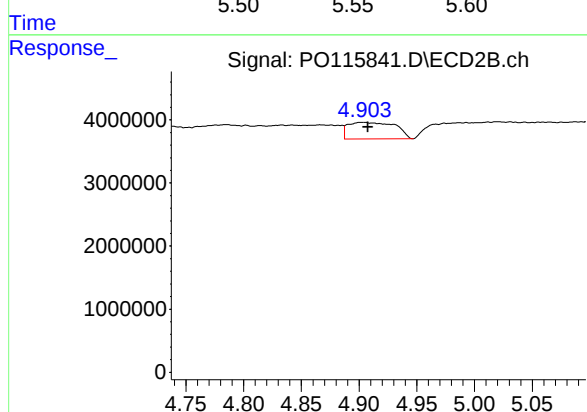

#18 AR-1242-3


R.T.: 4.904 min
Delta R.T.: -0.004 min
Response: 7468498
Conc: 62.53 ng/ml

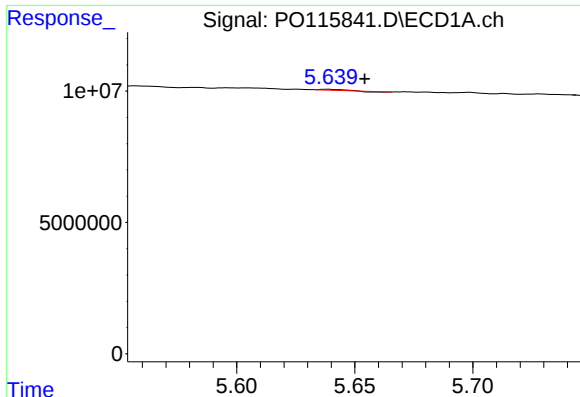

#19 AR-1242-4


R.T.: 5.639 min
Delta R.T.: -0.015 min
Response: 189540
Conc: 1.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

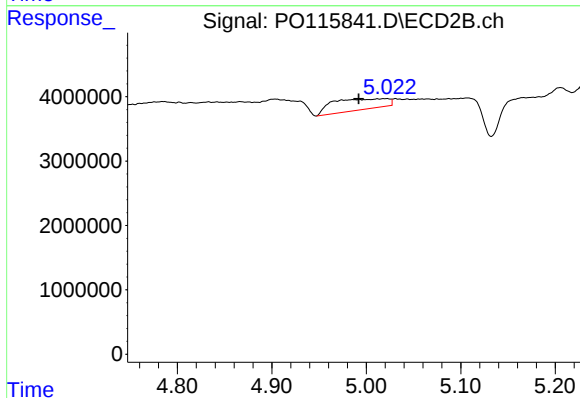


#19 AR-1242-4

R.T.: 5.021 min
Delta R.T.: 0.029 min
Response: 6906808
Conc: 63.31 ng/ml

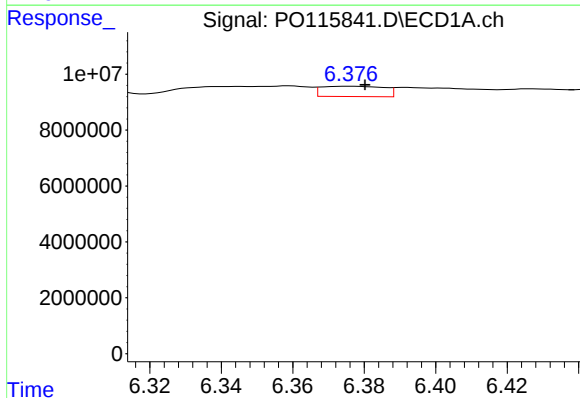


#20 AR-1242-5

R.T.: 6.376 min
Delta R.T.: -0.004 min
Response: 4491919
Conc: 29.66 ng/ml

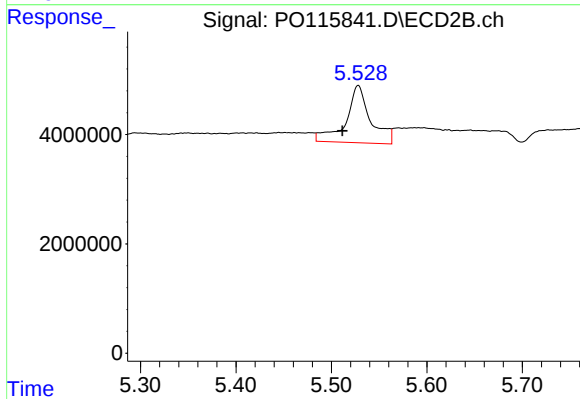

#20 AR-1242-5


R.T.: 5.528 min
Delta R.T.: 0.016 min
Response: 18832070
Conc: 136.34 ng/ml

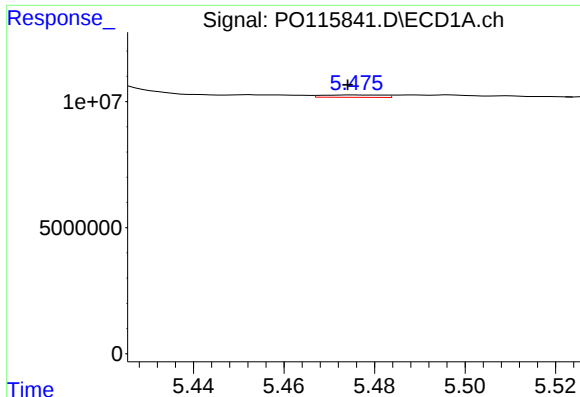

#21 AR-1248-1


R.T.: 5.476 min
Delta R.T.: 0.002 min
Response: 877597
Conc: 5.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

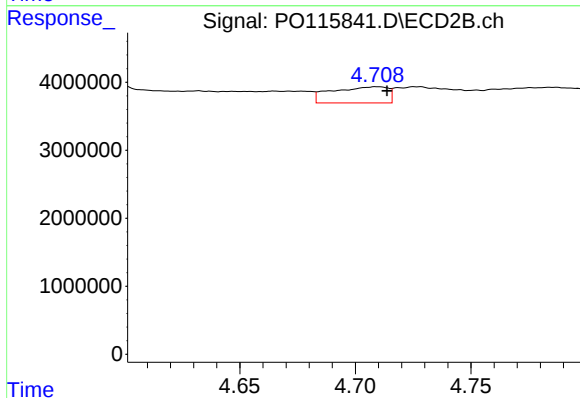


#21 AR-1248-1

R.T.: 4.709 min
Delta R.T.: -0.004 min
Response: 4014929
Conc: 35.90 ng/ml

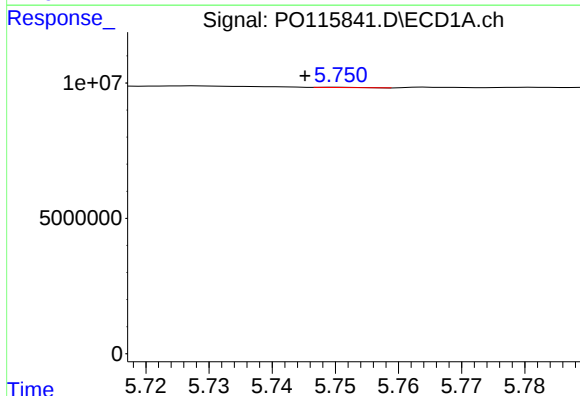


#22 AR-1248-2

R.T.: 5.750 min
Delta R.T.: 0.005 min
Response: 53848
Conc: 0.27 ng/ml

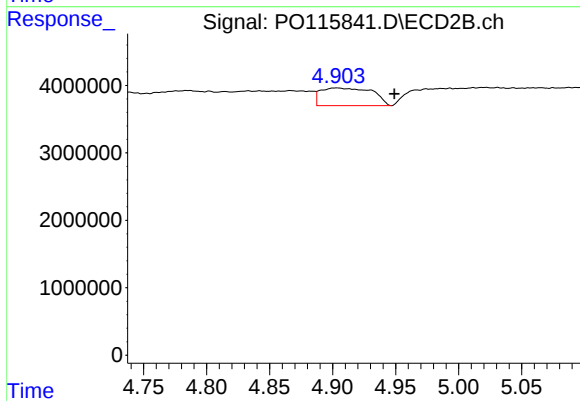

#22 AR-1248-2


R.T.: 4.904 min
Delta R.T.: -0.045 min
Response: 7468498
Conc: 49.04 ng/ml

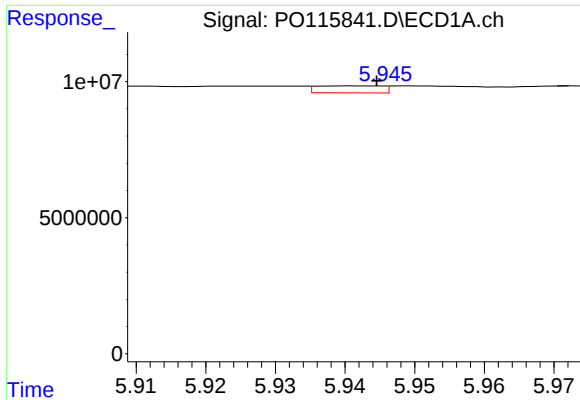

#23 AR-1248-3


R.T.: 5.942 min
Delta R.T.: -0.003 min
Response: 1669310
Conc: 6.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

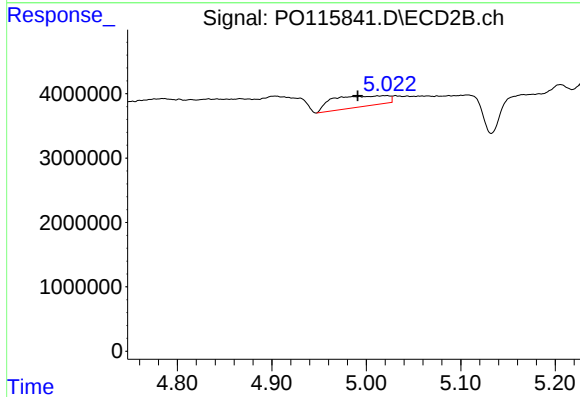


#23 AR-1248-3

R.T.: 5.021 min
Delta R.T.: 0.030 min
Response: 6906808
Conc: 43.03 ng/ml

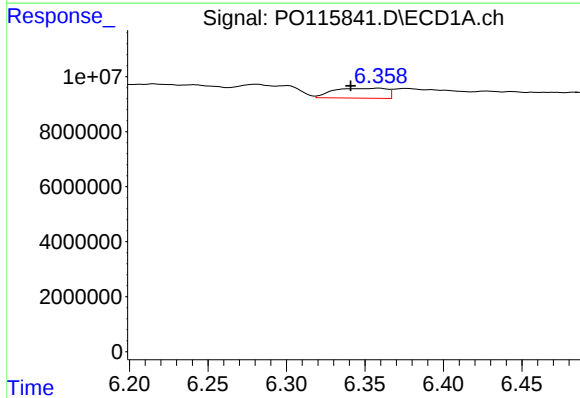


#24 AR-1248-4

R.T.: 6.359 min
Delta R.T.: 0.018 min
Response: 8495403
Conc: 28.81 ng/ml

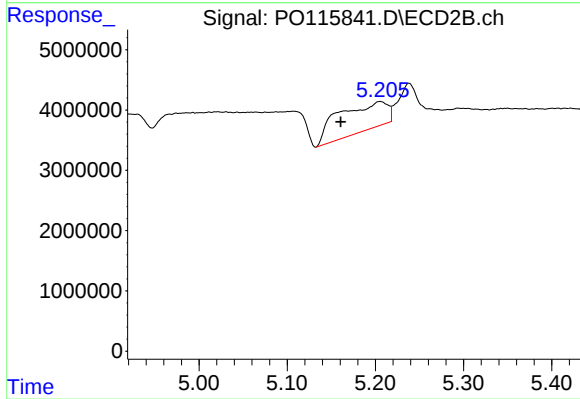

#24 AR-1248-4


R.T.: 5.205 min
Delta R.T.: 0.045 min
Response: 18071361
Conc: 96.56 ng/ml

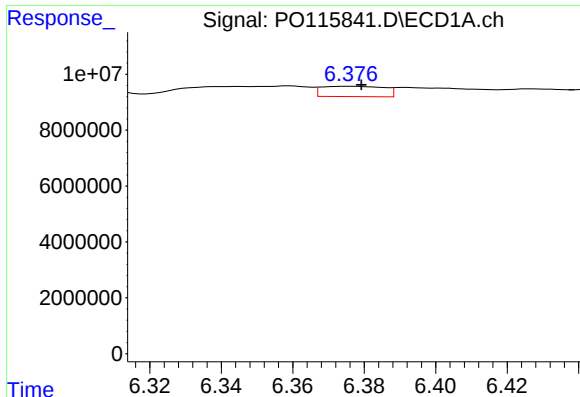

#25 AR-1248-5


R.T.: 6.376 min
Delta R.T.: -0.003 min
Response: 4491919
Conc: 17.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

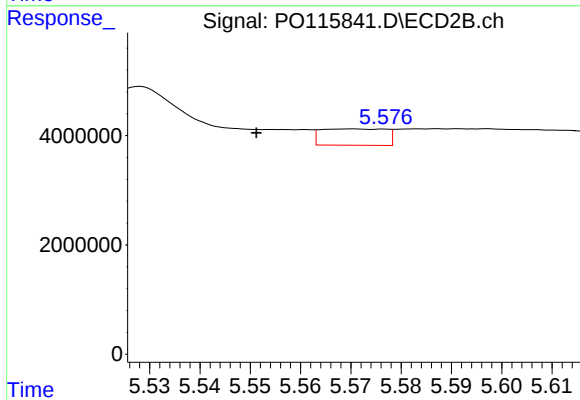


#25 AR-1248-5

R.T.: 5.570 min
Delta R.T.: 0.019 min
Response: 2674374
Conc: 13.51 ng/ml

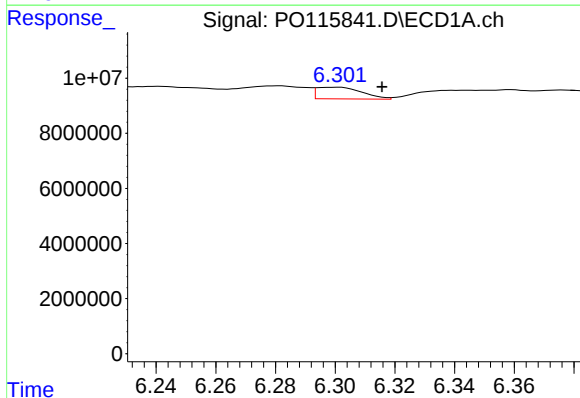


#26 AR-1254-1

R.T.: 6.301 min
Delta R.T.: -0.015 min
Response: 4488718
Conc: 17.35 ng/ml

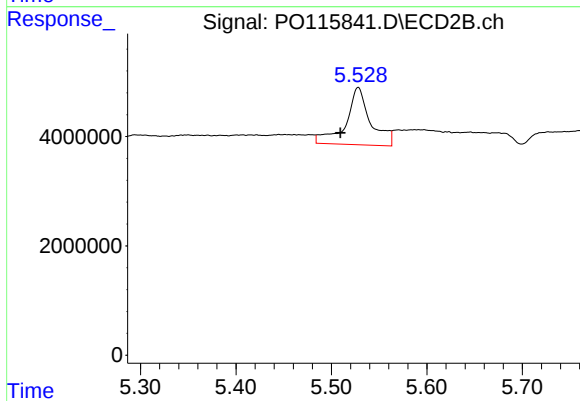

#26 AR-1254-1


R.T.: 5.528 min
Delta R.T.: 0.019 min
Response: 18832070
Conc: 64.43 ng/ml

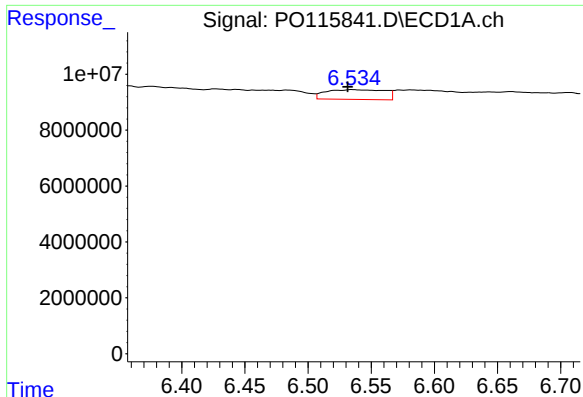

#27 AR-1254-2


R.T.: 6.535 min
Delta R.T.: 0.004 min
Response: 11302690
Conc: 28.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

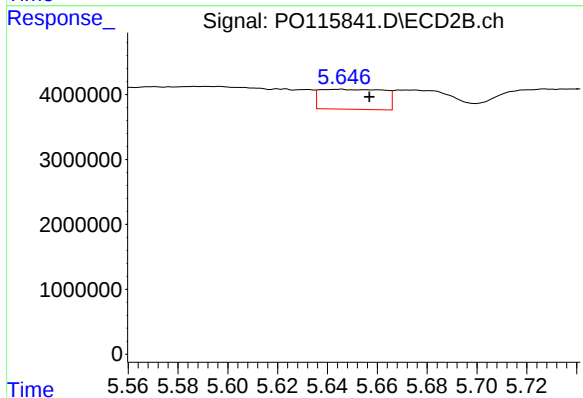


#27 AR-1254-2

R.T.: 5.645 min
Delta R.T.: -0.012 min
Response: 5478680
Conc: 21.76 ng/ml

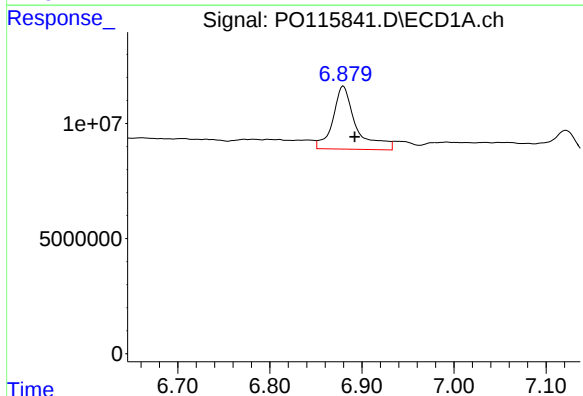


#28 AR-1254-3

R.T.: 6.880 min
Delta R.T.: -0.012 min
Response: 47897157
Conc: 116.66 ng/ml

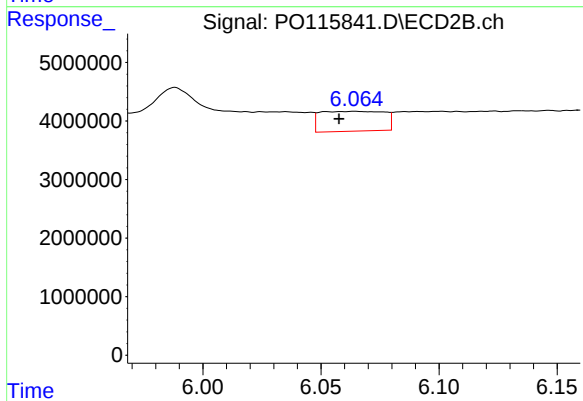

#28 AR-1254-3


R.T.: 6.064 min
Delta R.T.: 0.007 min
Response: 6374213
Conc: 16.20 ng/ml

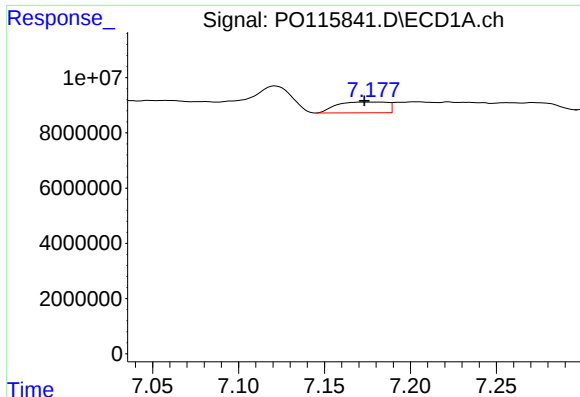

#29 AR-1254-4


R.T.: 7.178 min
Delta R.T.: 0.005 min
Response: 7999499
Conc: 23.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

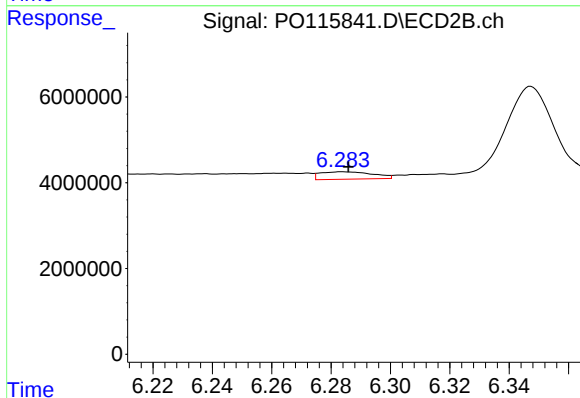


#29 AR-1254-4

R.T.: 6.284 min
Delta R.T.: -0.002 min
Response: 2140835
Conc: 8.00 ng/ml

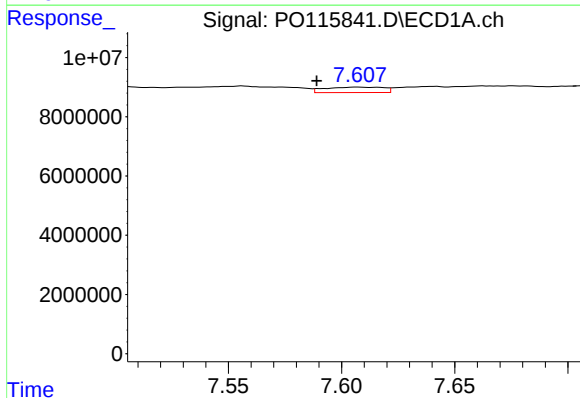


#30 AR-1254-5

R.T.: 7.607 min
Delta R.T.: 0.019 min
Response: 3324882
Conc: 10.26 ng/ml

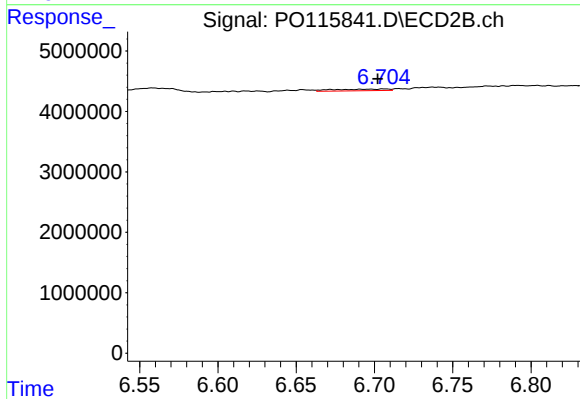

#30 AR-1254-5


R.T.: 6.706 min
Delta R.T.: 0.004 min
Response: 625899
Conc: 1.75 ng/ml

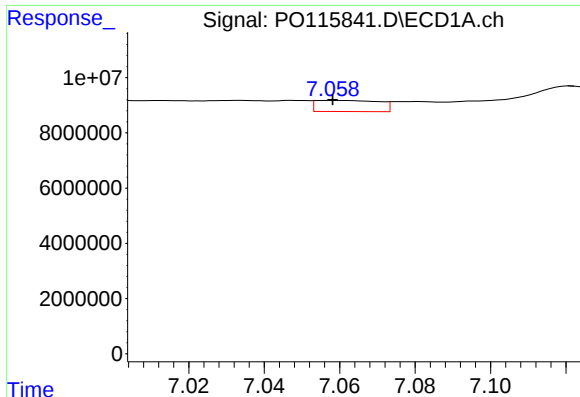

#31 AR-1260-1


R.T.: 7.058 min
Delta R.T.: 0.000 min
Response: 4703184
Conc: 16.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

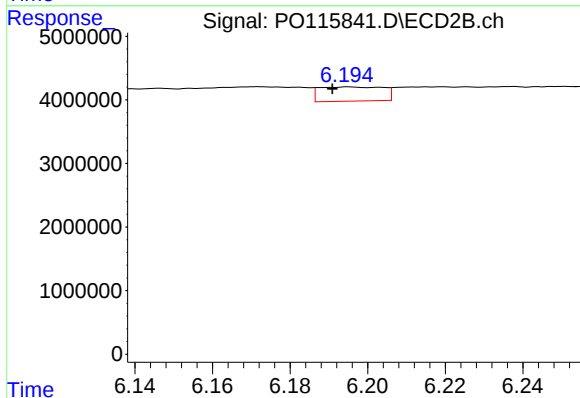


#31 AR-1260-1

R.T.: 6.195 min
Delta R.T.: 0.004 min
Response: 2557475
Conc: 9.76 ng/ml

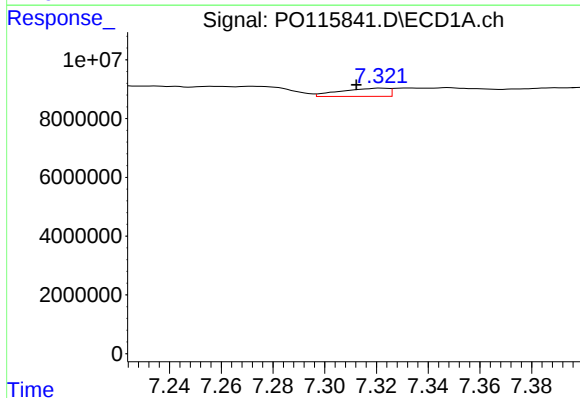


#32 AR-1260-2

R.T.: 7.322 min
Delta R.T.: 0.010 min
Response: 3554708
Conc: 8.12 ng/ml

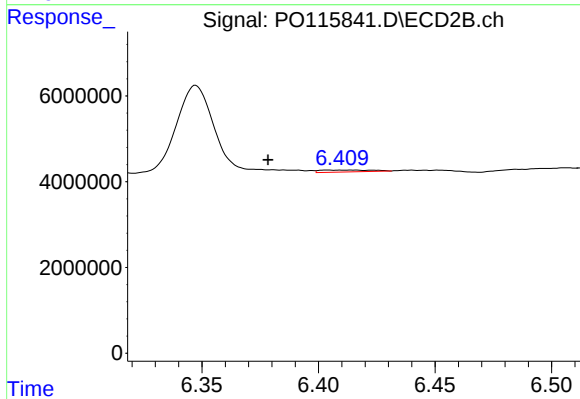

#32 AR-1260-2


R.T.: 6.404 min
Delta R.T.: 0.026 min
Response: 667907
Conc: 1.91 ng/ml

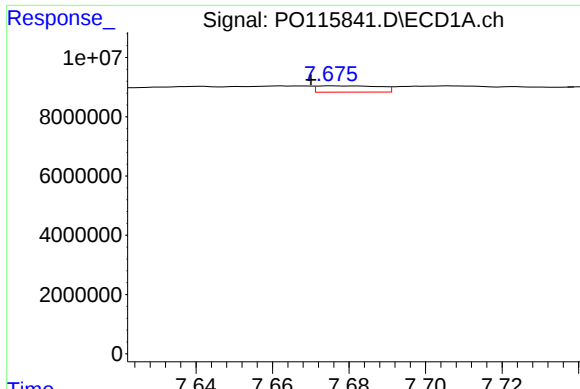

#33 AR-1260-3


R.T.: 7.676 min
Delta R.T.: 0.006 min
Response: 2416076
Conc: 7.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

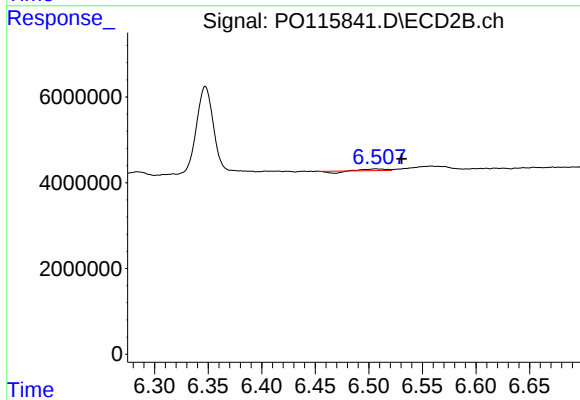


#33 AR-1260-3

R.T.: 6.507 min
Delta R.T.: -0.024 min
Response: 205050
Conc: 0.64 ng/ml

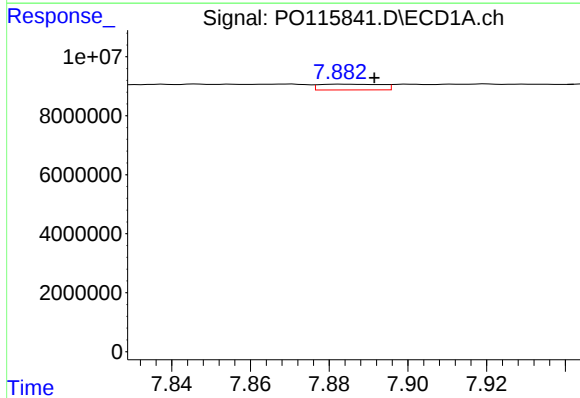


#34 AR-1260-4

R.T.: 7.883 min
Delta R.T.: -0.008 min
Response: 2165716
Conc: 7.04 ng/ml

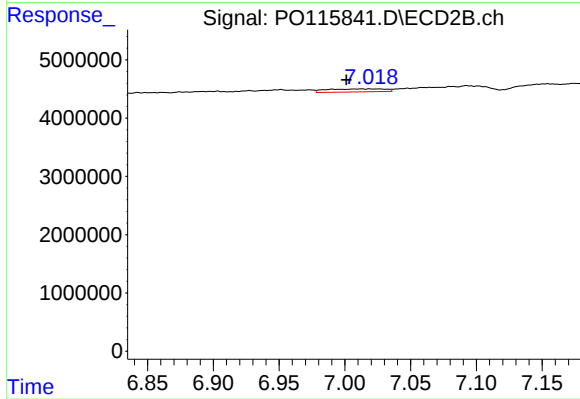

#34 AR-1260-4


R.T.: 7.019 min
Delta R.T.: 0.018 min
Response: 1615139
Conc: 6.29 ng/ml

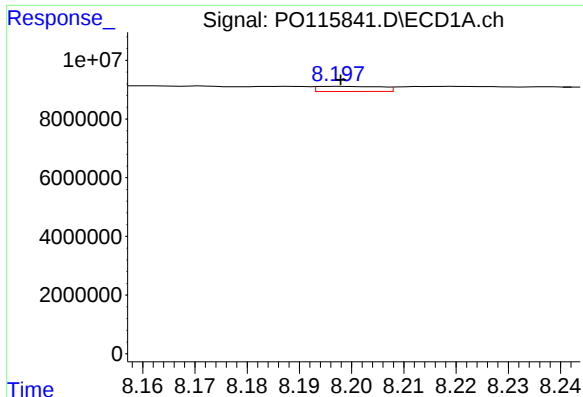

#35 AR-1260-5


R.T.: 8.197 min
Delta R.T.: 0.000 min
Response: 1468274
Conc: 2.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

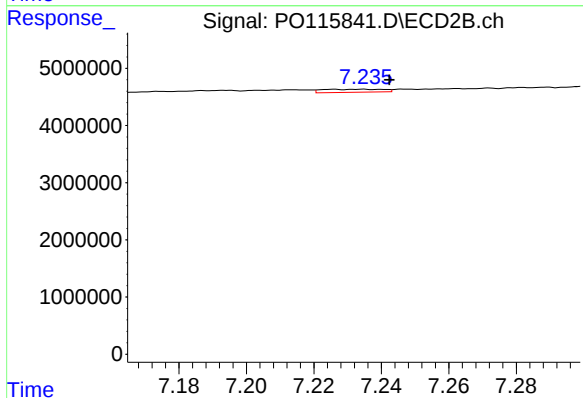


#35 AR-1260-5

R.T.: 7.234 min
Delta R.T.: -0.008 min
Response: 676711
Conc: 0.96 ng/ml

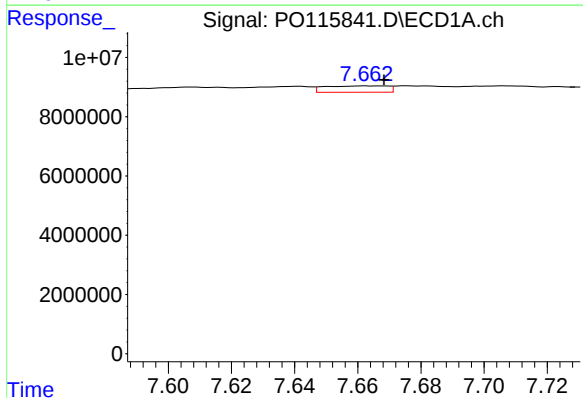


#36 AR-1262-1

R.T.: 7.662 min
Delta R.T.: -0.006 min
Response: 2949124
Conc: 11.95 ng/ml

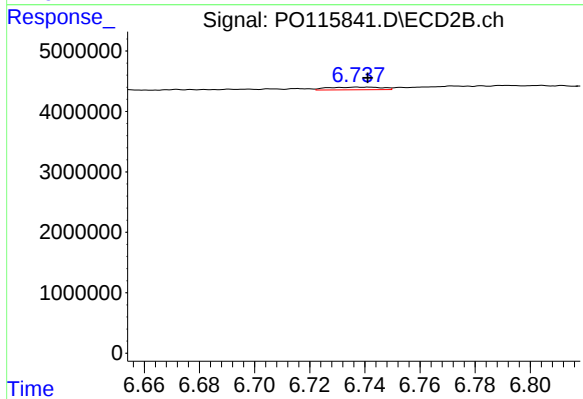

#36 AR-1262-1


R.T.: 6.738 min
Delta R.T.: -0.003 min
Response: 599086
Conc: 2.81 ng/ml

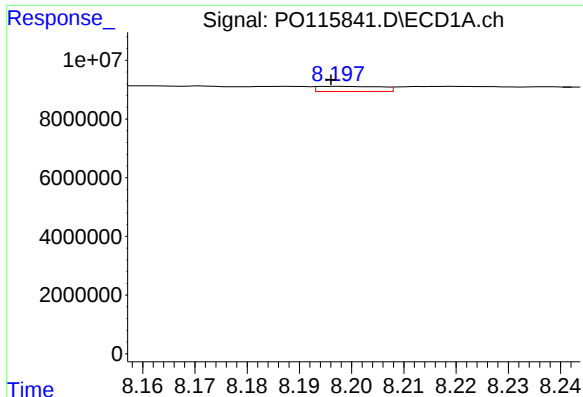

#37 AR-1262-2


R.T.: 8.197 min
Delta R.T.: 0.001 min
Response: 1468274
Conc: 3.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

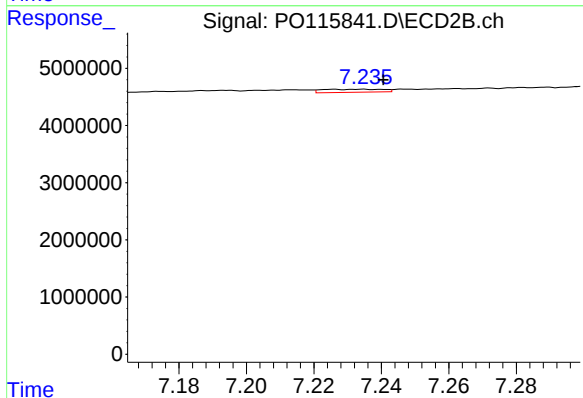


#37 AR-1262-2

R.T.: 7.234 min
Delta R.T.: -0.006 min
Response: 676711
Conc: 1.94 ng/ml

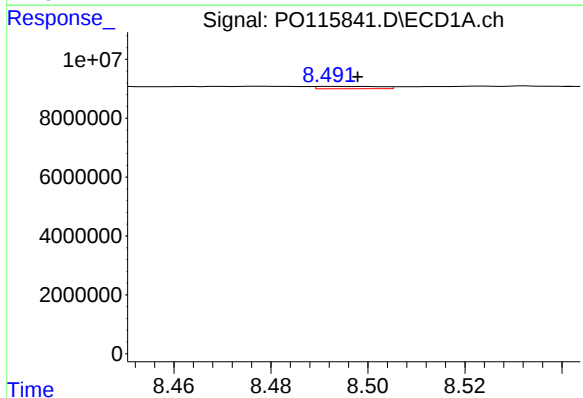


#38 AR-1262-3

R.T.: 8.493 min
Delta R.T.: -0.005 min
Response: 691286
Conc: 2.71 ng/ml

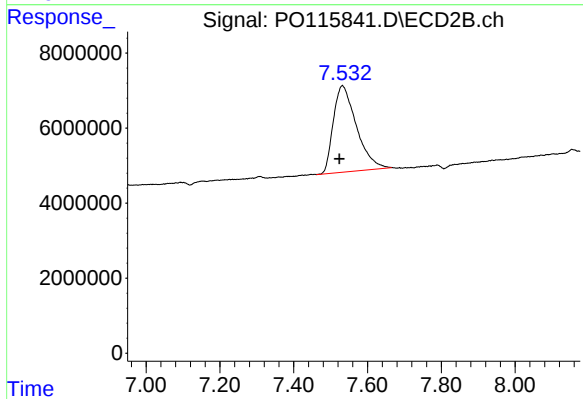

#38 AR-1262-3


R.T.: 7.532 min
Delta R.T.: 0.008 min
Response: 100084092
Conc: 639.96 ng/ml

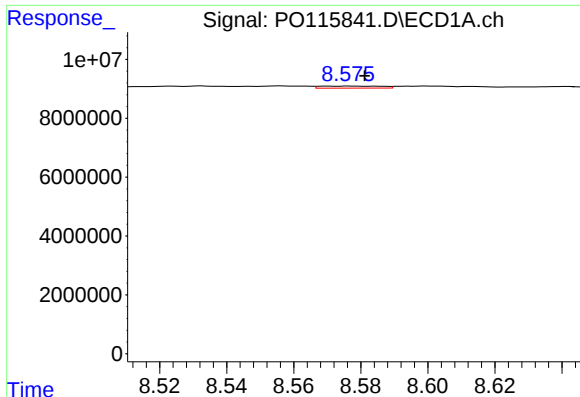

#39 AR-1262-4


R.T.: 8.577 min
Delta R.T.: -0.004 min
Response: 881327
Conc: 4.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

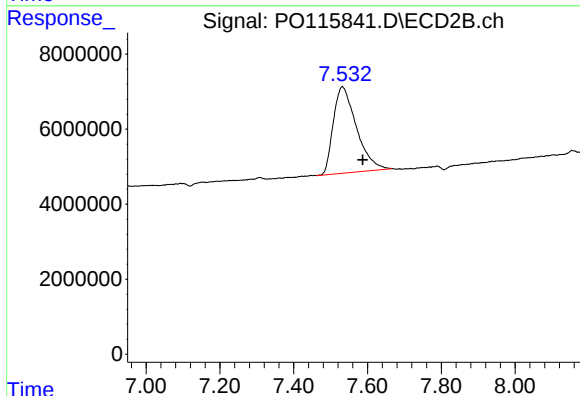


#39 AR-1262-4

R.T.: 7.532 min
Delta R.T.: -0.055 min
Response: 100084092
Conc: 404.59 ng/ml

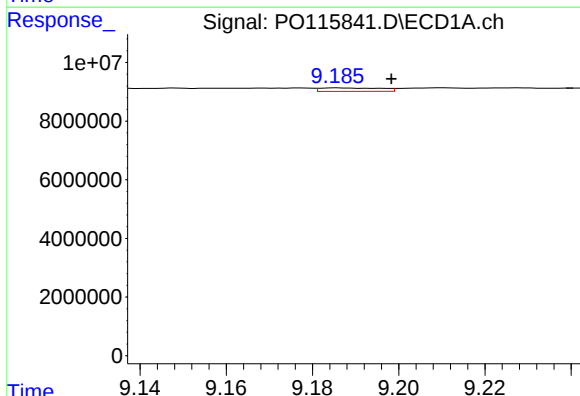


#40 AR-1262-5

R.T.: 9.186 min
Delta R.T.: -0.012 min
Response: 1135933
Conc: 8.43 ng/ml

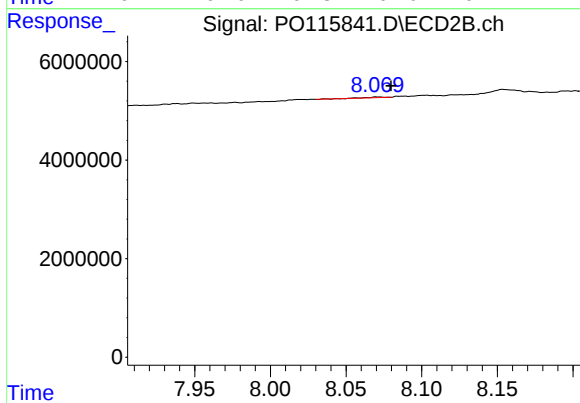

#40 AR-1262-5


R.T.: 8.071 min
Delta R.T.: -0.009 min
Response: 123656
Conc: 1.11 ng/ml

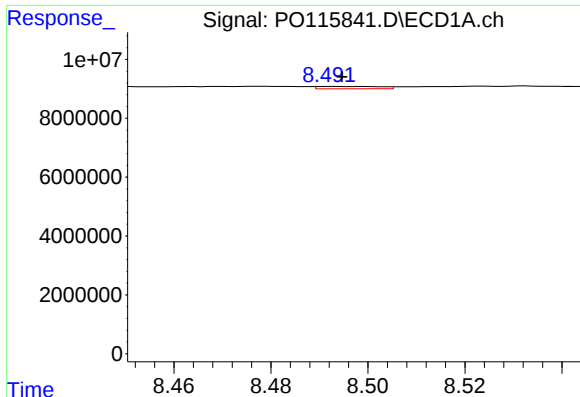

#41 AR-1268-1


R.T.: 8.493 min
Delta R.T.: -0.002 min
Response: 691286
Conc: 0.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

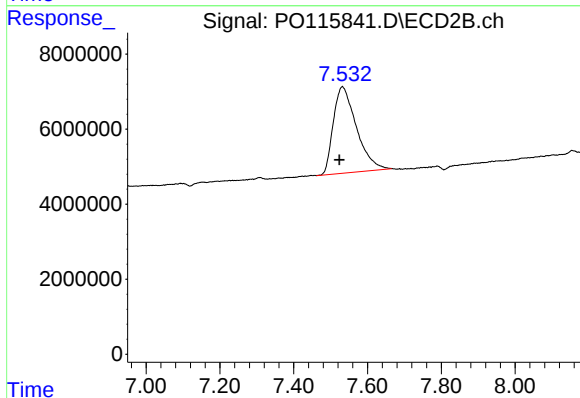


#41 AR-1268-1

R.T.: 7.532 min
Delta R.T.: 0.008 min
Response: 100084092
Conc: 112.97 ng/ml

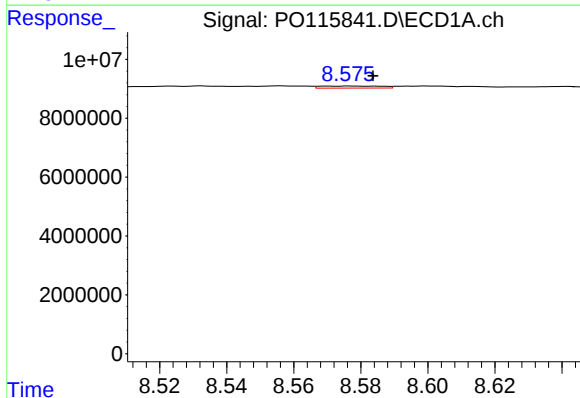


#42 AR-1268-2

R.T.: 8.577 min
Delta R.T.: -0.007 min
Response: 881327
Conc: 1.03 ng/ml

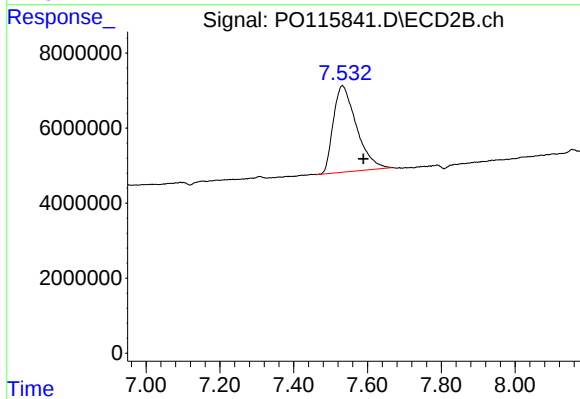

#42 AR-1268-2


R.T.: 7.532 min
Delta R.T.: -0.057 min
Response: 100084092
Conc: 133.61 ng/ml

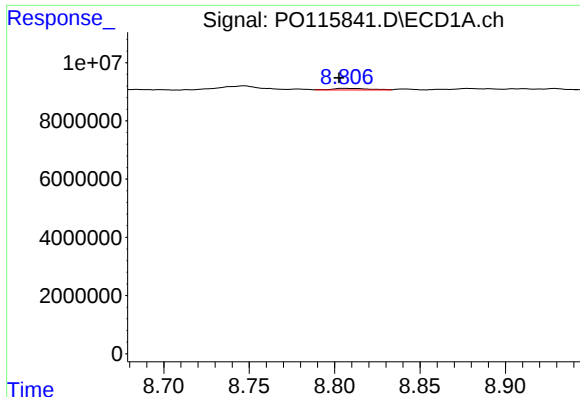

#43 AR-1268-3


R.T.: 8.806 min
Delta R.T.: 0.003 min
Response: 834768
Conc: 1.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

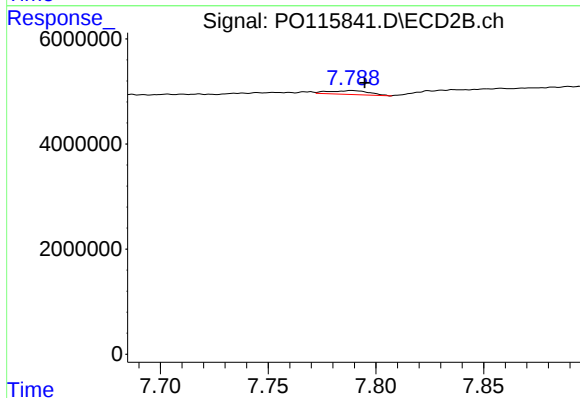


#43 AR-1268-3

R.T.: 7.789 min
Delta R.T.: -0.006 min
Response: 943006
Conc: 1.48 ng/ml

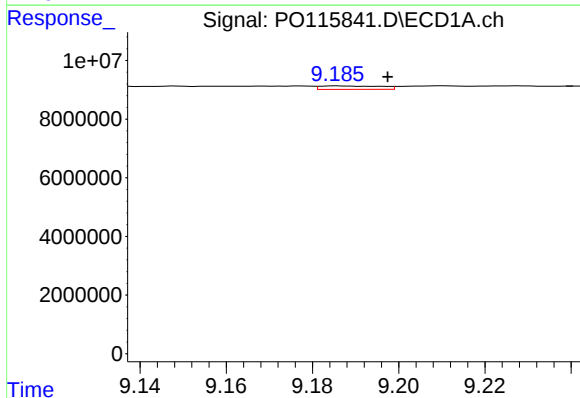


#44 AR-1268-4

R.T.: 9.186 min
Delta R.T.: -0.011 min
Response: 1135933
Conc: 3.64 ng/ml

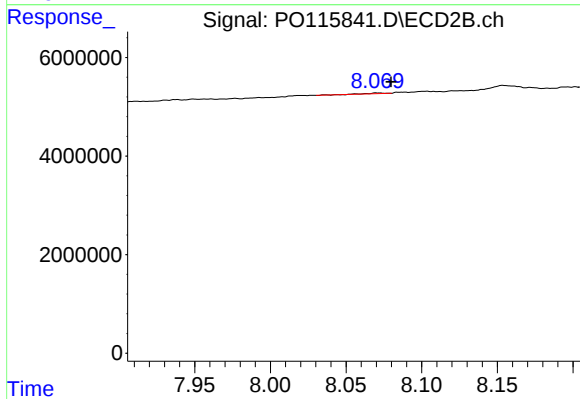

#44 AR-1268-4


R.T.: 8.071 min
Delta R.T.: -0.009 min
Response: 123656
Conc: 0.48 ng/ml

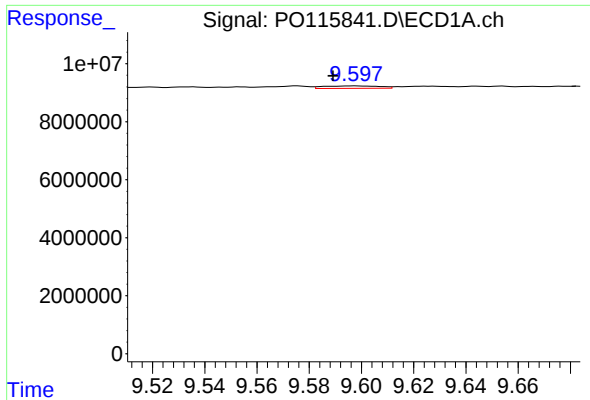

#45 AR-1268-5

R.T.: 9.597 min
Delta R.T.: 0.008 min
Response: 1261442
Conc: 0.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

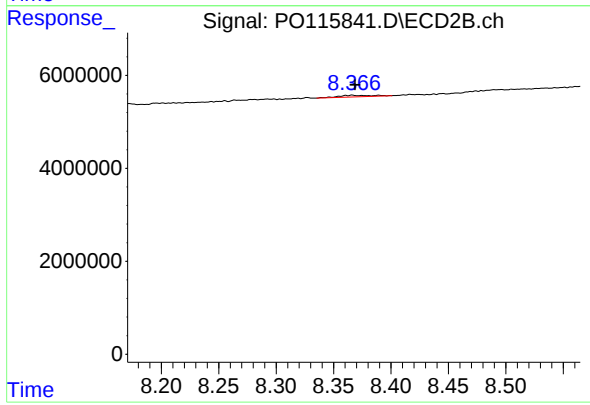

#45 AR-1268-5

R.T.: 8.366 min
Delta R.T.: -0.002 min
Response: 705769
Conc: 0.42 ng/ml