

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO121225\
 Data File : PO115842.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Dec 2025 09:42
 Operator : YP/AJ
 Sample : Q3530-09
 Misc : AR1232 25PPB WATER MDL
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 MDL-WATER-03-QT4-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 02:43:07 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO120425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 05 02:11:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.333	3.635	181.9E6	110.5E6	23.419	22.675
2)	SA Decachlor...	9.908	8.615	124.9E6	94514056	23.734	21.979
Target Compounds							
3)	L1 AR-1016-1	5.471	4.710	7385137	7077078	29.699	38.303 #
4)	L1 AR-1016-2	5.492	4.727	9257038	7124594	24.307	26.956
5)	L1 AR-1016-3	5.554	4.902	4205807	8755257	19.673	57.852 #
6)	L1 AR-1016-4	5.646	4.928	1290536	3195236	7.227	28.351 #
7)	L1 AR-1016-5	5.938	5.158	8408426	12673757	47.931	86.604 #
8)	L2 AR-1221-1	4.551	3.844	426194	1214913	5.249	21.539 #
9)	L2 AR-1221-2	4.629	3.931	3946080	3491989	62.617	82.273 #
10)	L2 AR-1221-3	4.691	4.005	8618005	3235023	46.156	25.157 #
11)	L3 AR-1232-1	4.691	4.005	8618005	3235023	57.582	30.280 #
12)	L3 AR-1232-2	5.209	4.727	17039140	7124594	210.748	64.191 #
13)	L3 AR-1232-3	5.492	4.902	9257038	8755257	60.148	133.941 #
14)	L3 AR-1232-4	5.646	4.986	1290536	7957067	18.428	155.017 #
15)	L3 AR-1232-5	5.743	5.158	1172052	12673757	22.567	231.492 #
16)	L4 AR-1242-1	5.471	4.710	7385137	7077078	37.182	49.703 #
17)	L4 AR-1242-2	5.492	4.727	9257038	7124594	31.606	34.030
18)	L4 AR-1242-3	5.554	4.902	4205807	8755257	24.914	73.301 #
19)	L4 AR-1242-4	5.646	4.986	1290536	7957067	9.443	72.939 #
20)	L4 AR-1242-5	6.375	5.529	16704448	55515400	110.301	401.921 #
21)	L5 AR-1248-1	5.471	4.710	7385137	7077078	48.661	63.285 #
22)	L5 AR-1248-2	5.743	4.928	1172052	3195236	5.836	20.981 #
23)	L5 AR-1248-3	5.938	4.986	8408426	7957067	34.098	49.568 #
24)	L5 AR-1248-4	6.335	5.158	11800806	12673757	40.022	67.721 #
25)	L5 AR-1248-5	6.375	5.529	16704448	55515400	64.514	280.444 #
26)	L6 AR-1254-1	6.309	5.529	31500407	55515400	121.758	189.945 #
27)	L6 AR-1254-2	6.532	5.646	14027452	9003547	34.859	35.755
28)	L6 AR-1254-3	6.881	6.056	96065173	12013345	233.982	30.523 #
29)	L6 AR-1254-4	7.177	6.287	13246629	7706813	38.168	28.802
30)	L6 AR-1254-5	7.566	6.697	5118921	2431037	15.797	6.800 #
31)	L7 AR-1260-1	7.057	6.196	9875189	1906407	34.088	7.272 #
32)	L7 AR-1260-2	7.322	6.397	8074032	490282	18.445	1.399 #
33)	L7 AR-1260-3	7.660	6.506	5893624	3455587	17.510	10.756 #
34)	L7 AR-1260-4	7.886	7.006	2524309	477797	8.210	1.860 #
35)	L7 AR-1260-5	8.221	7.207f	1999997	1888399	2.745	2.693
36)	L8 AR-1262-1	7.660	6.737	5893624	2333462	23.875	10.953 #
37)	L8 AR-1262-2	8.221	7.207	1999997	1888399	5.052	5.421
38)	L8 AR-1262-3	8.511	7.533	829598	282.2E6	3.256	1804.734 #
39)	L8 AR-1262-4	8.575	7.533f	977705	282.2E6	5.047	1140.969 #
40)	L8 AR-1262-5	9.198	8.055	1479382	97932	10.984	0.879 #
41)	L9 AR-1268-1	8.511	7.533	829598	282.2E6	0.833	318.576 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121225\
Data File : PO115842.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Dec 2025 09:42
Operator : YP/AJ
Sample : Q3530-09
Misc : AR1232 25PPB WATER MDL
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 02:43:07 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120425.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 05 02:11:05 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.575	7.533f	977705	282.2E6	1.143	376.791 #
43)	L9 AR-1268-3	8.802	7.790	191480	1037005	0.258	1.629 #
44)	L9 AR-1268-4	9.198	8.055	1479382	97932	4.738	0.380 #
45)	L9 AR-1268-5	9.593	8.363	2146165	875941	0.986	0.520 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121225\
Data File : PO115842.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Dec 2025 09:42
Operator : YP/AJ
Sample : Q3530-09
Misc : AR1232 25PPB WATER MDL
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 02:43:07 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120425.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 05 02:11:05 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

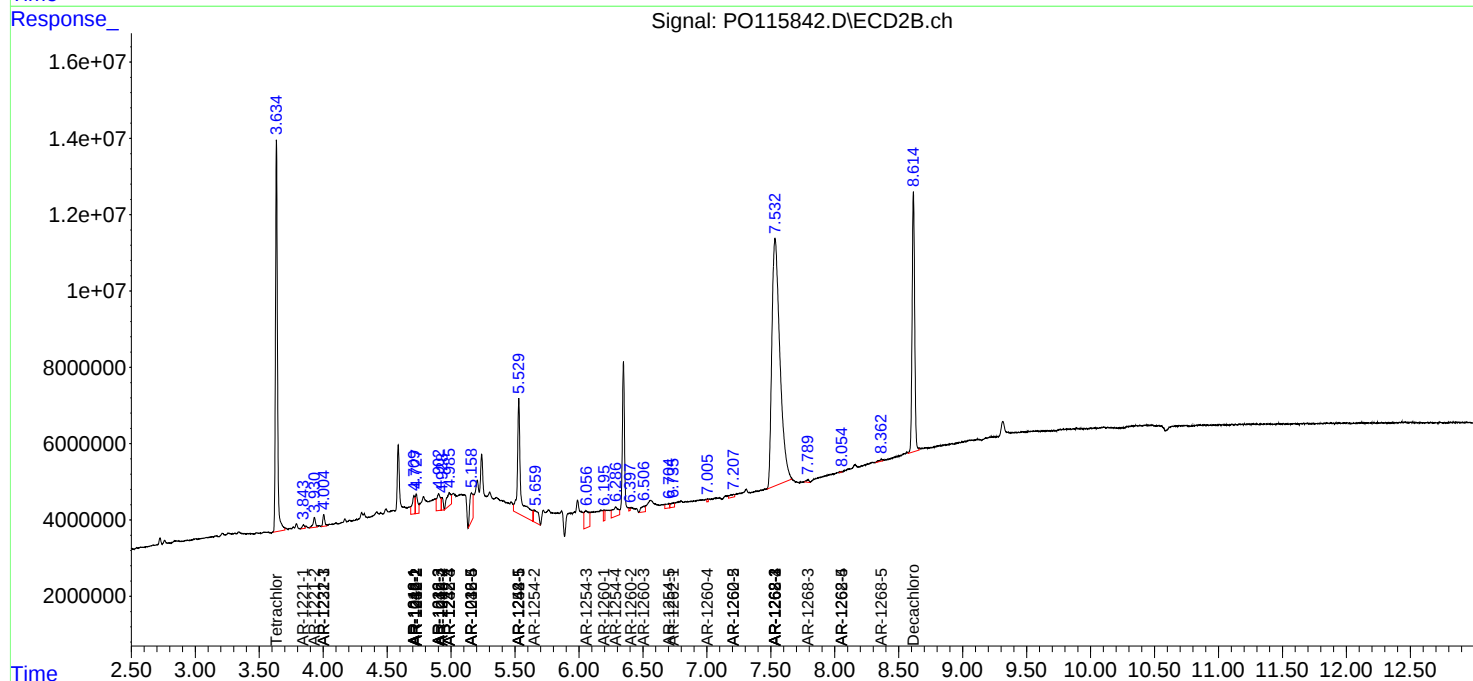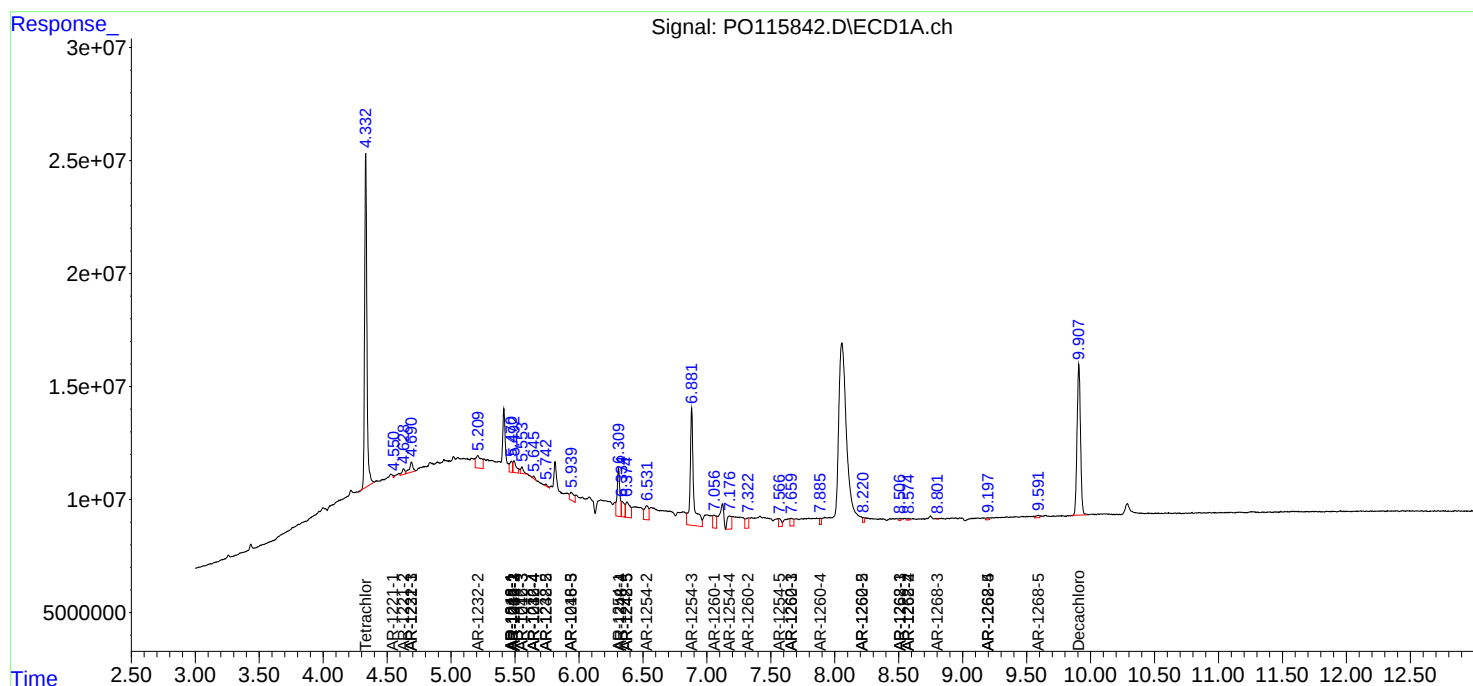


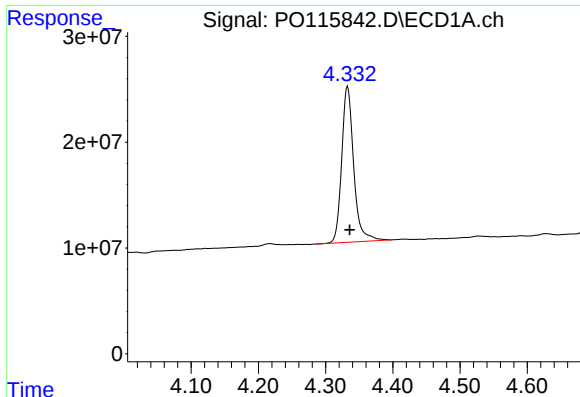

#1 Tetrachloro-m-xylene


R.T.: 4.333 min
Delta R.T.: -0.003 min
Response: 181900568
Conc: 23.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

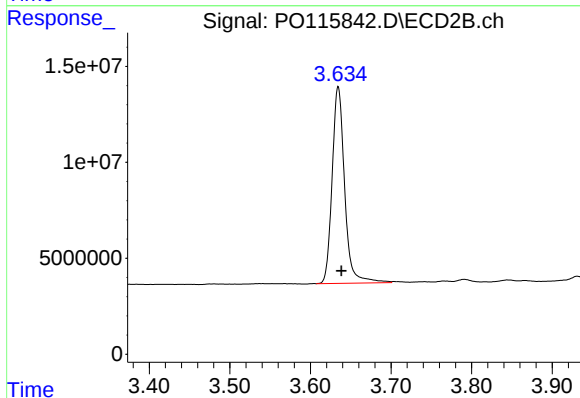


#1 Tetrachloro-m-xylene

R.T.: 3.635 min
Delta R.T.: -0.004 min
Response: 110503900
Conc: 22.68 ng/ml

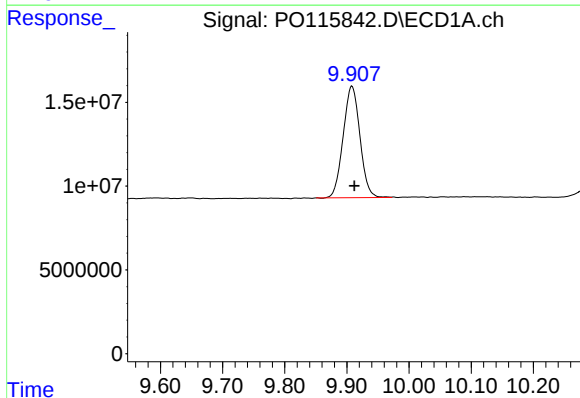


#2 Decachlorobiphenyl

R.T.: 9.908 min
Delta R.T.: -0.004 min
Response: 124867170
Conc: 23.73 ng/ml

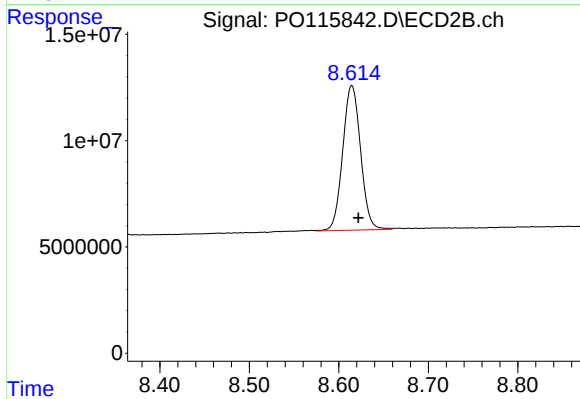

#2 Decachlorobiphenyl


R.T.: 8.615 min
Delta R.T.: -0.008 min
Response: 94514056
Conc: 21.98 ng/ml

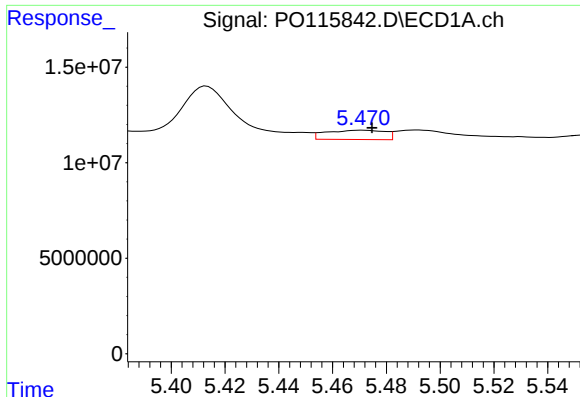

#3 AR-1016-1


R.T.: 5.471 min
Delta R.T.: -0.004 min
Response: 7385137
Conc: 29.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

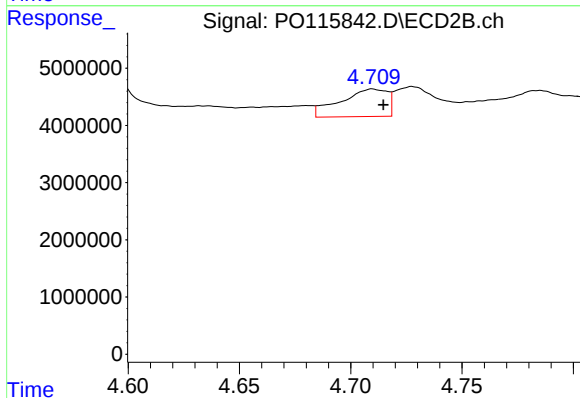


#3 AR-1016-1

R.T.: 4.710 min
Delta R.T.: -0.005 min
Response: 7077078
Conc: 38.30 ng/ml

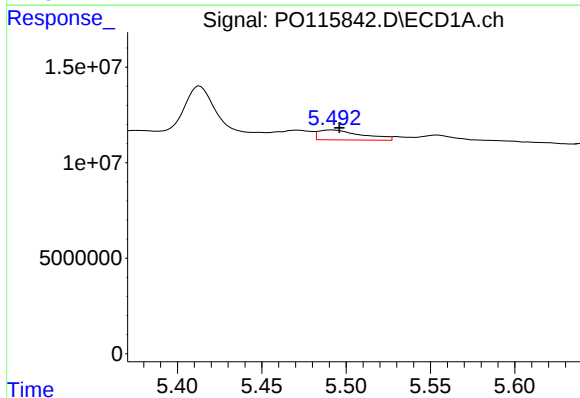


#4 AR-1016-2

R.T.: 5.492 min
Delta R.T.: -0.004 min
Response: 9257038
Conc: 24.31 ng/ml

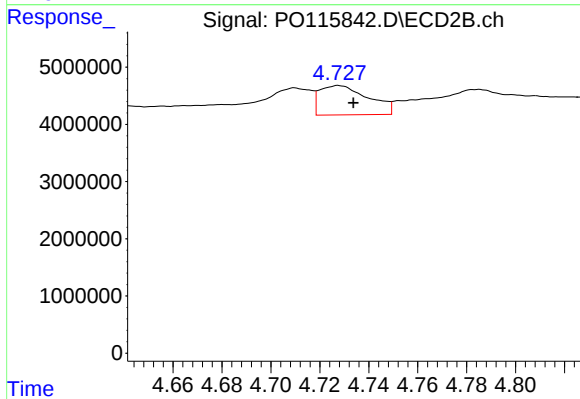

#4 AR-1016-2


R.T.: 4.727 min
Delta R.T.: -0.006 min
Response: 7124594
Conc: 26.96 ng/ml

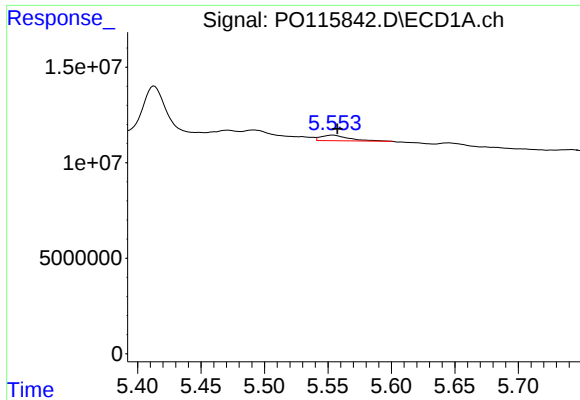

#5 AR-1016-3


R.T.: 5.554 min
Delta R.T.: -0.004 min
Response: 4205807
Conc: 19.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

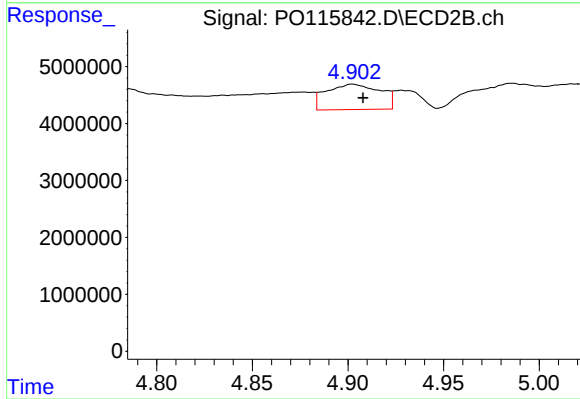


#5 AR-1016-3

R.T.: 4.902 min
Delta R.T.: -0.006 min
Response: 8755257
Conc: 57.85 ng/ml

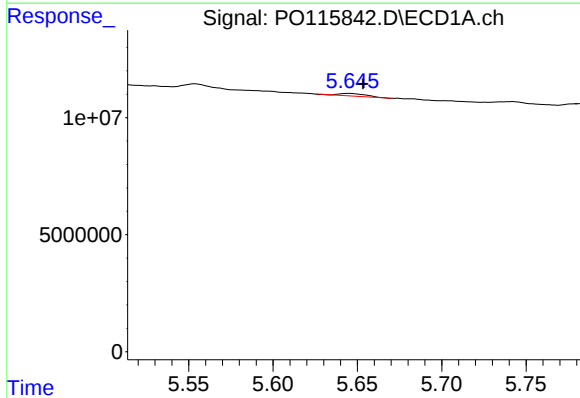


#6 AR-1016-4

R.T.: 5.646 min
Delta R.T.: -0.008 min
Response: 1290536
Conc: 7.23 ng/ml

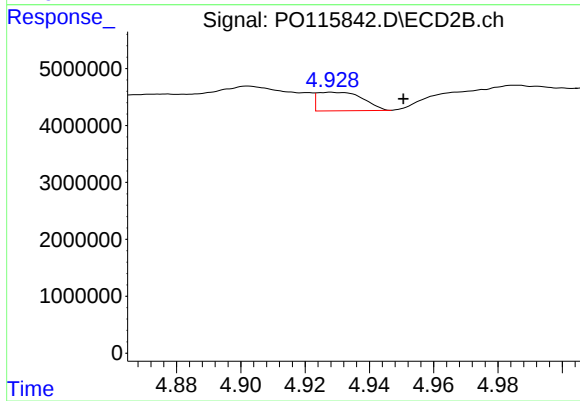

#6 AR-1016-4


R.T.: 4.928 min
Delta R.T.: -0.022 min
Response: 3195236
Conc: 28.35 ng/ml

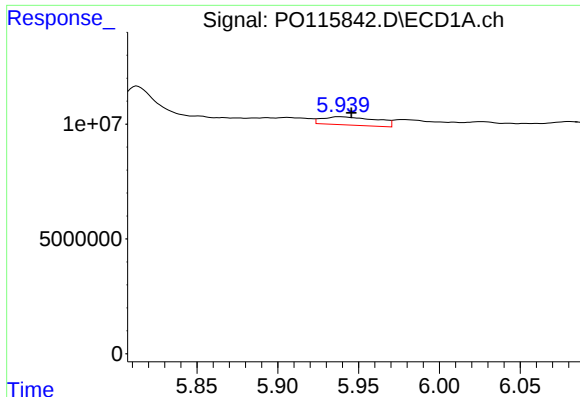

#7 AR-1016-5


R.T.: 5.938 min
Delta R.T.: -0.008 min
Response: 8408426
Conc: 47.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

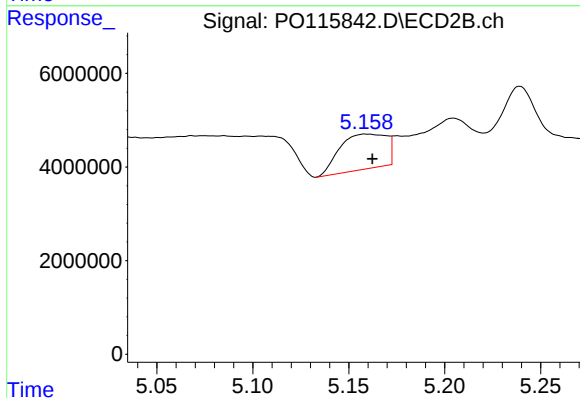


#7 AR-1016-5

R.T.: 5.158 min
Delta R.T.: -0.004 min
Response: 12673757
Conc: 86.60 ng/ml

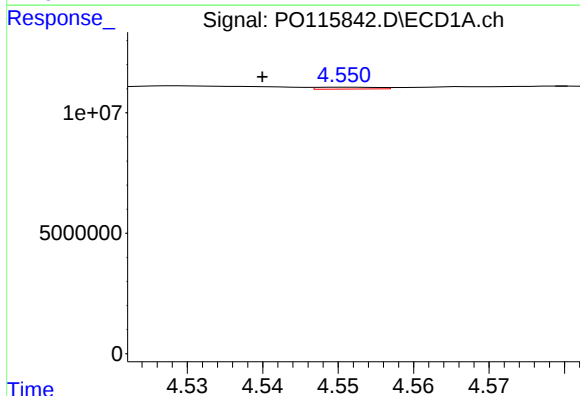


#8 AR-1221-1

R.T.: 4.551 min
Delta R.T.: 0.011 min
Response: 426194
Conc: 5.25 ng/ml

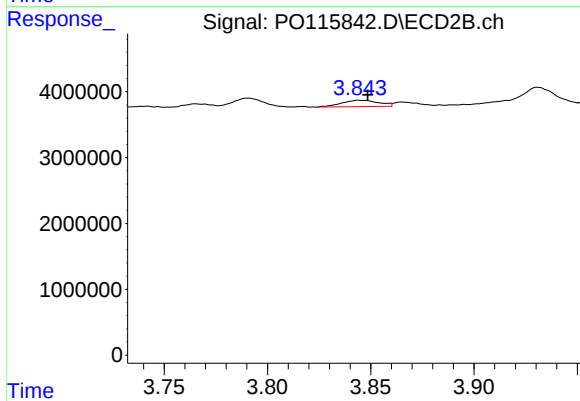

#8 AR-1221-1


R.T.: 3.844 min
Delta R.T.: -0.004 min
Response: 1214913
Conc: 21.54 ng/ml

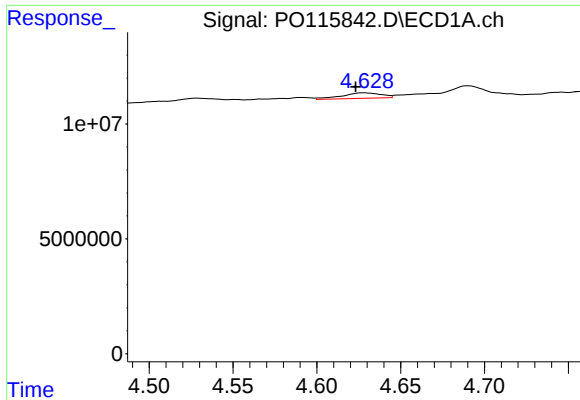

#9 AR-1221-2


R.T.: 4.629 min
Delta R.T.: 0.006 min
Response: 3946080
Conc: 62.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

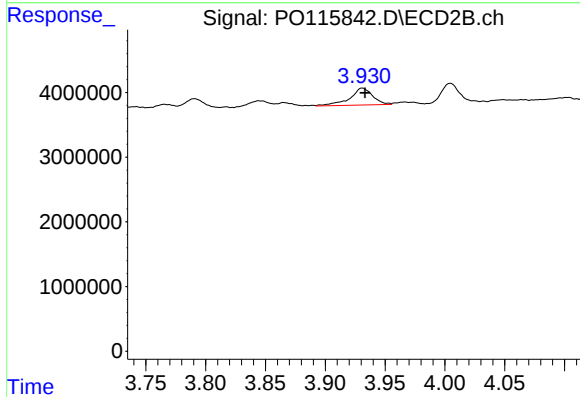


#9 AR-1221-2

R.T.: 3.931 min
Delta R.T.: -0.002 min
Response: 3491989
Conc: 82.27 ng/ml

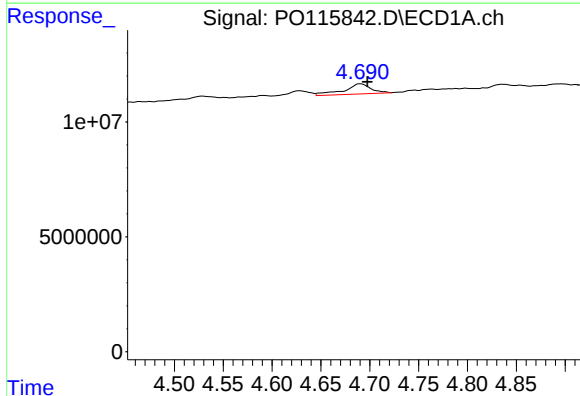


#10 AR-1221-3

R.T.: 4.691 min
Delta R.T.: -0.007 min
Response: 8618005
Conc: 46.16 ng/ml

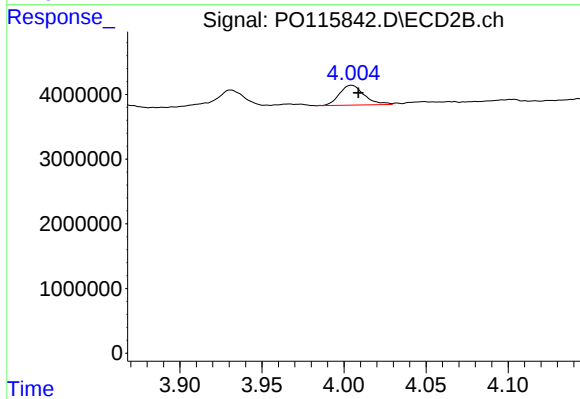

#10 AR-1221-3


R.T.: 4.005 min
Delta R.T.: -0.004 min
Response: 3235023
Conc: 25.16 ng/ml

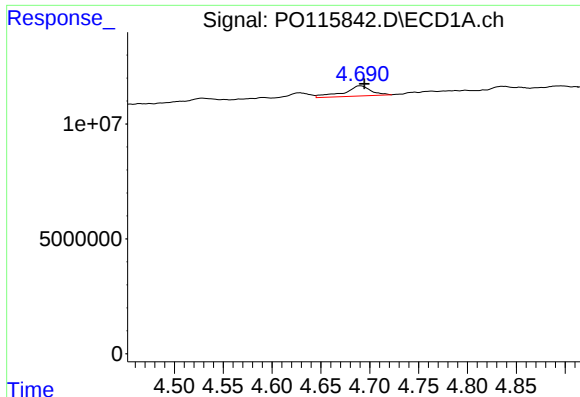

#11 AR-1232-1


R.T.: 4.691 min
Delta R.T.: -0.004 min
Response: 8618005
Conc: 57.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

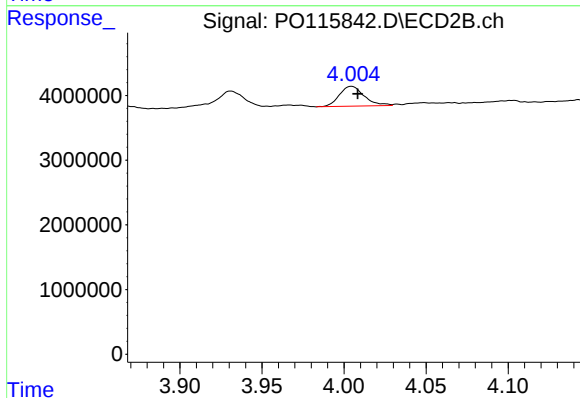


#11 AR-1232-1

R.T.: 4.005 min
Delta R.T.: -0.004 min
Response: 3235023
Conc: 30.28 ng/ml

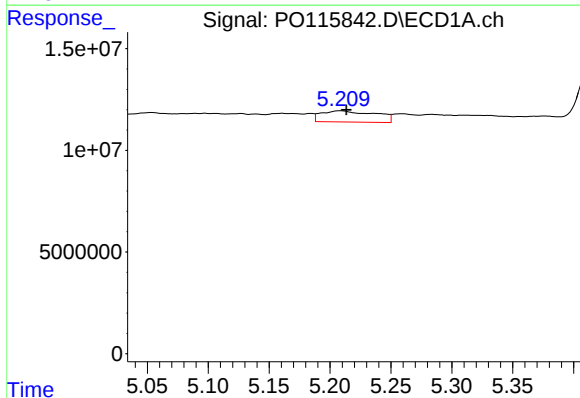


#12 AR-1232-2

R.T.: 5.209 min
Delta R.T.: -0.004 min
Response: 17039140
Conc: 210.75 ng/ml

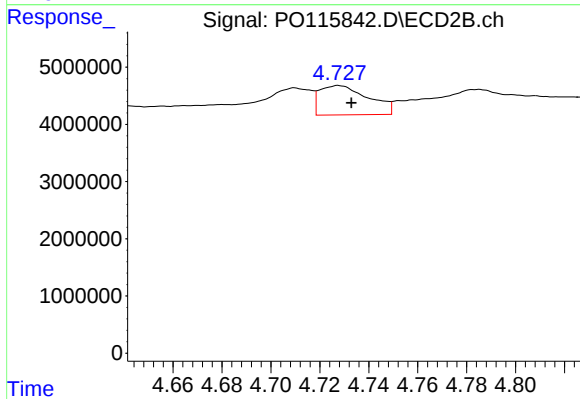

#12 AR-1232-2


R.T.: 4.727 min
Delta R.T.: -0.006 min
Response: 7124594
Conc: 64.19 ng/ml

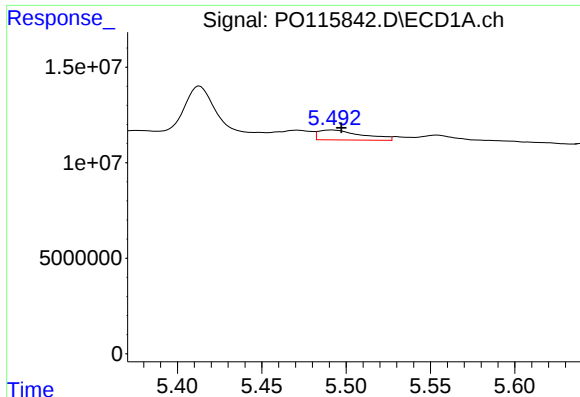

#13 AR-1232-3


R.T.: 5.492 min
Delta R.T.: -0.005 min
Response: 9257038
Conc: 60.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

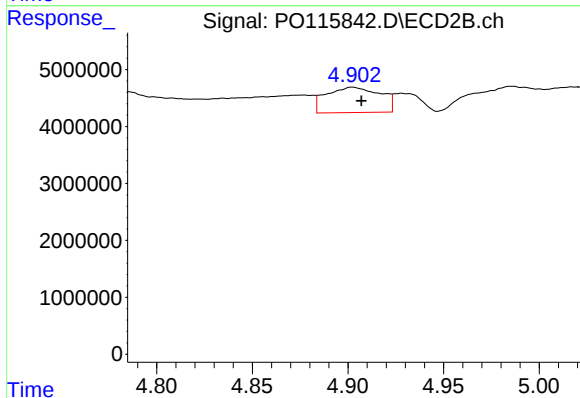


#13 AR-1232-3

R.T.: 4.902 min
Delta R.T.: -0.005 min
Response: 8755257
Conc: 133.94 ng/ml

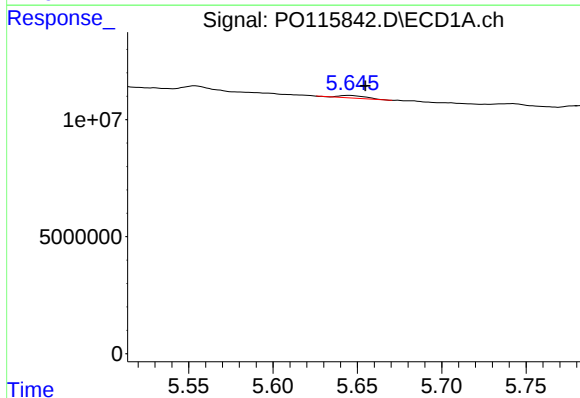


#14 AR-1232-4

R.T.: 5.646 min
Delta R.T.: -0.009 min
Response: 1290536
Conc: 18.43 ng/ml

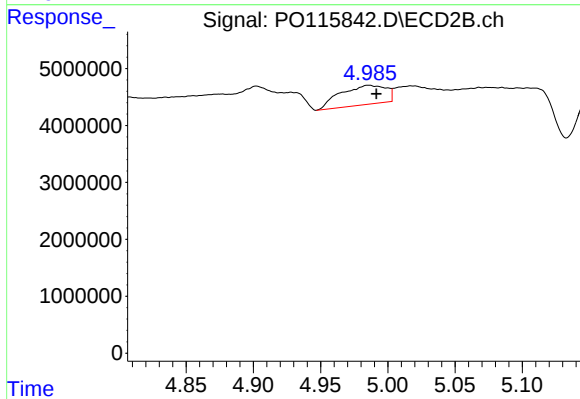

#14 AR-1232-4


R.T.: 4.986 min
Delta R.T.: -0.006 min
Response: 7957067
Conc: 155.02 ng/ml

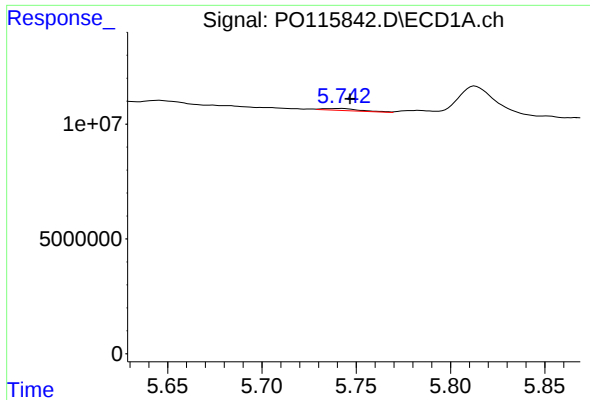

#15 AR-1232-5


R.T.: 5.743 min
Delta R.T.: -0.004 min
Response: 1172052
Conc: 22.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

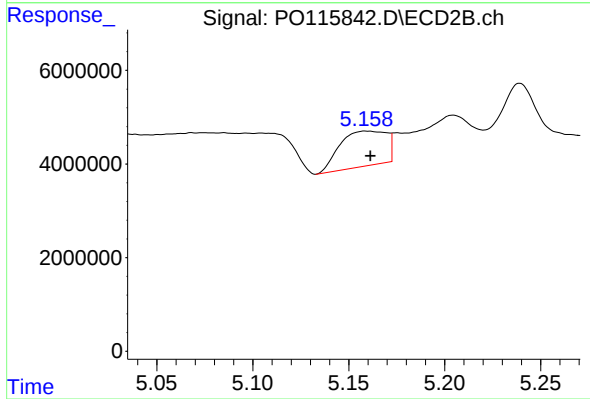


#15 AR-1232-5

R.T.: 5.158 min
Delta R.T.: -0.003 min
Response: 12673757
Conc: 231.49 ng/ml

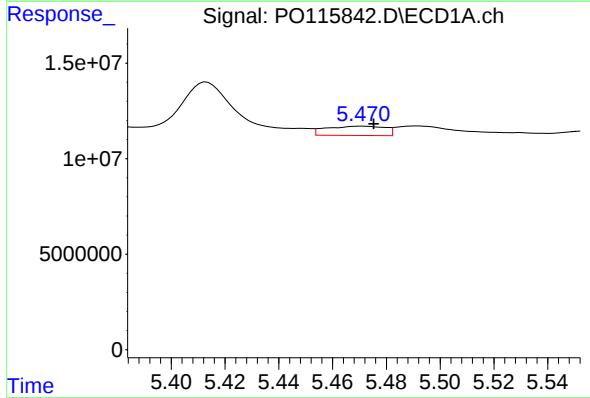


#16 AR-1242-1

R.T.: 5.471 min
Delta R.T.: -0.004 min
Response: 7385137
Conc: 37.18 ng/ml

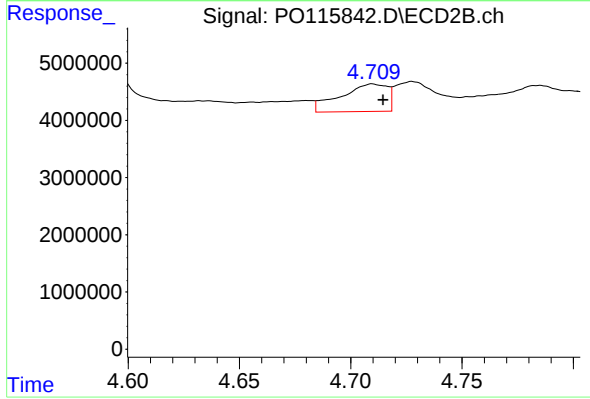

#16 AR-1242-1


R.T.: 4.710 min
Delta R.T.: -0.005 min
Response: 7077078
Conc: 49.70 ng/ml

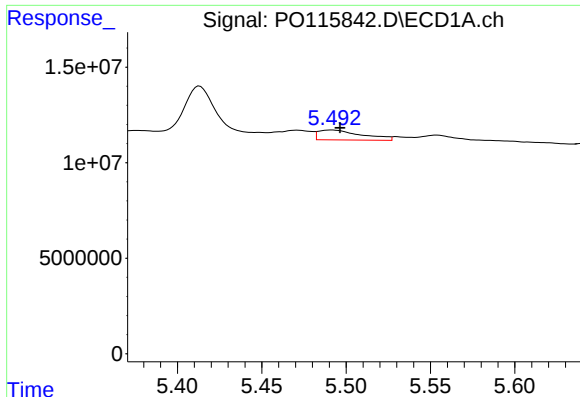

#17 AR-1242-2


R.T.: 5.492 min
Delta R.T.: -0.004 min
Response: 9257038
Conc: 31.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

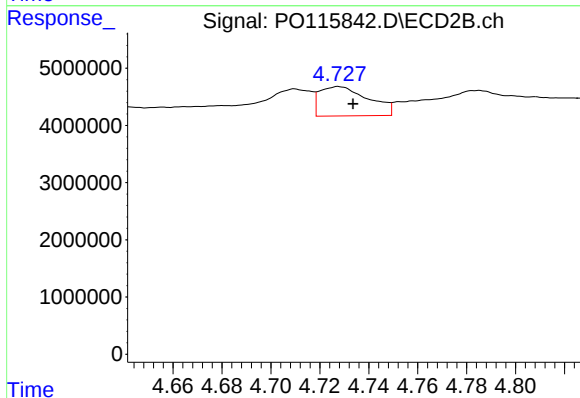


#17 AR-1242-2

R.T.: 4.727 min
Delta R.T.: -0.006 min
Response: 7124594
Conc: 34.03 ng/ml

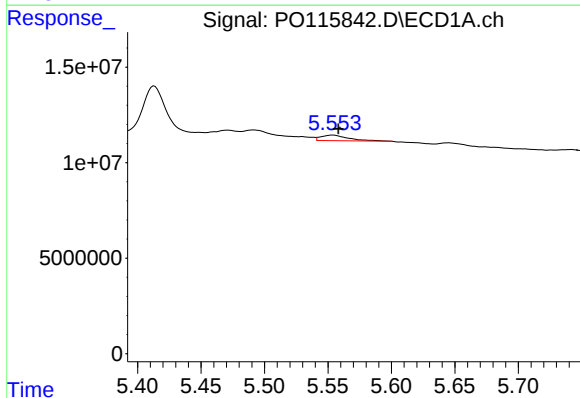


#18 AR-1242-3

R.T.: 5.554 min
Delta R.T.: -0.004 min
Response: 4205807
Conc: 24.91 ng/ml

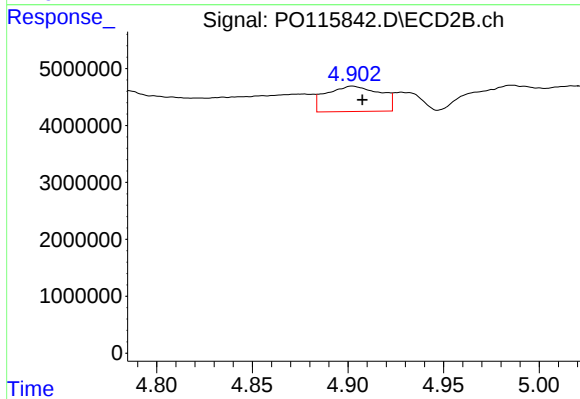

#18 AR-1242-3


R.T.: 4.902 min
Delta R.T.: -0.005 min
Response: 8755257
Conc: 73.30 ng/ml

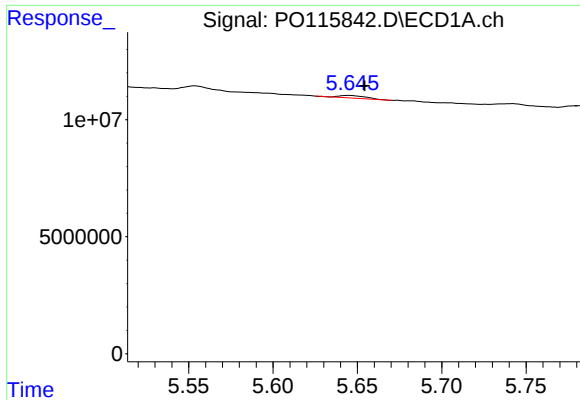

#19 AR-1242-4


R.T.: 5.646 min
Delta R.T.: -0.008 min
Response: 1290536
Conc: 9.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

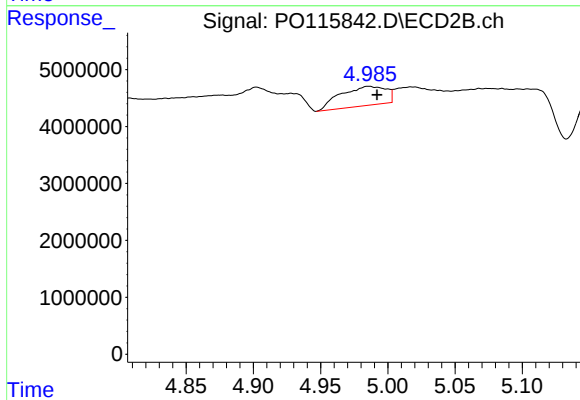


#19 AR-1242-4

R.T.: 4.986 min
Delta R.T.: -0.006 min
Response: 7957067
Conc: 72.94 ng/ml

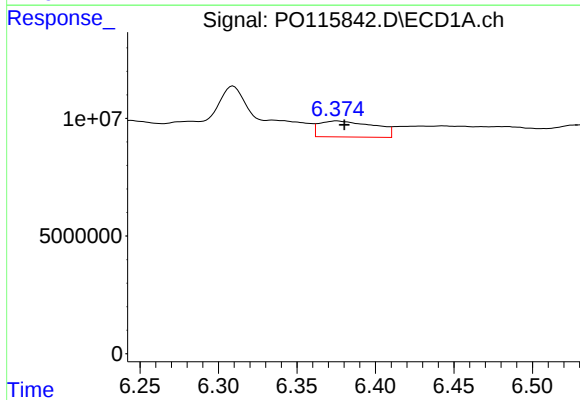


#20 AR-1242-5

R.T.: 6.375 min
Delta R.T.: -0.005 min
Response: 16704448
Conc: 110.30 ng/ml

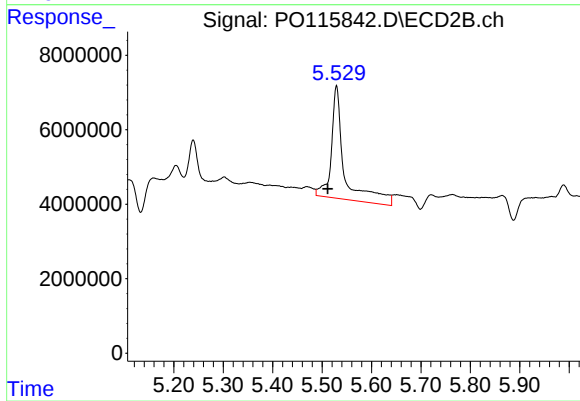

#20 AR-1242-5


R.T.: 5.529 min
Delta R.T.: 0.018 min
Response: 55515400
Conc: 401.92 ng/ml

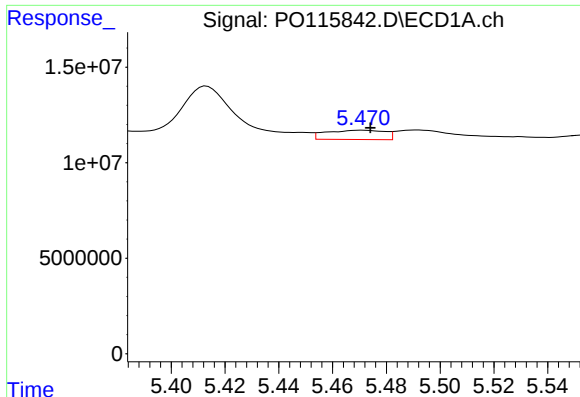

#21 AR-1248-1


R.T.: 5.471 min
Delta R.T.: -0.003 min
Response: 7385137
Conc: 48.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

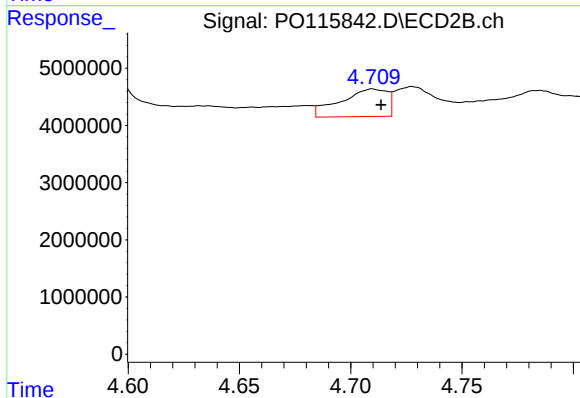


#21 AR-1248-1

R.T.: 4.710 min
Delta R.T.: -0.004 min
Response: 7077078
Conc: 63.28 ng/ml

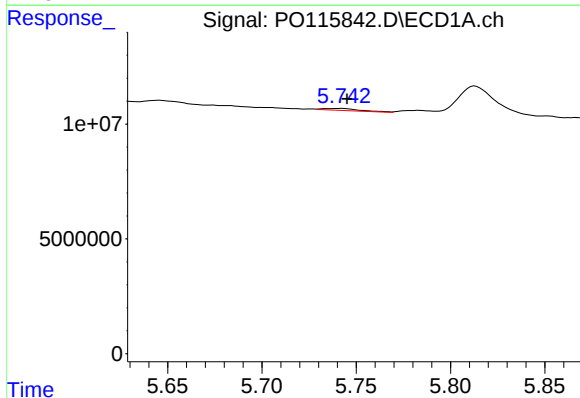


#22 AR-1248-2

R.T.: 5.743 min
Delta R.T.: -0.002 min
Response: 1172052
Conc: 5.84 ng/ml

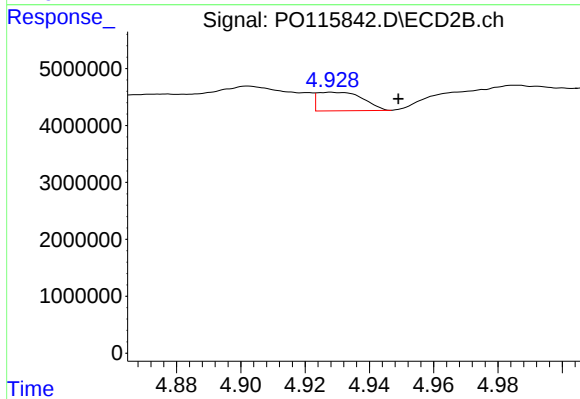

#22 AR-1248-2


R.T.: 4.928 min
Delta R.T.: -0.021 min
Response: 3195236
Conc: 20.98 ng/ml

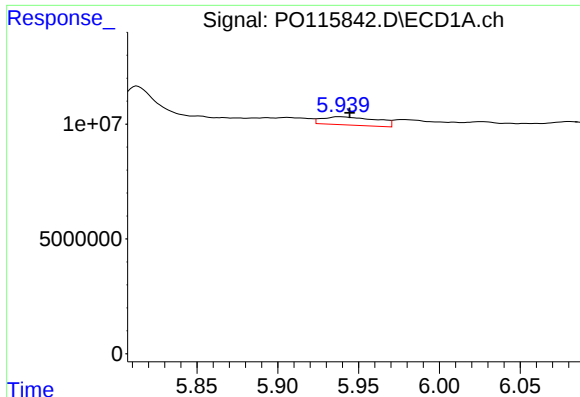

#23 AR-1248-3


R.T.: 5.938 min
Delta R.T.: -0.007 min
Response: 8408426
Conc: 34.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

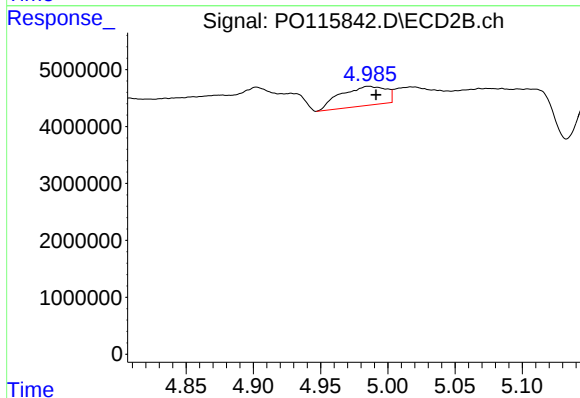


#23 AR-1248-3

R.T.: 4.986 min
Delta R.T.: -0.005 min
Response: 7957067
Conc: 49.57 ng/ml

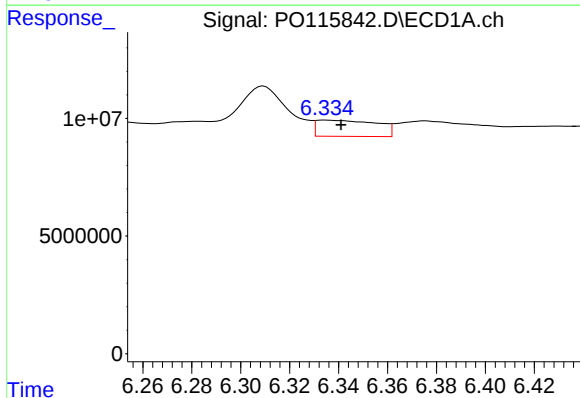


#24 AR-1248-4

R.T.: 6.335 min
Delta R.T.: -0.006 min
Response: 11800806
Conc: 40.02 ng/ml

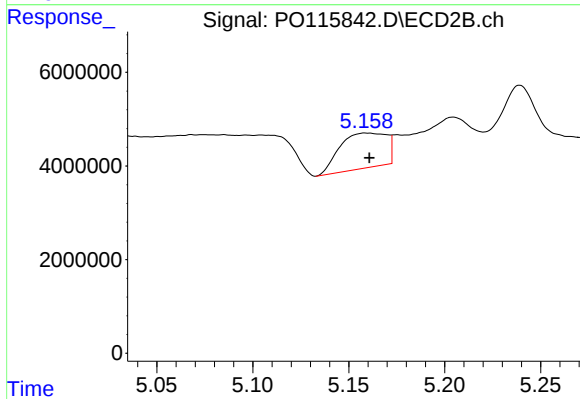

#24 AR-1248-4


R.T.: 5.158 min
Delta R.T.: -0.002 min
Response: 12673757
Conc: 67.72 ng/ml

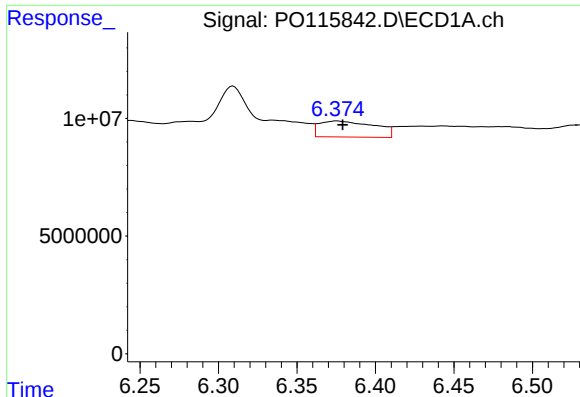

#25 AR-1248-5


R.T.: 6.375 min
Delta R.T.: -0.004 min
Response: 16704448
Conc: 64.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

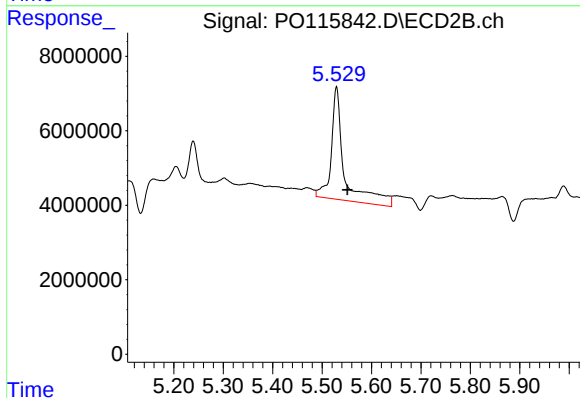


#25 AR-1248-5

R.T.: 5.529 min
Delta R.T.: -0.022 min
Response: 55515400
Conc: 280.44 ng/ml

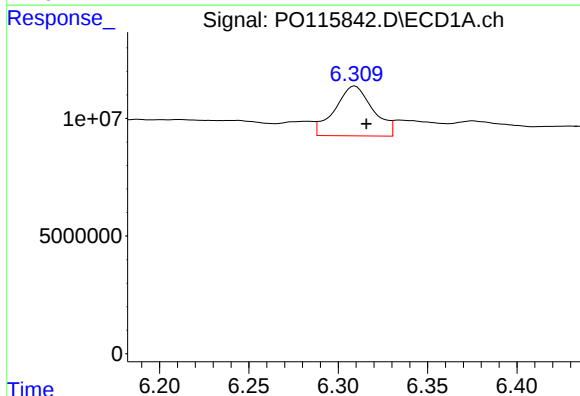


#26 AR-1254-1

R.T.: 6.309 min
Delta R.T.: -0.006 min
Response: 31500407
Conc: 121.76 ng/ml

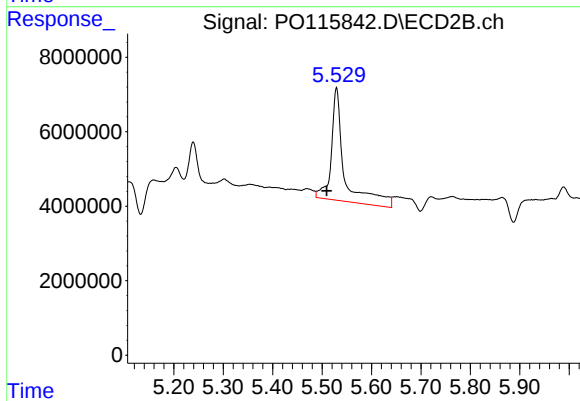

#26 AR-1254-1


R.T.: 5.529 min
Delta R.T.: 0.020 min
Response: 55515400
Conc: 189.94 ng/ml

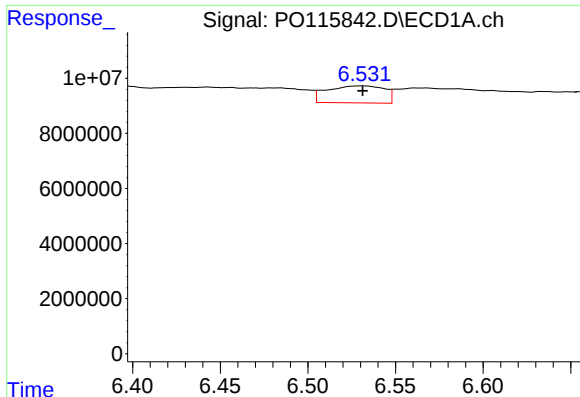

#27 AR-1254-2


R.T.: 6.532 min
Delta R.T.: 0.000 min
Response: 14027452
Conc: 34.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

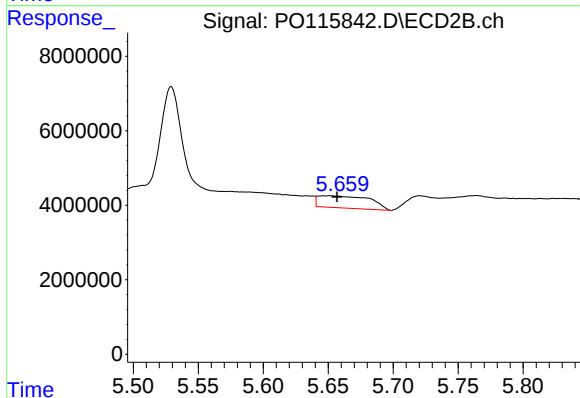


#27 AR-1254-2

R.T.: 5.646 min
Delta R.T.: -0.010 min
Response: 9003547
Conc: 35.75 ng/ml

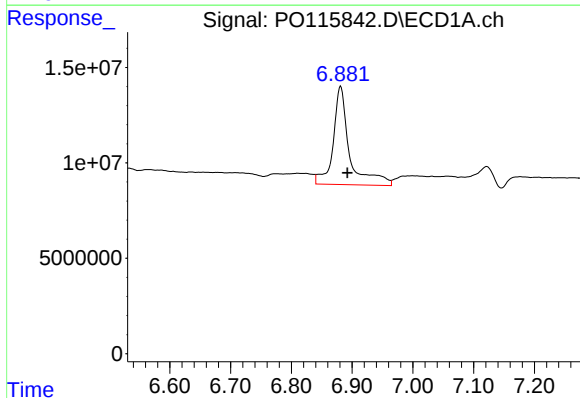


#28 AR-1254-3

R.T.: 6.881 min
Delta R.T.: -0.011 min
Response: 96065173
Conc: 233.98 ng/ml

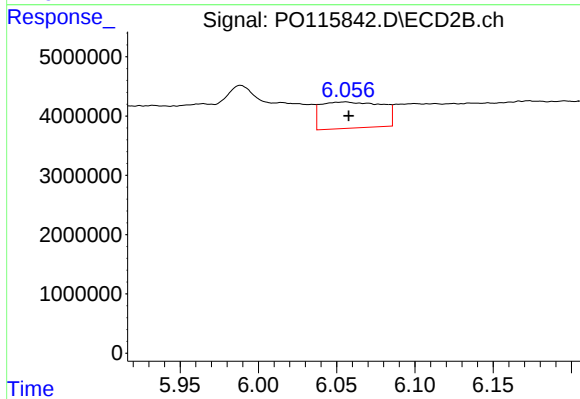

#28 AR-1254-3


R.T.: 6.056 min
Delta R.T.: -0.002 min
Response: 12013345
Conc: 30.52 ng/ml

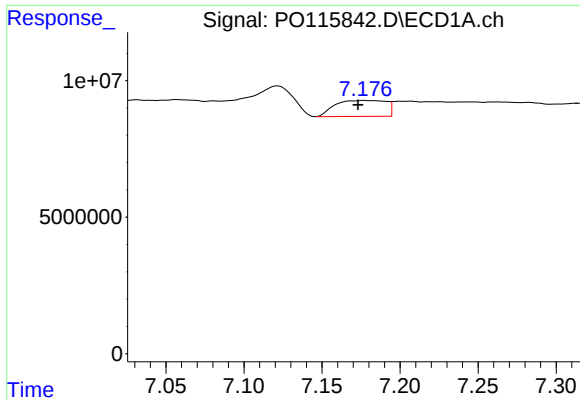

#29 AR-1254-4


R.T.: 7.177 min
Delta R.T.: 0.004 min
Response: 13246629
Conc: 38.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

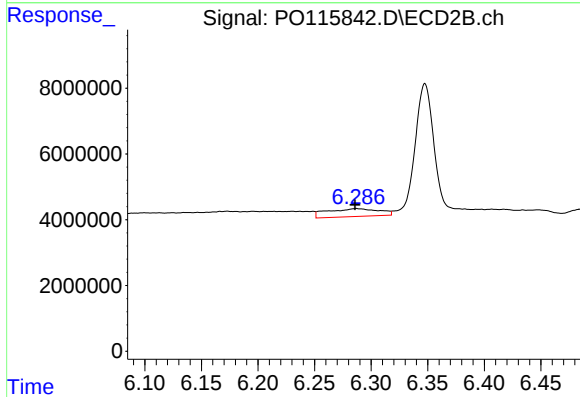


#29 AR-1254-4

R.T.: 6.287 min
Delta R.T.: 0.001 min
Response: 7706813
Conc: 28.80 ng/ml

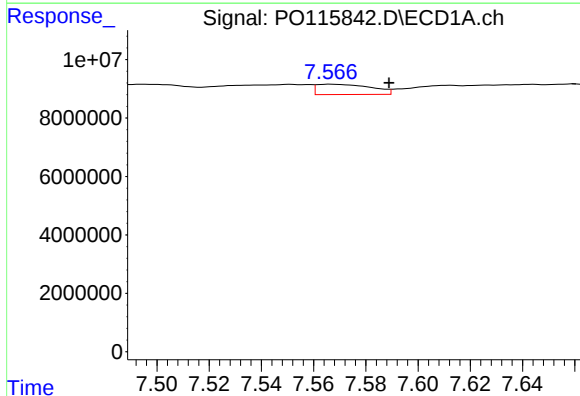


#30 AR-1254-5

R.T.: 7.566 min
Delta R.T.: -0.022 min
Response: 5118921
Conc: 15.80 ng/ml

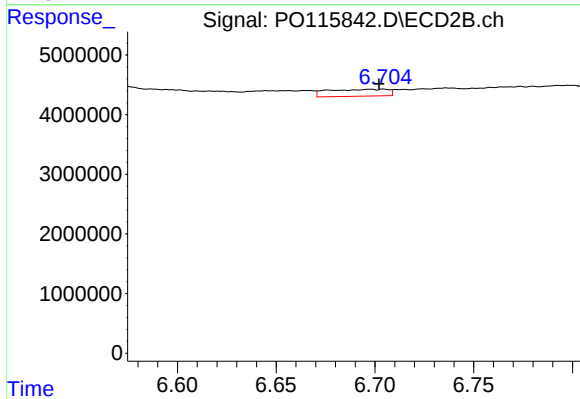

#30 AR-1254-5


R.T.: 6.697 min
Delta R.T.: -0.005 min
Response: 2431037
Conc: 6.80 ng/ml

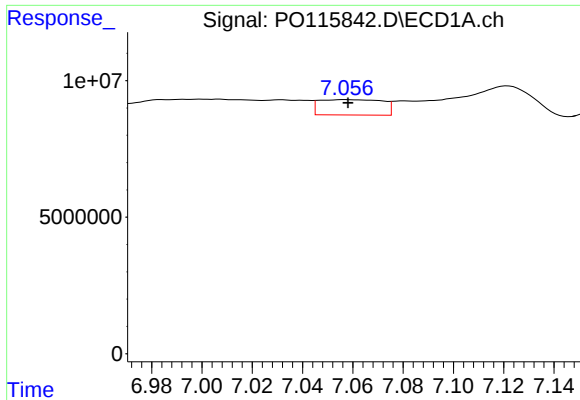

#31 AR-1260-1


R.T.: 7.057 min
Delta R.T.: -0.001 min
Response: 9875189
Conc: 34.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

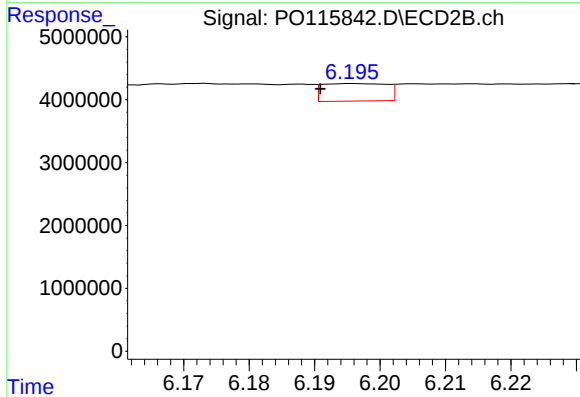


#31 AR-1260-1

R.T.: 6.196 min
Delta R.T.: 0.005 min
Response: 1906407
Conc: 7.27 ng/ml

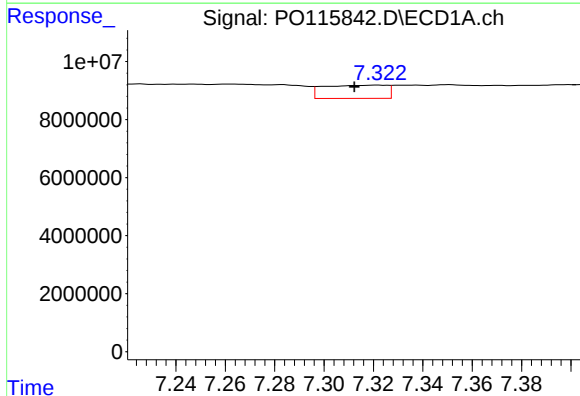


#32 AR-1260-2

R.T.: 7.322 min
Delta R.T.: 0.009 min
Response: 8074032
Conc: 18.45 ng/ml

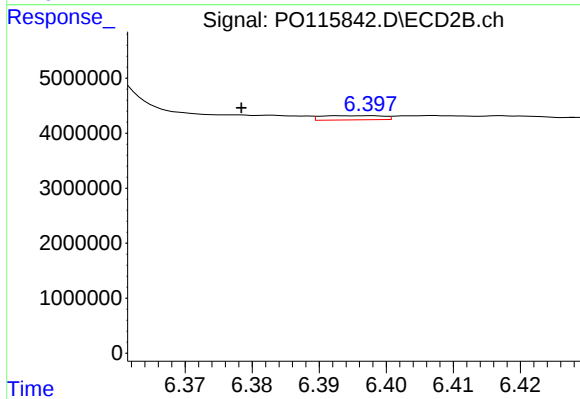

#32 AR-1260-2


R.T.: 6.397 min
Delta R.T.: 0.018 min
Response: 490282
Conc: 1.40 ng/ml

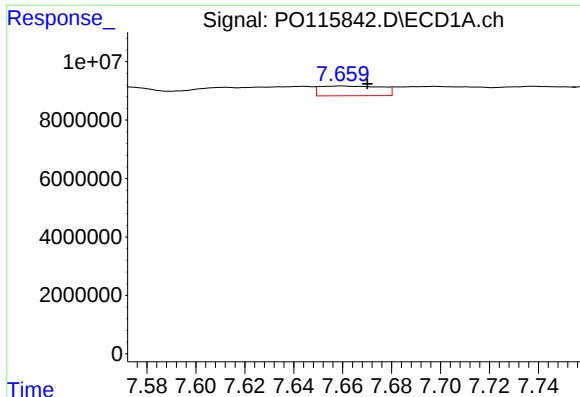

#33 AR-1260-3


R.T.: 7.660 min
Delta R.T.: -0.011 min
Response: 5893624
Conc: 17.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

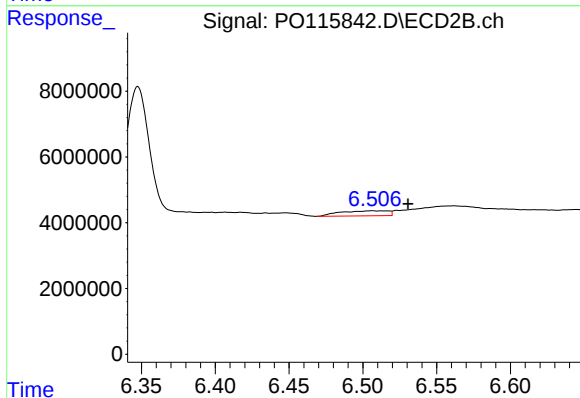


#33 AR-1260-3

R.T.: 6.506 min
Delta R.T.: -0.024 min
Response: 3455587
Conc: 10.76 ng/ml

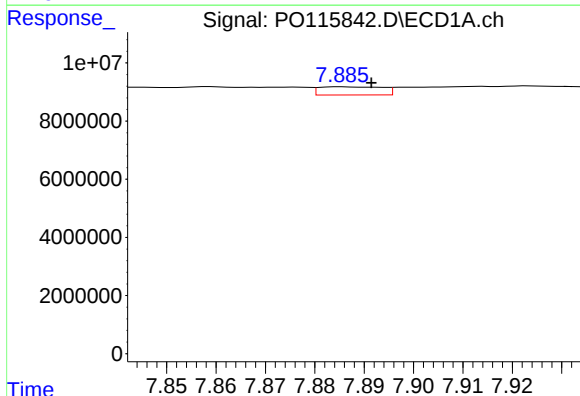


#34 AR-1260-4

R.T.: 7.886 min
Delta R.T.: -0.006 min
Response: 2524309
Conc: 8.21 ng/ml

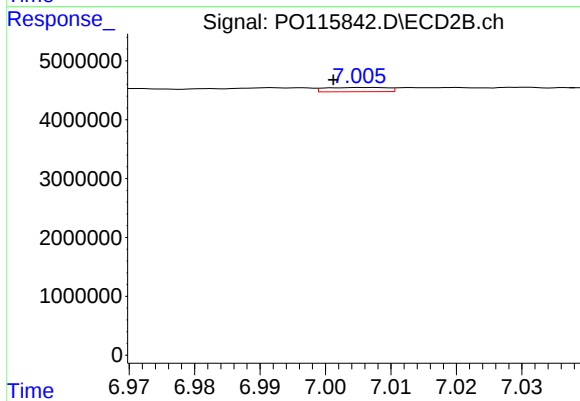

#34 AR-1260-4


R.T.: 7.006 min
Delta R.T.: 0.005 min
Response: 477797
Conc: 1.86 ng/ml

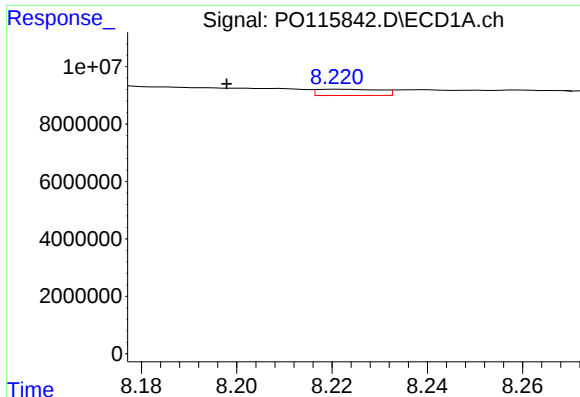

#35 AR-1260-5


R.T.: 8.221 min
Delta R.T.: 0.023 min
Response: 1999997
Conc: 2.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

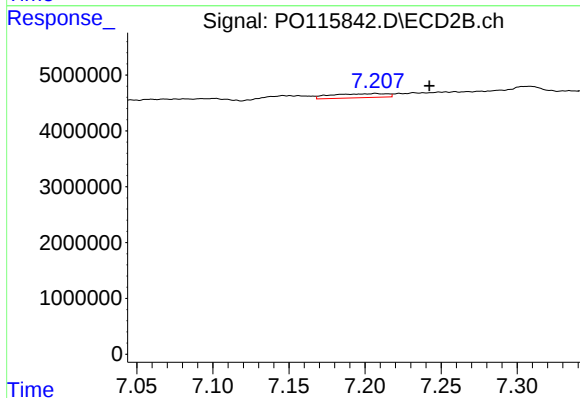


#35 AR-1260-5

R.T.: 7.207 min
Delta R.T.: -0.035 min
Response: 1888399
Conc: 2.69 ng/ml

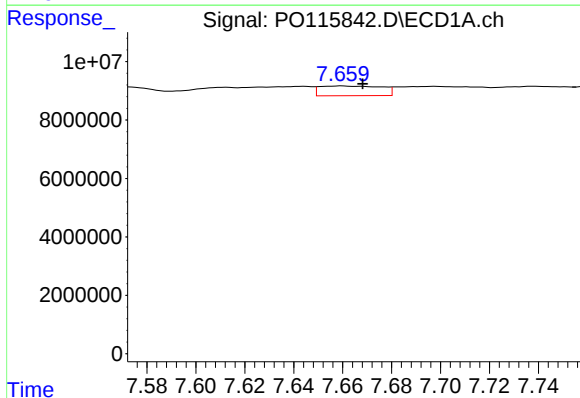


#36 AR-1262-1

R.T.: 7.660 min
Delta R.T.: -0.009 min
Response: 5893624
Conc: 23.87 ng/ml

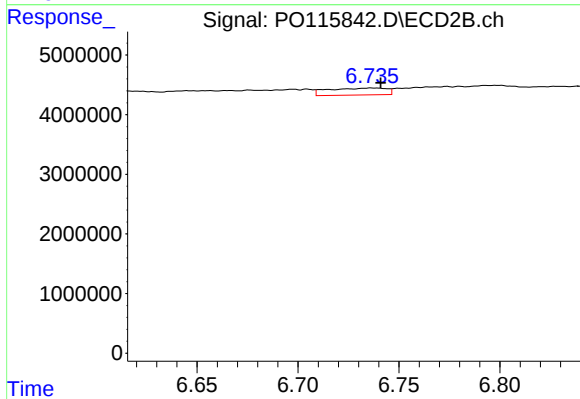

#36 AR-1262-1


R.T.: 6.737 min
Delta R.T.: -0.004 min
Response: 2333462
Conc: 10.95 ng/ml

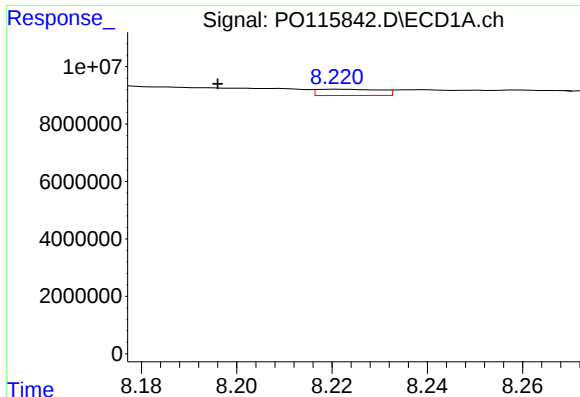

#37 AR-1262-2


R.T.: 8.221 min
Delta R.T.: 0.025 min
Response: 1999997
Conc: 5.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

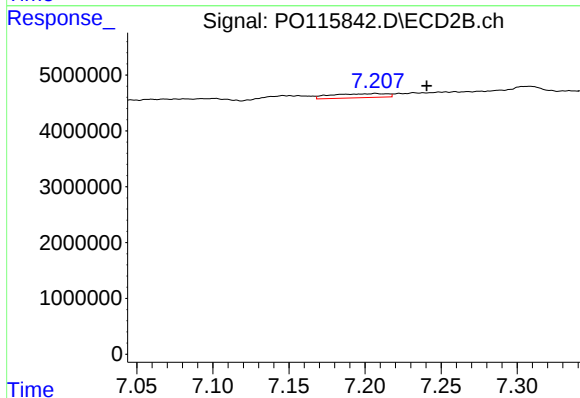


#37 AR-1262-2

R.T.: 7.207 min
Delta R.T.: -0.034 min
Response: 1888399
Conc: 5.42 ng/ml

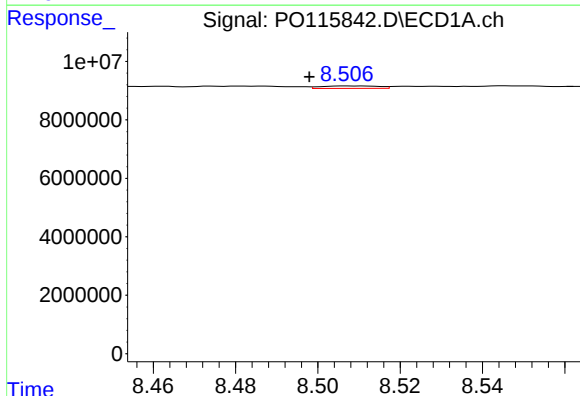


#38 AR-1262-3

R.T.: 8.511 min
Delta R.T.: 0.013 min
Response: 829598
Conc: 3.26 ng/ml

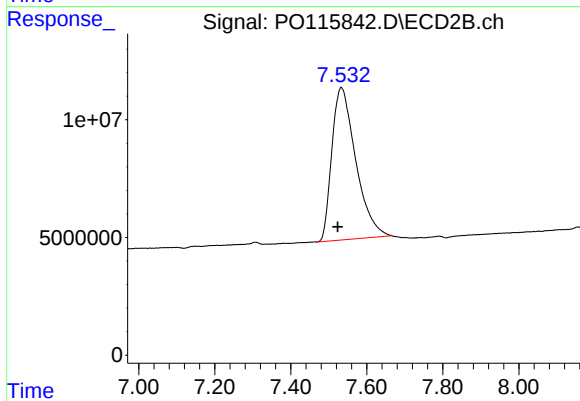

#38 AR-1262-3


R.T.: 7.533 min
Delta R.T.: 0.009 min
Response: 282243223
Conc: 1804.73 ng/ml

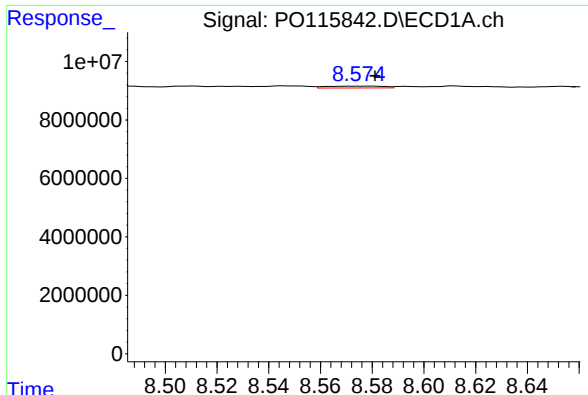

#39 AR-1262-4


R.T.: 8.575 min
Delta R.T.: -0.006 min
Response: 977705
Conc: 5.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

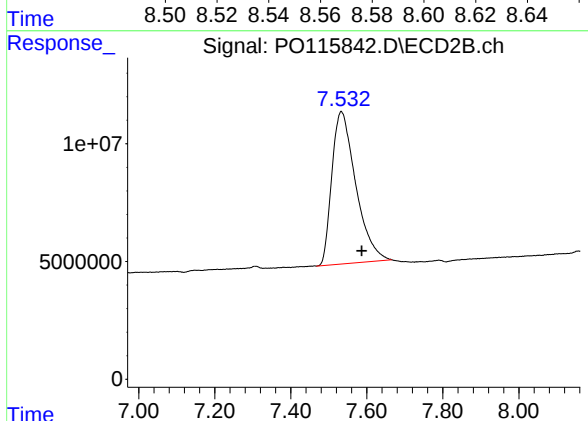


#39 AR-1262-4

R.T.: 7.533 min
Delta R.T.: -0.054 min
Response: 282243223
Conc: 1140.97 ng/ml

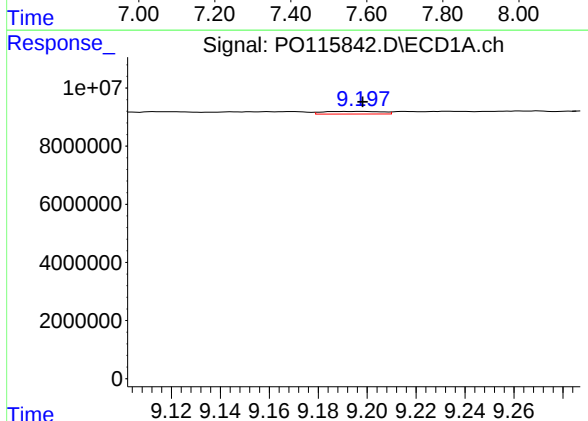


#40 AR-1262-5

R.T.: 9.198 min
Delta R.T.: 0.000 min
Response: 1479382
Conc: 10.98 ng/ml

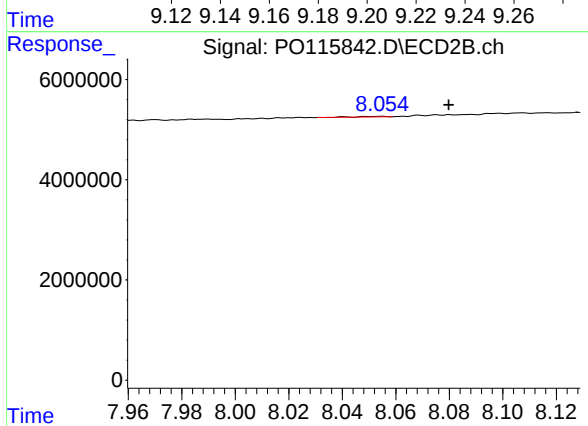

#40 AR-1262-5


R.T.: 8.055 min
Delta R.T.: -0.025 min
Response: 97932
Conc: 0.88 ng/ml

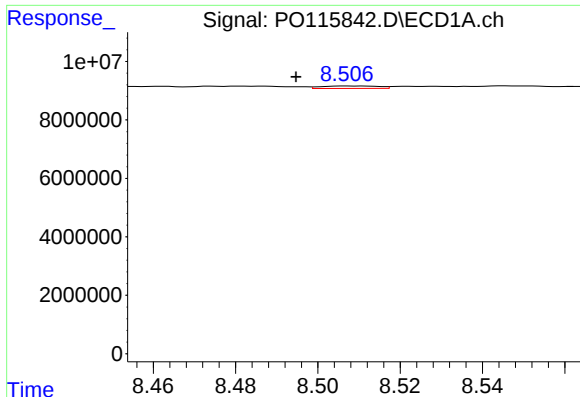

#41 AR-1268-1


R.T.: 8.511 min
Delta R.T.: 0.016 min
Response: 829598
Conc: 0.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

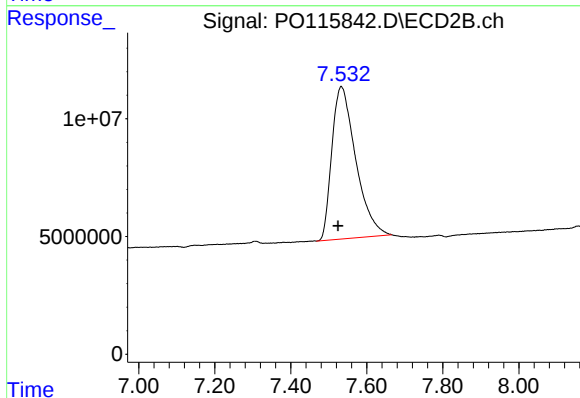


#41 AR-1268-1

R.T.: 7.533 min
Delta R.T.: 0.008 min
Response: 282243223
Conc: 318.58 ng/ml

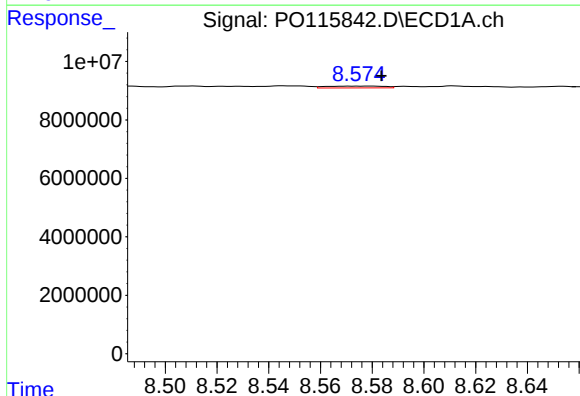


#42 AR-1268-2

R.T.: 8.575 min
Delta R.T.: -0.009 min
Response: 977705
Conc: 1.14 ng/ml

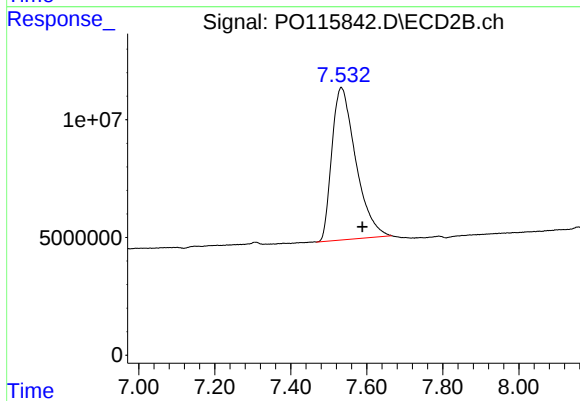

#42 AR-1268-2


R.T.: 7.533 min
Delta R.T.: -0.056 min
Response: 282243223
Conc: 376.79 ng/ml

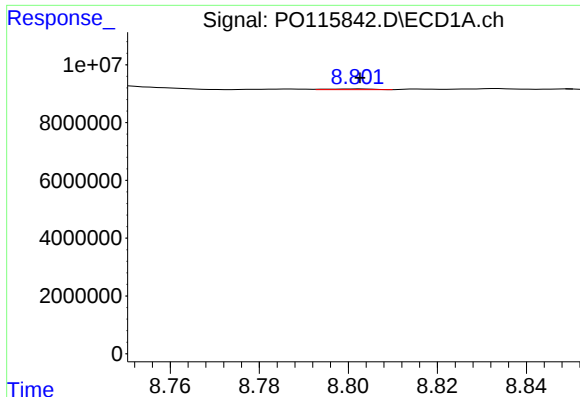

#43 AR-1268-3


R.T.: 8.802 min
Delta R.T.: 0.000 min
Response: 191480
Conc: 0.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

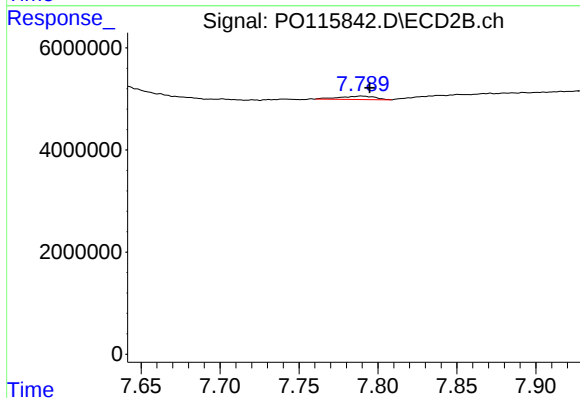


#43 AR-1268-3

R.T.: 7.790 min
Delta R.T.: -0.005 min
Response: 1037005
Conc: 1.63 ng/ml

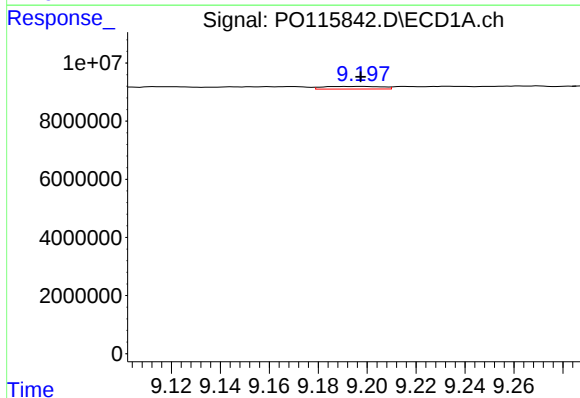


#44 AR-1268-4

R.T.: 9.198 min
Delta R.T.: 0.000 min
Response: 1479382
Conc: 4.74 ng/ml

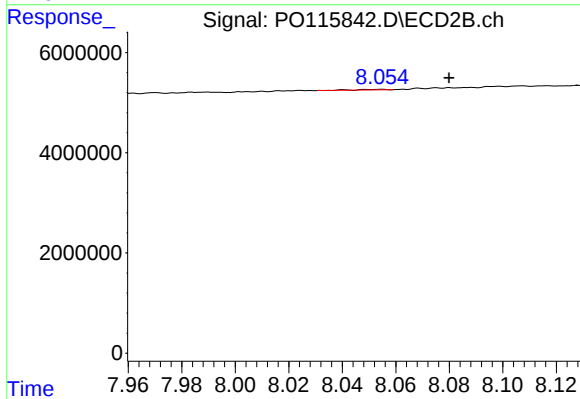

#44 AR-1268-4


R.T.: 8.055 min
Delta R.T.: -0.025 min
Response: 97932
Conc: 0.38 ng/ml

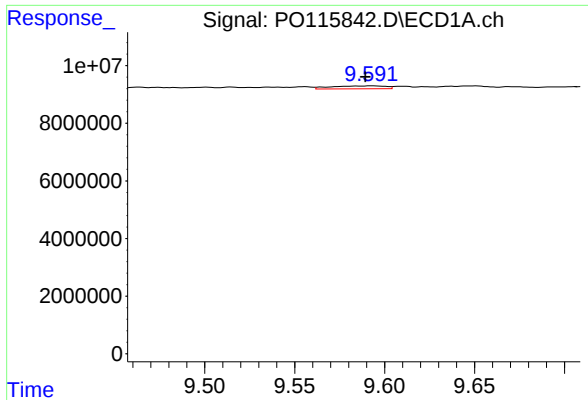

#45 AR-1268-5

R.T.: 9.593 min
Delta R.T.: 0.003 min
Response: 2146165
Conc: 0.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

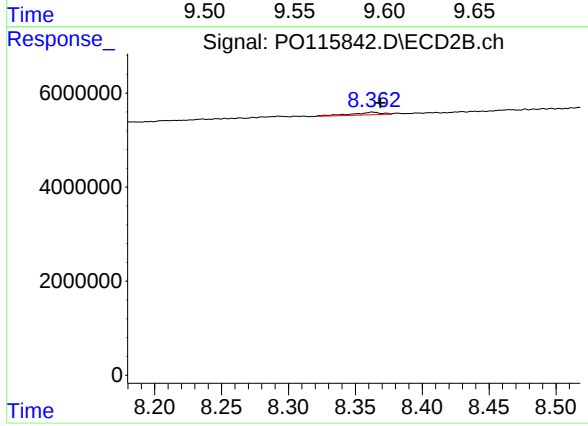

#45 AR-1268-5

R.T.: 8.363 min
Delta R.T.: -0.006 min
Response: 875941
Conc: 0.52 ng/ml