

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121225\
 Data File : PO115843.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Dec 2025 10:01
 Operator : YP/AJ
 Sample : Q3530-09
 Misc : AR1242 25PPB WATER MDL
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT4-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 02:43:47 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 05 02:11:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.333	3.635	341.8E6	207.3E6	44.001	42.540
2)	SA Decachlor...	9.907	8.615	240.1E6	176.5E6	45.630	41.042
Target Compounds							
3)	L1 AR-1016-1	5.472	4.709	12174893	9201942	48.961	49.804
4)	L1 AR-1016-2	5.493	4.728	17388206	11713247	45.657	44.317
5)	L1 AR-1016-3	5.555	4.902	10789703	7297592	50.470	48.220
6)	L1 AR-1016-4	5.651	4.938	6439603	1218269	36.062	10.809 #
7)	L1 AR-1016-5	5.942	5.156	17407353	18483225	99.229	126.302 #
8)	L2 AR-1221-1	4.527	3.845	7624589	336454	93.902	5.965 #
9)	L2 AR-1221-2	4.630	3.931	5634202	6544340	89.405	154.188 #
10)	L2 AR-1221-3	4.691	4.004	9880333	4353694	52.916	33.857 #
11)	L3 AR-1232-1	4.691	4.004	9880333	4353694	66.017	40.751 #
12)	L3 AR-1232-2	5.209	4.728	9586513	11713247	118.571	105.534
13)	L3 AR-1232-3	5.493	4.902	17388206	7297592	112.982	111.641
14)	L3 AR-1232-4	5.651	4.986	6439603	6725603	91.954	131.026 #
15)	L3 AR-1232-5	5.742	5.156	6185782	18483225	119.101	337.605 #
16)	L4 AR-1242-1	5.472	4.709	12174893	9201942	61.296	64.626
17)	L4 AR-1242-2	5.493	4.728	17388206	11713247	59.367	55.947
18)	L4 AR-1242-3	5.555	4.902	10789703	7297592	63.914	61.097
19)	L4 AR-1242-4	5.651	4.986	6439603	6725603	47.119	61.651 #
20)	L4 AR-1242-5	6.376	5.505	24865014	9688719	164.186	70.145 #
21)	L5 AR-1248-1	5.472	4.709	12174893	9201942	80.221	82.286
22)	L5 AR-1248-2	5.742	4.938	6185782	1218269	30.803	8.000 #
23)	L5 AR-1248-3	5.942	4.986	17407353	6725603	70.590	41.897 #
24)	L5 AR-1248-4	6.339	5.156	18716960	18483225	63.479	98.764 #
25)	L5 AR-1248-5	6.376	5.528	24865014	33923101	96.031	171.368 #
26)	L6 AR-1254-1	6.307	5.505	19872495	9688719	76.813	33.150 #
27)	L6 AR-1254-2	6.533	5.652	20732382	15883188	51.521	63.075
28)	L6 AR-1254-3	6.881	6.054	89857157	14555558	218.862	36.982 #
29)	L6 AR-1254-4	7.172	6.286	19608719	8752072	56.499	32.708 #
30)	L6 AR-1254-5	7.607	6.699	4671928	2157849	14.418	6.035 #
31)	L7 AR-1260-1	7.058	6.196	12003174	6537446	41.433	24.936 #
32)	L7 AR-1260-2	7.325	6.348	31424081	39077159	71.789	111.505 #
33)	L7 AR-1260-3	7.669	6.506	9836073	17408350	29.222	54.186 #
34)	L7 AR-1260-4	7.882	6.997	4963598	2023443	16.143	7.878 #
35)	L7 AR-1260-5	8.199	7.244	792637	2248425	1.088	3.206 #
36)	L8 AR-1262-1	7.669	6.734	9836073	4442568	39.845	20.853 #
37)	L8 AR-1262-2	8.199	7.244	792637	2248425	2.002	6.455 #
38)	L8 AR-1262-3	8.498	7.533	1432436	228.6E6	5.621	1462.027 #
39)	L8 AR-1262-4	8.573	7.533f	1979443	228.6E6	10.219	924.307 #
40)	L8 AR-1262-5	9.209	8.083	913478	108232	6.782	0.971 #
41)	L9 AR-1268-1	8.498	7.533	1432436	228.6E6	1.439	258.081 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121225\
Data File : PO115843.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Dec 2025 10:01
Operator : YP/AJ
Sample : Q3530-09
Misc : AR1242 25PPB WATER MDL
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 02:43:47 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120425.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 05 02:11:05 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.573	7.533f	1979443	228.6E6	2.314	305.241 #
43)	L9 AR-1268-3	8.801	7.790	248811	1245784	0.335	1.957 #
44)	L9 AR-1268-4	9.209	8.083	913478	108232	2.926	0.420 #
45)	L9 AR-1268-5	9.586	8.363	3651911	908232	1.677	0.539 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121225\
Data File : PO115843.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Dec 2025 10:01
Operator : YP/AJ
Sample : Q3530-09
Misc : AR1242 25PPB WATER MDL
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 02:43:47 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120425.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 05 02:11:05 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

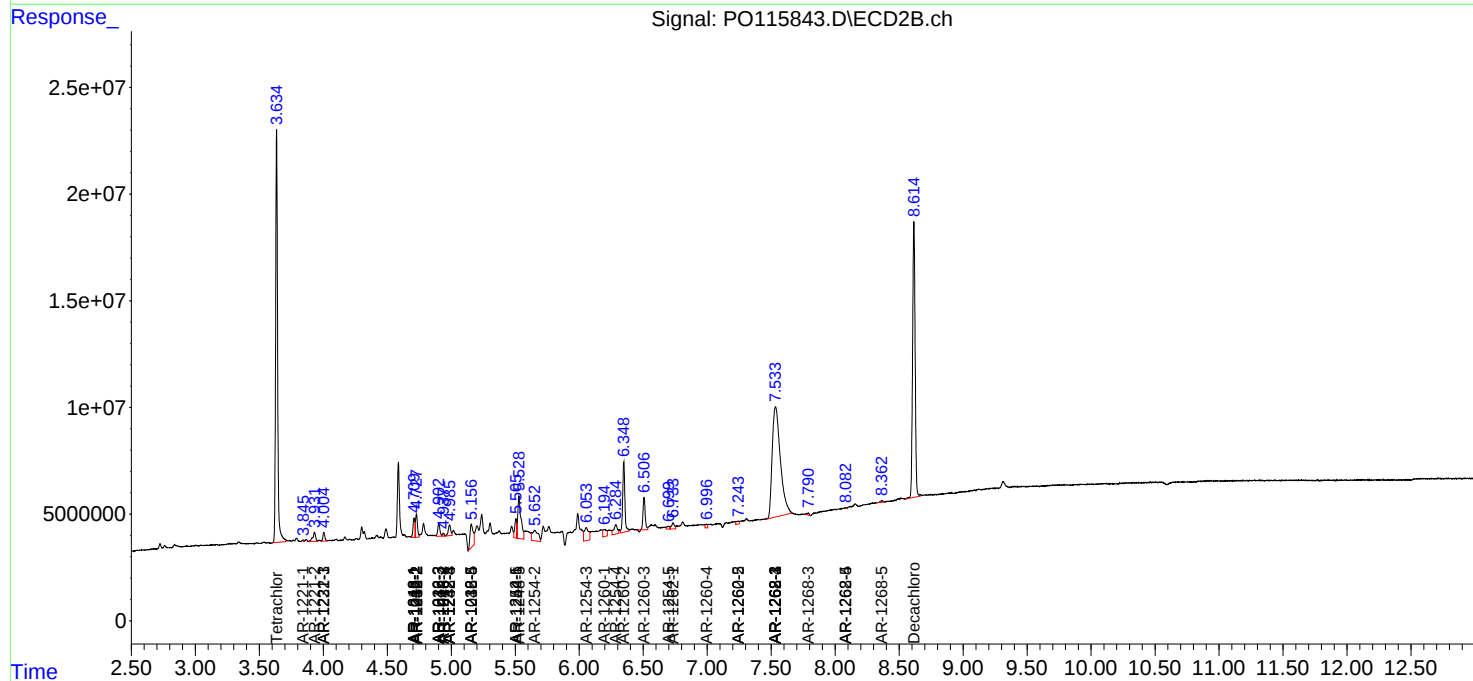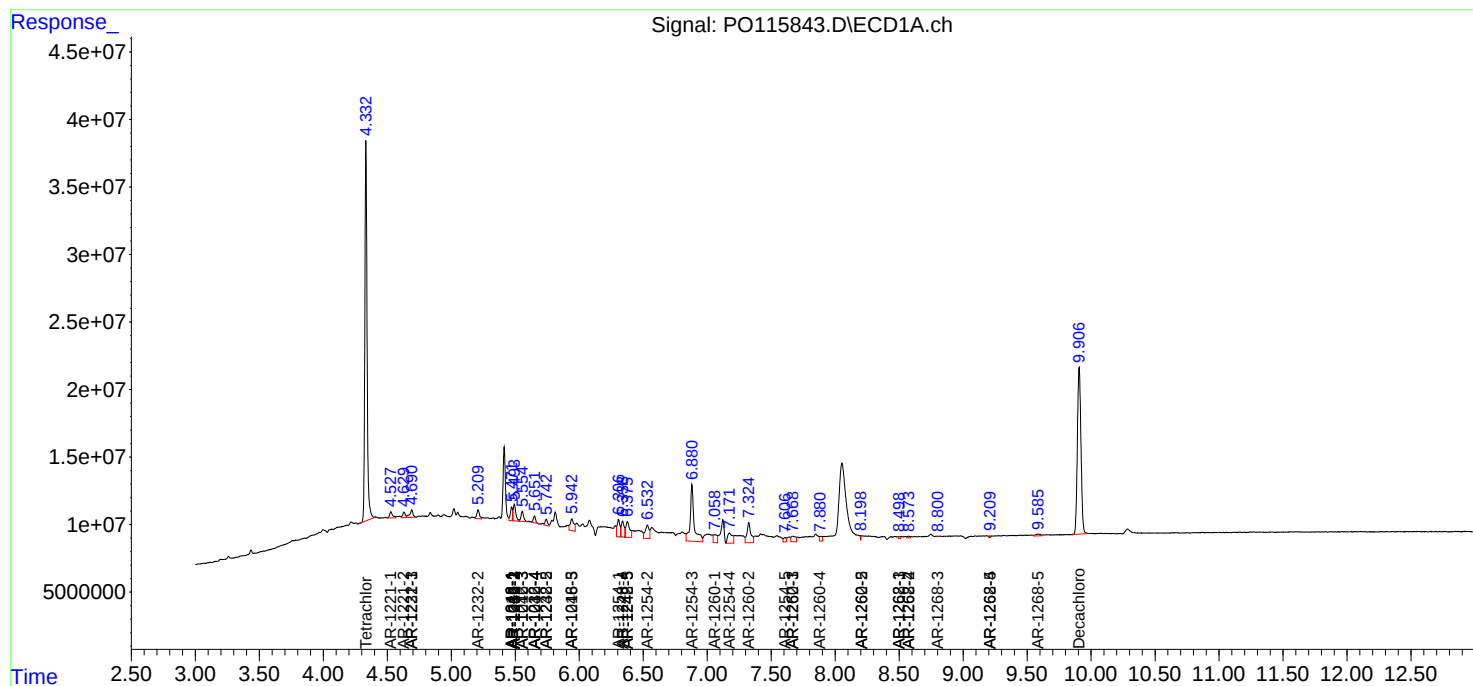


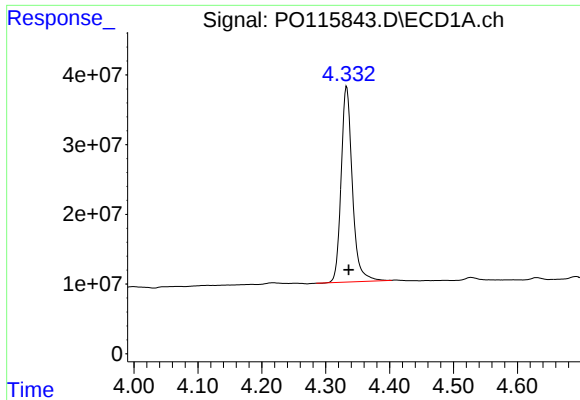

#1 Tetrachloro-m-xylene


R.T.: 4.333 min
Delta R.T.: -0.003 min
Response: 341765282
Conc: 44.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

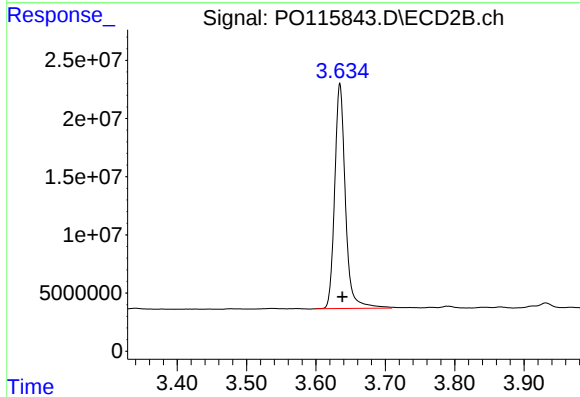


#1 Tetrachloro-m-xylene

R.T.: 3.635 min
Delta R.T.: -0.004 min
Response: 207309225
Conc: 42.54 ng/ml

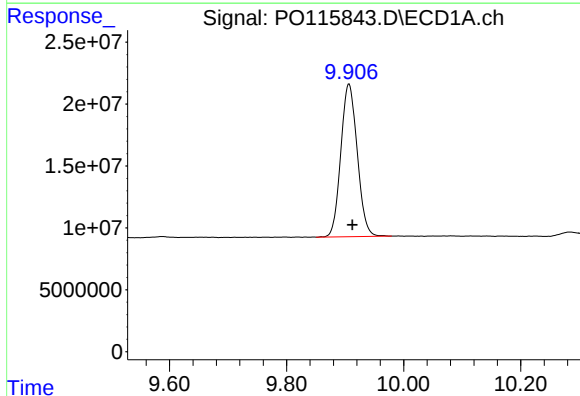


#2 Decachlorobiphenyl

R.T.: 9.907 min
Delta R.T.: -0.006 min
Response: 240064521
Conc: 45.63 ng/ml

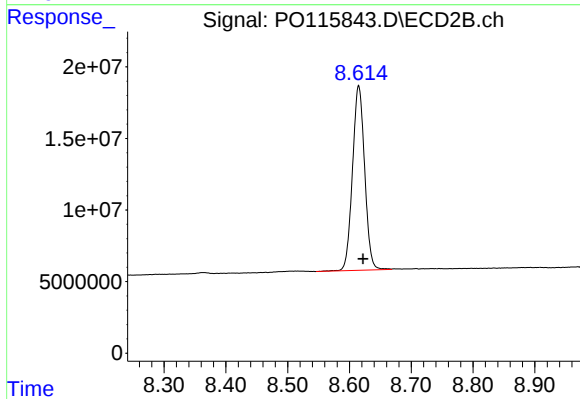

#2 Decachlorobiphenyl


R.T.: 8.615 min
Delta R.T.: -0.007 min
Response: 176487261
Conc: 41.04 ng/ml

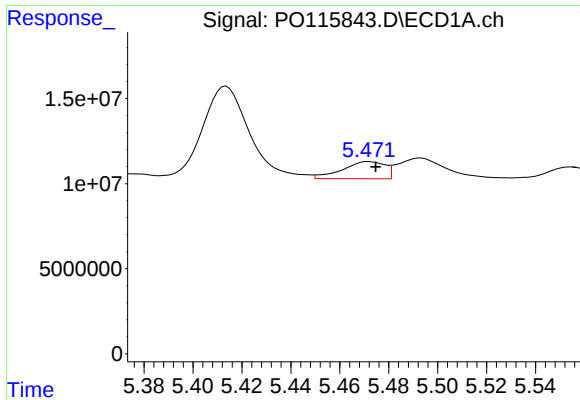

#3 AR-1016-1


R.T.: 5.472 min
Delta R.T.: -0.003 min
Response: 12174893
Conc: 48.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

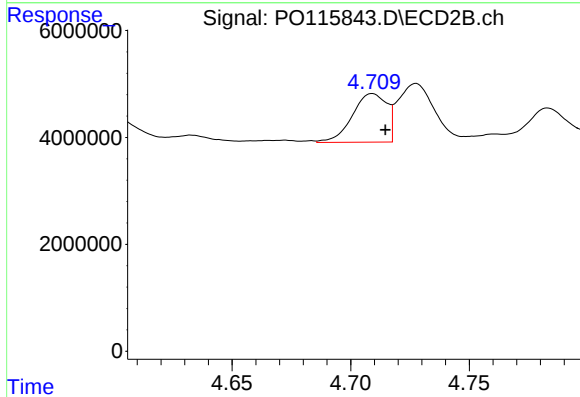


#3 AR-1016-1

R.T.: 4.709 min
Delta R.T.: -0.006 min
Response: 9201942
Conc: 49.80 ng/ml

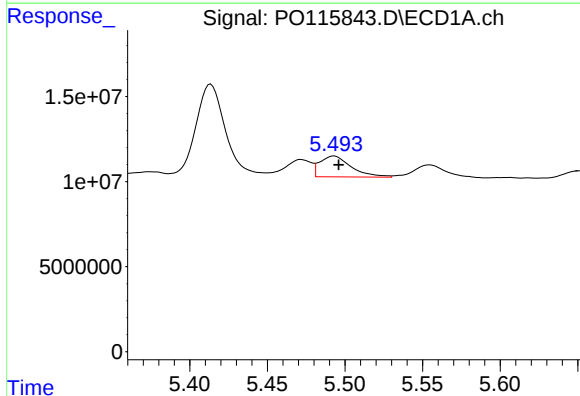


#4 AR-1016-2

R.T.: 5.493 min
Delta R.T.: -0.003 min
Response: 17388206
Conc: 45.66 ng/ml

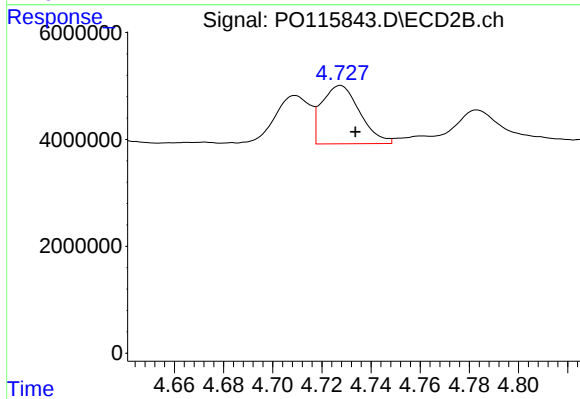

#4 AR-1016-2


R.T.: 4.728 min
Delta R.T.: -0.006 min
Response: 11713247
Conc: 44.32 ng/ml

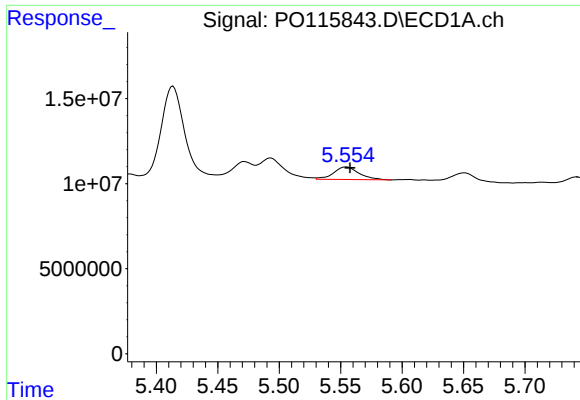

#5 AR-1016-3


R.T.: 5.555 min
Delta R.T.: -0.003 min
Response: 10789703
Conc: 50.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

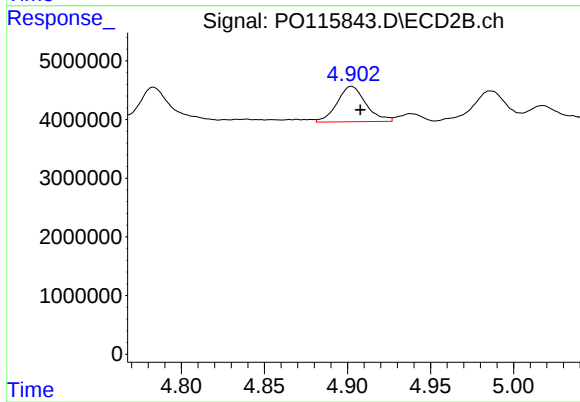


#5 AR-1016-3

R.T.: 4.902 min
Delta R.T.: -0.005 min
Response: 7297592
Conc: 48.22 ng/ml

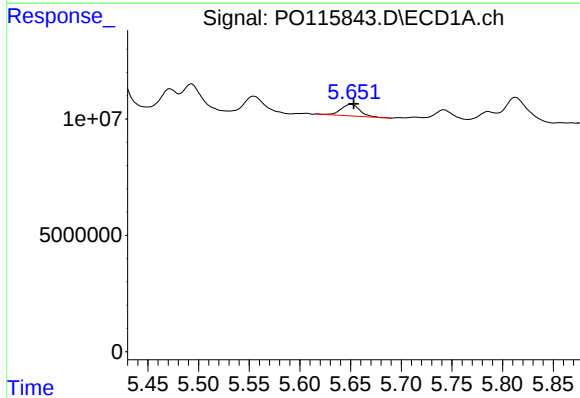


#6 AR-1016-4

R.T.: 5.651 min
Delta R.T.: -0.002 min
Response: 6439603
Conc: 36.06 ng/ml

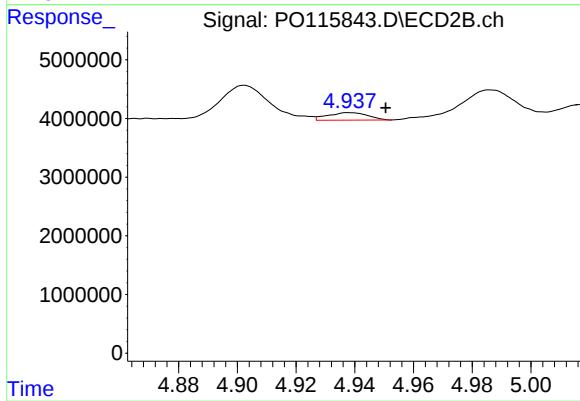

#6 AR-1016-4


R.T.: 4.938 min
Delta R.T.: -0.013 min
Response: 1218269
Conc: 10.81 ng/ml

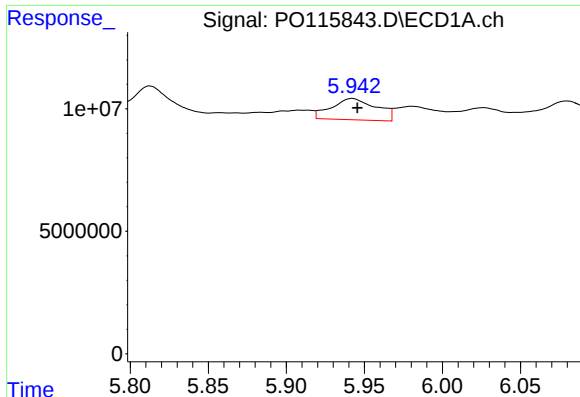

#7 AR-1016-5


R.T.: 5.942 min
Delta R.T.: -0.003 min
Response: 17407353
Conc: 99.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

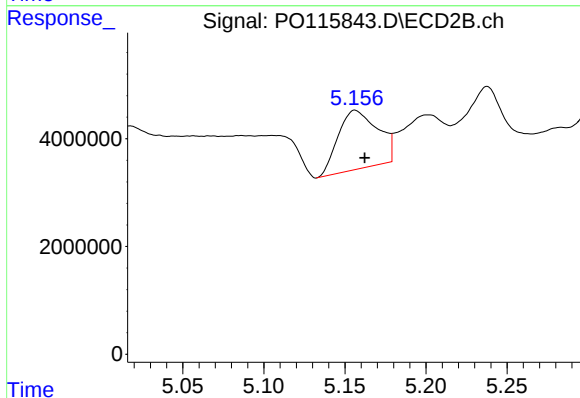


#7 AR-1016-5

R.T.: 5.156 min
Delta R.T.: -0.006 min
Response: 18483225
Conc: 126.30 ng/ml

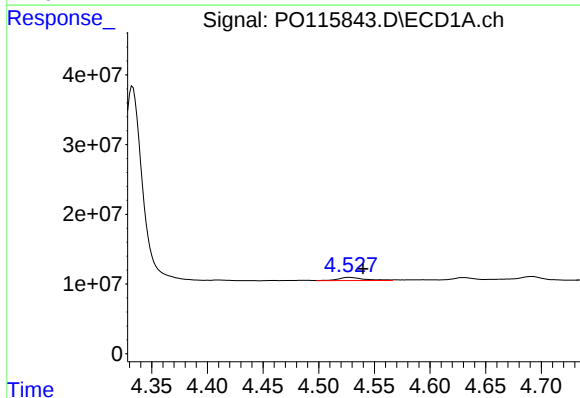


#8 AR-1221-1

R.T.: 4.527 min
Delta R.T.: -0.013 min
Response: 7624589
Conc: 93.90 ng/ml

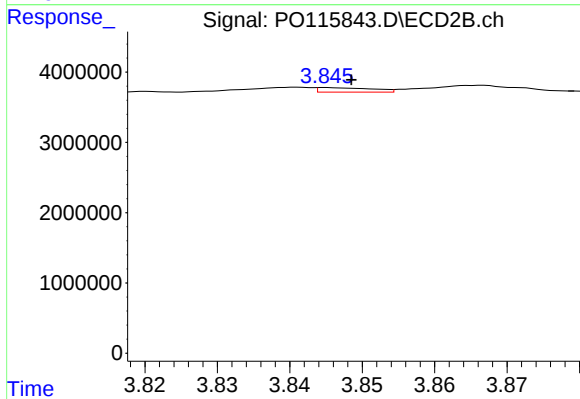

#8 AR-1221-1


R.T.: 3.845 min
Delta R.T.: -0.004 min
Response: 336454
Conc: 5.96 ng/ml

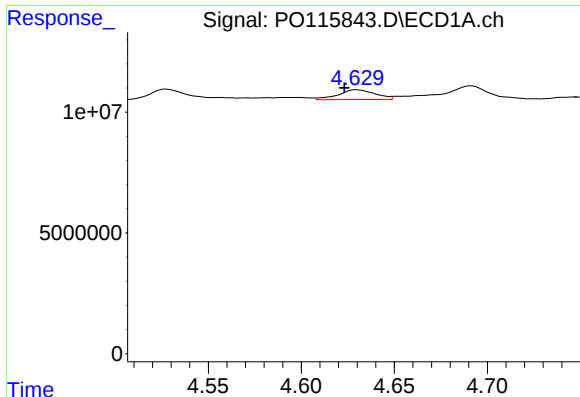

#9 AR-1221-2


R.T.: 4.630 min
Delta R.T.: 0.007 min
Response: 5634202
Conc: 89.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

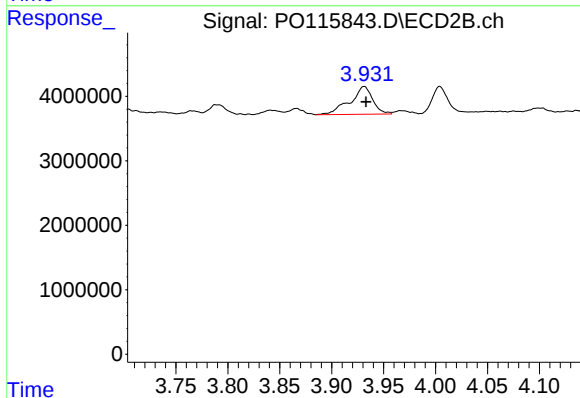


#9 AR-1221-2

R.T.: 3.931 min
Delta R.T.: -0.002 min
Response: 6544340
Conc: 154.19 ng/ml

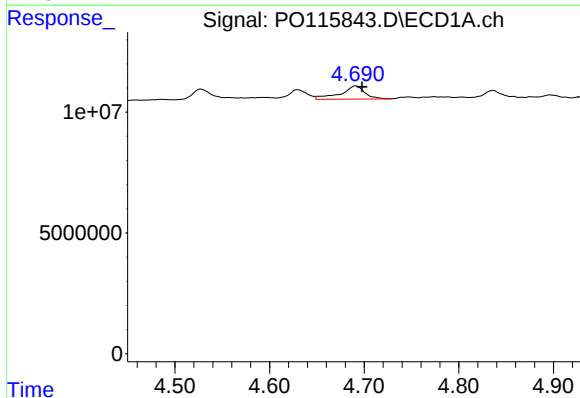


#10 AR-1221-3

R.T.: 4.691 min
Delta R.T.: -0.006 min
Response: 9880333
Conc: 52.92 ng/ml

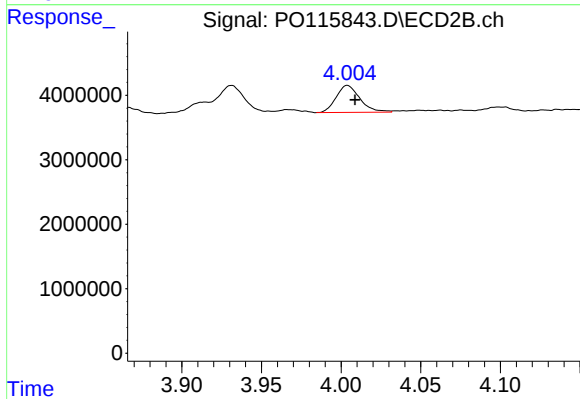

#10 AR-1221-3


R.T.: 4.004 min
Delta R.T.: -0.005 min
Response: 4353694
Conc: 33.86 ng/ml

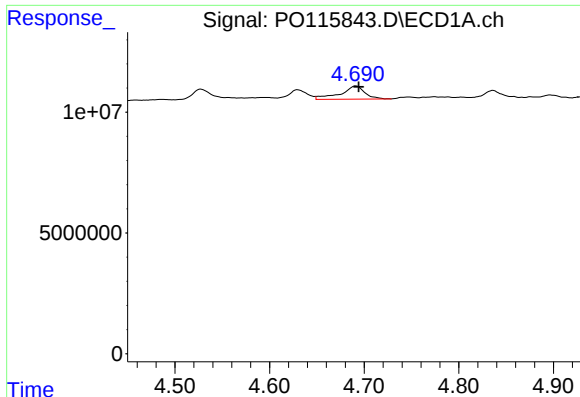

#11 AR-1232-1


R.T.: 4.691 min
Delta R.T.: -0.003 min
Response: 9880333
Conc: 66.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

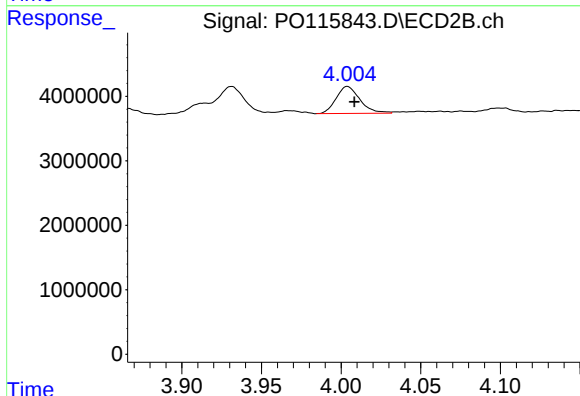


#11 AR-1232-1

R.T.: 4.004 min
Delta R.T.: -0.004 min
Response: 4353694
Conc: 40.75 ng/ml

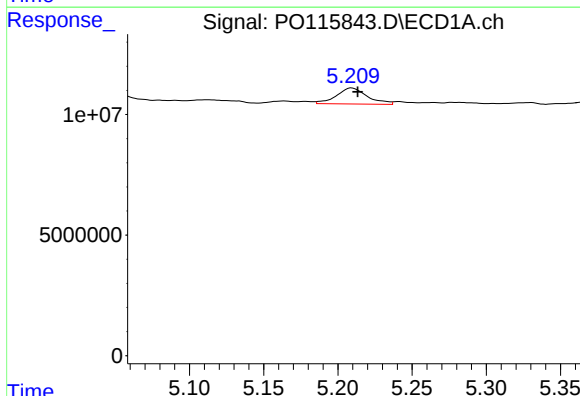


#12 AR-1232-2

R.T.: 5.209 min
Delta R.T.: -0.004 min
Response: 9586513
Conc: 118.57 ng/ml

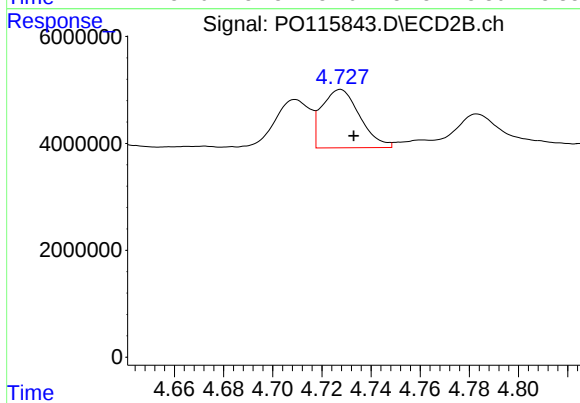

#12 AR-1232-2


R.T.: 4.728 min
Delta R.T.: -0.005 min
Response: 11713247
Conc: 105.53 ng/ml

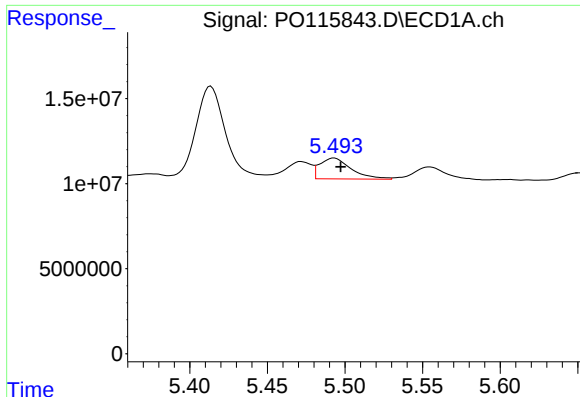

#13 AR-1232-3


R.T.: 5.493 min
Delta R.T.: -0.004 min
Response: 17388206
Conc: 112.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

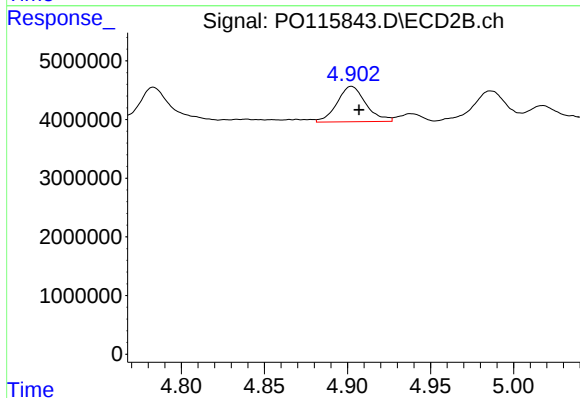


#13 AR-1232-3

R.T.: 4.902 min
Delta R.T.: -0.005 min
Response: 7297592
Conc: 111.64 ng/ml

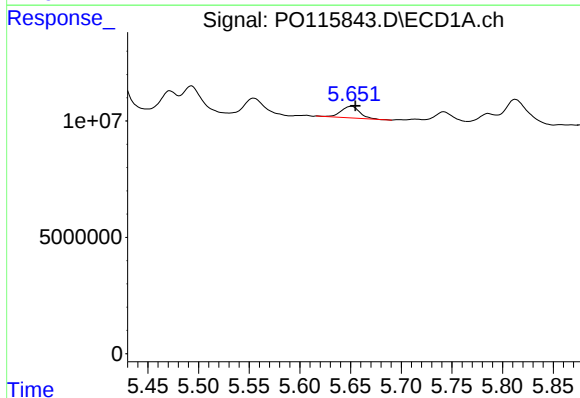


#14 AR-1232-4

R.T.: 5.651 min
Delta R.T.: -0.004 min
Response: 6439603
Conc: 91.95 ng/ml

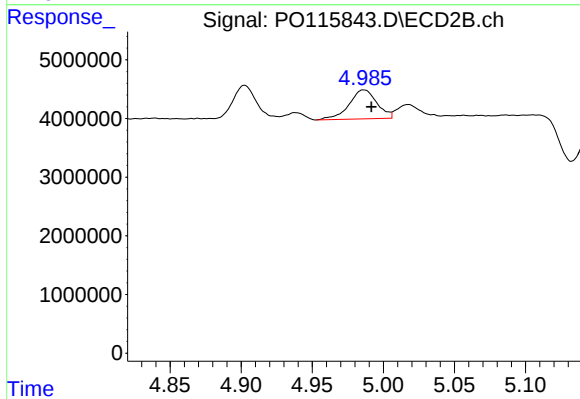

#14 AR-1232-4


R.T.: 4.986 min
Delta R.T.: -0.005 min
Response: 6725603
Conc: 131.03 ng/ml

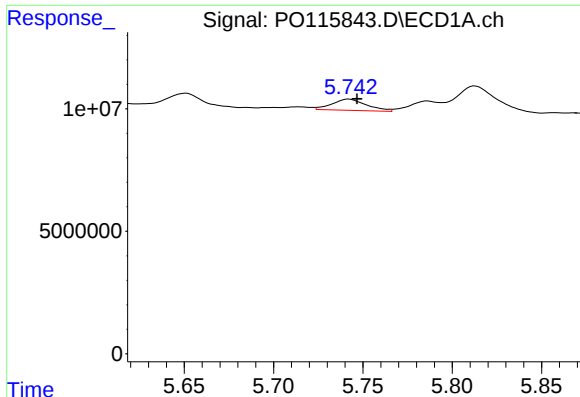

#15 AR-1232-5


R.T.: 5.742 min
Delta R.T.: -0.005 min
Response: 6185782
Conc: 119.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

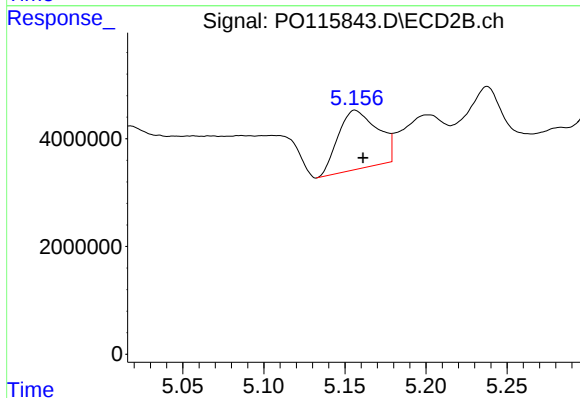


#15 AR-1232-5

R.T.: 5.156 min
Delta R.T.: -0.005 min
Response: 18483225
Conc: 337.60 ng/ml

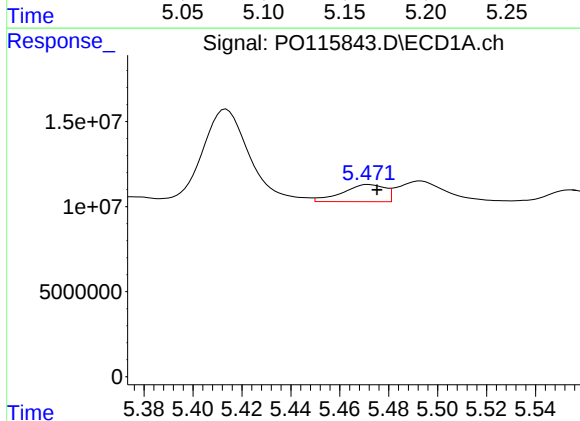


#16 AR-1242-1

R.T.: 5.472 min
Delta R.T.: -0.003 min
Response: 12174893
Conc: 61.30 ng/ml

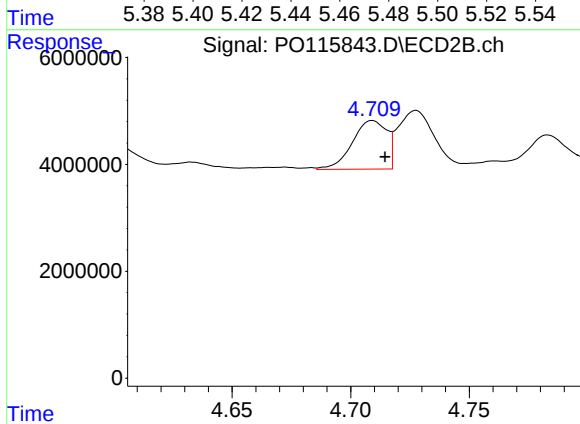

#16 AR-1242-1


R.T.: 4.709 min
Delta R.T.: -0.005 min
Response: 9201942
Conc: 64.63 ng/ml

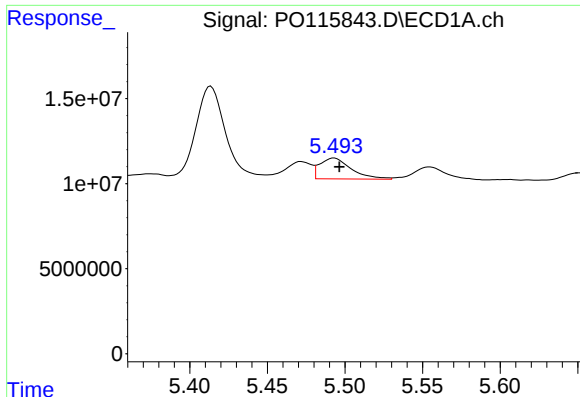

#17 AR-1242-2


R.T.: 5.493 min
Delta R.T.: -0.003 min
Response: 17388206
Conc: 59.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

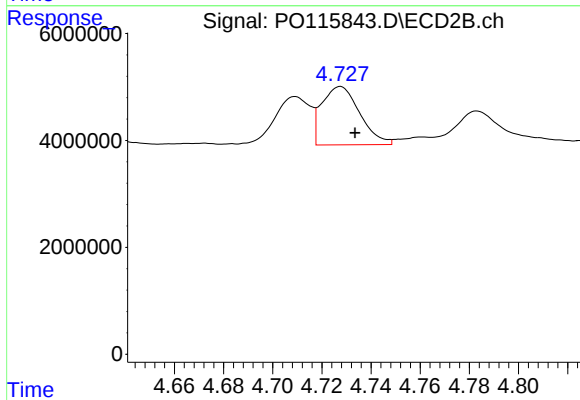


#17 AR-1242-2

R.T.: 4.728 min
Delta R.T.: -0.006 min
Response: 11713247
Conc: 55.95 ng/ml

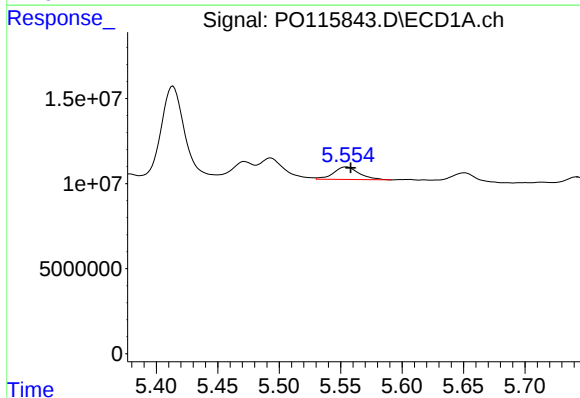


#18 AR-1242-3

R.T.: 5.555 min
Delta R.T.: -0.004 min
Response: 10789703
Conc: 63.91 ng/ml

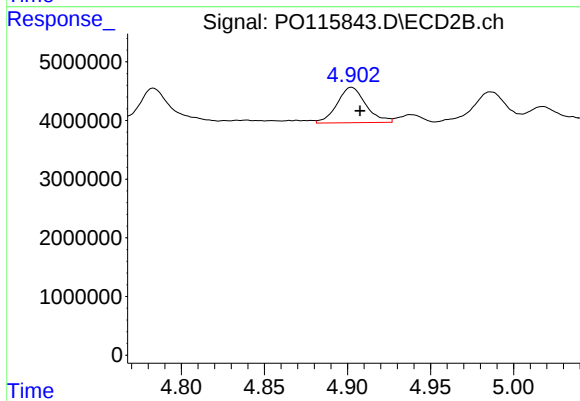

#18 AR-1242-3


R.T.: 4.902 min
Delta R.T.: -0.005 min
Response: 7297592
Conc: 61.10 ng/ml

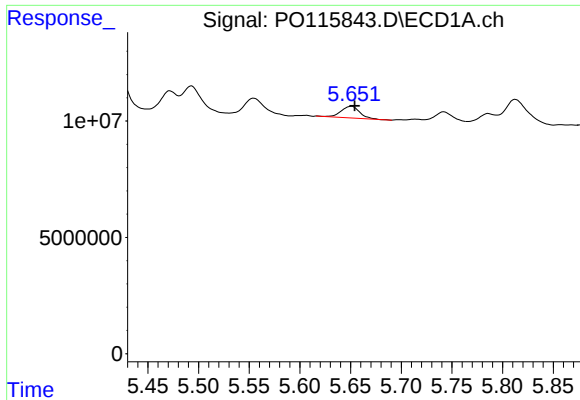

#19 AR-1242-4


R.T.: 5.651 min
Delta R.T.: -0.003 min
Response: 6439603
Conc: 47.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

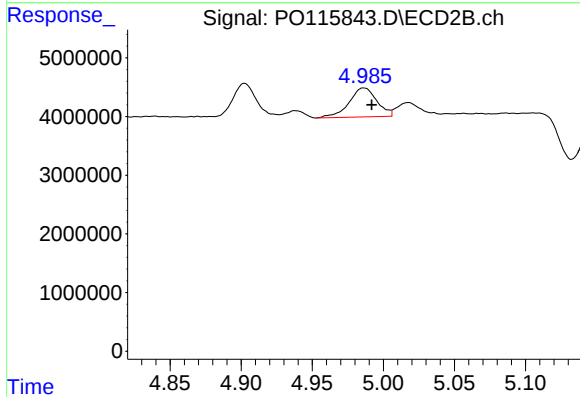


#19 AR-1242-4

R.T.: 4.986 min
Delta R.T.: -0.006 min
Response: 6725603
Conc: 61.65 ng/ml

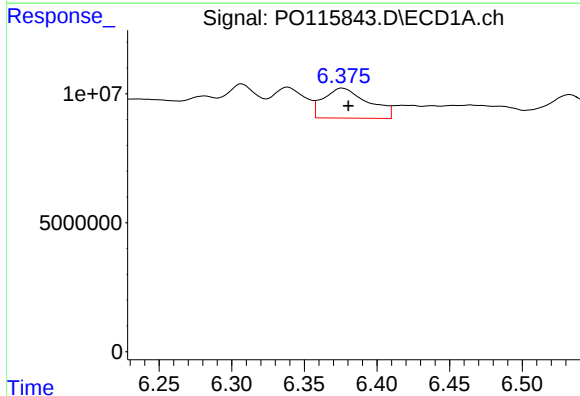


#20 AR-1242-5

R.T.: 6.376 min
Delta R.T.: -0.004 min
Response: 24865014
Conc: 164.19 ng/ml

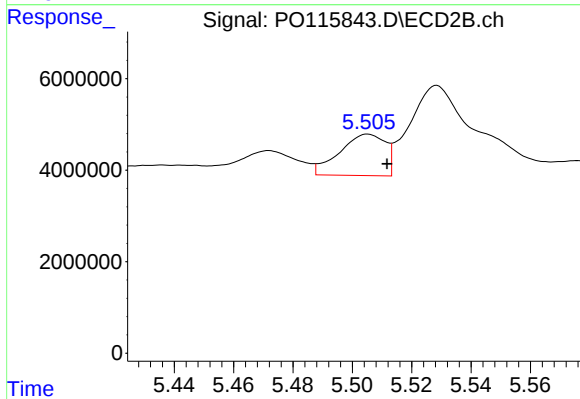

#20 AR-1242-5


R.T.: 5.505 min
Delta R.T.: -0.006 min
Response: 9688719
Conc: 70.14 ng/ml

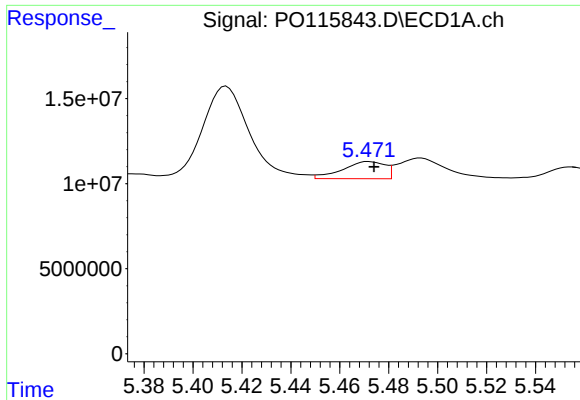

#21 AR-1248-1


R.T.: 5.472 min
Delta R.T.: -0.002 min
Response: 12174893
Conc: 80.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

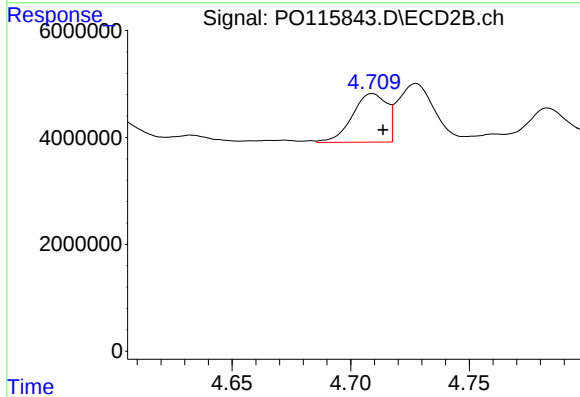


#21 AR-1248-1

R.T.: 4.709 min
Delta R.T.: -0.005 min
Response: 9201942
Conc: 82.29 ng/ml

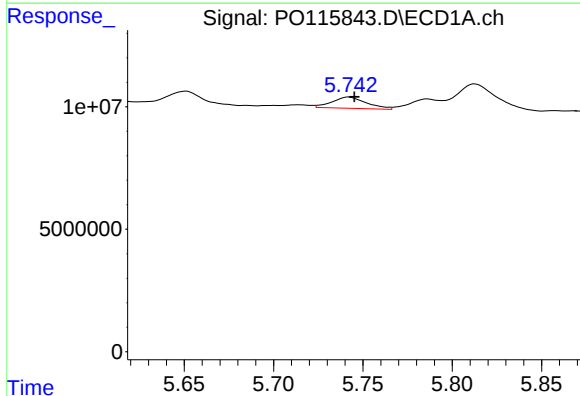


#22 AR-1248-2

R.T.: 5.742 min
Delta R.T.: -0.003 min
Response: 6185782
Conc: 30.80 ng/ml

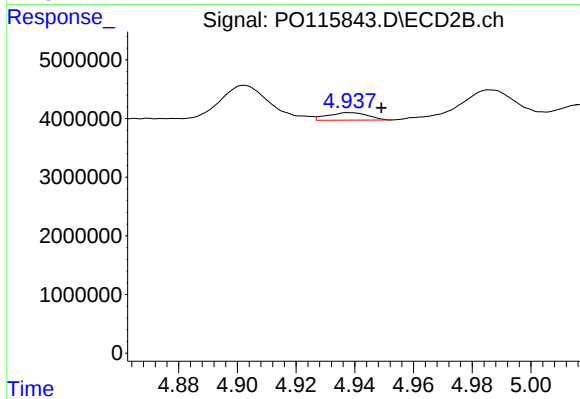

#22 AR-1248-2


R.T.: 4.938 min
Delta R.T.: -0.011 min
Response: 1218269
Conc: 8.00 ng/ml

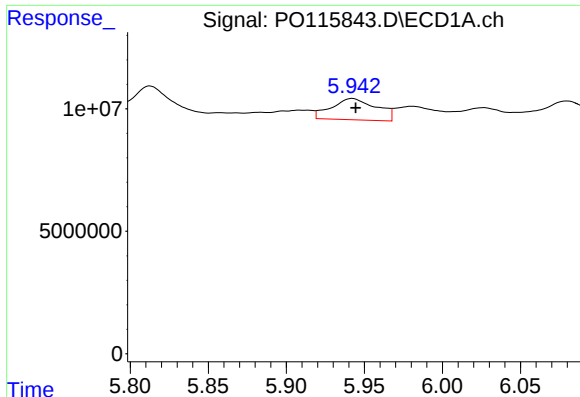

#23 AR-1248-3


R.T.: 5.942 min
Delta R.T.: -0.002 min
Response: 17407353
Conc: 70.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

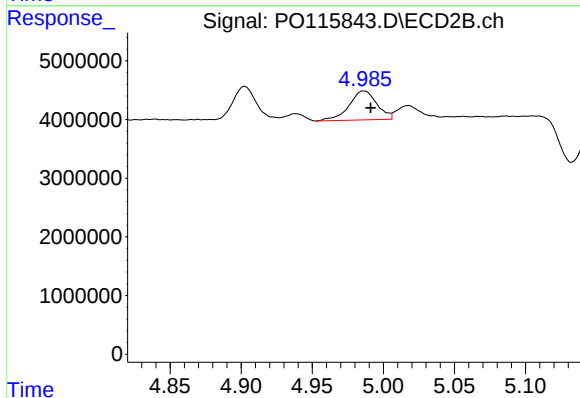


#23 AR-1248-3

R.T.: 4.986 min
Delta R.T.: -0.005 min
Response: 6725603
Conc: 41.90 ng/ml

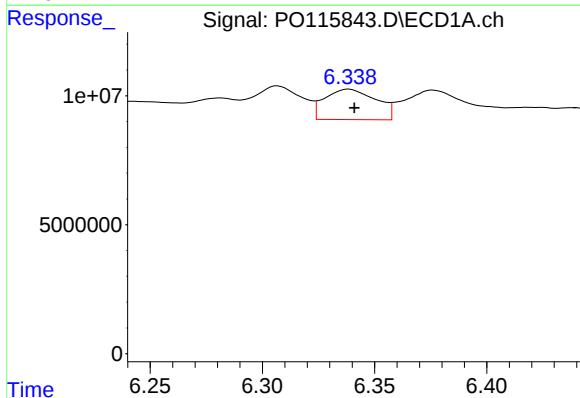


#24 AR-1248-4

R.T.: 6.339 min
Delta R.T.: -0.002 min
Response: 18716960
Conc: 63.48 ng/ml

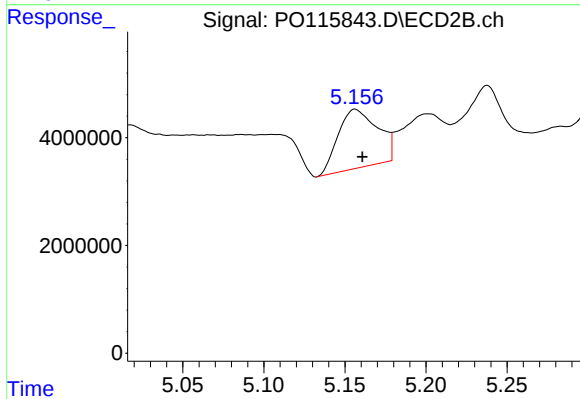

#24 AR-1248-4


R.T.: 5.156 min
Delta R.T.: -0.005 min
Response: 18483225
Conc: 98.76 ng/ml

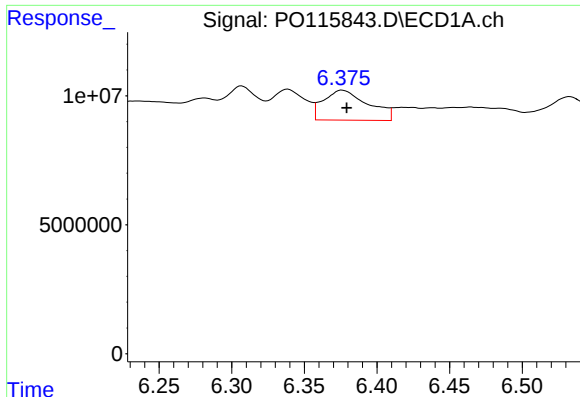

#25 AR-1248-5


R.T.: 6.376 min
Delta R.T.: -0.003 min
Response: 24865014
Conc: 96.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

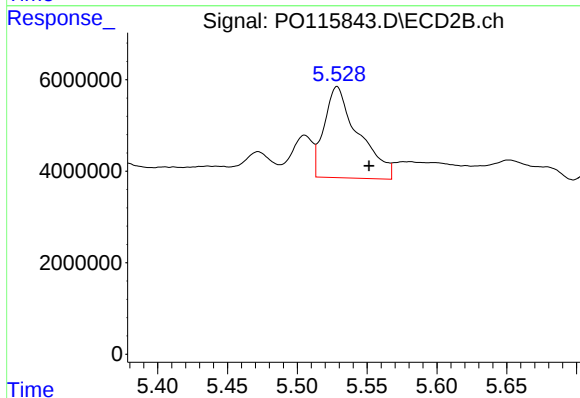


#25 AR-1248-5

R.T.: 5.528 min
Delta R.T.: -0.023 min
Response: 33923101
Conc: 171.37 ng/ml

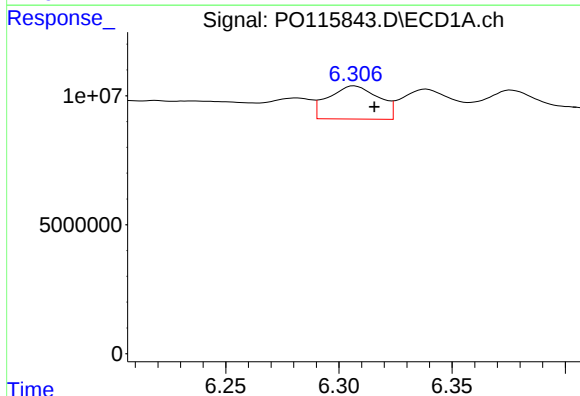


#26 AR-1254-1

R.T.: 6.307 min
Delta R.T.: -0.009 min
Response: 19872495
Conc: 76.81 ng/ml

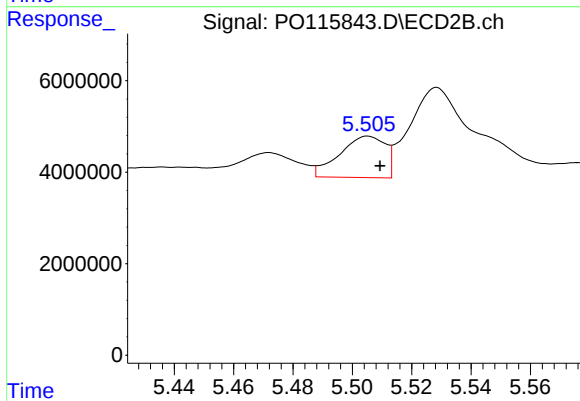

#26 AR-1254-1


R.T.: 5.505 min
Delta R.T.: -0.004 min
Response: 9688719
Conc: 33.15 ng/ml

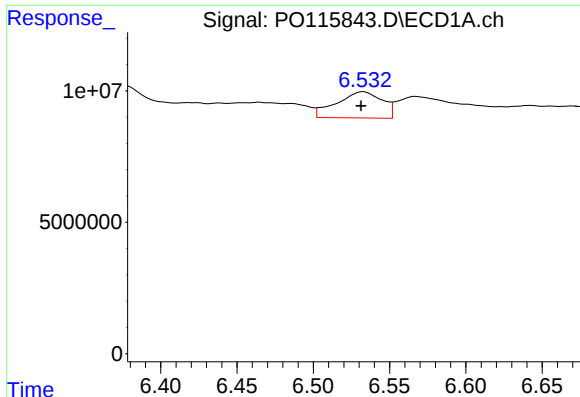

#27 AR-1254-2


R.T.: 6.533 min
Delta R.T.: 0.001 min
Response: 20732382
Conc: 51.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

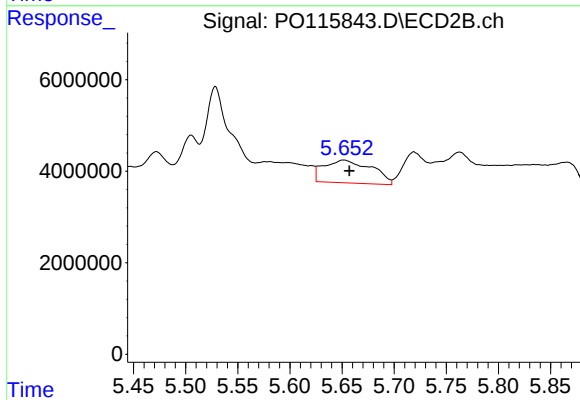


#27 AR-1254-2

R.T.: 5.652 min
Delta R.T.: -0.005 min
Response: 15883188
Conc: 63.08 ng/ml

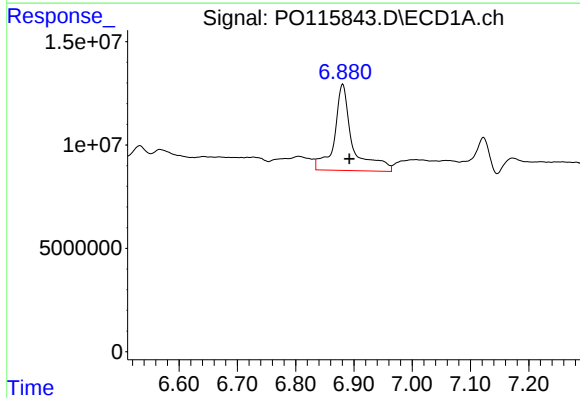


#28 AR-1254-3

R.T.: 6.881 min
Delta R.T.: -0.011 min
Response: 89857157
Conc: 218.86 ng/ml

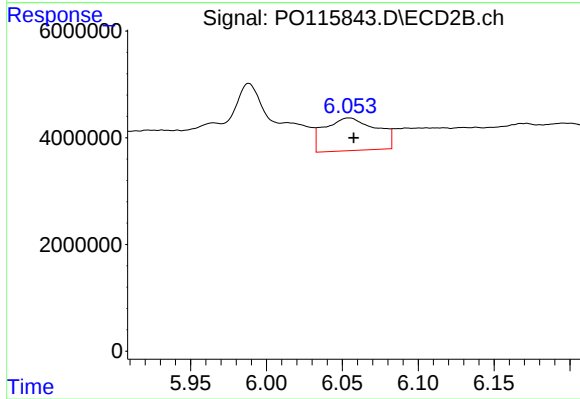

#28 AR-1254-3


R.T.: 6.054 min
Delta R.T.: -0.003 min
Response: 14555558
Conc: 36.98 ng/ml

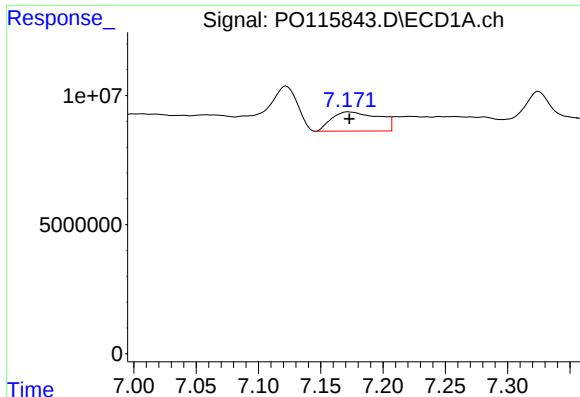

#29 AR-1254-4


R.T.: 7.172 min
Delta R.T.: -0.001 min
Response: 19608719
Conc: 56.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

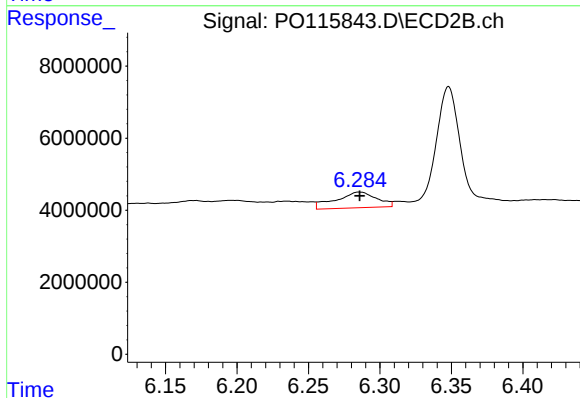


#29 AR-1254-4

R.T.: 6.286 min
Delta R.T.: 0.000 min
Response: 8752072
Conc: 32.71 ng/ml

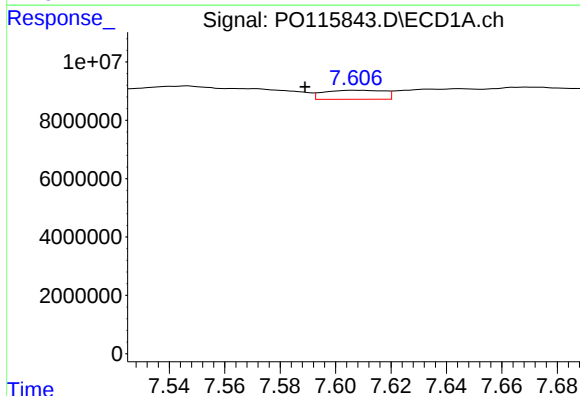


#30 AR-1254-5

R.T.: 7.607 min
Delta R.T.: 0.018 min
Response: 4671928
Conc: 14.42 ng/ml

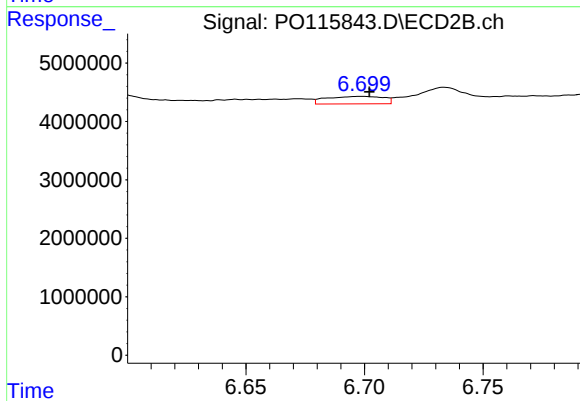

#30 AR-1254-5


R.T.: 6.699 min
Delta R.T.: -0.003 min
Response: 2157849
Conc: 6.04 ng/ml

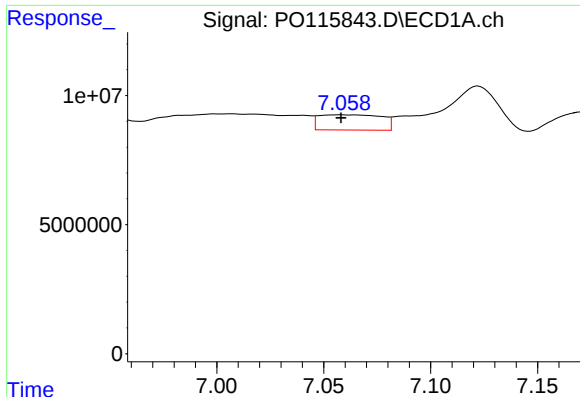

#31 AR-1260-1


R.T.: 7.058 min
Delta R.T.: 0.000 min
Response: 12003174
Conc: 41.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

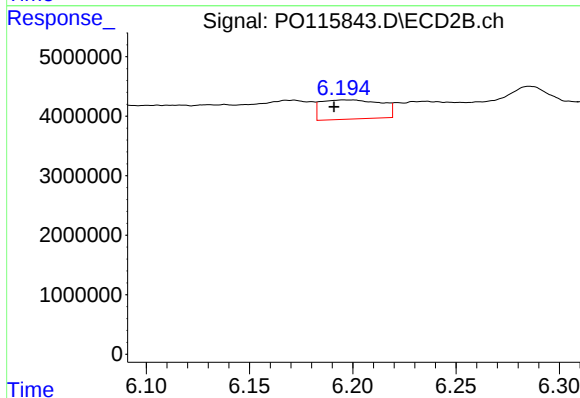


#31 AR-1260-1

R.T.: 6.196 min
Delta R.T.: 0.005 min
Response: 6537446
Conc: 24.94 ng/ml

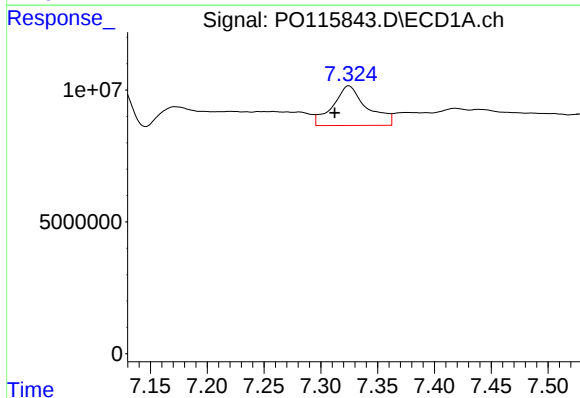


#32 AR-1260-2

R.T.: 7.325 min
Delta R.T.: 0.013 min
Response: 31424081
Conc: 71.79 ng/ml

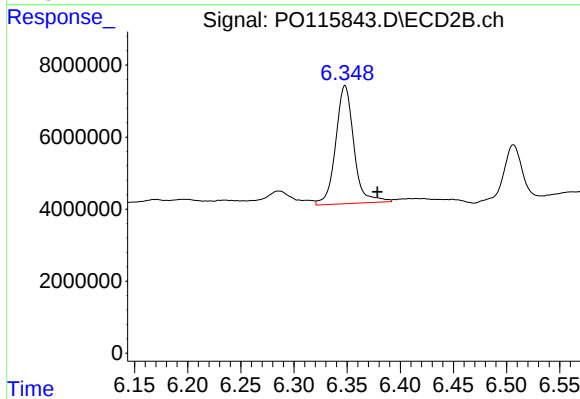

#32 AR-1260-2


R.T.: 6.348 min
Delta R.T.: -0.030 min
Response: 39077159
Conc: 111.50 ng/ml

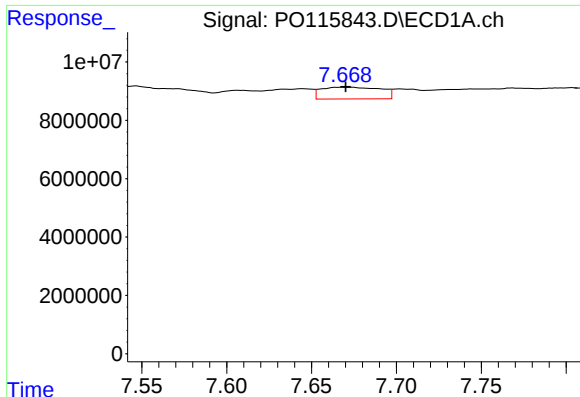

#33 AR-1260-3


R.T.: 7.669 min
Delta R.T.: 0.000 min
Response: 9836073
Conc: 29.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

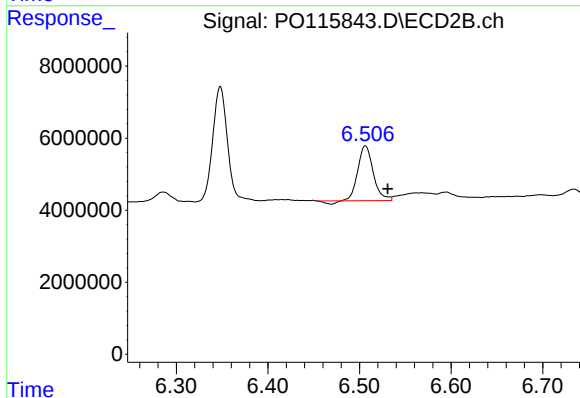


#33 AR-1260-3

R.T.: 6.506 min
Delta R.T.: -0.024 min
Response: 17408350
Conc: 54.19 ng/ml

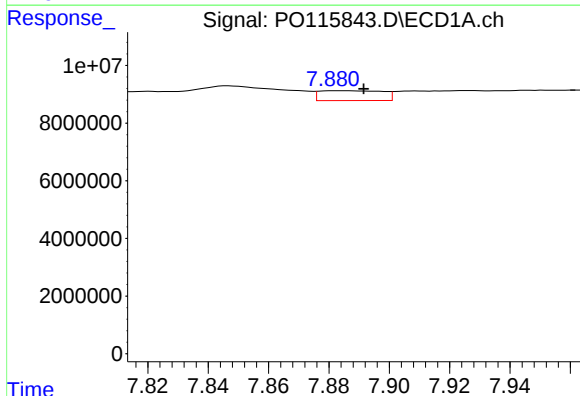


#34 AR-1260-4

R.T.: 7.882 min
Delta R.T.: -0.009 min
Response: 4963598
Conc: 16.14 ng/ml

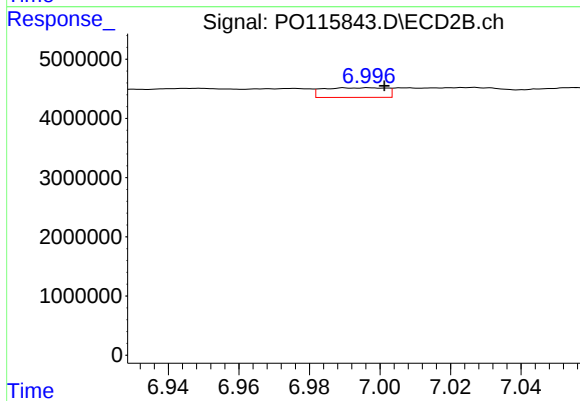

#34 AR-1260-4


R.T.: 6.997 min
Delta R.T.: -0.004 min
Response: 2023443
Conc: 7.88 ng/ml

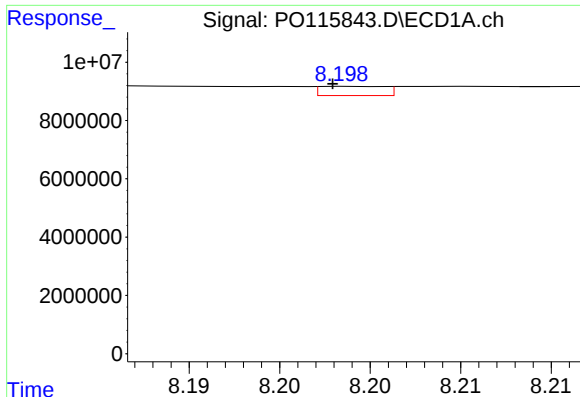

#35 AR-1260-5


R.T.: 8.199 min
Delta R.T.: 0.000 min
Response: 792637
Conc: 1.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

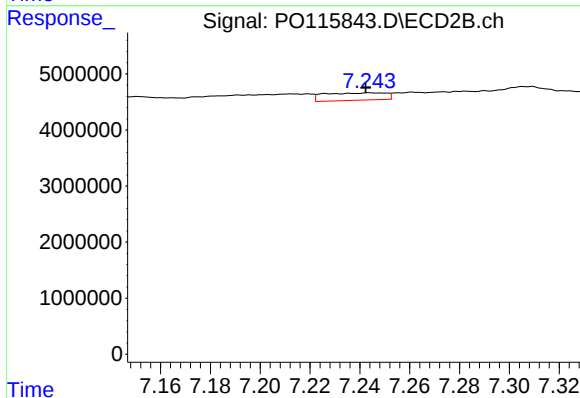


#35 AR-1260-5

R.T.: 7.244 min
Delta R.T.: 0.001 min
Response: 2248425
Conc: 3.21 ng/ml

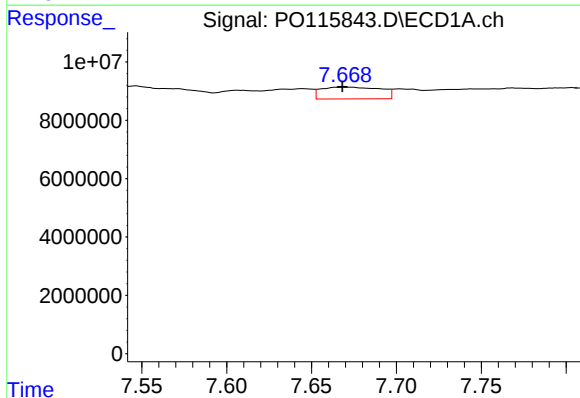


#36 AR-1262-1

R.T.: 7.669 min
Delta R.T.: 0.000 min
Response: 9836073
Conc: 39.85 ng/ml

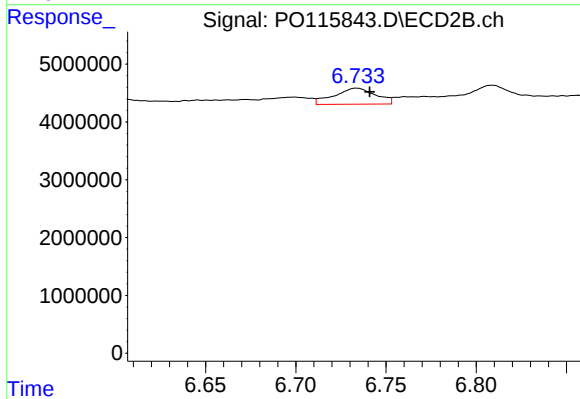

#36 AR-1262-1


R.T.: 6.734 min
Delta R.T.: -0.007 min
Response: 4442568
Conc: 20.85 ng/ml

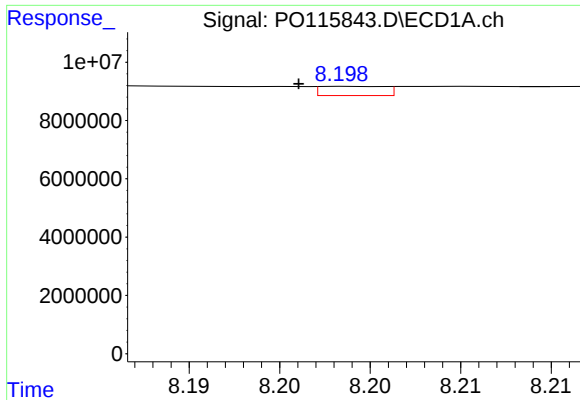

#37 AR-1262-2


R.T.: 8.199 min
Delta R.T.: 0.003 min
Response: 792637
Conc: 2.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

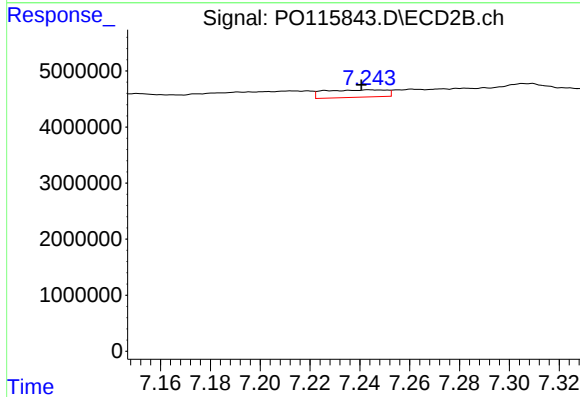


#37 AR-1262-2

R.T.: 7.244 min
Delta R.T.: 0.003 min
Response: 2248425
Conc: 6.45 ng/ml

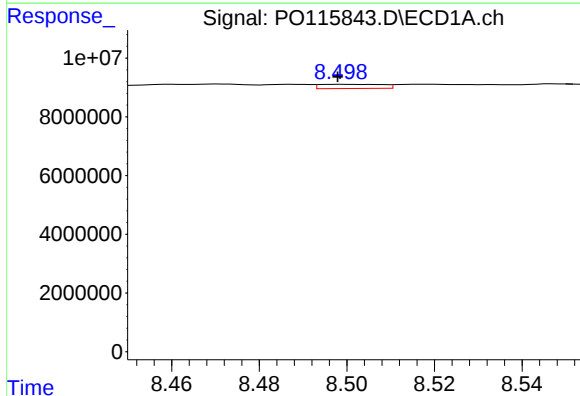


#38 AR-1262-3

R.T.: 8.498 min
Delta R.T.: 0.000 min
Response: 1432436
Conc: 5.62 ng/ml

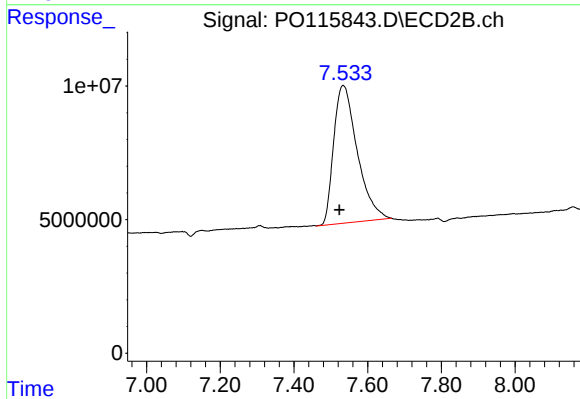

#38 AR-1262-3


R.T.: 7.533 min
Delta R.T.: 0.010 min
Response: 228647125
Conc: 1462.03 ng/ml

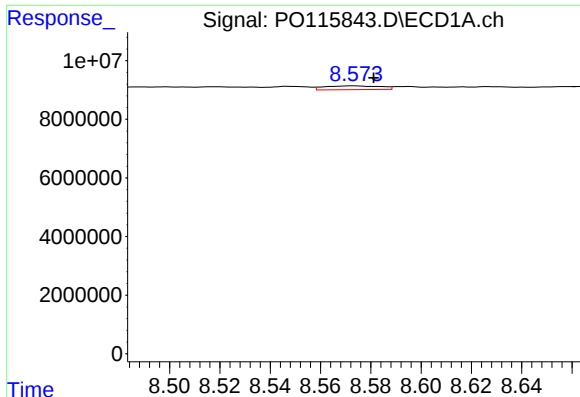

#39 AR-1262-4


R.T.: 8.573 min
Delta R.T.: -0.008 min
Response: 1979443
Conc: 10.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

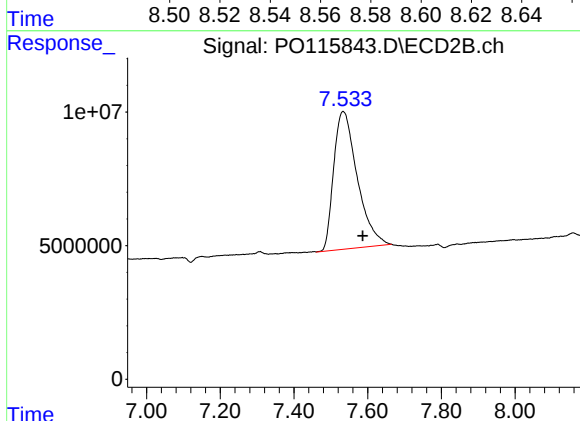


#39 AR-1262-4

R.T.: 7.533 min
Delta R.T.: -0.054 min
Response: 228647125
Conc: 924.31 ng/ml

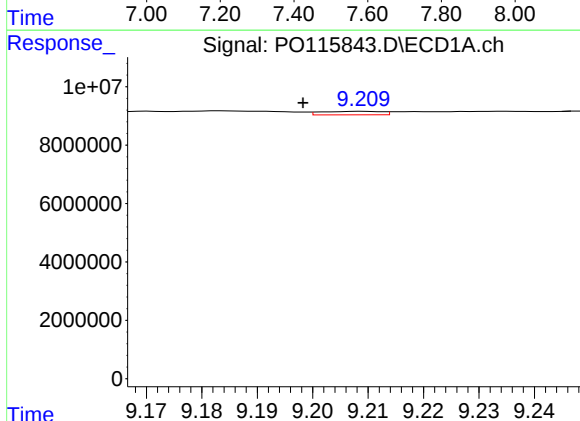


#40 AR-1262-5

R.T.: 9.209 min
Delta R.T.: 0.011 min
Response: 913478
Conc: 6.78 ng/ml

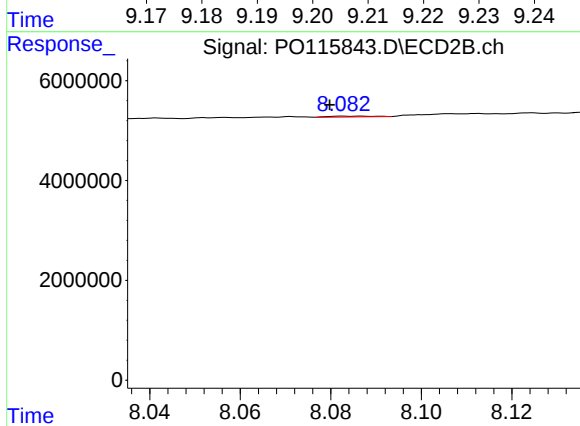

#40 AR-1262-5


R.T.: 8.083 min
Delta R.T.: 0.003 min
Response: 108232
Conc: 0.97 ng/ml

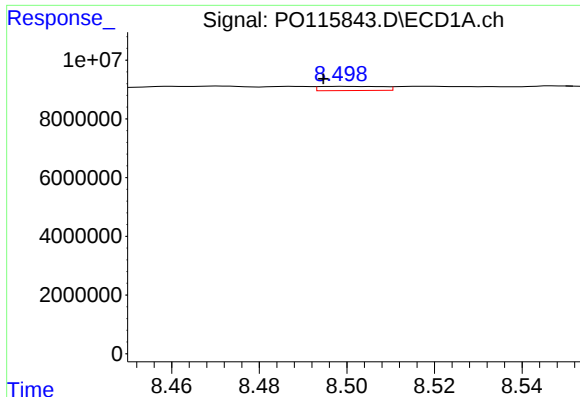

#41 AR-1268-1


R.T.: 8.498 min
Delta R.T.: 0.004 min
Response: 1432436
Conc: 1.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

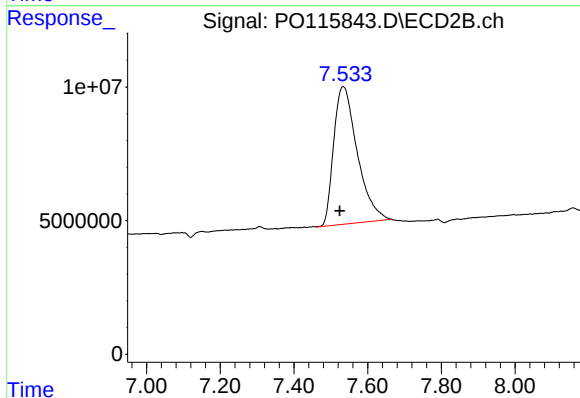


#41 AR-1268-1

R.T.: 7.533 min
Delta R.T.: 0.009 min
Response: 228647125
Conc: 258.08 ng/ml

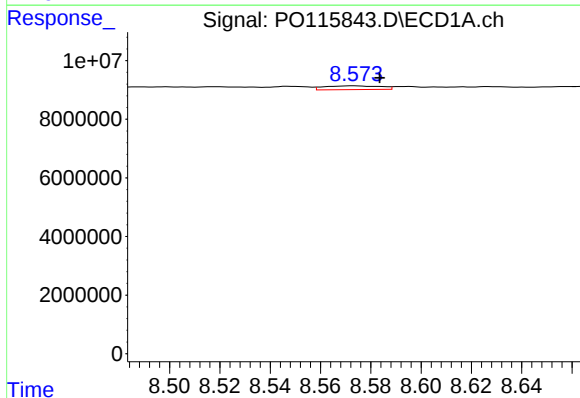


#42 AR-1268-2

R.T.: 8.573 min
Delta R.T.: -0.010 min
Response: 1979443
Conc: 2.31 ng/ml

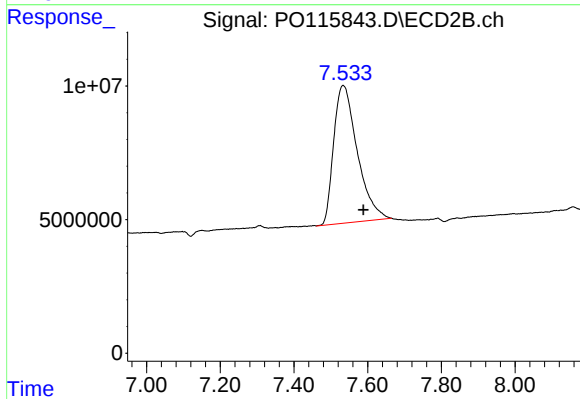

#42 AR-1268-2


R.T.: 7.533 min
Delta R.T.: -0.055 min
Response: 228647125
Conc: 305.24 ng/ml

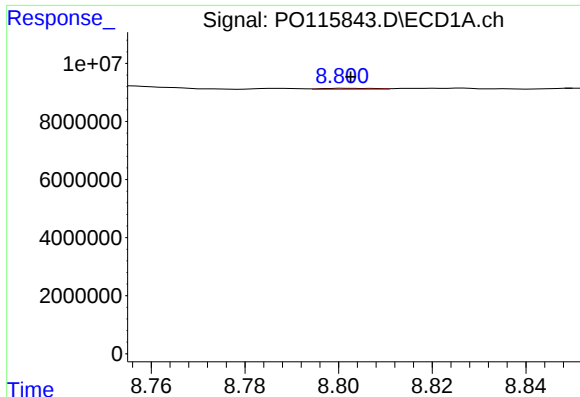

#43 AR-1268-3


R.T.: 8.801 min
Delta R.T.: -0.001 min
Response: 248811
Conc: 0.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

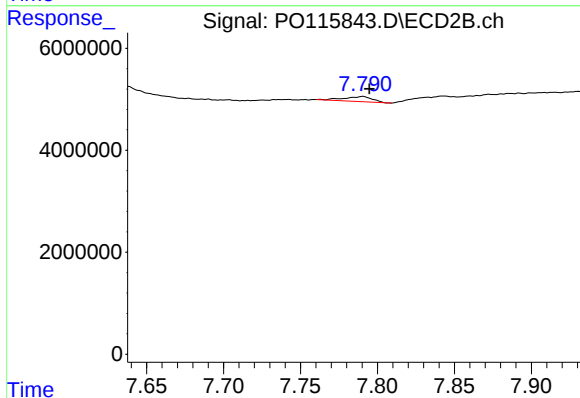


#43 AR-1268-3

R.T.: 7.790 min
Delta R.T.: -0.004 min
Response: 1245784
Conc: 1.96 ng/ml

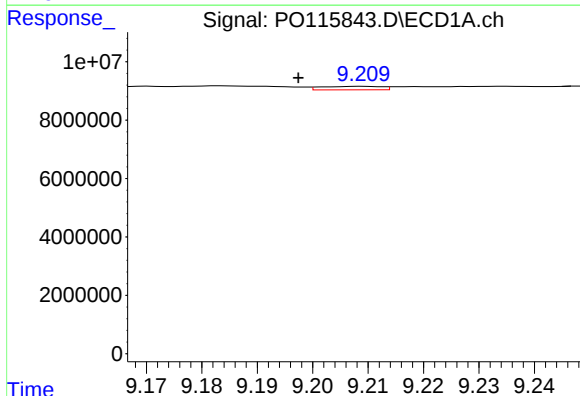


#44 AR-1268-4

R.T.: 9.209 min
Delta R.T.: 0.012 min
Response: 913478
Conc: 2.93 ng/ml

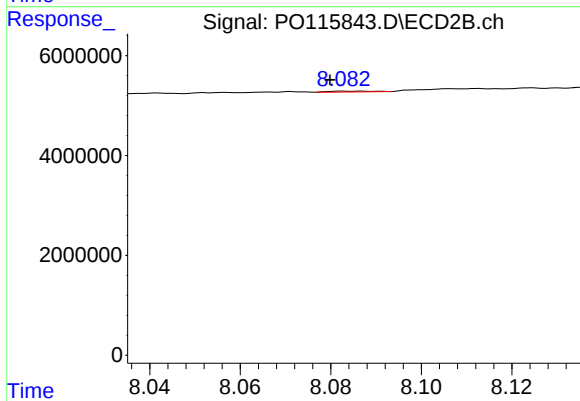

#44 AR-1268-4


R.T.: 8.083 min
Delta R.T.: 0.003 min
Response: 108232
Conc: 0.42 ng/ml

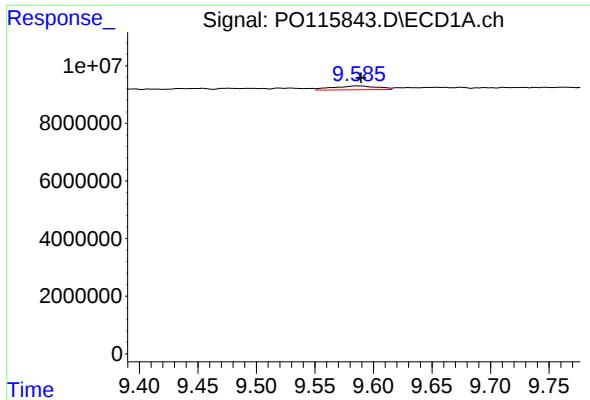

#45 AR-1268-5

R.T.: 9.586 min
Delta R.T.: -0.003 min
Response: 3651911
Conc: 1.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

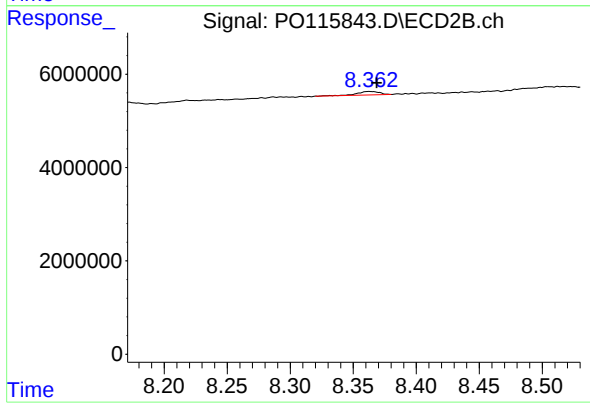

#45 AR-1268-5

R.T.: 8.363 min
Delta R.T.: -0.006 min
Response: 908232
Conc: 0.54 ng/ml