

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121225\
 Data File : PO115844.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Dec 2025 10:19
 Operator : YP/AJ
 Sample : Q3530-09
 Misc : AR1248 25PPB WATER MDL
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT4-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 02:45:15 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 05 02:11:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.333	3.634	194.1E6	118.8E6	24.995	24.378
2)	SA Decachlor...	9.907	8.615	133.3E6	100.4E6	25.343	23.354
Target Compounds							
3)	L1 AR-1016-1	5.471	4.709	7551280	4206773	30.368	22.768 #
4)	L1 AR-1016-2	5.495	4.727	8834607	3665471	23.198	13.868 #
5)	L1 AR-1016-3	5.555	4.903	4619669	2791448	21.609	18.445
6)	L1 AR-1016-4	5.648	4.941	2054863	2067009	11.507	18.340 #
7)	L1 AR-1016-5	5.942	5.156	11136399	15774723	63.482	107.794 #
8)	L2 AR-1221-1	4.528	3.843	7244584	32013	89.222	0.568 #
9)	L2 AR-1221-2	4.628	3.934	3123348	3057958	49.562	72.047 #
10)	L2 AR-1221-3	4.692	4.008	1573534	324177	8.427	2.521 #
11)	L3 AR-1232-1	4.692	4.008	1573534	324177	10.514	3.034 #
12)	L3 AR-1232-2	5.210	4.727	6462450	3665471	79.931	33.025 #
13)	L3 AR-1232-3	5.495	4.903	8834607	2791448	57.404	42.705 #
14)	L3 AR-1232-4	5.648	4.986	2054863	5324696	29.342	103.734 #
15)	L3 AR-1232-5	5.742	5.156	5102335	15774723	98.241	288.133 #
16)	L4 AR-1242-1	5.471	4.709	7551280	4206773	38.018	29.544
17)	L4 AR-1242-2	5.495	4.727	8834607	3665471	30.163	17.508 #
18)	L4 AR-1242-3	5.555	4.903	4619669	2791448	27.365	23.371
19)	L4 AR-1242-4	5.648	4.986	2054863	5324696	15.035	48.809 #
20)	L4 AR-1242-5	6.376	5.505	18717810	9284032	123.596	67.215 #
21)	L5 AR-1248-1	5.471	4.709	7551280	4206773	49.756	37.618
22)	L5 AR-1248-2	5.742	4.941	5102335	2067009	25.408	13.573 #
23)	L5 AR-1248-3	5.942	4.986	11136399	5324696	45.160	33.170 #
24)	L5 AR-1248-4	6.339	5.156	14880944	15774723	50.469	84.291 #
25)	L5 AR-1248-5	6.376	5.529	18717810	27904493	72.290	140.964 #
26)	L6 AR-1254-1	6.310	5.505	20034577	9284032	77.440	31.765 #
27)	L6 AR-1254-2	6.531	5.653	16182225	8597987	40.214	34.144
28)	L6 AR-1254-3	6.881	6.054	54212441	11673469	132.043	29.660 #
29)	L6 AR-1254-4	7.172	6.284	15029040	7329785	43.303	27.393 #
30)	L6 AR-1254-5	7.606	6.697	2133112	2078166	6.583	5.813
31)	L7 AR-1260-1	7.057	6.198	5555425	4895755	19.177	18.674
32)	L7 AR-1260-2	7.325	6.398	9885816	215719	22.584	0.616 #
33)	L7 AR-1260-3	7.678	6.531	2390364	577110	7.102	1.796 #
34)	L7 AR-1260-4	7.892	7.003	1209636	572519	3.934	2.229 #
35)	L7 AR-1260-5	8.193	7.240	3124468	581061	4.289	0.829 #
36)	L8 AR-1262-1	7.678	6.734	2390364	1997906	9.683	9.378
37)	L8 AR-1262-2	8.193	7.240	3124468	581061	7.892	1.668 #
38)	L8 AR-1262-3	8.510	7.531	653785	148.2E6	2.566	947.405 #
39)	L8 AR-1262-4	8.571	7.531f	850608	148.2E6	4.391	598.958 #
40)	L8 AR-1262-5	9.199	8.079	696272	196241	5.169	1.760 #
41)	L9 AR-1268-1	8.510	7.531	653785	148.2E6	0.657	167.238 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121225\
Data File : PO115844.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Dec 2025 10:19
Operator : YP/AJ
Sample : Q3530-09
Misc : AR1248 25PPB WATER MDL
ALS Vial : 23 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 02:45:15 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120425.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 05 02:11:05 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.593	7.531f	278534	148.2E6	0.326	197.799 #
43)	L9 AR-1268-3	8.808	7.793	104341	521707	0.140	0.819 #
44)	L9 AR-1268-4	9.199	8.079	696272	196241	2.230	0.762 #
45)	L9 AR-1268-5	9.588	8.368	1417644	528472	0.651	0.313 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

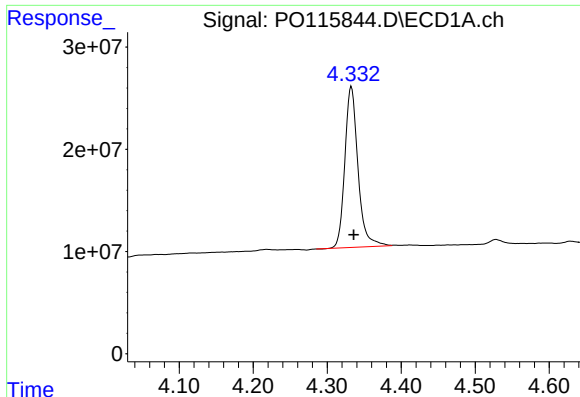

#1 Tetrachloro-m-xylene


R.T.: 4.333 min
Delta R.T.: -0.003 min
Response: 194138926
Conc: 24.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

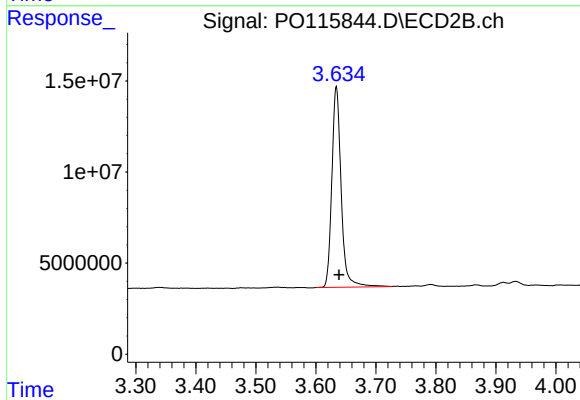


#1 Tetrachloro-m-xylene

R.T.: 3.634 min
Delta R.T.: -0.004 min
Response: 118803402
Conc: 24.38 ng/ml

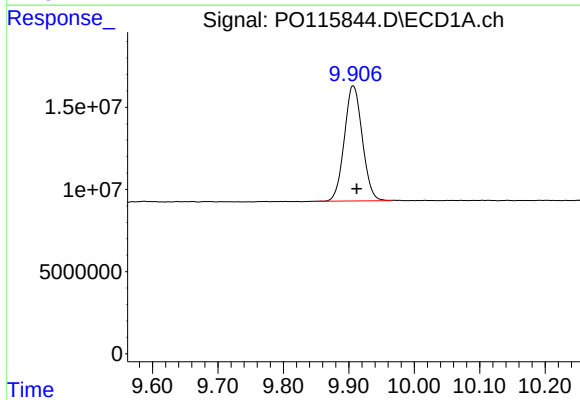


#2 Decachlorobiphenyl

R.T.: 9.907 min
Delta R.T.: -0.005 min
Response: 133330230
Conc: 25.34 ng/ml

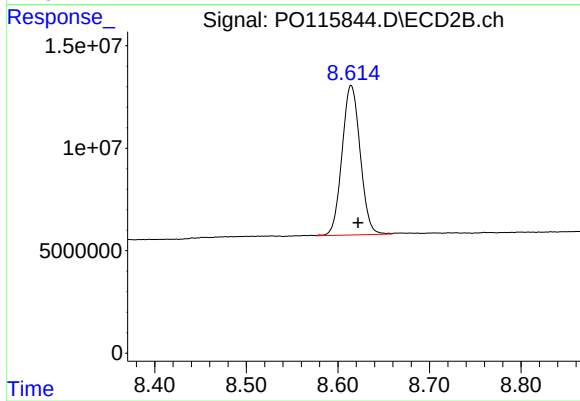

#2 Decachlorobiphenyl


R.T.: 8.615 min
Delta R.T.: -0.008 min
Response: 100426184
Conc: 23.35 ng/ml

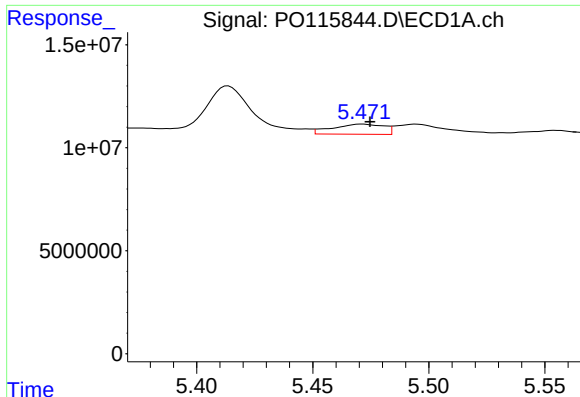

#3 AR-1016-1


R.T.: 5.471 min
Delta R.T.: -0.003 min
Response: 7551280
Conc: 30.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

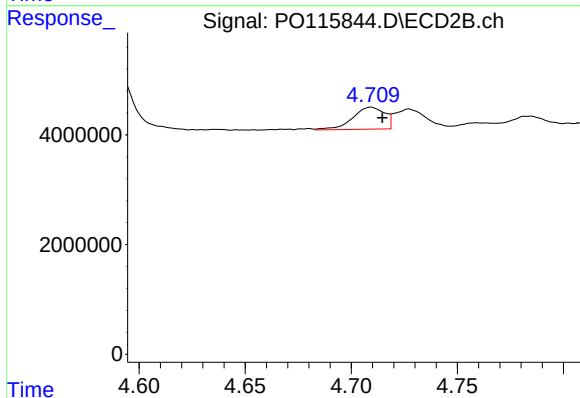


#3 AR-1016-1

R.T.: 4.709 min
Delta R.T.: -0.005 min
Response: 4206773
Conc: 22.77 ng/ml

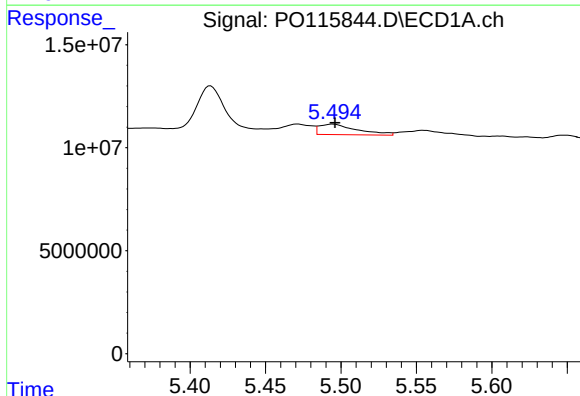


#4 AR-1016-2

R.T.: 5.495 min
Delta R.T.: -0.001 min
Response: 8834607
Conc: 23.20 ng/ml

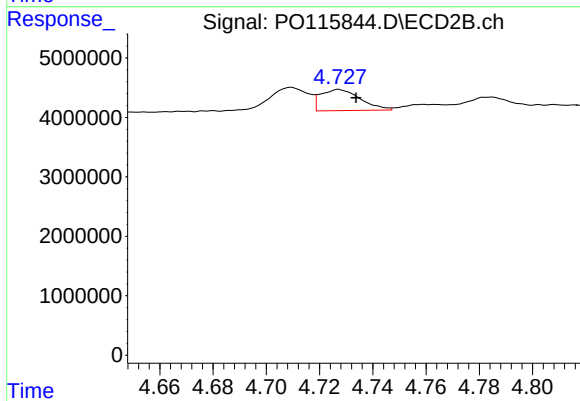

#4 AR-1016-2


R.T.: 4.727 min
Delta R.T.: -0.006 min
Response: 3665471
Conc: 13.87 ng/ml

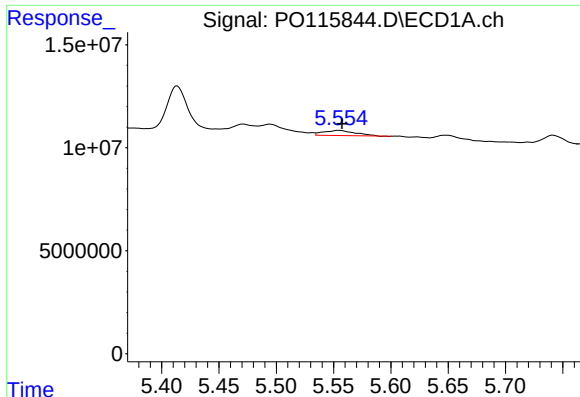

#5 AR-1016-3


R.T.: 5.555 min
Delta R.T.: -0.002 min
Response: 4619669
Conc: 21.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

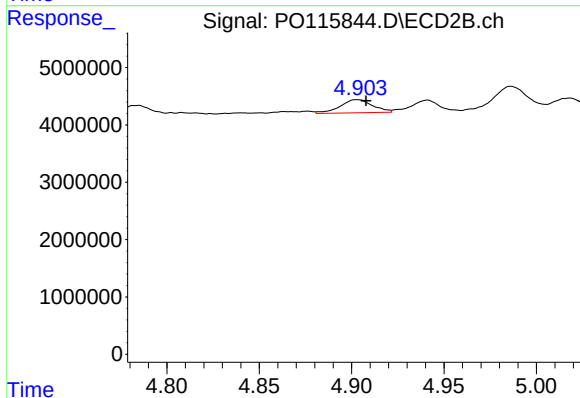


#5 AR-1016-3

R.T.: 4.903 min
Delta R.T.: -0.005 min
Response: 2791448
Conc: 18.45 ng/ml

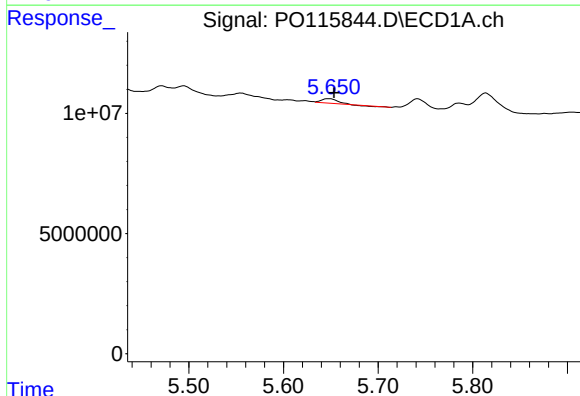


#6 AR-1016-4

R.T.: 5.648 min
Delta R.T.: -0.005 min
Response: 2054863
Conc: 11.51 ng/ml

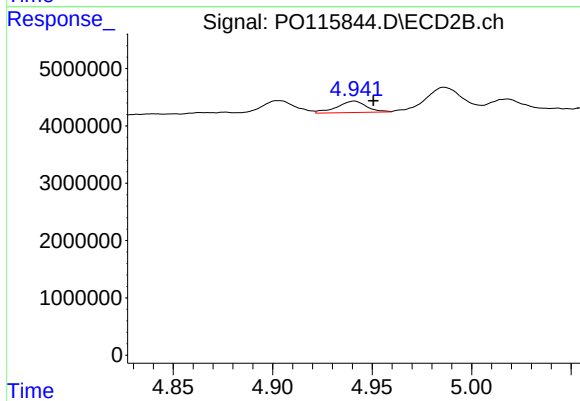

#6 AR-1016-4


R.T.: 4.941 min
Delta R.T.: -0.009 min
Response: 2067009
Conc: 18.34 ng/ml

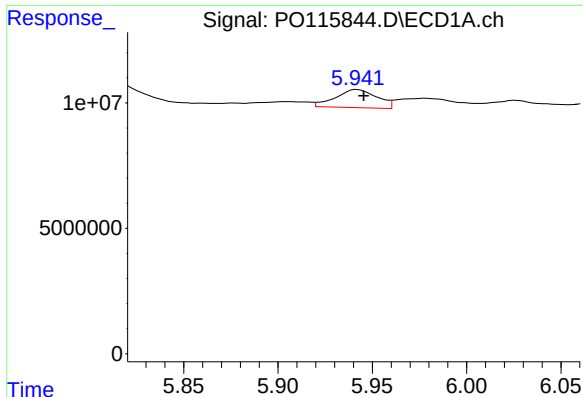

#7 AR-1016-5


R.T.: 5.942 min
Delta R.T.: -0.004 min
Response: 11136399
Conc: 63.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

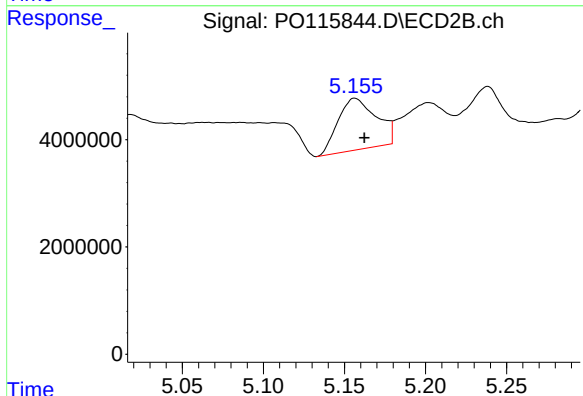


#7 AR-1016-5

R.T.: 5.156 min
Delta R.T.: -0.006 min
Response: 15774723
Conc: 107.79 ng/ml

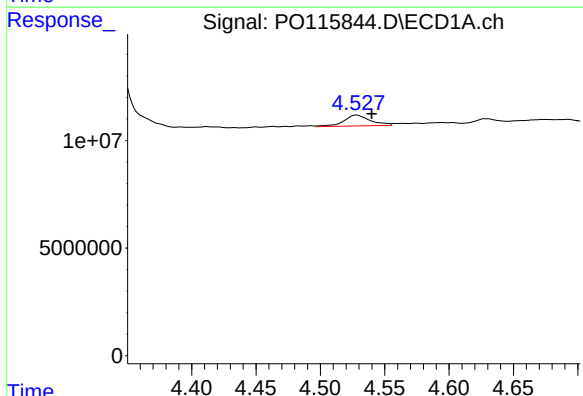


#8 AR-1221-1

R.T.: 4.528 min
Delta R.T.: -0.012 min
Response: 7244584
Conc: 89.22 ng/ml

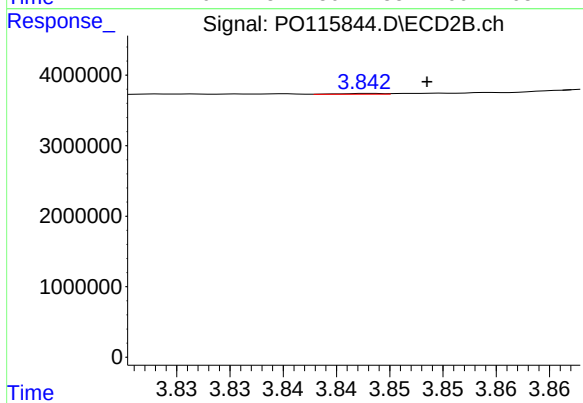

#8 AR-1221-1


R.T.: 3.843 min
Delta R.T.: -0.005 min
Response: 32013
Conc: 0.57 ng/ml

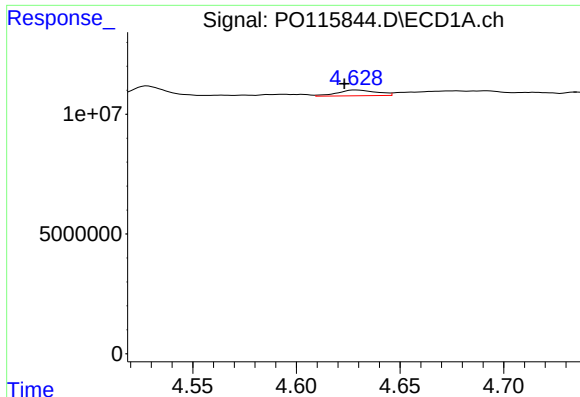

#9 AR-1221-2


R.T.: 4.628 min
Delta R.T.: 0.005 min
Response: 3123348
Conc: 49.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

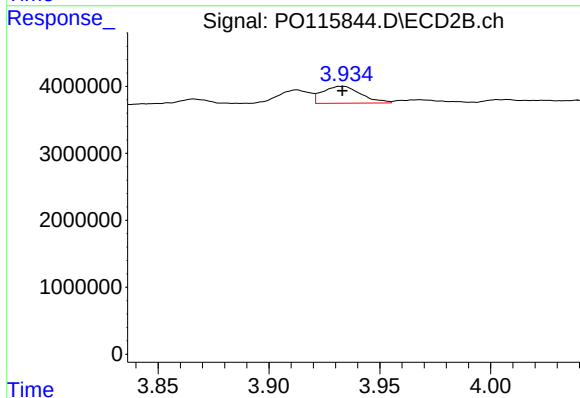


#9 AR-1221-2

R.T.: 3.934 min
Delta R.T.: 0.000 min
Response: 3057958
Conc: 72.05 ng/ml

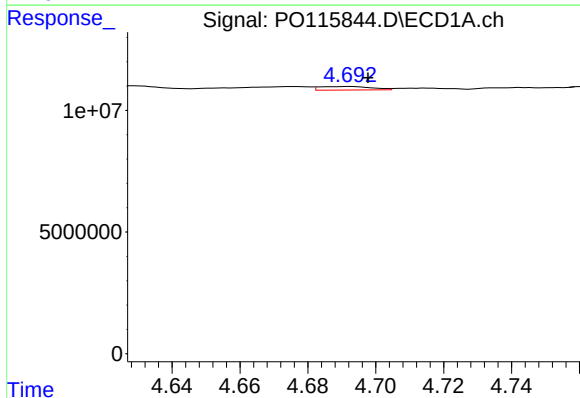


#10 AR-1221-3

R.T.: 4.692 min
Delta R.T.: -0.005 min
Response: 1573534
Conc: 8.43 ng/ml

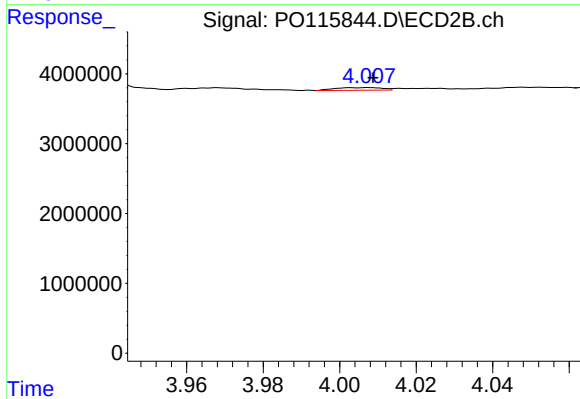

#10 AR-1221-3


R.T.: 4.008 min
Delta R.T.: -0.001 min
Response: 324177
Conc: 2.52 ng/ml

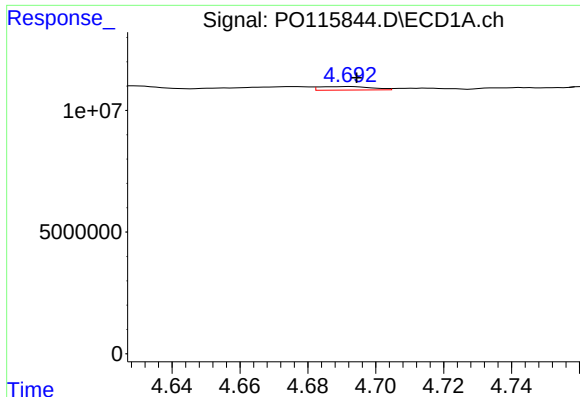

#11 AR-1232-1


R.T.: 4.692 min
Delta R.T.: -0.002 min
Response: 1573534
Conc: 10.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

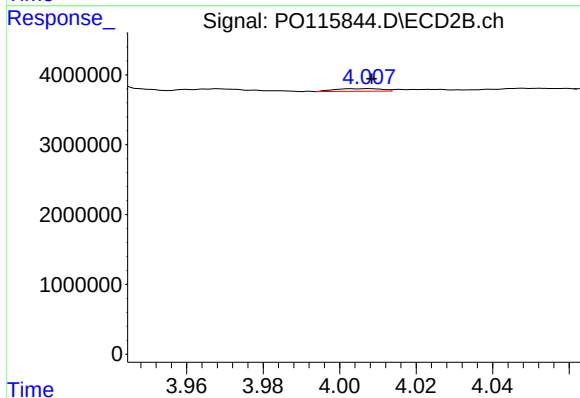


#11 AR-1232-1

R.T.: 4.008 min
Delta R.T.: 0.000 min
Response: 324177
Conc: 3.03 ng/ml

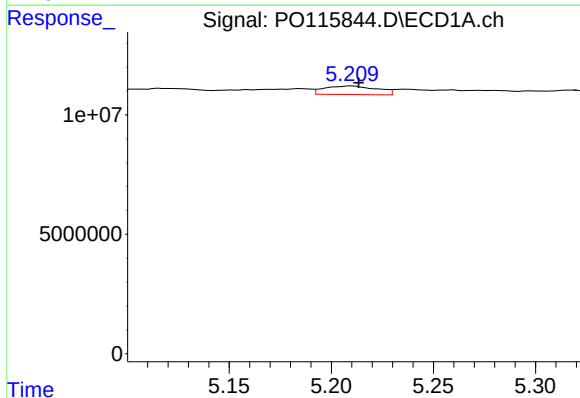


#12 AR-1232-2

R.T.: 5.210 min
Delta R.T.: -0.004 min
Response: 6462450
Conc: 79.93 ng/ml

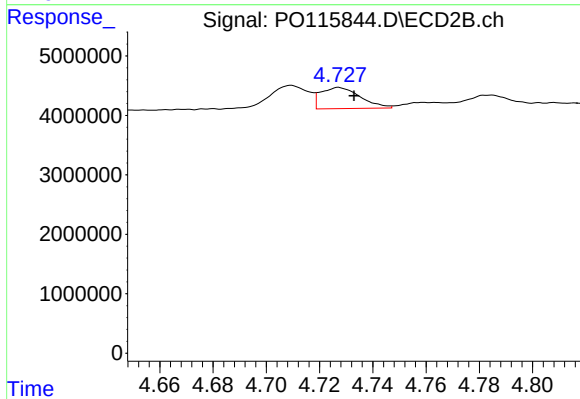

#12 AR-1232-2


R.T.: 4.727 min
Delta R.T.: -0.006 min
Response: 3665471
Conc: 33.03 ng/ml

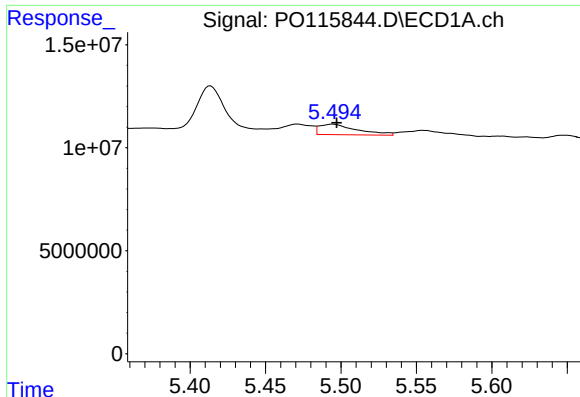

#13 AR-1232-3


R.T.: 5.495 min
Delta R.T.: -0.002 min
Response: 8834607
Conc: 57.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

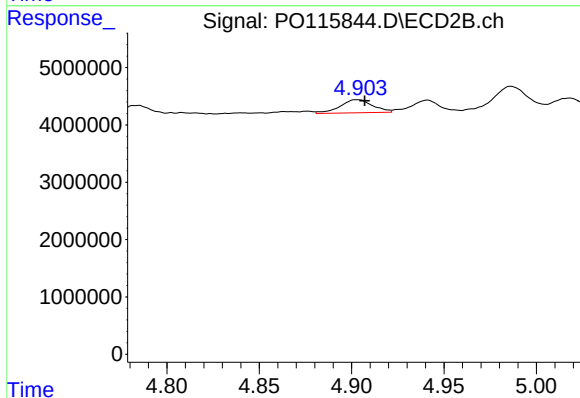


#13 AR-1232-3

R.T.: 4.903 min
Delta R.T.: -0.004 min
Response: 2791448
Conc: 42.70 ng/ml

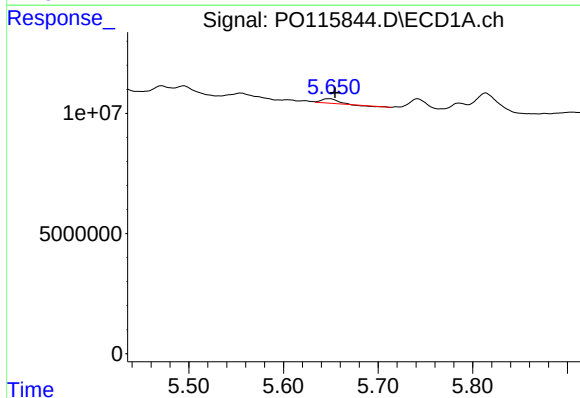


#14 AR-1232-4

R.T.: 5.648 min
Delta R.T.: -0.007 min
Response: 2054863
Conc: 29.34 ng/ml

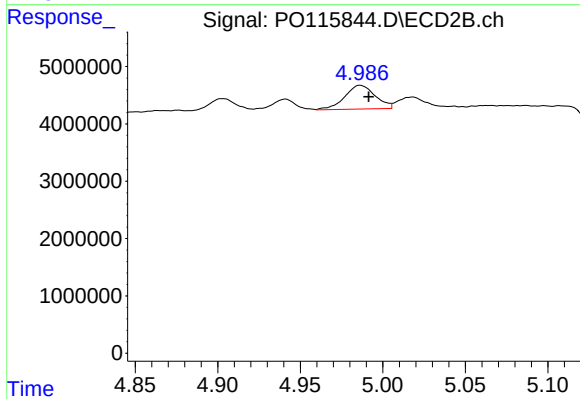

#14 AR-1232-4


R.T.: 4.986 min
Delta R.T.: -0.005 min
Response: 5324696
Conc: 103.73 ng/ml

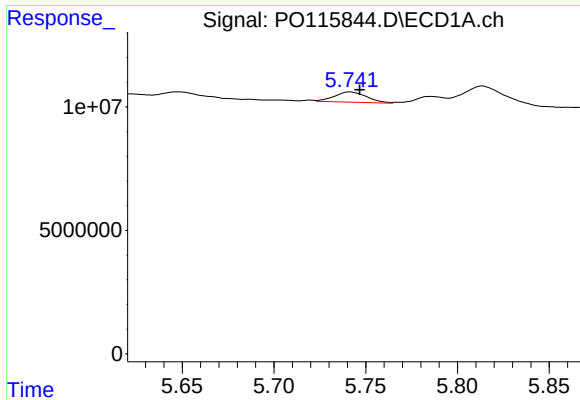

#15 AR-1232-5


R.T.: 5.742 min
Delta R.T.: -0.005 min
Response: 5102335
Conc: 98.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

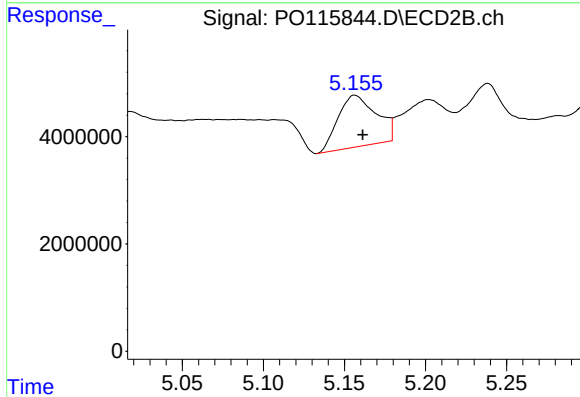


#15 AR-1232-5

R.T.: 5.156 min
Delta R.T.: -0.005 min
Response: 15774723
Conc: 288.13 ng/ml

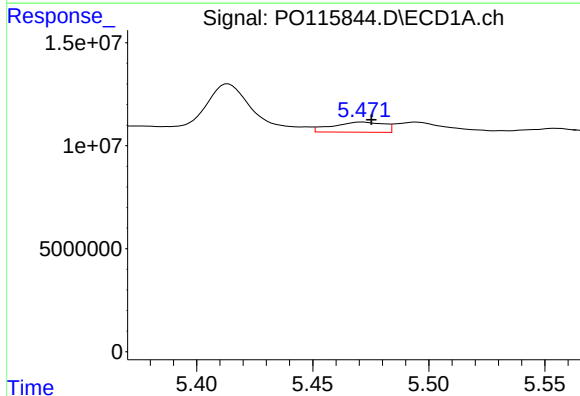


#16 AR-1242-1

R.T.: 5.471 min
Delta R.T.: -0.004 min
Response: 7551280
Conc: 38.02 ng/ml

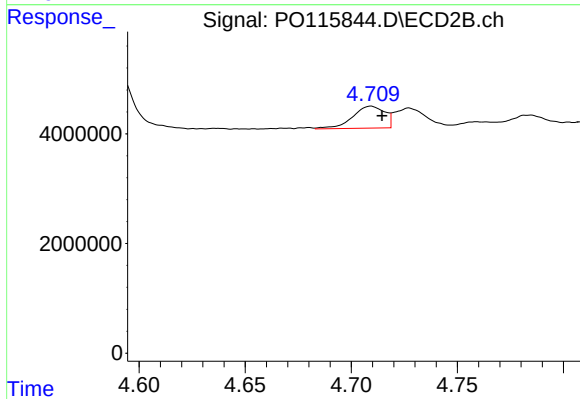

#16 AR-1242-1


R.T.: 4.709 min
Delta R.T.: -0.005 min
Response: 4206773
Conc: 29.54 ng/ml

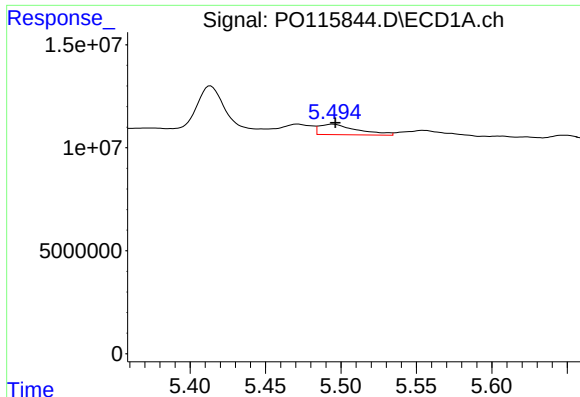

#17 AR-1242-2


R.T.: 5.495 min
Delta R.T.: -0.002 min
Response: 8834607
Conc: 30.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

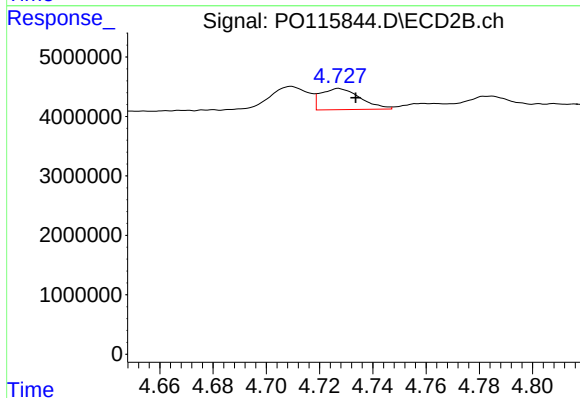


#17 AR-1242-2

R.T.: 4.727 min
Delta R.T.: -0.006 min
Response: 3665471
Conc: 17.51 ng/ml

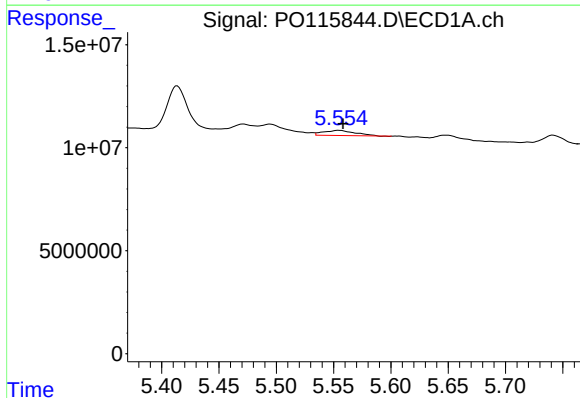


#18 AR-1242-3

R.T.: 5.555 min
Delta R.T.: -0.003 min
Response: 4619669
Conc: 27.37 ng/ml

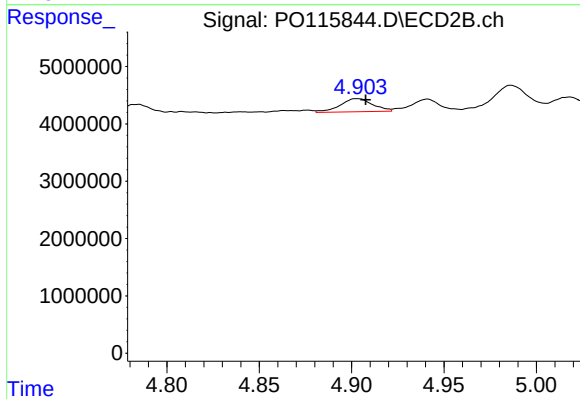

#18 AR-1242-3


R.T.: 4.903 min
Delta R.T.: -0.005 min
Response: 2791448
Conc: 23.37 ng/ml

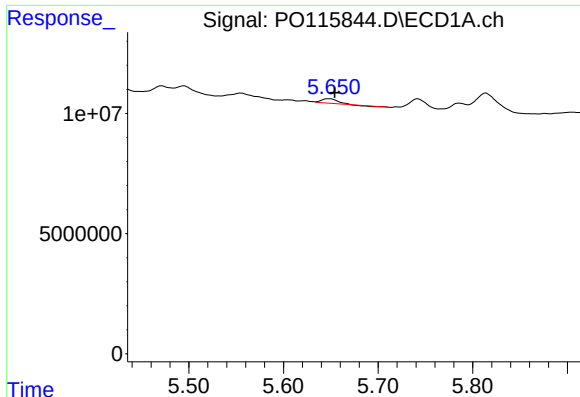

#19 AR-1242-4


R.T.: 5.648 min
Delta R.T.: -0.006 min
Response: 2054863
Conc: 15.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

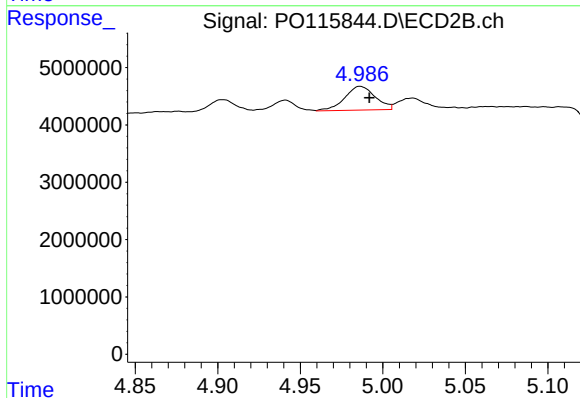


#19 AR-1242-4

R.T.: 4.986 min
Delta R.T.: -0.006 min
Response: 5324696
Conc: 48.81 ng/ml

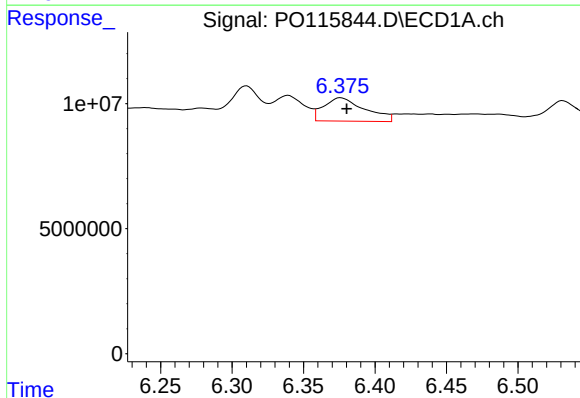


#20 AR-1242-5

R.T.: 6.376 min
Delta R.T.: -0.004 min
Response: 18717810
Conc: 123.60 ng/ml

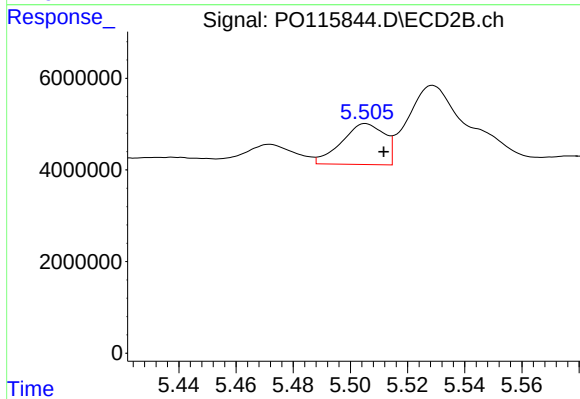

#20 AR-1242-5


R.T.: 5.505 min
Delta R.T.: -0.006 min
Response: 9284032
Conc: 67.21 ng/ml

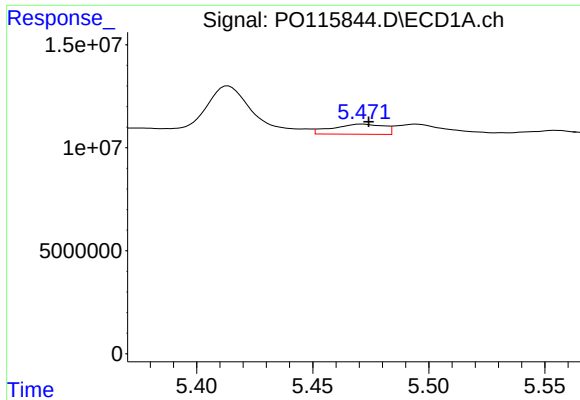

#21 AR-1248-1


R.T.: 5.471 min
Delta R.T.: -0.003 min
Response: 7551280
Conc: 49.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

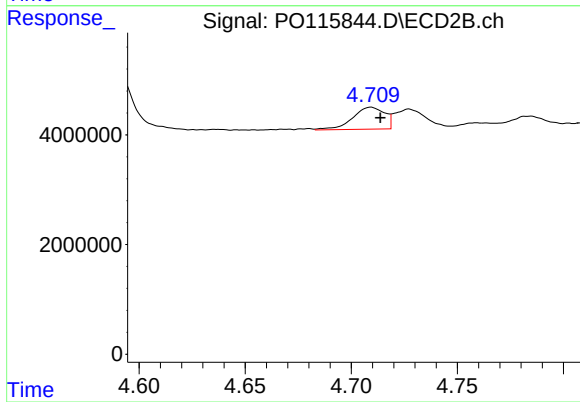


#21 AR-1248-1

R.T.: 4.709 min
Delta R.T.: -0.004 min
Response: 4206773
Conc: 37.62 ng/ml

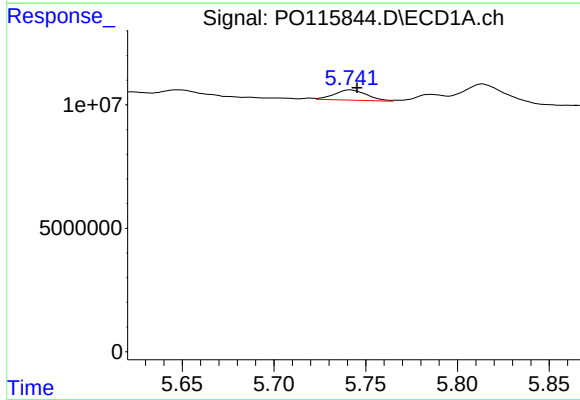


#22 AR-1248-2

R.T.: 5.742 min
Delta R.T.: -0.004 min
Response: 5102335
Conc: 25.41 ng/ml

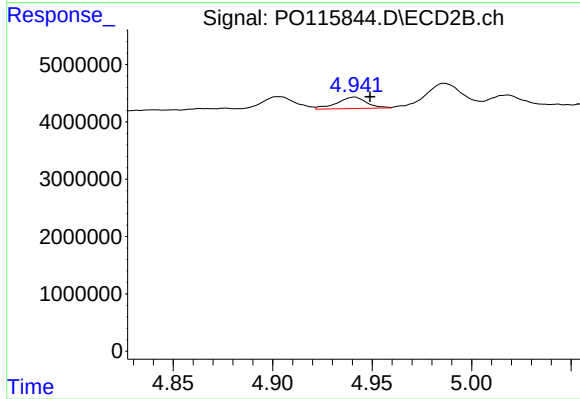

#22 AR-1248-2


R.T.: 4.941 min
Delta R.T.: -0.008 min
Response: 2067009
Conc: 13.57 ng/ml

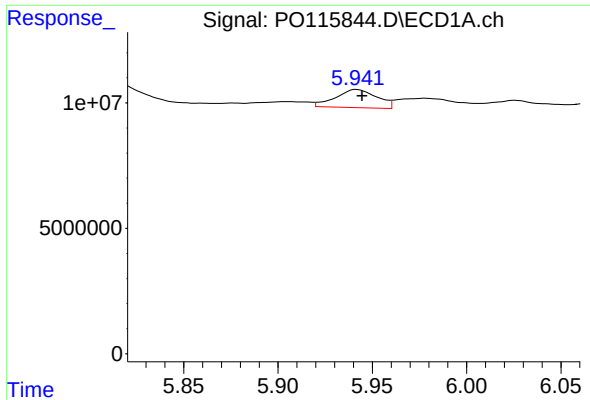

#23 AR-1248-3


R.T.: 5.942 min
Delta R.T.: -0.003 min
Response: 11136399
Conc: 45.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

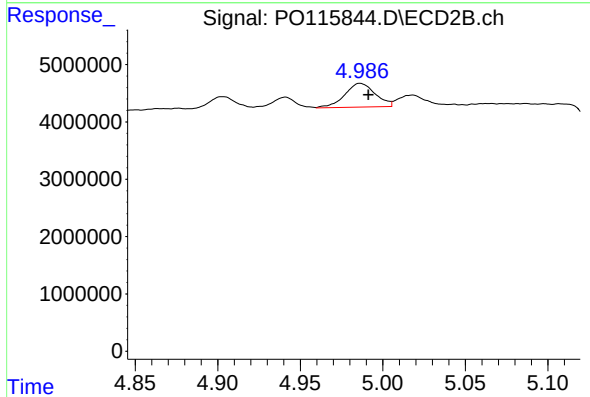


#23 AR-1248-3

R.T.: 4.986 min
Delta R.T.: -0.005 min
Response: 5324696
Conc: 33.17 ng/ml

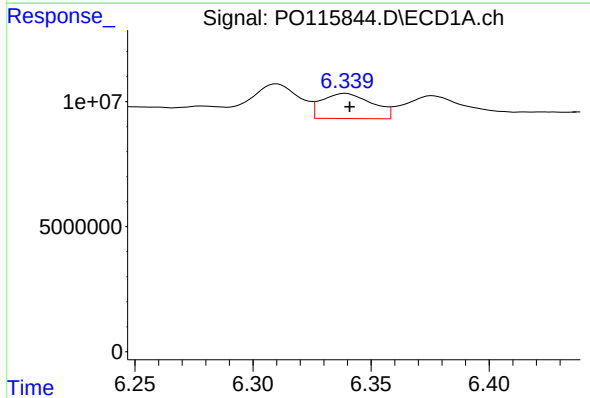


#24 AR-1248-4

R.T.: 6.339 min
Delta R.T.: -0.002 min
Response: 14880944
Conc: 50.47 ng/ml

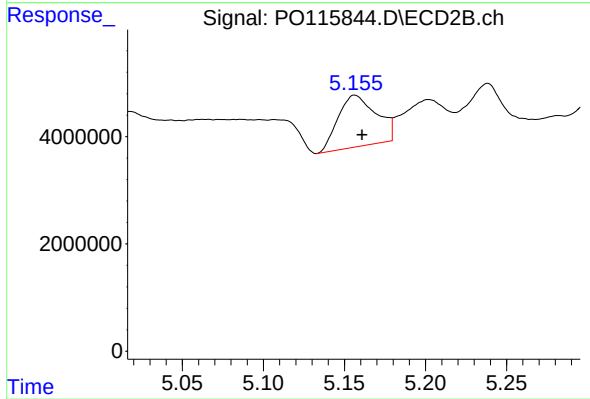

#24 AR-1248-4


R.T.: 5.156 min
Delta R.T.: -0.005 min
Response: 15774723
Conc: 84.29 ng/ml

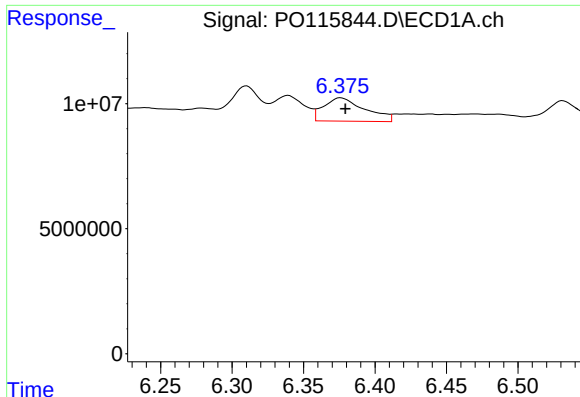

#25 AR-1248-5


R.T.: 6.376 min
Delta R.T.: -0.003 min
Response: 18717810
Conc: 72.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

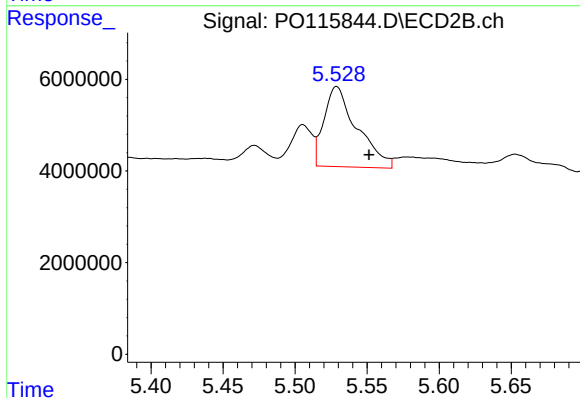


#25 AR-1248-5

R.T.: 5.529 min
Delta R.T.: -0.022 min
Response: 27904493
Conc: 140.96 ng/ml

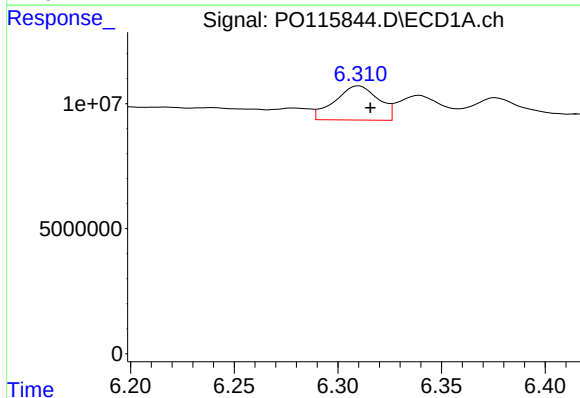


#26 AR-1254-1

R.T.: 6.310 min
Delta R.T.: -0.006 min
Response: 20034577
Conc: 77.44 ng/ml

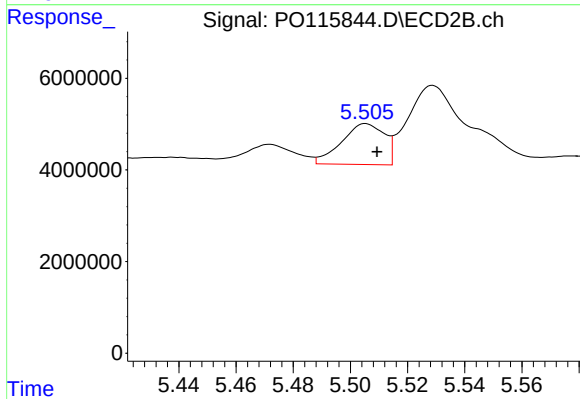

#26 AR-1254-1


R.T.: 5.505 min
Delta R.T.: -0.004 min
Response: 9284032
Conc: 31.77 ng/ml

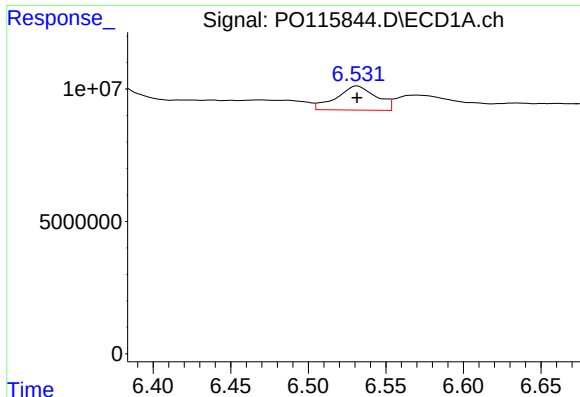

#27 AR-1254-2


R.T.: 6.531 min
Delta R.T.: 0.000 min
Response: 16182225
Conc: 40.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

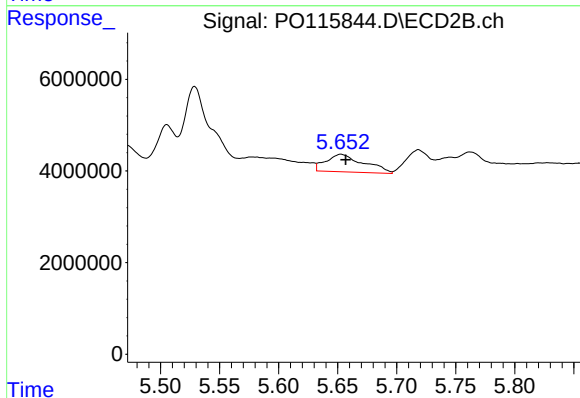


#27 AR-1254-2

R.T.: 5.653 min
Delta R.T.: -0.004 min
Response: 8597987
Conc: 34.14 ng/ml

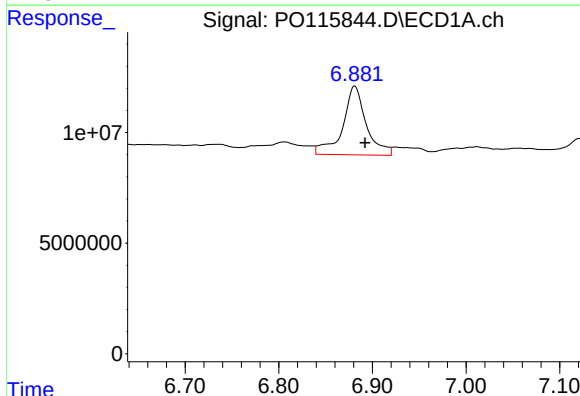


#28 AR-1254-3

R.T.: 6.881 min
Delta R.T.: -0.011 min
Response: 54212441
Conc: 132.04 ng/ml

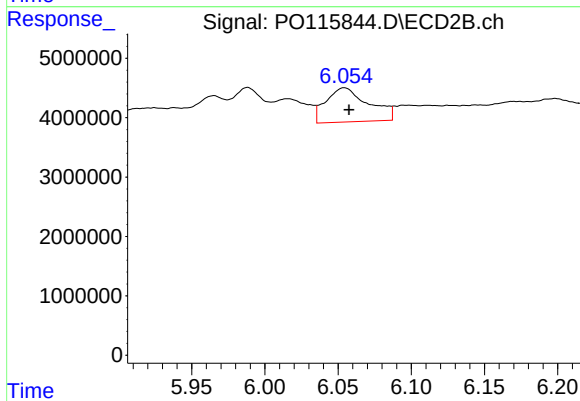

#28 AR-1254-3


R.T.: 6.054 min
Delta R.T.: -0.003 min
Response: 11673469
Conc: 29.66 ng/ml

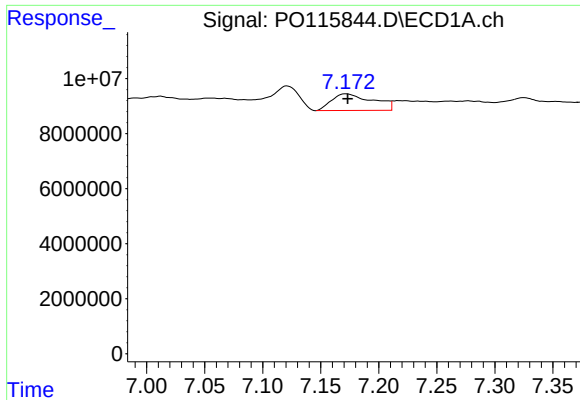

#29 AR-1254-4


R.T.: 7.172 min
Delta R.T.: -0.001 min
Response: 15029040
Conc: 43.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

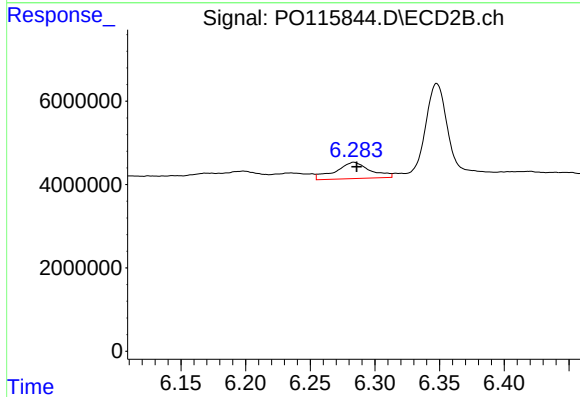


#29 AR-1254-4

R.T.: 6.284 min
Delta R.T.: -0.002 min
Response: 7329785
Conc: 27.39 ng/ml

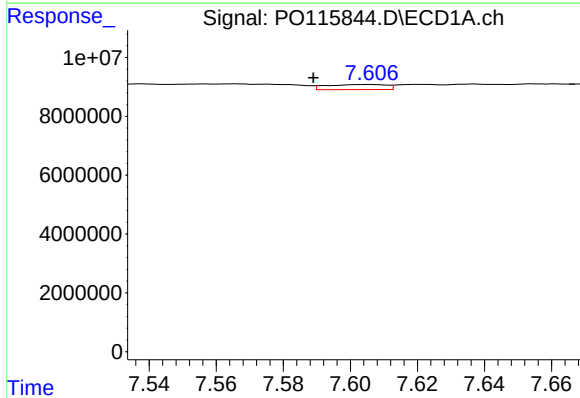


#30 AR-1254-5

R.T.: 7.606 min
Delta R.T.: 0.017 min
Response: 2133112
Conc: 6.58 ng/ml

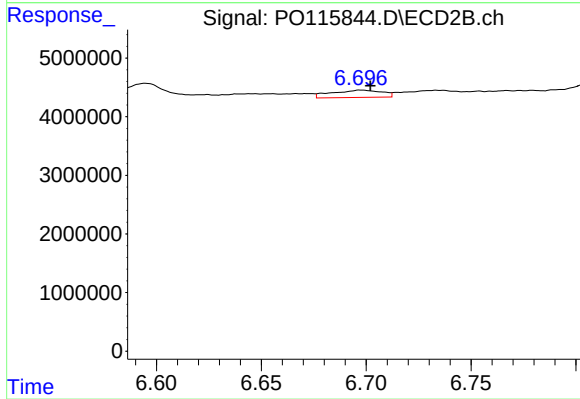

#30 AR-1254-5


R.T.: 6.697 min
Delta R.T.: -0.005 min
Response: 2078166
Conc: 5.81 ng/ml

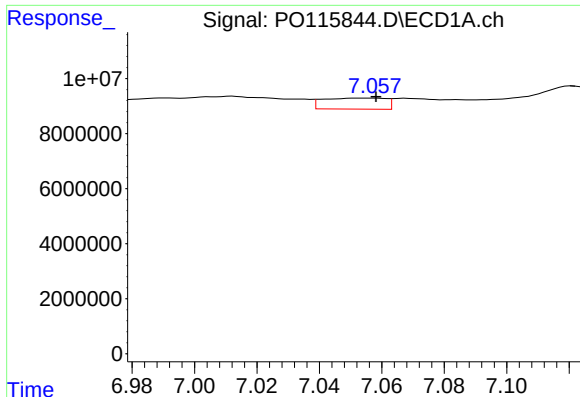

#31 AR-1260-1


R.T.: 7.057 min
Delta R.T.: -0.001 min
Response: 5555425
Conc: 19.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

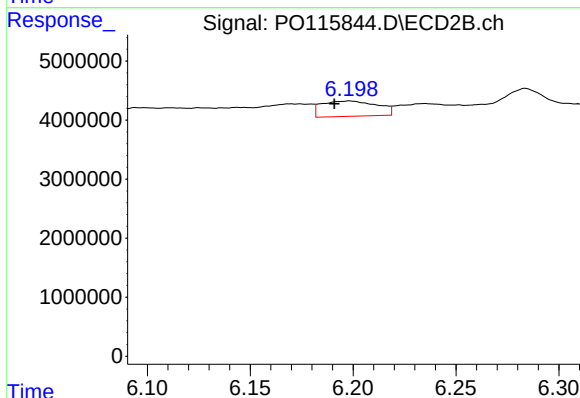


#31 AR-1260-1

R.T.: 6.198 min
Delta R.T.: 0.007 min
Response: 4895755
Conc: 18.67 ng/ml

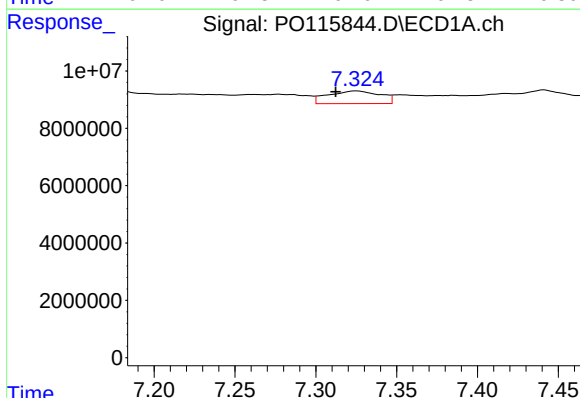


#32 AR-1260-2

R.T.: 7.325 min
Delta R.T.: 0.013 min
Response: 9885816
Conc: 22.58 ng/ml

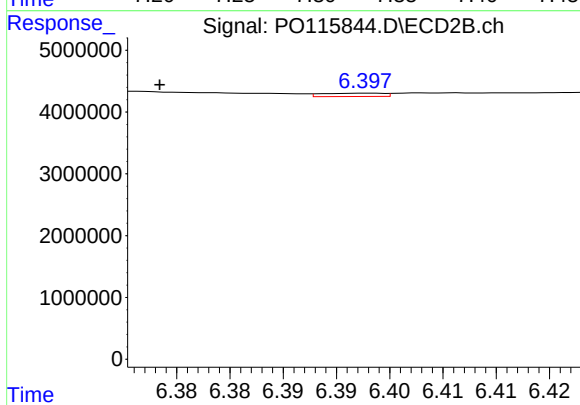

#32 AR-1260-2


R.T.: 6.398 min
Delta R.T.: 0.020 min
Response: 215719
Conc: 0.62 ng/ml

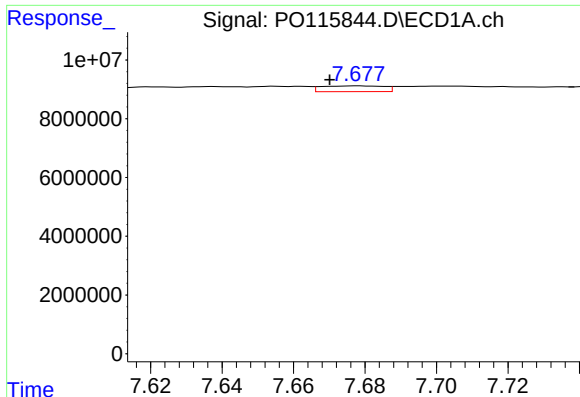

#33 AR-1260-3


R.T.: 7.678 min
Delta R.T.: 0.008 min
Response: 2390364
Conc: 7.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

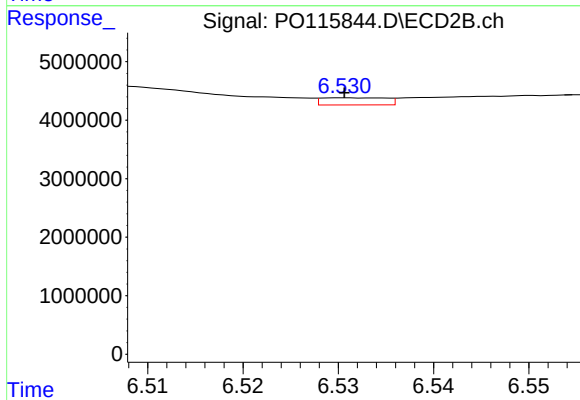


#33 AR-1260-3

R.T.: 6.531 min
Delta R.T.: 0.000 min
Response: 577110
Conc: 1.80 ng/ml

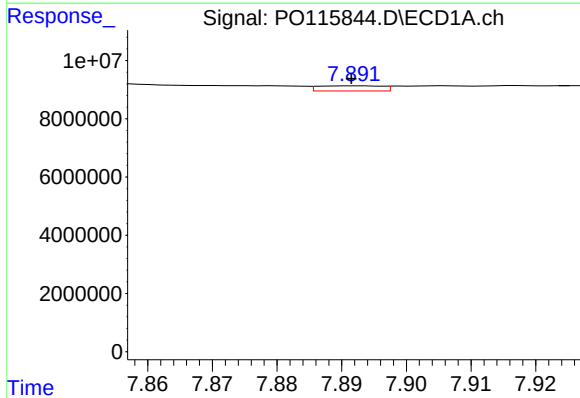


#34 AR-1260-4

R.T.: 7.892 min
Delta R.T.: 0.000 min
Response: 1209636
Conc: 3.93 ng/ml

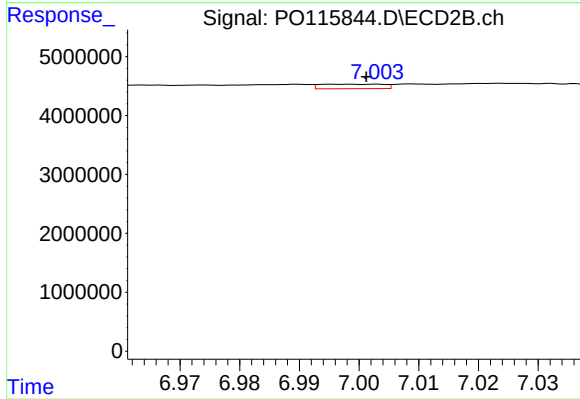

#34 AR-1260-4


R.T.: 7.003 min
Delta R.T.: 0.002 min
Response: 572519
Conc: 2.23 ng/ml

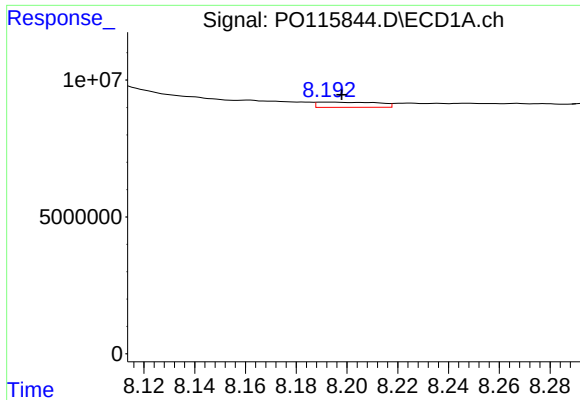

#35 AR-1260-5


R.T.: 8.193 min
Delta R.T.: -0.005 min
Response: 3124468
Conc: 4.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

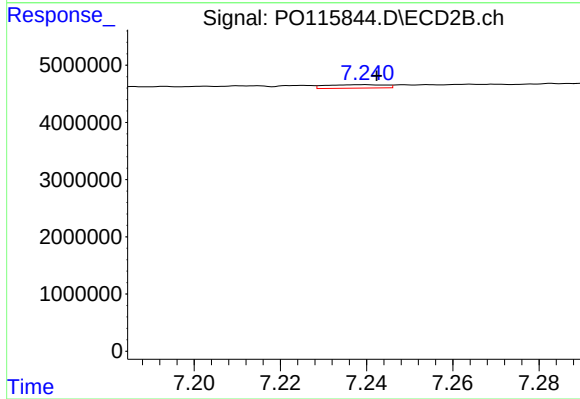


#35 AR-1260-5

R.T.: 7.240 min
Delta R.T.: -0.003 min
Response: 581061
Conc: 0.83 ng/ml

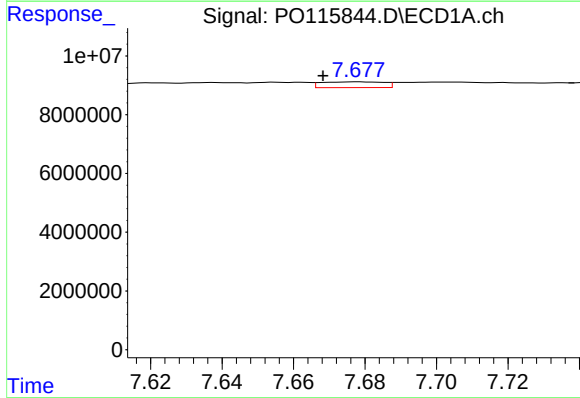


#36 AR-1262-1

R.T.: 7.678 min
Delta R.T.: 0.010 min
Response: 2390364
Conc: 9.68 ng/ml

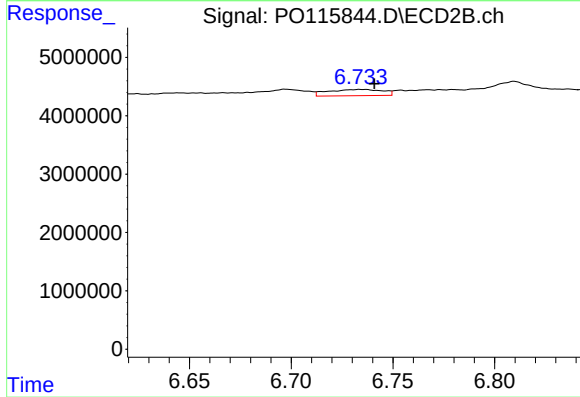

#36 AR-1262-1


R.T.: 6.734 min
Delta R.T.: -0.007 min
Response: 1997906
Conc: 9.38 ng/ml

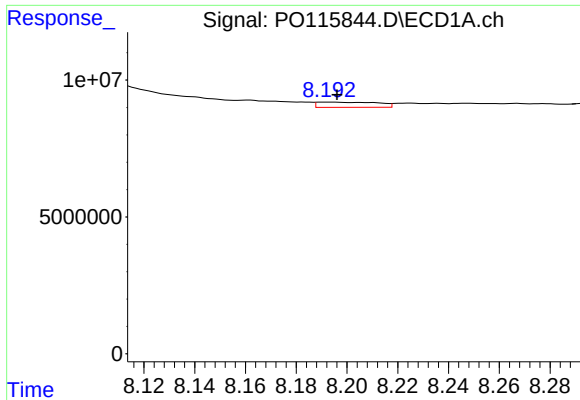

#37 AR-1262-2


R.T.: 8.193 min
Delta R.T.: -0.003 min
Response: 3124468
Conc: 7.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

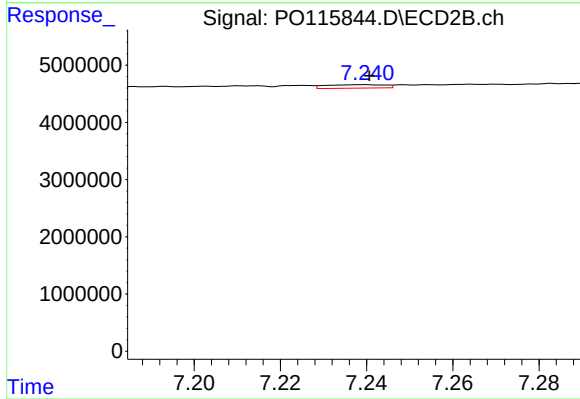


#37 AR-1262-2

R.T.: 7.240 min
Delta R.T.: 0.000 min
Response: 581061
Conc: 1.67 ng/ml

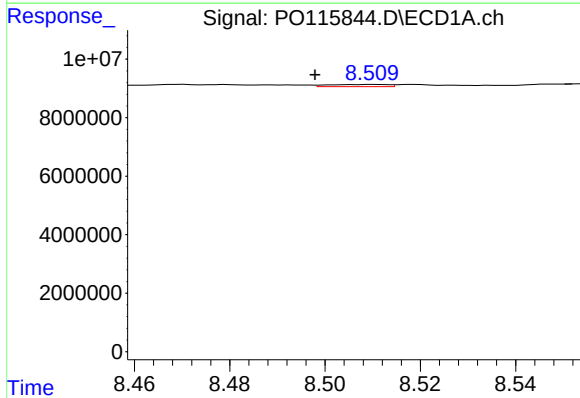


#38 AR-1262-3

R.T.: 8.510 min
Delta R.T.: 0.012 min
Response: 653785
Conc: 2.57 ng/ml

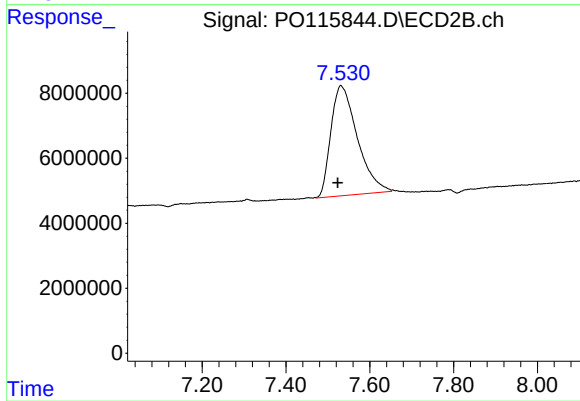

#38 AR-1262-3


R.T.: 7.531 min
Delta R.T.: 0.007 min
Response: 148165182
Conc: 947.41 ng/ml

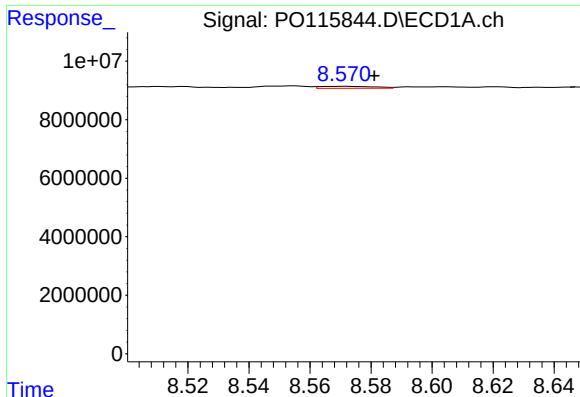

#39 AR-1262-4


R.T.: 8.571 min
Delta R.T.: -0.010 min
Response: 850608
Conc: 4.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

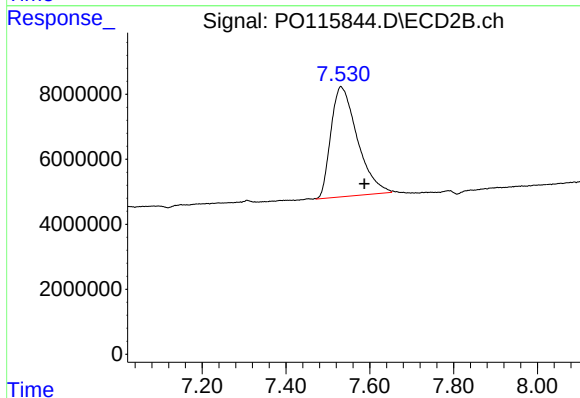


#39 AR-1262-4

R.T.: 7.531 min
Delta R.T.: -0.056 min
Response: 148165182
Conc: 598.96 ng/ml

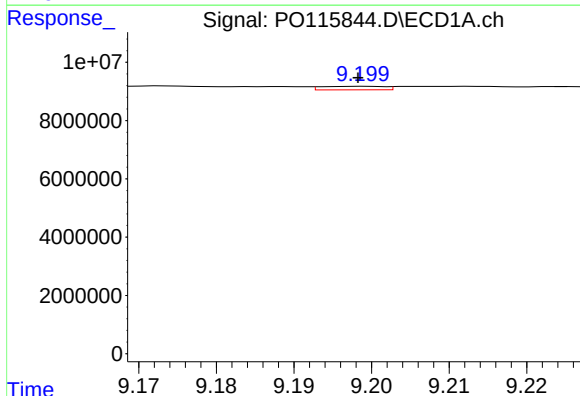


#40 AR-1262-5

R.T.: 9.199 min
Delta R.T.: 0.000 min
Response: 696272
Conc: 5.17 ng/ml

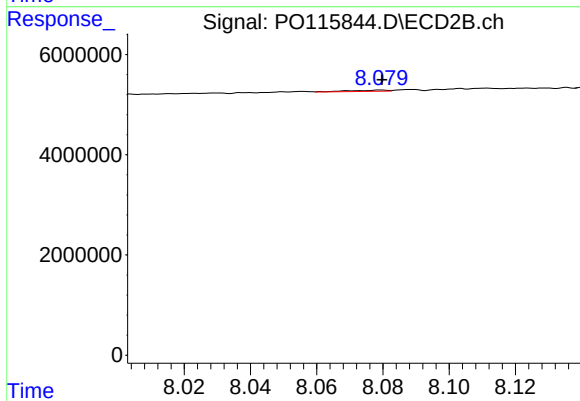

#40 AR-1262-5


R.T.: 8.079 min
Delta R.T.: 0.000 min
Response: 196241
Conc: 1.76 ng/ml

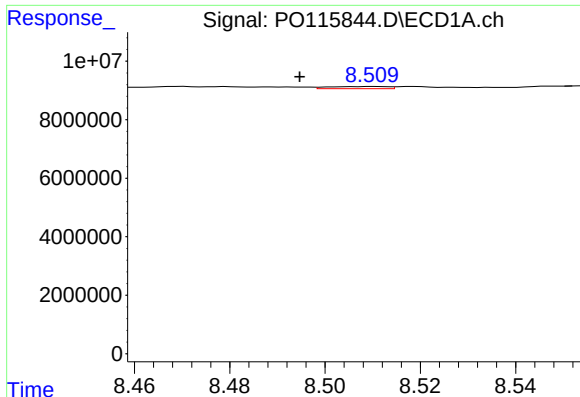

#41 AR-1268-1


R.T.: 8.510 min
Delta R.T.: 0.016 min
Response: 653785
Conc: 0.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

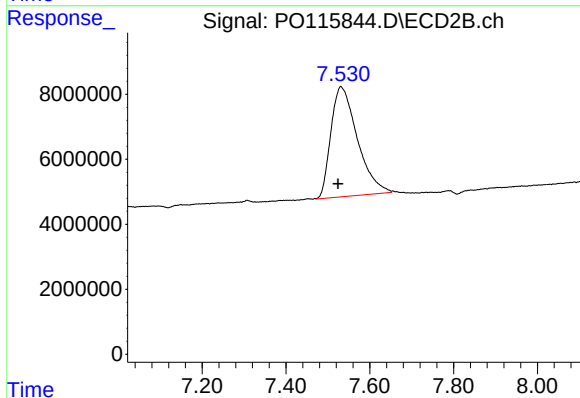


#41 AR-1268-1

R.T.: 7.531 min
Delta R.T.: 0.007 min
Response: 148165182
Conc: 167.24 ng/ml

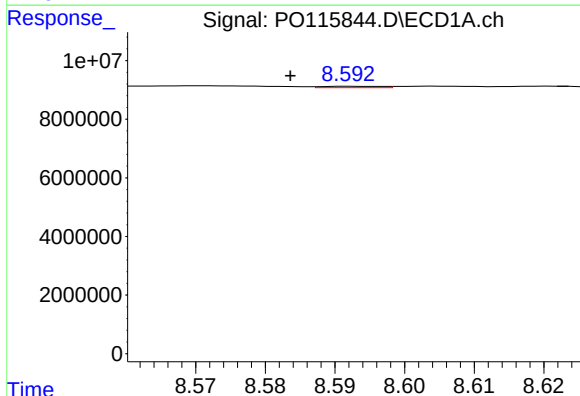


#42 AR-1268-2

R.T.: 8.593 min
Delta R.T.: 0.009 min
Response: 278534
Conc: 0.33 ng/ml

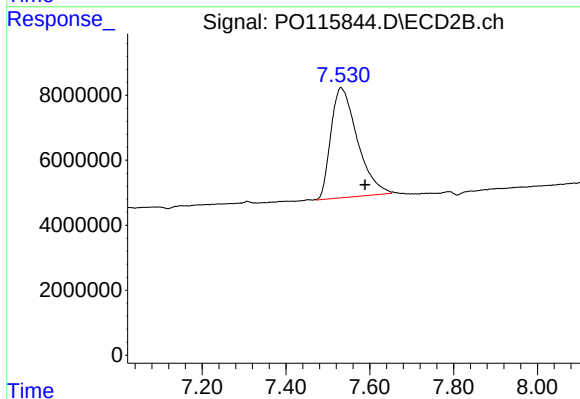

#42 AR-1268-2


R.T.: 7.531 min
Delta R.T.: -0.058 min
Response: 148165182
Conc: 197.80 ng/ml

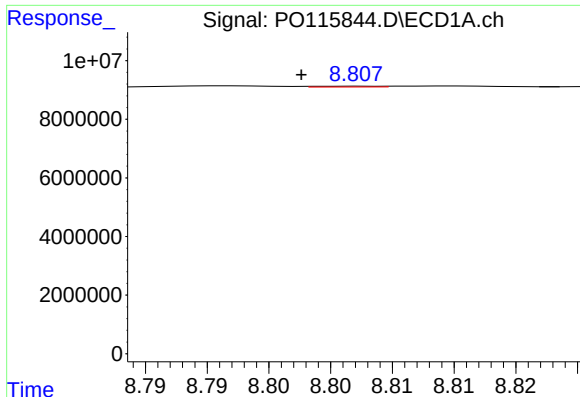

#43 AR-1268-3


R.T.: 8.808 min
Delta R.T.: 0.005 min
Response: 104341
Conc: 0.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

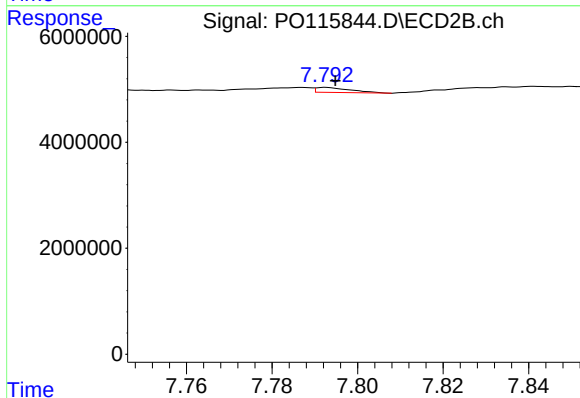


#43 AR-1268-3

R.T.: 7.793 min
Delta R.T.: -0.002 min
Response: 521707
Conc: 0.82 ng/ml

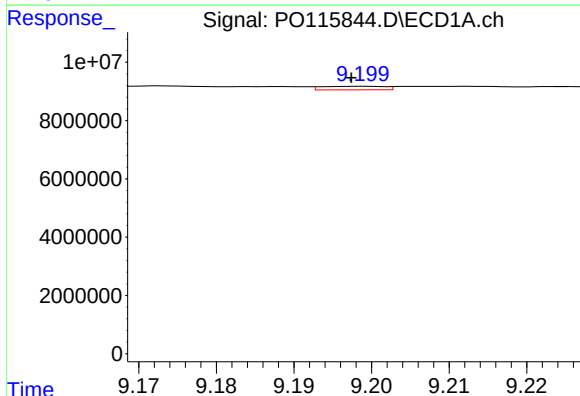


#44 AR-1268-4

R.T.: 9.199 min
Delta R.T.: 0.002 min
Response: 696272
Conc: 2.23 ng/ml

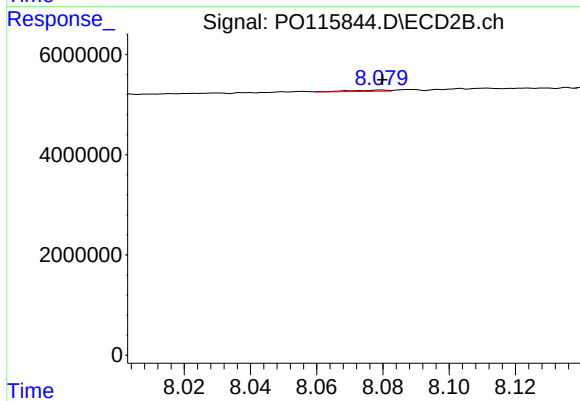

#44 AR-1268-4


R.T.: 8.079 min
Delta R.T.: 0.000 min
Response: 196241
Conc: 0.76 ng/ml

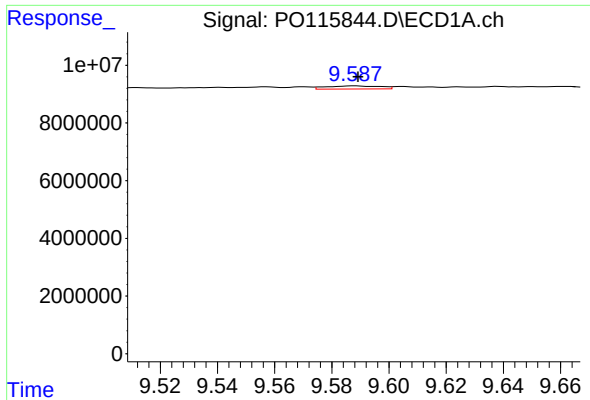

#45 AR-1268-5

R.T.: 9.588 min
Delta R.T.: -0.001 min
Response: 1417644
Conc: 0.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

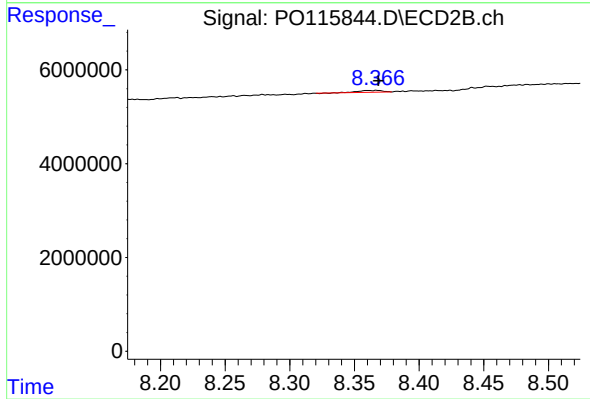

#45 AR-1268-5

R.T.: 8.368 min
Delta R.T.: -0.001 min
Response: 528472
Conc: 0.31 ng/ml