

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121225\
 Data File : PO115846.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Dec 2025 10:56
 Operator : YP/AJ
 Sample : Q3530-09
 Misc : AR1262 25PPB WATER MDL
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT4-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 02:46:18 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 05 02:11:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.332	3.634	409.2E6	252.3E6	52.681	51.777
2)	SA Decachlor...	9.906	8.615	273.6E6	202.7E6	52.000	47.147
Target Compounds							
3)	L1 AR-1016-1	5.497	4.709	2450968	17339523	9.857	93.847 #
4)	L1 AR-1016-2	5.497	4.709	2450968	17339523	6.436	65.603 #
5)	L1 AR-1016-3	5.558	4.903	2832473	12245987	13.249	80.918 #
6)	L1 AR-1016-4	5.667	4.925	209266	6577770	1.172	58.363 #
7)	L1 AR-1016-5	5.941	5.170	32152505	16436823	183.282	112.319 #
8)	L2 AR-1221-1	4.529	3.841	9538843	33827	117.478	0.600 #
9)	L2 AR-1221-2	4.631	3.931	5346160	6291333	84.834	148.227 #
10)	L2 AR-1221-3	4.705	4.007	803932	1949158	4.306	15.158 #
11)	L3 AR-1232-1	4.686	4.007	2573369	1949158	17.194	18.244
12)	L3 AR-1232-2	5.215	4.709	1008965	17339523	12.479	156.226 #
13)	L3 AR-1232-3	5.497	4.903	2450968	12245987	15.925	187.344 #
14)	L3 AR-1232-4	5.667	4.990	209266	2748132	2.988	53.538 #
15)	L3 AR-1232-5	5.739	5.170	4351917	16436823	83.792	300.226 #
16)	L4 AR-1242-1	5.497	4.709	2450968	17339523	12.340	121.776 #
17)	L4 AR-1242-2	5.497	4.709	2450968	17339523	8.368	82.820 #
18)	L4 AR-1242-3	5.558	4.903	2832473	12245987	16.778	102.526 #
19)	L4 AR-1242-4	5.667	4.990	209266	2748132	1.531	25.191 #
20)	L4 AR-1242-5	6.374	5.529	31639823	47227594	208.921	341.919 #
21)	L5 AR-1248-1	5.497	4.709	2450968	17339523	16.150	155.054 #
22)	L5 AR-1248-2	5.739	4.925	4351917	6577770	21.671	43.192 #
23)	L5 AR-1248-3	5.941	4.990	32152505	2748132	130.384	17.119 #
24)	L5 AR-1248-4	6.348	5.170	23602147	16436823	80.047	87.829
25)	L5 AR-1248-5	6.374	5.562	31639823	2277731	122.196	11.506 #
26)	L6 AR-1254-1	6.303	5.529	27170036	47227594	105.020	161.588 #
27)	L6 AR-1254-2	6.530	5.653	45418220	23179591	112.867	92.051
28)	L6 AR-1254-3	6.881	6.070	71030256	26261243	173.006	66.724 #
29)	L6 AR-1254-4	7.175	6.289	24193459	7924870	69.709	29.617 #
30)	L6 AR-1254-5	7.583	6.697	44786373	12464344	138.211	34.863 #
31)	L7 AR-1260-1	7.056	6.185	53857034	31603327	185.907	120.546 #
32)	L7 AR-1260-2	7.309	6.372	48685510	20835178	111.223	59.452 #
33)	L7 AR-1260-3	7.666	6.527	56594240	19470277	168.138	60.604 #
34)	L7 AR-1260-4	7.888	6.995	45566138	20048459	148.197	78.060 #
35)	L7 AR-1260-5	8.194	7.236	59064142	42212342	81.079	60.193 #
36)	L8 AR-1262-1	7.666	6.738	56594240	26755158	229.259	125.586 #
37)	L8 AR-1262-2	8.194	7.236	59064142	42212342	149.190	121.186
38)	L8 AR-1262-3	8.496	7.521	34868460	83152459	136.834	531.698 #
39)	L8 AR-1262-4	8.577	7.583	27002876	49485912	139.401	200.047 #
40)	L8 AR-1262-5	9.196	8.075	18577082	12321517	137.924	110.532
41)	L9 AR-1268-1	8.496	7.521	34868460	83152459	35.018	93.857 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121225\
 Data File : PO115846.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Dec 2025 10:56
 Operator : YP/AJ
 Sample : Q3530-09
 Misc : AR1262 25PPB WATER MDL
 ALS Vial : 25 Sample Multiplier: 1


Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT4-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 02:46:18 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 05 02:11:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.577	7.583	27002876	49485912	31.569	66.063 #
43) L9	AR-1268-3	8.798	7.790	1833526	1714098	2.469	2.692
44) L9	AR-1268-4	9.196	8.075	18577082	12321517	59.497	47.828
45) L9	AR-1268-5	9.587	8.363	7901728	5087300	3.629	3.018


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

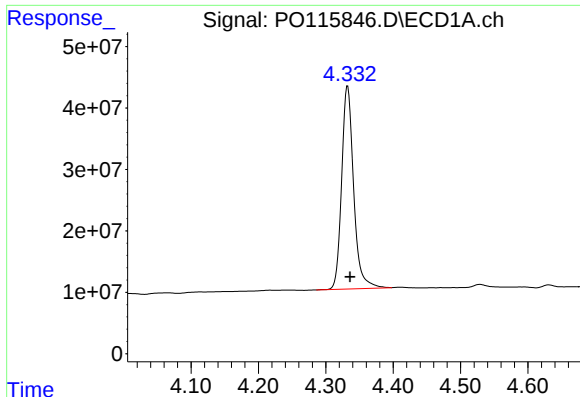

#1 Tetrachloro-m-xylene


R.T.: 4.332 min
Delta R.T.: -0.004 min
Response: 409184936
Conc: 52.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

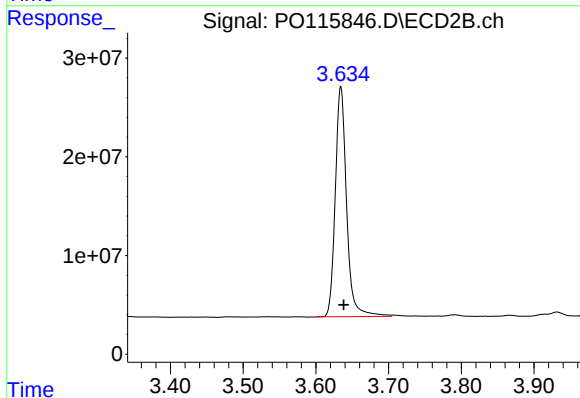


#1 Tetrachloro-m-xylene

R.T.: 3.634 min
Delta R.T.: -0.004 min
Response: 252327987
Conc: 51.78 ng/ml

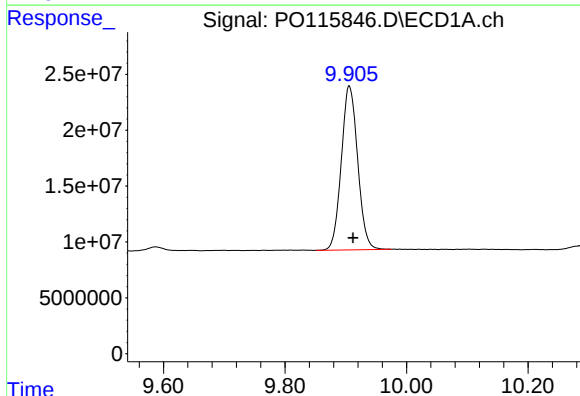


#2 Decachlorobiphenyl

R.T.: 9.906 min
Delta R.T.: -0.006 min
Response: 273572646
Conc: 52.00 ng/ml

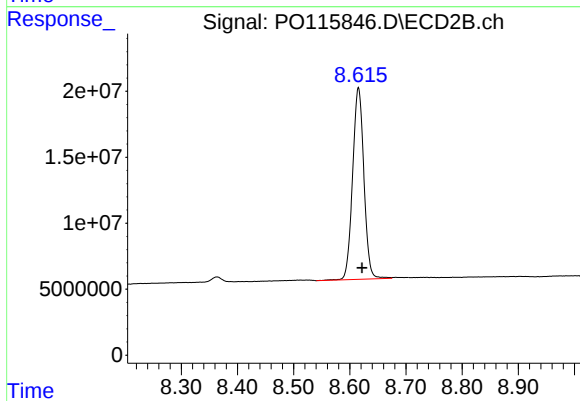

#2 Decachlorobiphenyl


R.T.: 8.615 min
Delta R.T.: -0.007 min
Response: 202742757
Conc: 47.15 ng/ml

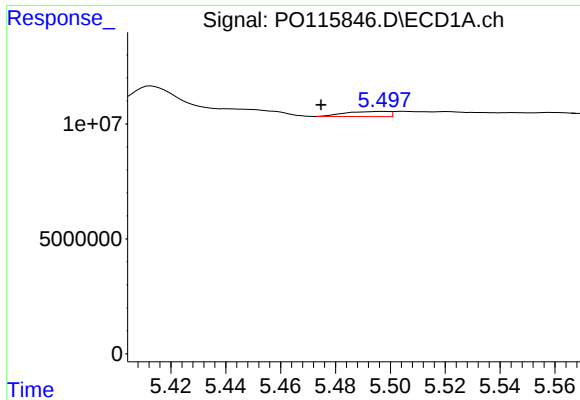

#3 AR-1016-1


R.T.: 5.497 min
Delta R.T.: 0.023 min
Response: 2450968
Conc: 9.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

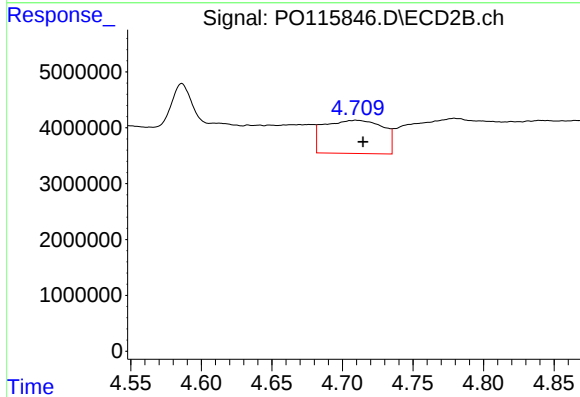


#3 AR-1016-1

R.T.: 4.709 min
Delta R.T.: -0.005 min
Response: 17339523
Conc: 93.85 ng/ml

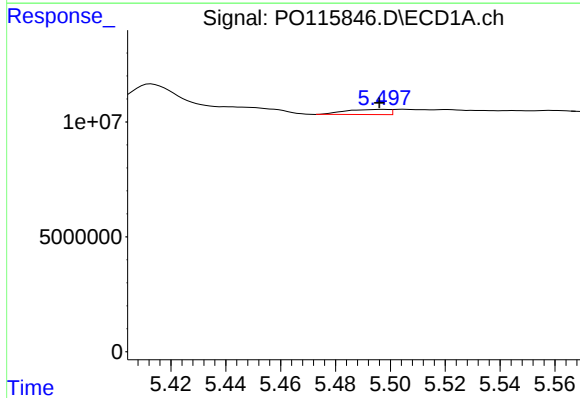


#4 AR-1016-2

R.T.: 5.497 min
Delta R.T.: 0.001 min
Response: 2450968
Conc: 6.44 ng/ml

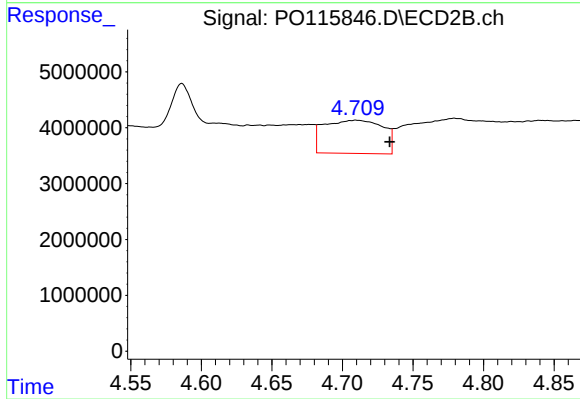

#4 AR-1016-2


R.T.: 4.709 min
Delta R.T.: -0.024 min
Response: 17339523
Conc: 65.60 ng/ml

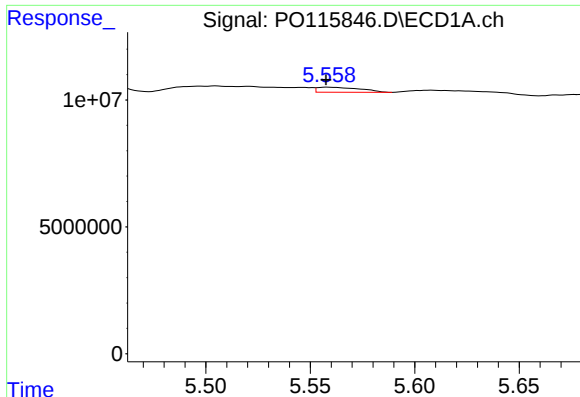

#5 AR-1016-3


R.T.: 5.558 min
Delta R.T.: 0.000 min
Response: 2832473
Conc: 13.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

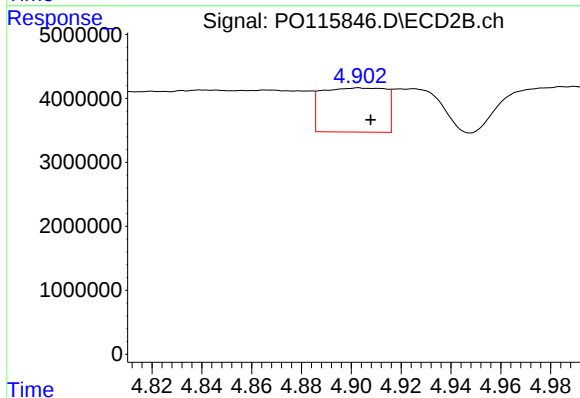


#5 AR-1016-3

R.T.: 4.903 min
Delta R.T.: -0.005 min
Response: 12245987
Conc: 80.92 ng/ml

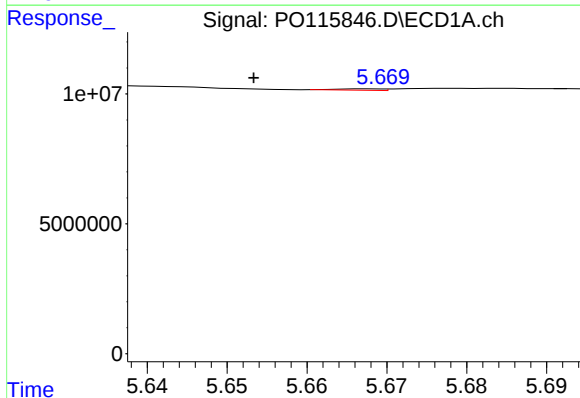


#6 AR-1016-4

R.T.: 5.667 min
Delta R.T.: 0.014 min
Response: 209266
Conc: 1.17 ng/ml

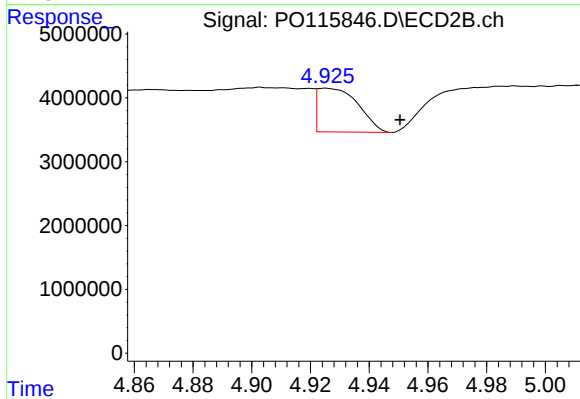

#6 AR-1016-4


R.T.: 4.925 min
Delta R.T.: -0.025 min
Response: 6577770
Conc: 58.36 ng/ml

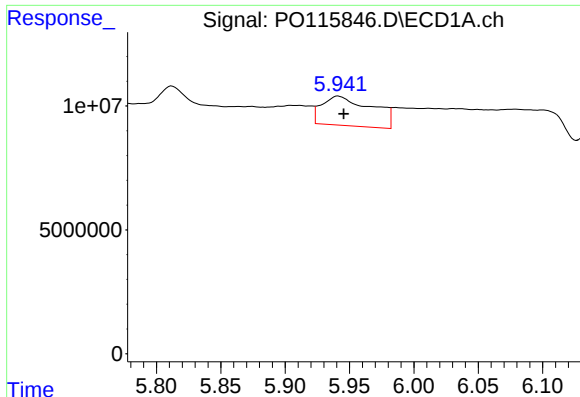

#7 AR-1016-5


R.T.: 5.941 min
Delta R.T.: -0.004 min
Response: 32152505
Conc: 183.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

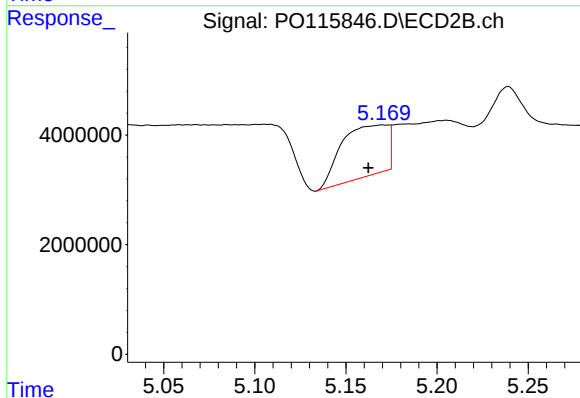


#7 AR-1016-5

R.T.: 5.170 min
Delta R.T.: 0.008 min
Response: 16436823
Conc: 112.32 ng/ml

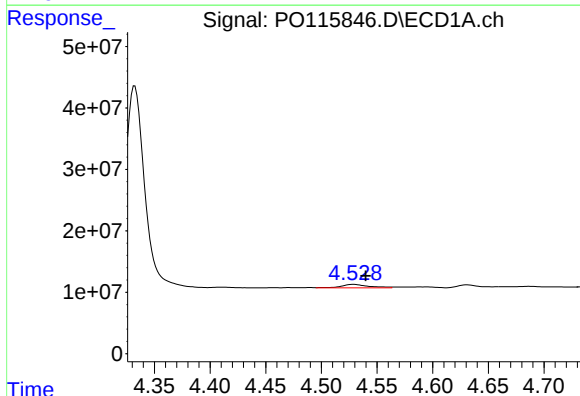


#8 AR-1221-1

R.T.: 4.529 min
Delta R.T.: -0.011 min
Response: 9538843
Conc: 117.48 ng/ml

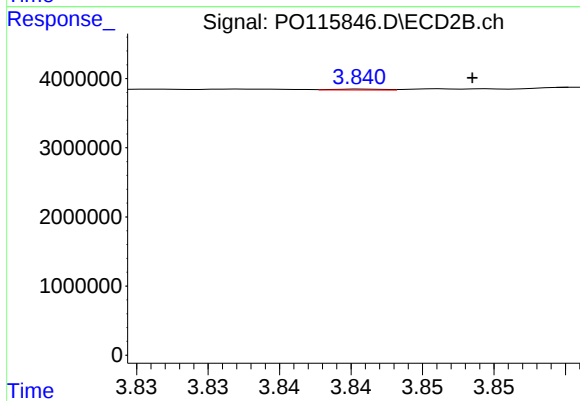

#8 AR-1221-1


R.T.: 3.841 min
Delta R.T.: -0.008 min
Response: 33827
Conc: 0.60 ng/ml

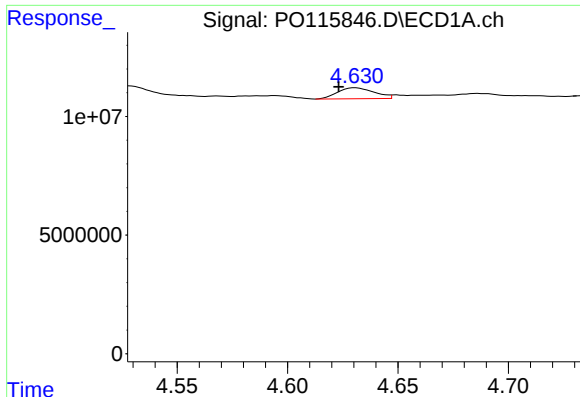

#9 AR-1221-2


R.T.: 4.631 min
Delta R.T.: 0.008 min
Response: 5346160
Conc: 84.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

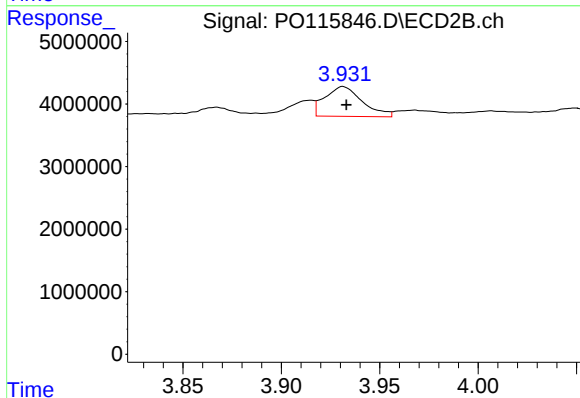


#9 AR-1221-2

R.T.: 3.931 min
Delta R.T.: -0.002 min
Response: 6291333
Conc: 148.23 ng/ml

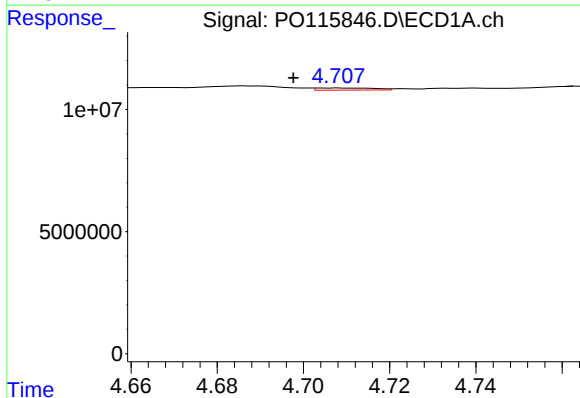


#10 AR-1221-3

R.T.: 4.705 min
Delta R.T.: 0.007 min
Response: 803932
Conc: 4.31 ng/ml

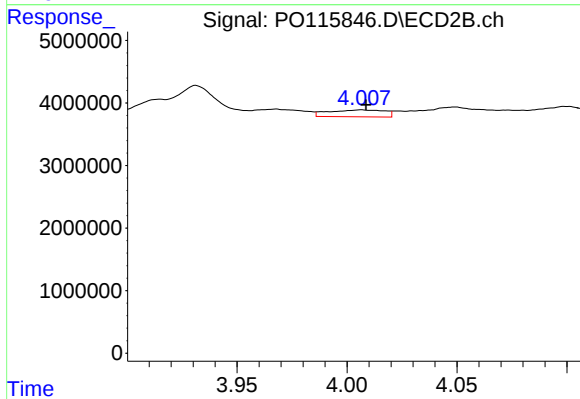

#10 AR-1221-3


R.T.: 4.007 min
Delta R.T.: -0.002 min
Response: 1949158
Conc: 15.16 ng/ml

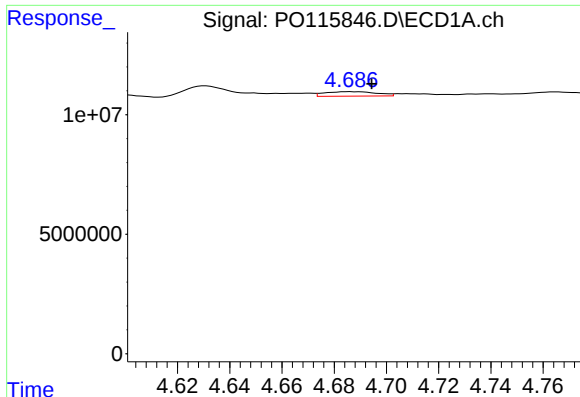

#11 AR-1232-1


R.T.: 4.686 min
Delta R.T.: -0.008 min
Response: 2573369
Conc: 17.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

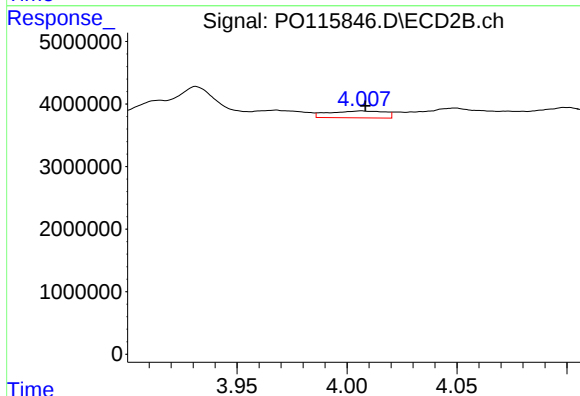


#11 AR-1232-1

R.T.: 4.007 min
Delta R.T.: -0.002 min
Response: 1949158
Conc: 18.24 ng/ml

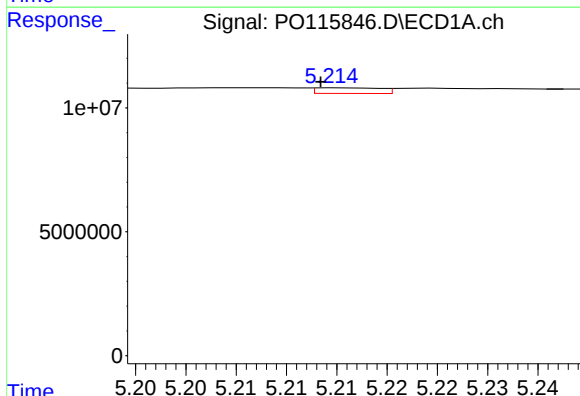


#12 AR-1232-2

R.T.: 5.215 min
Delta R.T.: 0.002 min
Response: 1008965
Conc: 12.48 ng/ml

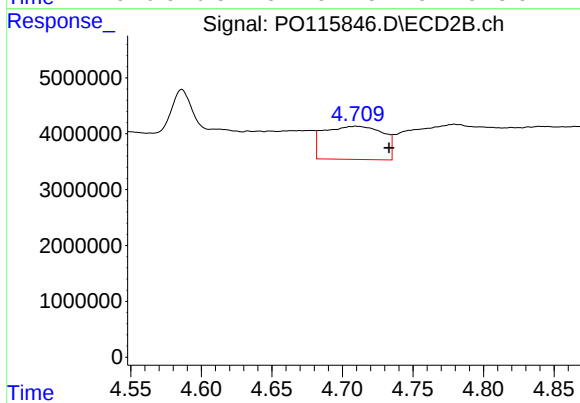

#12 AR-1232-2


R.T.: 4.709 min
Delta R.T.: -0.023 min
Response: 17339523
Conc: 156.23 ng/ml

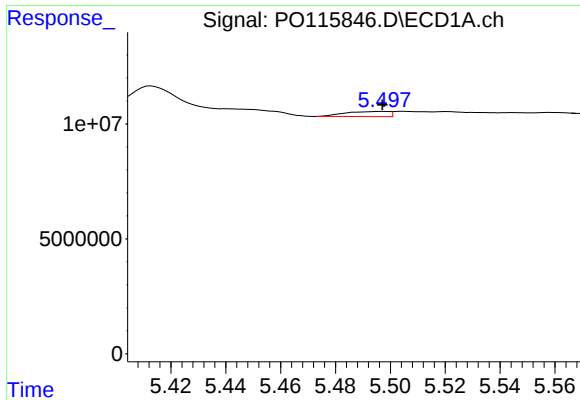

#13 AR-1232-3


R.T.: 5.497 min
Delta R.T.: 0.000 min
Response: 2450968
Conc: 15.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

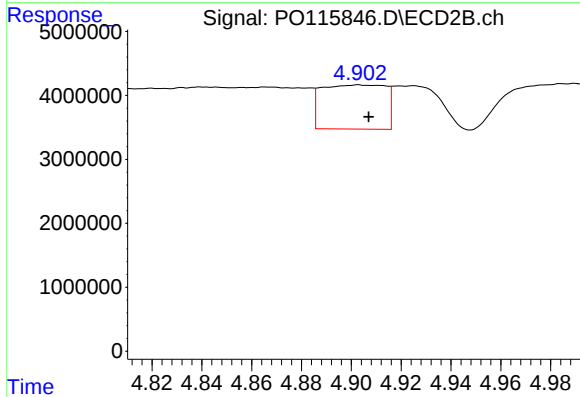


#13 AR-1232-3

R.T.: 4.903 min
Delta R.T.: -0.004 min
Response: 12245987
Conc: 187.34 ng/ml

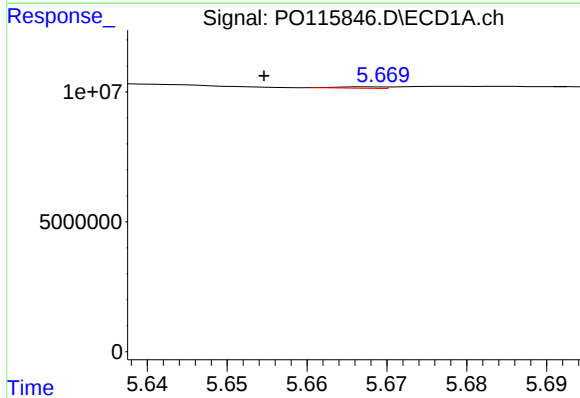


#14 AR-1232-4

R.T.: 5.667 min
Delta R.T.: 0.013 min
Response: 209266
Conc: 2.99 ng/ml

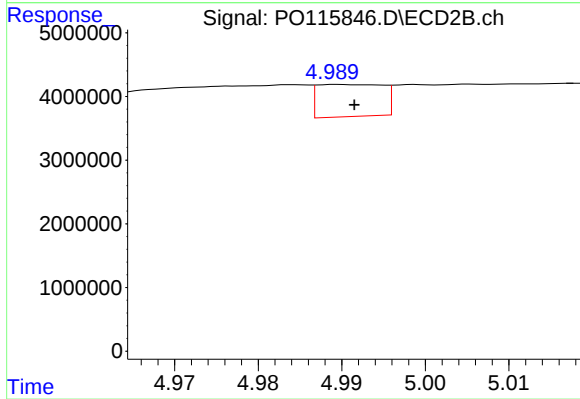

#14 AR-1232-4


R.T.: 4.990 min
Delta R.T.: -0.002 min
Response: 2748132
Conc: 53.54 ng/ml

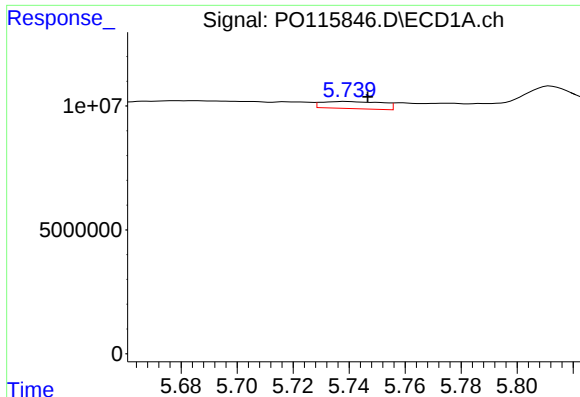

#15 AR-1232-5


R.T.: 5.739 min
Delta R.T.: -0.008 min
Response: 4351917
Conc: 83.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

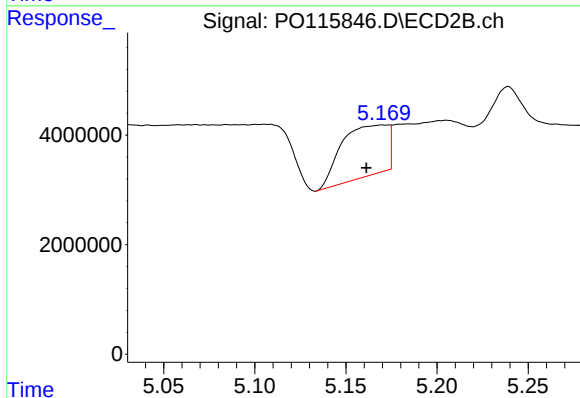


#15 AR-1232-5

R.T.: 5.170 min
Delta R.T.: 0.009 min
Response: 16436823
Conc: 300.23 ng/ml

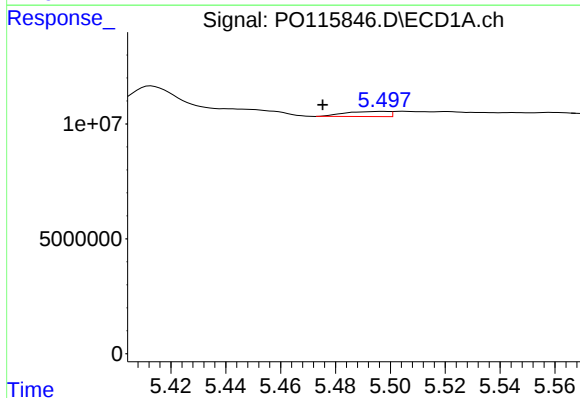


#16 AR-1242-1

R.T.: 5.497 min
Delta R.T.: 0.022 min
Response: 2450968
Conc: 12.34 ng/ml

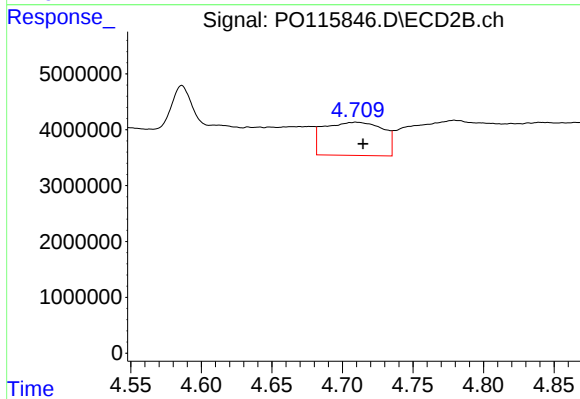

#16 AR-1242-1


R.T.: 4.709 min
Delta R.T.: -0.005 min
Response: 17339523
Conc: 121.78 ng/ml

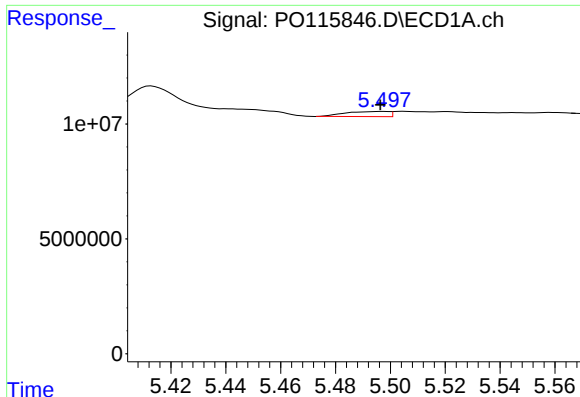

#17 AR-1242-2


R.T.: 5.497 min
Delta R.T.: 0.001 min
Response: 2450968
Conc: 8.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

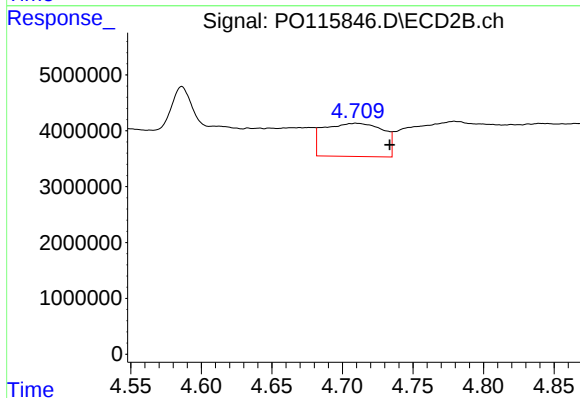


#17 AR-1242-2

R.T.: 4.709 min
Delta R.T.: -0.024 min
Response: 17339523
Conc: 82.82 ng/ml

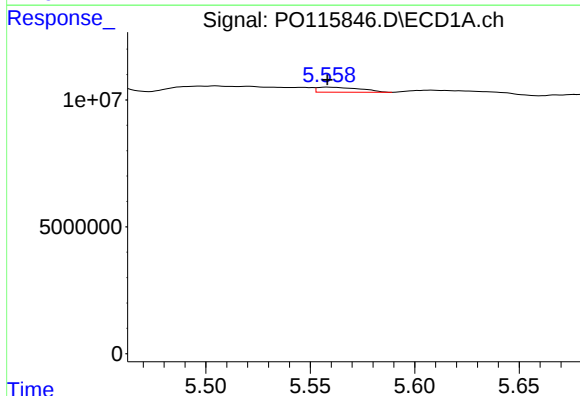


#18 AR-1242-3

R.T.: 5.558 min
Delta R.T.: 0.000 min
Response: 2832473
Conc: 16.78 ng/ml

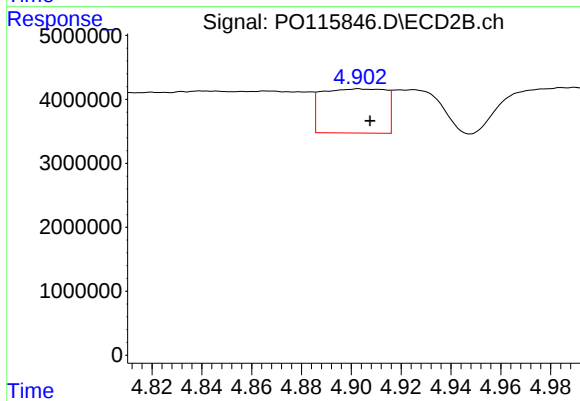

#18 AR-1242-3


R.T.: 4.903 min
Delta R.T.: -0.005 min
Response: 12245987
Conc: 102.53 ng/ml

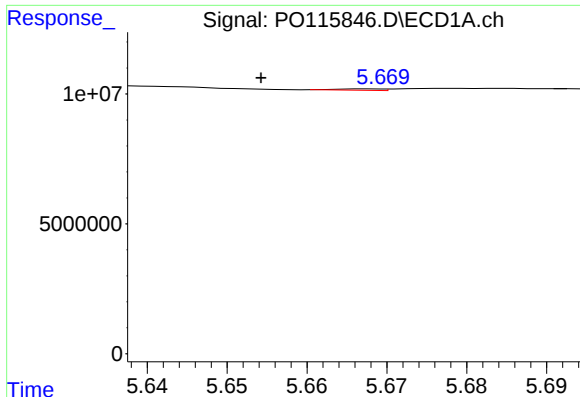

#19 AR-1242-4


R.T.: 5.667 min
Delta R.T.: 0.013 min
Response: 209266
Conc: 1.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

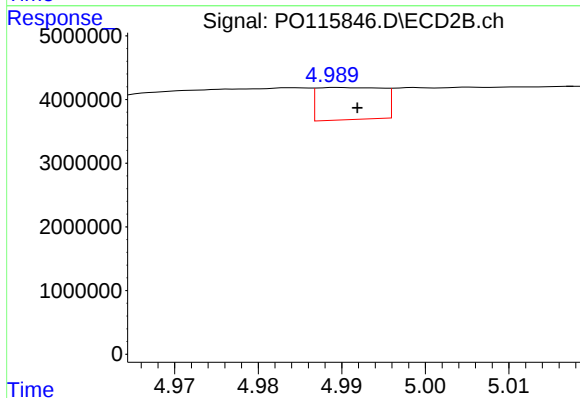


#19 AR-1242-4

R.T.: 4.990 min
Delta R.T.: -0.002 min
Response: 2748132
Conc: 25.19 ng/ml

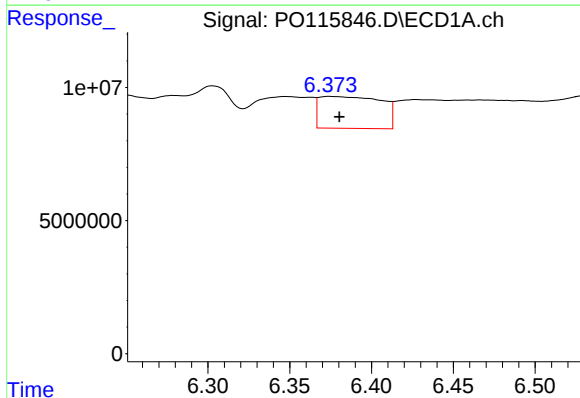


#20 AR-1242-5

R.T.: 6.374 min
Delta R.T.: -0.006 min
Response: 31639823
Conc: 208.92 ng/ml

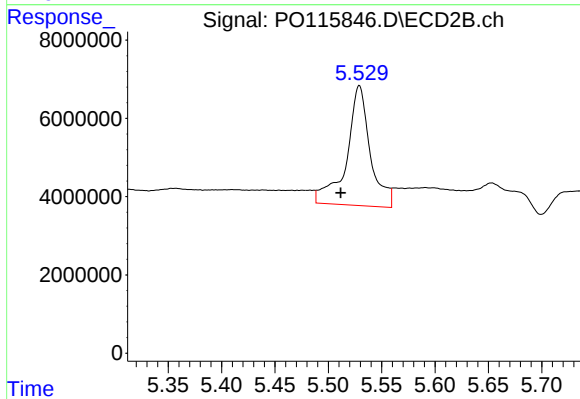

#20 AR-1242-5


R.T.: 5.529 min
Delta R.T.: 0.017 min
Response: 47227594
Conc: 341.92 ng/ml

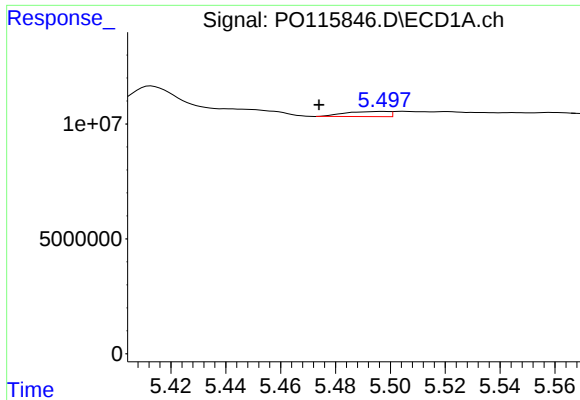

#21 AR-1248-1


R.T.: 5.497 min
Delta R.T.: 0.023 min
Response: 2450968
Conc: 16.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

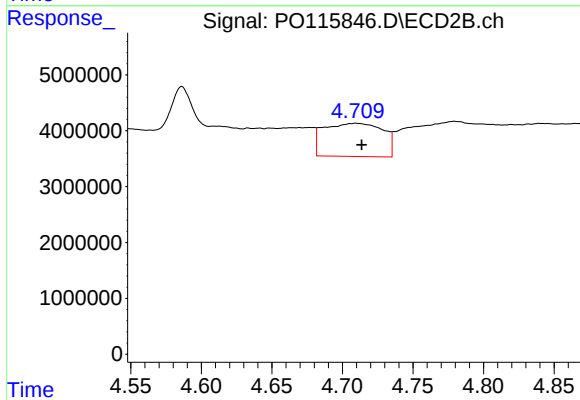


#21 AR-1248-1

R.T.: 4.709 min
Delta R.T.: -0.004 min
Response: 17339523
Conc: 155.05 ng/ml

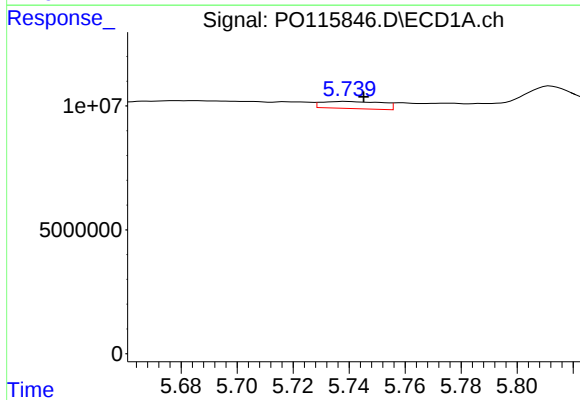


#22 AR-1248-2

R.T.: 5.739 min
Delta R.T.: -0.006 min
Response: 4351917
Conc: 21.67 ng/ml

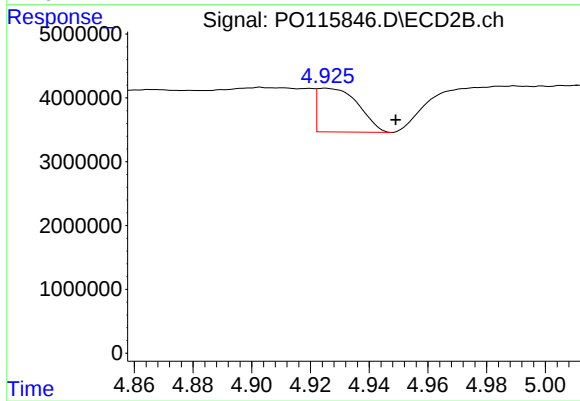

#22 AR-1248-2


R.T.: 4.925 min
Delta R.T.: -0.024 min
Response: 6577770
Conc: 43.19 ng/ml

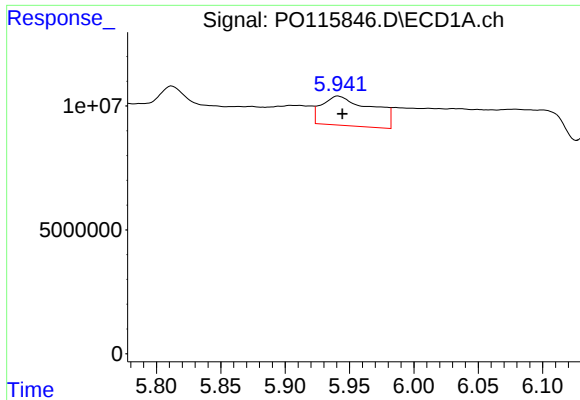

#23 AR-1248-3


R.T.: 5.941 min
Delta R.T.: -0.003 min
Response: 32152505
Conc: 130.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

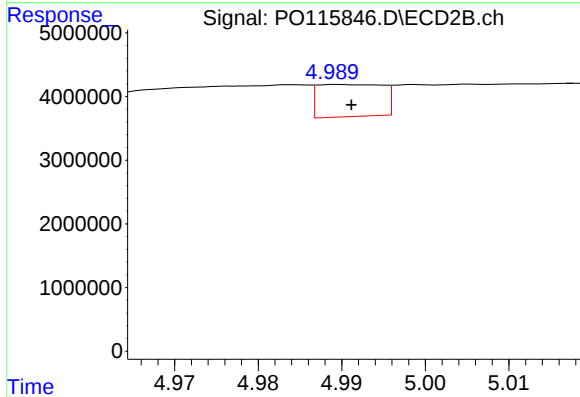


#23 AR-1248-3

R.T.: 4.990 min
Delta R.T.: -0.002 min
Response: 2748132
Conc: 17.12 ng/ml

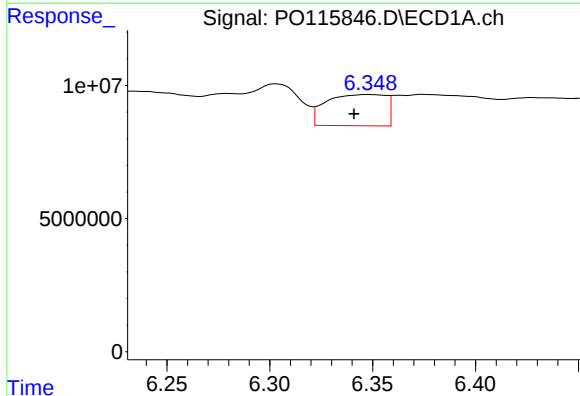


#24 AR-1248-4

R.T.: 6.348 min
Delta R.T.: 0.007 min
Response: 23602147
Conc: 80.05 ng/ml

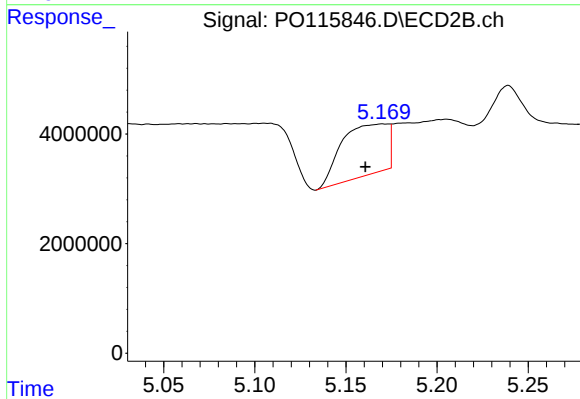

#24 AR-1248-4


R.T.: 5.170 min
Delta R.T.: 0.009 min
Response: 16436823
Conc: 87.83 ng/ml

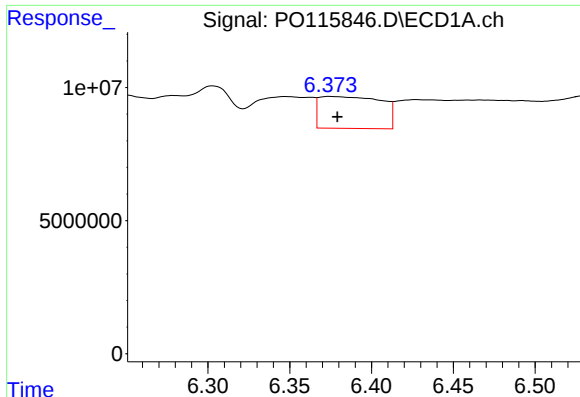

#25 AR-1248-5


R.T.: 6.374 min
Delta R.T.: -0.005 min
Response: 31639823
Conc: 122.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

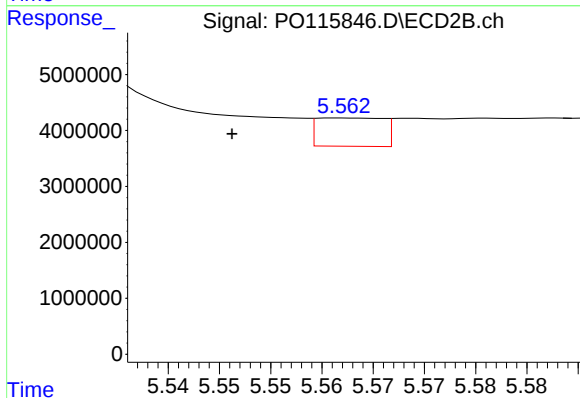


#25 AR-1248-5

R.T.: 5.562 min
Delta R.T.: 0.011 min
Response: 2277731
Conc: 11.51 ng/ml

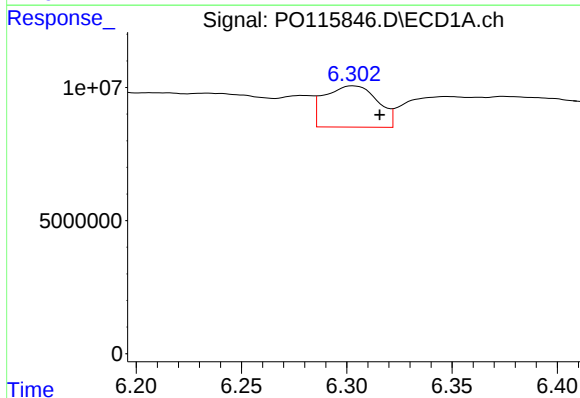


#26 AR-1254-1

R.T.: 6.303 min
Delta R.T.: -0.013 min
Response: 27170036
Conc: 105.02 ng/ml

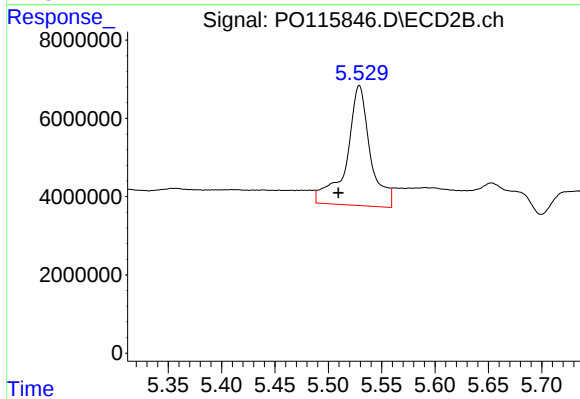

#26 AR-1254-1


R.T.: 5.529 min
Delta R.T.: 0.020 min
Response: 47227594
Conc: 161.59 ng/ml

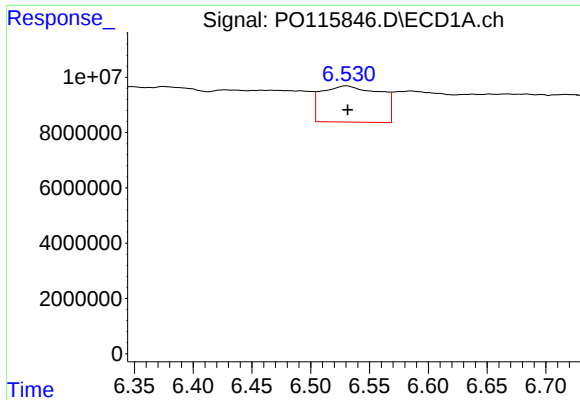

#27 AR-1254-2


R.T.: 6.530 min
Delta R.T.: 0.000 min
Response: 45418220
Conc: 112.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

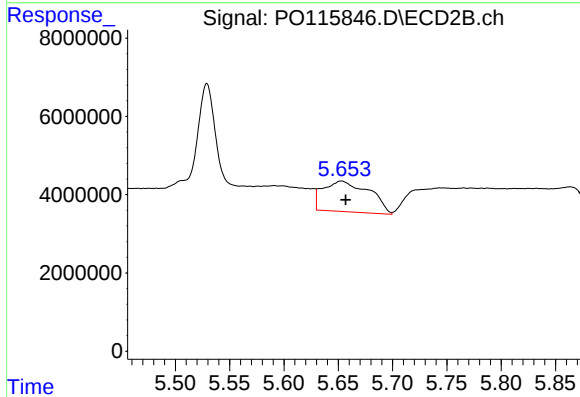


#27 AR-1254-2

R.T.: 5.653 min
Delta R.T.: -0.004 min
Response: 23179591
Conc: 92.05 ng/ml

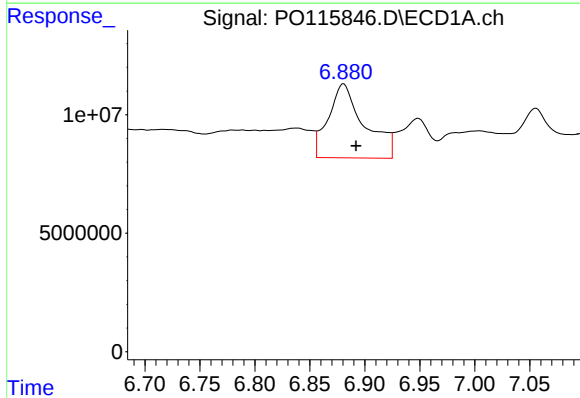


#28 AR-1254-3

R.T.: 6.881 min
Delta R.T.: -0.011 min
Response: 71030256
Conc: 173.01 ng/ml

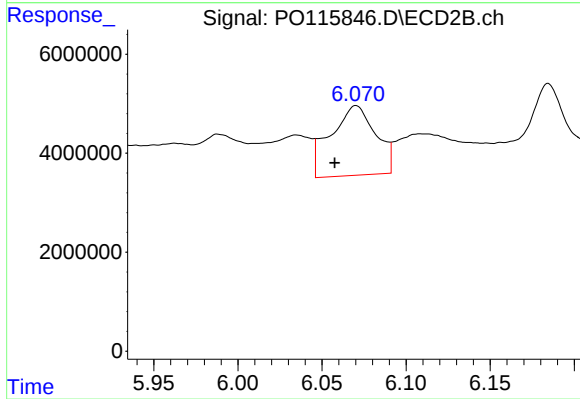

#28 AR-1254-3


R.T.: 6.070 min
Delta R.T.: 0.013 min
Response: 26261243
Conc: 66.72 ng/ml

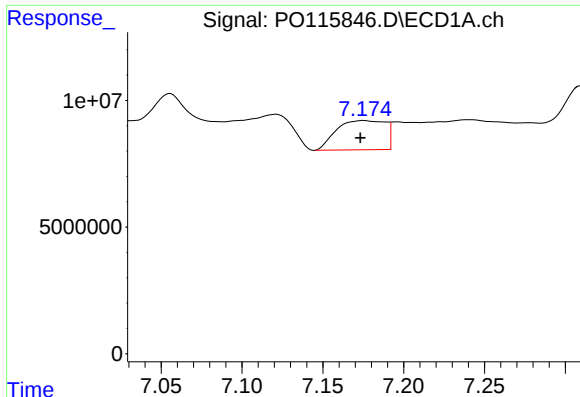

#29 AR-1254-4


R.T.: 7.175 min
Delta R.T.: 0.002 min
Response: 24193459
Conc: 69.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

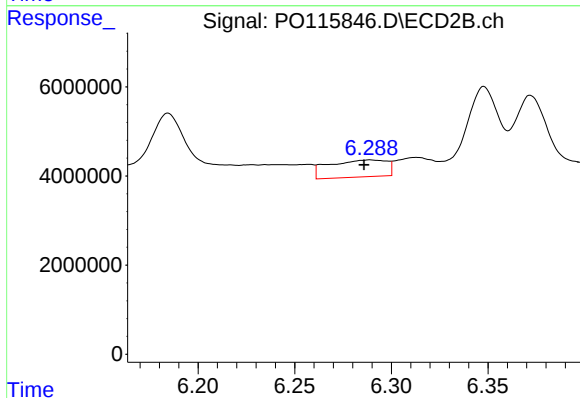


#29 AR-1254-4

R.T.: 6.289 min
Delta R.T.: 0.003 min
Response: 7924870
Conc: 29.62 ng/ml

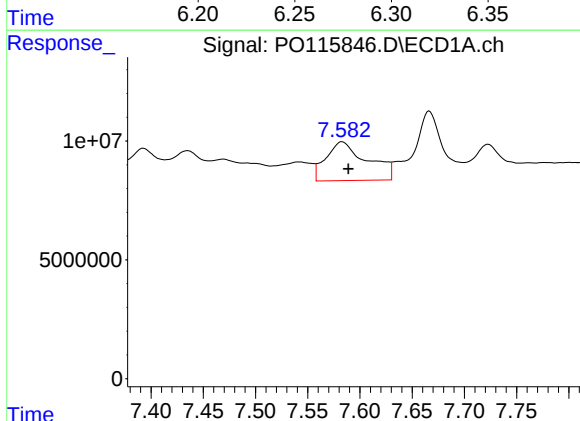


#30 AR-1254-5

R.T.: 7.583 min
Delta R.T.: -0.006 min
Response: 44786373
Conc: 138.21 ng/ml

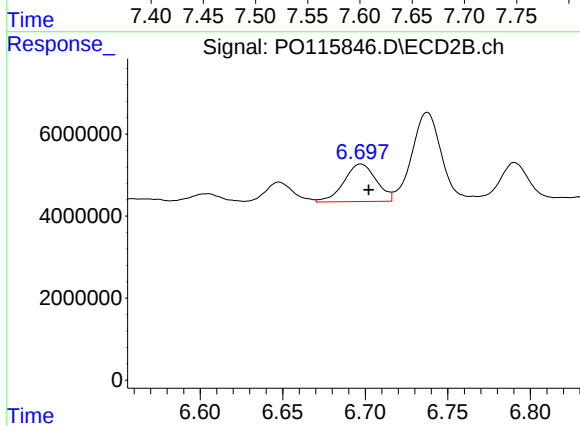

#30 AR-1254-5


R.T.: 6.697 min
Delta R.T.: -0.005 min
Response: 12464344
Conc: 34.86 ng/ml

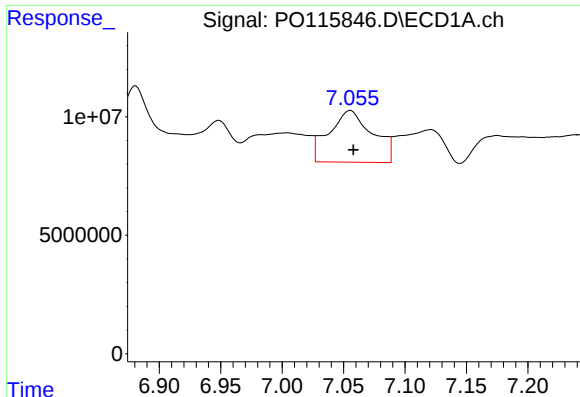

#31 AR-1260-1


R.T.: 7.056 min
Delta R.T.: -0.002 min
Response: 53857034
Conc: 185.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

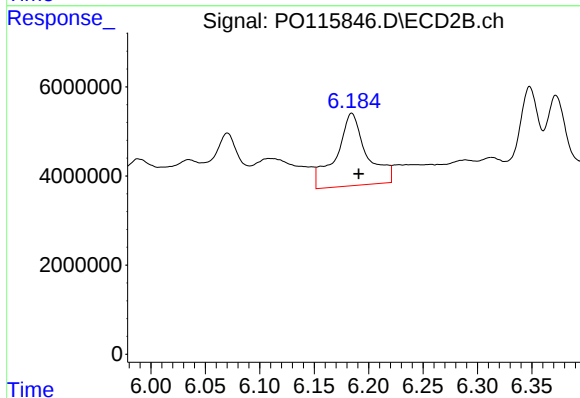


#31 AR-1260-1

R.T.: 6.185 min
Delta R.T.: -0.006 min
Response: 31603327
Conc: 120.55 ng/ml

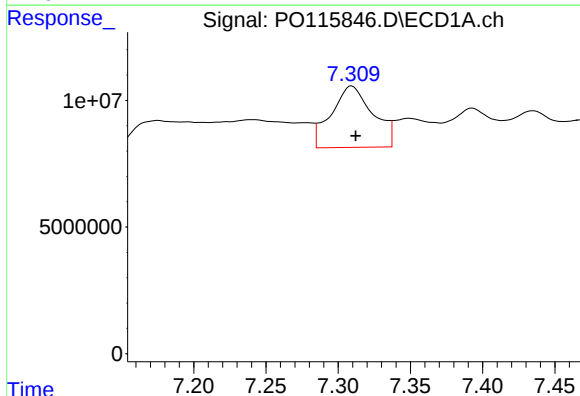


#32 AR-1260-2

R.T.: 7.309 min
Delta R.T.: -0.003 min
Response: 48685510
Conc: 111.22 ng/ml

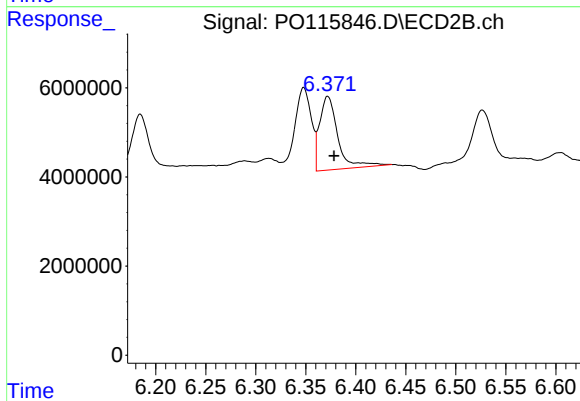

#32 AR-1260-2


R.T.: 6.372 min
Delta R.T.: -0.006 min
Response: 20835178
Conc: 59.45 ng/ml

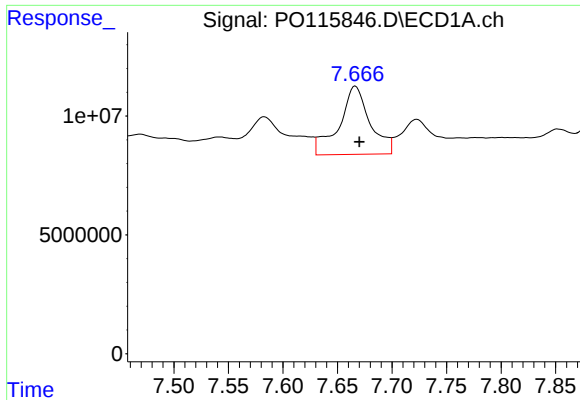

#33 AR-1260-3


R.T.: 7.666 min
Delta R.T.: -0.004 min
Response: 56594240
Conc: 168.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

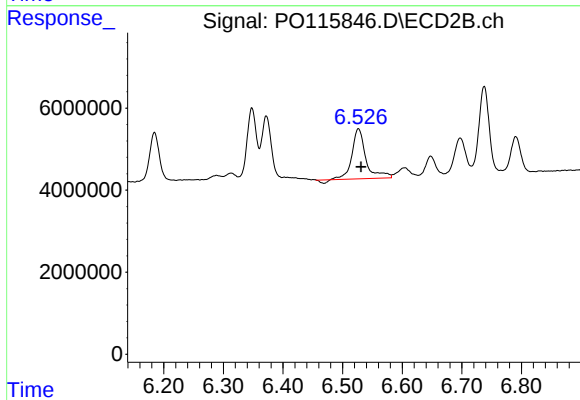


#33 AR-1260-3

R.T.: 6.527 min
Delta R.T.: -0.004 min
Response: 19470277
Conc: 60.60 ng/ml

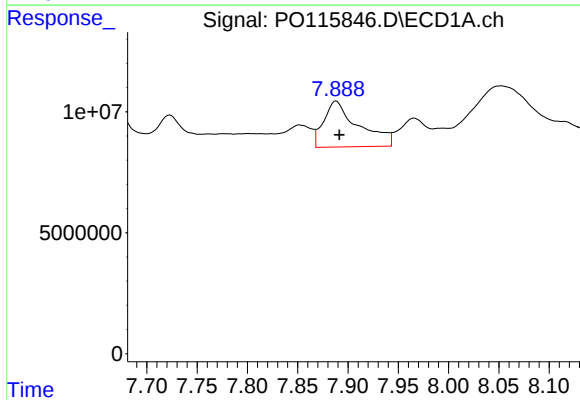


#34 AR-1260-4

R.T.: 7.888 min
Delta R.T.: -0.003 min
Response: 45566138
Conc: 148.20 ng/ml

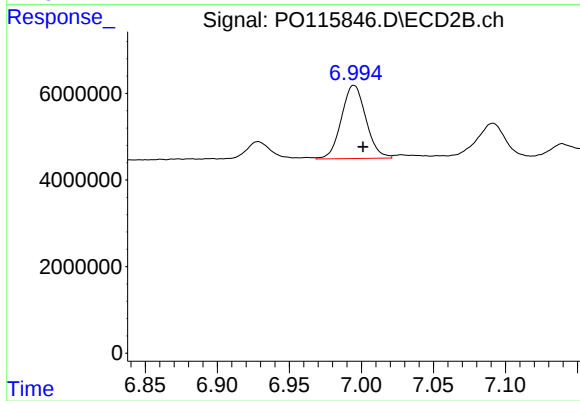

#34 AR-1260-4


R.T.: 6.995 min
Delta R.T.: -0.006 min
Response: 20048459
Conc: 78.06 ng/ml

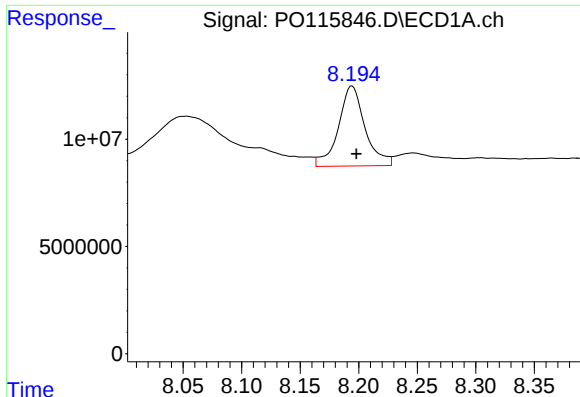

#35 AR-1260-5


R.T.: 8.194 min
Delta R.T.: -0.004 min
Response: 59064142
Conc: 81.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

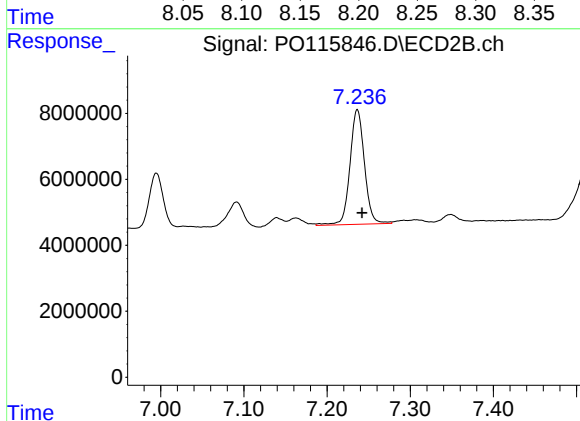


#35 AR-1260-5

R.T.: 7.236 min
Delta R.T.: -0.006 min
Response: 42212342
Conc: 60.19 ng/ml

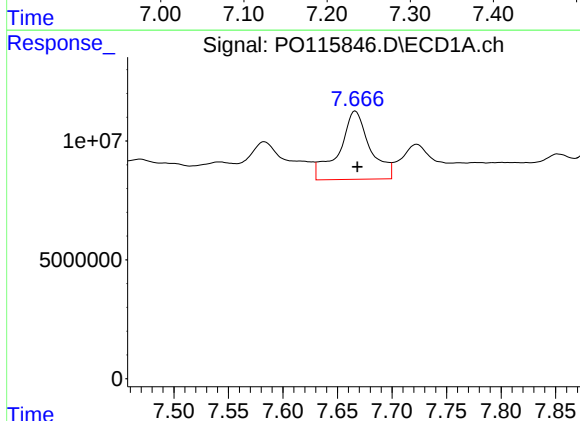


#36 AR-1262-1

R.T.: 7.666 min
Delta R.T.: -0.002 min
Response: 56594240
Conc: 229.26 ng/ml

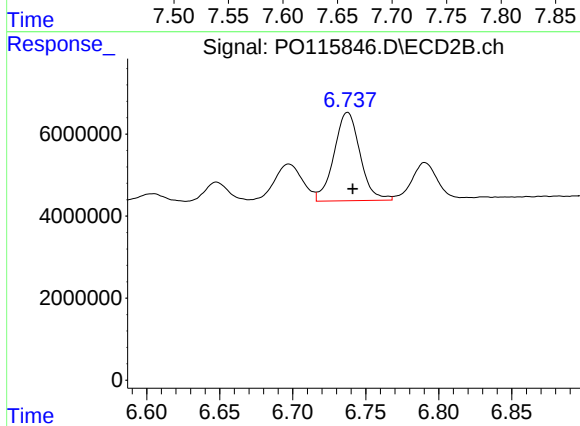

#36 AR-1262-1


R.T.: 6.738 min
Delta R.T.: -0.003 min
Response: 26755158
Conc: 125.59 ng/ml

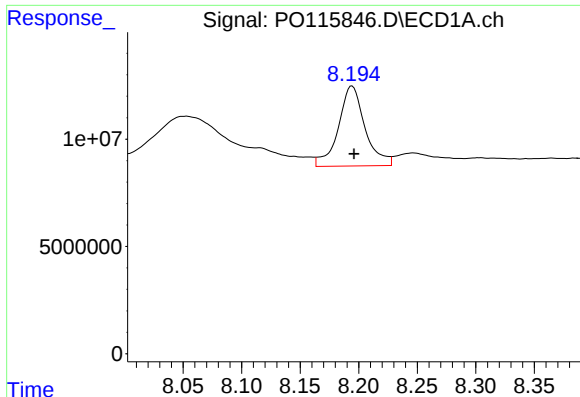

#37 AR-1262-2


R.T.: 8.194 min
Delta R.T.: -0.002 min
Response: 59064142
Conc: 149.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

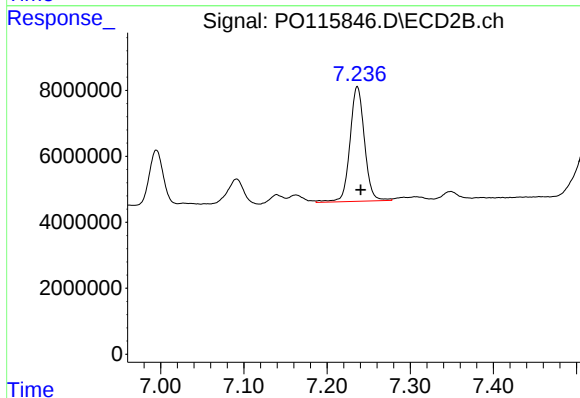


#37 AR-1262-2

R.T.: 7.236 min
Delta R.T.: -0.004 min
Response: 42212342
Conc: 121.19 ng/ml

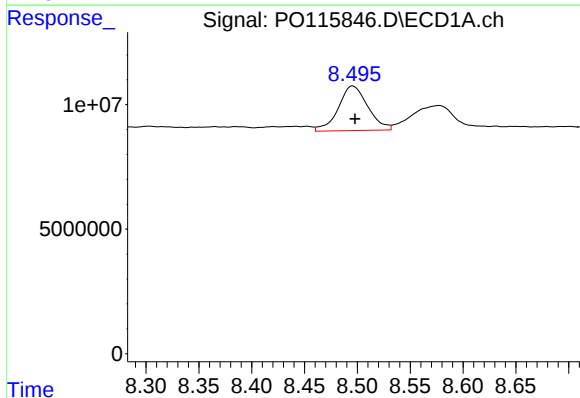


#38 AR-1262-3

R.T.: 8.496 min
Delta R.T.: -0.002 min
Response: 34868460
Conc: 136.83 ng/ml

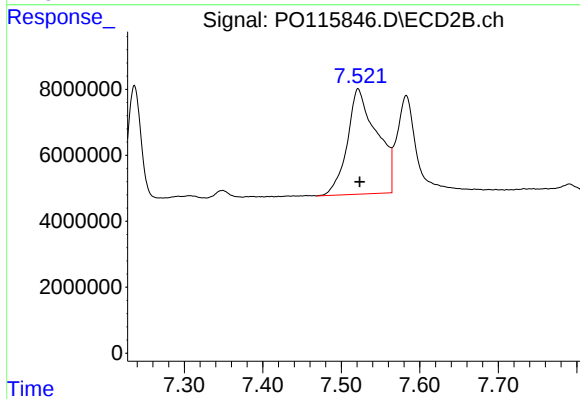

#38 AR-1262-3


R.T.: 7.521 min
Delta R.T.: -0.002 min
Response: 83152459
Conc: 531.70 ng/ml

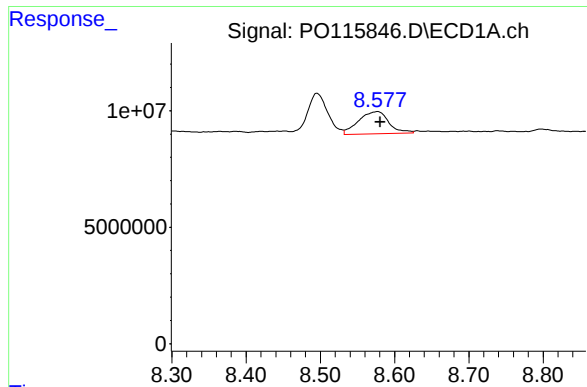

#39 AR-1262-4


R.T.: 8.577 min
Delta R.T.: -0.004 min
Response: 27002876
Conc: 139.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

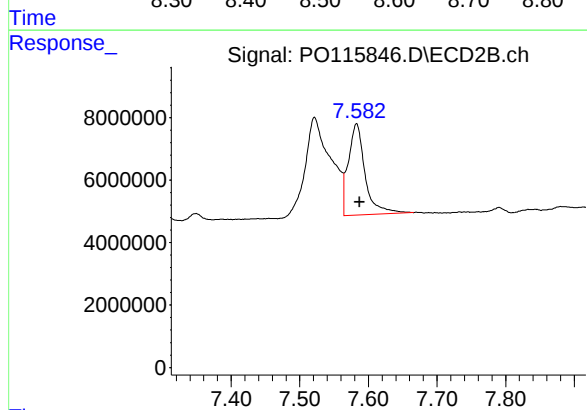


#39 AR-1262-4

R.T.: 7.583 min
Delta R.T.: -0.004 min
Response: 49485912
Conc: 200.05 ng/ml

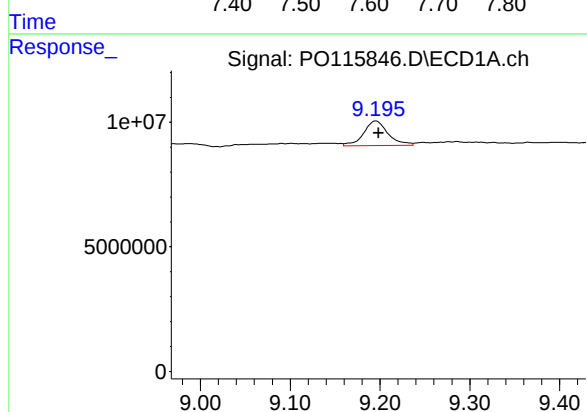


#40 AR-1262-5

R.T.: 9.196 min
Delta R.T.: -0.003 min
Response: 18577082
Conc: 137.92 ng/ml

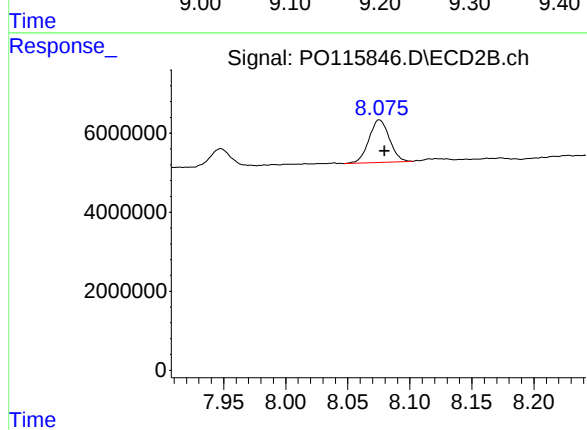

#40 AR-1262-5


R.T.: 8.075 min
Delta R.T.: -0.004 min
Response: 12321517
Conc: 110.53 ng/ml

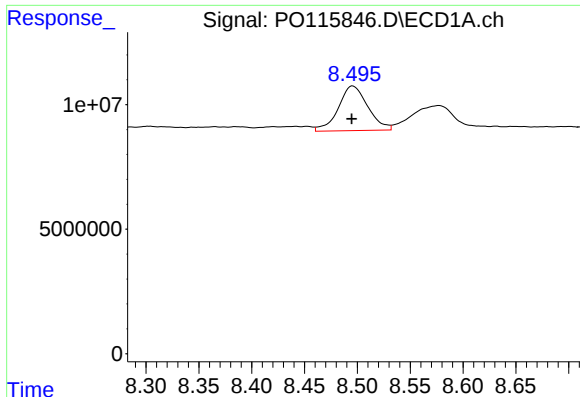

#41 AR-1268-1


R.T.: 8.496 min
Delta R.T.: 0.000 min
Response: 34868460
Conc: 35.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

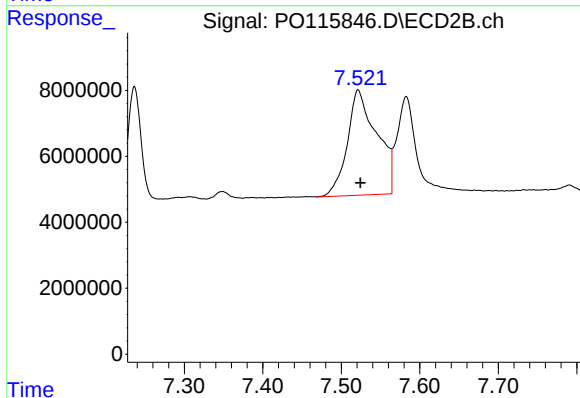


#41 AR-1268-1

R.T.: 7.521 min
Delta R.T.: -0.003 min
Response: 83152459
Conc: 93.86 ng/ml

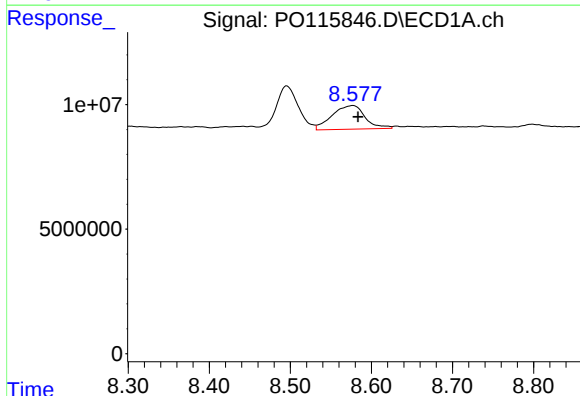


#42 AR-1268-2

R.T.: 8.577 min
Delta R.T.: -0.006 min
Response: 27002876
Conc: 31.57 ng/ml

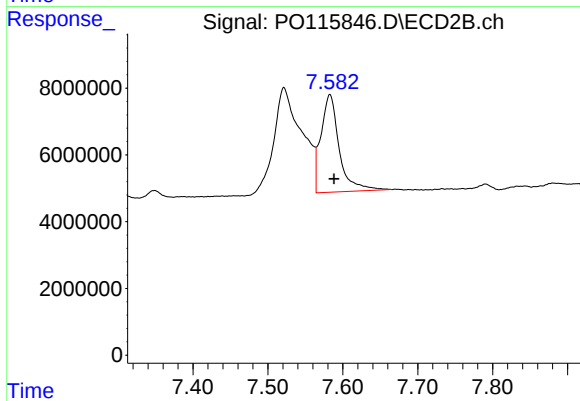

#42 AR-1268-2


R.T.: 7.583 min
Delta R.T.: -0.006 min
Response: 49485912
Conc: 66.06 ng/ml

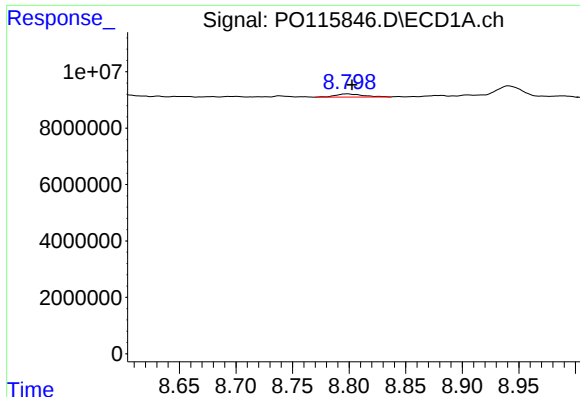

#43 AR-1268-3


R.T.: 8.798 min
Delta R.T.: -0.004 min
Response: 1833526
Conc: 2.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

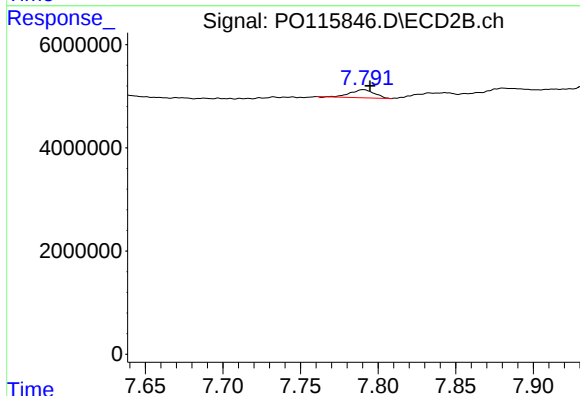


#43 AR-1268-3

R.T.: 7.790 min
Delta R.T.: -0.004 min
Response: 1714098
Conc: 2.69 ng/ml

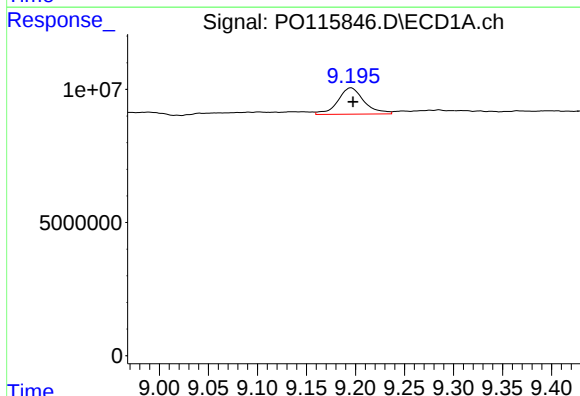


#44 AR-1268-4

R.T.: 9.196 min
Delta R.T.: -0.002 min
Response: 18577082
Conc: 59.50 ng/ml

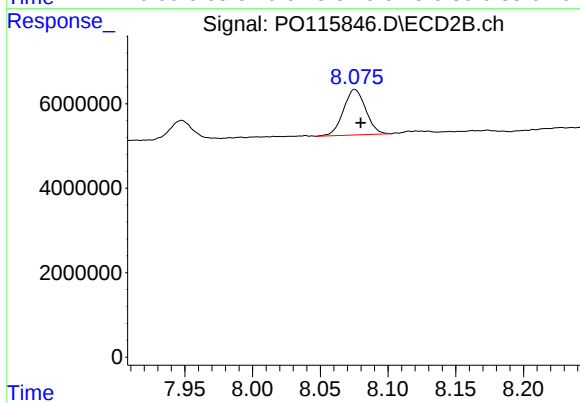

#44 AR-1268-4


R.T.: 8.075 min
Delta R.T.: -0.004 min
Response: 12321517
Conc: 47.83 ng/ml

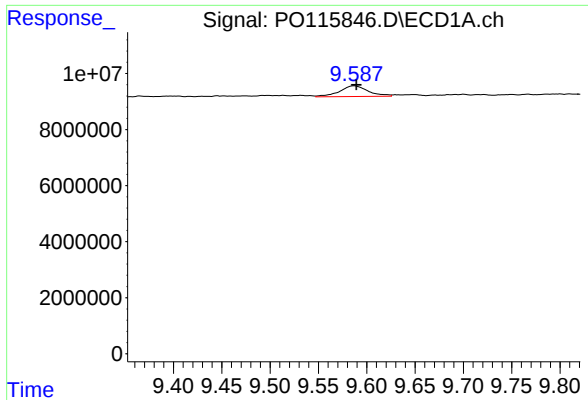

#45 AR-1268-5

R.T.: 9.587 min
Delta R.T.: -0.002 min
Response: 7901728
Conc: 3.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

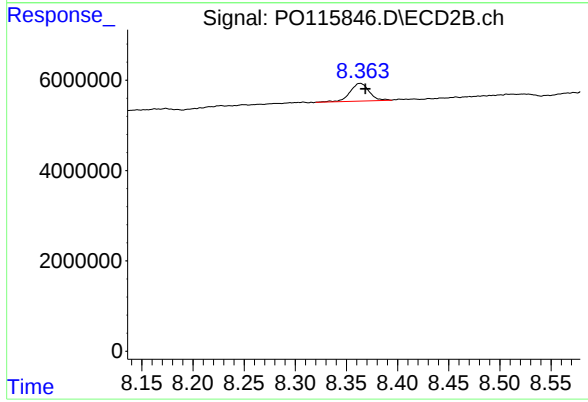

#45 AR-1268-5

R.T.: 8.363 min
Delta R.T.: -0.005 min
Response: 5087300
Conc: 3.02 ng/ml