

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO121225\
 Data File : PO115847.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Dec 2025 11:14
 Operator : YP/AJ
 Sample : Q3530-09
 Misc : AR1268 25PPB WATER MDL
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 MDL-WATER-03-QT4-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 02:47:39 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO120425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 05 02:11:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.332	3.634	204.4E6	125.3E6	26.318	25.720
2)	SA Decachlor...	9.905	8.615	148.3E6	111.3E6	28.195	25.871
Target Compounds							
3)	L1 AR-1016-1	5.481	4.716	750220	1031933	3.017	5.585 #
4)	L1 AR-1016-2	5.495	4.735	1410175	1372019	3.703	5.191 #
5)	L1 AR-1016-3	5.552	4.906	572934	1553429	2.680	10.265 #
6)	L1 AR-1016-4	5.662	4.927	99375	2318371	0.557	20.570 #
7)	L1 AR-1016-5	5.953	5.165	2466911	7702719	14.062	52.635 #
8)	L2 AR-1221-1	4.550	3.834	321959	20320	3.965	0.360 #
9)	L2 AR-1221-2	4.630	3.932	4046940	3110772	64.218	73.292
10)	L2 AR-1221-3	4.683	4.008	1208672	275526	6.473	2.143 #
11)	L3 AR-1232-1	4.683	4.008	1208672	275526	8.076	2.579 #
12)	L3 AR-1232-2	5.211	4.735	558622	1372019	6.909	12.362 #
13)	L3 AR-1232-3	5.495	4.906	1410175	1553429	9.163	23.765 #
14)	L3 AR-1232-4	5.662	4.987	99375	1159015	1.419	22.580 #
15)	L3 AR-1232-5	5.757	5.165	265831	7702719	5.118	140.694 #
16)	L4 AR-1242-1	5.481	4.716	750220	1031933	3.777	7.247 #
17)	L4 AR-1242-2	5.495	4.735	1410175	1372019	4.815	6.553 #
18)	L4 AR-1242-3	5.552	4.906	572934	1553429	3.394	13.006 #
19)	L4 AR-1242-4	5.662	4.987	99375	1159015	0.727	10.624 #
20)	L4 AR-1242-5	6.381	5.496	5305027	658263	35.030	4.766 #
21)	L5 AR-1248-1	5.481	4.716	750220	1031933	4.943	9.228 #
22)	L5 AR-1248-2	5.737	4.927	569610	2318371	2.836	15.223 #
23)	L5 AR-1248-3	5.938	4.987	1174811	1159015	4.764	7.220 #
24)	L5 AR-1248-4	6.350	5.165	10130286	7702719	34.357	41.159
25)	L5 AR-1248-5	6.381	5.563	5305027	797274	20.489	4.028 #
26)	L6 AR-1254-1	6.303	5.496	8289582	658263	32.042	2.252 #
27)	L6 AR-1254-2	6.530	5.657	2387563	1043425	5.933	4.144 #
28)	L6 AR-1254-3	6.880	6.059	42224183	5260350	102.844	13.365 #
29)	L6 AR-1254-4	7.174	6.290	1869046	4541759	5.385	16.974 #
30)	L6 AR-1254-5	7.605	6.707	1804000	465125	5.567	1.301 #
31)	L7 AR-1260-1	7.056	6.195	1983406	797291	6.846	3.041 #
32)	L7 AR-1260-2	7.313	6.376	2098274	644979	4.794	1.840 #
33)	L7 AR-1260-3	7.667	6.532	9759395	1128375	28.995	3.512 #
34)	L7 AR-1260-4	7.886	6.993	1137677	8234460	3.700	32.061 #
35)	L7 AR-1260-5	8.195	7.236	6817882	3808550	9.359	5.431 #
36)	L8 AR-1262-1	7.667	6.736	9759395	6037685	39.535	28.340 #
37)	L8 AR-1262-2	8.195	7.236	6817882	3808550	17.221	10.934 #
38)	L8 AR-1262-3	8.493	7.520	25815827	93212951	101.309	596.027 #
39)	L8 AR-1262-4	8.582	7.583	21816156	38530215	112.625	155.759 #
40)	L8 AR-1262-5	9.195	8.076	10646820	5854762	79.047	52.521 #
41)	L9 AR-1268-1	8.493	7.520	25815827	93212951	25.927	105.212 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO121225\
Data File : PO115847.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Dec 2025 11:14
Operator : YP/AJ
Sample : Q3530-09
Misc : AR1268 25PPB WATER MDL
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_0
ClientSampleId :
MDL-WATER-03-QT4-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 02:47:39 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO120425.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 05 02:11:05 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.582	7.583	21816156	38530215	25.505	51.437 #
43)	L9 AR-1268-3	8.801	7.790	17303812	15214360	23.297	23.895
44)	L9 AR-1268-4	9.195	8.076	10646820	5854762	34.099	22.726 #
45)	L9 AR-1268-5	9.587	8.363	52845986	39831293	24.270	23.626



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121225\
Data File : PO115847.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Dec 2025 11:14
Operator : YP/AJ
Sample : Q3530-09
Misc : AR1268 25PPB WATER MDL
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 02:47:39 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120425.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 05 02:11:05 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

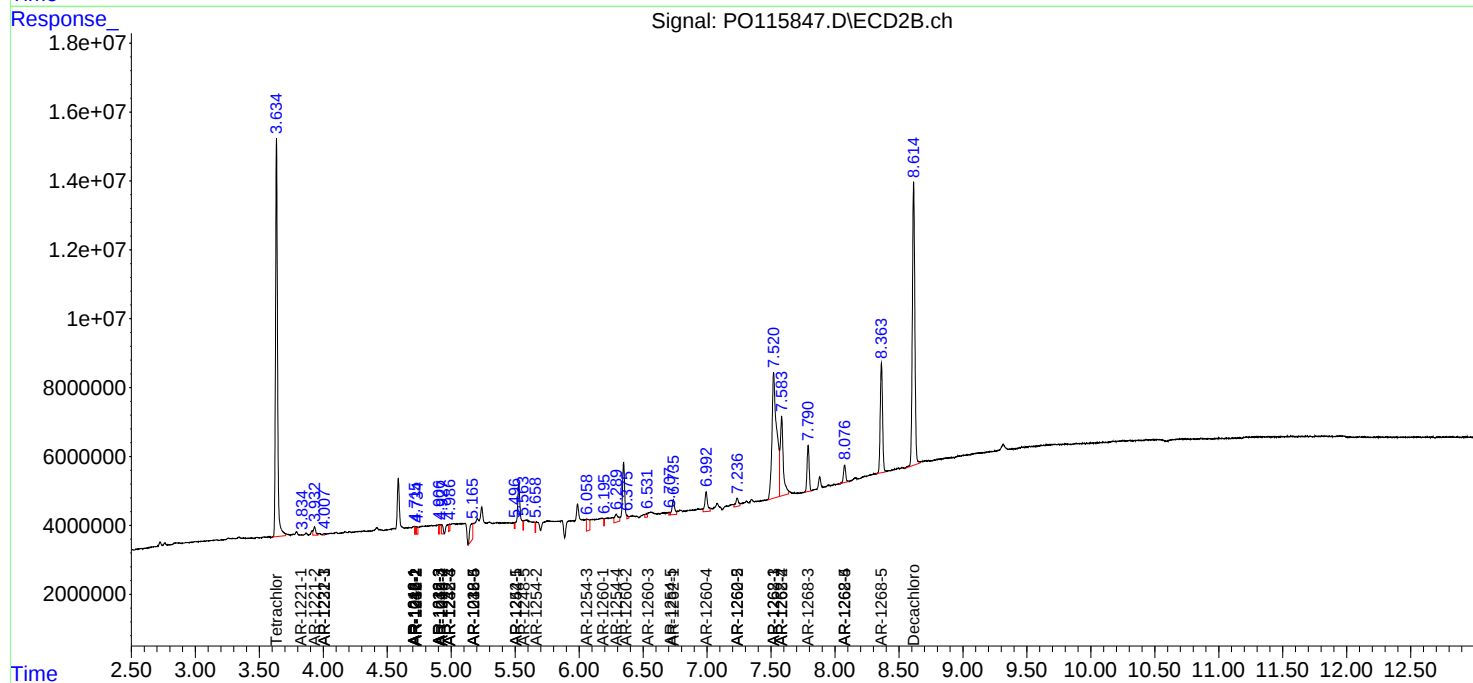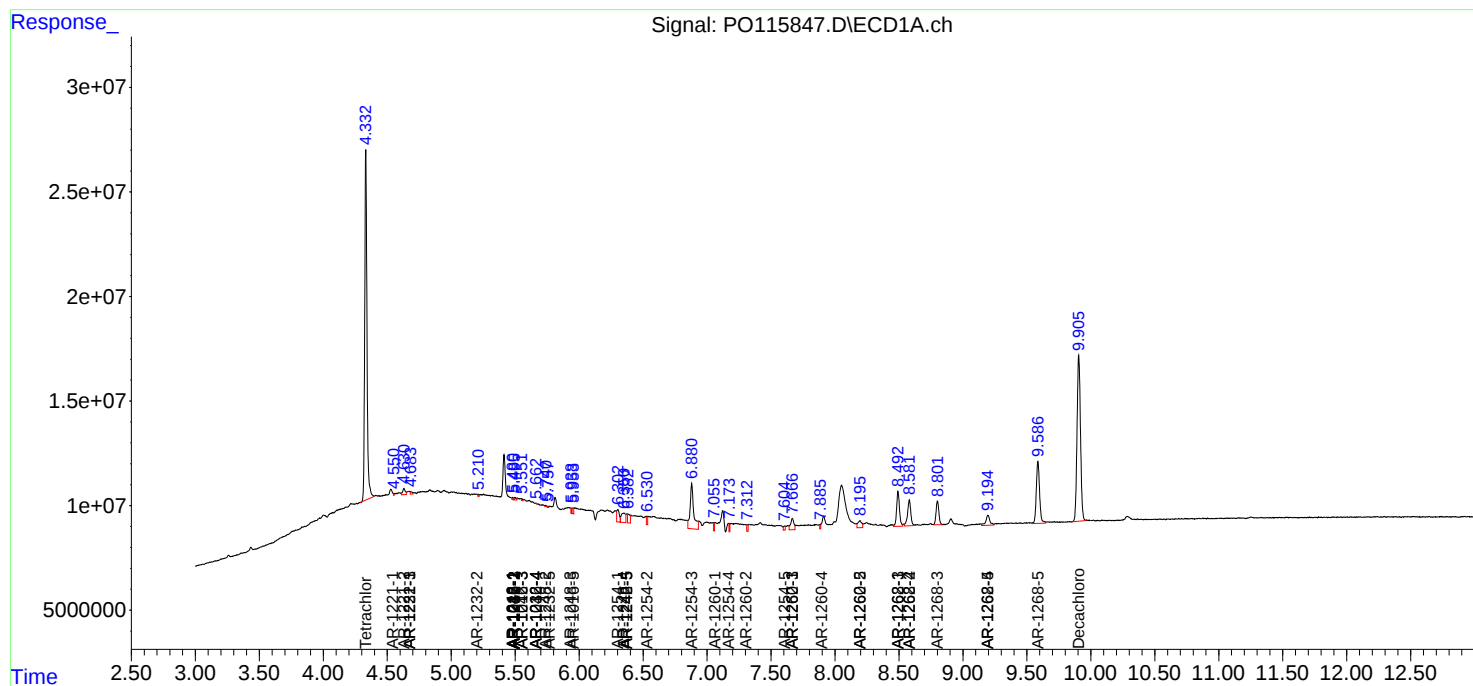


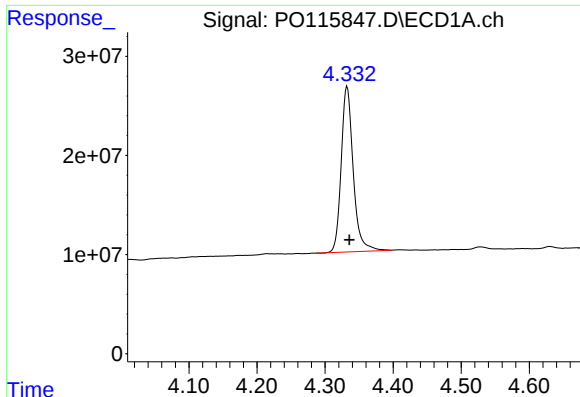

#1 Tetrachloro-m-xylene


R.T.: 4.332 min
Delta R.T.: -0.004 min
Response: 204417375
Conc: 26.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

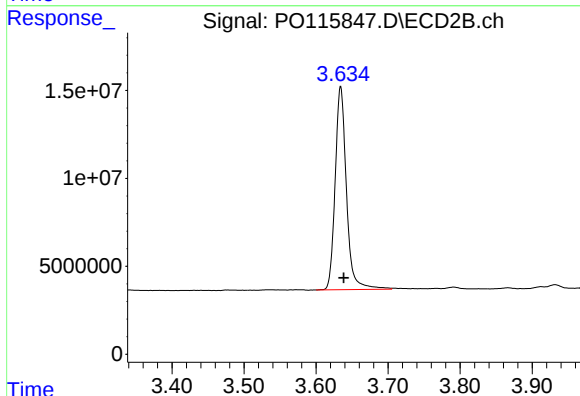


#1 Tetrachloro-m-xylene

R.T.: 3.634 min
Delta R.T.: -0.004 min
Response: 125342458
Conc: 25.72 ng/ml

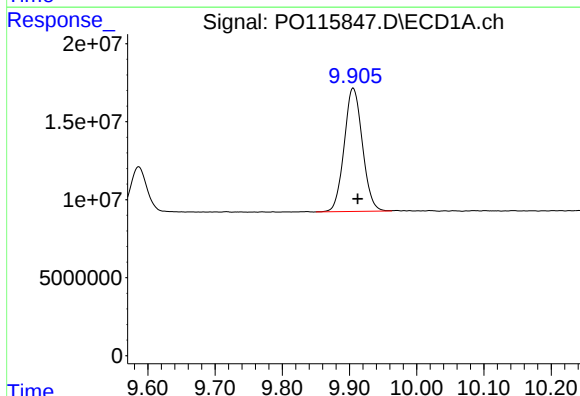


#2 Decachlorobiphenyl

R.T.: 9.905 min
Delta R.T.: -0.007 min
Response: 148333256
Conc: 28.19 ng/ml

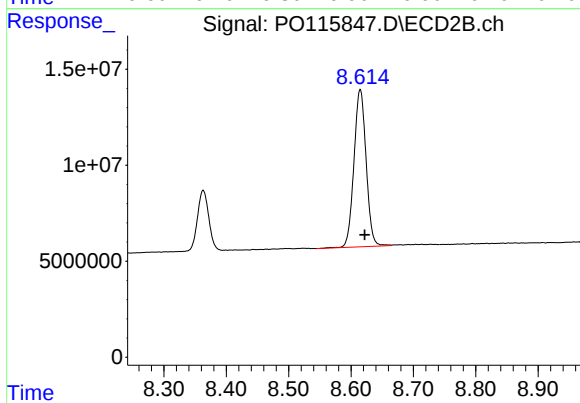

#2 Decachlorobiphenyl


R.T.: 8.615 min
Delta R.T.: -0.007 min
Response: 111250630
Conc: 25.87 ng/ml

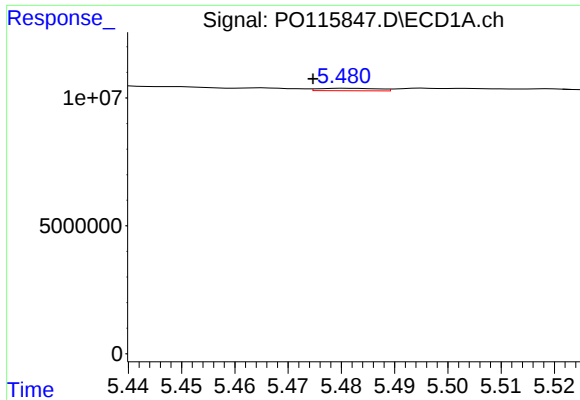

#3 AR-1016-1


R.T.: 5.481 min
Delta R.T.: 0.006 min
Response: 750220
Conc: 3.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

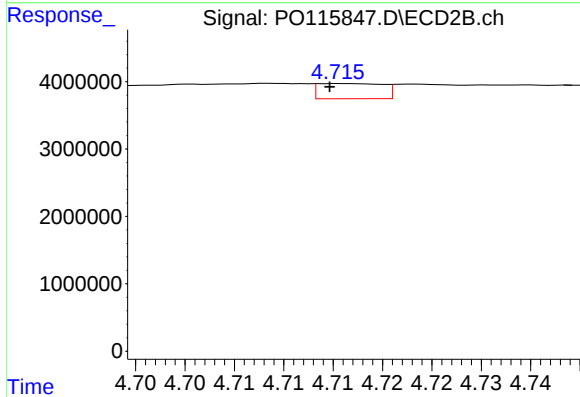


#3 AR-1016-1

R.T.: 4.716 min
Delta R.T.: 0.001 min
Response: 1031933
Conc: 5.59 ng/ml

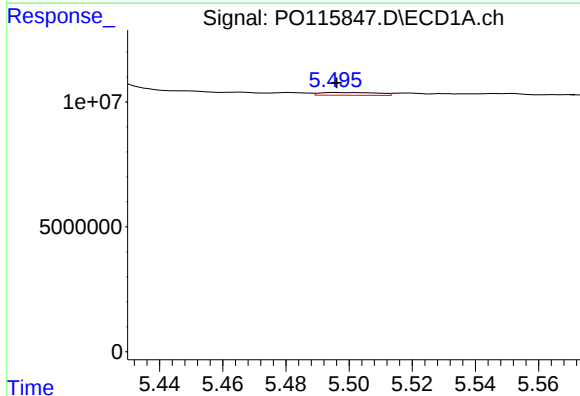


#4 AR-1016-2

R.T.: 5.495 min
Delta R.T.: 0.000 min
Response: 1410175
Conc: 3.70 ng/ml

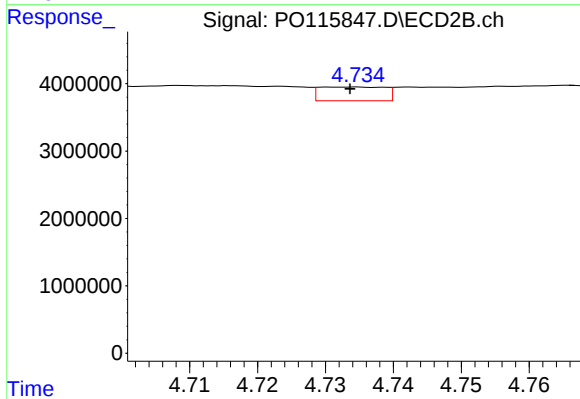

#4 AR-1016-2


R.T.: 4.735 min
Delta R.T.: 0.001 min
Response: 1372019
Conc: 5.19 ng/ml

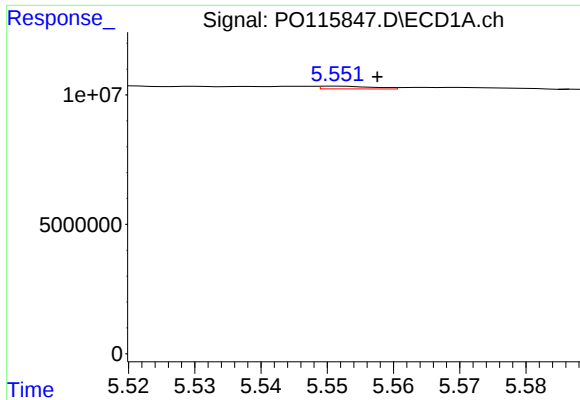

#5 AR-1016-3


R.T.: 5.552 min
Delta R.T.: -0.006 min
Response: 572934
Conc: 2.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

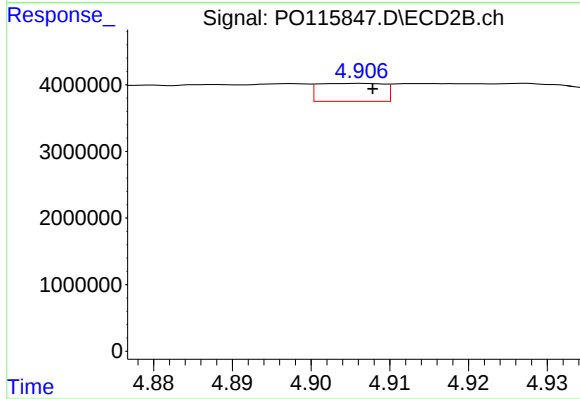


#5 AR-1016-3

R.T.: 4.906 min
Delta R.T.: -0.001 min
Response: 1553429
Conc: 10.26 ng/ml

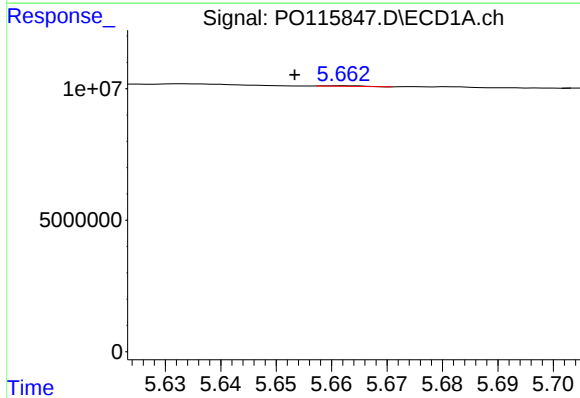


#6 AR-1016-4

R.T.: 5.662 min
Delta R.T.: 0.009 min
Response: 99375
Conc: 0.56 ng/ml

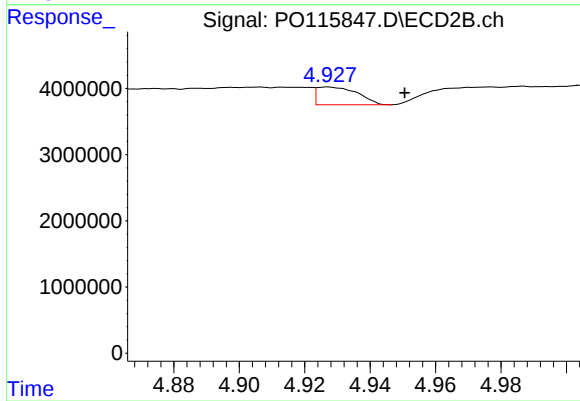

#6 AR-1016-4


R.T.: 4.927 min
Delta R.T.: -0.023 min
Response: 2318371
Conc: 20.57 ng/ml

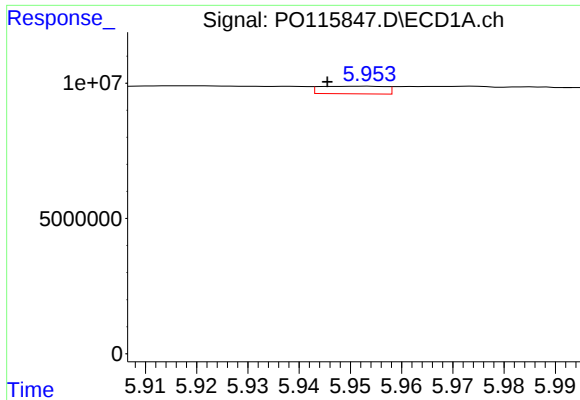

#7 AR-1016-5


R.T.: 5.953 min
Delta R.T.: 0.008 min
Response: 2466911
Conc: 14.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

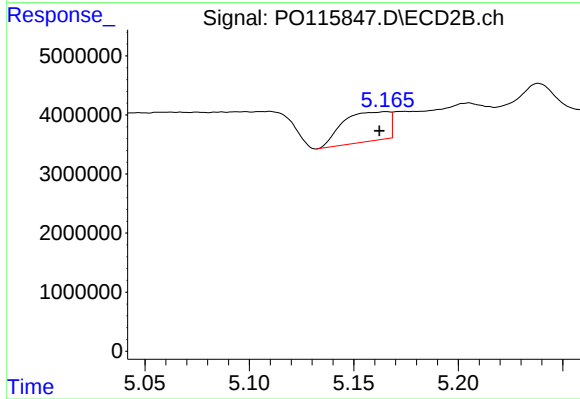


#7 AR-1016-5

R.T.: 5.165 min
Delta R.T.: 0.003 min
Response: 7702719
Conc: 52.64 ng/ml

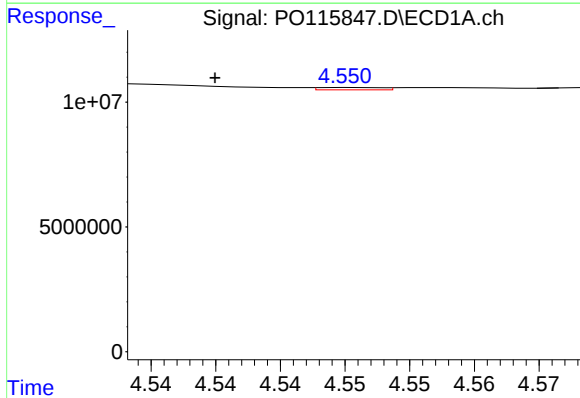


#8 AR-1221-1

R.T.: 4.550 min
Delta R.T.: 0.010 min
Response: 321959
Conc: 3.97 ng/ml

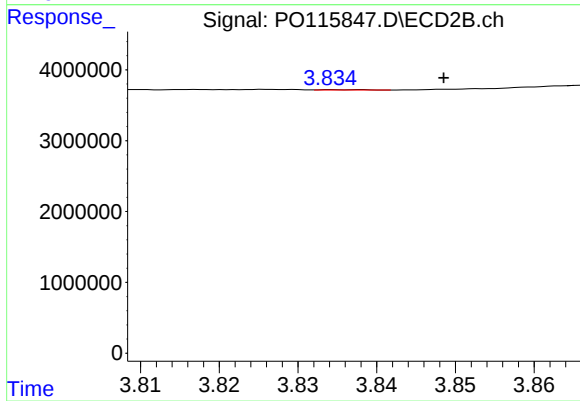

#8 AR-1221-1


R.T.: 3.834 min
Delta R.T.: -0.014 min
Response: 20320
Conc: 0.36 ng/ml

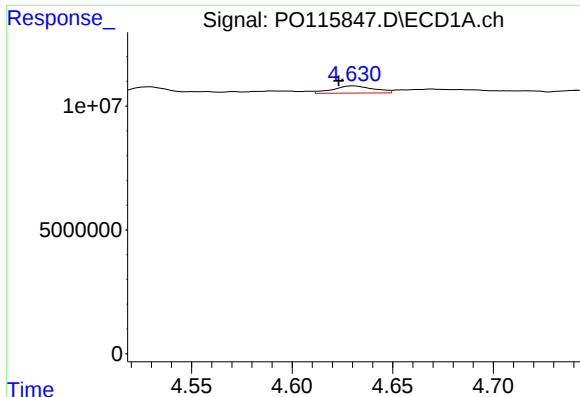

#9 AR-1221-2


R.T.: 4.630 min
Delta R.T.: 0.007 min
Response: 4046940
Conc: 64.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

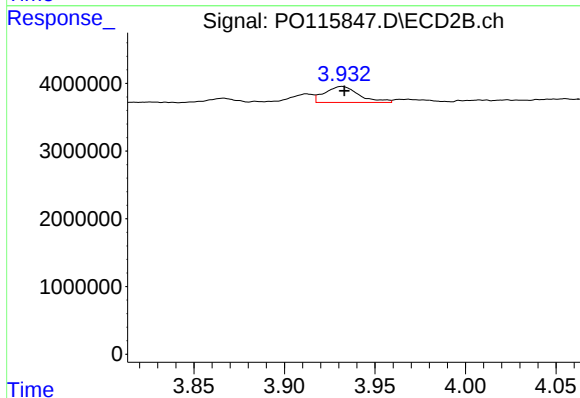


#9 AR-1221-2

R.T.: 3.932 min
Delta R.T.: -0.001 min
Response: 3110772
Conc: 73.29 ng/ml

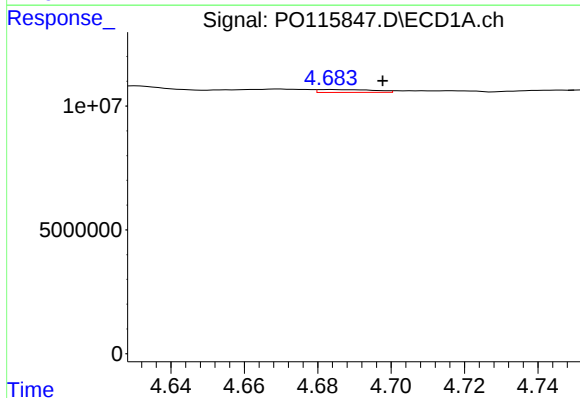


#10 AR-1221-3

R.T.: 4.683 min
Delta R.T.: -0.014 min
Response: 1208672
Conc: 6.47 ng/ml

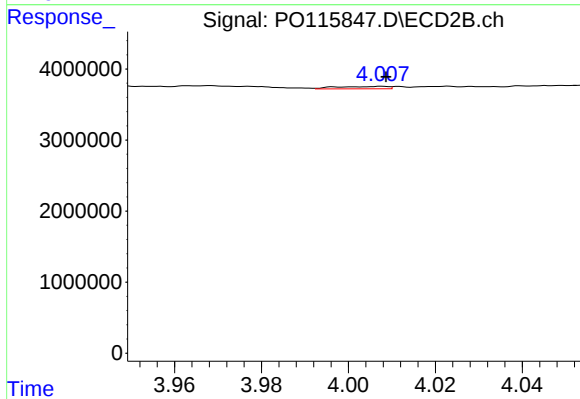

#10 AR-1221-3


R.T.: 4.008 min
Delta R.T.: 0.000 min
Response: 275526
Conc: 2.14 ng/ml

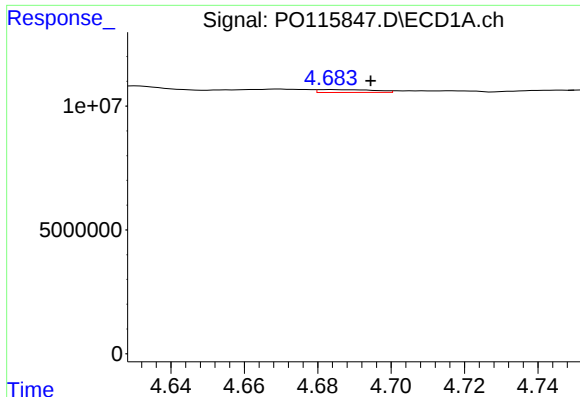

#11 AR-1232-1


R.T.: 4.683 min
Delta R.T.: -0.011 min
Response: 1208672
Conc: 8.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

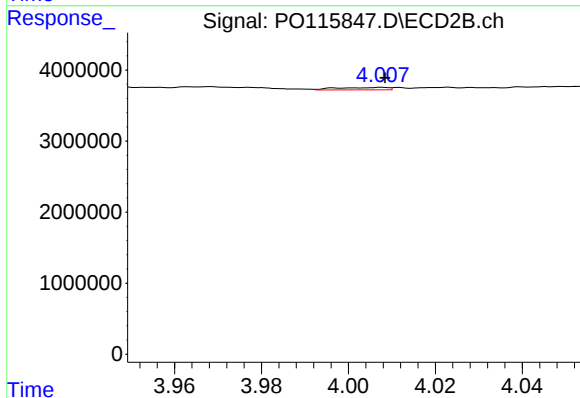


#11 AR-1232-1

R.T.: 4.008 min
Delta R.T.: 0.000 min
Response: 275526
Conc: 2.58 ng/ml

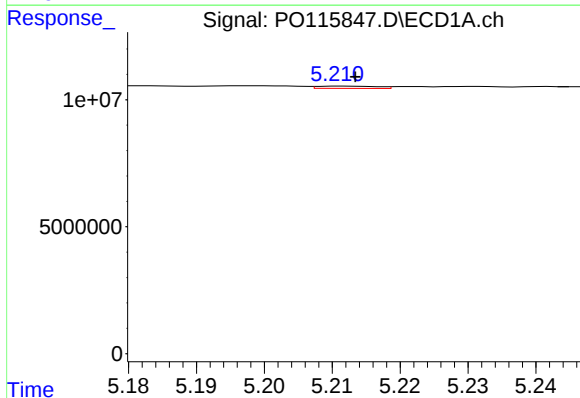


#12 AR-1232-2

R.T.: 5.211 min
Delta R.T.: -0.002 min
Response: 558622
Conc: 6.91 ng/ml

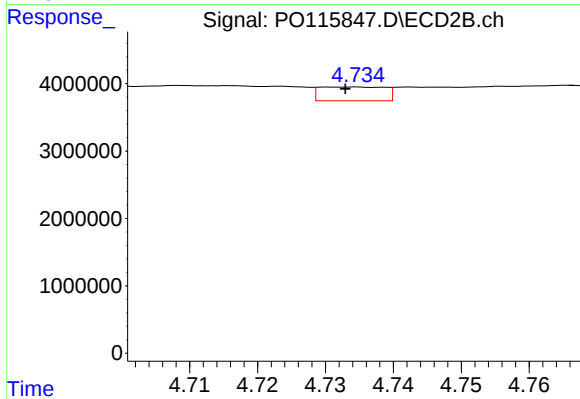

#12 AR-1232-2


R.T.: 4.735 min
Delta R.T.: 0.002 min
Response: 1372019
Conc: 12.36 ng/ml

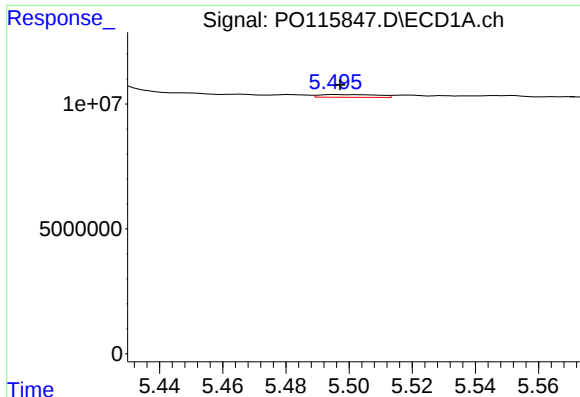

#13 AR-1232-3


R.T.: 5.495 min
Delta R.T.: -0.002 min
Response: 1410175
Conc: 9.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

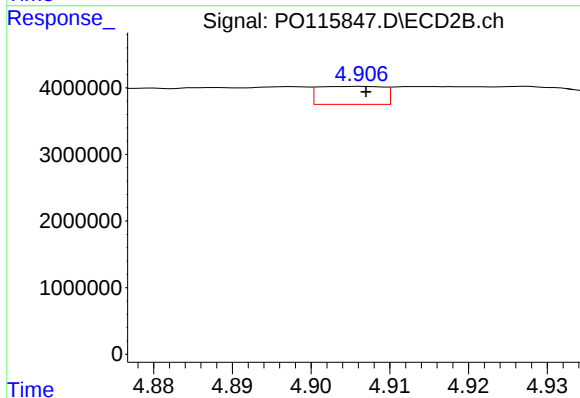


#13 AR-1232-3

R.T.: 4.906 min
Delta R.T.: 0.000 min
Response: 1553429
Conc: 23.76 ng/ml

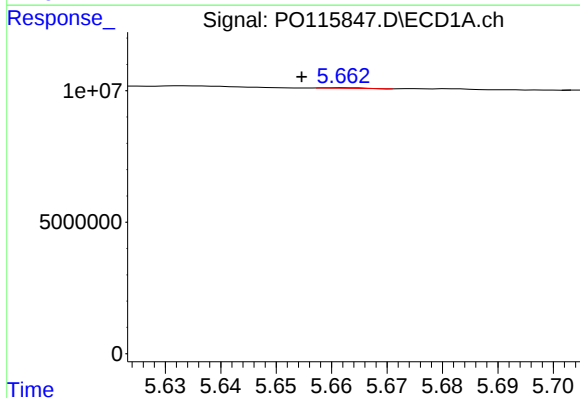


#14 AR-1232-4

R.T.: 5.662 min
Delta R.T.: 0.008 min
Response: 99375
Conc: 1.42 ng/ml

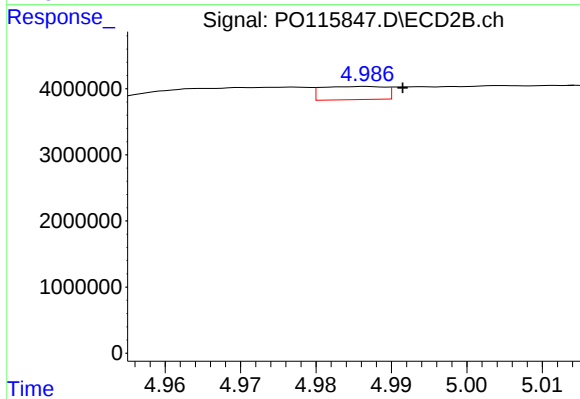

#14 AR-1232-4


R.T.: 4.987 min
Delta R.T.: -0.005 min
Response: 1159015
Conc: 22.58 ng/ml

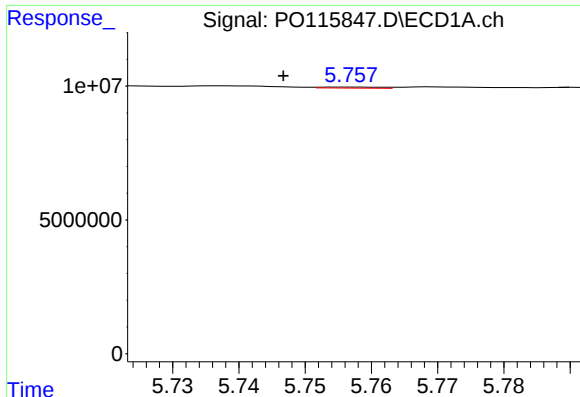

#15 AR-1232-5


R.T.: 5.757 min
Delta R.T.: 0.010 min
Response: 265831
Conc: 5.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

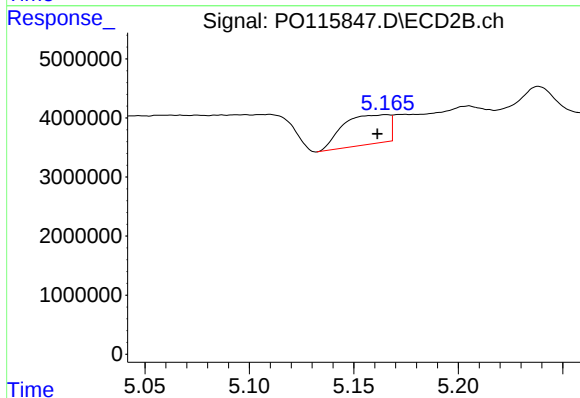


#15 AR-1232-5

R.T.: 5.165 min
Delta R.T.: 0.004 min
Response: 7702719
Conc: 140.69 ng/ml

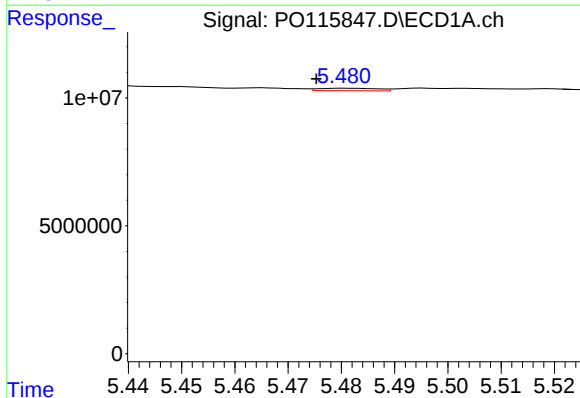


#16 AR-1242-1

R.T.: 5.481 min
Delta R.T.: 0.005 min
Response: 750220
Conc: 3.78 ng/ml

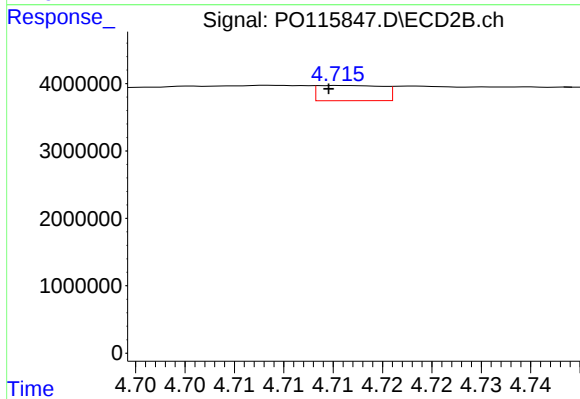

#16 AR-1242-1


R.T.: 4.716 min
Delta R.T.: 0.001 min
Response: 1031933
Conc: 7.25 ng/ml

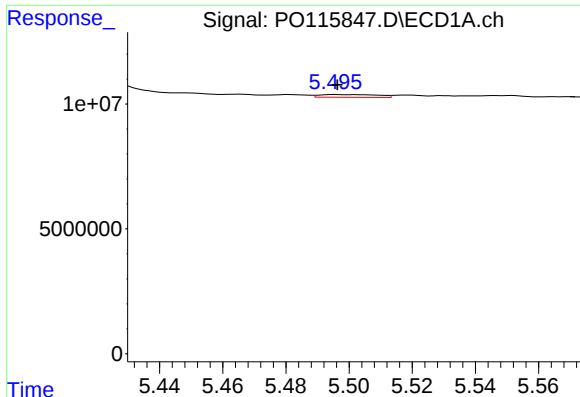

#17 AR-1242-2


R.T.: 5.495 min
Delta R.T.: -0.001 min
Response: 1410175
Conc: 4.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

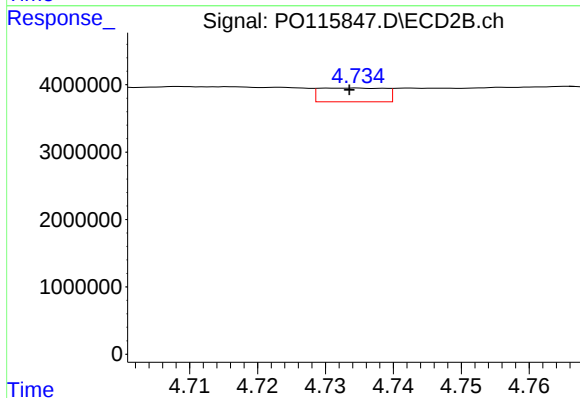


#17 AR-1242-2

R.T.: 4.735 min
Delta R.T.: 0.001 min
Response: 1372019
Conc: 6.55 ng/ml

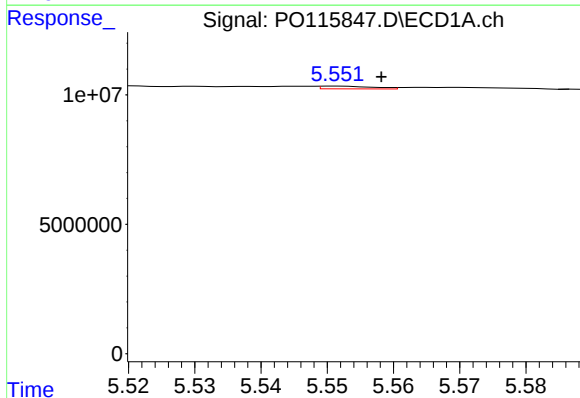


#18 AR-1242-3

R.T.: 5.552 min
Delta R.T.: -0.006 min
Response: 572934
Conc: 3.39 ng/ml

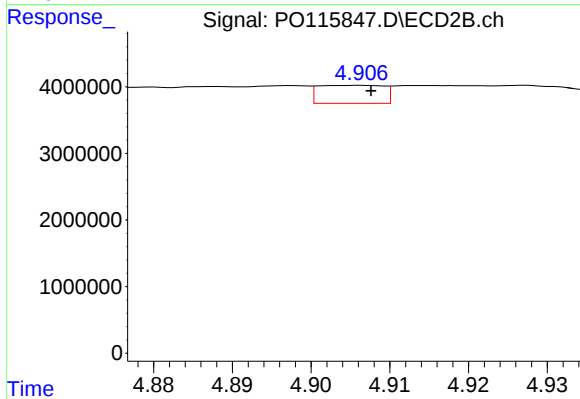

#18 AR-1242-3


R.T.: 4.906 min
Delta R.T.: -0.001 min
Response: 1553429
Conc: 13.01 ng/ml

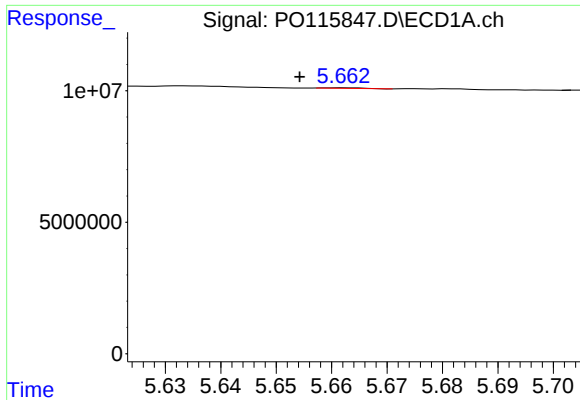

#19 AR-1242-4


R.T.: 5.662 min
Delta R.T.: 0.008 min
Response: 99375
Conc: 0.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

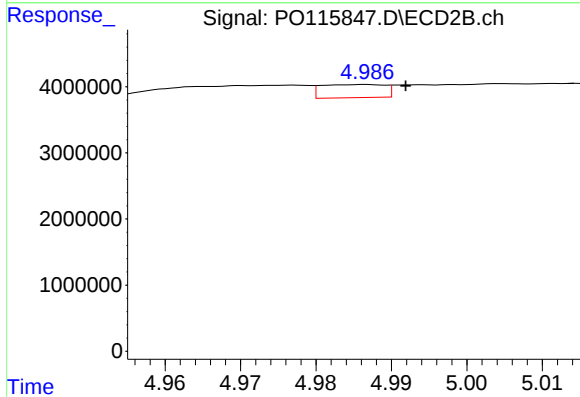


#19 AR-1242-4

R.T.: 4.987 min
Delta R.T.: -0.005 min
Response: 1159015
Conc: 10.62 ng/ml

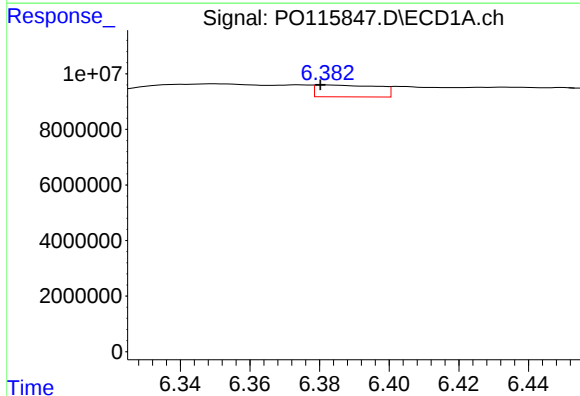


#20 AR-1242-5

R.T.: 6.381 min
Delta R.T.: 0.001 min
Response: 5305027
Conc: 35.03 ng/ml

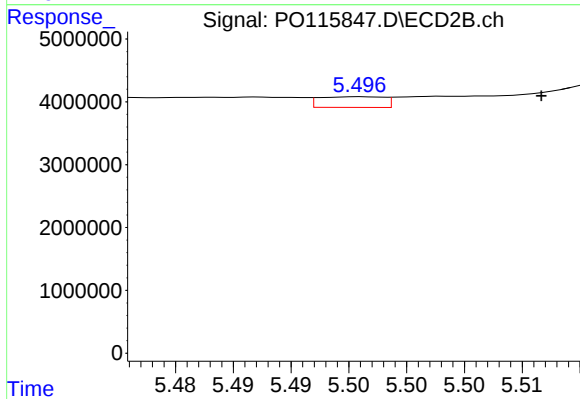

#20 AR-1242-5


R.T.: 5.496 min
Delta R.T.: -0.016 min
Response: 658263
Conc: 4.77 ng/ml

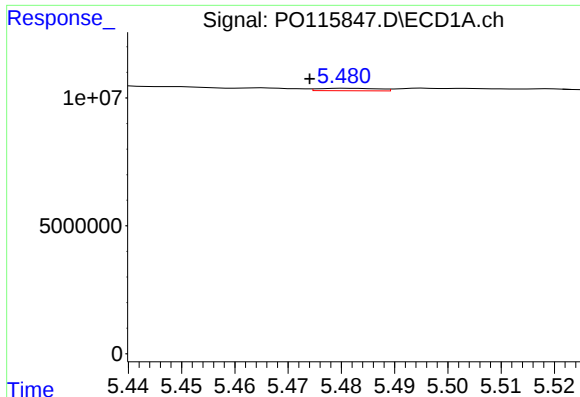

#21 AR-1248-1


R.T.: 5.481 min
Delta R.T.: 0.007 min
Response: 750220
Conc: 4.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

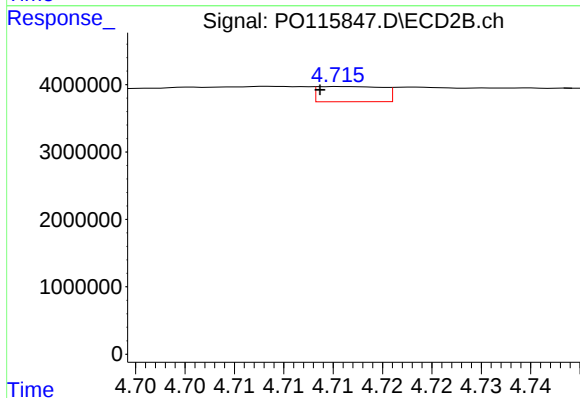


#21 AR-1248-1

R.T.: 4.716 min
Delta R.T.: 0.002 min
Response: 1031933
Conc: 9.23 ng/ml

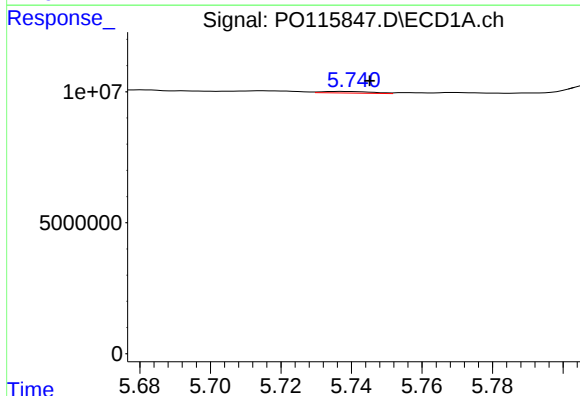


#22 AR-1248-2

R.T.: 5.737 min
Delta R.T.: -0.009 min
Response: 569610
Conc: 2.84 ng/ml

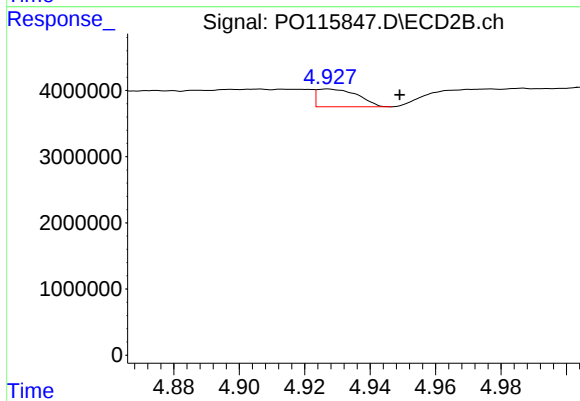

#22 AR-1248-2


R.T.: 4.927 min
Delta R.T.: -0.022 min
Response: 2318371
Conc: 15.22 ng/ml

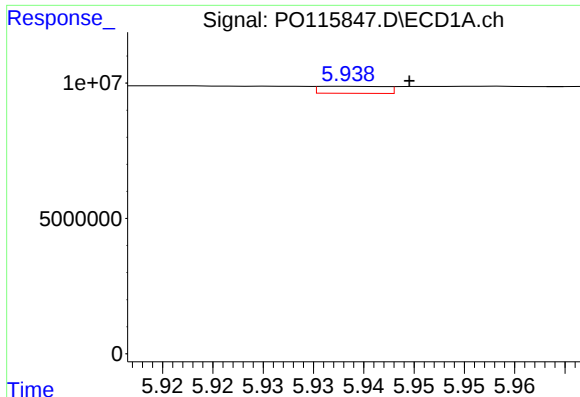

#23 AR-1248-3


R.T.: 5.938 min
Delta R.T.: -0.007 min
Response: 1174811
Conc: 4.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

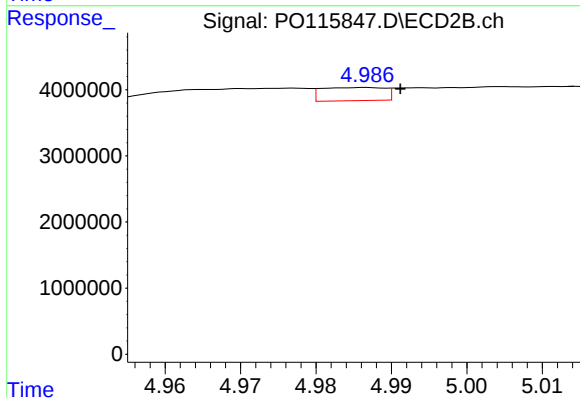


#23 AR-1248-3

R.T.: 4.987 min
Delta R.T.: -0.005 min
Response: 1159015
Conc: 7.22 ng/ml

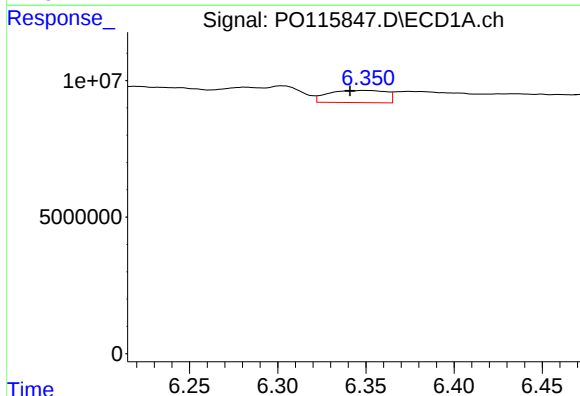


#24 AR-1248-4

R.T.: 6.350 min
Delta R.T.: 0.009 min
Response: 10130286
Conc: 34.36 ng/ml

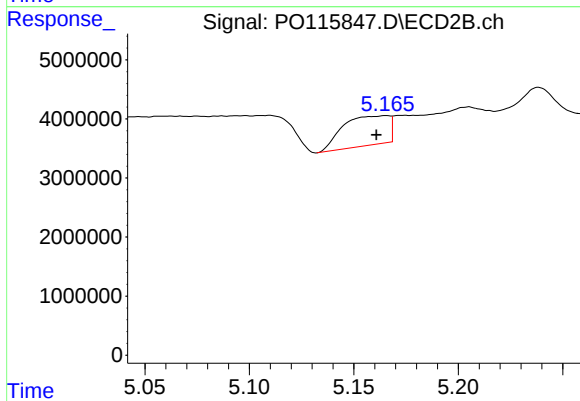

#24 AR-1248-4


R.T.: 5.165 min
Delta R.T.: 0.004 min
Response: 7702719
Conc: 41.16 ng/ml

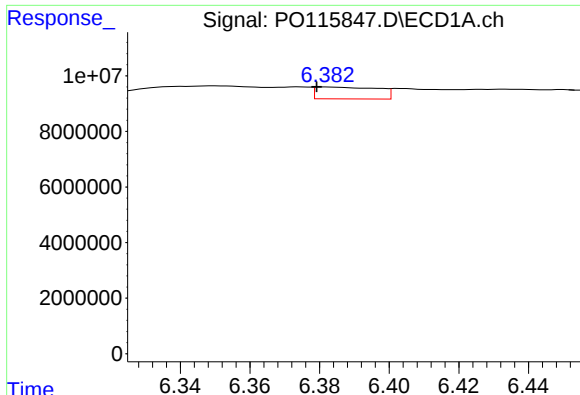

#25 AR-1248-5


R.T.: 6.381 min
Delta R.T.: 0.002 min
Response: 5305027
Conc: 20.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

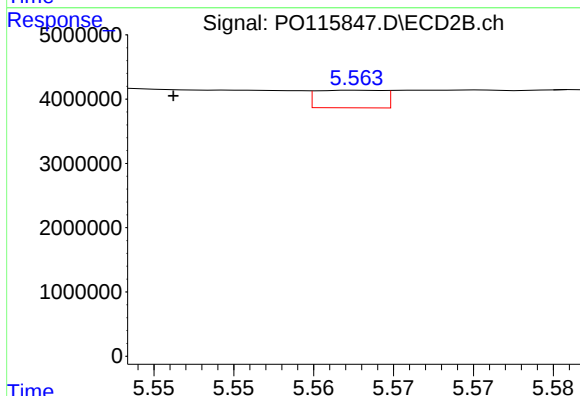


#25 AR-1248-5

R.T.: 5.563 min
Delta R.T.: 0.012 min
Response: 797274
Conc: 4.03 ng/ml

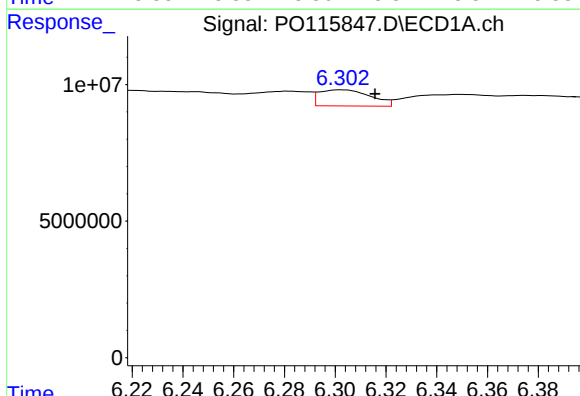


#26 AR-1254-1

R.T.: 6.303 min
Delta R.T.: -0.013 min
Response: 8289582
Conc: 32.04 ng/ml

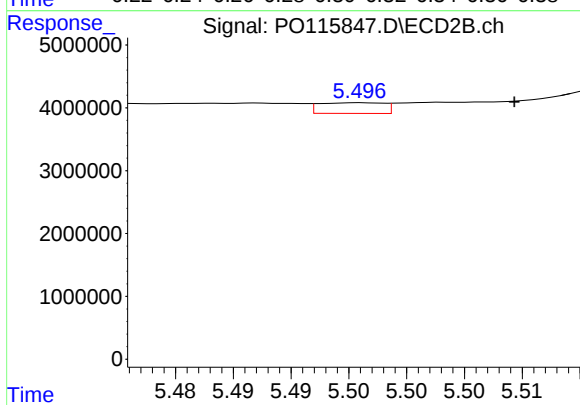

#26 AR-1254-1


R.T.: 5.496 min
Delta R.T.: -0.013 min
Response: 658263
Conc: 2.25 ng/ml

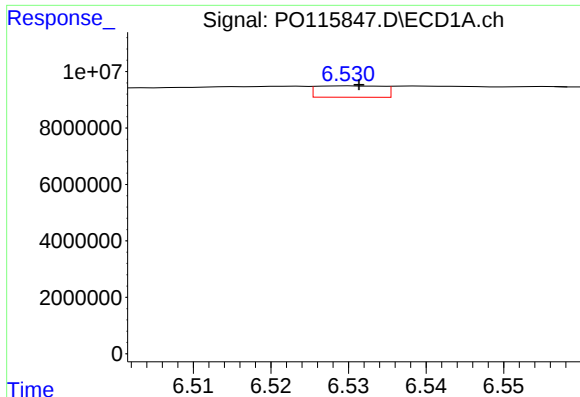

#27 AR-1254-2


R.T.: 6.530 min
Delta R.T.: -0.001 min
Response: 2387563
Conc: 5.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

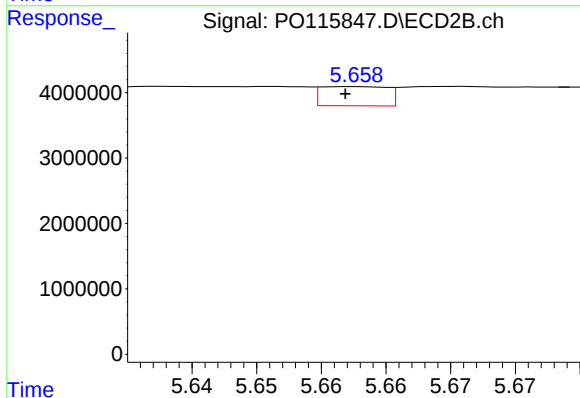


#27 AR-1254-2

R.T.: 5.657 min
Delta R.T.: 0.000 min
Response: 1043425
Conc: 4.14 ng/ml

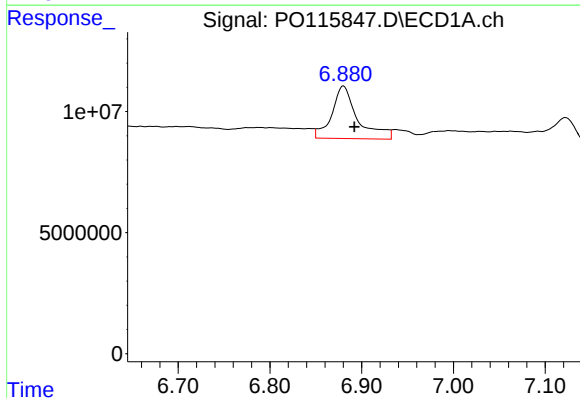


#28 AR-1254-3

R.T.: 6.880 min
Delta R.T.: -0.012 min
Response: 42224183
Conc: 102.84 ng/ml

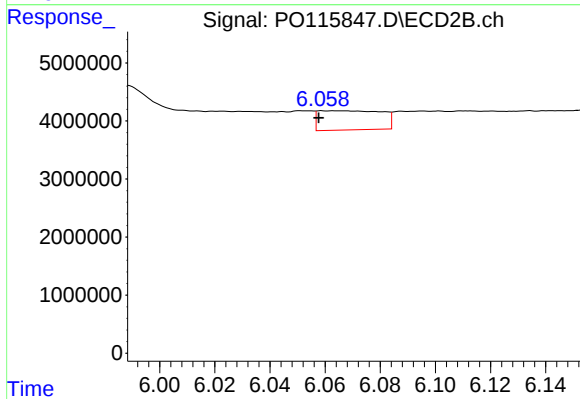

#28 AR-1254-3


R.T.: 6.059 min
Delta R.T.: 0.001 min
Response: 5260350
Conc: 13.37 ng/ml

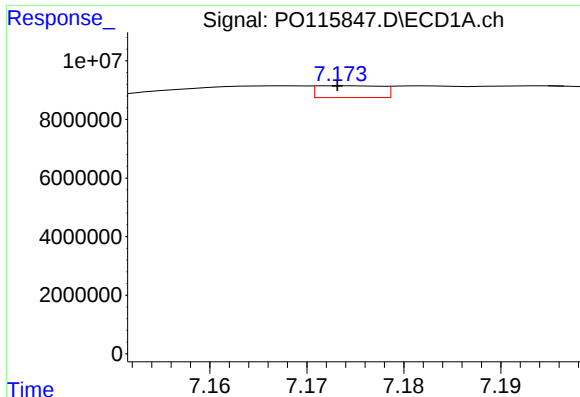

#29 AR-1254-4


R.T.: 7.174 min
Delta R.T.: 0.000 min
Response: 1869046
Conc: 5.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

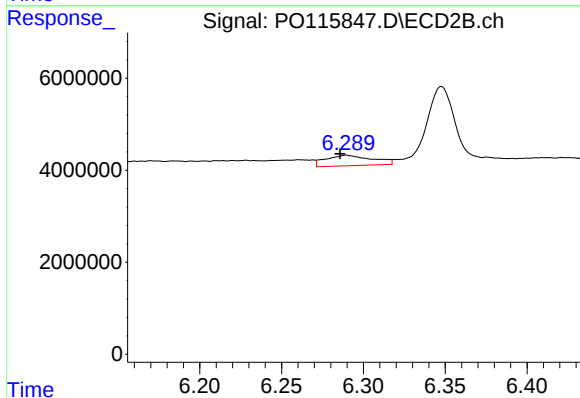


#29 AR-1254-4

R.T.: 6.290 min
Delta R.T.: 0.004 min
Response: 4541759
Conc: 16.97 ng/ml

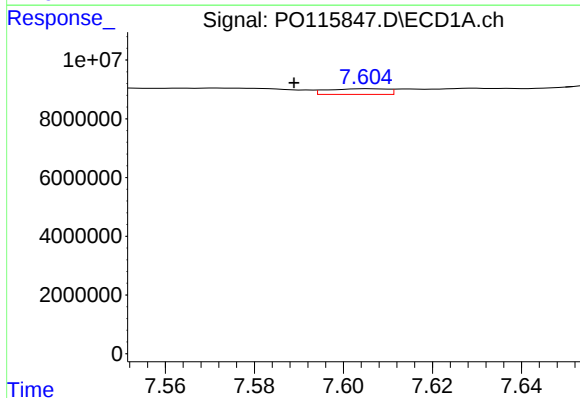


#30 AR-1254-5

R.T.: 7.605 min
Delta R.T.: 0.016 min
Response: 1804000
Conc: 5.57 ng/ml

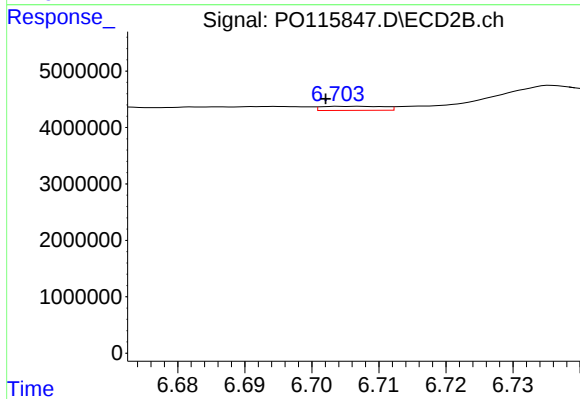

#30 AR-1254-5


R.T.: 6.707 min
Delta R.T.: 0.005 min
Response: 465125
Conc: 1.30 ng/ml

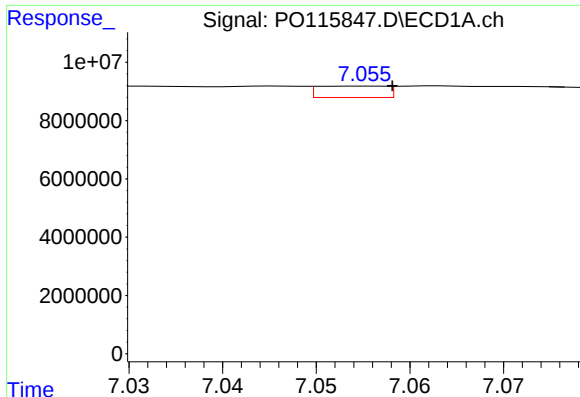

#31 AR-1260-1


R.T.: 7.056 min
Delta R.T.: -0.003 min
Response: 1983406
Conc: 6.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

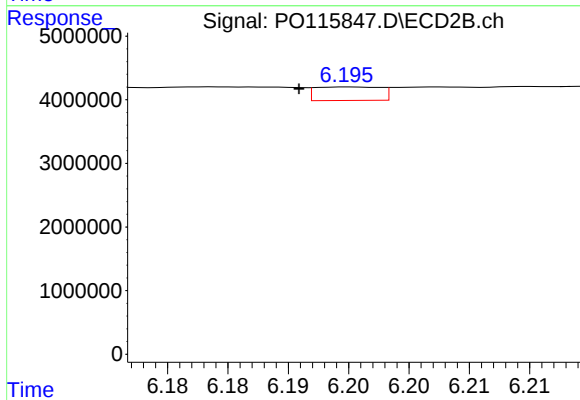


#31 AR-1260-1

R.T.: 6.195 min
Delta R.T.: 0.004 min
Response: 797291
Conc: 3.04 ng/ml

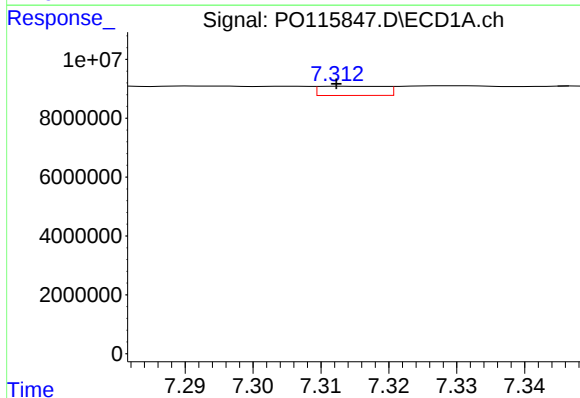


#32 AR-1260-2

R.T.: 7.313 min
Delta R.T.: 0.000 min
Response: 2098274
Conc: 4.79 ng/ml

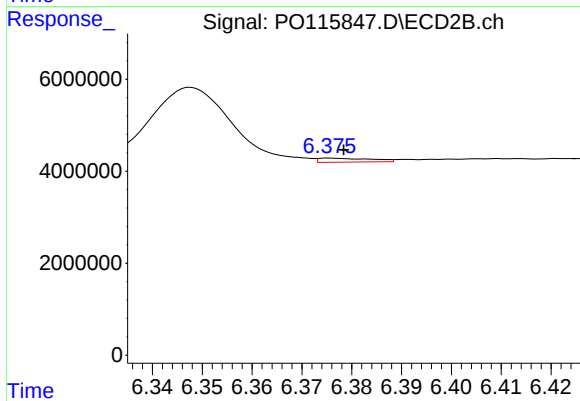

#32 AR-1260-2


R.T.: 6.376 min
Delta R.T.: -0.003 min
Response: 644979
Conc: 1.84 ng/ml

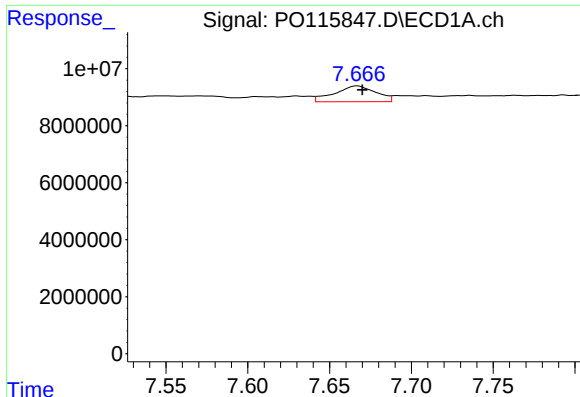

#33 AR-1260-3


R.T.: 7.667 min
Delta R.T.: -0.003 min
Response: 9759395
Conc: 28.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

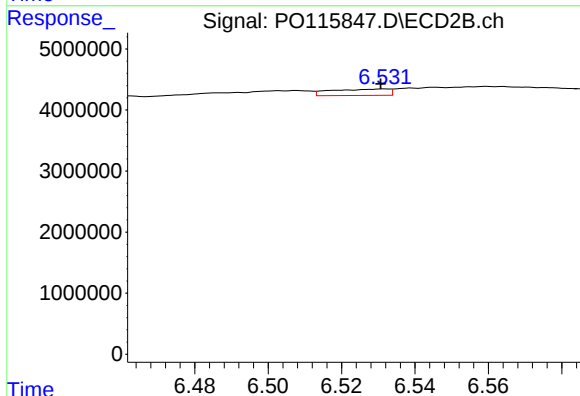


#33 AR-1260-3

R.T.: 6.532 min
Delta R.T.: 0.001 min
Response: 1128375
Conc: 3.51 ng/ml

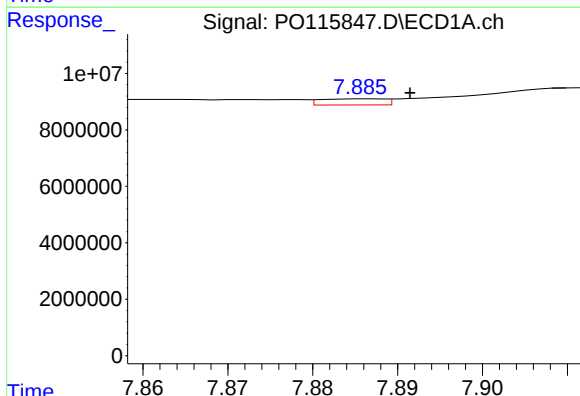


#34 AR-1260-4

R.T.: 7.886 min
Delta R.T.: -0.005 min
Response: 1137677
Conc: 3.70 ng/ml

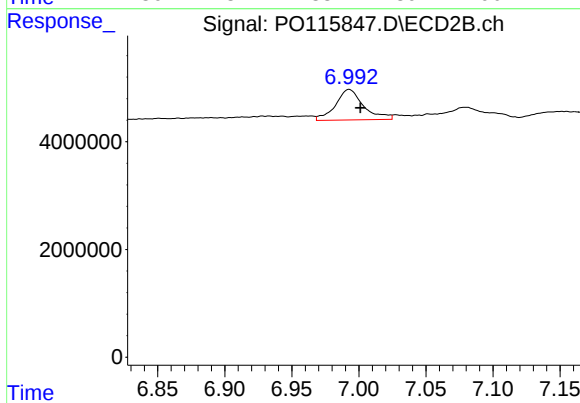

#34 AR-1260-4


R.T.: 6.993 min
Delta R.T.: -0.008 min
Response: 8234460
Conc: 32.06 ng/ml

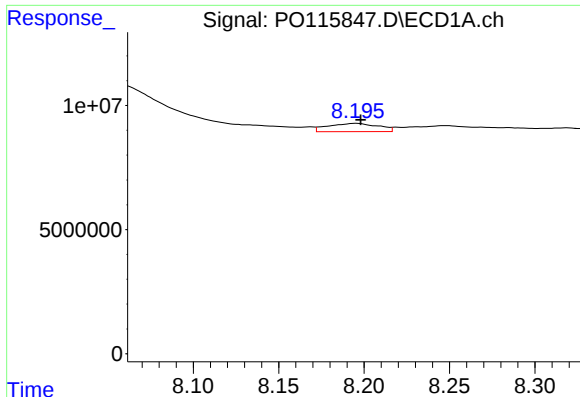

#35 AR-1260-5


R.T.: 8.195 min
Delta R.T.: -0.002 min
Response: 6817882
Conc: 9.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

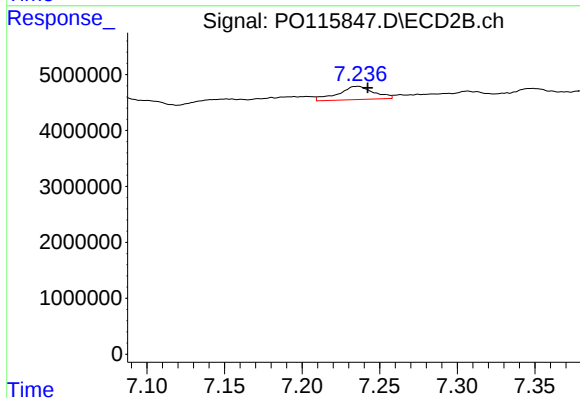


#35 AR-1260-5

R.T.: 7.236 min
Delta R.T.: -0.006 min
Response: 3808550
Conc: 5.43 ng/ml

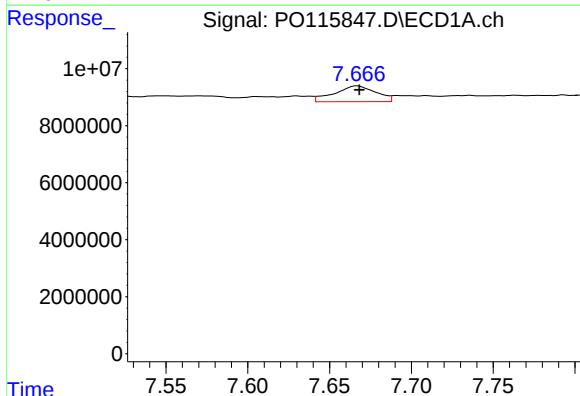


#36 AR-1262-1

R.T.: 7.667 min
Delta R.T.: -0.001 min
Response: 9759395
Conc: 39.53 ng/ml

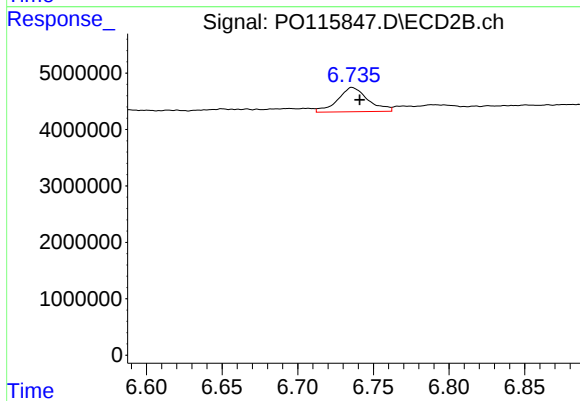

#36 AR-1262-1


R.T.: 6.736 min
Delta R.T.: -0.005 min
Response: 6037685
Conc: 28.34 ng/ml

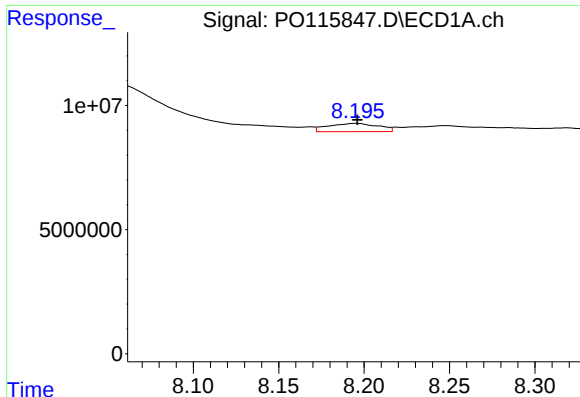

#37 AR-1262-2


R.T.: 8.195 min
Delta R.T.: 0.000 min
Response: 6817882
Conc: 17.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

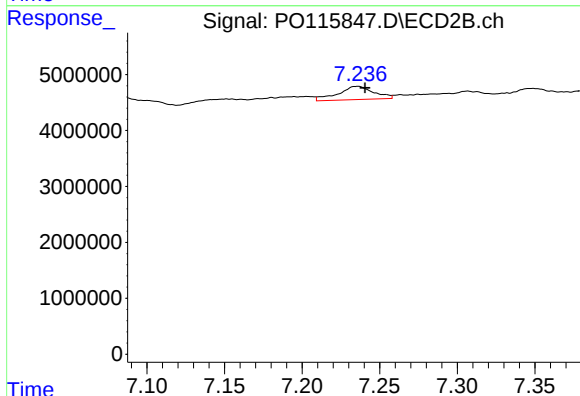


#37 AR-1262-2

R.T.: 7.236 min
Delta R.T.: -0.004 min
Response: 3808550
Conc: 10.93 ng/ml

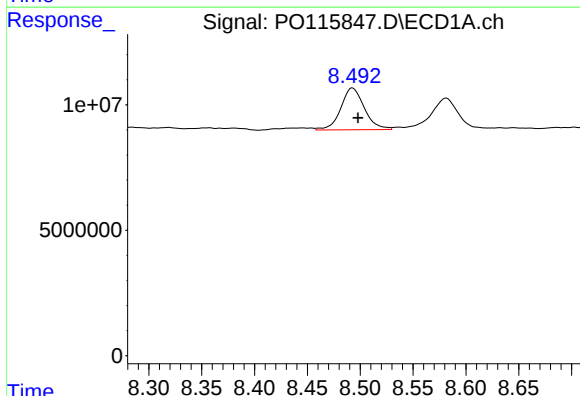


#38 AR-1262-3

R.T.: 8.493 min
Delta R.T.: -0.005 min
Response: 25815827
Conc: 101.31 ng/ml

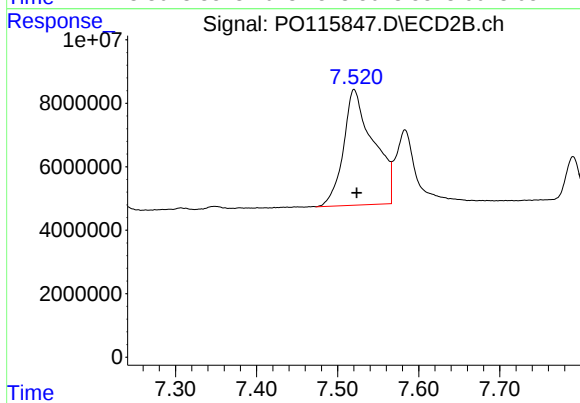

#38 AR-1262-3


R.T.: 7.520 min
Delta R.T.: -0.003 min
Response: 93212951
Conc: 596.03 ng/ml

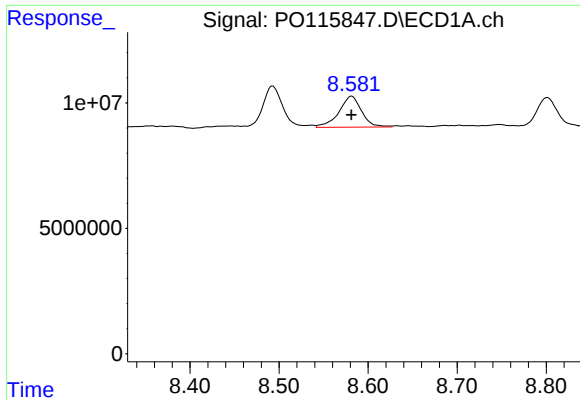

#39 AR-1262-4


R.T.: 8.582 min
Delta R.T.: 0.000 min
Response: 21816156
Conc: 112.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

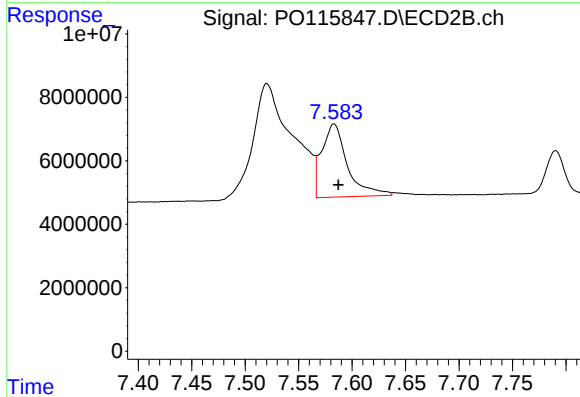


#39 AR-1262-4

R.T.: 7.583 min
Delta R.T.: -0.004 min
Response: 38530215
Conc: 155.76 ng/ml

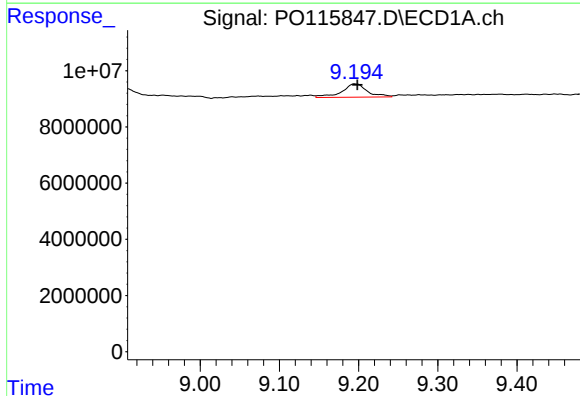


#40 AR-1262-5

R.T.: 9.195 min
Delta R.T.: -0.003 min
Response: 10646820
Conc: 79.05 ng/ml

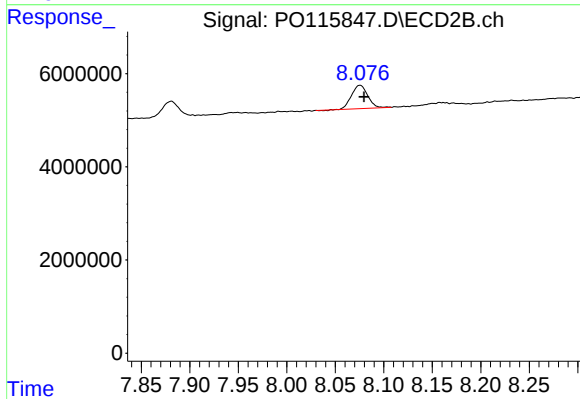

#40 AR-1262-5


R.T.: 8.076 min
Delta R.T.: -0.004 min
Response: 5854762
Conc: 52.52 ng/ml

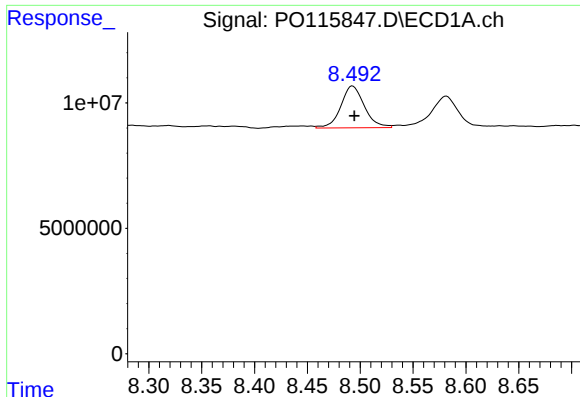

#41 AR-1268-1


R.T.: 8.493 min
Delta R.T.: -0.002 min
Response: 25815827
Conc: 25.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

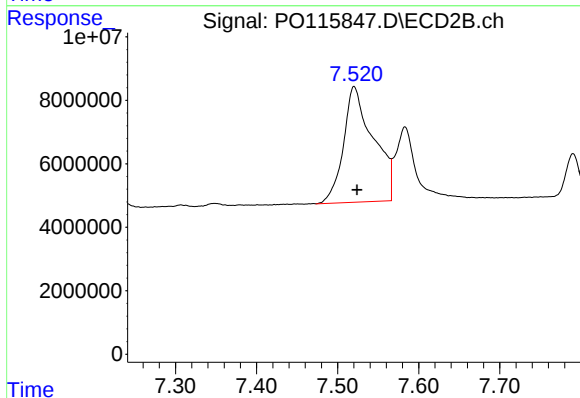


#41 AR-1268-1

R.T.: 7.520 min
Delta R.T.: -0.004 min
Response: 93212951
Conc: 105.21 ng/ml

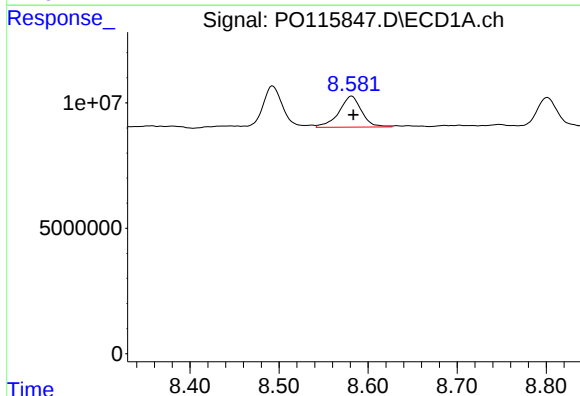


#42 AR-1268-2

R.T.: 8.582 min
Delta R.T.: -0.002 min
Response: 21816156
Conc: 25.50 ng/ml

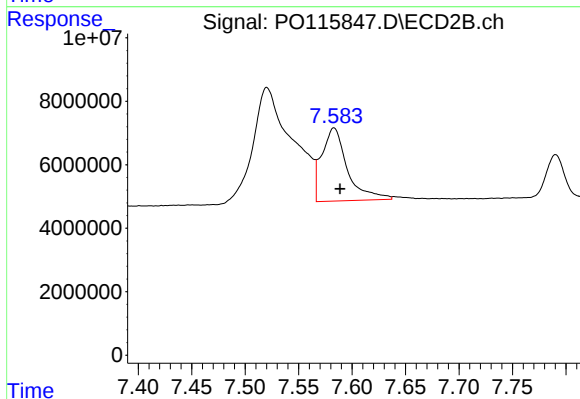

#42 AR-1268-2


R.T.: 7.583 min
Delta R.T.: -0.006 min
Response: 38530215
Conc: 51.44 ng/ml

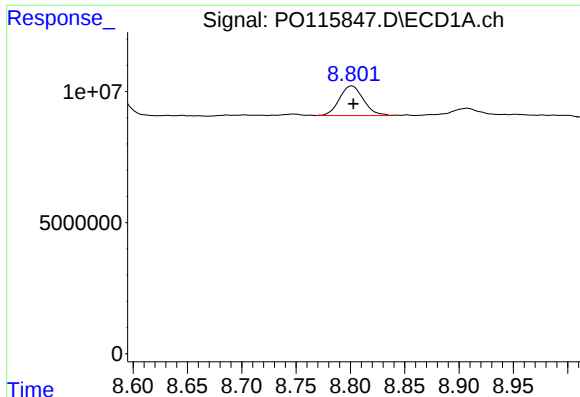

#43 AR-1268-3


R.T.: 8.801 min
Delta R.T.: -0.001 min
Response: 17303812
Conc: 23.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

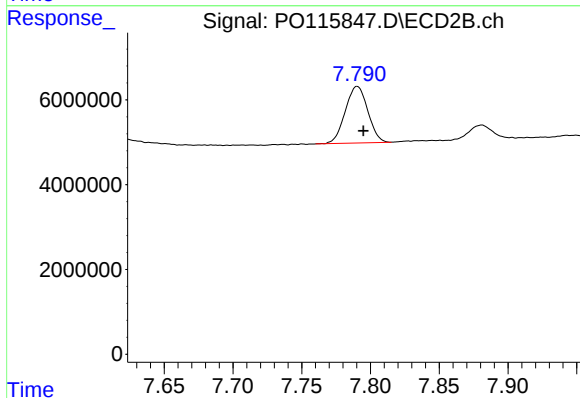


#43 AR-1268-3

R.T.: 7.790 min
Delta R.T.: -0.004 min
Response: 15214360
Conc: 23.90 ng/ml

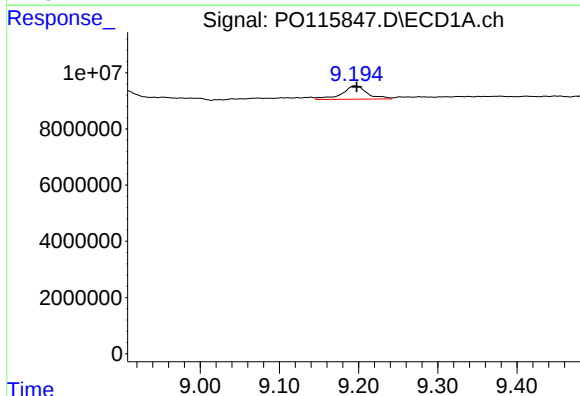


#44 AR-1268-4

R.T.: 9.195 min
Delta R.T.: -0.002 min
Response: 10646820
Conc: 34.10 ng/ml

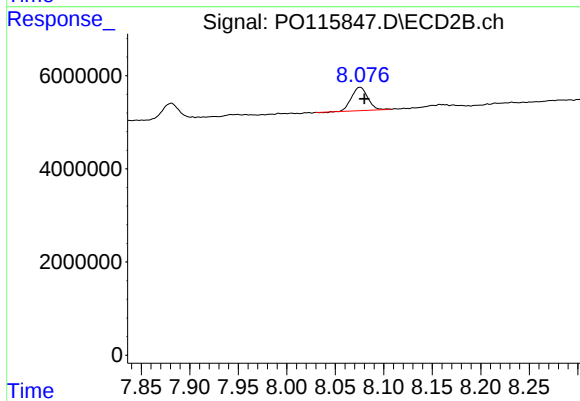

#44 AR-1268-4


R.T.: 8.076 min
Delta R.T.: -0.004 min
Response: 5854762
Conc: 22.73 ng/ml

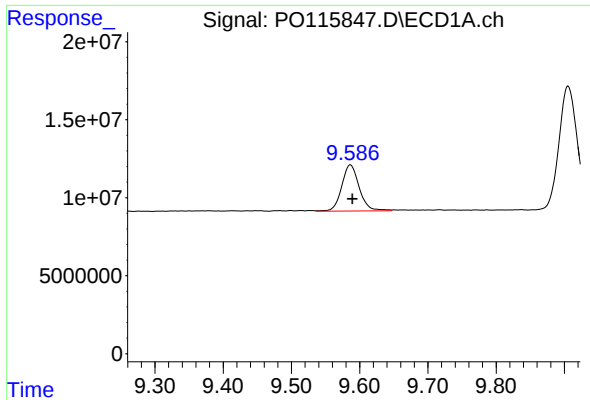

#45 AR-1268-5

R.T.: 9.587 min
Delta R.T.: -0.003 min
Response: 52845986
Conc: 24.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2025

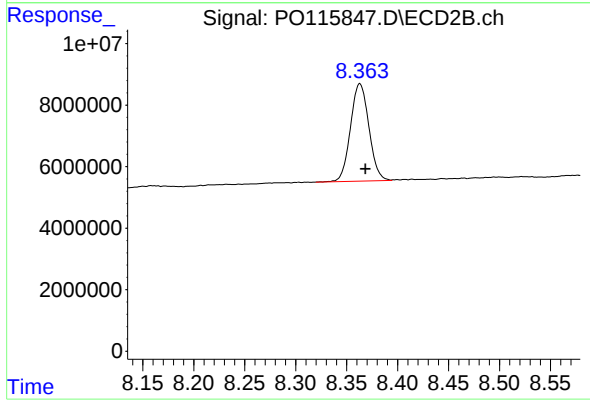

#45 AR-1268-5

R.T.: 8.363 min
Delta R.T.: -0.006 min
Response: 39831293
Conc: 23.63 ng/ml