

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO121321\
 Data File : PO083640.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Dec 2021 17:20
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 14 00:12:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO120621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 07 13:18:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.937	3.942	2161860	696189	22.660	22.381
2) SA Decachlor...	11.009	9.239	1639116	667106	22.945	20.448
Target Compounds						
8) L2 AR-1221-1	5.180	0.000	57434	0	57.114	N.D. #
9) L2 AR-1221-2	5.293	0.000	26449	0	36.720	N.D. #
10) L2 AR-1221-3	0.000	4.385	0	26746	N.D.	28.795 #
11) L3 AR-1232-1	0.000	4.385	0	26746	N.D.	33.834 #
24) L5 AR-1248-4	7.195f	0.000	37597	0	12.435	N.D. #
26) L6 AR-1254-1	7.195	0.000	37597	0	11.766	N.D. #
28) L6 AR-1254-3	7.821	0.000	19453	0	3.900	N.D. #
32) L7 AR-1260-2	8.215f	0.000	9153	0	2.193	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121321\
Data File : P0083640.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Dec 2021 17:20
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 14 00:12:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120621.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 07 13:18:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

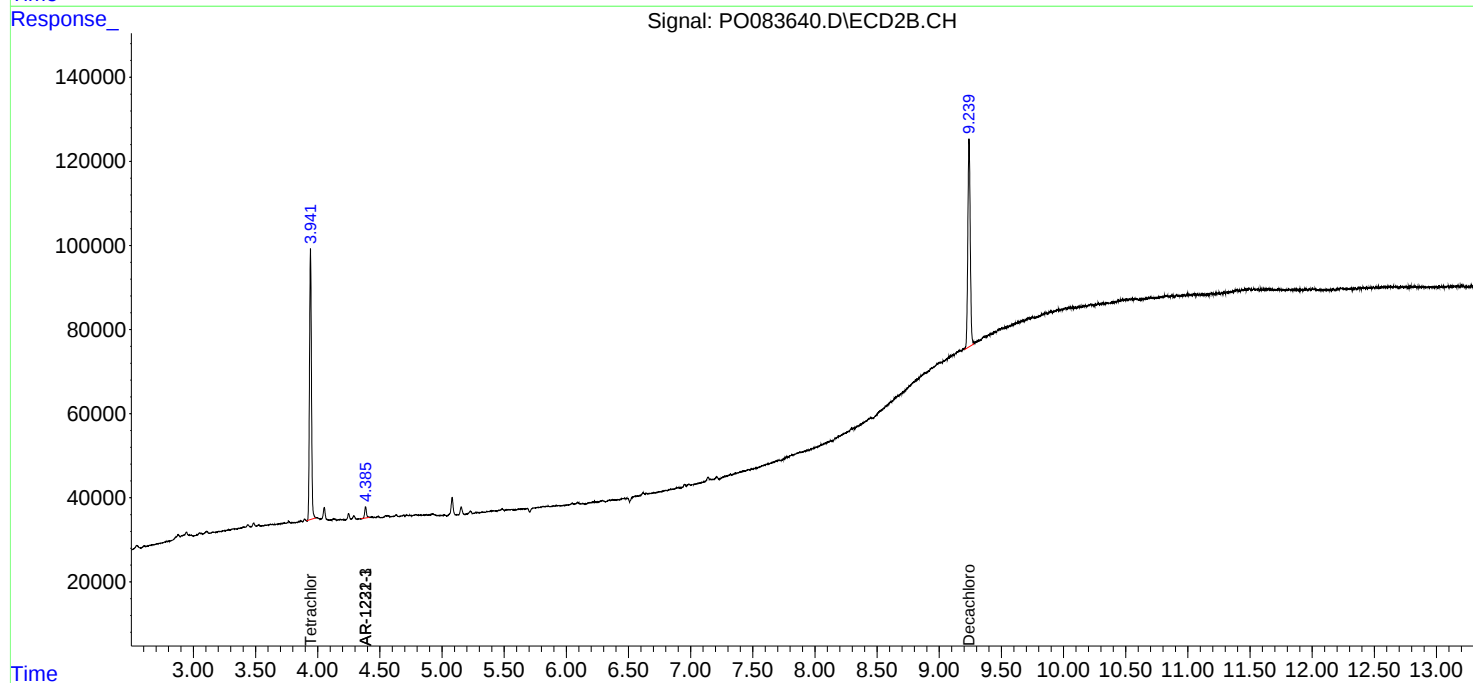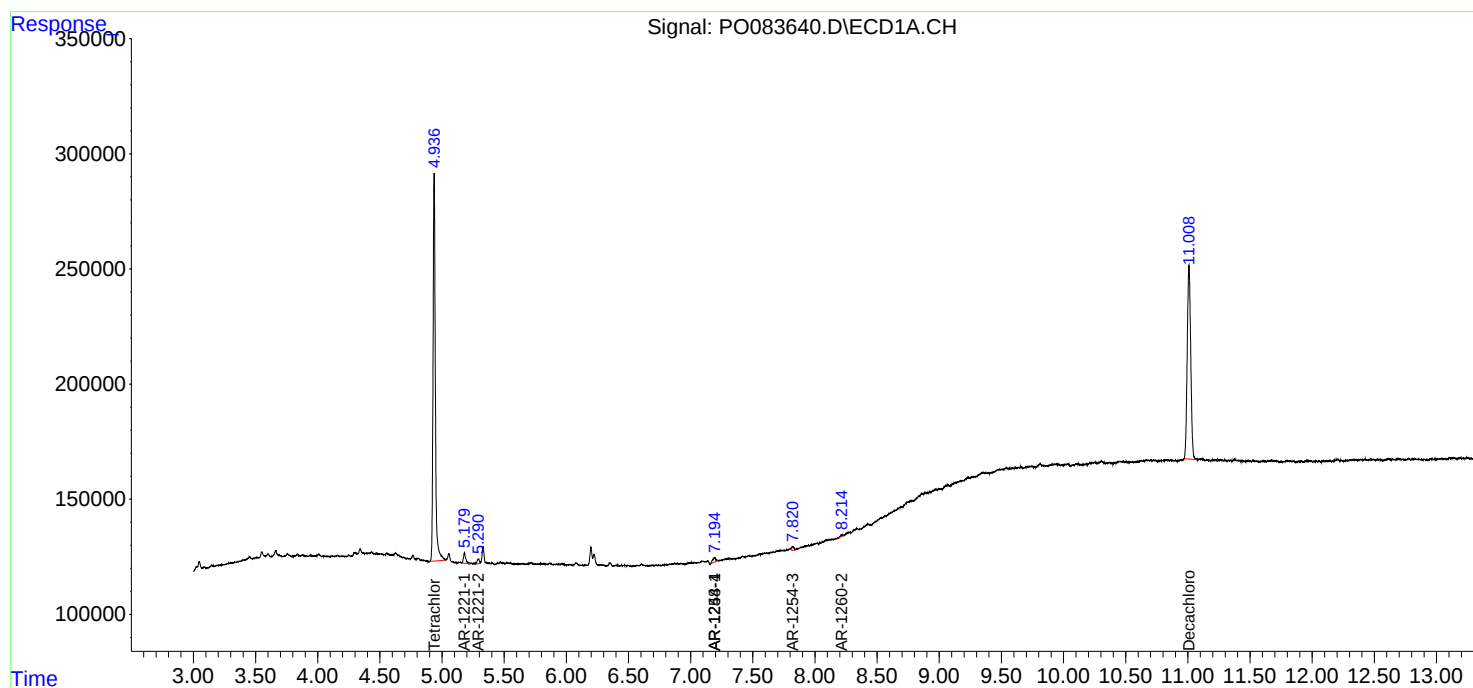


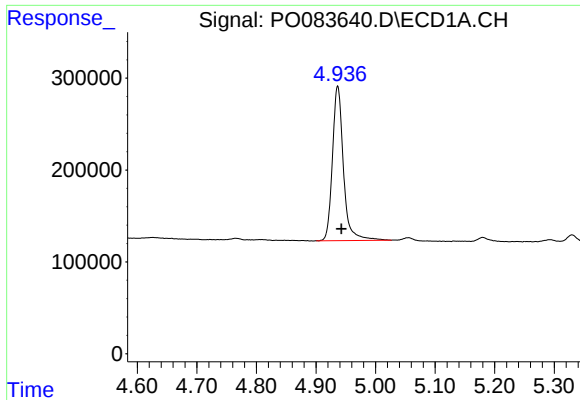

#1 Tetrachloro-m-xylene


R.T.: 4.937 min
Delta R.T.: -0.006 min
Response: 2161860
Conc: 22.66 ng/ml

Instrument :
ECD_O
ClientSampleId :

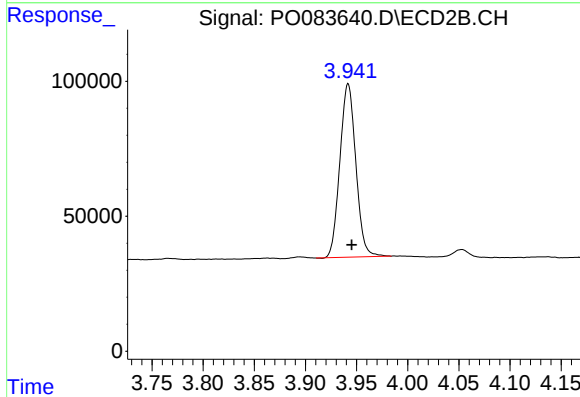


#1 Tetrachloro-m-xylene

R.T.: 3.942 min
Delta R.T.: -0.004 min
Response: 696189
Conc: 22.38 ng/ml

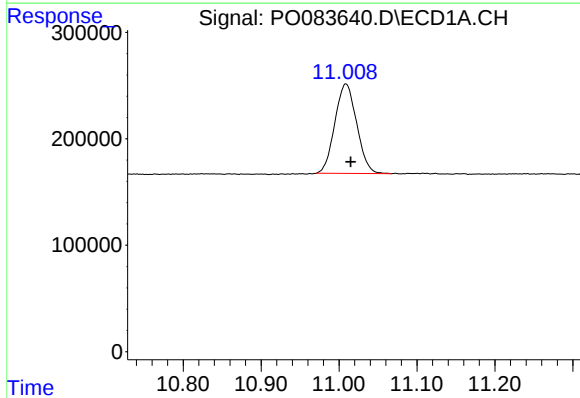


#2 Decachlorobiphenyl

R.T.: 11.009 min
Delta R.T.: -0.006 min
Response: 1639116
Conc: 22.94 ng/ml

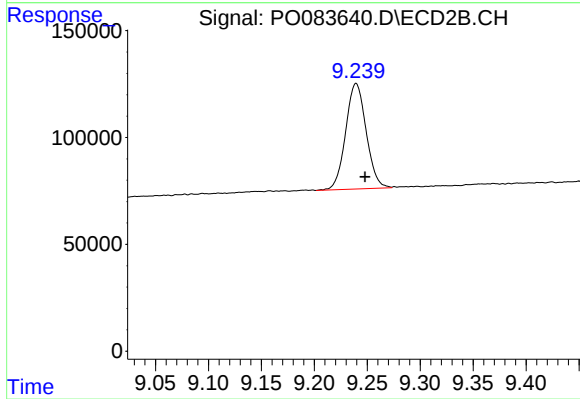

#2 Decachlorobiphenyl


R.T.: 9.239 min
Delta R.T.: -0.008 min
Response: 667106
Conc: 20.45 ng/ml

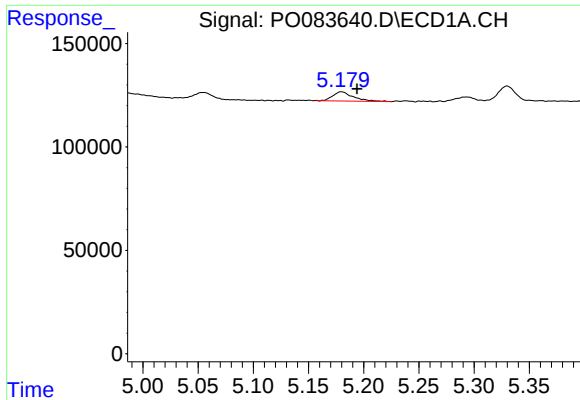

#8 AR-1221-1


R.T.: 5.180 min
Delta R.T.: -0.014 min
Response: 57434
Conc: 57.11 ng/ml

Instrument :
ECD_O
ClientSampleId :

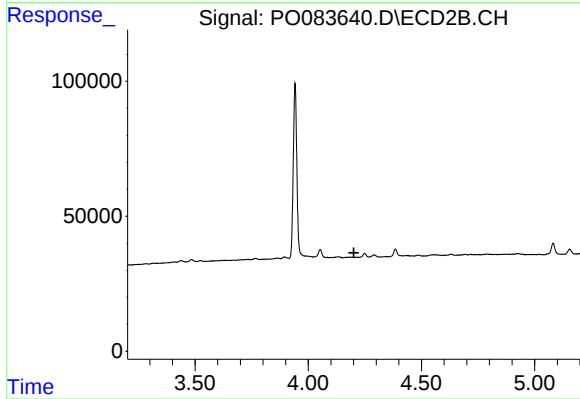


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.202 min
Response: 0
Conc: N.D.

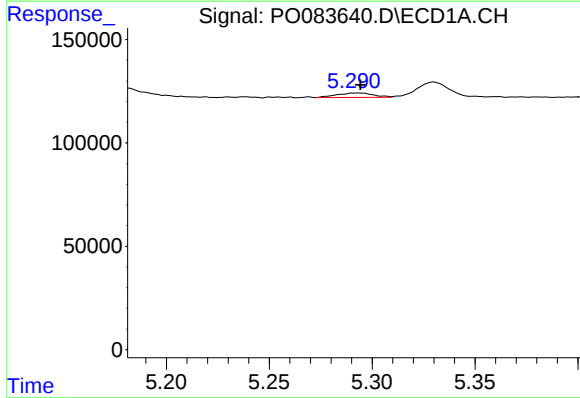


#9 AR-1221-2

R.T.: 5.293 min
Delta R.T.: -0.001 min
Response: 26449
Conc: 36.72 ng/ml

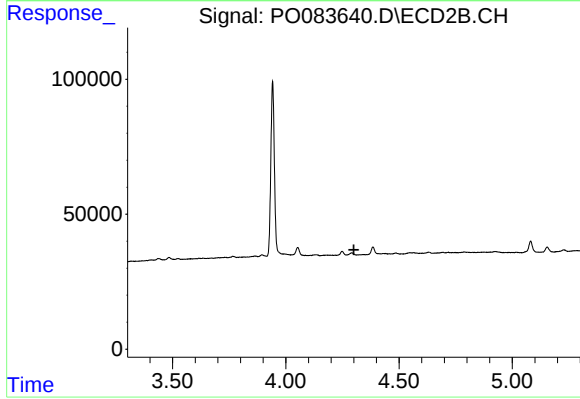

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.301 min
Response: 0
Conc: N.D.

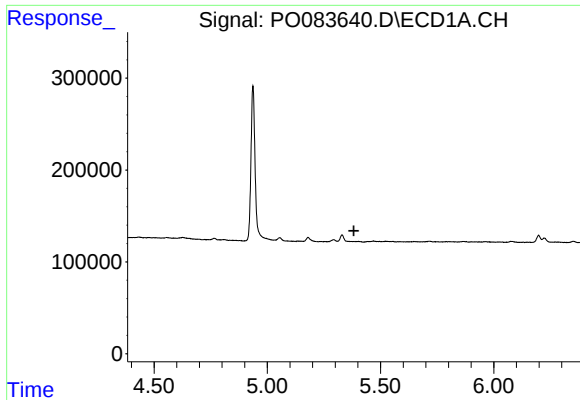

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T.: 5.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

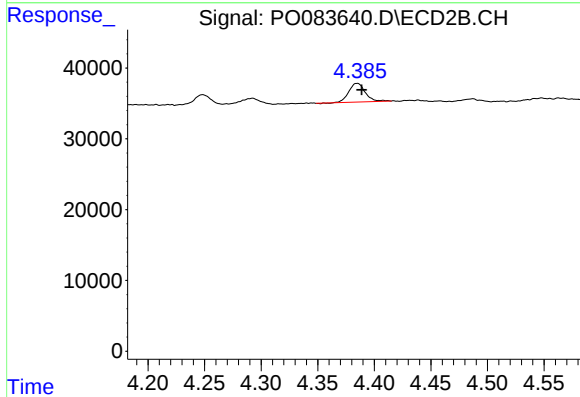


#10 AR-1221-3

R.T.: 4.385 min
Delta R.T.: -0.004 min
Response: 26746
Conc: 28.80 ng/ml

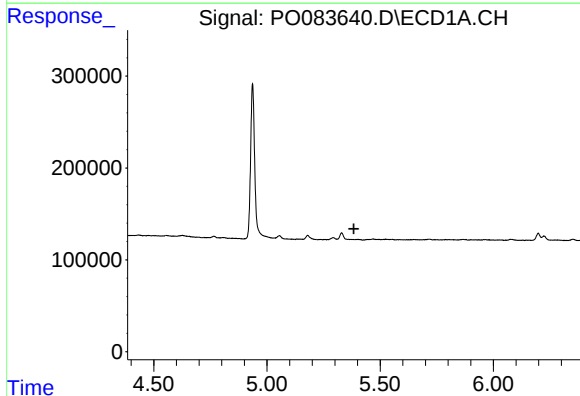


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T.: 5.384 min
Response: 0
Conc: N.D.

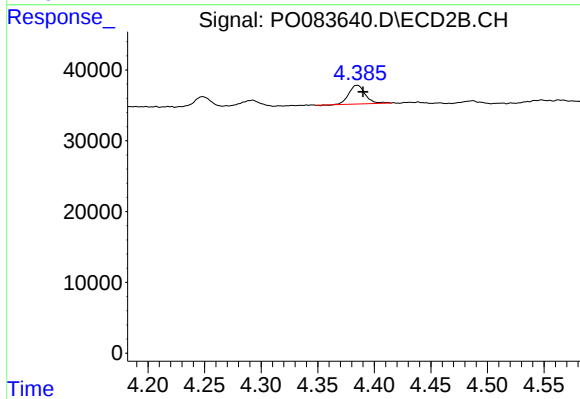

#11 AR-1232-1


R.T.: 4.385 min
Delta R.T.: -0.005 min
Response: 26746
Conc: 33.83 ng/ml

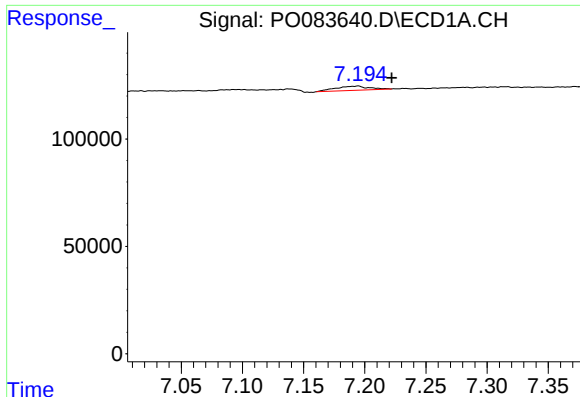

#24 AR-1248-4


R.T.: 7.195 min
Delta R.T.: -0.027 min
Response: 37597
Conc: 12.44 ng/ml

Instrument :
ECD_O
ClientSampleId :

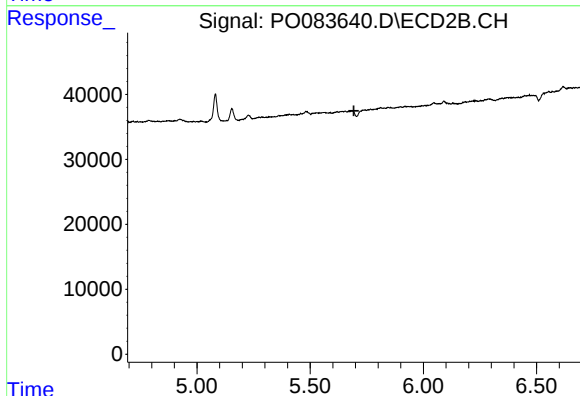


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.693 min
Response: 0
Conc: N.D.

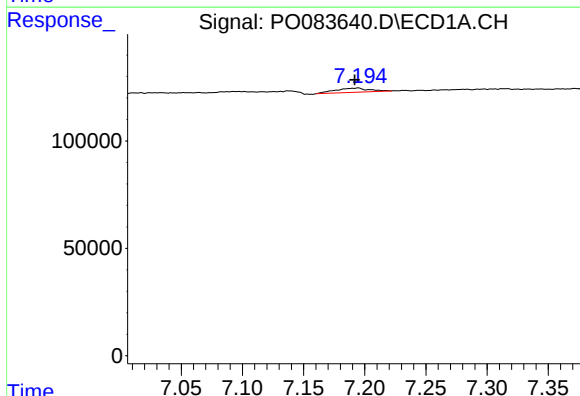


#26 AR-1254-1

R.T.: 7.195 min
Delta R.T.: 0.003 min
Response: 37597
Conc: 11.77 ng/ml

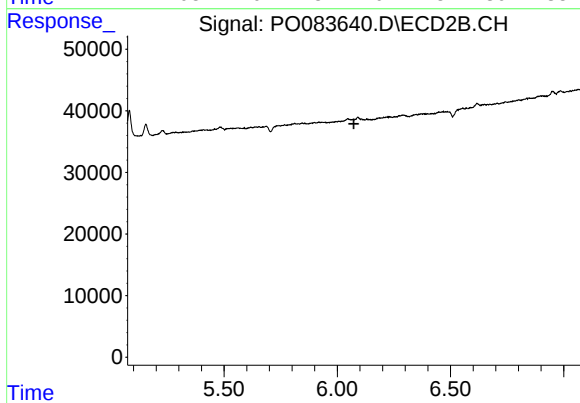

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 6.073 min
Response: 0
Conc: N.D.

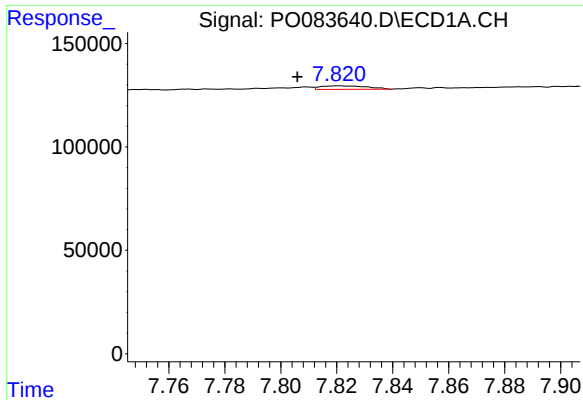

#28 AR-1254-3


R.T.: 7.821 min
Delta R.T.: 0.015 min
Response: 19453
Conc: 3.90 ng/ml

Instrument :
ECD_O
ClientSampleId :

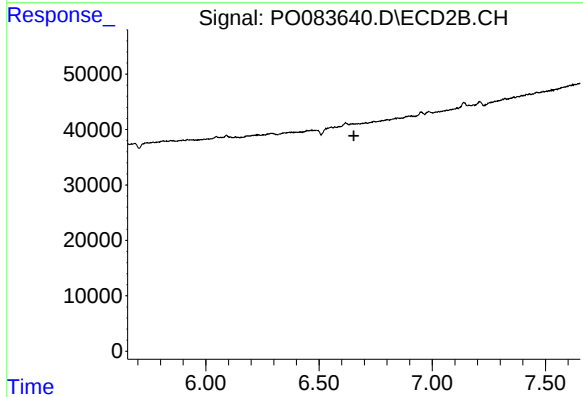


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.654 min
Response: 0
Conc: N.D.

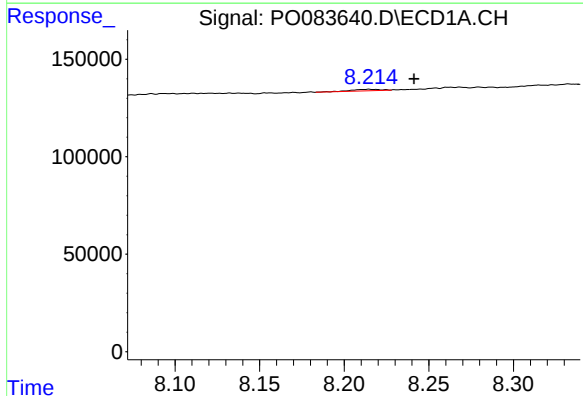

#32 AR-1260-2

R.T.: 8.215 min
Delta R.T.: -0.027 min
Response: 9153
Conc: 2.19 ng/ml

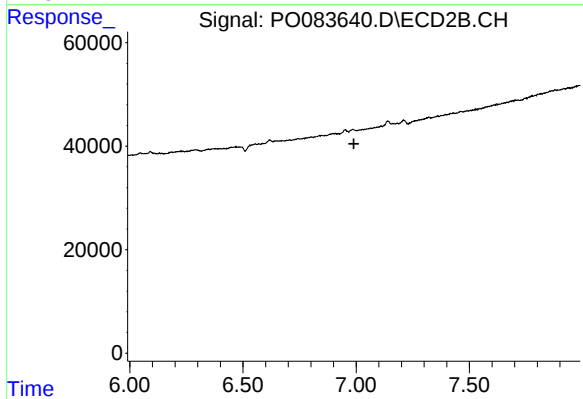

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.990 min
Response: 0
Conc: N.D.