

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121321\
 Data File : PO083634.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Dec 2021 15:35
 Operator : AJ\MA
 Sample : M5022-49
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP14

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 14 00:10:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 07 13:18:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.937	3.943	1947949	649001	20.418	20.864
2) SA Decachlor...	11.014	9.240	1262964	516999	17.679	15.847

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121321\
Data File : P0083634.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Dec 2021 15:35
Operator : AJ\MA
Sample : M5022-49
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP14

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 14 00:10:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120621.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 07 13:18:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

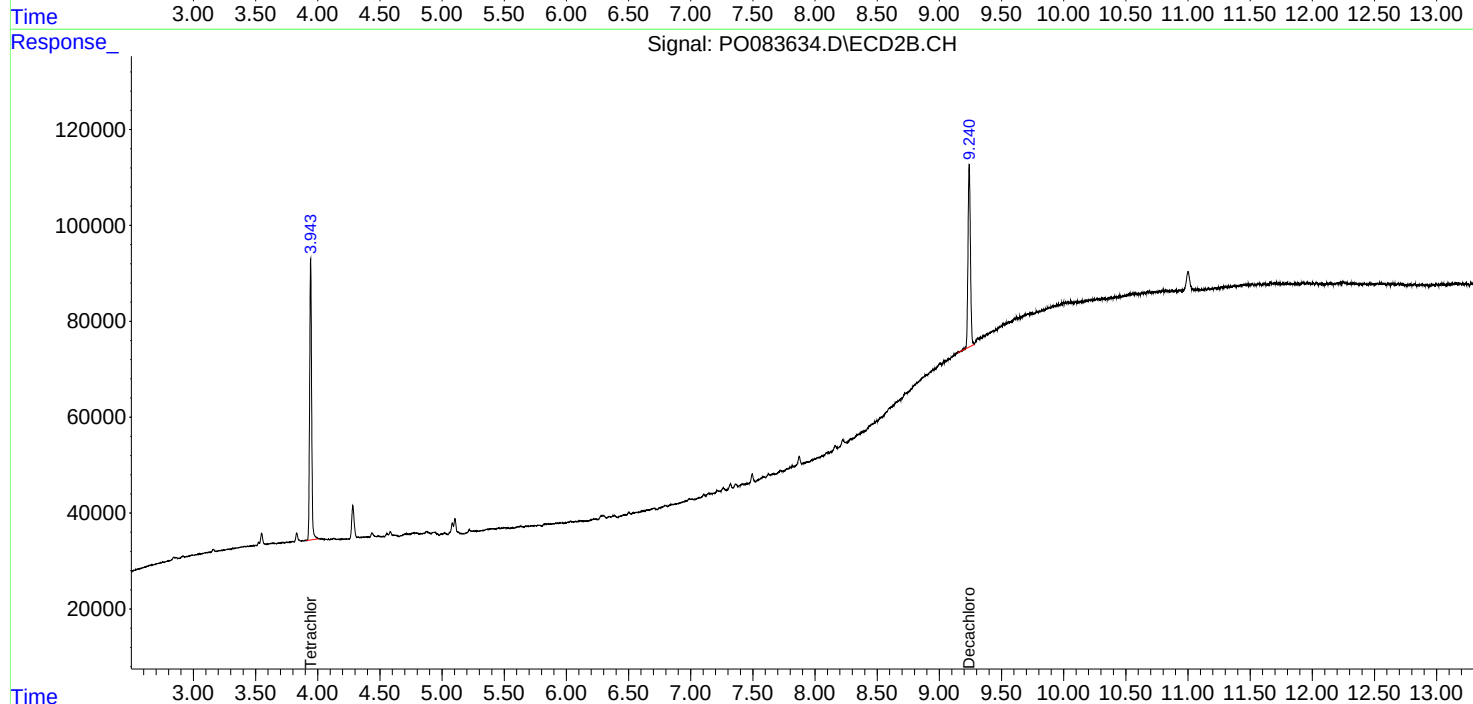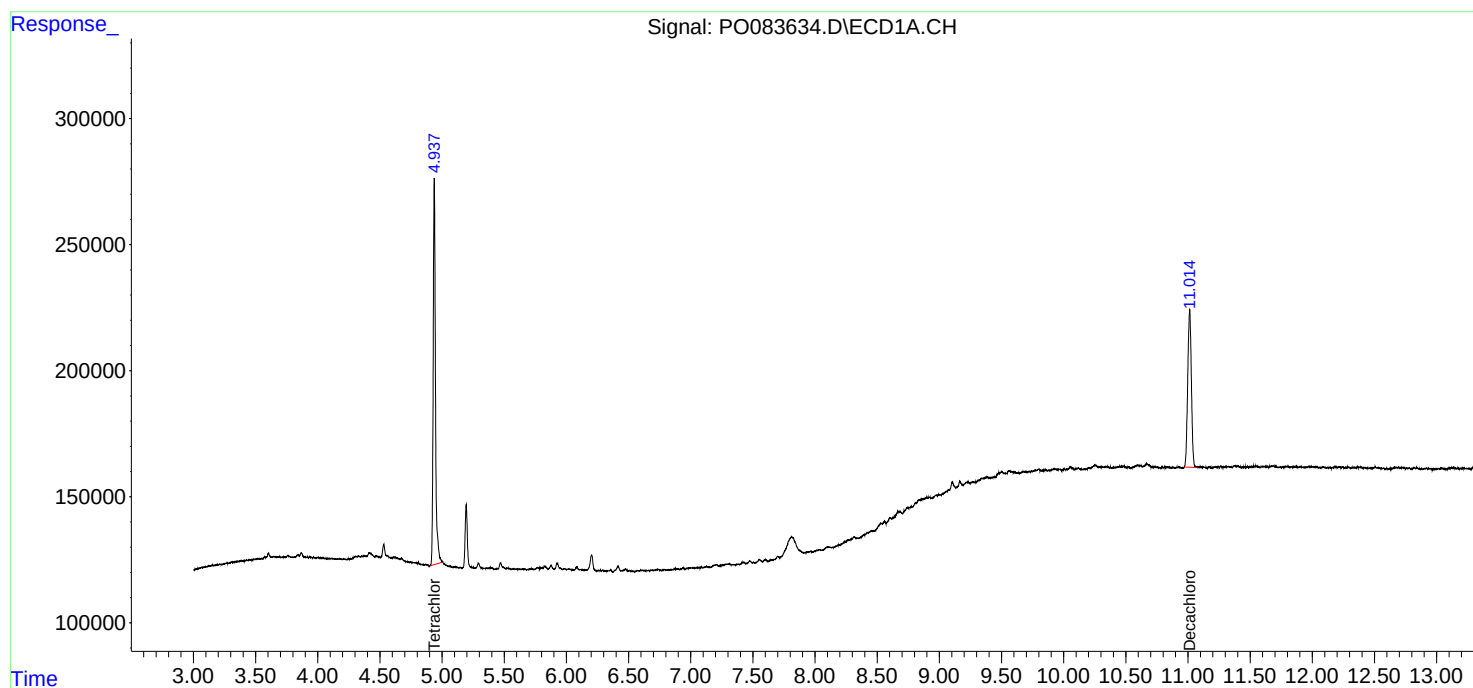


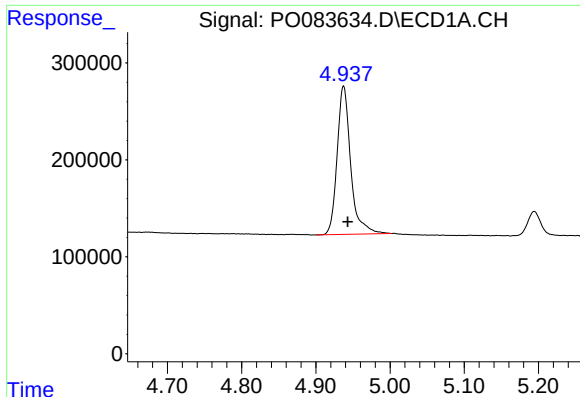

#1 Tetrachloro-m-xylene


R.T.: 4.937 min
Delta R.T.: -0.006 min
Response: 1947949
Conc: 20.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP14

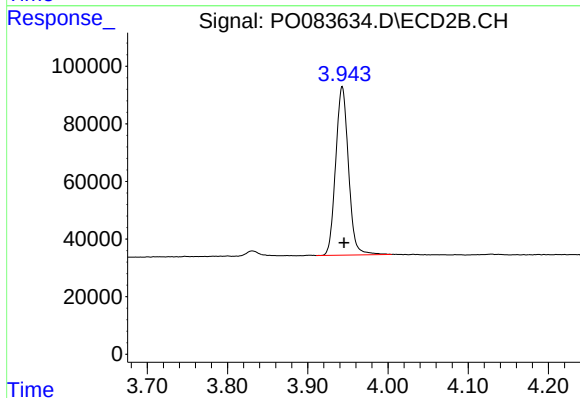


#1 Tetrachloro-m-xylene

R.T.: 3.943 min
Delta R.T.: -0.002 min
Response: 649001
Conc: 20.86 ng/ml

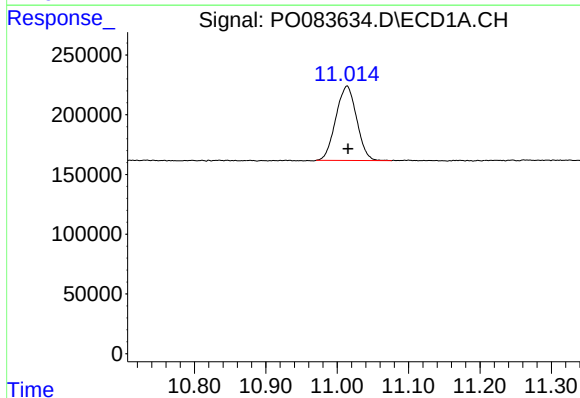

#2 Decachlorobiphenyl

R.T.: 11.014 min
Delta R.T.: -0.001 min
Response: 1262964
Conc: 17.68 ng/ml

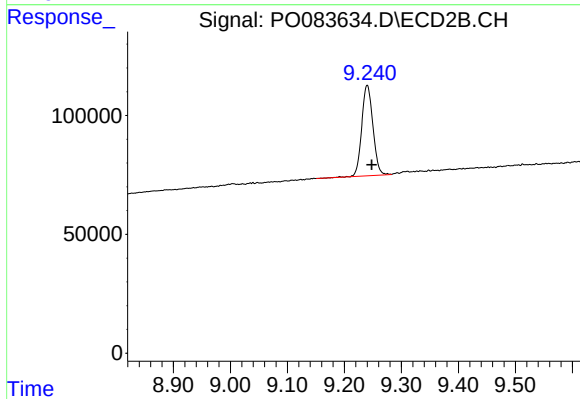

#2 Decachlorobiphenyl

R.T.: 9.240 min
Delta R.T.: -0.008 min
Response: 516999
Conc: 15.85 ng/ml