

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121418\
 Data File : P0052561.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Dec 2018 00:45
 Operator : SM/SJ
 Sample : J6374-01
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-GF-02-029-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 06:09:00 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120318.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 04 03:10:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.260	3.282	19156187	4087128	22.251	18.325
2) SA Decachlor...	9.814	7.967	6554492	2552323	13.097m	12.243

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121418\
Data File : PO052561.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Dec 2018 00:45
Operator : SM/SJ
Sample : J6374-01
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-GF-02-029-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 06:09:00 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 04 03:10:39 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

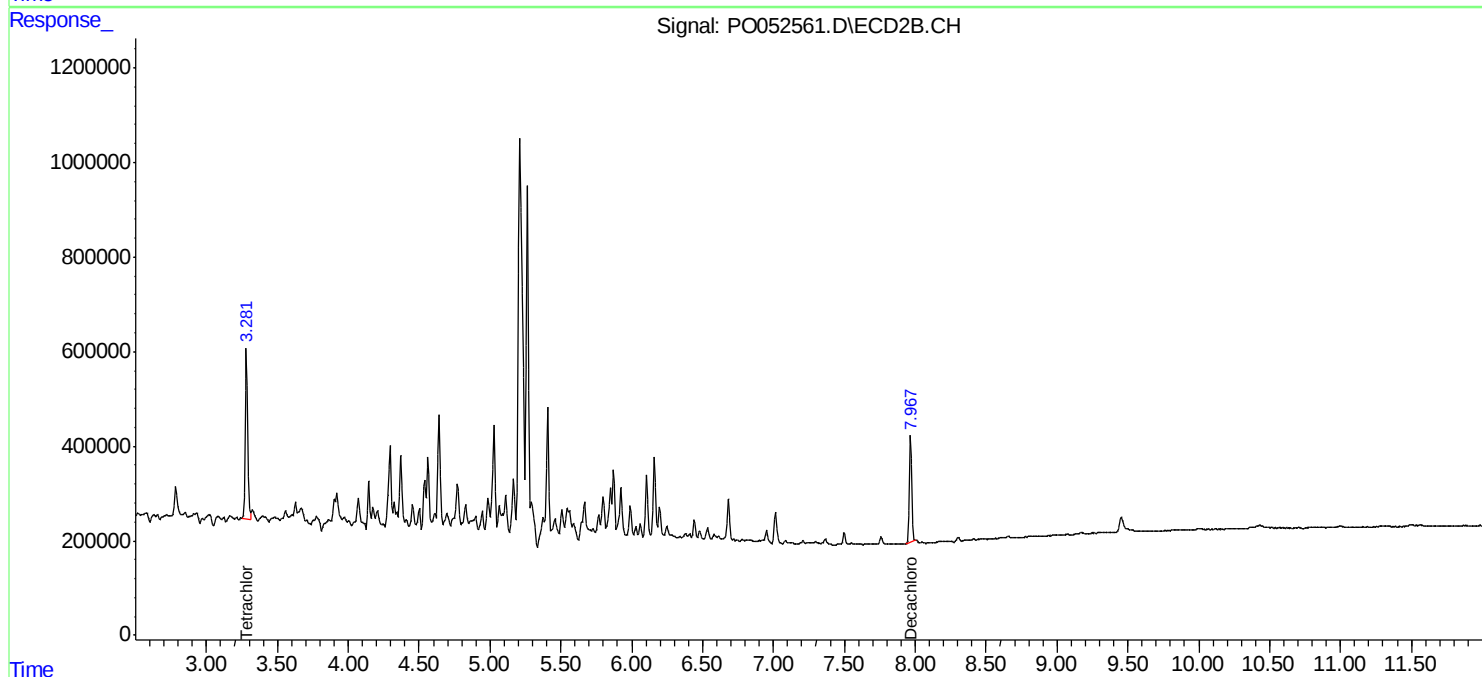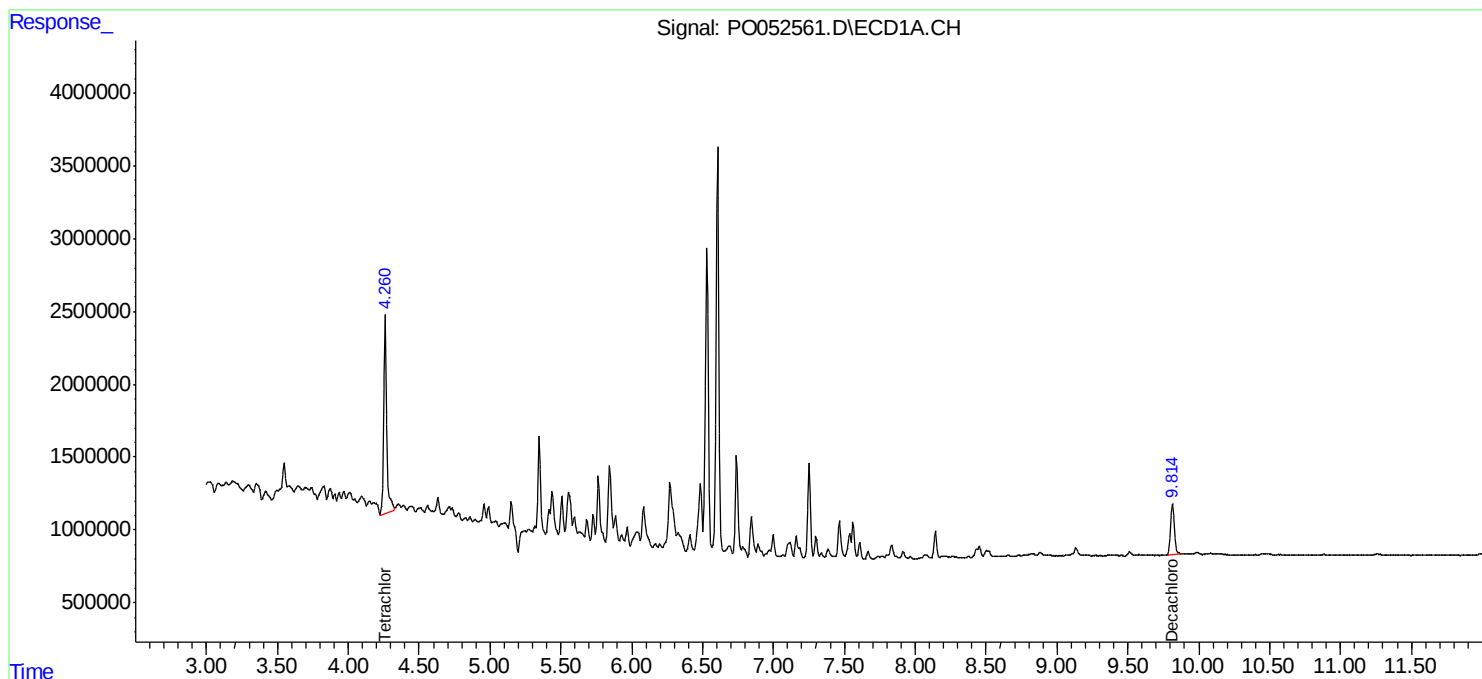


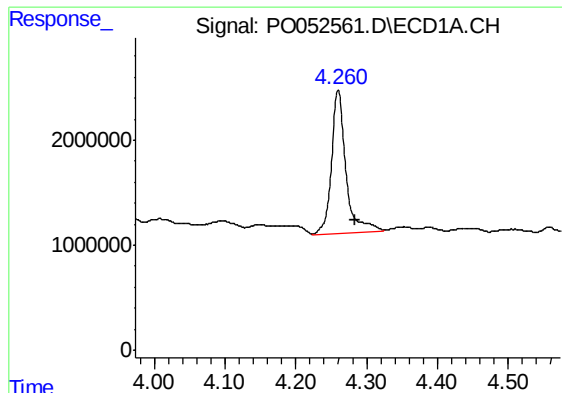

#1 Tetrachloro-m-xylene


R.T.: 4.260 min
Delta R.T.: -0.023 min
Response: 19156187
Conc: 22.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-GF-02-029-A

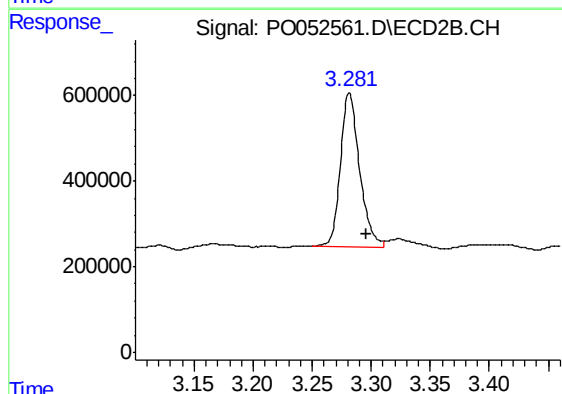


#1 Tetrachloro-m-xylene

R.T.: 3.282 min
Delta R.T.: -0.015 min
Response: 4087128
Conc: 18.33 ng/ml

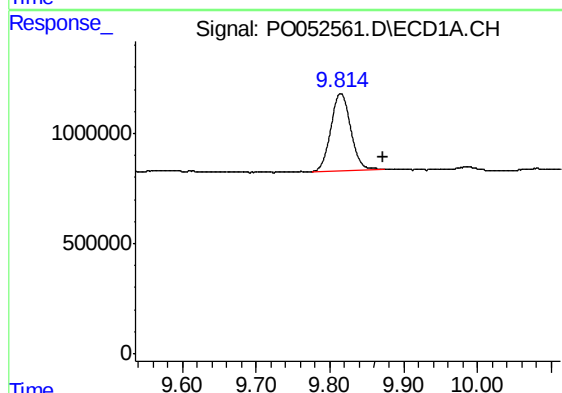

#2 Decachlorobiphenyl

R.T.: 9.814 min
Delta R.T.: -0.058 min
Response: 6554492
Conc: 13.10 ng/ml m

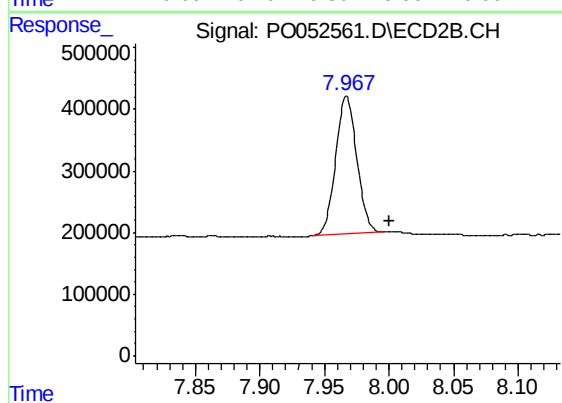

#2 Decachlorobiphenyl

R.T.: 7.967 min
Delta R.T.: -0.033 min
Response: 2552323
Conc: 12.24 ng/ml