

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121418\
 Data File : P0052567.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Dec 2018 2:27
 Operator : SM/SJ
 Sample : J6374-03
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-GF-02-029-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 06:34:52 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120318.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 04 03:10:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.260	3.281	12593233	2990193	14.628	13.407m
2) SA Decachlor...	9.815	7.968	5188012	1889071	10.367	9.061

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121418\
Data File : PO052567.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Dec 2018 2:27
Operator : SM/SJ
Sample : J6374-03
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-GF-02-029-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 06:34:52 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 04 03:10:39 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

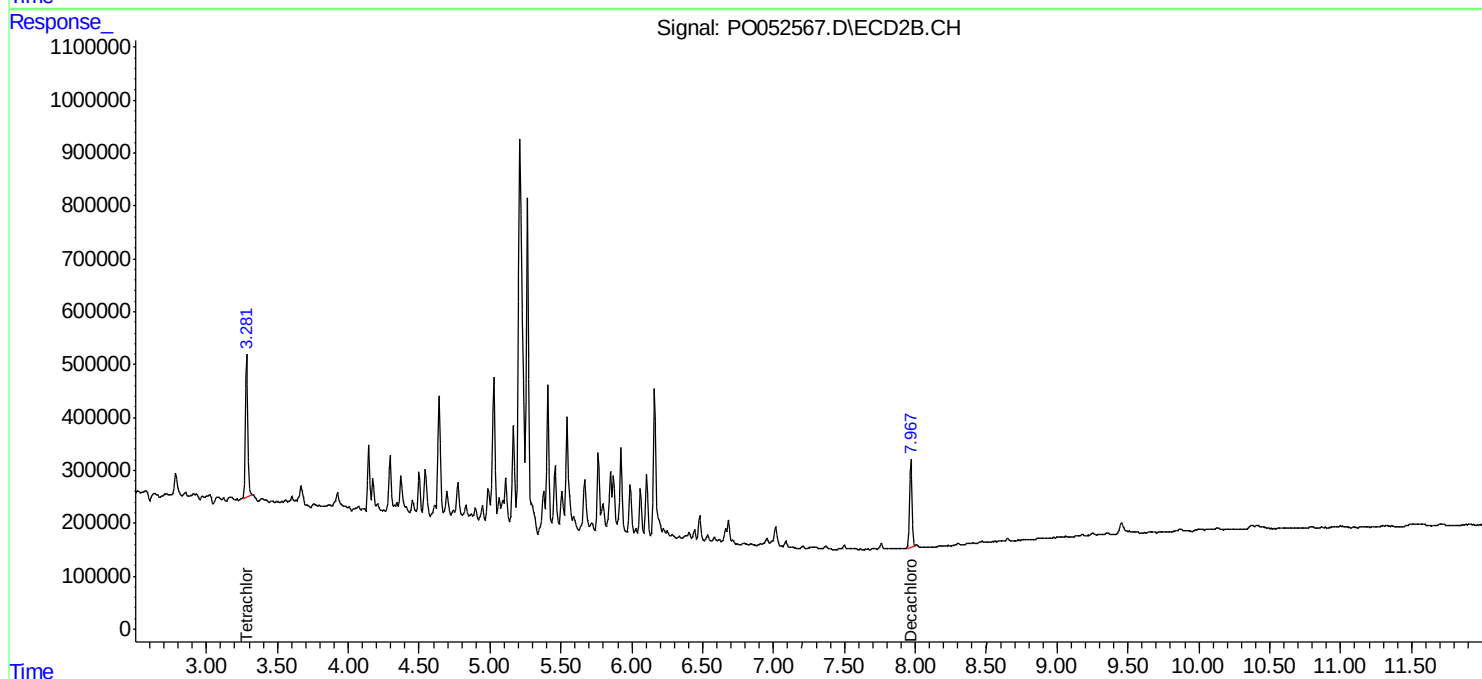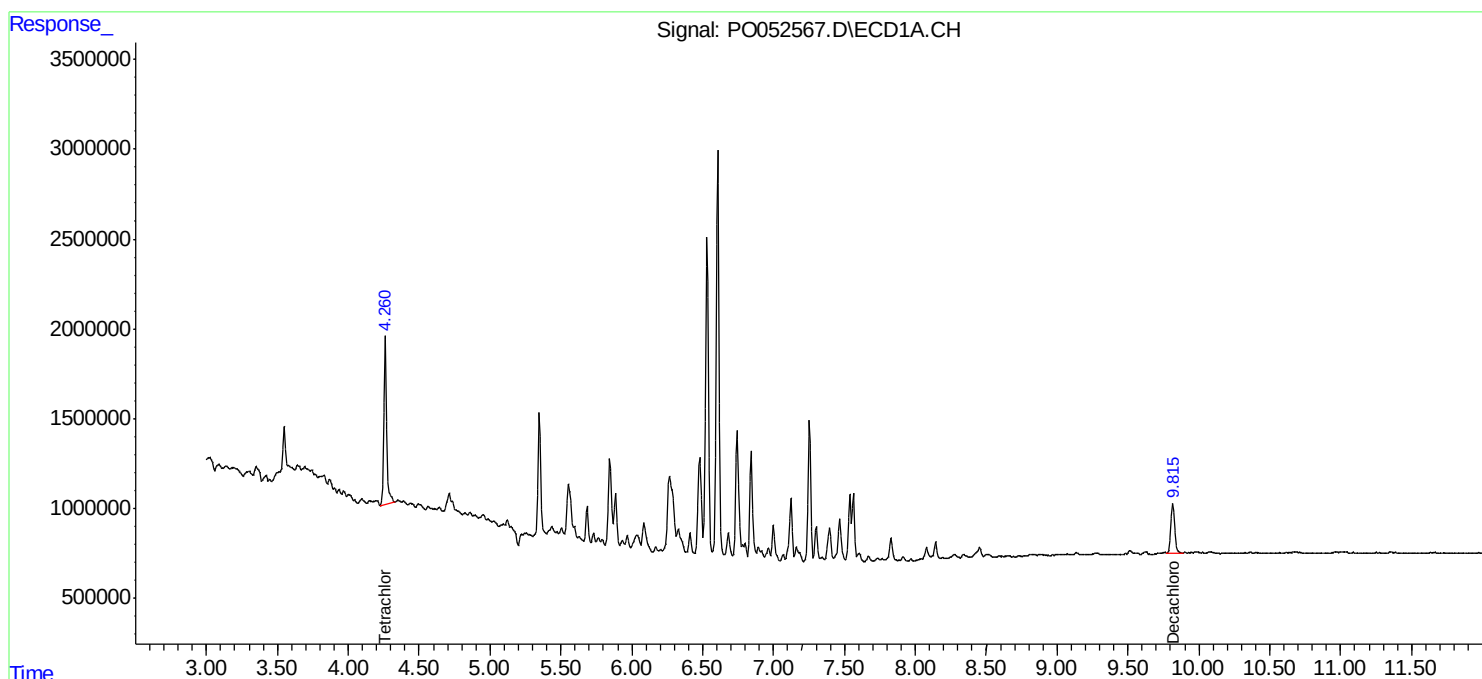


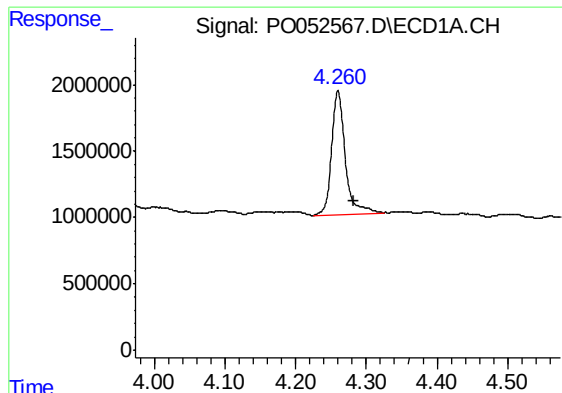

#1 Tetrachloro-m-xylene


R.T.: 4.260 min
Delta R.T.: -0.023 min
Response: 12593233
Conc: 14.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-GF-02-029-B

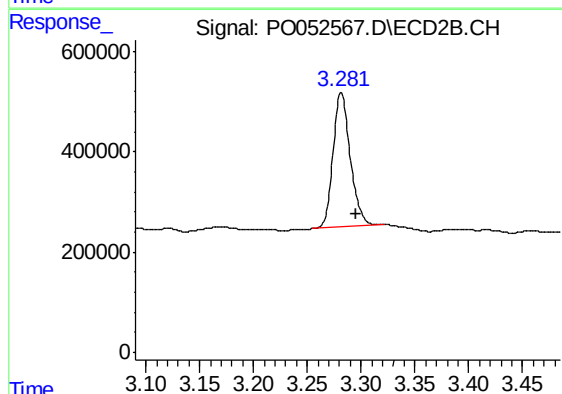


#1 Tetrachloro-m-xylene

R.T.: 3.281 min
Delta R.T.: -0.015 min
Response: 2990193
Conc: 13.41 ng/ml m

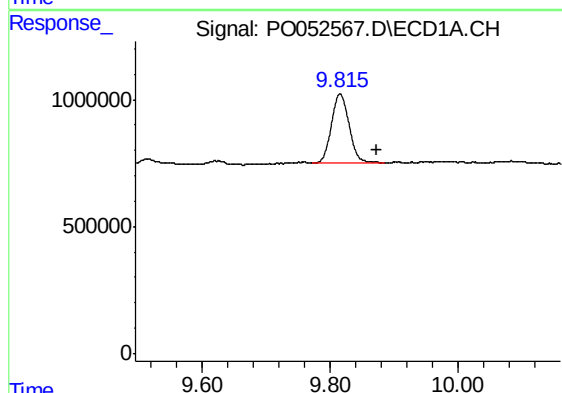

#2 Decachlorobiphenyl

R.T.: 9.815 min
Delta R.T.: -0.057 min
Response: 5188012
Conc: 10.37 ng/ml

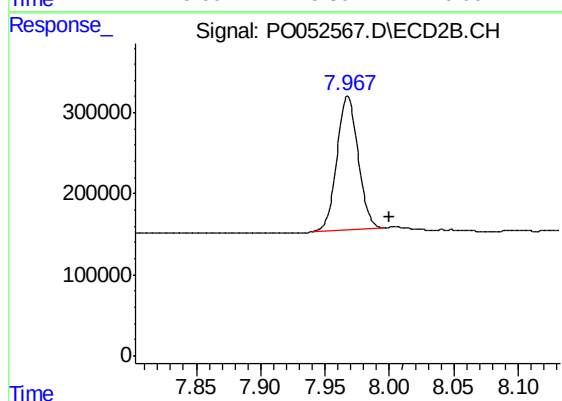

#2 Decachlorobiphenyl

R.T.: 7.968 min
Delta R.T.: -0.032 min
Response: 1889071
Conc: 9.06 ng/ml