

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121418\
 Data File : P0052572.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Dec 2018 3:51
 Operator : SM/SJ
 Sample : J6430-02 10X
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 B368121

Manual Integrations
 APPROVED

Sohil
 12/17/2018 2:23:57 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 22:49:30 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120318.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 04 03:10:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.263	3.282	1258757	323224	1.462m	1.449
2) SA Decachlor...	9.816	7.967	801434	257015	1.601m	1.233

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121418\
Data File : PO052572.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Dec 2018 3:51
Operator : SM/SJ
Sample : J6430-02 10X
Misc :
ALS Vial : 55 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
B368121


Manual Integrations
APPROVED

Sohil
12/17/2018 2:23:57 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 22:49:30 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 04 03:10:39 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

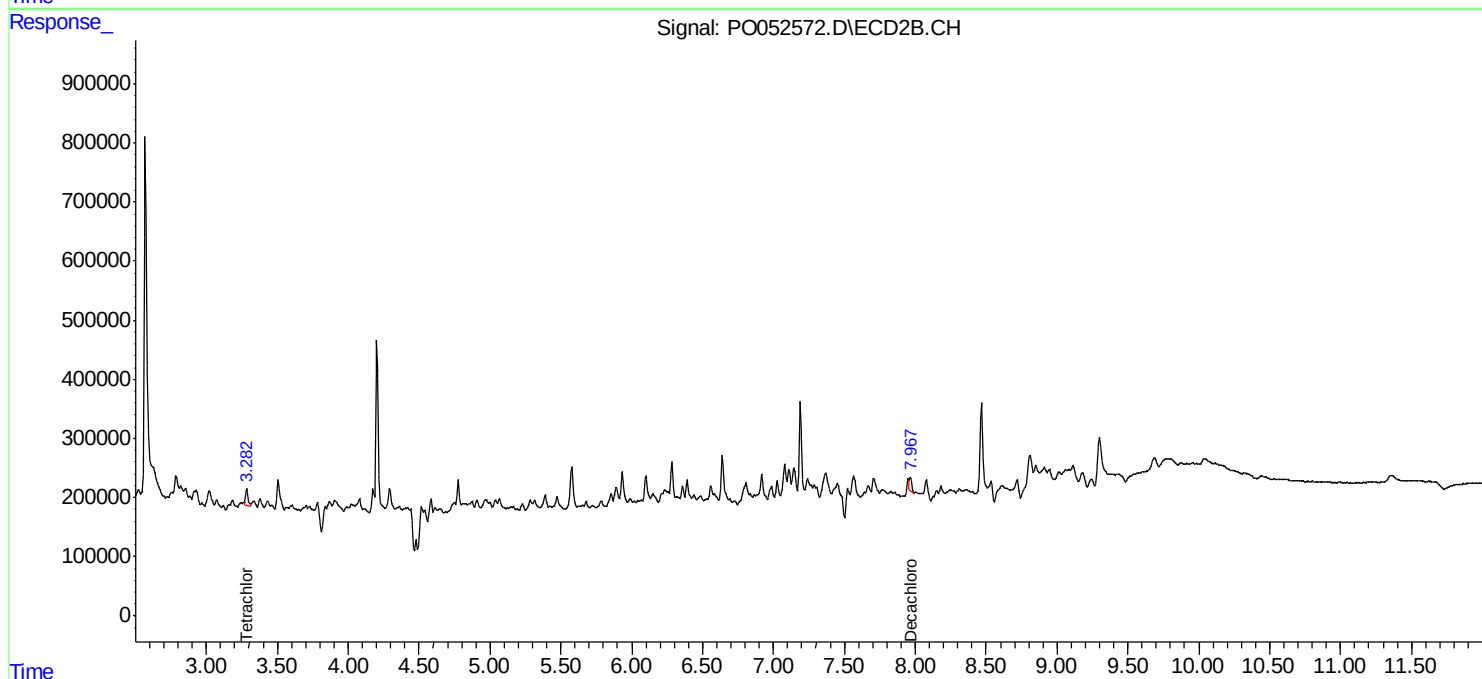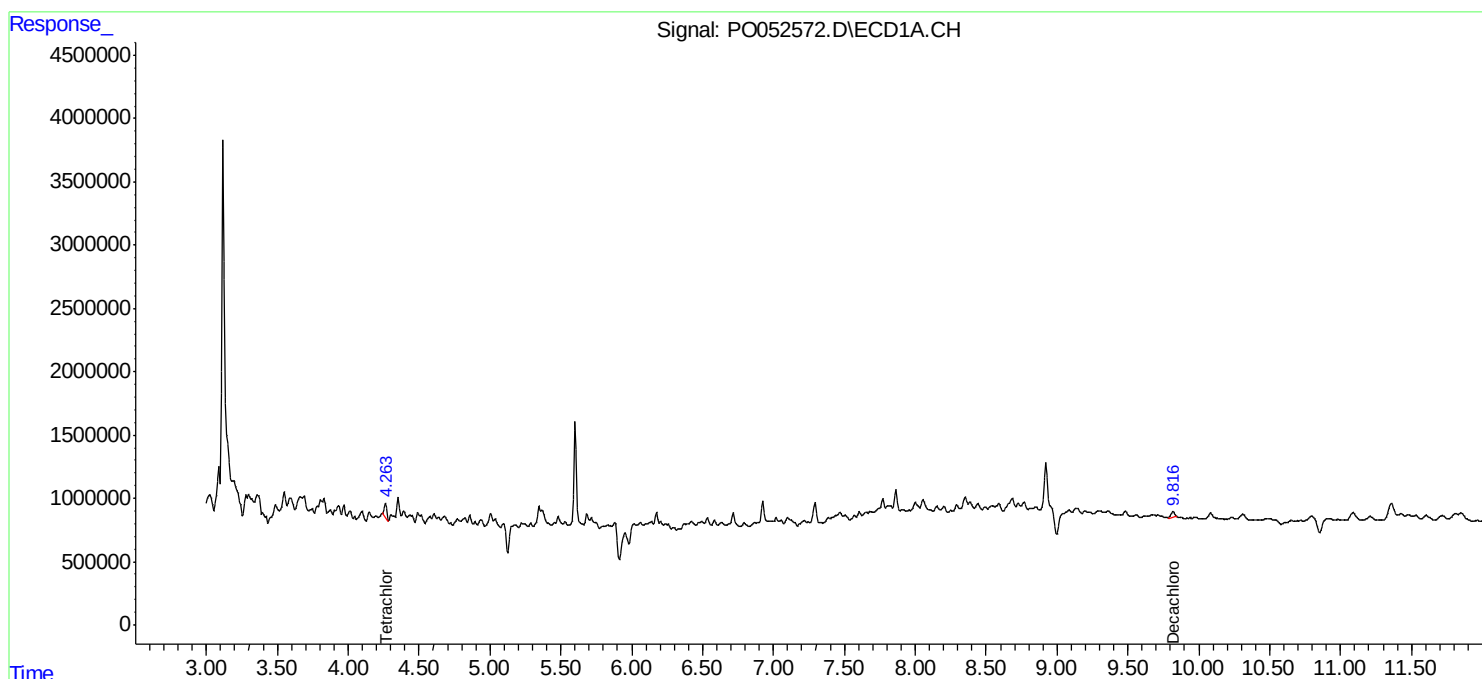

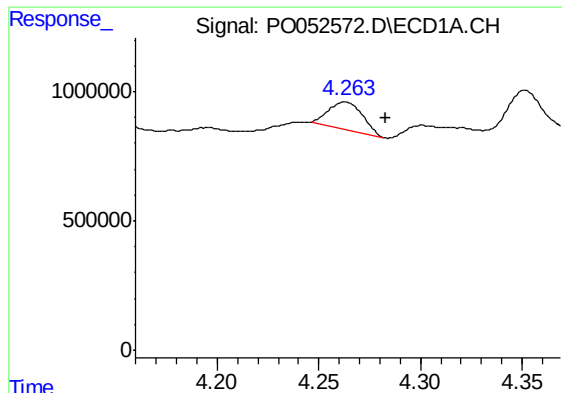


#1 Tetrachloro-m-xylene

R.T.: 4.263 min
Delta R.T.: -0.020 min
Response: 1258757
Conc: 1.46 ng/ml m

Instrument :
ECD_O
ClientSampleId :
B368121


Manual Integrations
APPROVED

Sohil
12/17/2018 2:23:57 PM

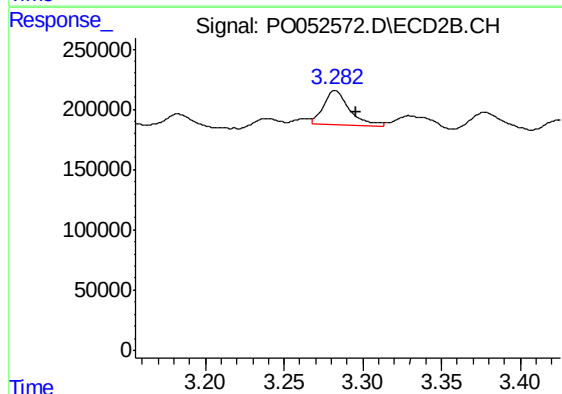


#1 Tetrachloro-m-xylene

R.T.: 3.282 min
Delta R.T.: -0.014 min
Response: 323224
Conc: 1.45 ng/ml

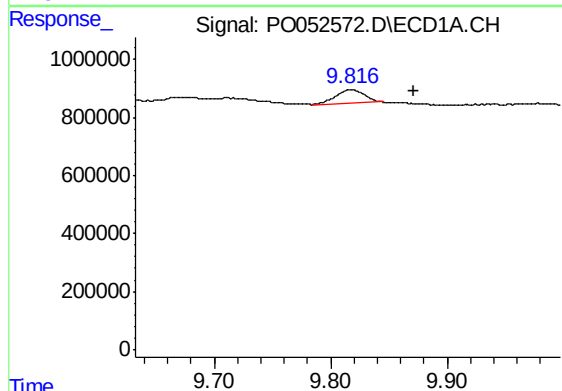

#2 Decachlorobiphenyl

R.T.: 9.816 min
Delta R.T.: -0.055 min
Response: 801434
Conc: 1.60 ng/ml m

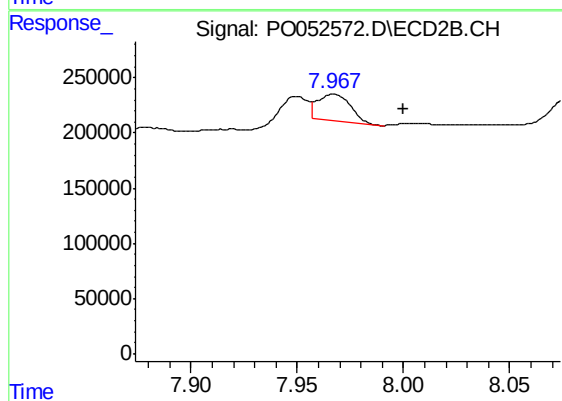

#2 Decachlorobiphenyl

R.T.: 7.967 min
Delta R.T.: -0.033 min
Response: 257015
Conc: 1.23 ng/ml