

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO121420\
 Data File : PO073756.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Dec 2020 11:58
 Operator : DD\AJ
 Sample : L5042-06MSD
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 KENS-B6-121020-0-6MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 03:26:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO121020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 11 03:58:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.938	3.998	2133776	1220778	23.338	22.760
2)	SA Decachlor...	10.965	9.264	1850020	1106044	22.387	23.638
Target Compounds							
3)	L1 AR-1016-1	6.262	5.247	2132342	1163481	606.851	532.644
4)	L1 AR-1016-2	6.286	5.267	2911404	1637652	595.658	541.183
5)	L1 AR-1016-3	6.353	5.457	1886109	857991	640.300	526.301
6)	L1 AR-1016-4	6.460	5.509	1529754	671853	620.686	509.478
7)	L1 AR-1016-5	6.776	5.736	1271661	872211	535.598	532.300
8)	L2 AR-1221-1	5.185	4.252	172604	92297	162.906	137.780
9)	L2 AR-1221-2	5.289	4.352	207284	140453	263.888	273.159
10)	L2 AR-1221-3	5.376	4.439	938160	561844	385.654	368.423
11)	L3 AR-1232-1	5.376	4.439	938160	561844	454.971	434.711
12)	L3 AR-1232-2	5.967	5.267	1567057	1637652	1465.587	1232.356
13)	L3 AR-1232-3	6.286	5.457	2911404	857991	1356.699	1178.974
14)	L3 AR-1232-4	6.460	5.553	1529754	798288	1436.410	1307.850
15)	L3 AR-1232-5	6.558	5.736	1112739	872211	1554.135	1305.078
16)	L4 AR-1242-1	6.262	5.247	2132342	1163481	752.351	661.514
17)	L4 AR-1242-2	6.286	5.267	2911404	1637652	747.528	669.596
18)	L4 AR-1242-3	6.353	5.457	1886109	857991	795.135	655.595
19)	L4 AR-1242-4	6.460	5.553	1529754	798288	776.067	637.858
20)	L4 AR-1242-5	7.246	6.113	191260	772482	87.580	453.176 #
21)	L5 AR-1248-1	6.262	5.247	2132342	1163481	981.337	849.772
22)	L5 AR-1248-2	6.558	5.509	1112739	671853	398.183	362.105
23)	L5 AR-1248-3	6.776	5.553	1271661	798288	388.294	425.490
24)	L5 AR-1248-4	7.206	5.736	231093	872211	57.785	387.506 #
25)	L5 AR-1248-5	7.246	6.156	191260	147075	50.575	63.300 #
26)	L6 AR-1254-1	7.176	6.113	997198	772482	262.712	218.582
27)	L6 AR-1254-2	7.405	6.272	1106865	692164	187.738	221.704
28)	L6 AR-1254-3	7.789	6.708	561811	1284935	91.692	262.446 #
29)	L6 AR-1254-4	8.084	6.927	391991	169242	74.722	48.258 #
30)	L6 AR-1254-5	8.514	7.353	3511108	2524204	681.699	572.430
31)	L7 AR-1260-1	7.956	6.825	2356724	1727945	557.615	558.971
32)	L7 AR-1260-2	8.222	7.022	3068966	2328524	546.292	574.021
33)	L7 AR-1260-3	8.589	7.175	2122688	1999782	464.369	572.952
34)	L7 AR-1260-4	8.820	7.656	2189548	1468418	462.475	486.272
35)	L7 AR-1260-5	9.148	7.902	4834270	3729201	484.408	499.219
36)	L8 AR-1262-1	8.589	7.353	2122688	2524204	283.547	1009.762 #
37)	L8 AR-1262-2	9.148	7.902	4834270	3729201	376.914	423.948
38)	L8 AR-1262-3	9.480f	8.188	2934745	725206	345.922	200.561 #
39)	L8 AR-1262-4	9.533f	8.249	1648826	2389907	492.988	388.408
40)	L8 AR-1262-5	10.219	8.745	1142311	712270	252.724	250.185
41)	L9 AR-1268-1	9.480f	8.188	2934745	725206	206.046	75.358 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121420\
 Data File : PO073756.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Dec 2020 11:58
 Operator : DD\AJ
 Sample : L5042-06MSD
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 KENS-B6-121020-0-6MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 03:26:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 11 03:58:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	9.533f	8.249	1648826	2389907	133.757	290.086 #
43) L9	AR-1268-3	9.780	8.459	113932	55954	10.498	7.925
44) L9	AR-1268-4	10.219	8.745	1142311	712270	243.848	240.631
45) L9	AR-1268-5	10.631	9.023	357643	221717	10.928	11.036



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121420\
Data File : P0073756.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Dec 2020 11:58
Operator : DD\AJ
Sample : L5042-06MSD
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
KENS-B6-121020-0-6MSD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 03:26:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 11 03:58:06 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

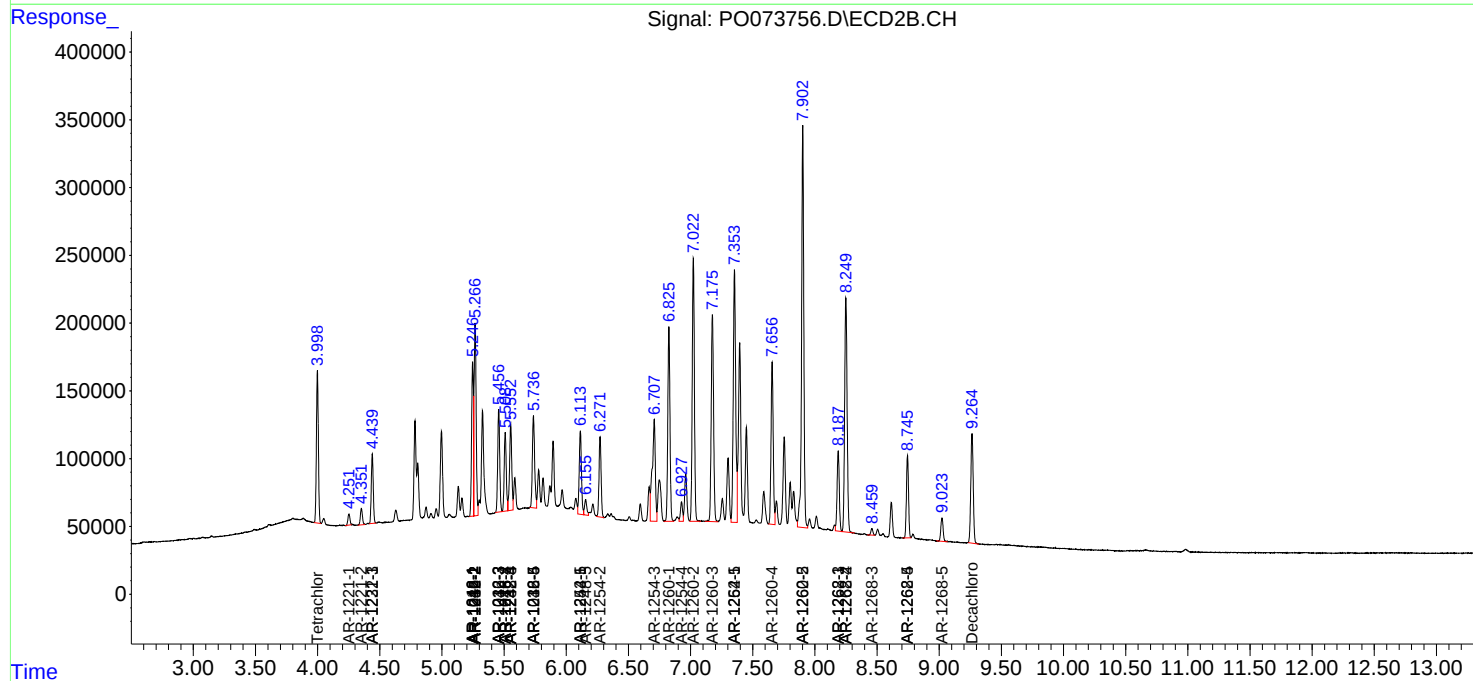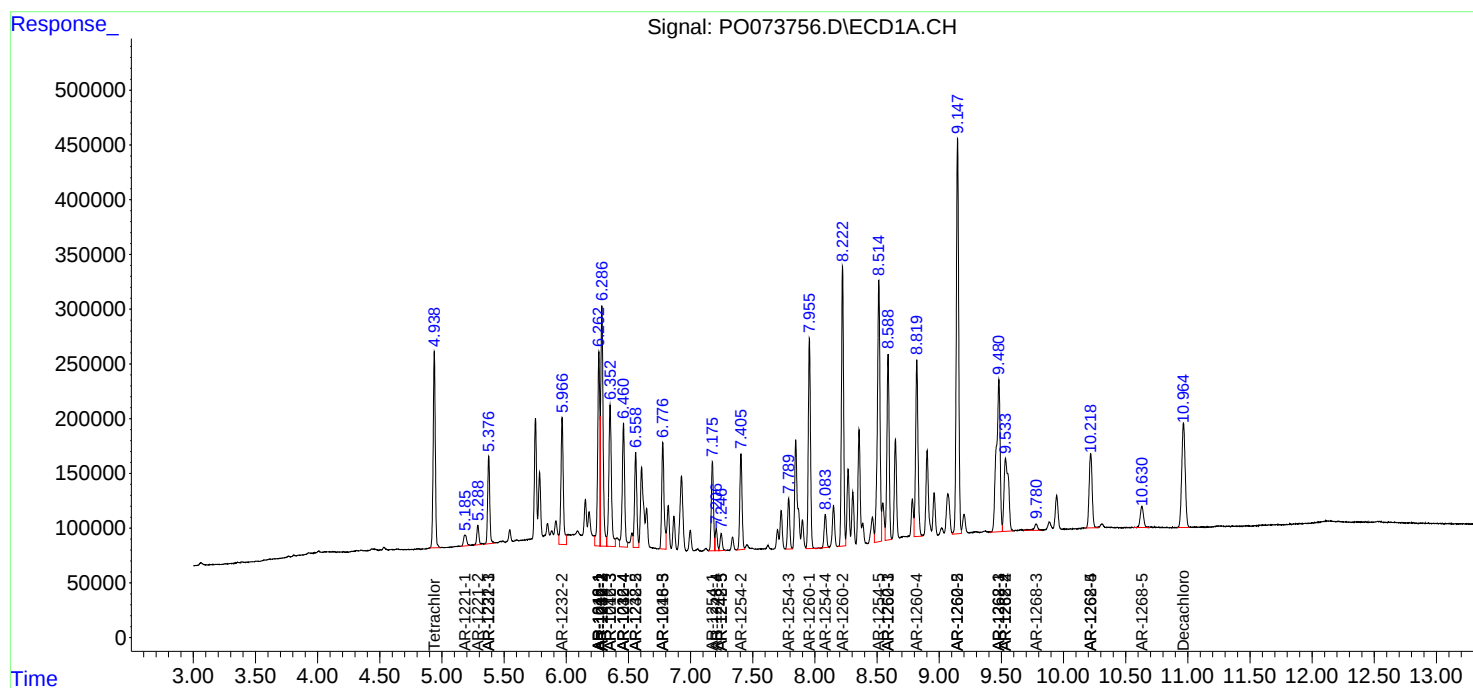


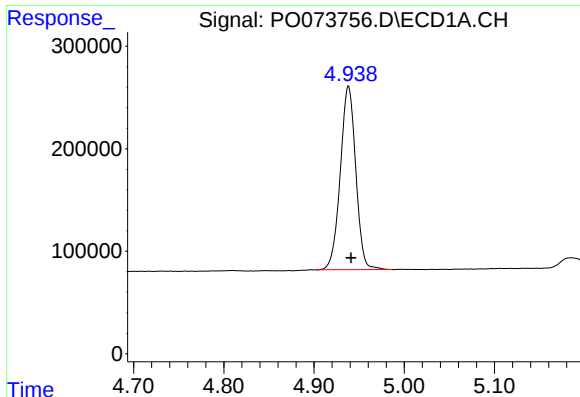

#1 Tetrachloro-m-xylene


R.T.: 4.938 min
Delta R.T.: -0.003 min
Response: 2133776
Conc: 23.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
KENS-B6-121020-0-6MSD

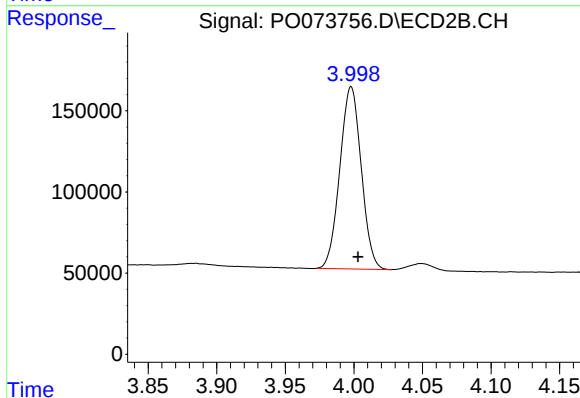


#1 Tetrachloro-m-xylene

R.T.: 3.998 min
Delta R.T.: -0.005 min
Response: 1220778
Conc: 22.76 ng/ml

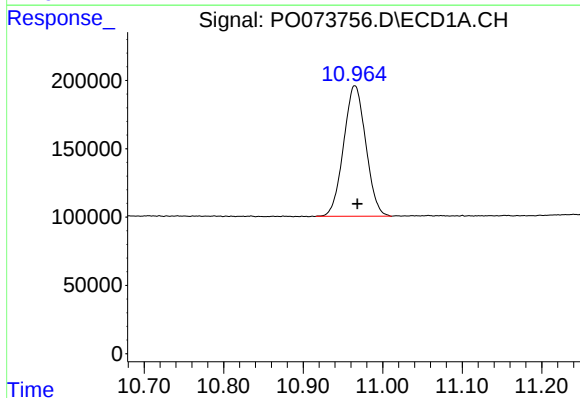


#2 Decachlorobiphenyl

R.T.: 10.965 min
Delta R.T.: -0.003 min
Response: 1850020
Conc: 22.39 ng/ml

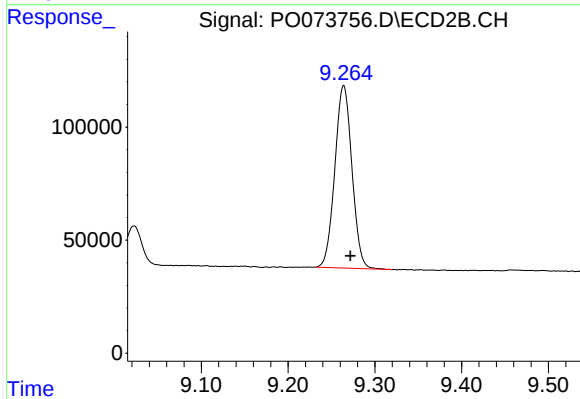

#2 Decachlorobiphenyl


R.T.: 9.264 min
Delta R.T.: -0.008 min
Response: 1106044
Conc: 23.64 ng/ml

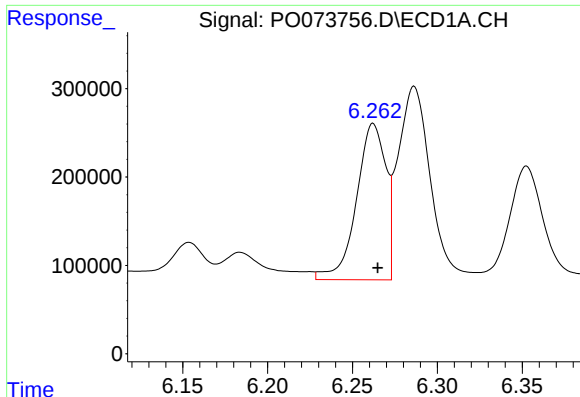

#3 AR-1016-1


R.T.: 6.262 min
Delta R.T.: -0.003 min
Response: 2132342
Conc: 606.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
KENS-B6-121020-0-6MSD

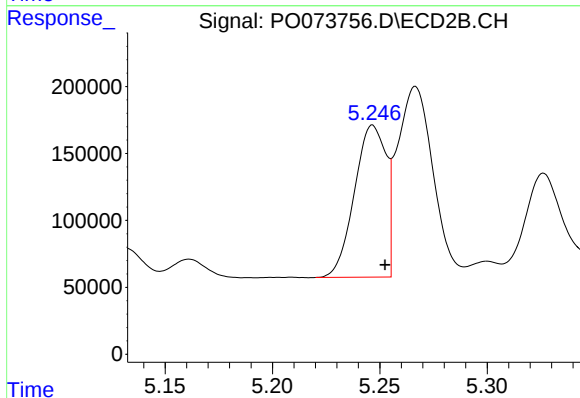


#3 AR-1016-1

R.T.: 5.247 min
Delta R.T.: -0.006 min
Response: 1163481
Conc: 532.64 ng/ml

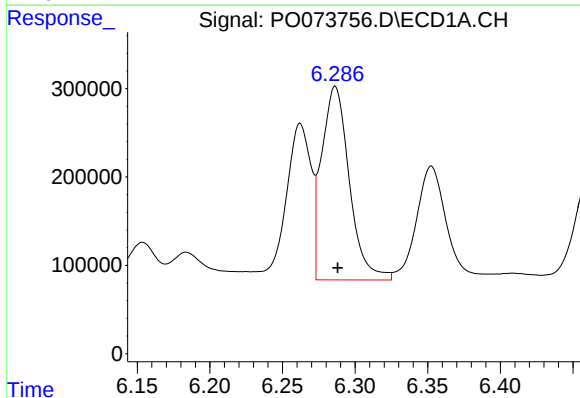


#4 AR-1016-2

R.T.: 6.286 min
Delta R.T.: -0.002 min
Response: 2911404
Conc: 595.66 ng/ml

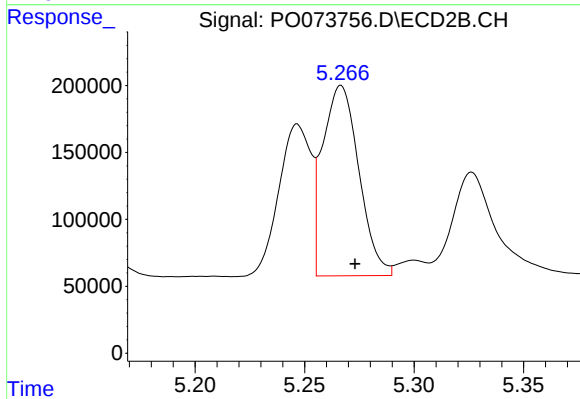

#4 AR-1016-2


R.T.: 5.267 min
Delta R.T.: -0.006 min
Response: 1637652
Conc: 541.18 ng/ml

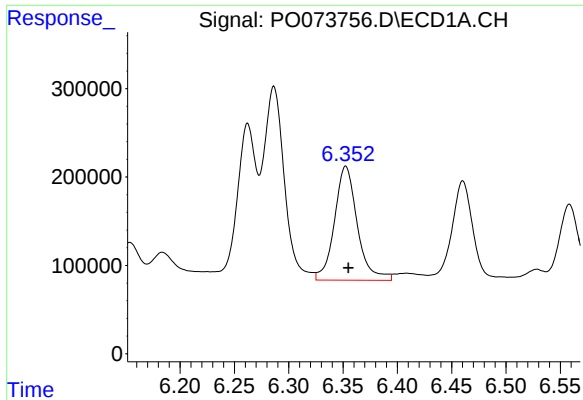

#5 AR-1016-3


R.T.: 6.353 min
Delta R.T.: -0.002 min
Response: 1886109
Conc: 640.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
KENS-B6-121020-0-6MSD

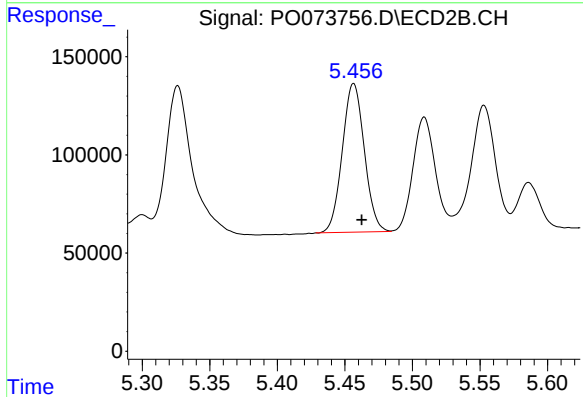


#5 AR-1016-3

R.T.: 5.457 min
Delta R.T.: -0.006 min
Response: 857991
Conc: 526.30 ng/ml

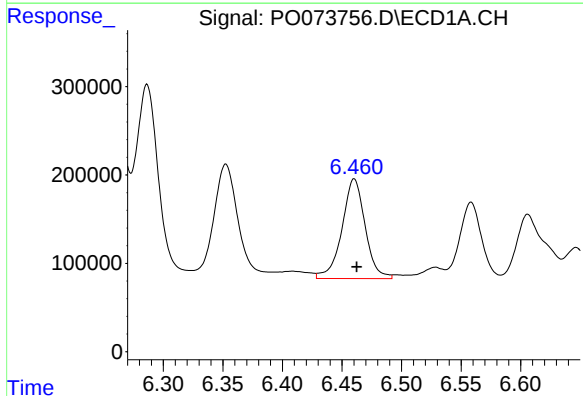


#6 AR-1016-4

R.T.: 6.460 min
Delta R.T.: -0.002 min
Response: 1529754
Conc: 620.69 ng/ml

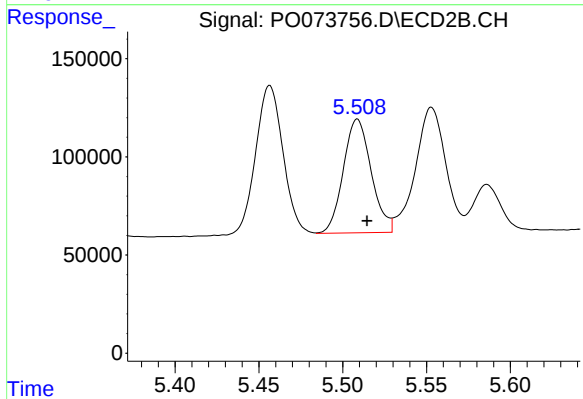

#6 AR-1016-4


R.T.: 5.509 min
Delta R.T.: -0.006 min
Response: 671853
Conc: 509.48 ng/ml

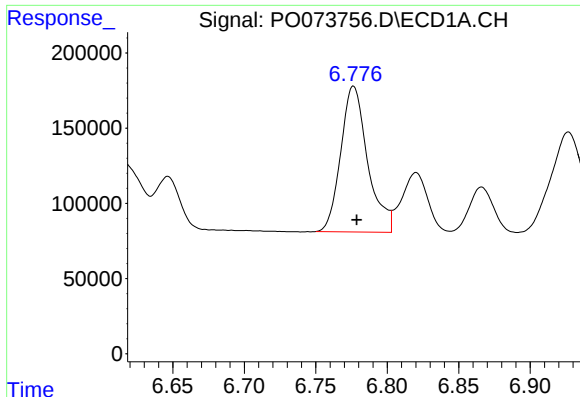

#7 AR-1016-5


R.T.: 6.776 min
Delta R.T.: -0.002 min
Response: 1271661
Conc: 535.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
KENS-B6-121020-0-6MSD

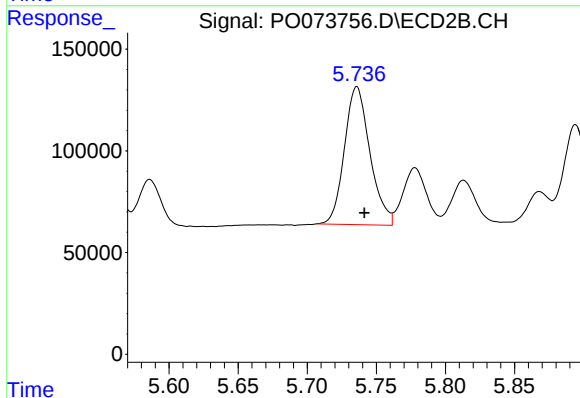


#7 AR-1016-5

R.T.: 5.736 min
Delta R.T.: -0.005 min
Response: 872211
Conc: 532.30 ng/ml

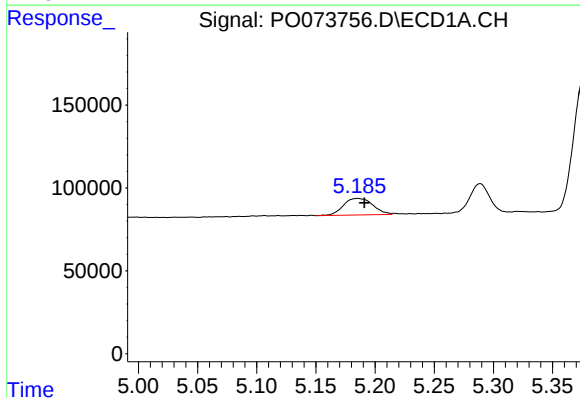


#8 AR-1221-1

R.T.: 5.185 min
Delta R.T.: -0.006 min
Response: 172604
Conc: 162.91 ng/ml

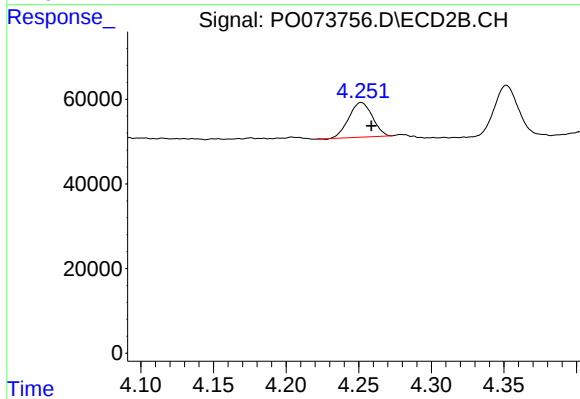

#8 AR-1221-1


R.T.: 4.252 min
Delta R.T.: -0.007 min
Response: 92297
Conc: 137.78 ng/ml

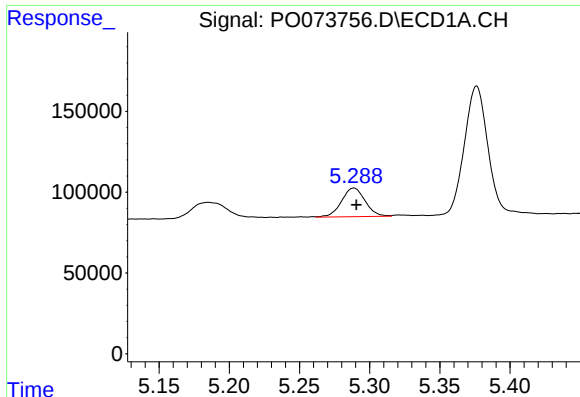

#9 AR-1221-2


R.T.: 5.289 min
Delta R.T.: -0.002 min
Response: 207284
Conc: 263.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
KENS-B6-121020-0-6MSD

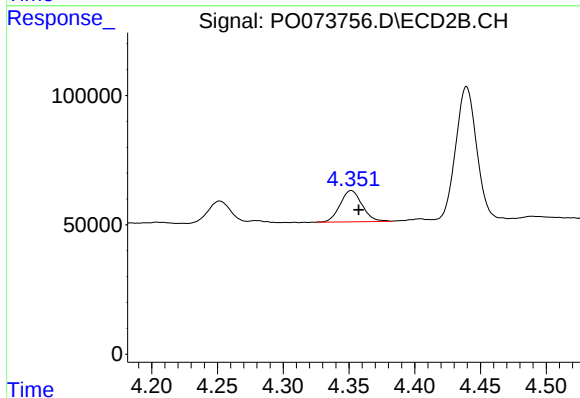


#9 AR-1221-2

R.T.: 4.352 min
Delta R.T.: -0.006 min
Response: 140453
Conc: 273.16 ng/ml

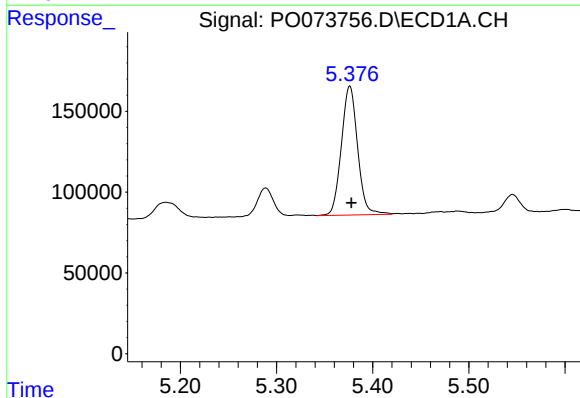


#10 AR-1221-3

R.T.: 5.376 min
Delta R.T.: -0.002 min
Response: 938160
Conc: 385.65 ng/ml

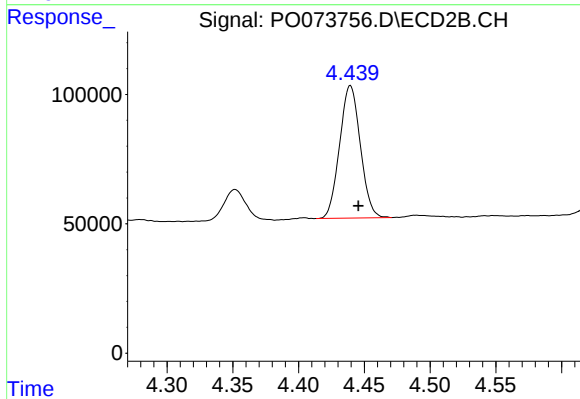

#10 AR-1221-3


R.T.: 4.439 min
Delta R.T.: -0.006 min
Response: 561844
Conc: 368.42 ng/ml

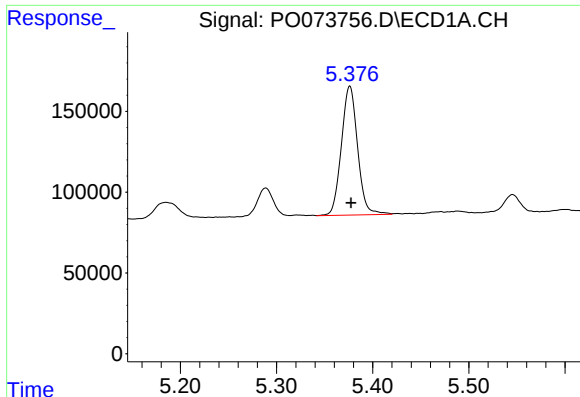

#11 AR-1232-1


R.T.: 5.376 min
Delta R.T.: -0.001 min
Response: 938160
Conc: 454.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
KENS-B6-121020-0-6MSD

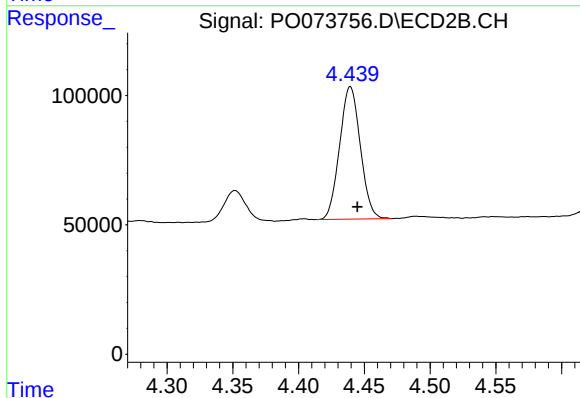


#11 AR-1232-1

R.T.: 4.439 min
Delta R.T.: -0.005 min
Response: 561844
Conc: 434.71 ng/ml

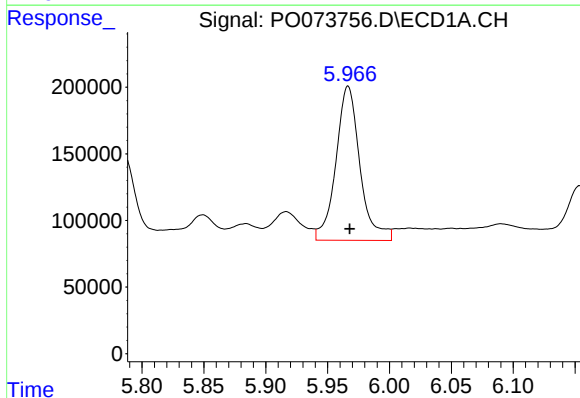


#12 AR-1232-2

R.T.: 5.967 min
Delta R.T.: -0.001 min
Response: 1567057
Conc: 1465.59 ng/ml

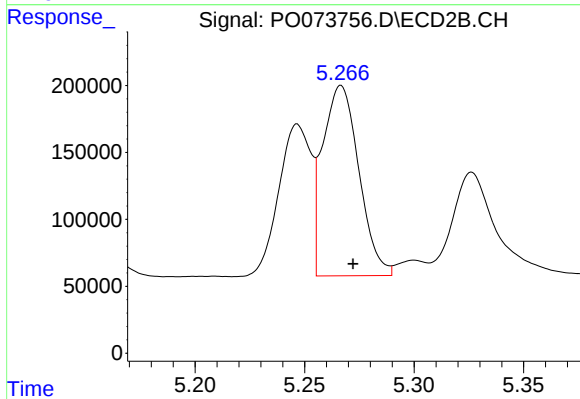

#12 AR-1232-2


R.T.: 5.267 min
Delta R.T.: -0.006 min
Response: 1637652
Conc: 1232.36 ng/ml

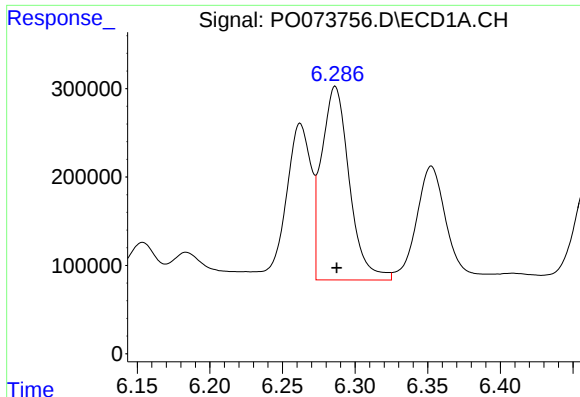

#13 AR-1232-3


R.T.: 6.286 min
Delta R.T.: -0.001 min
Response: 2911404
Conc: 1356.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
KENS-B6-121020-0-6MSD

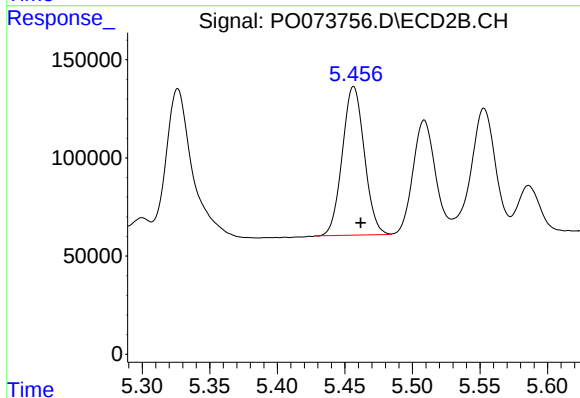


#13 AR-1232-3

R.T.: 5.457 min
Delta R.T.: -0.005 min
Response: 857991
Conc: 1178.97 ng/ml

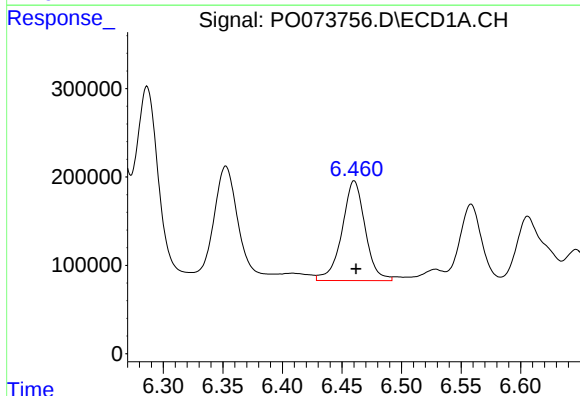


#14 AR-1232-4

R.T.: 6.460 min
Delta R.T.: -0.002 min
Response: 1529754
Conc: 1436.41 ng/ml

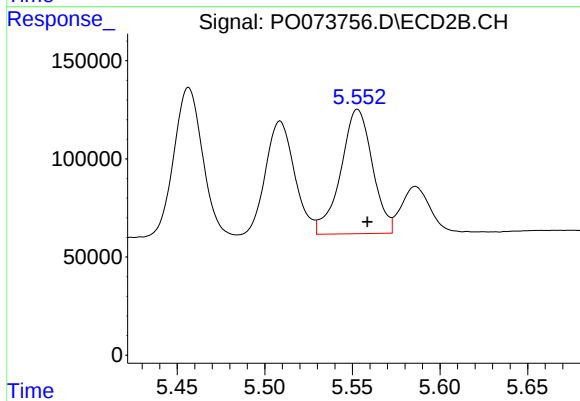

#14 AR-1232-4


R.T.: 5.553 min
Delta R.T.: -0.006 min
Response: 798288
Conc: 1307.85 ng/ml

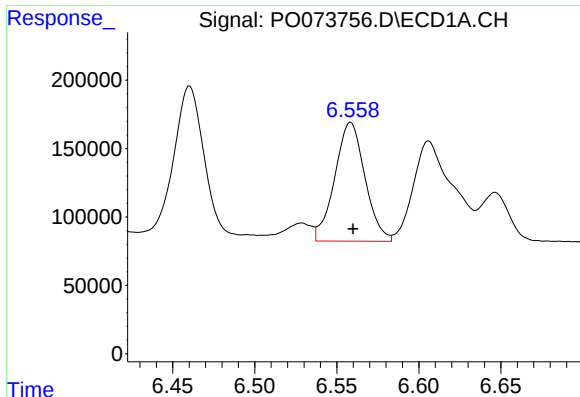

#15 AR-1232-5


R.T.: 6.558 min
Delta R.T.: -0.001 min
Response: 1112739
Conc: 1554.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
KENS-B6-121020-0-6MSD

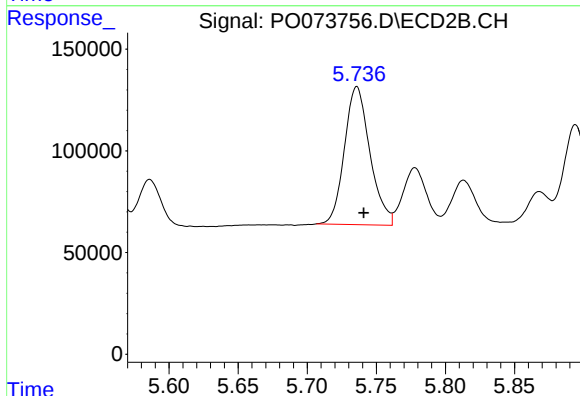


#15 AR-1232-5

R.T.: 5.736 min
Delta R.T.: -0.005 min
Response: 872211
Conc: 1305.08 ng/ml

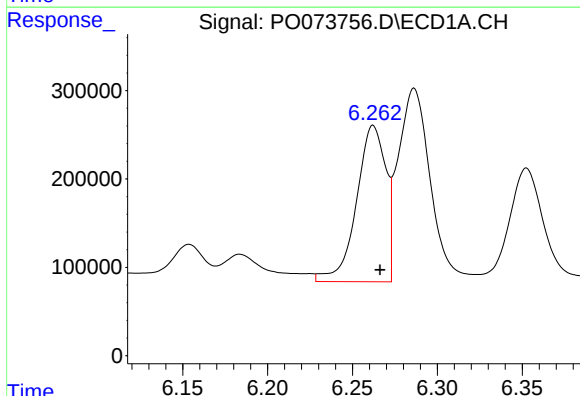


#16 AR-1242-1

R.T.: 6.262 min
Delta R.T.: -0.004 min
Response: 2132342
Conc: 752.35 ng/ml

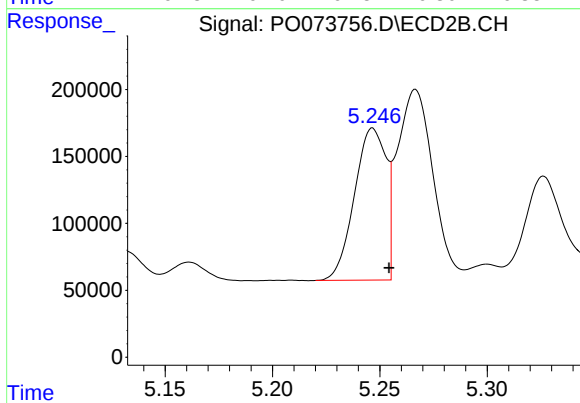

#16 AR-1242-1


R.T.: 5.247 min
Delta R.T.: -0.007 min
Response: 1163481
Conc: 661.51 ng/ml

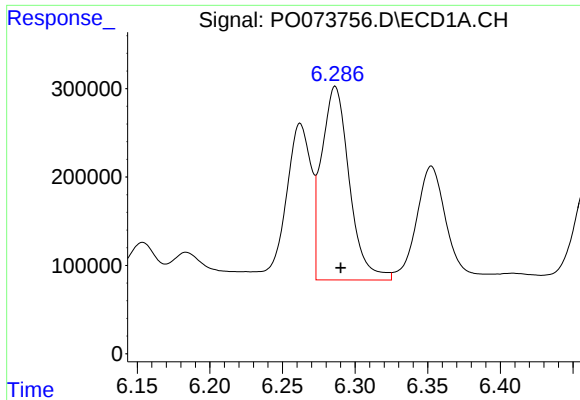

#17 AR-1242-2


R.T.: 6.286 min
Delta R.T.: -0.004 min
Response: 2911404
Conc: 747.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
KENS-B6-121020-0-6MSD

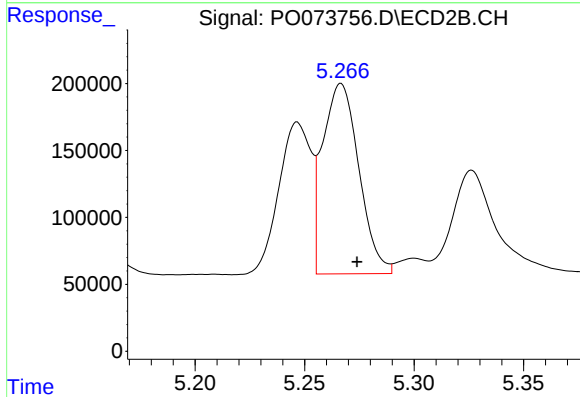


#17 AR-1242-2

R.T.: 5.267 min
Delta R.T.: -0.007 min
Response: 1637652
Conc: 669.60 ng/ml

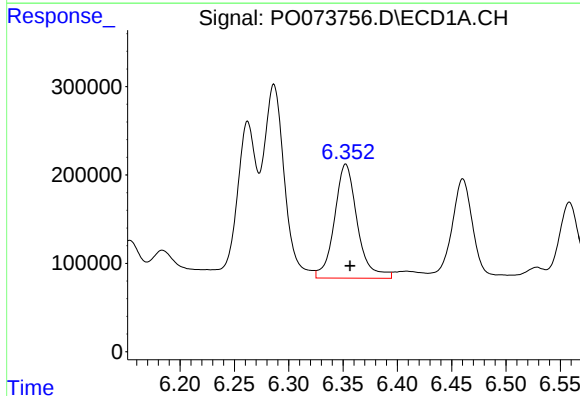


#18 AR-1242-3

R.T.: 6.353 min
Delta R.T.: -0.004 min
Response: 1886109
Conc: 795.14 ng/ml

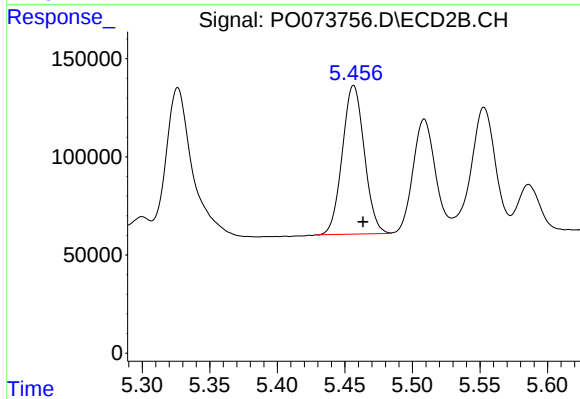

#18 AR-1242-3


R.T.: 5.457 min
Delta R.T.: -0.007 min
Response: 857991
Conc: 655.59 ng/ml

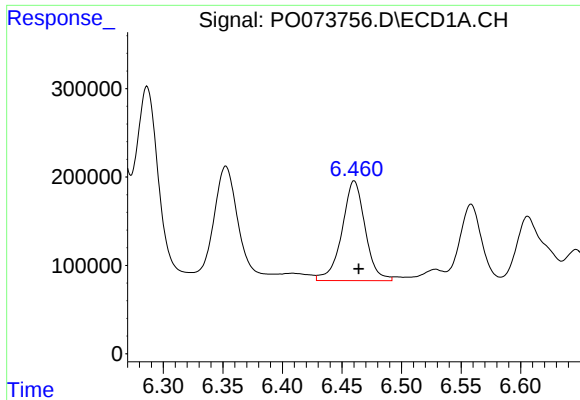

#19 AR-1242-4


R.T.: 6.460 min
Delta R.T.: -0.004 min
Response: 1529754
Conc: 776.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
KENS-B6-121020-0-6MSD

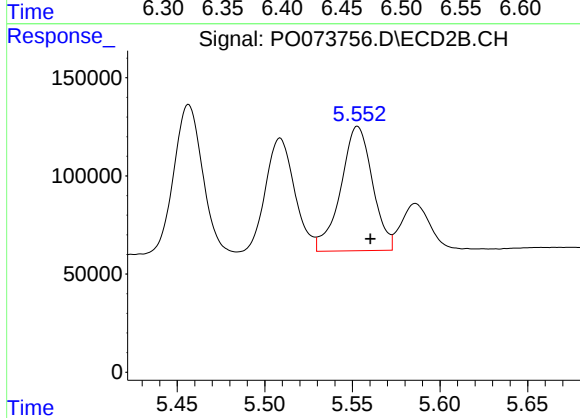


#19 AR-1242-4

R.T.: 5.553 min
Delta R.T.: -0.007 min
Response: 798288
Conc: 637.86 ng/ml

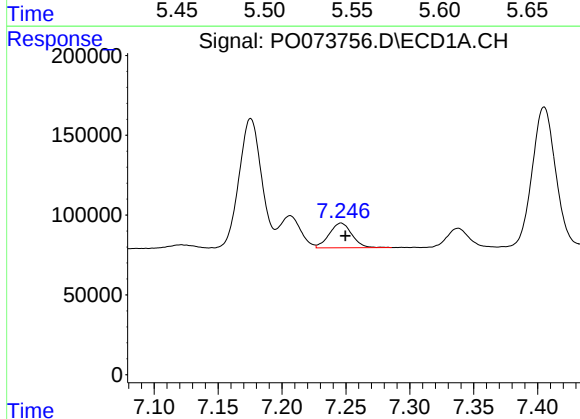


#20 AR-1242-5

R.T.: 7.246 min
Delta R.T.: -0.003 min
Response: 191260
Conc: 87.58 ng/ml

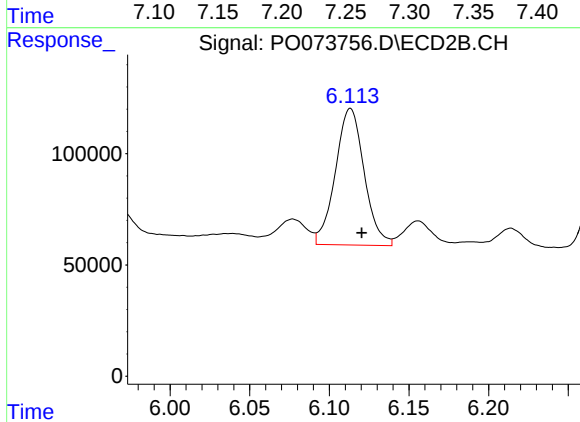

#20 AR-1242-5


R.T.: 6.113 min
Delta R.T.: -0.007 min
Response: 772482
Conc: 453.18 ng/ml

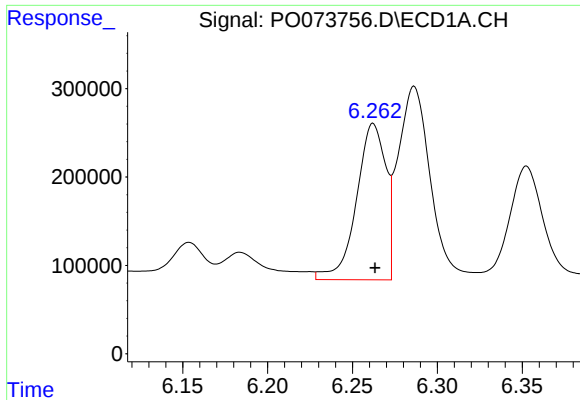

#21 AR-1248-1


R.T.: 6.262 min
Delta R.T.: -0.001 min
Response: 2132342
Conc: 981.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
KENS-B6-121020-0-6MSD

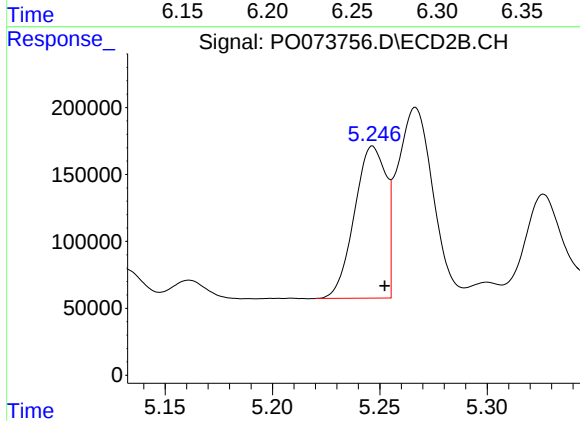


#21 AR-1248-1

R.T.: 5.247 min
Delta R.T.: -0.006 min
Response: 1163481
Conc: 849.77 ng/ml

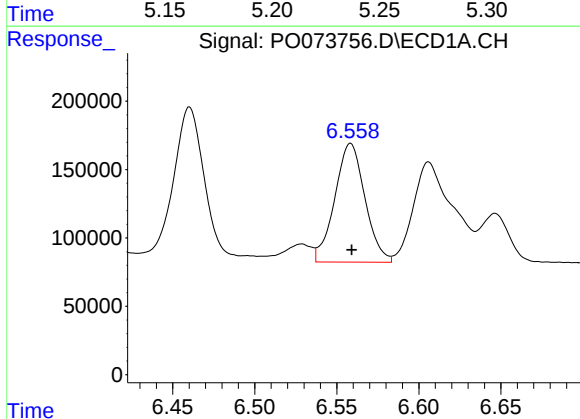


#22 AR-1248-2

R.T.: 6.558 min
Delta R.T.: 0.000 min
Response: 1112739
Conc: 398.18 ng/ml

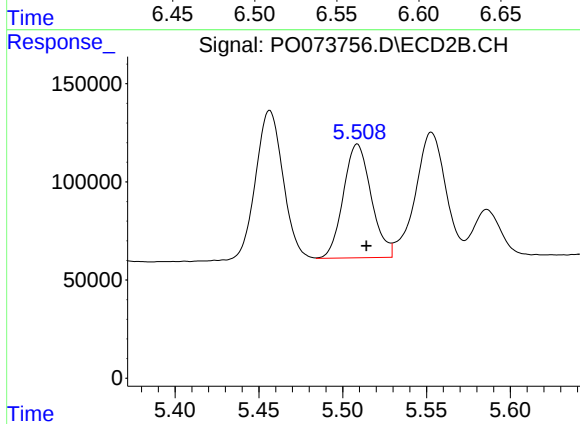

#22 AR-1248-2


R.T.: 5.509 min
Delta R.T.: -0.005 min
Response: 671853
Conc: 362.11 ng/ml

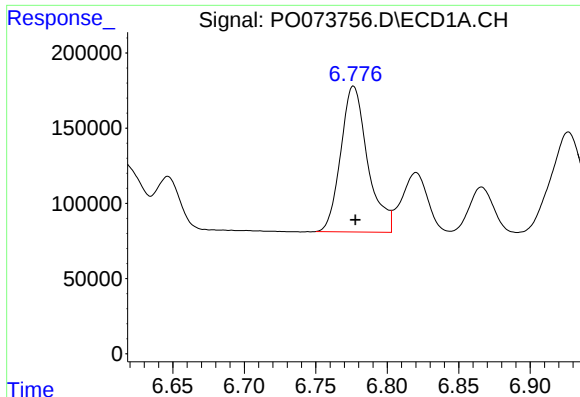

#23 AR-1248-3


R.T.: 6.776 min
Delta R.T.: -0.001 min
Response: 1271661
Conc: 388.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
KENS-B6-121020-0-6MSD

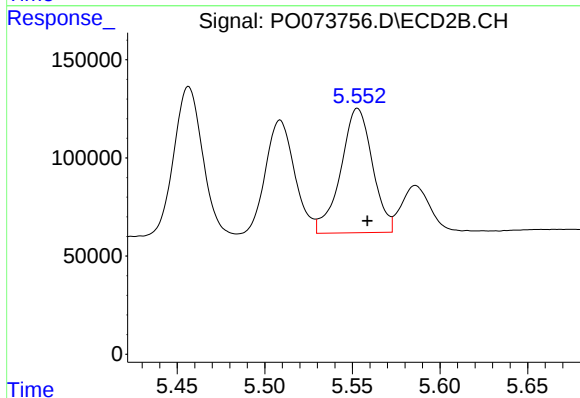


#23 AR-1248-3

R.T.: 5.553 min
Delta R.T.: -0.005 min
Response: 798288
Conc: 425.49 ng/ml

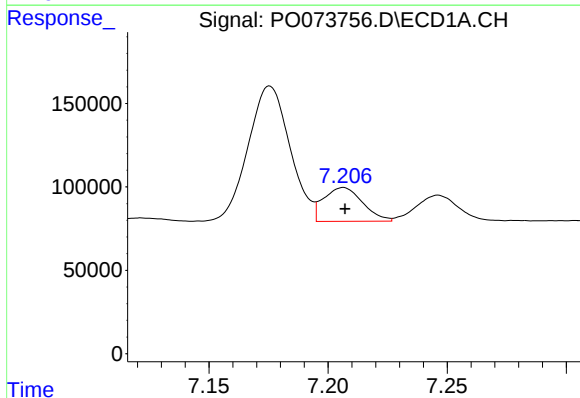


#24 AR-1248-4

R.T.: 7.206 min
Delta R.T.: 0.000 min
Response: 231093
Conc: 57.79 ng/ml

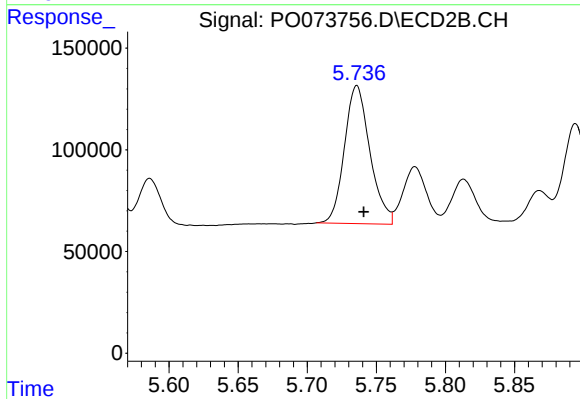

#24 AR-1248-4


R.T.: 5.736 min
Delta R.T.: -0.005 min
Response: 872211
Conc: 387.51 ng/ml

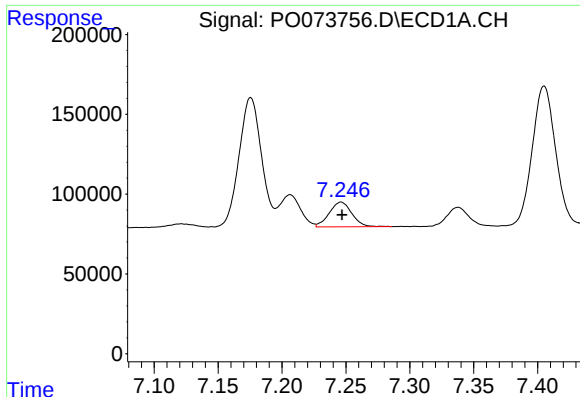

#25 AR-1248-5


R.T.: 7.246 min
Delta R.T.: 0.000 min
Response: 191260
Conc: 50.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
KENS-B6-121020-0-6MSD

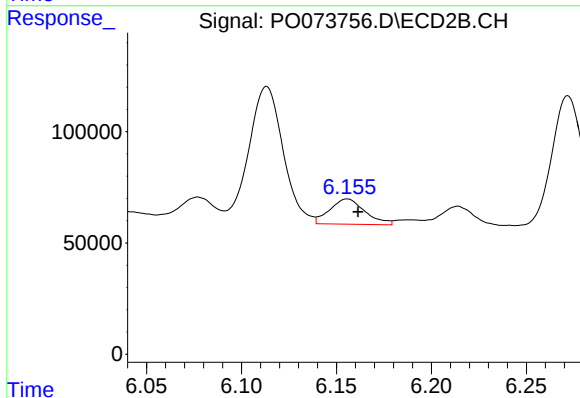


#25 AR-1248-5

R.T.: 6.156 min
Delta R.T.: -0.006 min
Response: 147075
Conc: 63.30 ng/ml

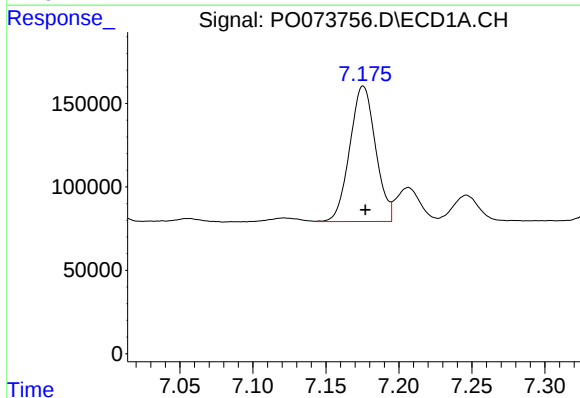


#26 AR-1254-1

R.T.: 7.176 min
Delta R.T.: -0.001 min
Response: 997198
Conc: 262.71 ng/ml

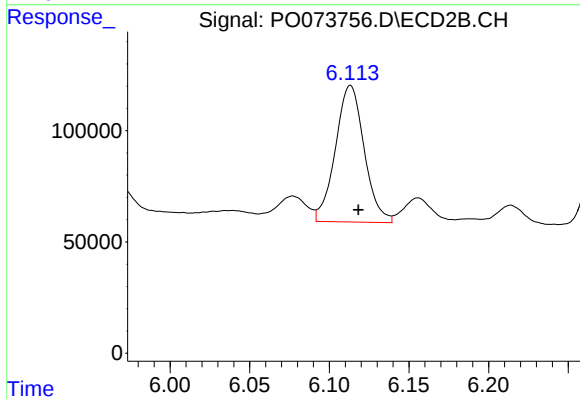

#26 AR-1254-1


R.T.: 6.113 min
Delta R.T.: -0.005 min
Response: 772482
Conc: 218.58 ng/ml

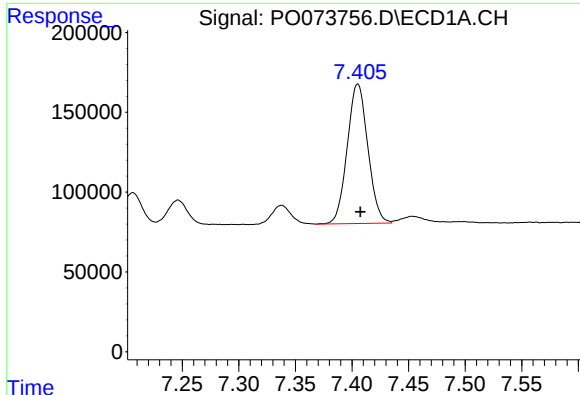

#27 AR-1254-2


R.T.: 7.405 min
Delta R.T.: -0.002 min
Response: 1106865
Conc: 187.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
KENS-B6-121020-0-6MSD

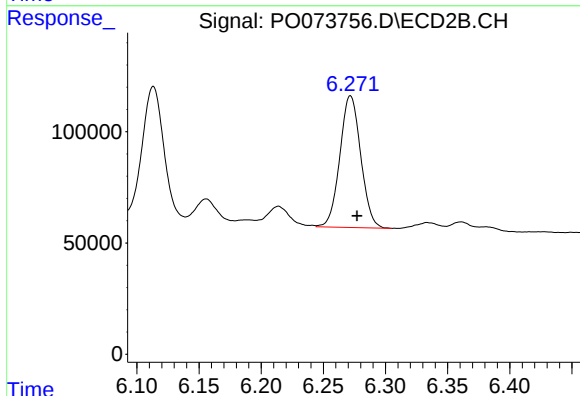


#27 AR-1254-2

R.T.: 6.272 min
Delta R.T.: -0.005 min
Response: 692164
Conc: 221.70 ng/ml

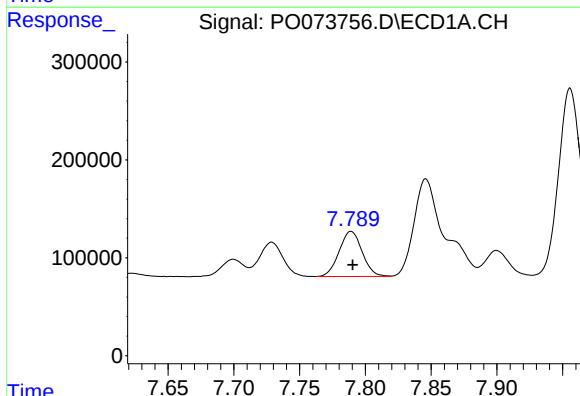


#28 AR-1254-3

R.T.: 7.789 min
Delta R.T.: -0.001 min
Response: 561811
Conc: 91.69 ng/ml

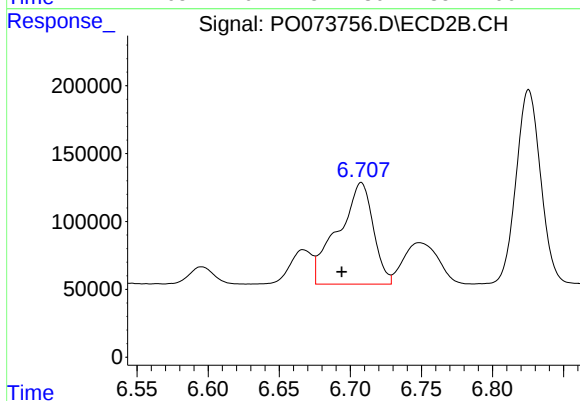

#28 AR-1254-3


R.T.: 6.708 min
Delta R.T.: 0.014 min
Response: 1284935
Conc: 262.45 ng/ml

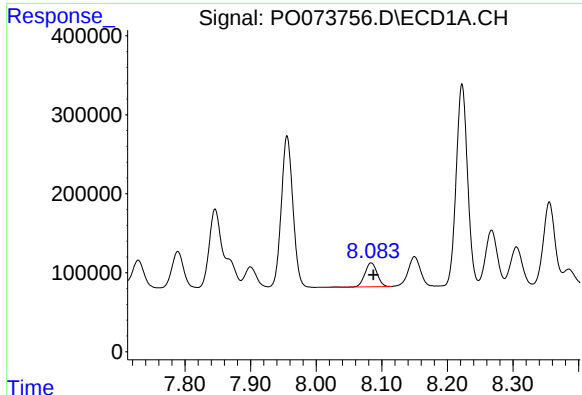

#29 AR-1254-4


R.T.: 8.084 min
Delta R.T.: -0.004 min
Response: 391991
Conc: 74.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
KENS-B6-121020-0-6MSD

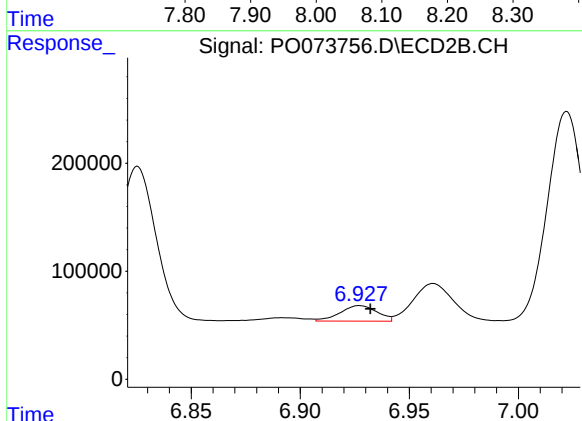


#29 AR-1254-4

R.T.: 6.927 min
Delta R.T.: -0.005 min
Response: 169242
Conc: 48.26 ng/ml

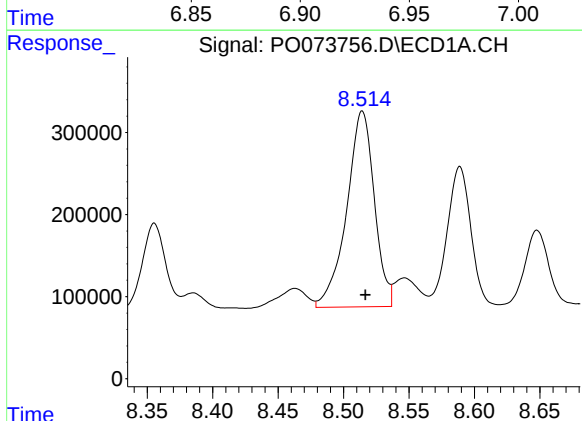


#30 AR-1254-5

R.T.: 8.514 min
Delta R.T.: -0.002 min
Response: 3511108
Conc: 681.70 ng/ml

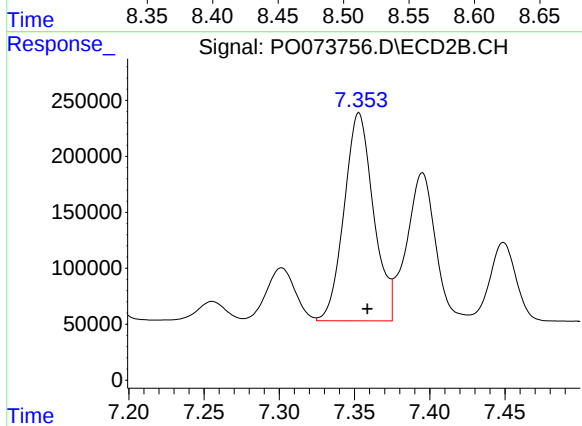

#30 AR-1254-5


R.T.: 7.353 min
Delta R.T.: -0.006 min
Response: 2524204
Conc: 572.43 ng/ml

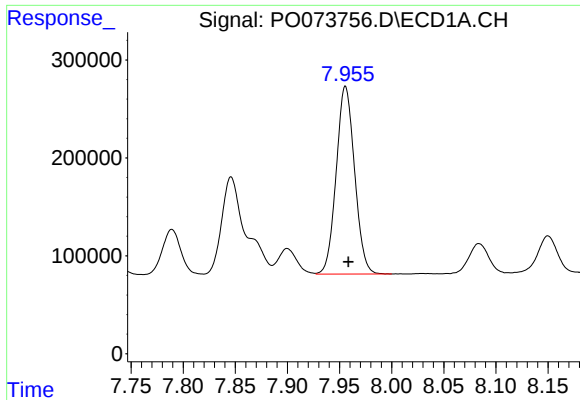

#31 AR-1260-1


R.T.: 7.956 min
Delta R.T.: -0.003 min
Response: 2356724
Conc: 557.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
KENS-B6-121020-0-6MSD

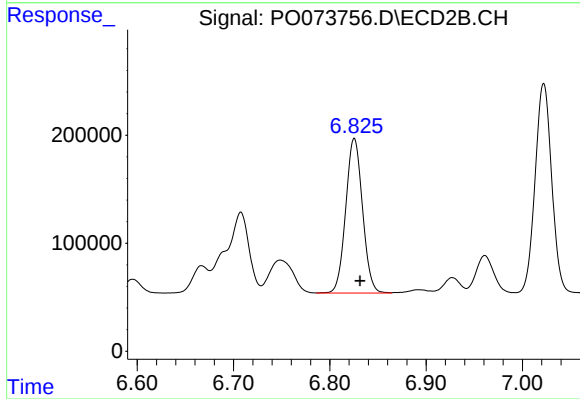


#31 AR-1260-1

R.T.: 6.825 min
Delta R.T.: -0.006 min
Response: 1727945
Conc: 558.97 ng/ml

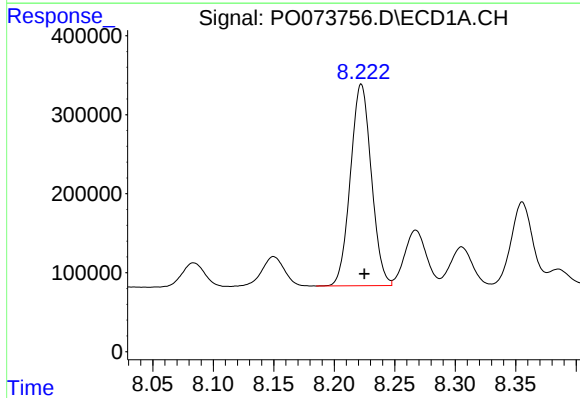


#32 AR-1260-2

R.T.: 8.222 min
Delta R.T.: -0.002 min
Response: 3068966
Conc: 546.29 ng/ml

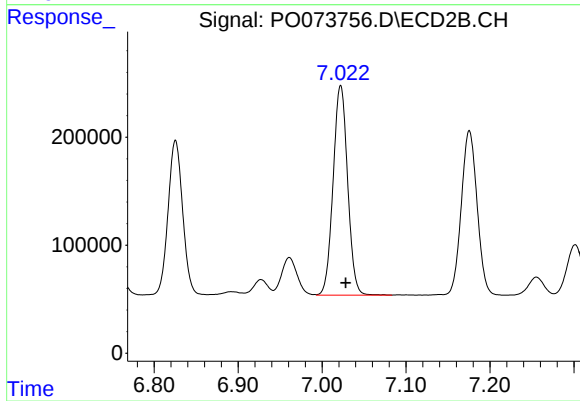

#32 AR-1260-2


R.T.: 7.022 min
Delta R.T.: -0.006 min
Response: 2328524
Conc: 574.02 ng/ml

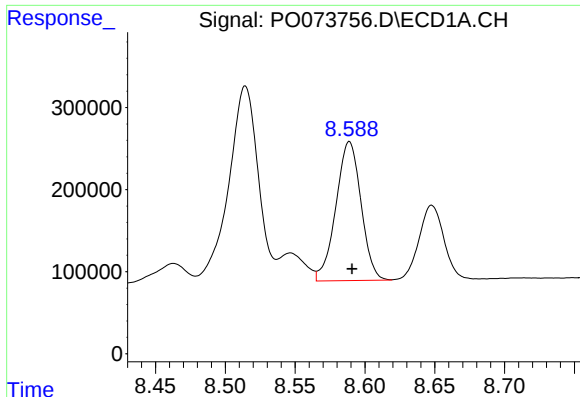

#33 AR-1260-3


R.T.: 8.589 min
Delta R.T.: -0.002 min
Response: 2122688
Conc: 464.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
KENS-B6-121020-0-6MSD

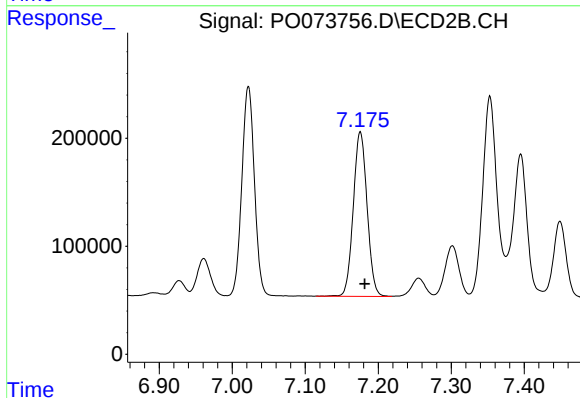


#33 AR-1260-3

R.T.: 7.175 min
Delta R.T.: -0.006 min
Response: 1999782
Conc: 572.95 ng/ml

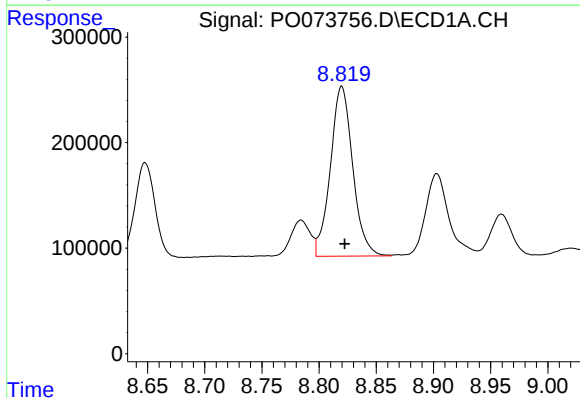


#34 AR-1260-4

R.T.: 8.820 min
Delta R.T.: -0.003 min
Response: 2189548
Conc: 462.47 ng/ml

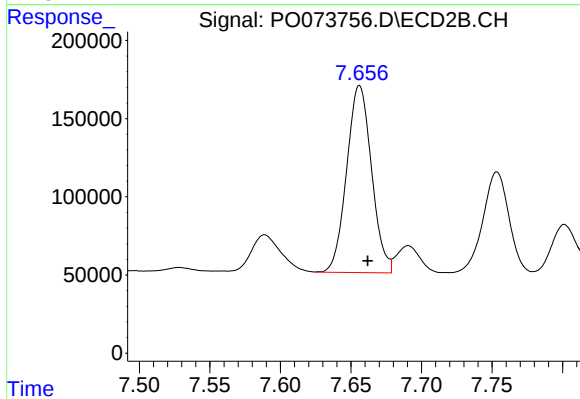

#34 AR-1260-4


R.T.: 7.656 min
Delta R.T.: -0.006 min
Response: 1468418
Conc: 486.27 ng/ml

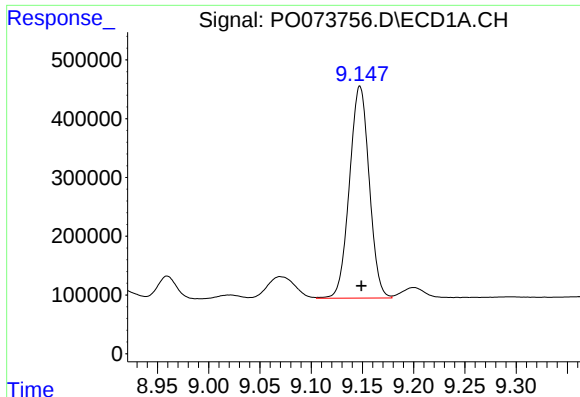

#35 AR-1260-5


R.T.: 9.148 min
Delta R.T.: -0.002 min
Response: 4834270
Conc: 484.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
KENS-B6-121020-0-6MSD

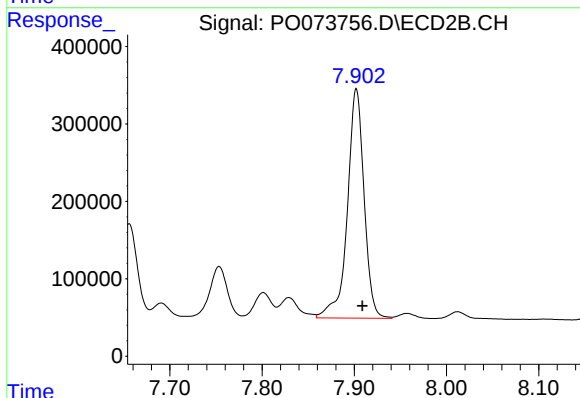


#35 AR-1260-5

R.T.: 7.902 min
Delta R.T.: -0.007 min
Response: 3729201
Conc: 499.22 ng/ml

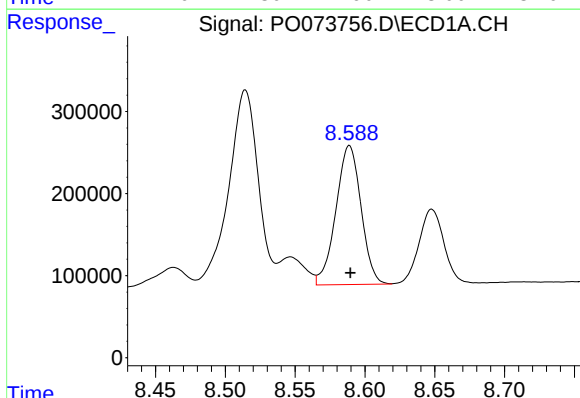


#36 AR-1262-1

R.T.: 8.589 min
Delta R.T.: 0.000 min
Response: 2122688
Conc: 283.55 ng/ml

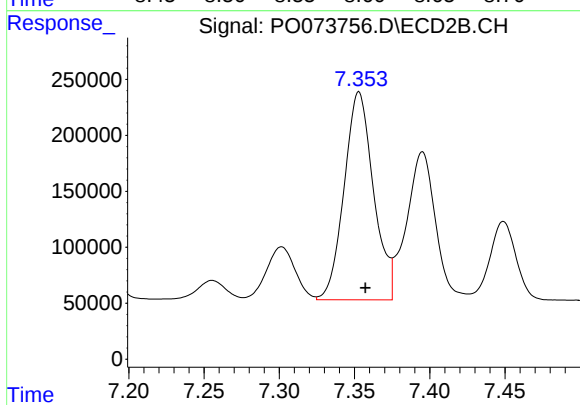

#36 AR-1262-1


R.T.: 7.353 min
Delta R.T.: -0.004 min
Response: 2524204
Conc: 1009.76 ng/ml

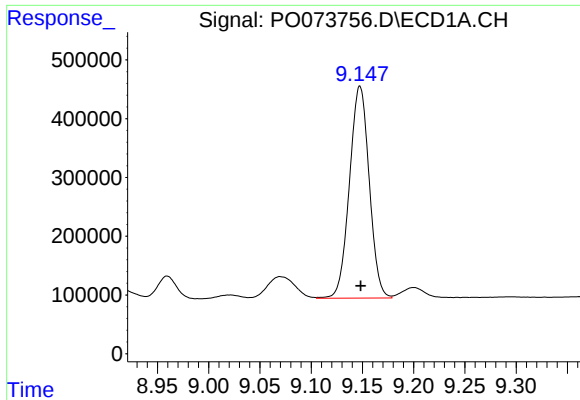

#37 AR-1262-2


R.T.: 9.148 min
Delta R.T.: 0.000 min
Response: 4834270
Conc: 376.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
KENS-B6-121020-0-6MSD

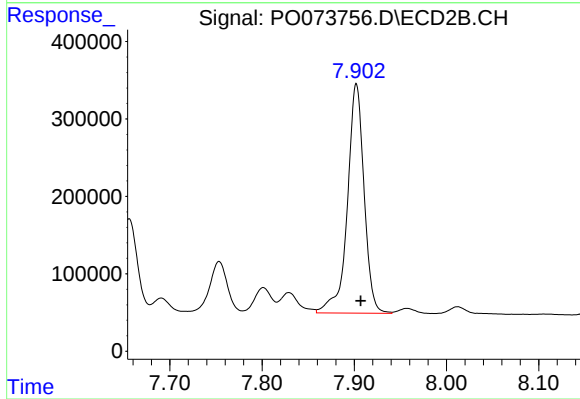


#37 AR-1262-2

R.T.: 7.902 min
Delta R.T.: -0.005 min
Response: 3729201
Conc: 423.95 ng/ml

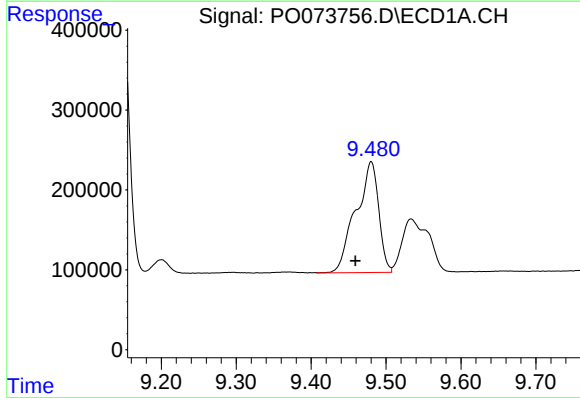


#38 AR-1262-3

R.T.: 9.480 min
Delta R.T.: 0.021 min
Response: 2934745
Conc: 345.92 ng/ml

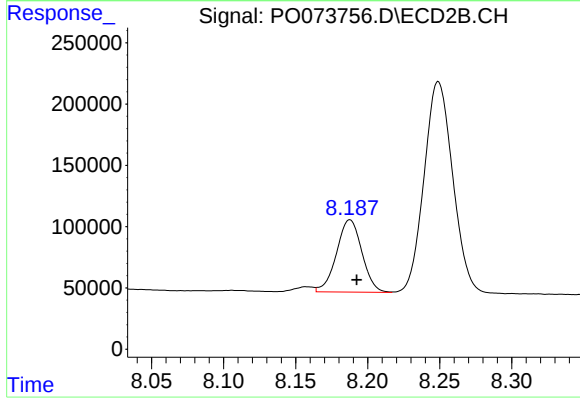

#38 AR-1262-3


R.T.: 8.188 min
Delta R.T.: -0.005 min
Response: 725206
Conc: 200.56 ng/ml

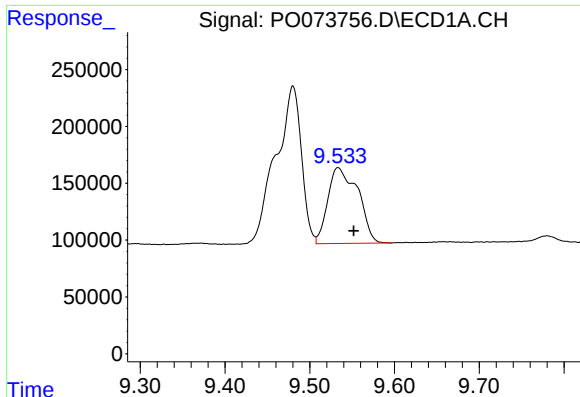

#39 AR-1262-4


R.T.: 9.533 min
Delta R.T.: -0.019 min
Response: 1648826
Conc: 492.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
KENS-B6-121020-0-6MSD

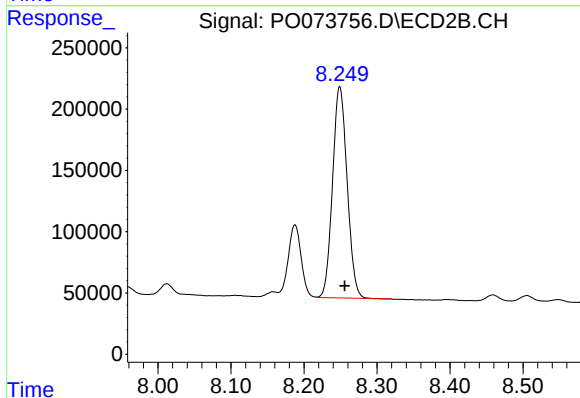


#39 AR-1262-4

R.T.: 8.249 min
Delta R.T.: -0.007 min
Response: 2389907
Conc: 388.41 ng/ml

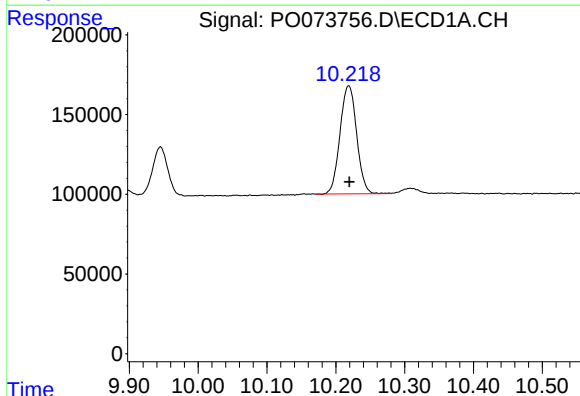


#40 AR-1262-5

R.T.: 10.219 min
Delta R.T.: -0.001 min
Response: 1142311
Conc: 252.72 ng/ml

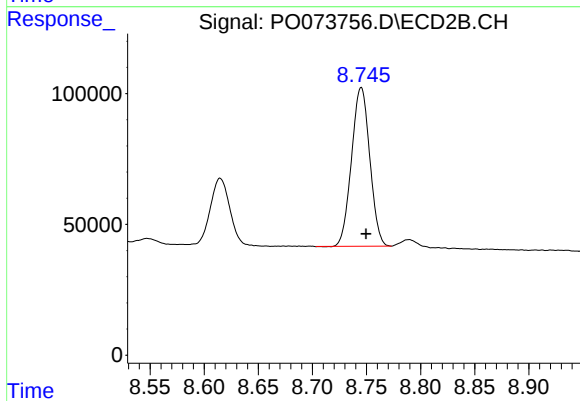

#40 AR-1262-5


R.T.: 8.745 min
Delta R.T.: -0.005 min
Response: 712270
Conc: 250.19 ng/ml

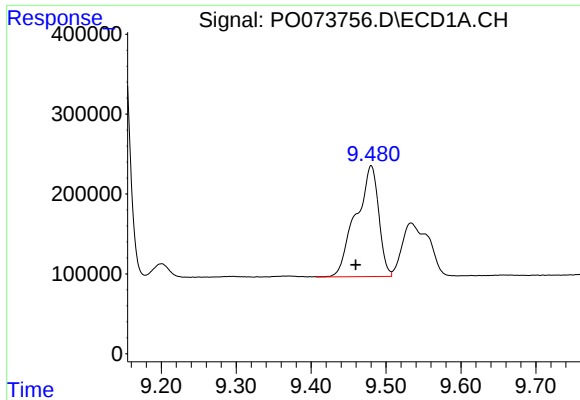

#41 AR-1268-1


R.T.: 9.480 min
Delta R.T.: 0.021 min
Response: 2934745
Conc: 206.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
KENS-B6-121020-0-6MSD

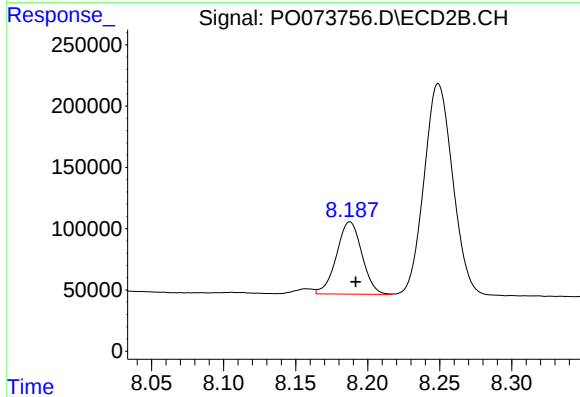


#41 AR-1268-1

R.T.: 8.188 min
Delta R.T.: -0.004 min
Response: 725206
Conc: 75.36 ng/ml

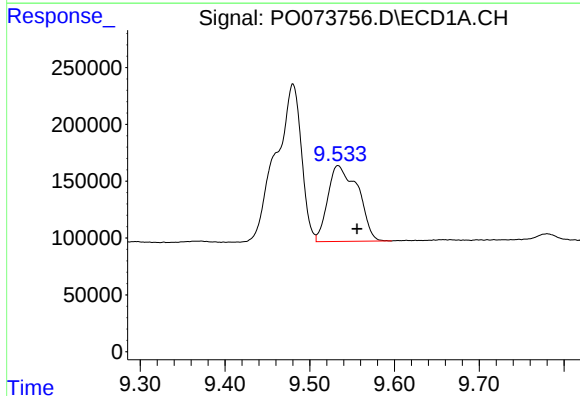


#42 AR-1268-2

R.T.: 9.533 min
Delta R.T.: -0.022 min
Response: 1648826
Conc: 133.76 ng/ml

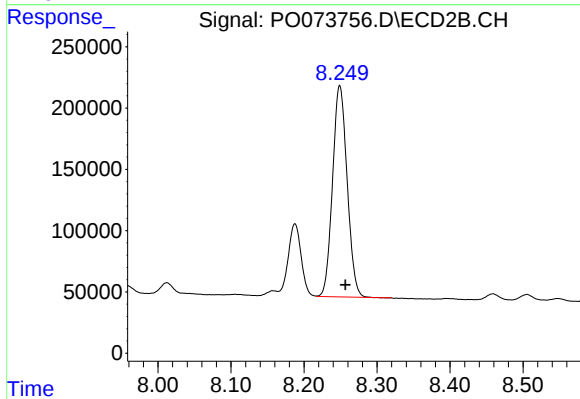

#42 AR-1268-2


R.T.: 8.249 min
Delta R.T.: -0.008 min
Response: 2389907
Conc: 290.09 ng/ml

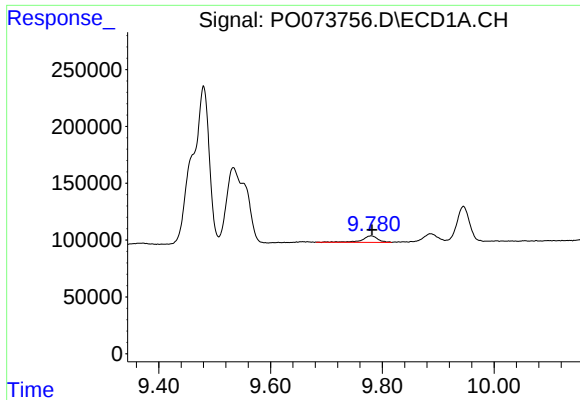

#43 AR-1268-3


R.T.: 9.780 min
Delta R.T.: -0.001 min
Response: 113932
Conc: 10.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
KENS-B6-121020-0-6MSD

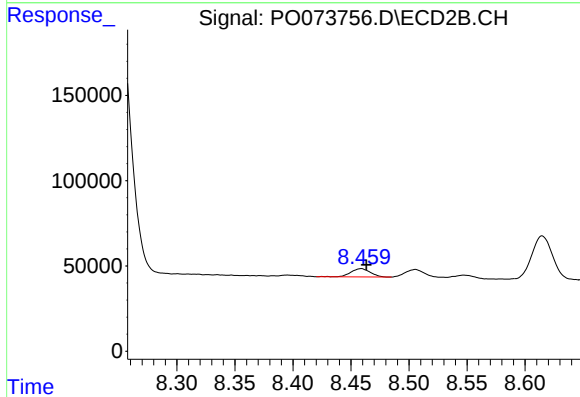


#43 AR-1268-3

R.T.: 8.459 min
Delta R.T.: -0.005 min
Response: 55954
Conc: 7.92 ng/ml

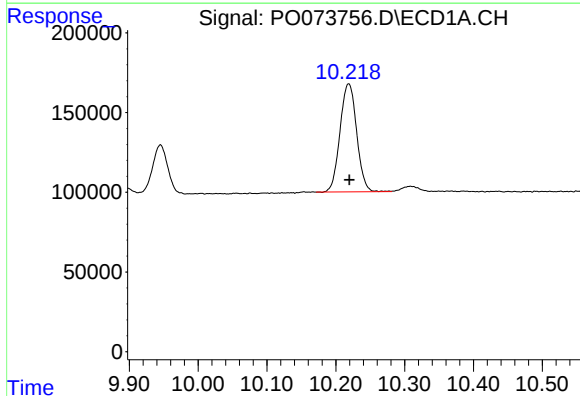


#44 AR-1268-4

R.T.: 10.219 min
Delta R.T.: 0.000 min
Response: 1142311
Conc: 243.85 ng/ml

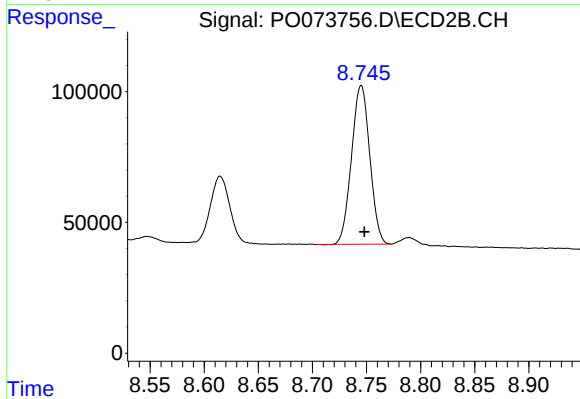

#44 AR-1268-4


R.T.: 8.745 min
Delta R.T.: -0.003 min
Response: 712270
Conc: 240.63 ng/ml

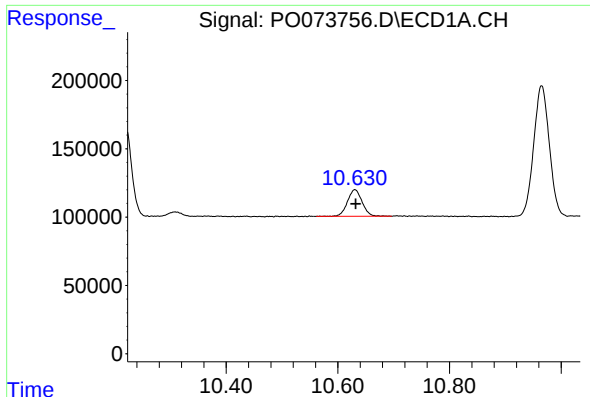

#45 AR-1268-5

R.T.: 10.631 min
Delta R.T.: -0.001 min
Response: 357643
Conc: 10.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
KENS-B6-121020-0-6MSD

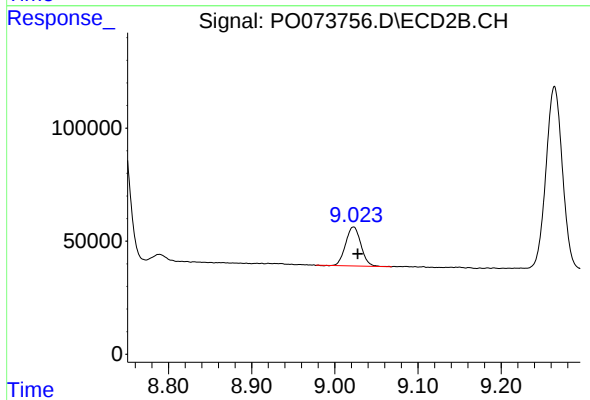

#45 AR-1268-5

R.T.: 9.023 min
Delta R.T.: -0.005 min
Response: 221717
Conc: 11.04 ng/ml