

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121420\
 Data File : PO073807.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Dec 2020 6:36
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 07:06:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 11 03:58:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.936	3.995	2089938	1268875	22.859	23.657
2)	SA Decachlor...	10.960	9.260	1962187	1157928	23.744	24.747
Target Compounds							
9)	L2 AR-1221-2	5.290	0.000	32190	0	40.980	N.D. #
24)	L5 AR-1248-4	7.179f	0.000	78280	0	19.574	N.D. #
26)	L6 AR-1254-1	7.179	0.000	78280	0	20.623	N.D. #
28)	L6 AR-1254-3	7.804	0.000	15357	0	2.506	N.D. #
29)	L6 AR-1254-4	8.080	0.000	18650	0	3.555	N.D. #
33)	L7 AR-1260-3	8.600	0.000	7069	0	1.546	N.D. #
34)	L7 AR-1260-4	8.812	0.000	7037	0	1.486	N.D. #
36)	L8 AR-1262-1	8.600	0.000	7069	0	0.944	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121420\
Data File : PO073807.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Dec 2020 6:36
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 07:06:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 11 03:58:06 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

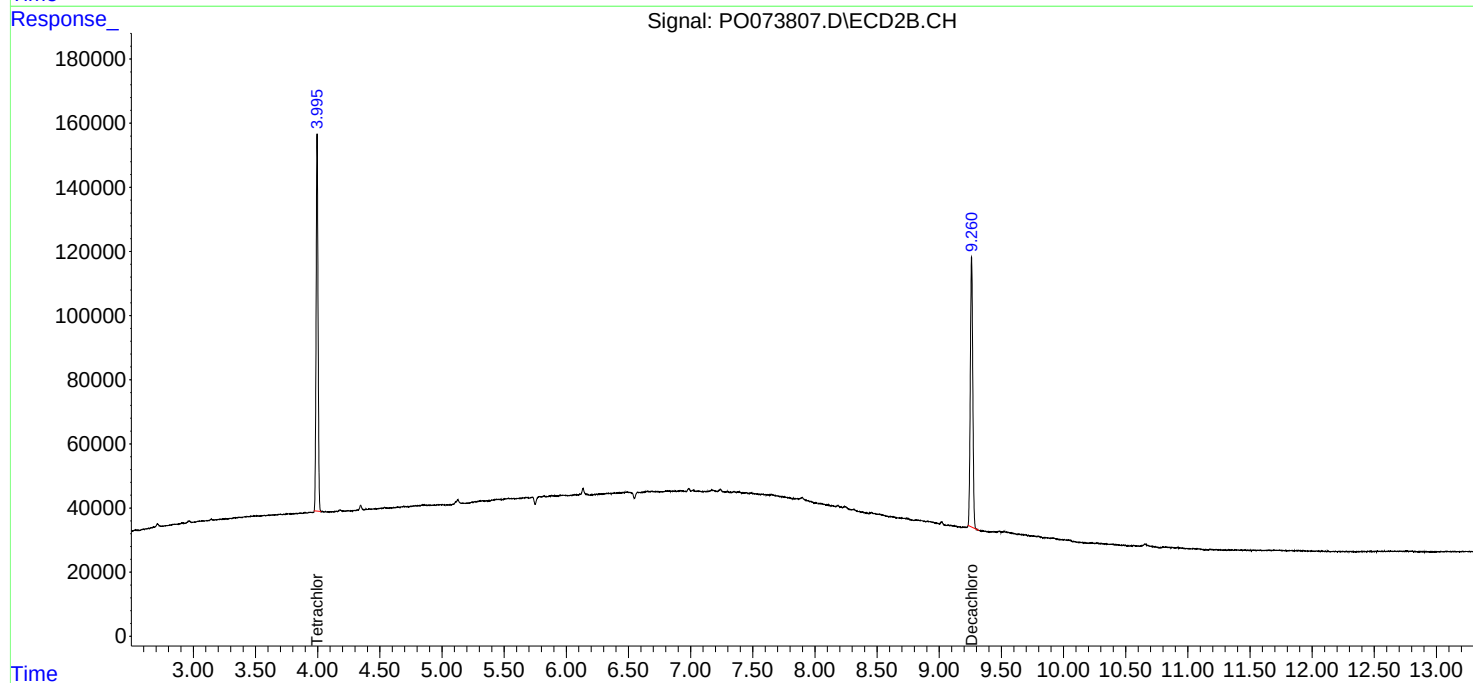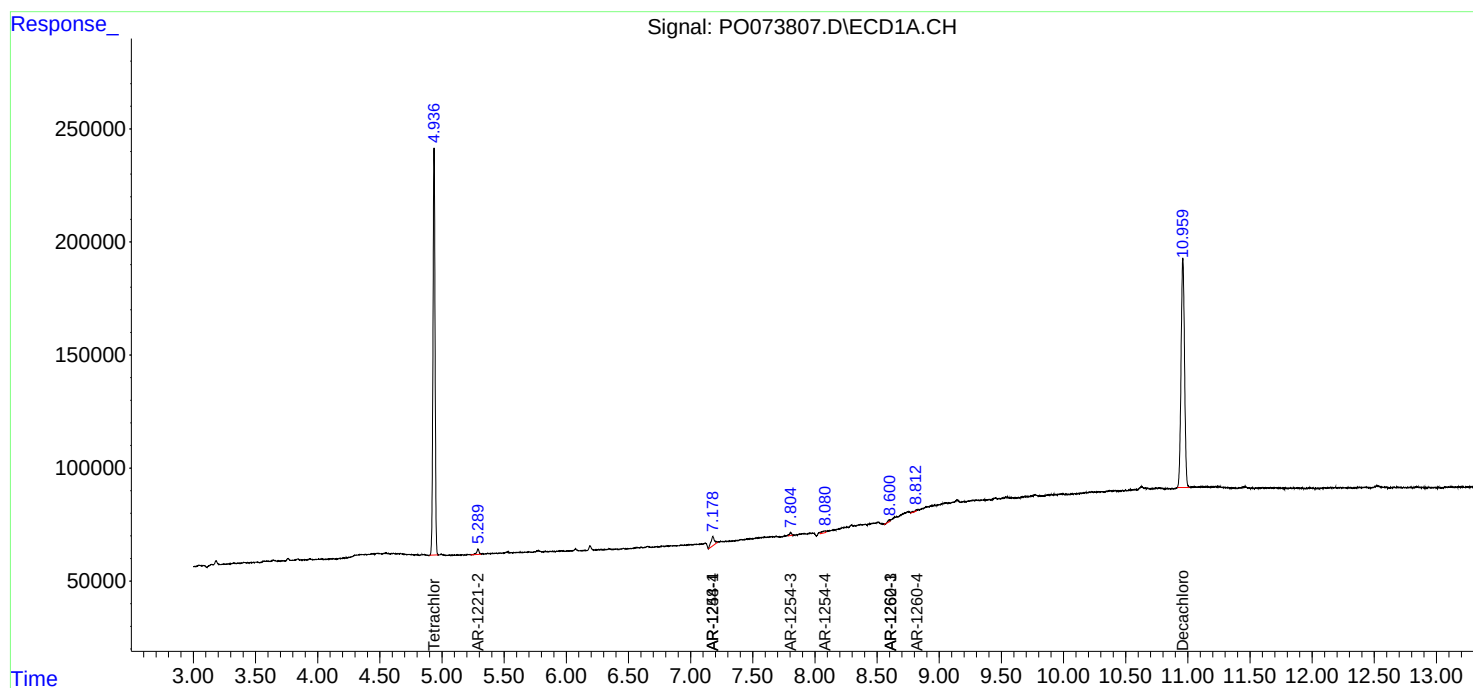


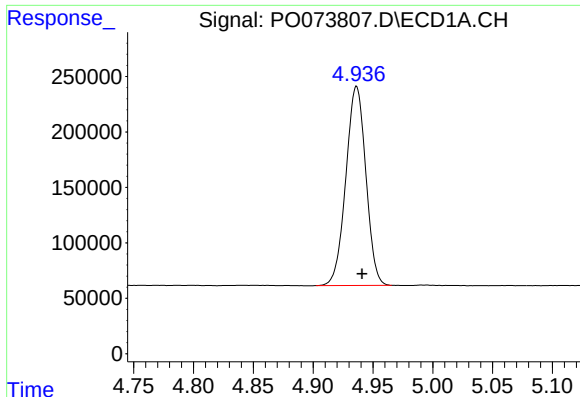

#1 Tetrachloro-m-xylene


R.T.: 4.936 min
Delta R.T.: -0.005 min
Response: 2089938
Conc: 22.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

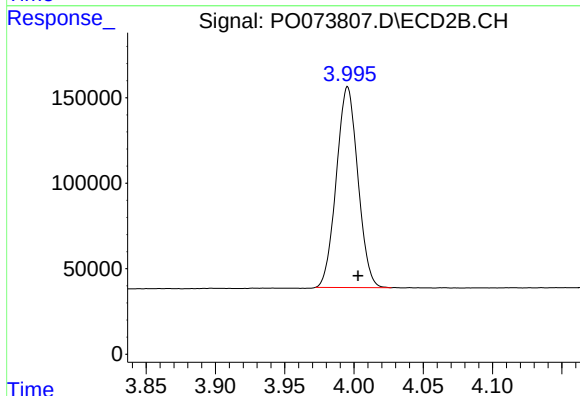


#1 Tetrachloro-m-xylene

R.T.: 3.995 min
Delta R.T.: -0.008 min
Response: 1268875
Conc: 23.66 ng/ml

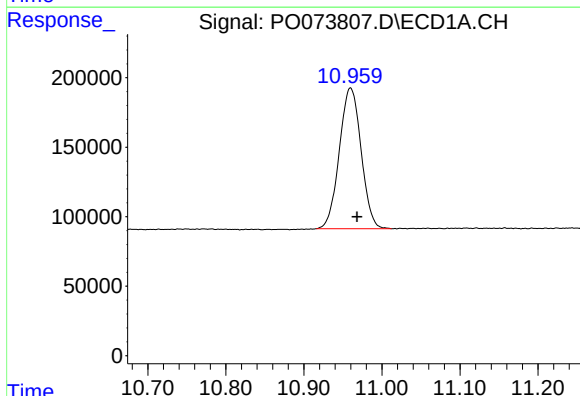


#2 Decachlorobiphenyl

R.T.: 10.960 min
Delta R.T.: -0.008 min
Response: 1962187
Conc: 23.74 ng/ml

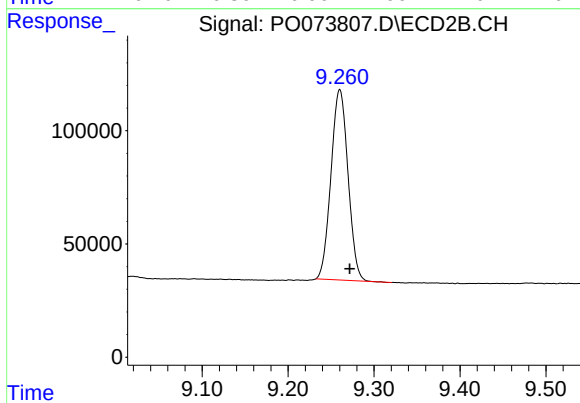

#2 Decachlorobiphenyl


R.T.: 9.260 min
Delta R.T.: -0.011 min
Response: 1157928
Conc: 24.75 ng/ml

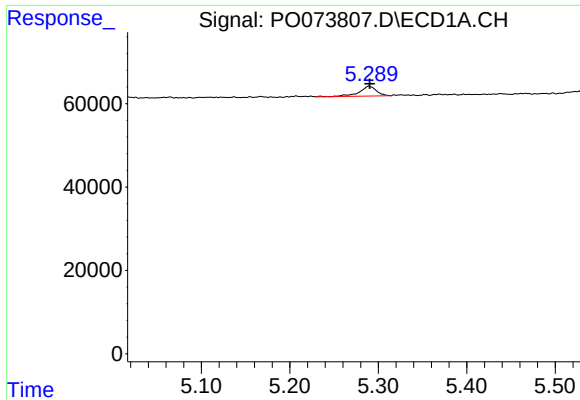

#9 AR-1221-2


R.T.: 5.290 min
Delta R.T.: 0.000 min
Response: 32190
Conc: 40.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

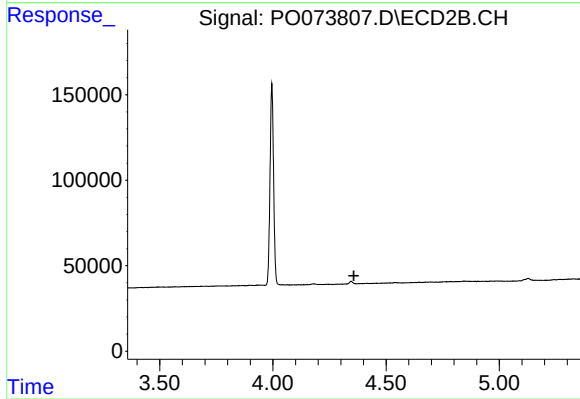


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.357 min
Response: 0
Conc: N.D.

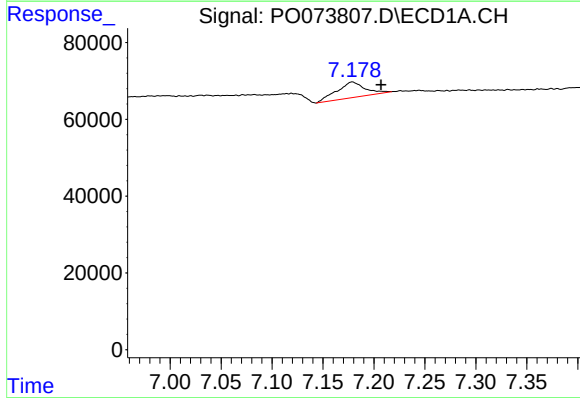


#24 AR-1248-4

R.T.: 7.179 min
Delta R.T.: -0.028 min
Response: 78280
Conc: 19.57 ng/ml

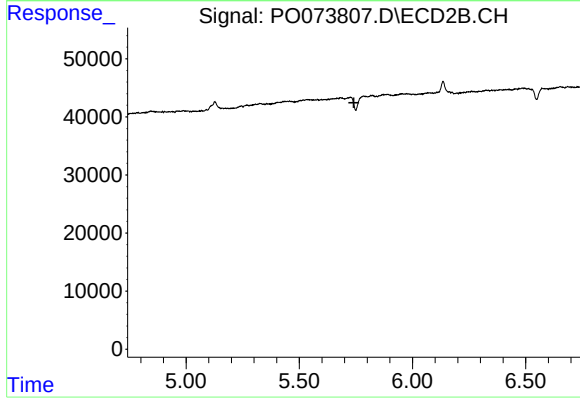

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.741 min
Response: 0
Conc: N.D.

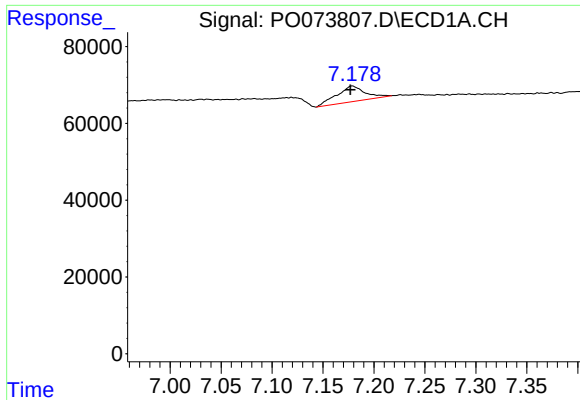

#26 AR-1254-1


R.T.: 7.179 min
Delta R.T.: 0.002 min
Response: 78280
Conc: 20.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

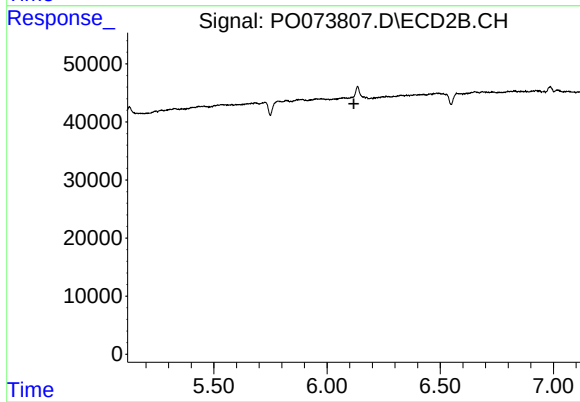


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 6.118 min
Response: 0
Conc: N.D.

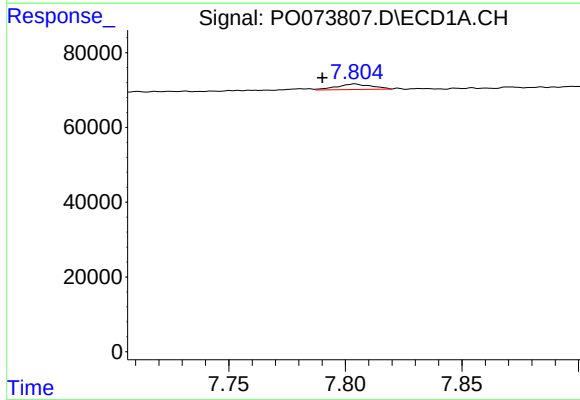


#28 AR-1254-3

R.T.: 7.804 min
Delta R.T.: 0.014 min
Response: 15357
Conc: 2.51 ng/ml

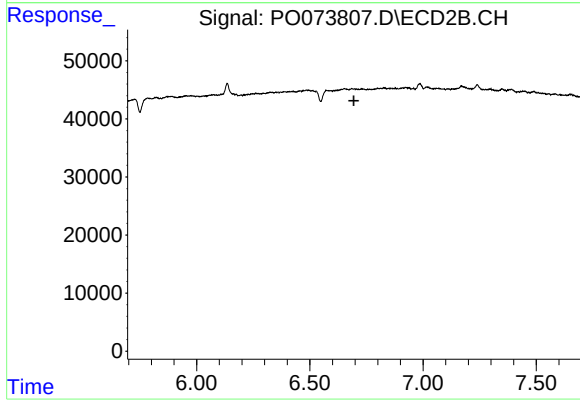

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.694 min
Response: 0
Conc: N.D.

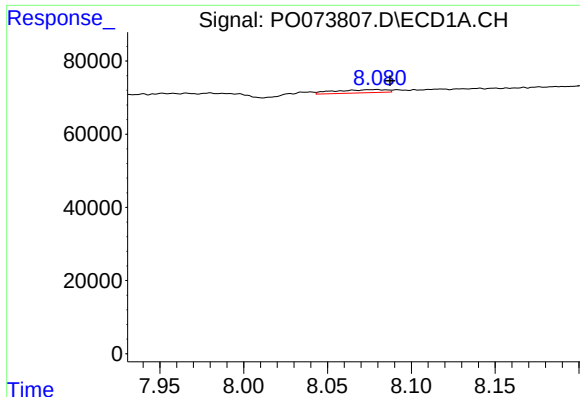

#29 AR-1254-4


R.T.: 8.080 min
Delta R.T.: -0.008 min
Response: 18650
Conc: 3.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

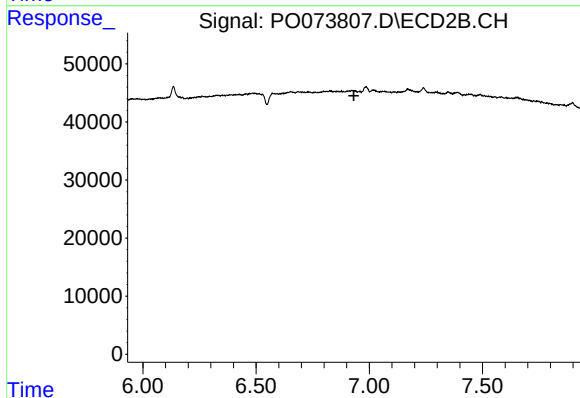


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.932 min
Response: 0
Conc: N.D.

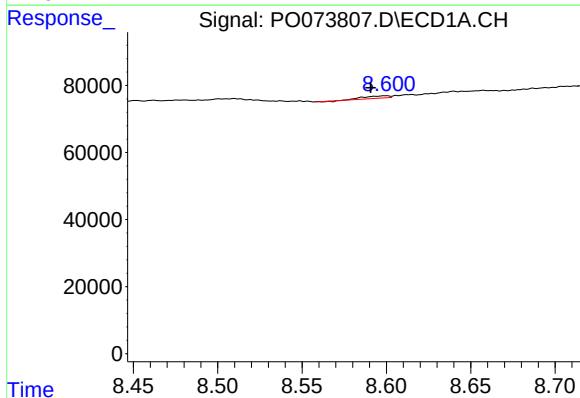


#33 AR-1260-3

R.T.: 8.600 min
Delta R.T.: 0.009 min
Response: 7069
Conc: 1.55 ng/ml

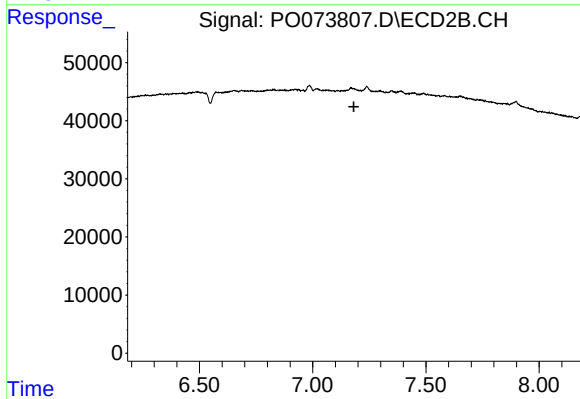

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T. : 7.182 min
Response: 0
Conc: N.D.

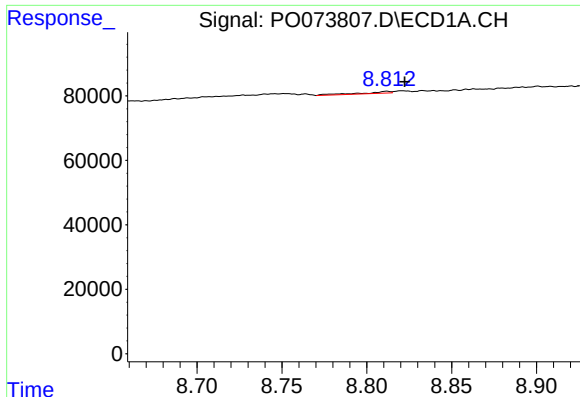

#34 AR-1260-4


R.T.: 8.812 min
Delta R.T.: -0.010 min
Response: 7037
Conc: 1.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

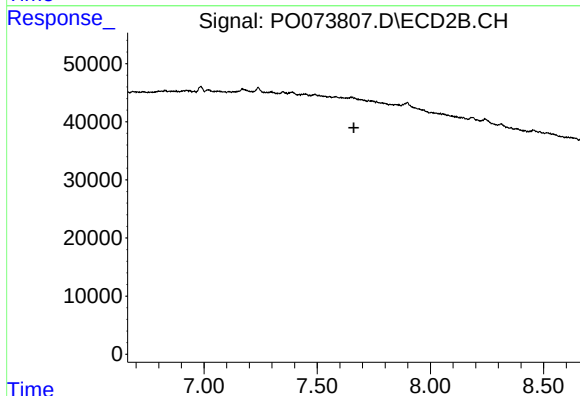


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.662 min
Response: 0
Conc: N.D.

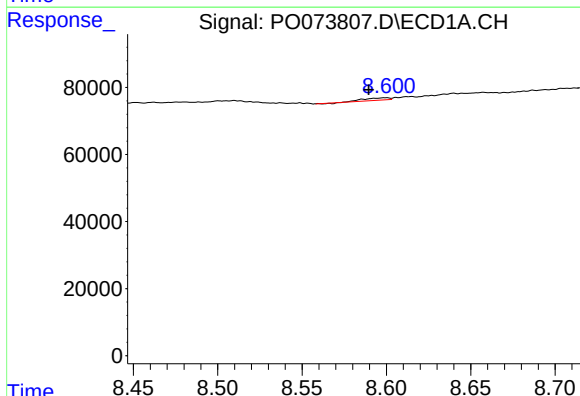

#36 AR-1262-1

R.T.: 8.600 min
Delta R.T.: 0.010 min
Response: 7069
Conc: 0.94 ng/ml

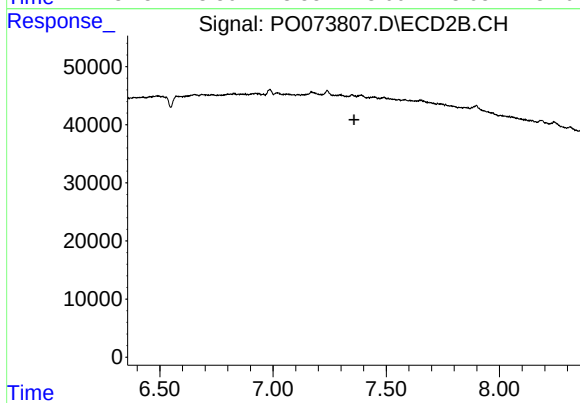

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.357 min
Response: 0
Conc: N.D.