

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\PO121420\  
 Data File : PO073757.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 14 Dec 2020 12:15  
 Operator : DD\AJ  
 Sample : L5042-08  
 Misc :  
 ALS Vial : 13 Sample Multiplier: 1

Instrument :  
 ECD\_O  
 ClientSampleId :  
 KENS-B6-121020-13-15

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Dec 15 03:27:01 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\PO121020.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri Dec 11 03:58:06 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1   | RT#2  | Resp#1  | Resp#2  | ng/ml  | ng/ml  |
|-----------------------------|--------|-------|---------|---------|--------|--------|
| -----                       |        |       |         |         |        |        |
| System Monitoring Compounds |        |       |         |         |        |        |
| 1) SA Tetrachlo...          | 4.939  | 3.998 | 2181381 | 1308583 | 23.859 | 24.397 |
| 2) SA Decachlor...          | 10.965 | 9.264 | 1926429 | 1152608 | 23.311 | 24.633 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\PO121420\  
Data File : PO073757.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 14 Dec 2020 12:15  
Operator : DD\AJ  
Sample : L5042-08  
Misc :  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
ECD\_O  
ClientSampleId :  
KENS-B6-121020-13-15

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Dec 15 03:27:01 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\PO121020.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Fri Dec 11 03:58:06 2020  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

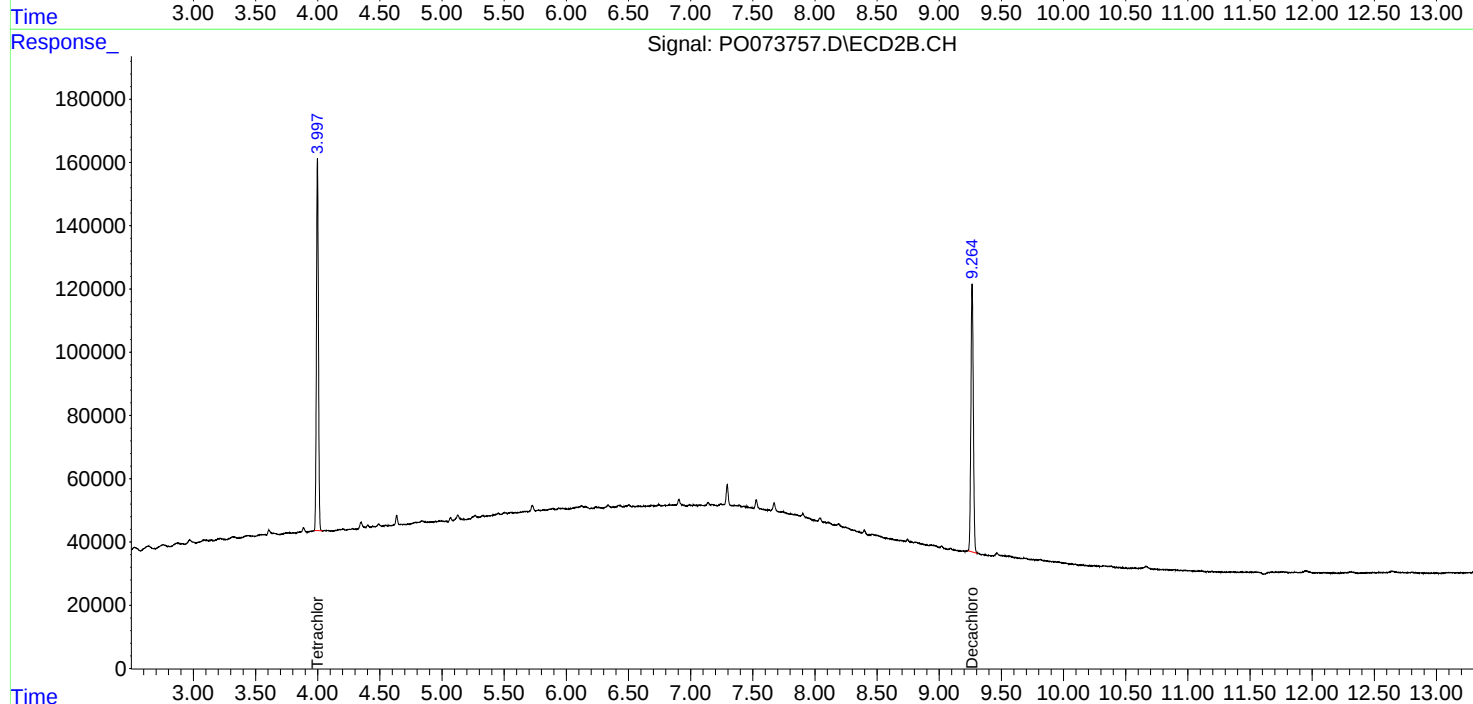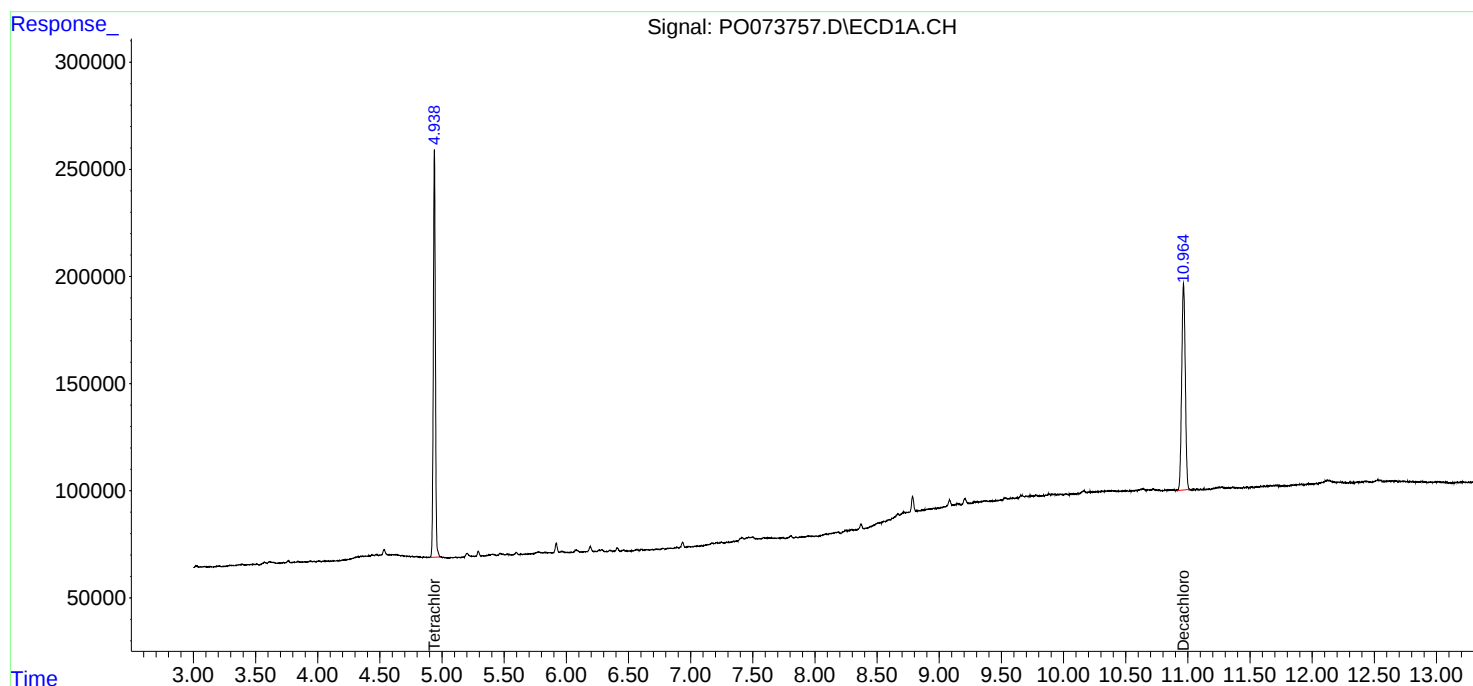


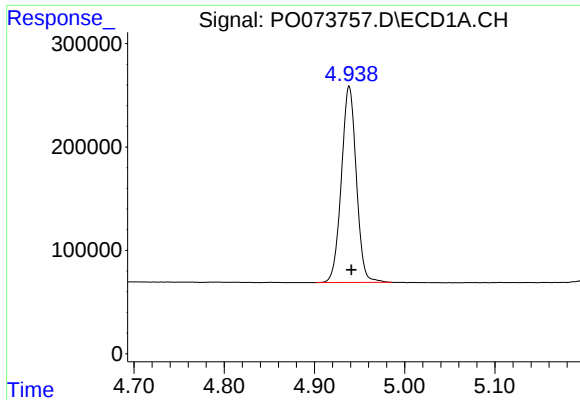

#1 Tetrachloro-m-xylene


R.T.: 4.939 min  
Delta R.T.: -0.002 min  
Response: 2181381  
Conc: 23.86 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
KENS-B6-121020-13-15

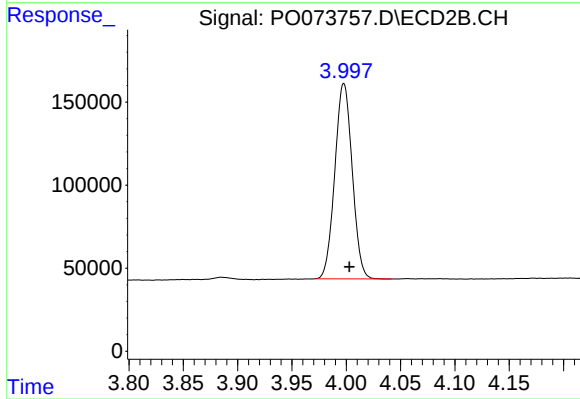


#1 Tetrachloro-m-xylene

R.T.: 3.998 min  
Delta R.T.: -0.005 min  
Response: 1308583  
Conc: 24.40 ng/ml

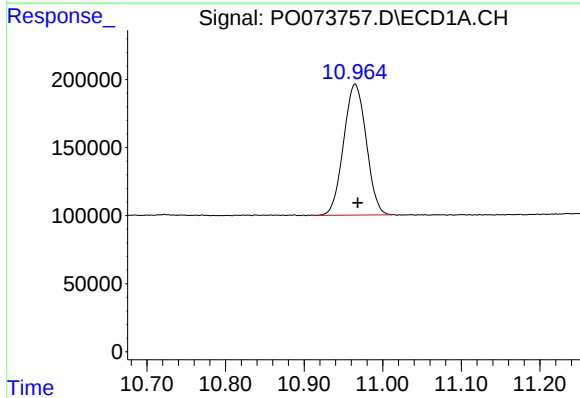

#2 Decachlorobiphenyl

R.T.: 10.965 min  
Delta R.T.: -0.003 min  
Response: 1926429  
Conc: 23.31 ng/ml

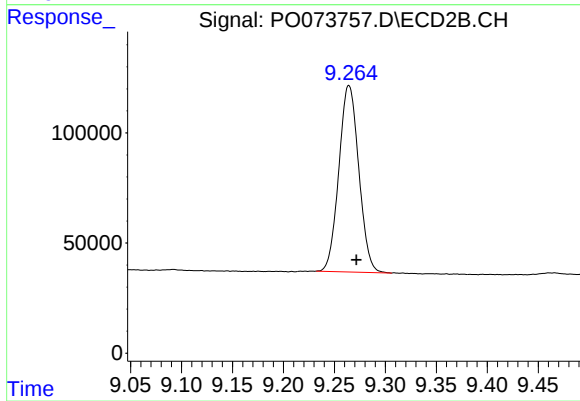

#2 Decachlorobiphenyl

R.T.: 9.264 min  
Delta R.T.: -0.008 min  
Response: 1152608  
Conc: 24.63 ng/ml