

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121420\
 Data File : PO073785.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Dec 2020 22:02
 Operator : DD\AJ
 Sample : L5081-05 10X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 WOOSPK-039-0002

Manual Integrations
 APPROVED

Ankita
 12/15/2020 1:09:56 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 03:42:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 11 03:58:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.938	3.998	127797	117492	1.398	2.191 #
2) SA Decachlor...	10.954	9.267	2092164	7043620	25.317m	150.535 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121420\
Data File : PO073785.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Dec 2020 22:02
Operator : DD\AJ
Sample : L5081-05 10X
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
WOOSPK-039-0002


Manual Integrations
APPROVED

Ankita
12/15/2020 1:09:56 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 03:42:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 11 03:58:06 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

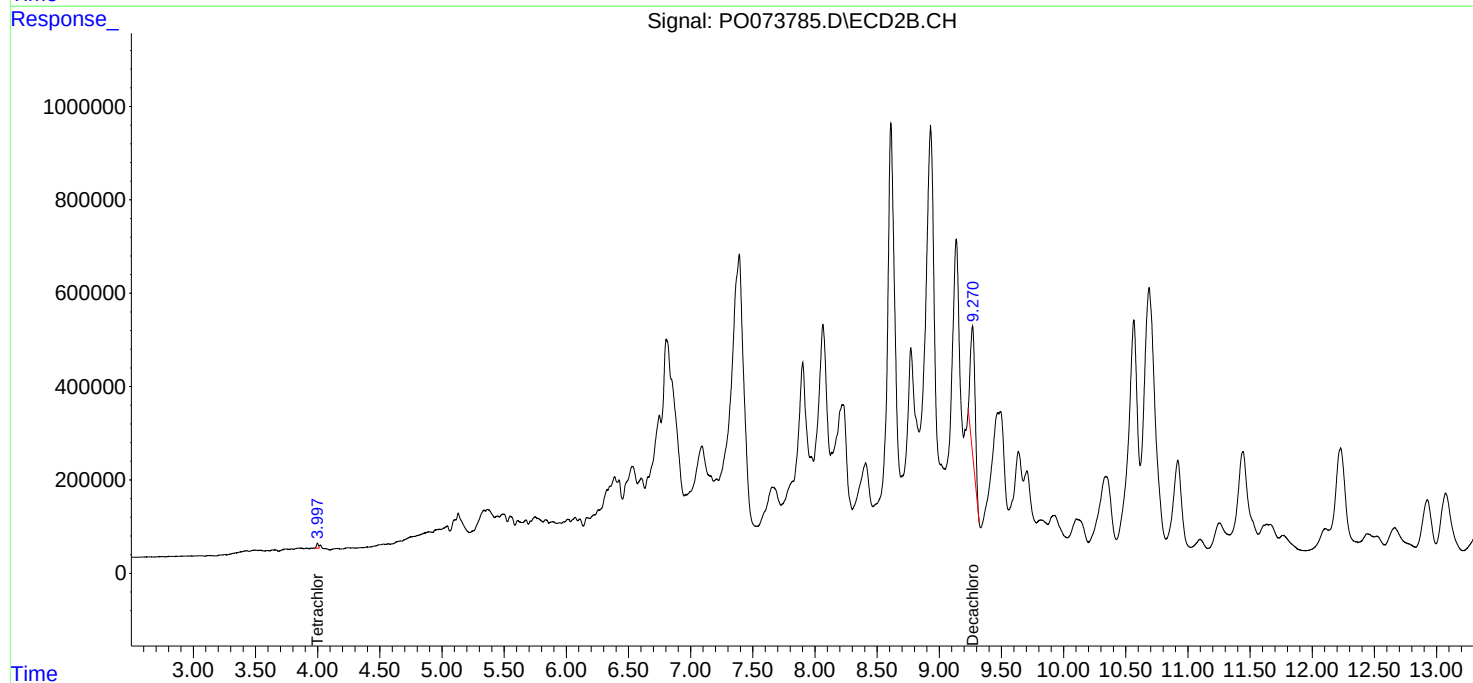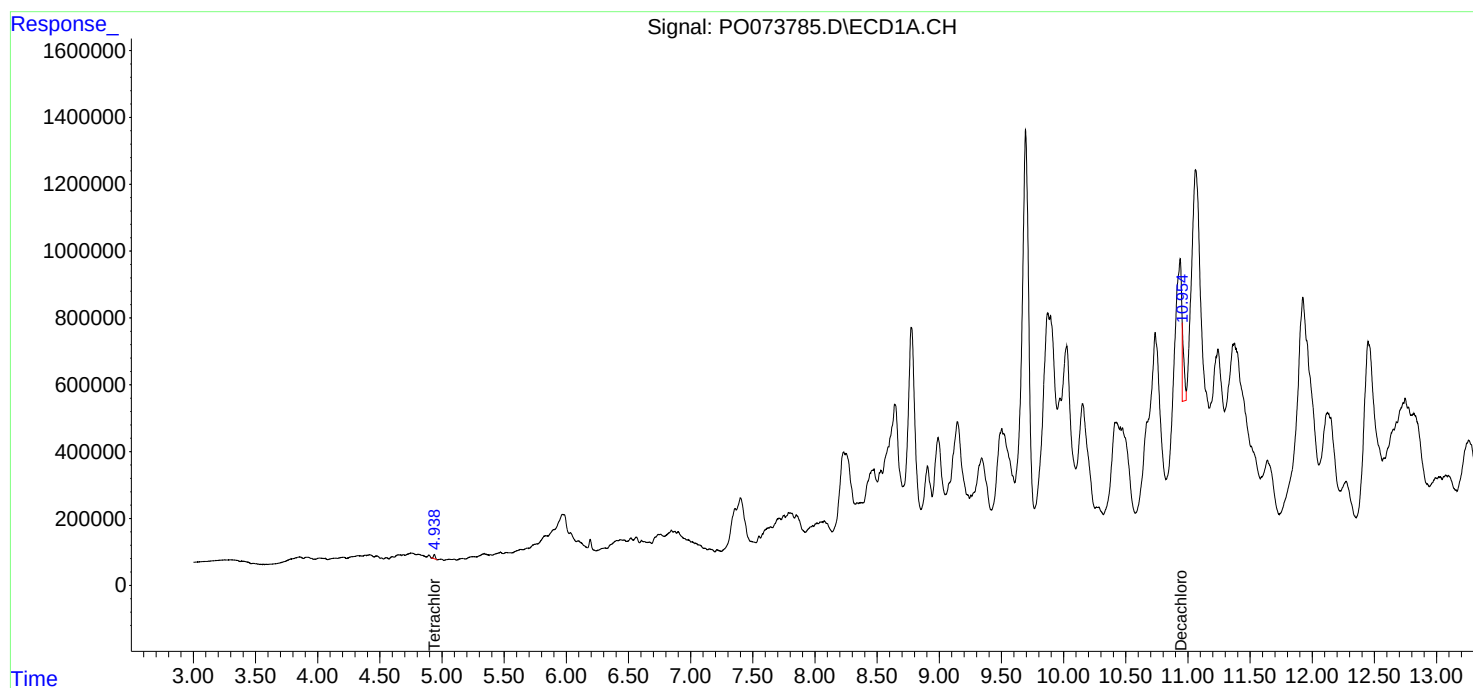

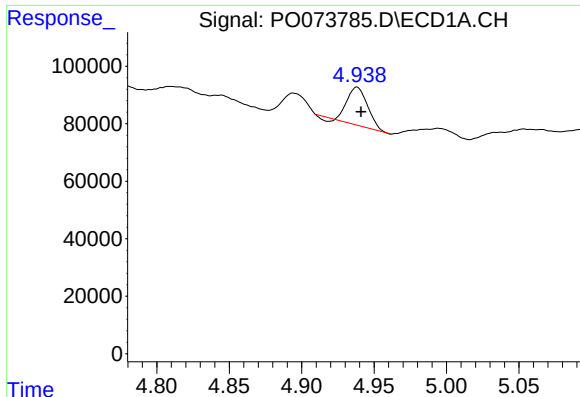


#1 Tetrachloro-m-xylene

R.T.: 4.938 min
Delta R.T.: -0.003 min
Response: 127797
Conc: 1.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
WOOSPK-039-0002


Manual Integrations
APPROVED

Ankita
12/15/2020 1:09:56 PM

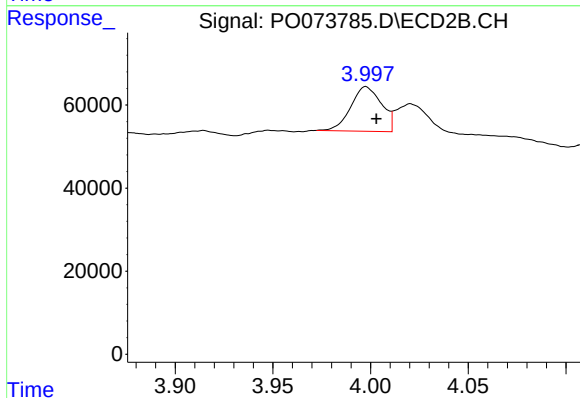


#1 Tetrachloro-m-xylene

R.T.: 3.998 min
Delta R.T.: -0.005 min
Response: 117492
Conc: 2.19 ng/ml

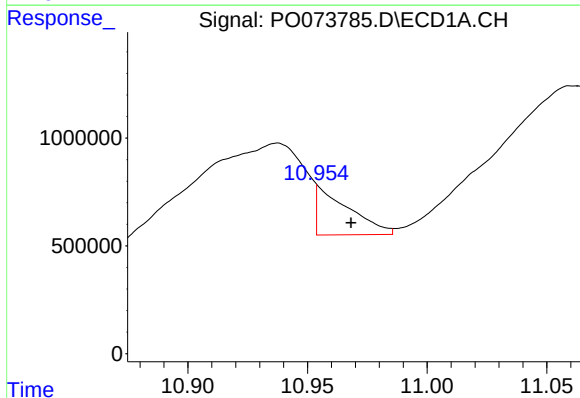

#2 Decachlorobiphenyl

R.T.: 10.954 min
Delta R.T.: -0.014 min
Response: 2092164
Conc: 25.32 ng/ml m

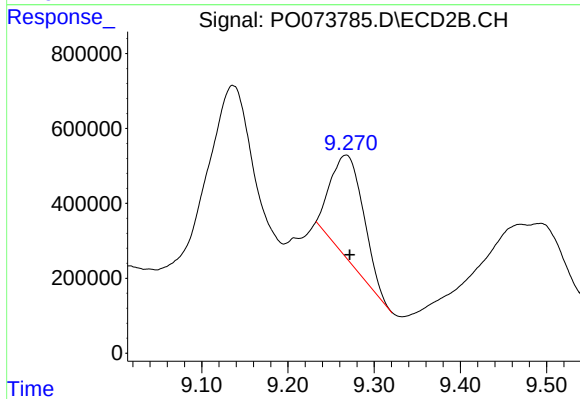

#2 Decachlorobiphenyl

R.T.: 9.267 min
Delta R.T.: -0.004 min
Response: 7043620
Conc: 150.53 ng/ml