

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121421\
 Data File : PO083658.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Dec 2021 14:02
 Operator : AJ\MA
 Sample : M5064-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 14 23:49:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 07 13:18:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.936	3.942	2149178	695630	22.527	22.363
2)	SA Decachlor...	11.005	9.237	1398290	590231	19.574	18.092
Target Compounds							
8)	L2 AR-1221-1	5.194	0.000	113599	0	112.966	N.D. #
9)	L2 AR-1221-2	5.292	4.288	32037	35400	44.479	122.968 #
12)	L3 AR-1232-2	5.987	0.000	25766	0	26.118	N.D. #
30)	L6 AR-1254-5	8.534	0.000	1554	0	0.433	N.D. #
32)	L7 AR-1260-2	8.262f	0.000	3672	0	0.880	N.D. #
33)	L7 AR-1260-3	8.614	0.000	9756	0	3.112	N.D. #
34)	L7 AR-1260-4	8.843	0.000	10146	0	2.898	N.D. #
36)	L8 AR-1262-1	8.614	0.000	9756	0	2.348	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121421\
Data File : P0083658.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Dec 2021 14:02
Operator : AJ\MA
Sample : M5064-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 14 23:49:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120621.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 07 13:18:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

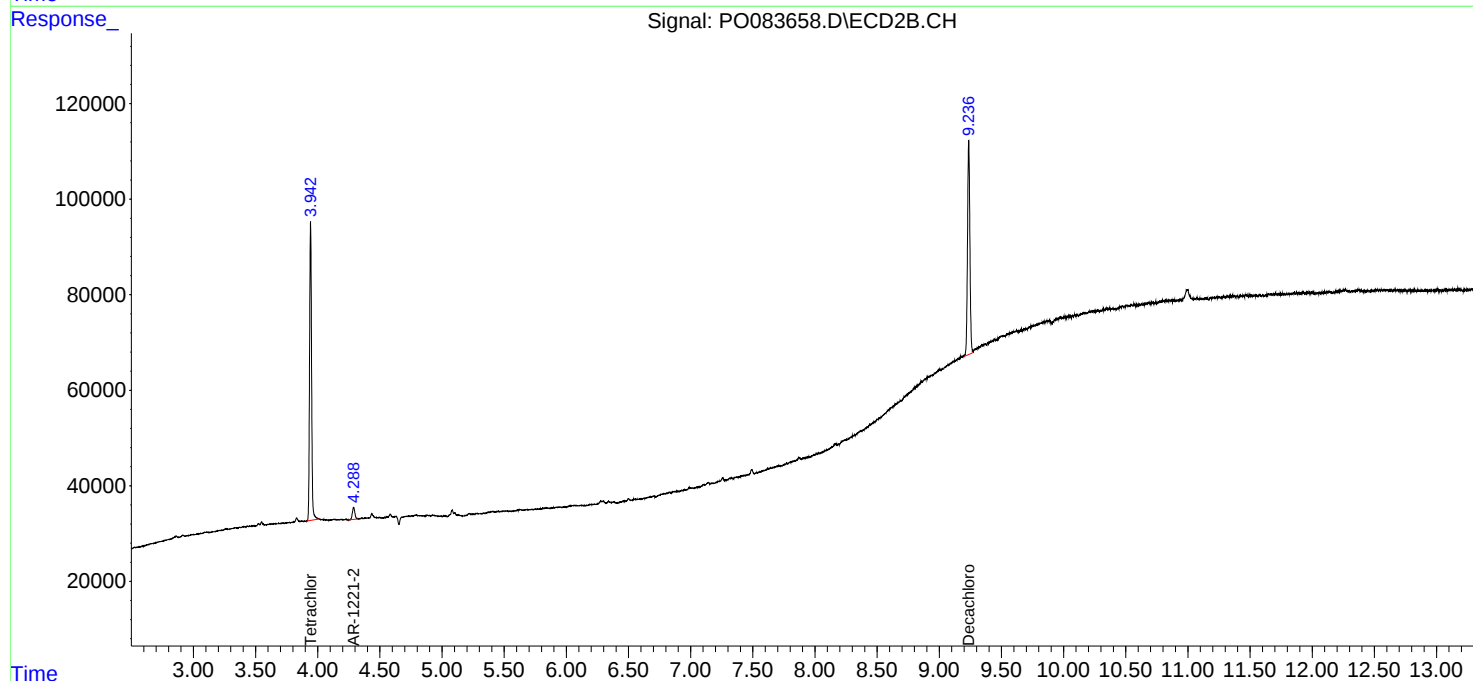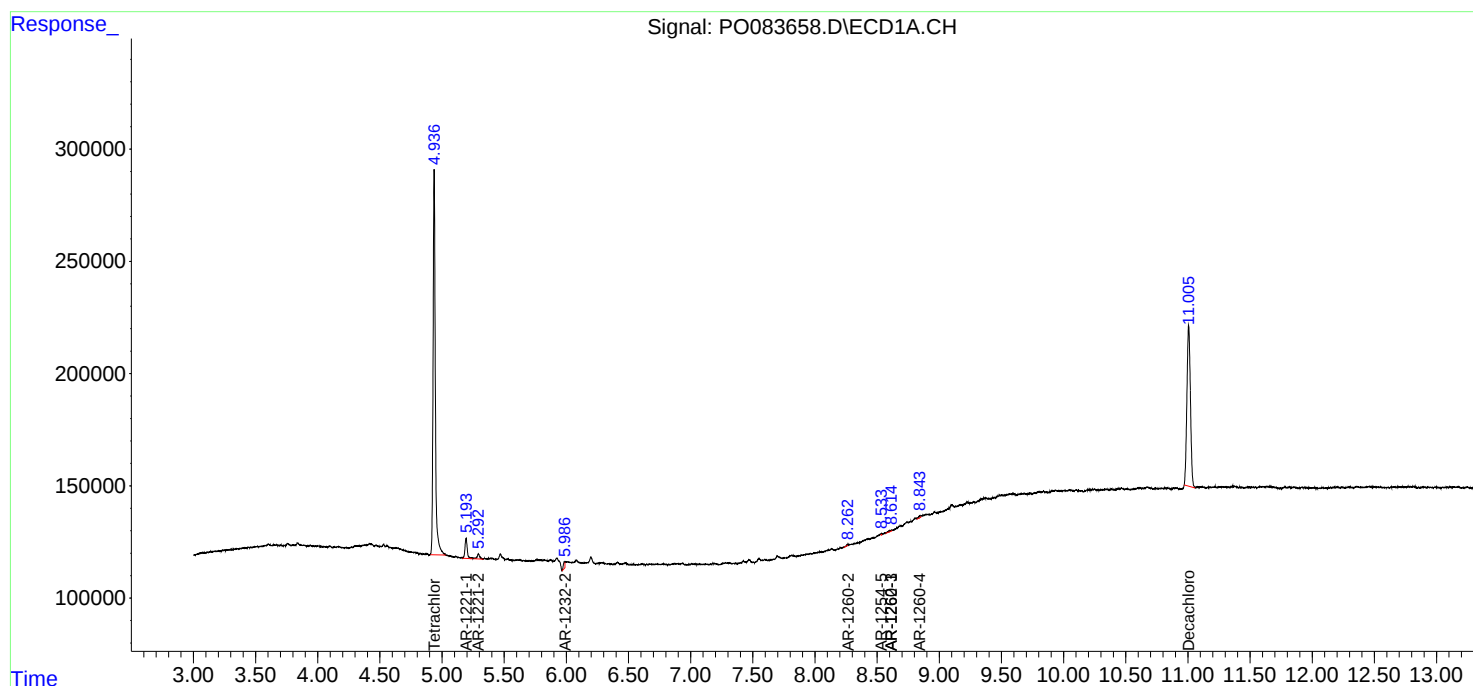


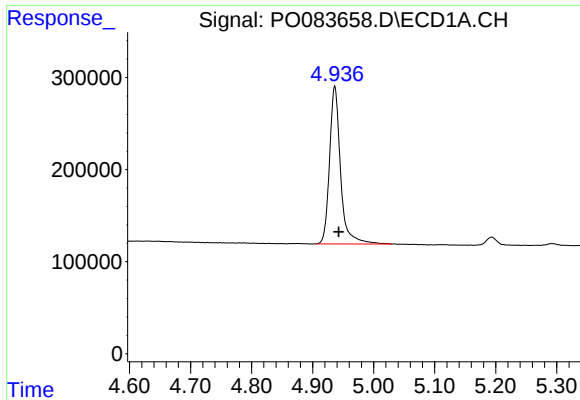

#1 Tetrachloro-m-xylene


R.T.: 4.936 min
Delta R.T.: -0.007 min
Response: 2149178
Conc: 22.53 ng/ml

Instrument :
ECD_O
ClientSampleId :

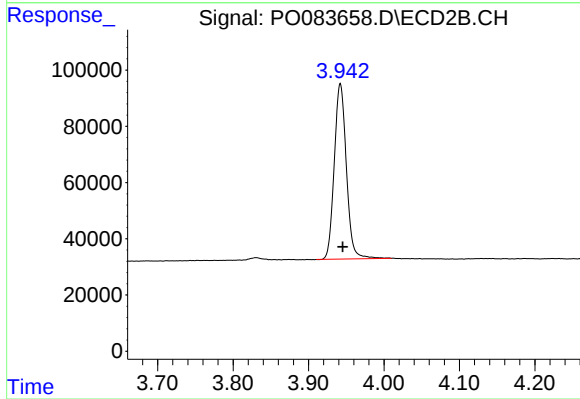


#1 Tetrachloro-m-xylene

R.T.: 3.942 min
Delta R.T.: -0.003 min
Response: 695630
Conc: 22.36 ng/ml

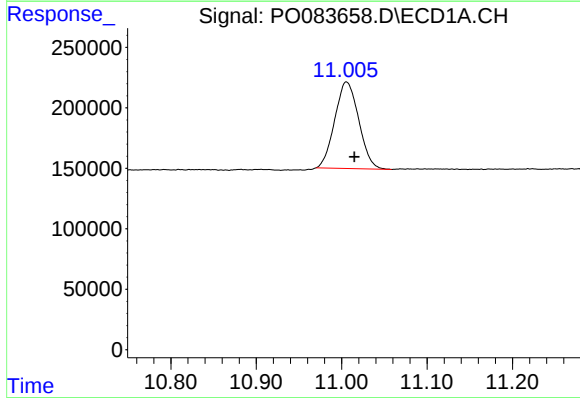


#2 Decachlorobiphenyl

R.T.: 11.005 min
Delta R.T.: -0.010 min
Response: 1398290
Conc: 19.57 ng/ml

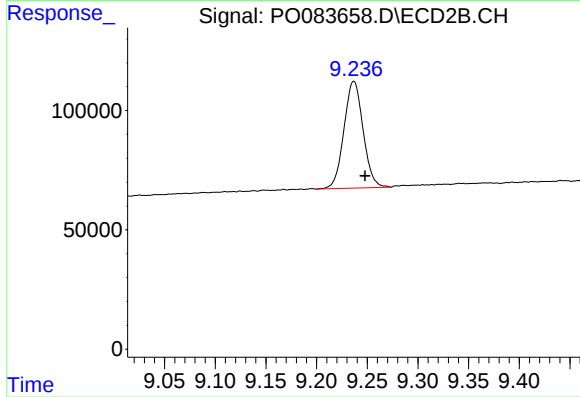

#2 Decachlorobiphenyl


R.T.: 9.237 min
Delta R.T.: -0.011 min
Response: 590231
Conc: 18.09 ng/ml

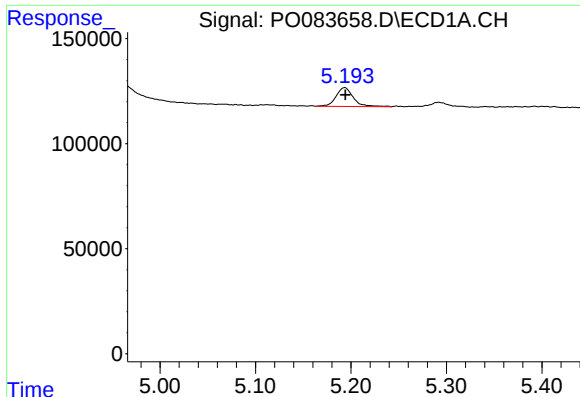

#8 AR-1221-1


R.T.: 5.194 min
Delta R.T.: 0.000 min
Response: 113599
Conc: 112.97 ng/ml

Instrument :
ECD_O
ClientSampleId :

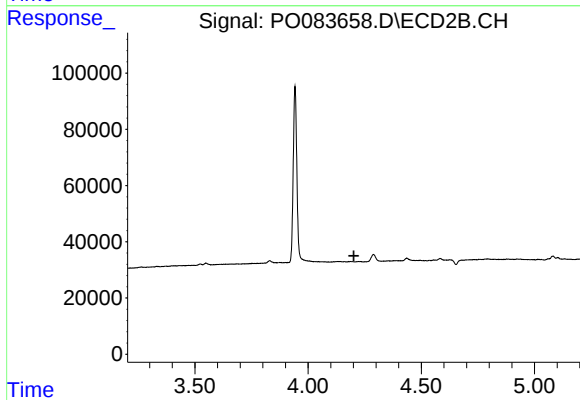


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.202 min
Response: 0
Conc: N.D.

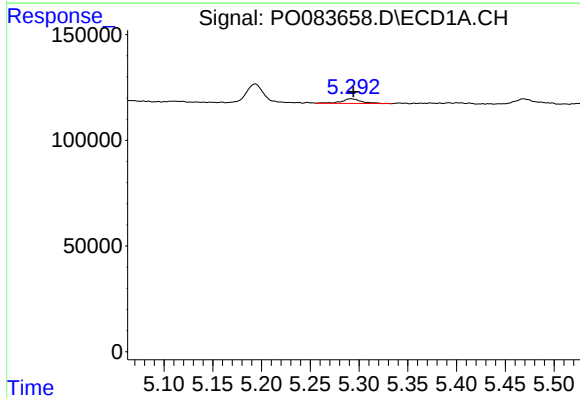


#9 AR-1221-2

R.T.: 5.292 min
Delta R.T.: -0.002 min
Response: 32037
Conc: 44.48 ng/ml

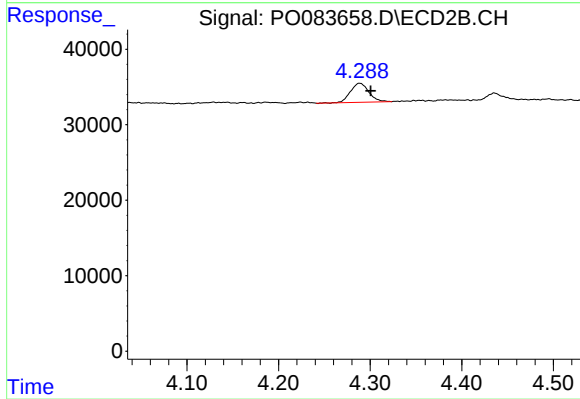

#9 AR-1221-2


R.T.: 4.288 min
Delta R.T.: -0.012 min
Response: 35400
Conc: 122.97 ng/ml

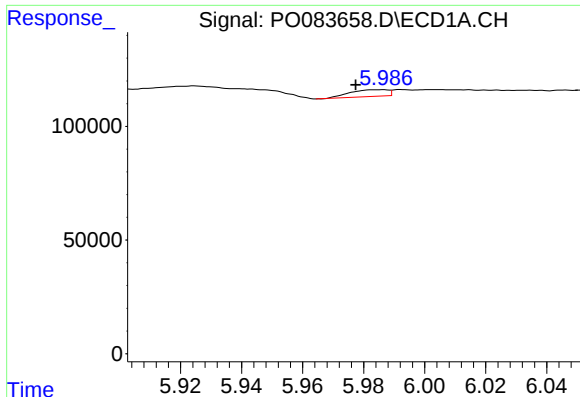

#12 AR-1232-2


R.T.: 5.987 min
Delta R.T.: 0.009 min
Response: 25766
Conc: 26.12 ng/ml

Instrument :
ECD_O
ClientSampleId :

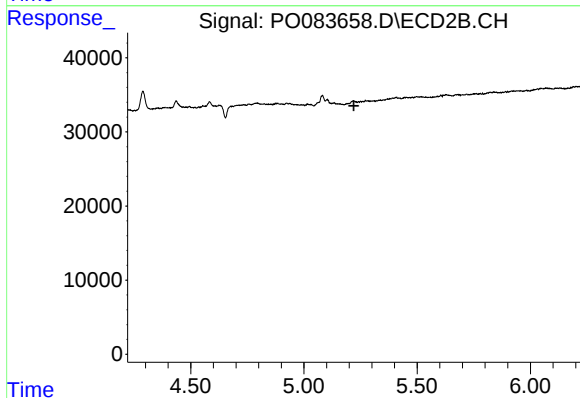


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 5.221 min
Response: 0
Conc: N.D.

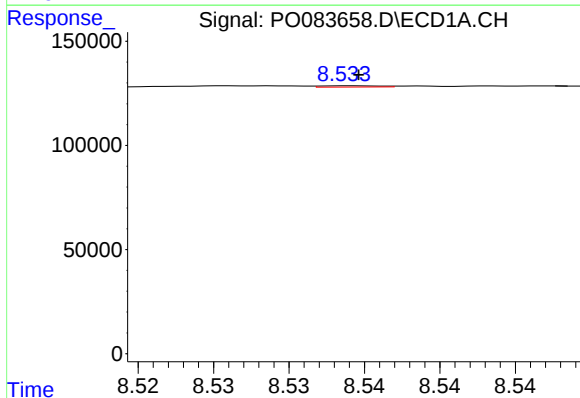


#30 AR-1254-5

R.T.: 8.534 min
Delta R.T.: 0.000 min
Response: 1554
Conc: 0.43 ng/ml

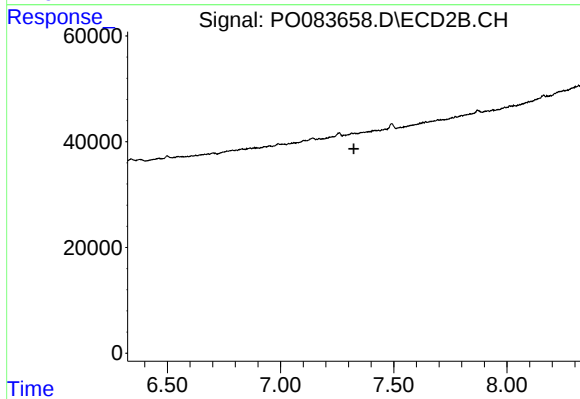

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.324 min
Response: 0
Conc: N.D.

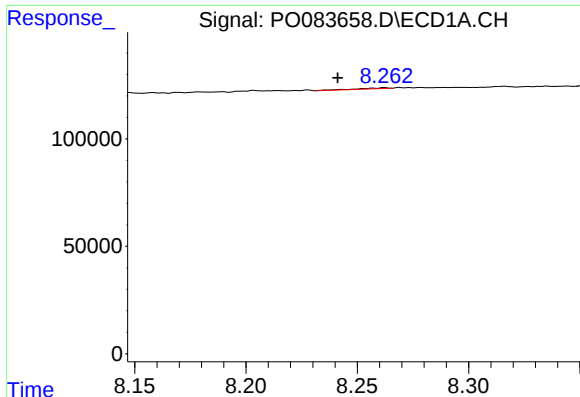

#32 AR-1260-2


R.T.: 8.262 min
Delta R.T.: 0.021 min
Response: 3672
Conc: 0.88 ng/ml

Instrument :
ECD_O
ClientSampleId :

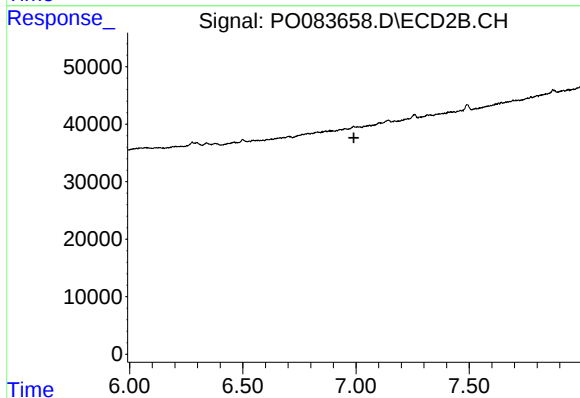


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.990 min
Response: 0
Conc: N.D.

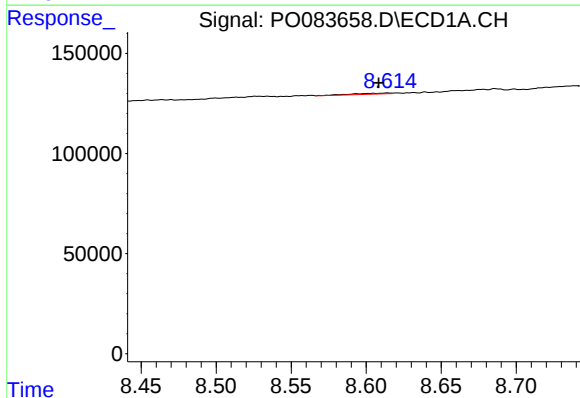


#33 AR-1260-3

R.T.: 8.614 min
Delta R.T.: 0.006 min
Response: 9756
Conc: 3.11 ng/ml

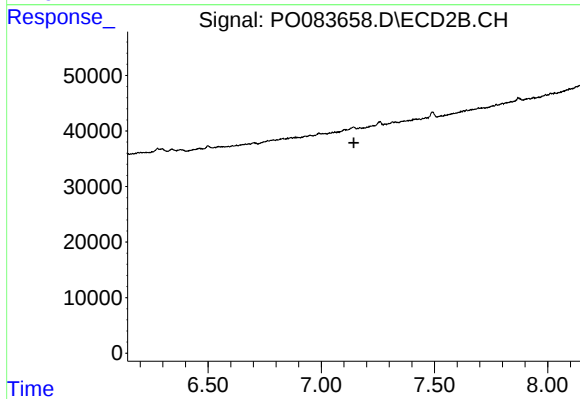

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T. : 7.144 min
Response: 0
Conc: N.D.

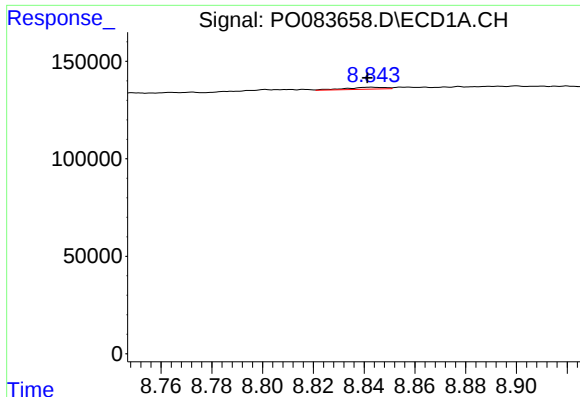

#34 AR-1260-4


R.T.: 8.843 min
Delta R.T.: 0.002 min
Response: 10146
Conc: 2.90 ng/ml

Instrument :
ECD_O
ClientSampleId :

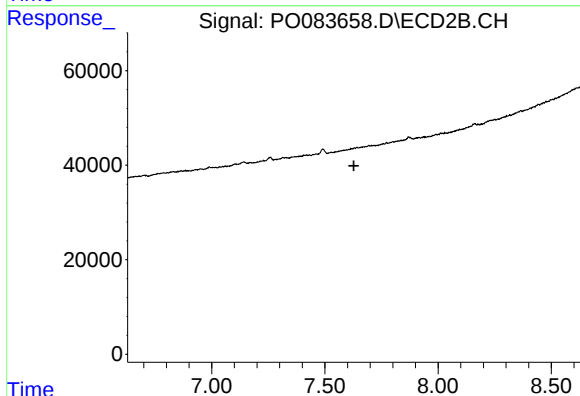


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.628 min
Response: 0
Conc: N.D.

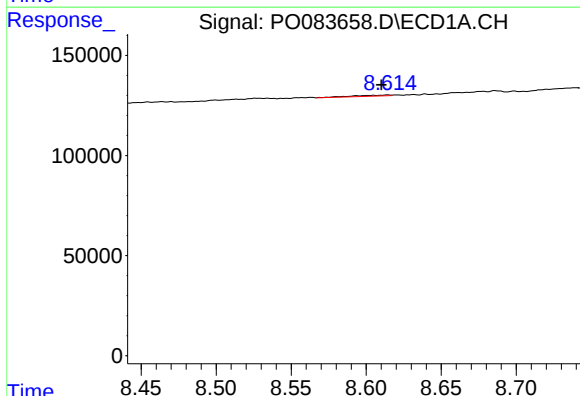

#36 AR-1262-1

R.T.: 8.614 min
Delta R.T.: 0.004 min
Response: 9756
Conc: 2.35 ng/ml

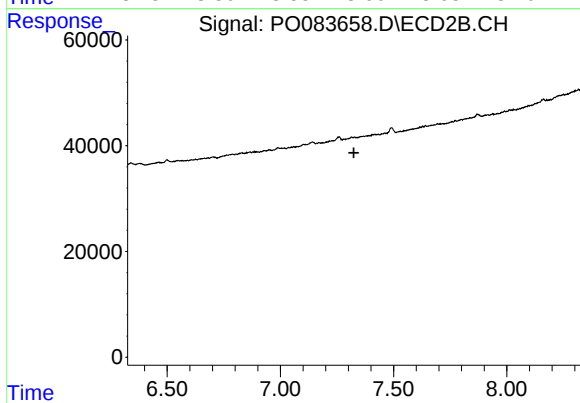

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.324 min
Response: 0
Conc: N.D.