

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121421\
 Data File : PO083674.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Dec 2021 18:38
 Operator : AJ\MA
 Sample : M5071-02 10X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 00:02:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 07 13:18:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.933	3.939	115975	46386	1.216	1.491
2)	SA Decachlor...	10.999f	9.235	120076	48807	1.681	1.496
Target Compounds							
8)	L2 AR-1221-1	5.168f	0.000	8137	0	8.092	N.D. #
30)	L6 AR-1254-5	8.513f	0.000	18937	0	5.280	N.D. #
33)	L7 AR-1260-3	8.588f	0.000	6970	0	2.223	N.D. #
34)	L7 AR-1260-4	8.858f	0.000	17731	0	5.064	N.D. #
36)	L8 AR-1262-1	8.588f	0.000	6970	0	1.678	N.D. #
39)	L8 AR-1262-4	9.608f	0.000	28898	0	14.851	N.D. #
42)	L9 AR-1268-2	9.608f	0.000	28898	0	3.498	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121421\
Data File : PO083674.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Dec 2021 18:38
Operator : AJ\MA
Sample : M5071-02 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 00:02:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120621.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 07 13:18:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

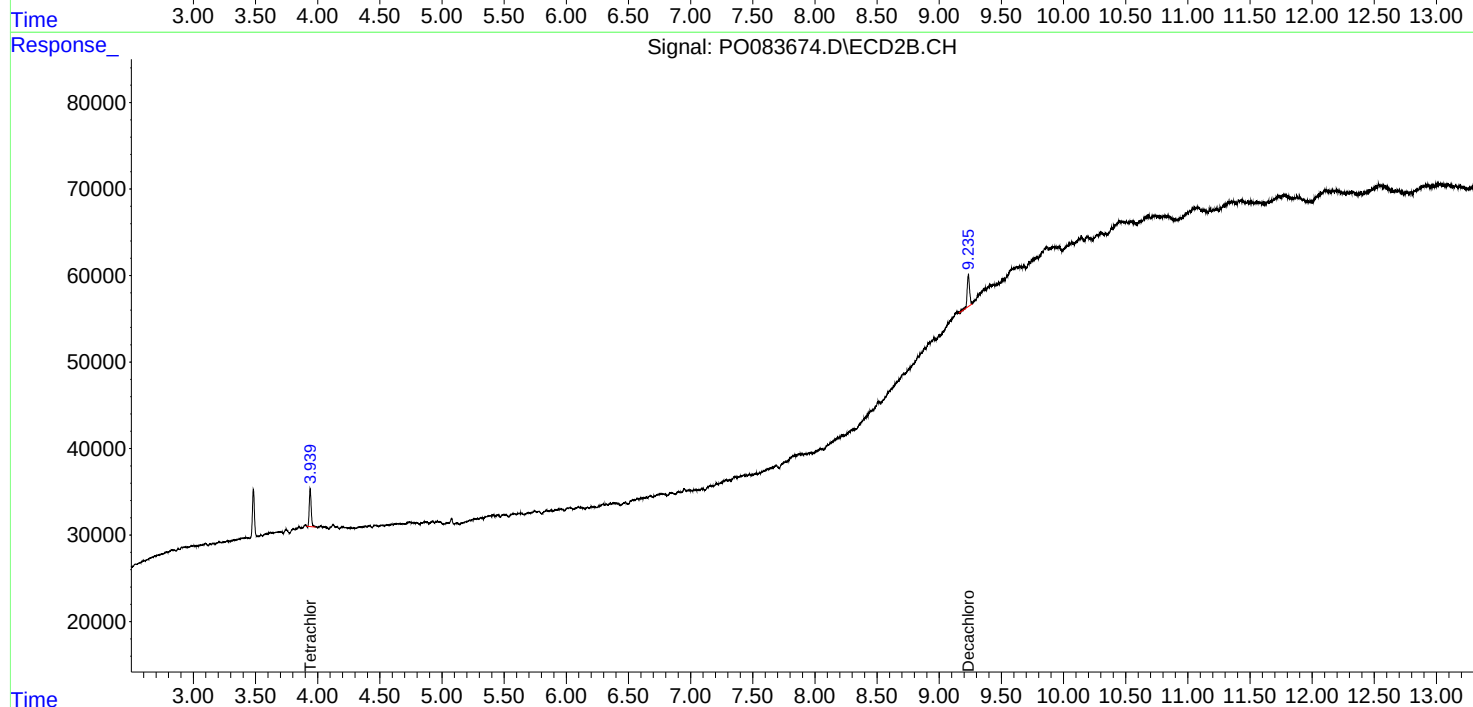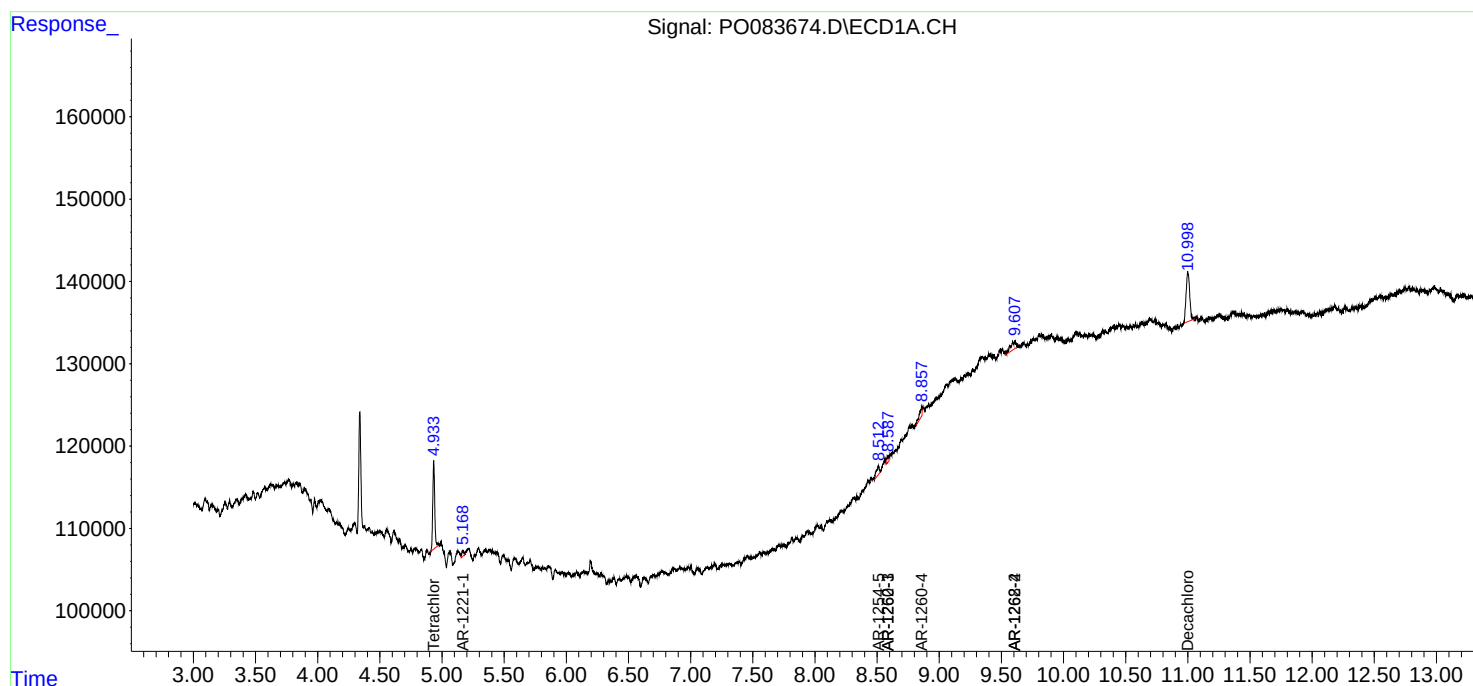


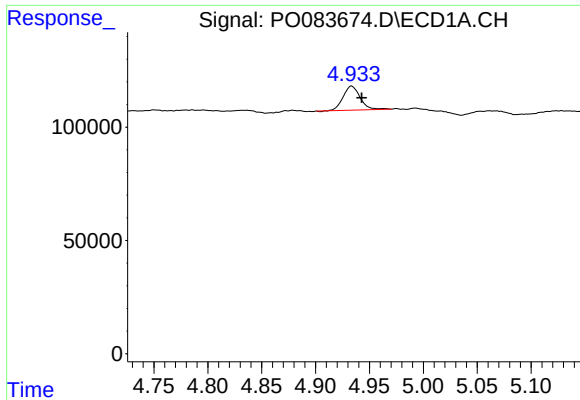

#1 Tetrachloro-m-xylene


R.T.: 4.933 min
Delta R.T.: -0.010 min
Response: 115975
Conc: 1.22 ng/ml

Instrument :
ECD_O
ClientSampleId :

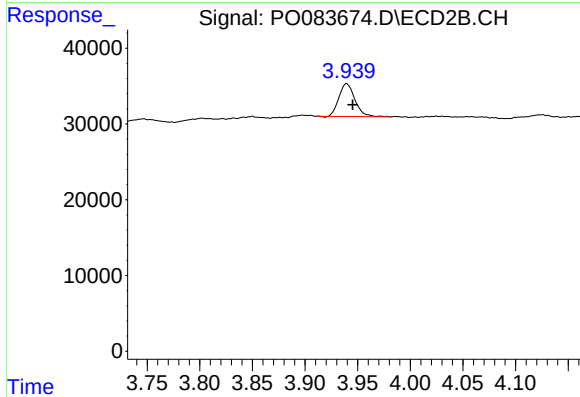


#1 Tetrachloro-m-xylene

R.T.: 3.939 min
Delta R.T.: -0.006 min
Response: 46386
Conc: 1.49 ng/ml

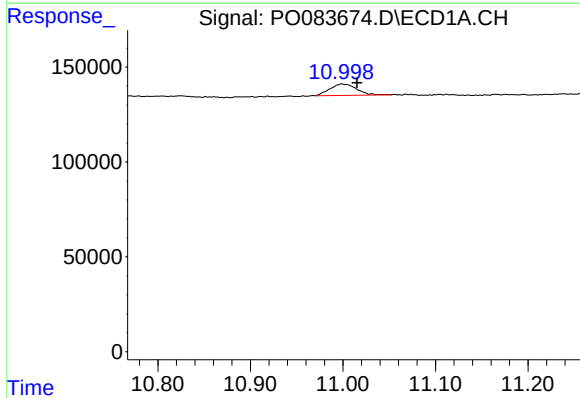


#2 Decachlorobiphenyl

R.T.: 10.999 min
Delta R.T.: -0.016 min
Response: 120076
Conc: 1.68 ng/ml

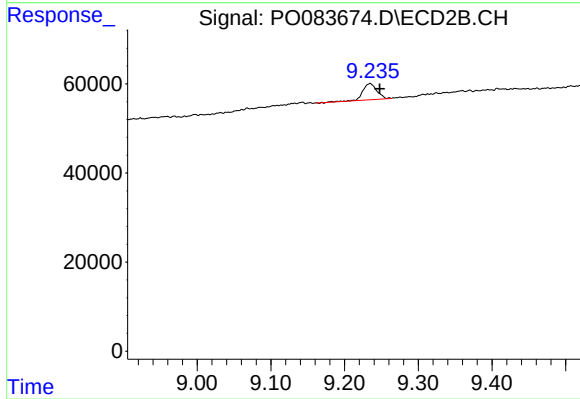

#2 Decachlorobiphenyl


R.T.: 9.235 min
Delta R.T.: -0.013 min
Response: 48807
Conc: 1.50 ng/ml

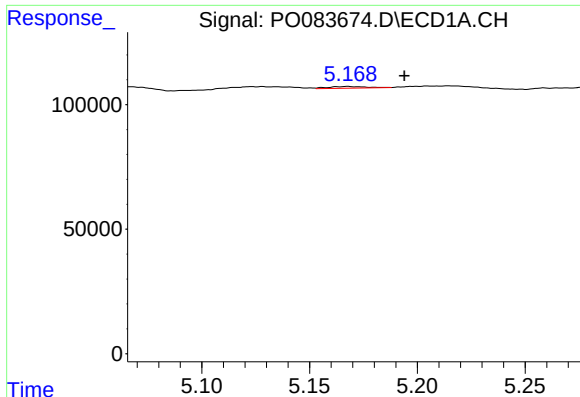

#8 AR-1221-1


R.T.: 5.168 min
Delta R.T.: -0.026 min
Response: 8137
Conc: 8.09 ng/ml

Instrument :
ECD_O
ClientSampleId :

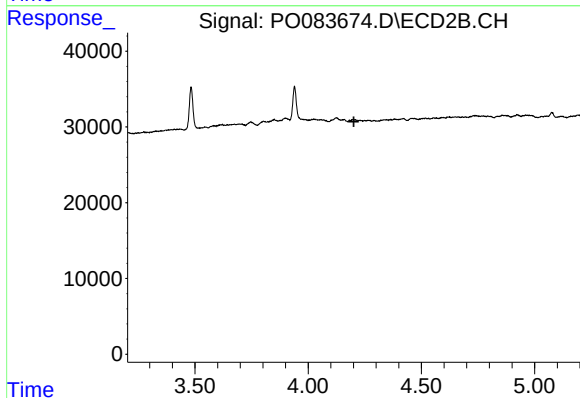


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.202 min
Response: 0
Conc: N.D.

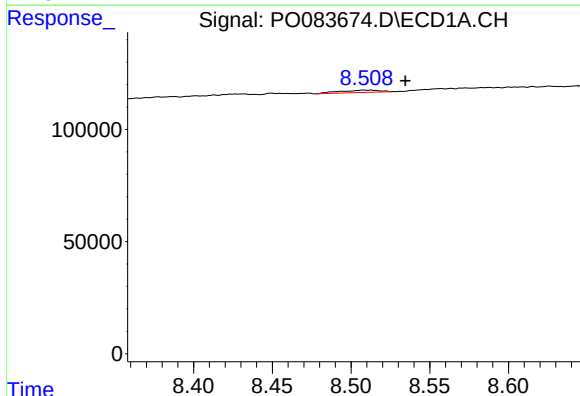


#30 AR-1254-5

R.T.: 8.513 min
Delta R.T.: -0.022 min
Response: 18937
Conc: 5.28 ng/ml

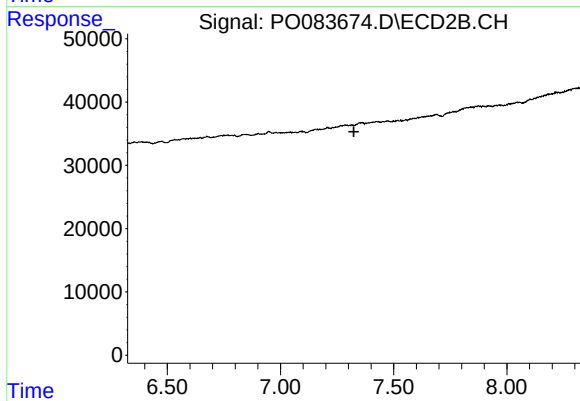

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.324 min
Response: 0
Conc: N.D.

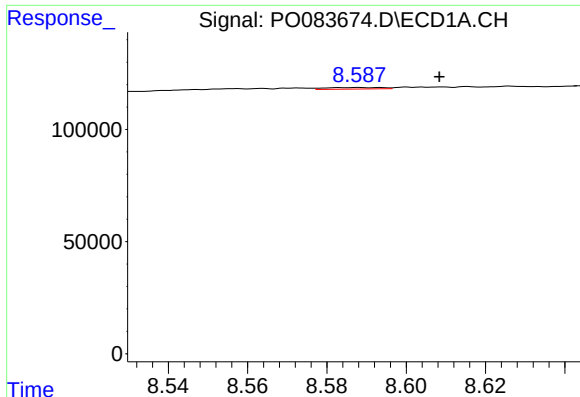

#33 AR-1260-3


R.T.: 8.588 min
Delta R.T.: -0.020 min
Response: 6970
Conc: 2.22 ng/ml

Instrument :
ECD_O
ClientSampleId :

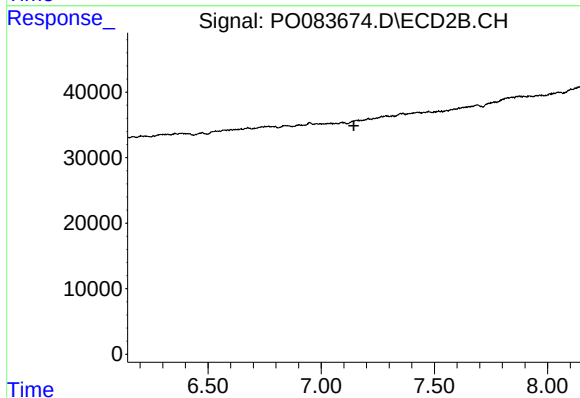


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 7.144 min
Response: 0
Conc: N.D.

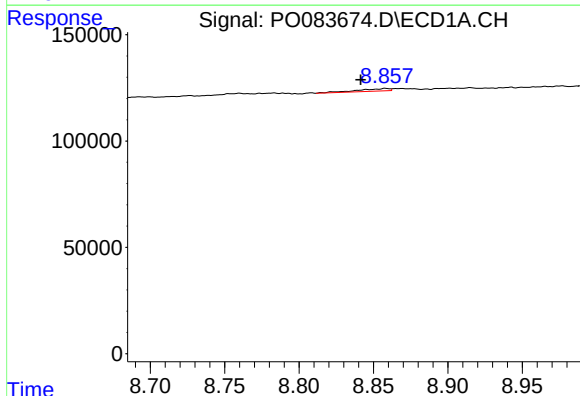


#34 AR-1260-4

R.T.: 8.858 min
Delta R.T.: 0.016 min
Response: 17731
Conc: 5.06 ng/ml

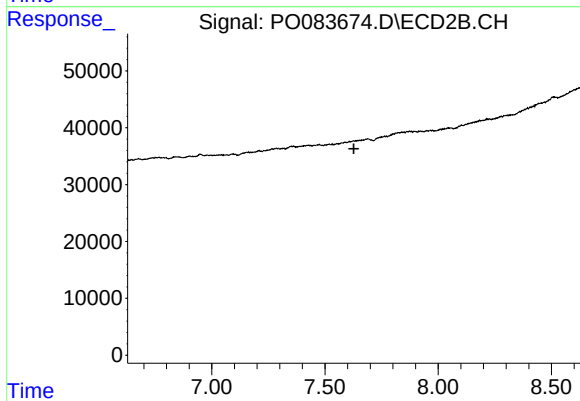

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 7.628 min
Response: 0
Conc: N.D.

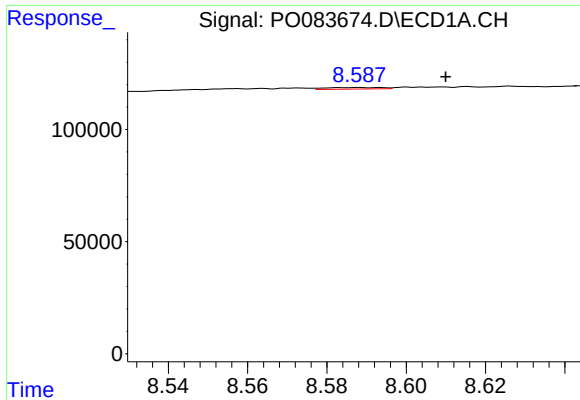

#36 AR-1262-1


R.T.: 8.588 min
Delta R.T.: -0.022 min
Response: 6970
Conc: 1.68 ng/ml

Instrument :
ECD_O
ClientSampleId :

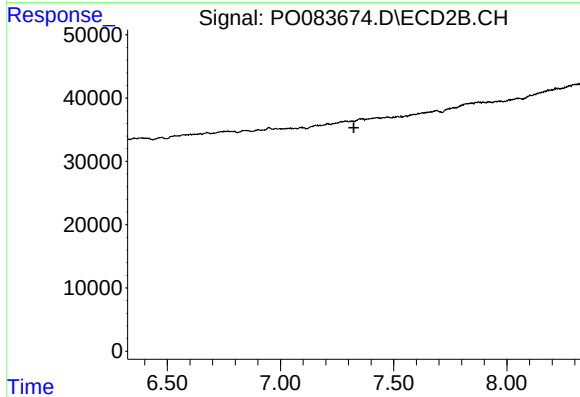


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.324 min
Response: 0
Conc: N.D.

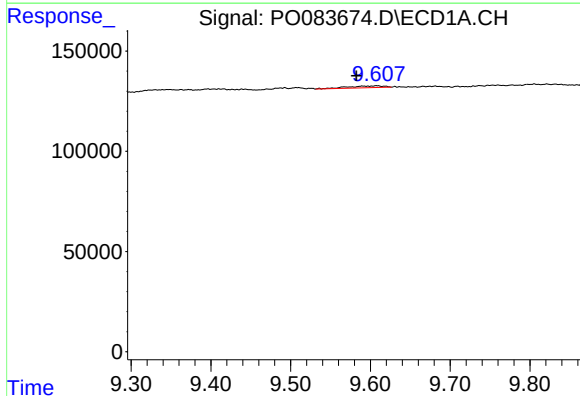


#39 AR-1262-4

R.T.: 9.608 min
Delta R.T.: 0.025 min
Response: 28898
Conc: 14.85 ng/ml

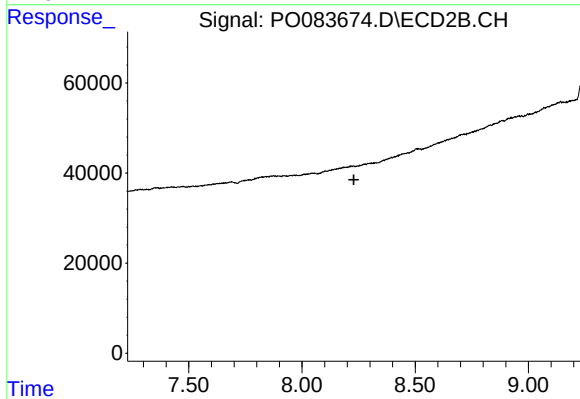

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 8.229 min
Response: 0
Conc: N.D.

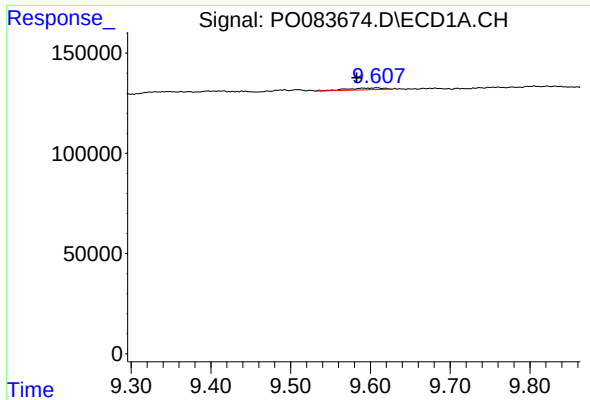

#42 AR-1268-2

R.T.: 9.608 min
Delta R.T.: 0.025 min
Response: 28898
Conc: 3.50 ng/ml

Instrument :
ECD_O
ClientSampleId :

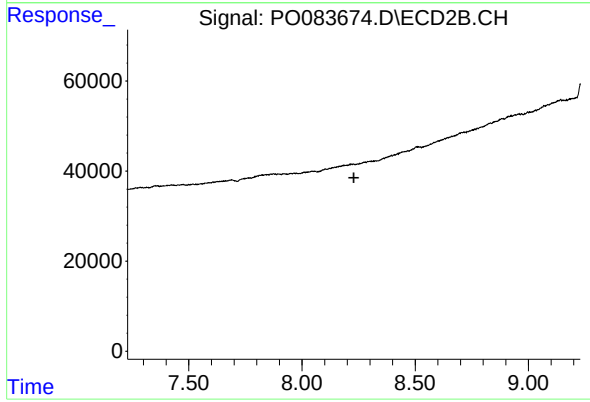

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 8.229 min
Response: 0
Conc: N.D.