

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0121421\
 Data File : P0083663.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Dec 2021 15:29
 Operator : AJ\MA
 Sample : M5064-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SASP2-121-1-(17-32)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 00:48:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0120621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 07 13:18:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.935	3.941	2171986	702704	22.766	22.591
2) SA Decachlor...	11.003	9.236	1460406	593529	20.443	18.193

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121421\
Data File : P0083663.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Dec 2021 15:29
Operator : AJ\MA
Sample : M5064-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SASP2-121-1-(17-32)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 00:48:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120621.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 07 13:18:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

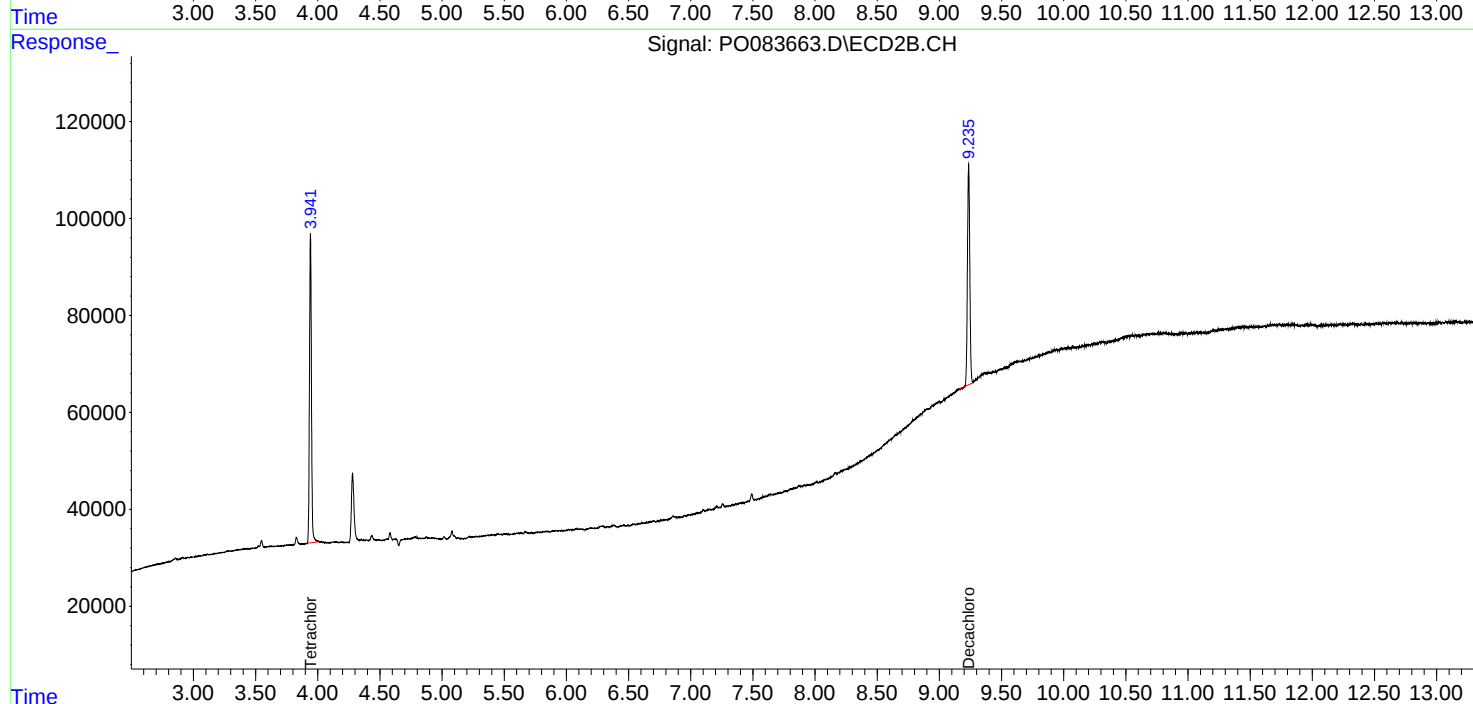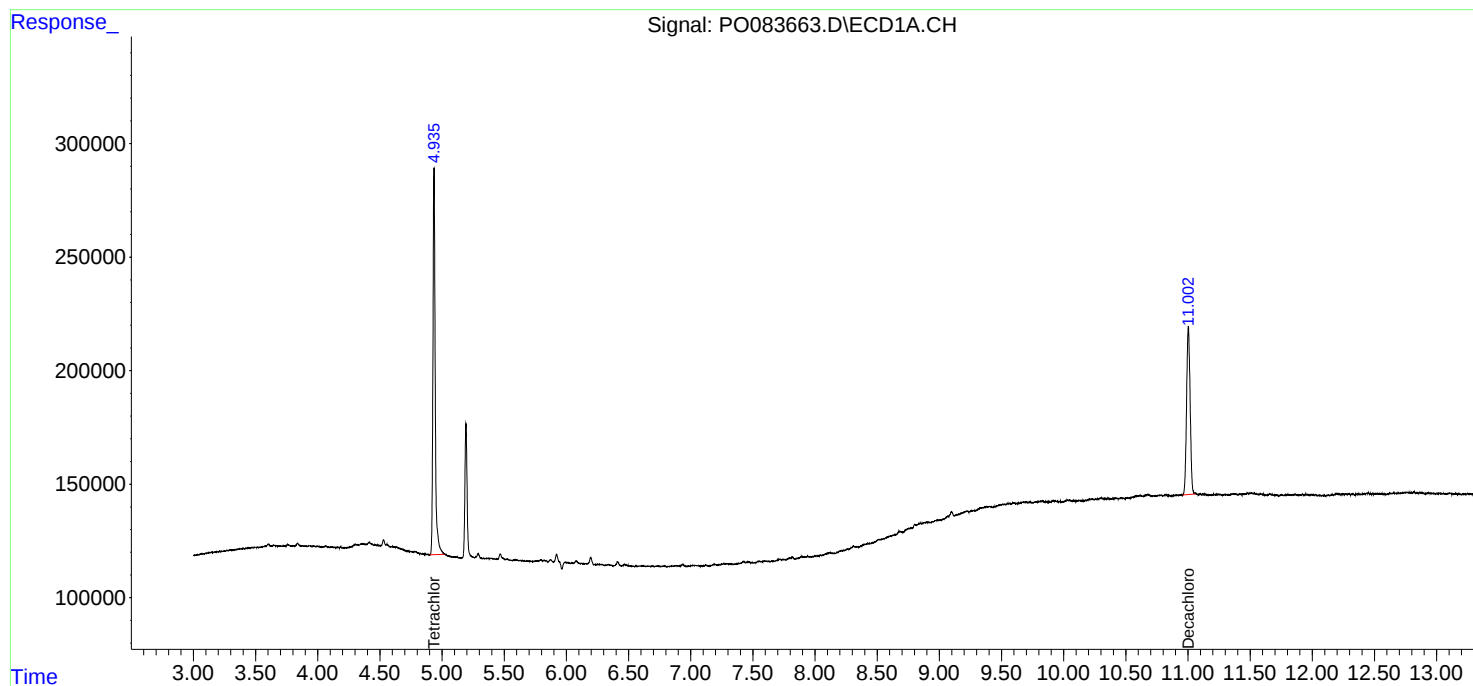


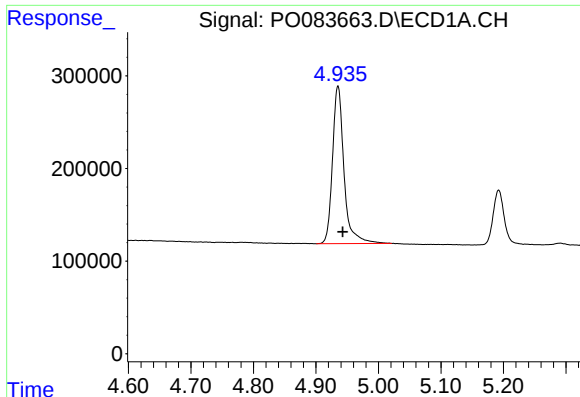

#1 Tetrachloro-m-xylene


R.T.: 4.935 min
Delta R.T.: -0.008 min
Response: 2171986
Conc: 22.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
SASP2-121-1-(17-32)

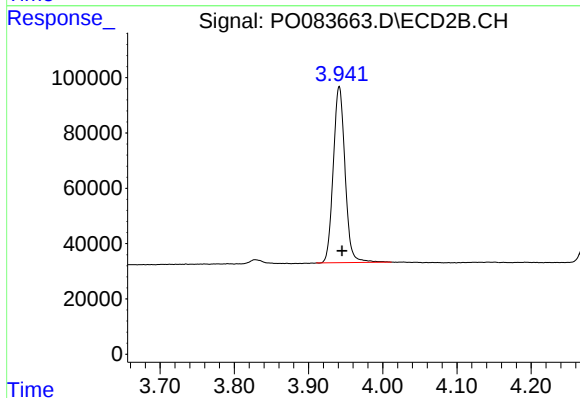


#1 Tetrachloro-m-xylene

R.T.: 3.941 min
Delta R.T.: -0.004 min
Response: 702704
Conc: 22.59 ng/ml

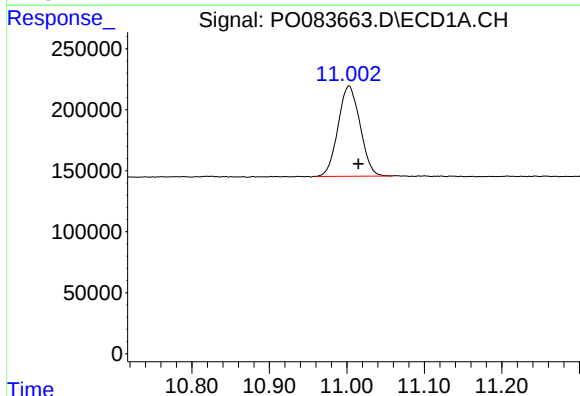

#2 Decachlorobiphenyl

R.T.: 11.003 min
Delta R.T.: -0.012 min
Response: 1460406
Conc: 20.44 ng/ml

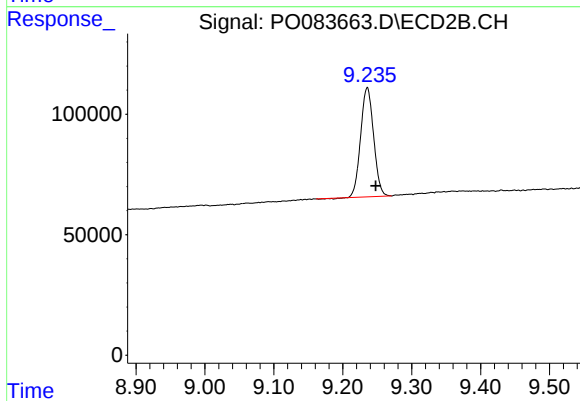

#2 Decachlorobiphenyl

R.T.: 9.236 min
Delta R.T.: -0.012 min
Response: 593529
Conc: 18.19 ng/ml