

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121421\
 Data File : PO083679.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Dec 2021 20:04
 Operator : AJ\MA
 Sample : M5073-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 EO-02-121321

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 05:00:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 07 13:18:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.934	3.940	1720920	554412	18.038	17.823
2) SA Decachlor...	11.001f	9.235	1276935	434903	17.875	13.331 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121421\
Data File : PO083679.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Dec 2021 20:04
Operator : AJ\MA
Sample : M5073-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
EO-02-121321

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 05:00:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120621.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 07 13:18:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

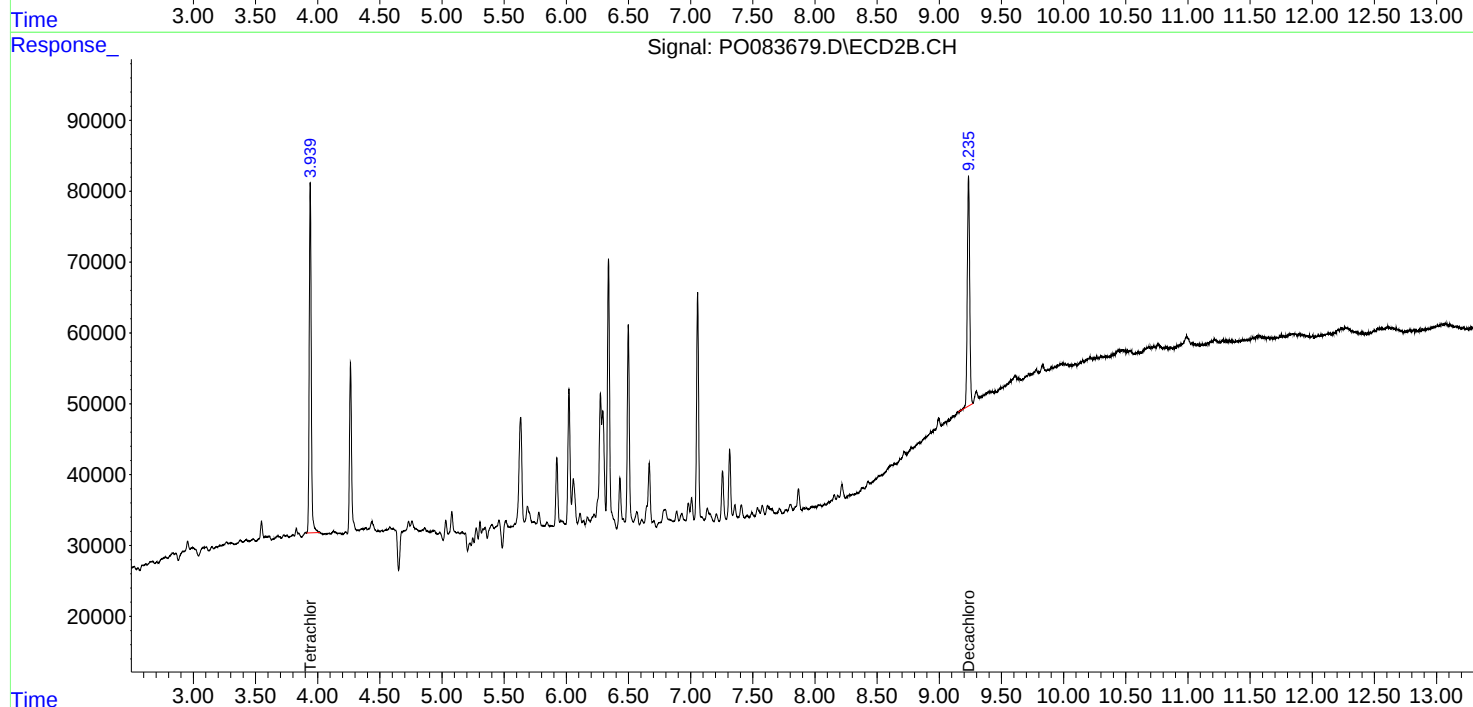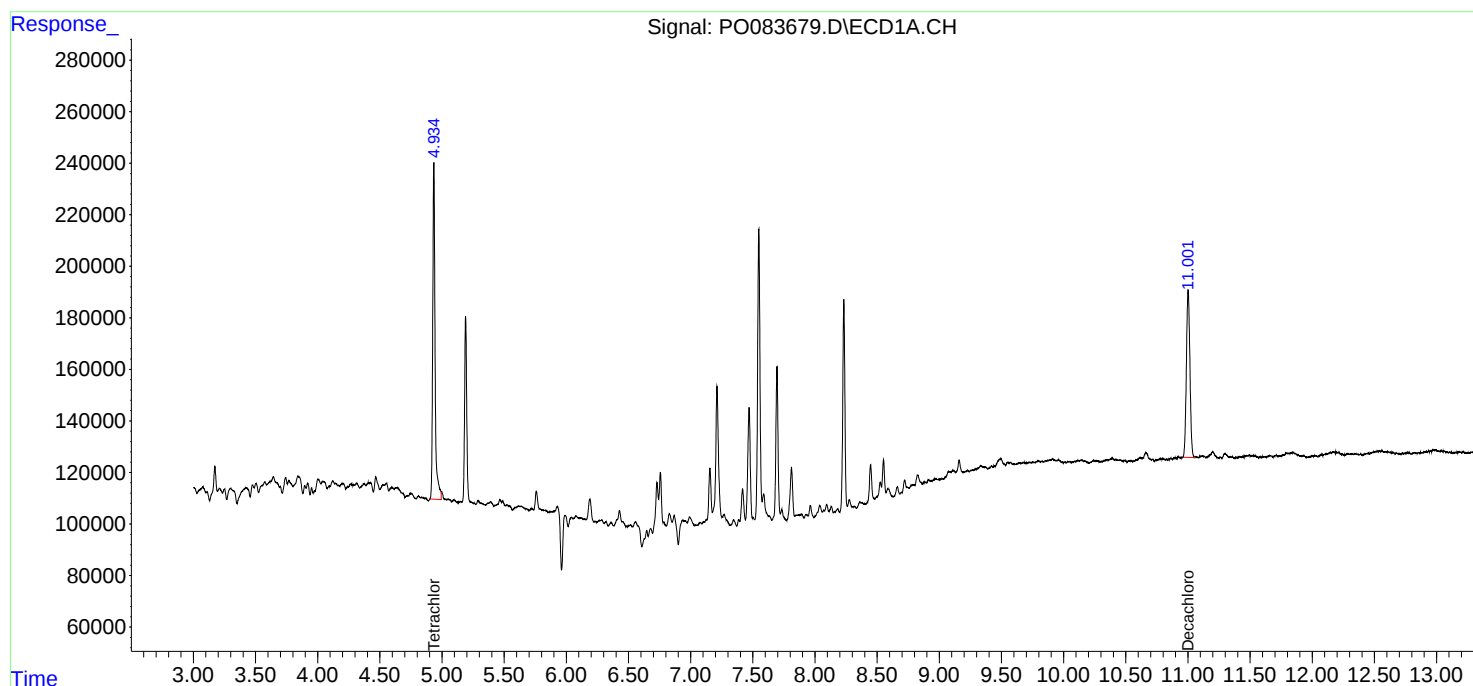


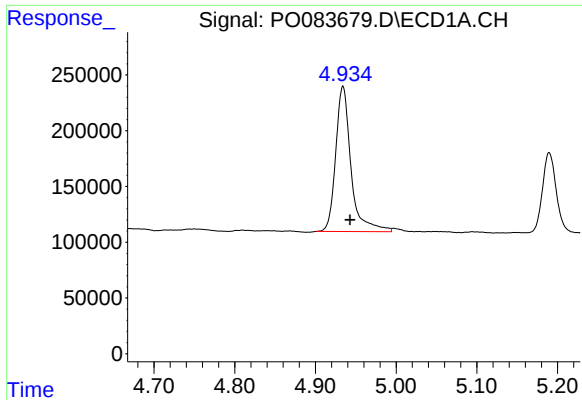

#1 Tetrachloro-m-xylene


R.T.: 4.934 min
Delta R.T.: -0.009 min
Response: 1720920
Conc: 18.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
EO-02-121321

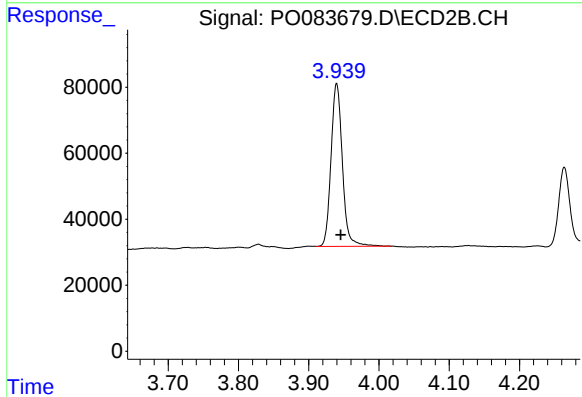


#1 Tetrachloro-m-xylene

R.T.: 3.940 min
Delta R.T.: -0.006 min
Response: 554412
Conc: 17.82 ng/ml

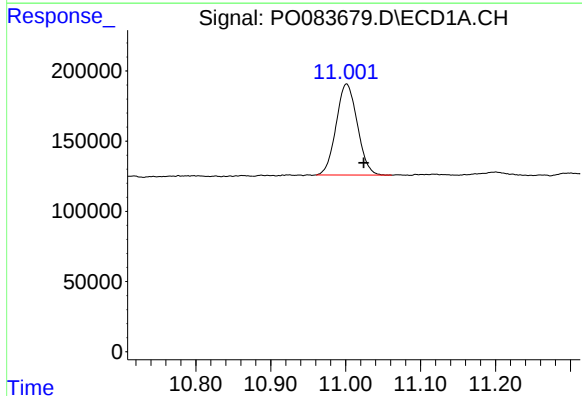

#2 Decachlorobiphenyl

R.T.: 11.001 min
Delta R.T.: -0.023 min
Response: 1276935
Conc: 17.87 ng/ml

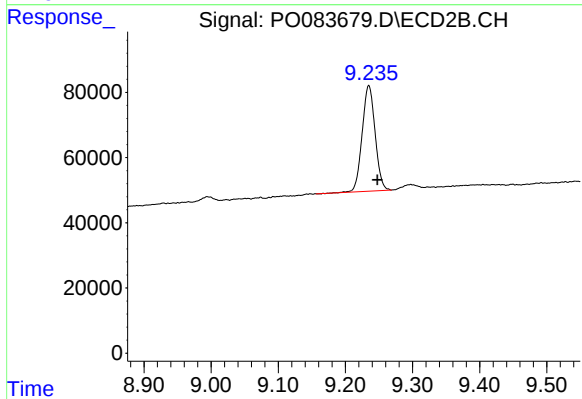

#2 Decachlorobiphenyl

R.T.: 9.235 min
Delta R.T.: -0.013 min
Response: 434903
Conc: 13.33 ng/ml