

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121421\
 Data File : PO083687.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Dec 2021 22:57
 Operator : AJ\MA
 Sample : M5077-01 10X
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 01-A-01-B-01-C

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 02:48:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 07 13:18:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.933	3.940	175735	57864	1.842	1.860
2) SA Decachlor...	10.997f	9.232f	125851	53613	1.762	1.643

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121421\
Data File : PO083687.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Dec 2021 22:57
Operator : AJ\MA
Sample : M5077-01 10X
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
01-A-01-B-01-C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 02:48:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120621.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 07 13:18:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

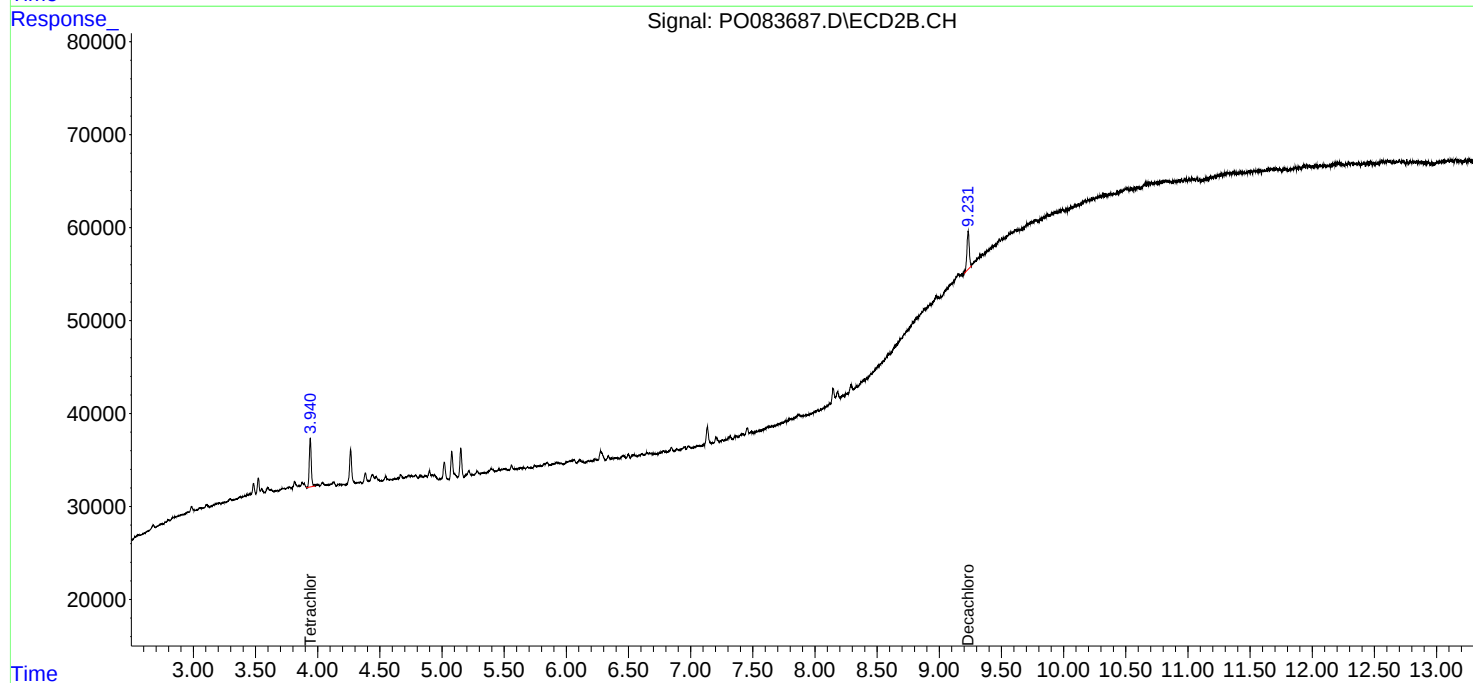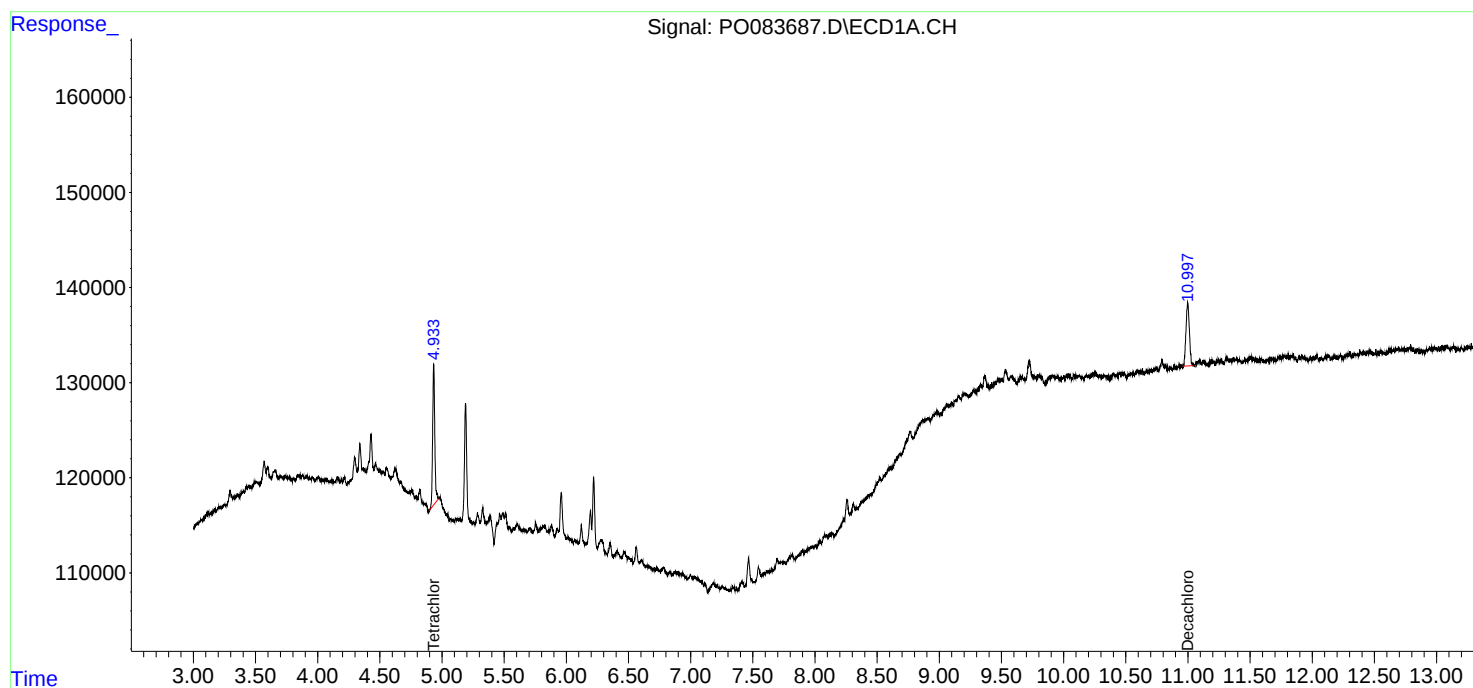


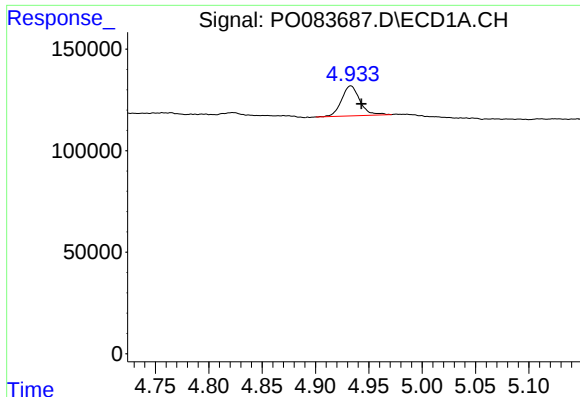

#1 Tetrachloro-m-xylene


R.T.: 4.933 min
Delta R.T.: -0.010 min
Response: 175735
Conc: 1.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
01-A-01-B-01-C

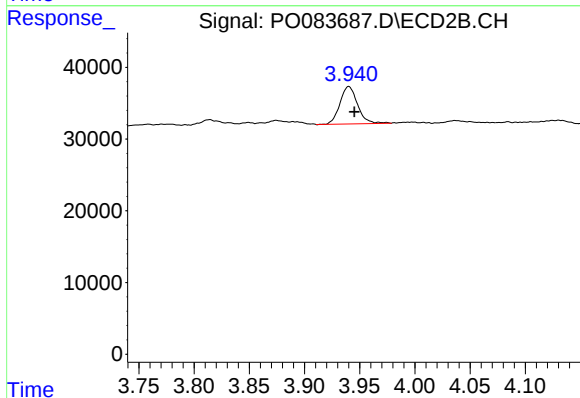


#1 Tetrachloro-m-xylene

R.T.: 3.940 min
Delta R.T.: -0.005 min
Response: 57864
Conc: 1.86 ng/ml

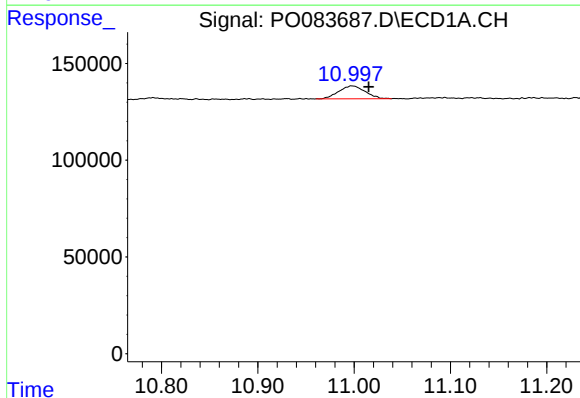

#2 Decachlorobiphenyl

R.T.: 10.997 min
Delta R.T.: -0.018 min
Response: 125851
Conc: 1.76 ng/ml

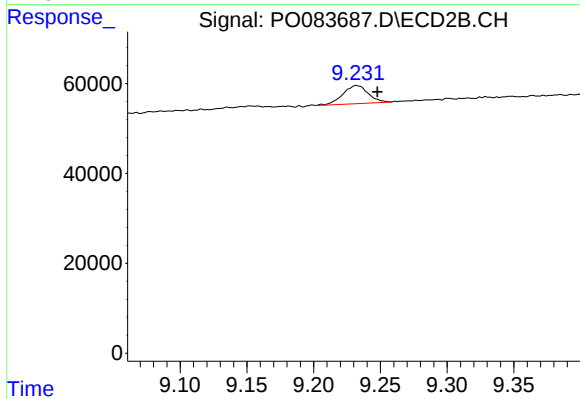

#2 Decachlorobiphenyl

R.T.: 9.232 min
Delta R.T.: -0.016 min
Response: 53613
Conc: 1.64 ng/ml