

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121422\
 Data File : PO091359.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Dec 2022 17:34
 Operator : YP/AJ
 Sample : N6038-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 RB-29-(2.5-4.5)

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/15/2022
 Supervised By :Ankita Jodhani 12/15/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 08:14:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112522.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Nov 28 11:25:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.296	3.472	59889332	18193064	17.713	17.334
2) SA Decachlor...	10.042	8.473	45467485	20527270	17.118	21.143m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121422\
Data File : P0091359.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Dec 2022 17:34
Operator : YP/AJ
Sample : N6038-01
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
RB-29-(2.5-4.5)


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/15/2022
Supervised By :Ankita Jodhani 12/15/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 08:14:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112522.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Nov 28 11:25:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

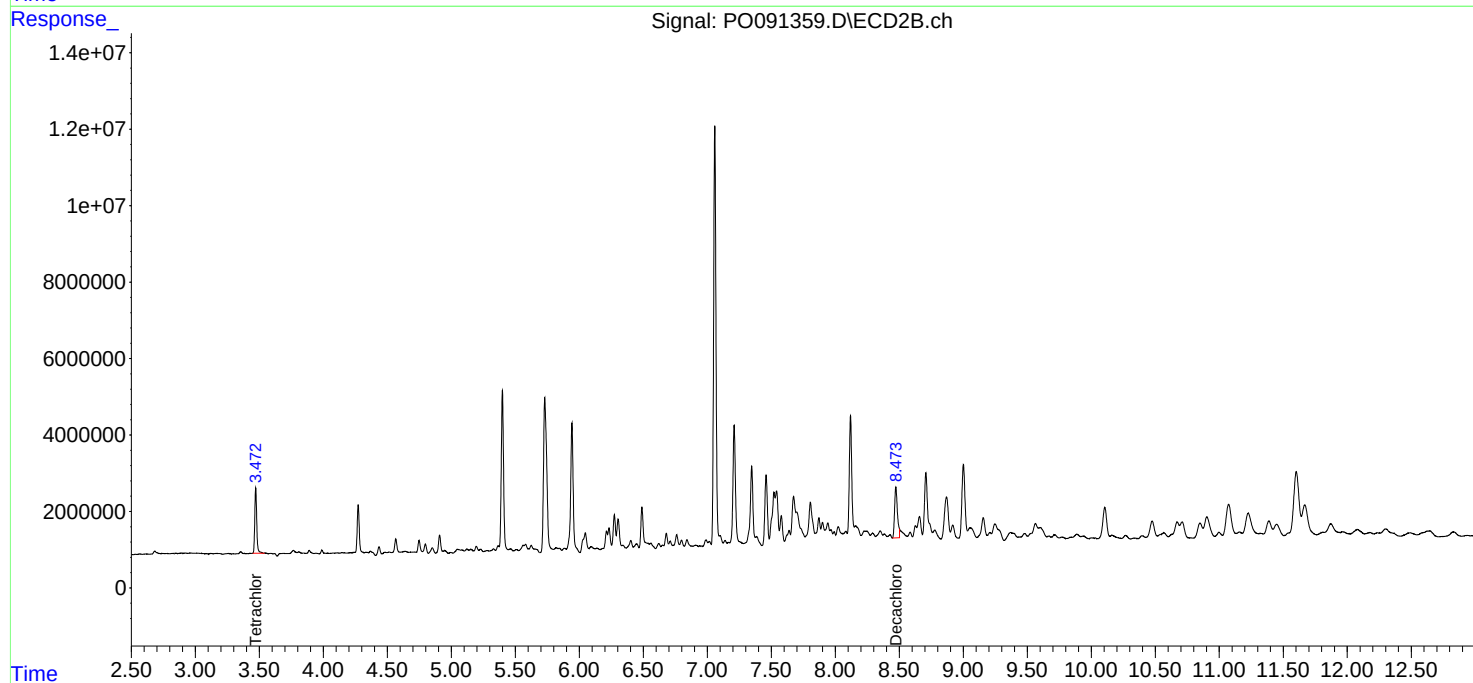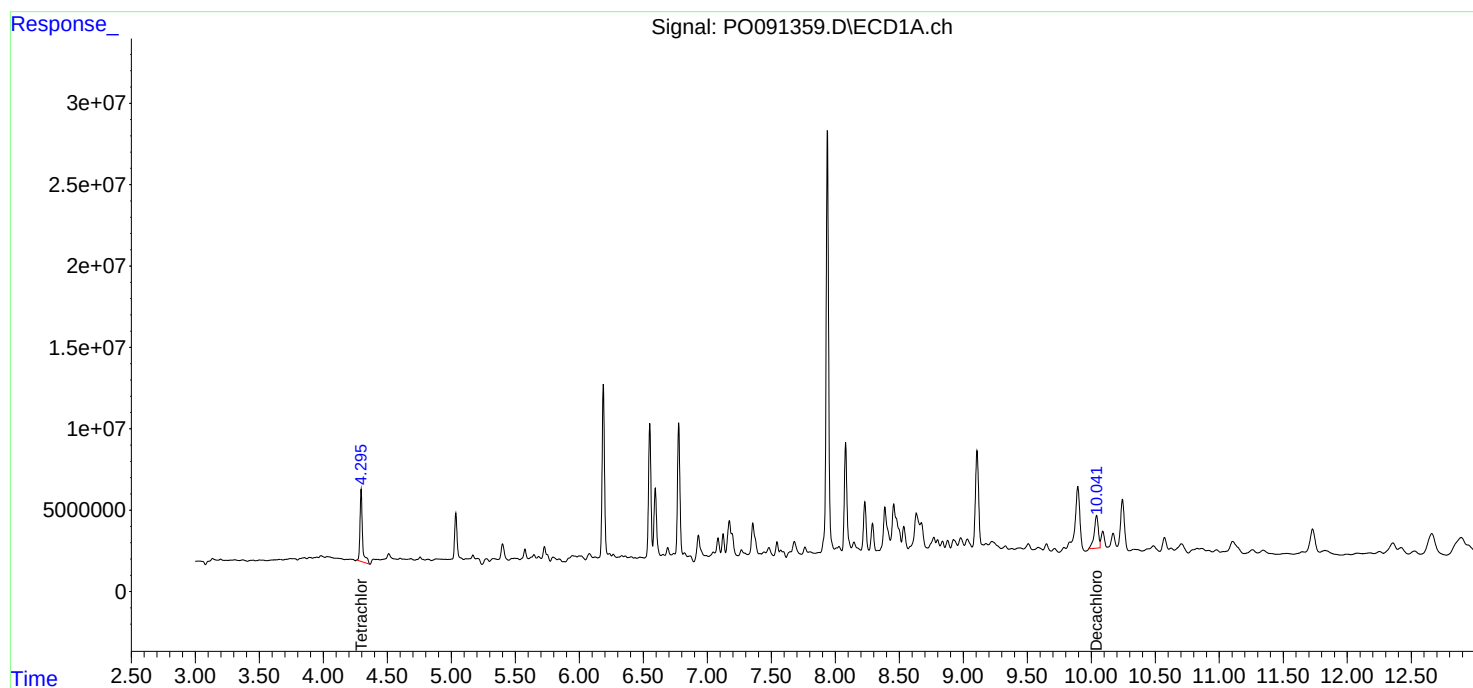

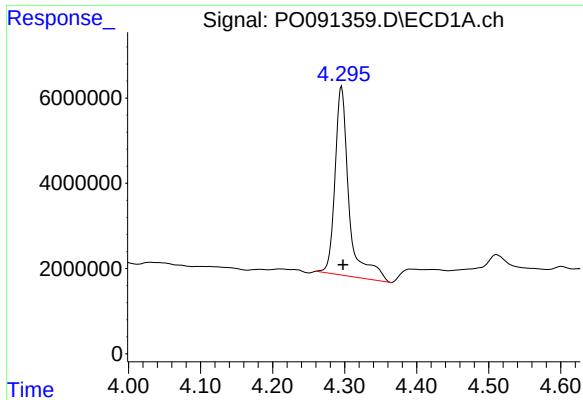


#1 Tetrachloro-m-xylene

R.T.: 4.296 min
Delta R.T.: -0.002 min
Response: 59889332
Conc: 17.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
RB-29-(2.5-4.5)


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/15/2022
Supervised By :Ankita Jodhani 12/15/2022

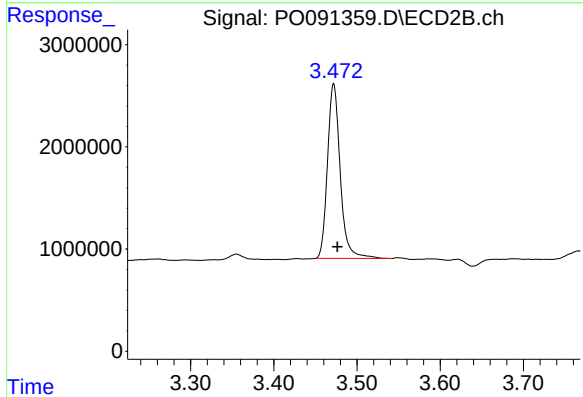


#1 Tetrachloro-m-xylene

R.T.: 3.472 min
Delta R.T.: -0.004 min
Response: 18193064
Conc: 17.33 ng/ml

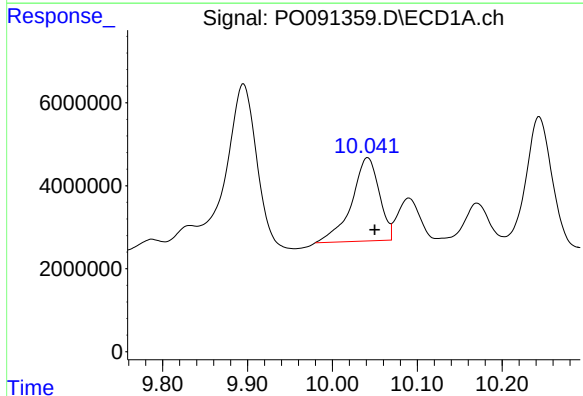

#2 Decachlorobiphenyl

R.T.: 10.042 min
Delta R.T.: -0.008 min
Response: 45467485
Conc: 17.12 ng/ml

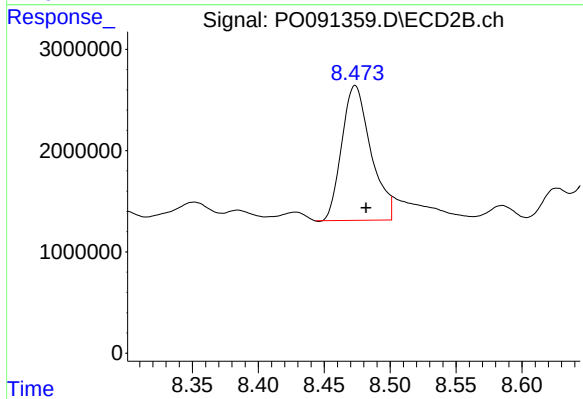

#2 Decachlorobiphenyl

R.T.: 8.473 min
Delta R.T.: -0.009 min
Response: 20527270
Conc: 21.14 ng/ml m