

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121423\
 Data File : PO100487.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Dec 2023 14:55
 Operator : YP/AJ
 Sample : 05759-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AU-06-121323

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/15/2023
 Supervised By :Ankita Jodhani 12/15/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 14 23:22:15 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 14 05:06:46 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.468	3.694	32124277	31879070	20.990	21.565
2) SA Decachlor...	10.326	8.773	19491929	22241472	20.680	20.836

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121423\
Data File : PO100487.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Dec 2023 14:55
Operator : YP/AJ
Sample : 05759-03
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AU-06-121323


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/15/2023
Supervised By :Ankita Jodhani 12/15/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 14 23:22:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121323.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 14 05:06:46 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

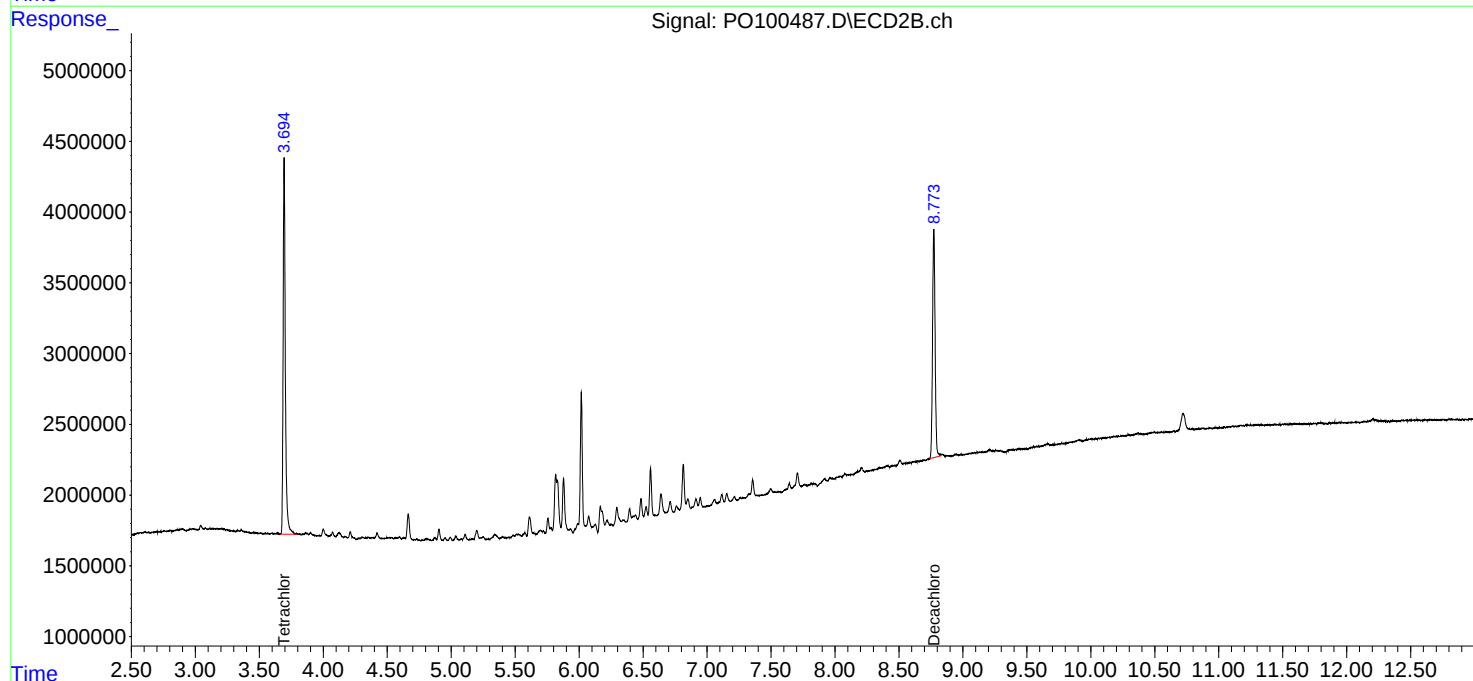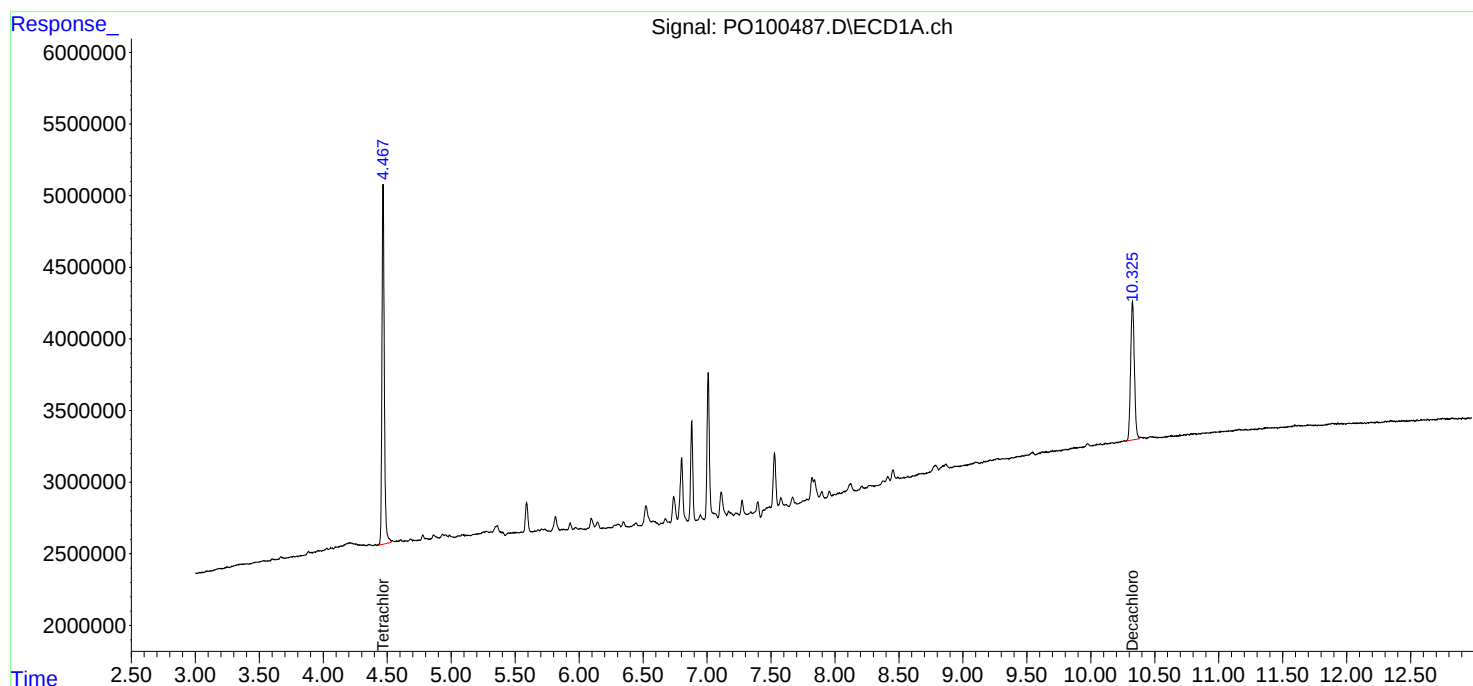

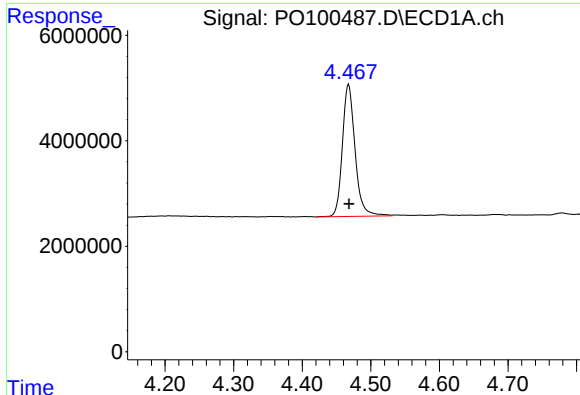

#1 Tetrachloro-m-xylene

R.T.: 4.468 min
Delta R.T.: 0.000 min
Response: 32124277
Conc: 20.99 ng/ml

Instrument :

ECD_O


ClientSampleId :

AU-06-121323

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 12/15/2023
Supervised By :Ankita Jodhani 12/15/2023

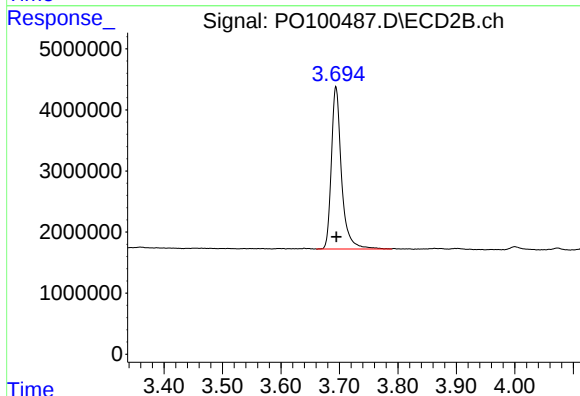


#1 Tetrachloro-m-xylene

R.T.: 3.694 min
Delta R.T.: 0.000 min
Response: 31879070
Conc: 21.57 ng/ml

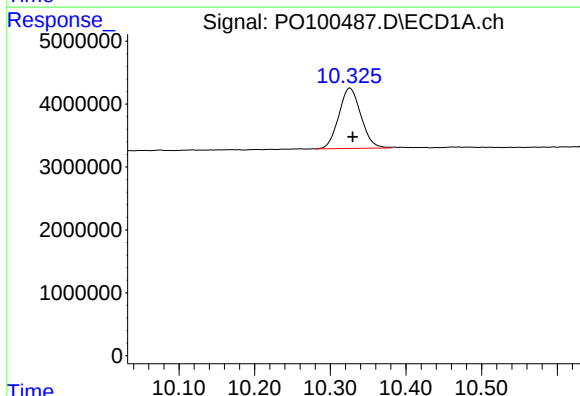

#2 Decachlorobiphenyl

R.T.: 10.326 min
Delta R.T.: -0.004 min
Response: 19491929
Conc: 20.68 ng/ml

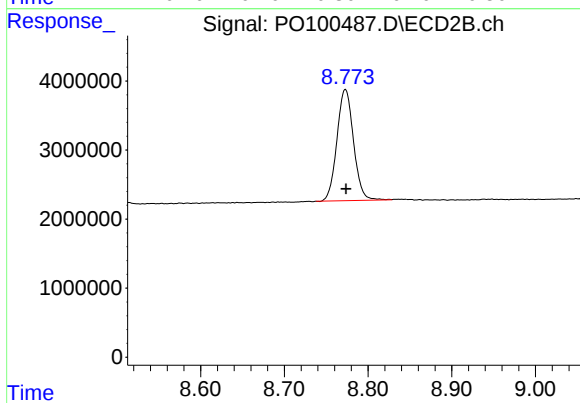

#2 Decachlorobiphenyl

R.T.: 8.773 min
Delta R.T.: -0.001 min
Response: 22241472
Conc: 20.84 ng/ml